



AD615955

AD

CCL REPORT NO. 180

IDENTIFICATION AND DETERMINATION
OF REACTIVE EPOXY DILUENTS BY
GAS-LIQUID CHROMATOGRAPHY

FINAL REPORT

BY

GEORGE G. ESPOSITO

24 MAY 1965

D
JUN 14 1965
COPY 2 OF 3
HARD COPY \$.0.50
MICROFICHE \$.0.50

AMCMS CODE NO. 5025.11.842
DA PROJECT NO. IC024401A329

118

U. S. ARMY COATING & CHEMICAL LABORATORY

Aberdeen Proving Ground
Maryland

ARCHIVE COPY

DDC AVAILABILITY NOTICE

Qualified requesters may obtain copies of this report from Defense Documentation Center, Cameron Station, Alexandria, Virginia 22314.

Copies Available at Office of Technical Services, \$0.50.

THE FINDINGS IN THIS REPORT ARE NOT TO BE CONSTRUED AS AN OFFICIAL DEPARTMENT OF THE ARMY POSITION, UNLESS SO DESIGNATED BY OTHER AUTHORIZED DOCUMENTS.

DESTROY THIS REPORT WHEN IT IS NO LONGER NEEDED. DO NOT RETURN IT TO THE ORIGINATOR.

BLANK PAGE

UNCLASSIFIED

CCL REPORT NO. 180

IDENTIFICATION AND DETERMINATION OF REACTIVE EPOXY
DILUENTS BY GAS-LIQUID CHROMATOGRAPHY

BY

GEORGE G. ESPOSITO

AMCMS CODE NO. 5025.11.842

DEPARTMENT OF THE ARMY PROJECT NO.
1C024401A329

U. S. ARMY COATING AND CHEMICAL LABORATORY
ABERDEEN PROVING GROUND
MARYLAND

UNCLASSIFIED

ABSTRACT

Programmed temperature gas chromatography (PTGC) is employed for the identification and determination of epoxy type reactive diluents in solventless epoxy compounds. The analysis can be applied directly to the product to be tested or, in the case of butyl glycidyl ether, to a sample separated from the resin.

TABLE OF CONTENTS

	<u>Page No.</u>
TITLE PAGE	i
ABSTRACT	ii
INTRODUCTION	1
DETAILS OF TEST	1 - 2
DISCUSSION	2
DISTRIBUTION LIST	3 - 5
APPENDIX A	6
Tables 1 - 11	6
APPENDIX B	7
Figures 1 - 3	7 - 9
DD FORM 1473	10

BLANK PAGE

I. INTRODUCTION

Reactive diluents such as butyl glycidyl ether (BGE), allyl glycidyl ether (AGE), phenyl glycidyl ether (PGE), butanediol diglycidyl ether (BDE) and styrene oxide are used to modify epoxy resins used in coatings, adhesives, laminates, castings and sealants. Handling problems are encountered when unmodified epoxies are employed and diluents must be added to reduce the viscosity. Organic solvents are not recommended for this purpose because solvents are retained in the polymer resulting in lower polymer strength.

When reactive diluents are incorporated into epoxy formulations, there is a great improvement in handling properties and only a minor sacrifice in the physical properties of the cured resin. The diluents contain epoxy groups which are capable of reacting in a manner similar to the epoxy resin and become an integral part of the polymer. These materials generally should not exceed 15 to 20 parts per hundred parts of resin.

Caulking compounds, based on a two component epoxy resin system, have been recommended for sealing weld joints in fuel tankers to prevent corrosion of the tank's interior and contamination of the fuel. It is essential that certain diluents be used in their proper proportion and analytical procedures are needed to insure conformity. The description of definitive analytical procedures for these materials could not be found in the literature. General tests such as epoxy equivalent, nonvolatile, etc. are inadequate and a more specific and accurate method is necessary. The objective of this investigation is to provide such a procedure.

PTGC has found broad utilization in the field of solvent analysis and this technique was also found suitable for the analysis of reactive epoxy diluents. The method can be applied directly to the epoxy component which has been weighed with an internal standard and thinned with acetone. Samples containing BGE are determined by thinning the sample with ethyl ether and immersing in an acetone-dry ice bath. After the resin precipitates, a portion of the liquid is reserved for the gas chromatographic analysis. The various reactive epoxy diluents are identified and determined by relating their retention times and peak areas to that of the internal standard.

II. DETAILS OF TEST

Chromatographic Unit

The instrument used to obtain the chromatograms was a Model 500 Linear Programmed Temperature Gas Chromatograph (F & M Scientific Co.) equipped with a Brown Elektronik Recorder (Minneapolis-Honeywell Regulator Co.)

Operating Conditions

Detector cell temperature, °C.	300
Detector cell current, ma.	150
Injection port temperature, °C.	250
Helium flow at exit, cc. per minute	85
Initial column temperature, °C.	100
Terminal column temperature, °C.	200
Column heating rate, °C. per minute	7.9

Gas Chromatographic Column

A 10-ft. length of 1/4 inch copper tubing was packed with 20 parts silicone grease on 80 parts of acid washed 60-80 mesh chromosorb W.

Analysis

Accurately weigh about 2 grams of sample and 0.2 grams of methyl benzoate into a 25 ml. flask.

Direct. Thin with two milliliters of acetone and inject 3 microliters of thinned sample onto the column; follow the operating conditions described above.

Indirect. Dissolve or disperse the sample and methyl benzoate in 10 milliliters of ethyl ether and immerse in a dry ice-acetone bath. After the resin separates, isolate a few mls. by pouring the supernatant liquid into a small test tube. Allow the sample in the test tube to warm to room temperature and inject 10 microliters onto the column. Comply with the operating conditions described above.

Results

The separation of reactive diluents is shown in Figure 1. Figure 2 illustrates a separation obtained from a commercial product which was found to contain butyl glycidyl ether. A synthetic mixture of two reactive diluents with an epoxy resin produced the chromatogram shown in Figure 3.

Retention times, relative to methyl benzoate, are presented in Table I. Analytical results, obtained from mixtures of known composition, are shown in Table II. The analysis of a commercial product yielded 14.5% of butyl glycidyl ether which was in good agreement with the 15% indicated by the manufacturer.

III. DISCUSSION

The direct method works well, but epoxy resin is introduced into the injection port with every injection of sample, and the accumulation of carbonaceous material in the vaporization chamber is objectionable. In this investigation primary interest was centered on butyl glycidyl ether, since this was the reactive diluent used in the caulking compound being evaluated. Decomposition of resin in the injection port can be circumvented by using the indirect method in which the resin is separated prior to the introduction of the sample into the instrument. This method works well with BGE, but is not applicable to the other reactive diluents.

Butanediol diglycidyl ether was investigated along with the other reactive diluents and produced a peak which was not in proportion to the amount used. The procedure proposed can be used to identify BDE but is not recommended as a quantitative method for this compound.

The procedure described in this report enhances the capability of the laboratory in an area where little or no information was available. The procedure is relatively rapid and accurate.

DISTRIBUTION LIST FOR AMCMS CODE NO. 5025.11.842

<u>Department of Defense</u>	<u>No. of Copies</u>
Defense Documentation Center Cameron Station Alexandria, Virginia 22314	20
<u>Department of the Army - Technical Services</u>	
Commanding General U.S. Army Materiel Command ATTN: AMCRD-RS-CM Washington, D. C. 20315	1
Continental Army Command Department of the Army Fort Monroe, Virginia 23351	3
Commanding General U.S. Army Tank-Automotive Center ATTN: Mr. J. P. Jones Warren, Michigan 48090	1
Commanding Officer Frankford Arsenal ATTN: SMUFA 1320 Library Philadelphia, Pa. 19137	1 1
Commanding Officer Harry Diamond Laboratory ATTN: Library Washington, D. C. 20425	1
Commanding Officer U.S. Army Test Activity Yuma Test Activity Yuma, Arizona 85364	1
Commanding General U.S. Army Weapons Command ATTN: ANSWE-RDR Rock Island, Illinois 61200	2
Commanding Officer U.S. Army Materials Research Agency ATTN: Technical Information Center Watertown, Mass. 02172	2

DISTRIBUTION LIST CONTINUED

	<u>No. of Copies</u>
Commanding Officer U.S. Army Chemical Research & Development Laboratories ATTN: Librarian Edgewood Arsenal, Maryland 21040	1
U.S. Army Engineer Research and Development Laboratories ATTN: STINFO Branch Fort Belvoir, Virginia 22060	2
Commanding Officer Rock Island Arsenal ATTN: Laboratory 9320 Rock Island, Illinois 61200	1
Commanding Officer Springfield Armory ATTN: Engineering Division Springfield, Mass. 01101	1
Commanding Officer Watervliet Arsenal ATTN: Dr. R. Weigle Watervliet, New York 12189	1
Commanding Officer Picatinny Arsenal ATTN: Mr. J. J. Begley Dover, New Jersey 07801	1
Commanding Officer U.S. Army Ballistic Research Laboratories ATTN: Mr. W. C. Pless Mr. R. Eichelberger Mr. J. Sperrazza Aberdeen Proving Ground, Maryland 21005	1 1 1
Technical Library Aberdeen Proving Ground, Maryland 21005	1
<u>Department of the Navy</u>	
Department of the Navy c/o Navy Liaison Aberdeen Proving Ground, Maryland 21005	1

DISTRIBUTION LIST CONTINUED

No. of Copies

Commander
U.S. Naval Weapons Laboratory
Dahlgren, Virginia

1

Department of the Navy
Chief, Bureau of Naval Weapons
Washington 25, D. C.

1

Department of the Air Force

Headquarters
Aeronautical System Division
Air Force Systems Command
ATTN: ASRCE-31
Wright Patterson Air Force Base, Ohio

1

Other Government Agencies

Scientific and Technical Information Facility
ATTN: NASA Representative (S-AK/DL)
P.O. Box 5700
Bethesda, Maryland 20014

3

Chief, Input Section
Clearinghouse for Federal Scientific
and Technical Information, CFSTI
Sills Building
5285 Port Royal Road
Springfield, Virginia 22151

100

Foreign Address

Commander
British Army Staff
3100 Massachusetts Avenue, N. W.
Washington 8, D. C.

2

Canadian Army Staff
ATTN: GSO-1, A&R Section
2450 Massachusetts Avenue, N. W.
Washington 8, D. C.

2

APPENDIX A

TABLE I

RELATIVE RETENTION TIME DATA FOR DILUENTS

	Relative Retention Time (methyl benzoate = 1)
Allyl glycidyl ether	0.51
Butyl glycidyl ether	0.73
Styrene oxide	0.90
Phenyl glycidyl ether	1.40
Butanediol diglycidyl ether	2.0

TABLE II

ANALYSIS OF KNOWN MIXTURES

Sample Type	Present, %	Found, %
1. Butyl glycidyl ether*	18.2	18.2; 18.3
2. Phenyl glycidyl ether**	9.8	9.5; 9.7
Allyl glycidyl ether	8.6	8.4; 8.6

*Blended with liquid epoxy resin, indirect method used.

**Blended with liquid epoxy resin, direct method used.

APPENDIX B

Figure 1
Separation of reactive epoxy diluents.

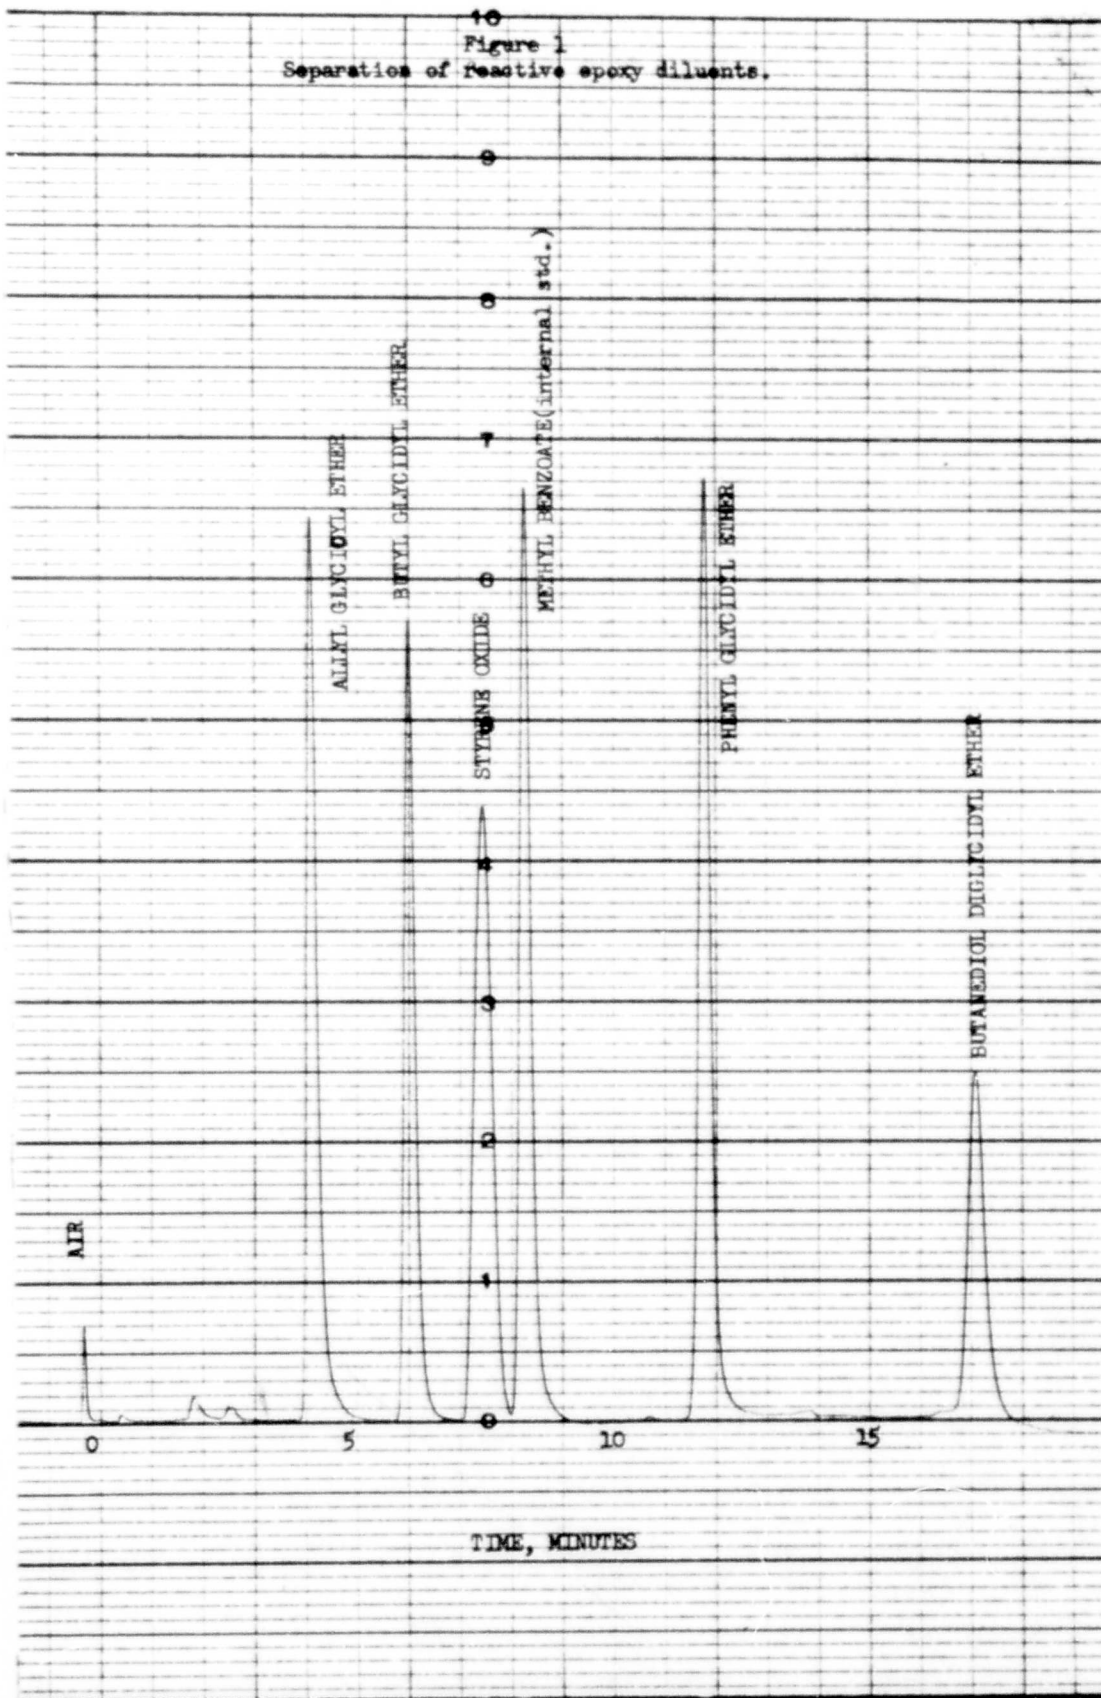


Figure 2
Analysis of commercial product.

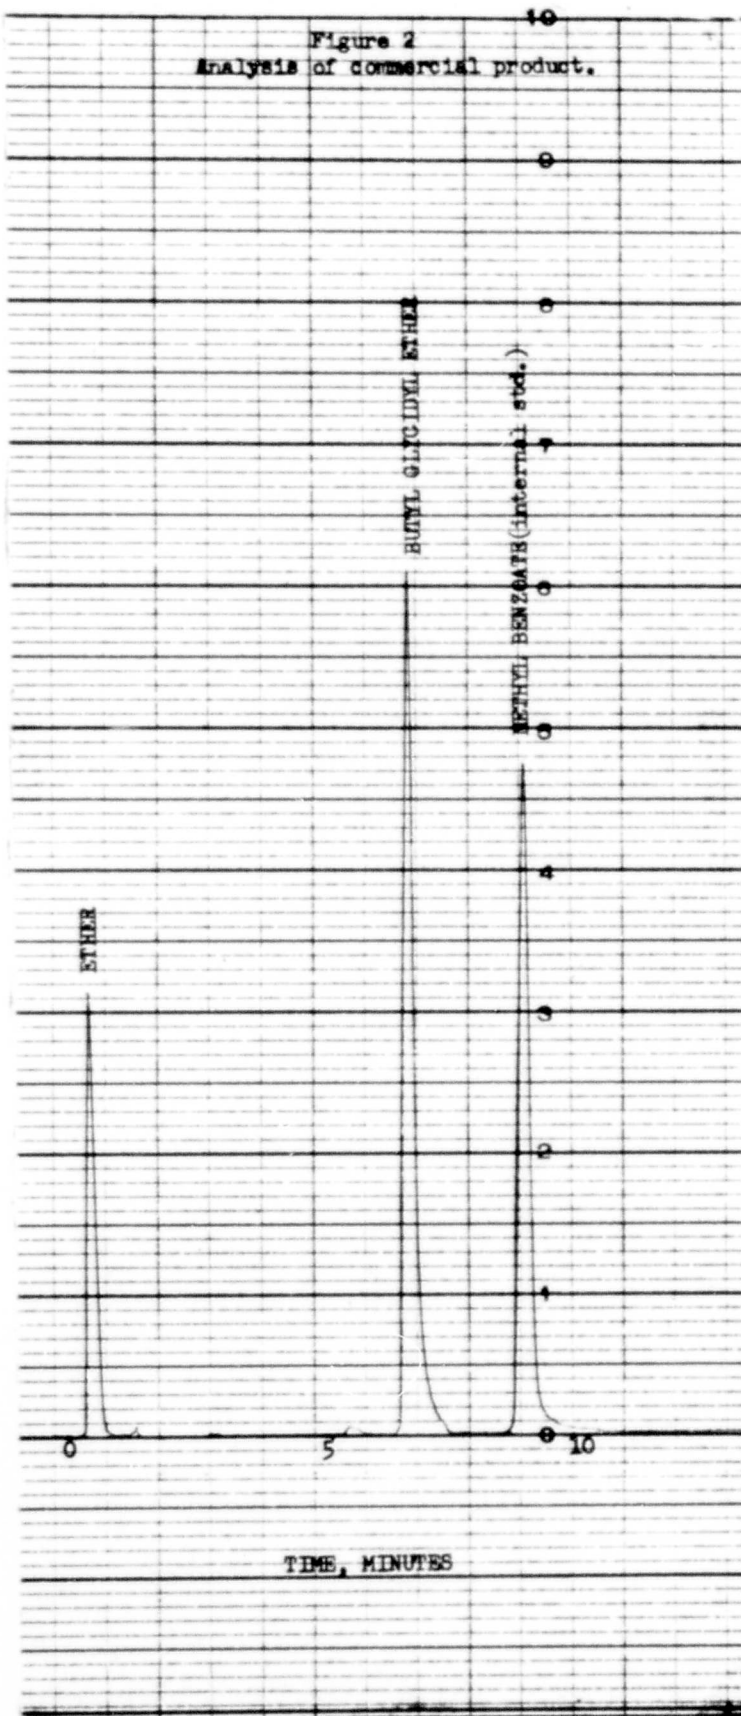


Figure 3
Analysis of synthetic mixture.

