

UNCLASSIFIED

AD 664 465

A PORTABLE DEVICE FOR THE MEASUREMENT OF
EVAPORATIVE WATER LOSS

G.E. Funkhouser, et al

Civil Aeromedical Institute
Oklahoma City, Oklahoma

August 1967

Processed for . . .

DEFENSE DOCUMENTATION CENTER
DEFENSE SUPPLY AGENCY



U. S. DEPARTMENT OF COMMERCE / NATIONAL BUREAU OF STANDARDS / INSTITUTE FOR APPLIED TECHNOLOGY

UNCLASSIFIED

AD 664465



A Portable Device for the Measurement of Evaporative Water Loss

August, 1967

D D C
RECEIVED
FEB 1 1968
B

Approved by the
CLEARINGHOUSE
for general dissemination
Information Report No. 67-17

**OFFICE OF AVIATION MEDICINE
DEPARTMENT OF TRANSPORTATION
FEDERAL AVIATION ADMINISTRATION**



This document has been approved
for public release and other dis-
tribution is authorized.

Federal Aviation Administration, Office of Aviation Medicine, Civil Aeromedical Institute, Oklahoma City, Oklahoma. **A PORTABLE DEVICE FOR THE MEASUREMENT OF EVAPORATIVE WATER LOSS** by G. E. Funkhouser and S. M. Billings, August 1967. 7 pp., Report No. AM 67-17.

A portable device has been developed for the precise measurement of evaporative water loss. Under appropriate conditions the measurement of evaporative water loss may be used as an index of "emotional stress" in flying personnel. The apparatus incorporates a thermal conductivity cell as a moisture sensor, a proportional heater control to maintain the cell at the proper temperature, and a compressed air circuit to act as a carrier for water vapor. The unit is entirely battery powered.

I. Funkhouser,
G. E.
II. Billings, S. M.

Descriptors
Instrumentation
Evaporative
Water Loss
Sweating
Temperature
Regulation
Psychology

Federal Aviation Administration, Office of Aviation Medicine, Civil Aeromedical Institute, Oklahoma City, Oklahoma. **A PORTABLE DEVICE FOR THE MEASUREMENT OF EVAPORATIVE WATER LOSS** by G. E. Funkhouser and S. M. Billings, August 1967. 7 pp., Report No. AM 67-17.

A portable device has been developed for the precise measurement of evaporative water loss. Under appropriate conditions the measurement of evaporative water loss may be used as an index of "emotional stress" in flying personnel. The apparatus incorporates a thermal conductivity cell as a moisture sensor, a proportional heater control to maintain the cell at the proper temperature, and a compressed air circuit to act as a carrier for water vapor. The unit is entirely battery powered.

I. Funkhouser,
G. E.
II. Billings, S. M.

Descriptors
Instrumentation
Evaporative
Water Loss
Sweating
Temperature
Regulation
Psychology

Federal Aviation Administration, Office of Aviation Medicine, Civil Aeromedical Institute, Oklahoma City, Oklahoma. **A PORTABLE DEVICE FOR THE MEASUREMENT OF EVAPORATIVE WATER LOSS** by G. E. Funkhouser and S. M. Billings, August 1967. 7 pp., Report No. AM 67-17.

A portable device has been developed for the precise measurement of evaporative water loss. Under appropriate conditions the measurement of evaporative water loss may be used as an index of "emotional stress" in flying personnel. The apparatus incorporates a thermal conductivity cell as a moisture sensor, a proportional heater control to maintain the cell at the proper temperature, and a compressed air circuit to act as a carrier for water vapor. The unit is entirely battery powered.

I. Funkhouser,
G. E.
II. Billings, S. M.

Descriptors
Instrumentation
Evaporative
Water Loss
Sweating
Temperature
Regulation
Psychology

Federal Aviation Administration, Office of Aviation Medicine, Civil Aeromedical Institute, Oklahoma City, Oklahoma. **A PORTABLE DEVICE FOR THE MEASUREMENT OF EVAPORATIVE WATER LOSS** by G. E. Funkhouser and S. M. Billings, August 1967. 7 pp., Report No. AM 67-17.

A portable device has been developed for the precise measurement of evaporative water loss. Under appropriate conditions the measurement of evaporative water loss may be used as an index of "emotional stress" in flying personnel. The apparatus incorporates a thermal conductivity cell as a moisture sensor, a proportional heater control to maintain the cell at the proper temperature, and a compressed air circuit to act as a carrier for water vapor. The unit is entirely battery powered.


I. Funkhouser,
G. E.
II. Billings, S. M.

Descriptors
Instrumentation
Evaporative
Water Loss
Sweating
Temperature
Regulation
Psychology

**A PORTABLE DEVICE FOR THE MEASUREMENT OF
EVAPORATIVE WATER LOSS**

**G. E. Funkhouser
S. M. Billings**

Approved by



**J. ROBERT DILLE, M.D.
CHIEF, CIVIL AEROMEDICAL
INSTITUTE**

Released by



**P. V. SIEGEL, M.D.
FEDERAL AIR SURGEON**

August 1967

**FEDERAL AVIATION ADMINISTRATION
Office of Aviation Medicine**

Qualified requesters may obtain Aviation Medical Reports from Defense Documentation Center. The general public may purchase from Clearinghouse for Federal Scientific and Technical Information, U.S. Dept. of Commerce, Springfield, Va. 22151

A PORTABLE DEVICE FOR THE MEASUREMENT OF EVAPORATIVE WATER LOSS

G. E. FUNKHOUSER and S. M. BILLINGS

I. Introduction.

Haywood and Shoemaker have stated, "Many investigators . . . have demonstrated an increase in palmar sweating associated with the imposition of some anxiety-arousing stimulus situation into the subject's life."¹ A method for measuring evaporative water loss by using a thermal conductivity cell as a moisture detector has been described by Adams et al.^{2,3} and has been used to measure palmar sweat production^{4,5,6}. The method reported by Adams is precise, stable, and sensitive, but is dependent upon a 110 V AC power source. This report describes modifications of the method which permit its use in aircraft or in other field situations where electrical power sources are varied or non-existent.

II. Description.

The original method has been modified to provide a lighter, smaller, simpler device with self-contained DC power sources. The modifications include the use of proportional heater control and minor changes in the bridge circuit.

The "off-on" type of heater control maintains a nearly constant temperature more precisely when the heater voltage is adjusted so that heat gain in the constant-temperature enclosure is slightly greater than heat loss. Variations in environmental temperature consequently necessitate readjustment of the heater voltage to obtain maximum control precision. Proportional heater control, on the other hand, automatically provides maximum heater output for the initial rise to operating temperature, and thereafter continuously adjusts heater voltage to maintain the operating temperature. Changes in environmental temperatures commonly encountered in field studies do not affect temperature stability


with this system. The proportional heater control circuit is shown in Fig. 1.

No temperature indicator has been incorporated into this unit; however, a thermistor was mounted inside the constant-temperature enclosure with an external jack. The jack provides a means of connecting a YSI¹ Tele-thermometer for checking temperature stability when heater malfunction is suspected.

The bridge for the thermal conductivity cell has been changed to exclude the potentiometers for voltage, coarse current, and sensitivity adjustments (Fig. 2). The voltage to the bridge was reduced to six volts, permitting deletion of the voltage and coarse-current potentiometers. Sensitivity can still be regulated by varying the size of the moisture pick-up capsule or by placing an appropriate resistor in series with the recorder. The voltmeter in the circuit could also be eliminated because its only function is a rapid check of bridge battery condition.

Three six-volt nickel-cadmium batteries (Eveready, N67) were used, one in the bridge circuit and two connected in parallel to drive a 12-volt Pittman miniature motor (Model DC-71B) fitted with a one-inch nylon propeller located inside the constant-temperature enclosure. Operation of the fan motor at six volts provides ample mixing of air. Two 16-volt batteries (Eveready, N40) were connected in series to the proportional heater control as shown in Fig. 1. The use of the 32-volt transformer to operate the heater and a battery eliminator to drive the stirring motor prior to actual testing conserves battery power. At present, recordings are made on a Mosely strip-chart recorder (Model 680) powered by a

¹YSI; Yellow Springs Instrument Co., Yellow Springs, Ohio.

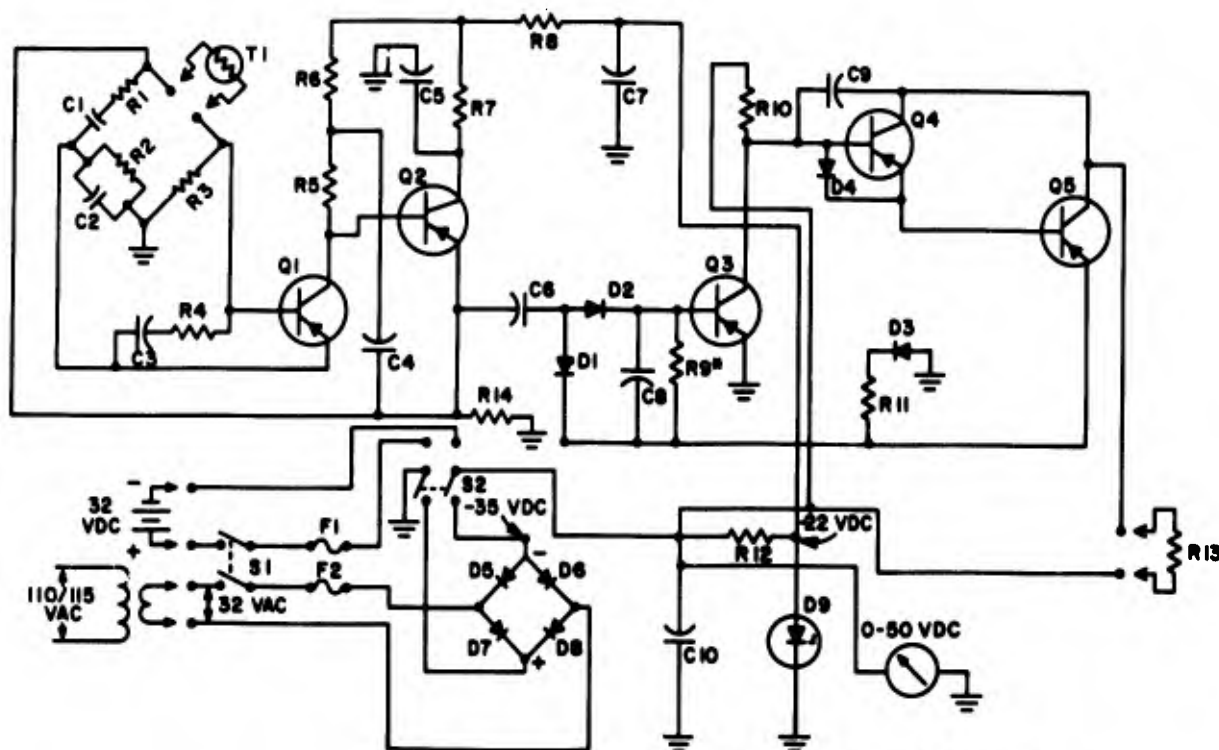

* Indicates Selected Component.

Q1, Q2, Q3 - 2N652A
 Q4 - 2N303
 Q5 - 2N1103B
 C1 - .1 μ f
 C2 - .047 μ f
 C3 - .022 μ f
 C4, C5, C6, C7, C8 - 4.7 μ f
 C9 - 20 μ f
 C10 - 500 μ f
 F1, F2 - .5 amp
 T1 - YSI Thermistor Probe Type 417

R1 - 600 Ω 1/2 W
 R2 - 2200 Ω 1/2 W
 R3 - 1027 Ω 1/2 W
 R4 - 22 Ω
 R5, R6 - 4300 Ω
 R7, R14 - 820 Ω
 R8 - 100 Ω
 R9 - 12K Ω
 R10 - 18K Ω
 R11 - 6.8 Ω 1W
 R12 - 400 Ω 3W
 R13 - 150 Ω Oven Heater

D1, D2 - Si-50 at IV 200 me PIV
 D3, D5, D6, D7, D8 - IN2070
 D4 - Ge-100 me at IV 60 PIV
 D9 - IN1597A 22v Regulator
 S1 - Dpst- ON OFF
 S2 - Dpst- AC-DC Operation

FIGURE 1. Diagram of proportional heater control circuit.*
 *Reproduced by permission of Hewlett-Packard Company, Palo Alto, California; modification of Oven Control Assembly 5243A-65T.

12-volt Centralab Power Pack (Cr1-1200) through a Terado 12 V DC to 110 V AC converter (Model 50122).

Air for the pneumatic system is supplied by a 96 cubic-inch gas cylinder fitted with a K-valve and a Cornelius Company pressure-reduction regulator (Model 2). The air passes through a small cylinder filled with "Drierite" to a Nupro-fine needle valve (Model B4M), then through the reference side of the thermal conductivity cell to the moisture pick-up capsule. The air is

returned from the capsule through the other side of the cell and is exhausted through a flow meter. After the proper flow rate is established, the flow meter is disconnected.

Shielding of electrical connections to the thermal conductivity cell was not necessary, probably because of the elimination of AC voltage from the circuits.

The batteries mentioned above will operate the heater and stirring motor for four to five hours. The recorder will operate approximately

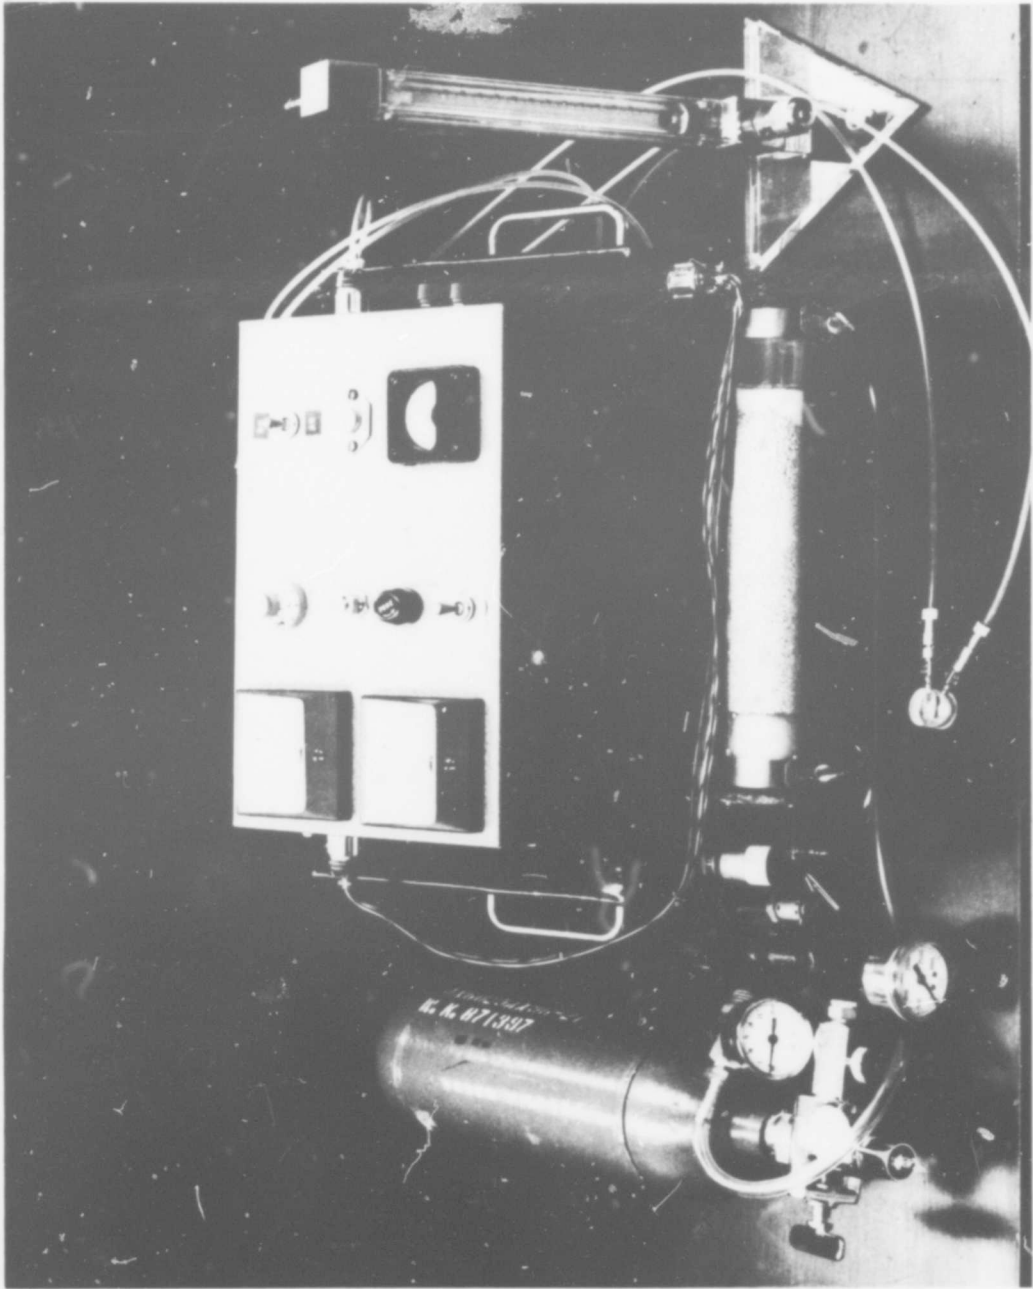


FIGURE 3. Portable evaporative water loss device.



FIGURE 4. Portable evaporative water loss device in use.

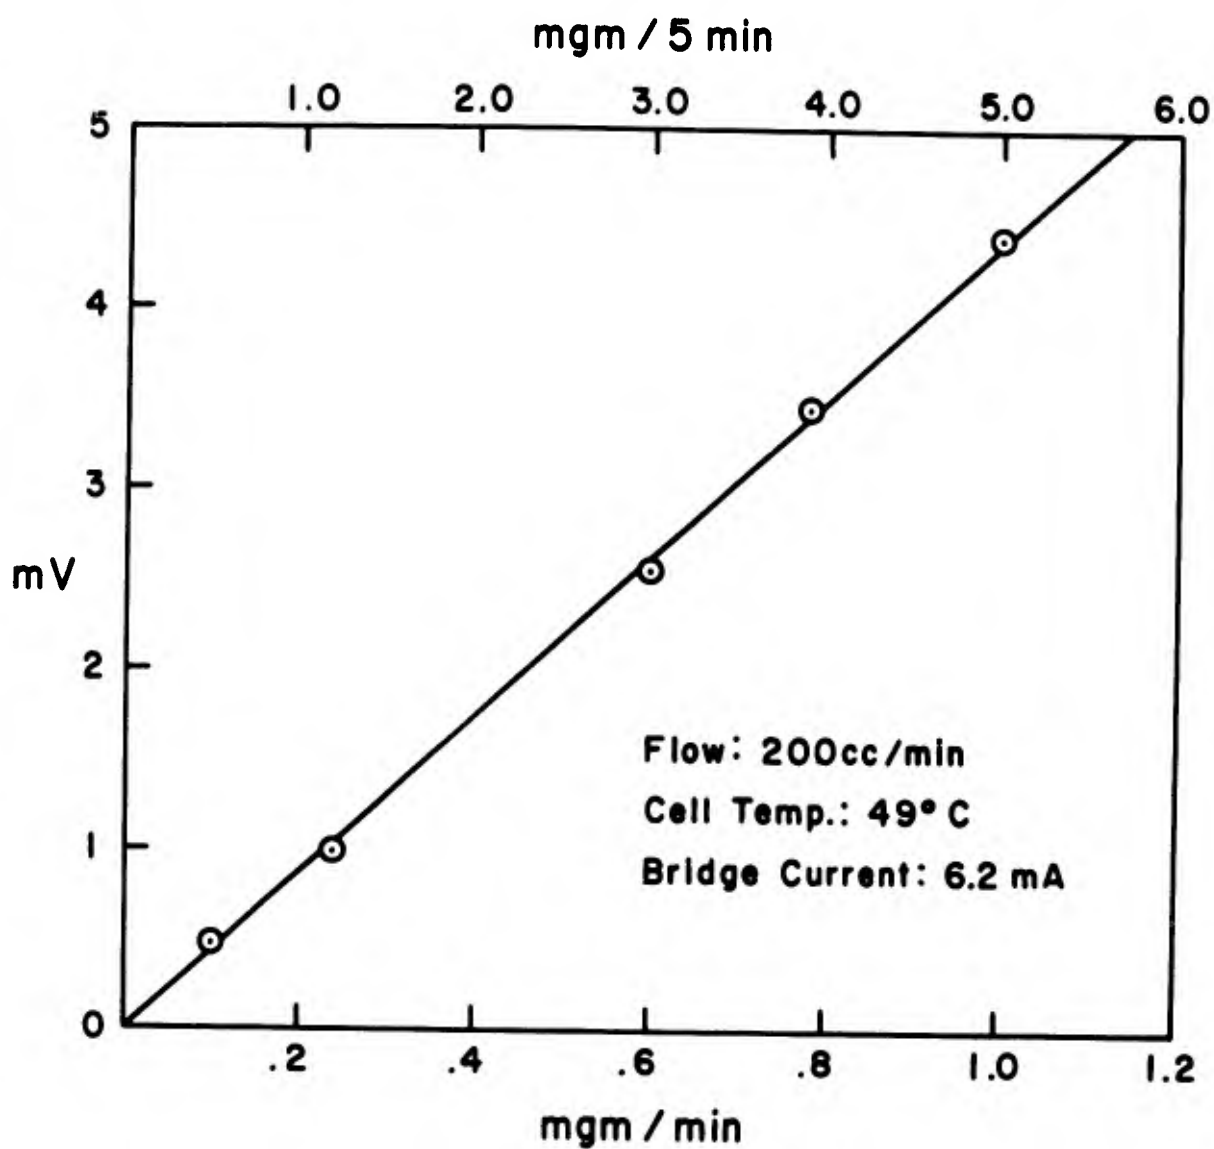


FIGURE 5. Calibration curve for portable evaporative water loss device.

REFERENCES

1. HAYWOOD, H. D. and D. J. SHOEMAKER. "Measurement of Palmar Sweating: Effect of Repeated Measurement from the Same Area." *J. Psychol.* 55:363-369 (1963).
2. ADAMS, T., G. E. FUNKHOUSER, and W. W. KENDALL. "Measurement of Evaporative Water Loss by a Thermal Conductivity Cell." *J. Appl. Physiol.* 18(6): 1291-1293. (1963).
3. ADAMS, T., G. E. FUNKHOUSER, and W. W. KENDALL. "Measurement of Evaporative Water Loss by a Thermal Conductivity Cell." *OAM Report No. AM 63-25.* (1963).
4. HAUTY, G. T., and T. ADAMS. "Phase Shifts of the Human Circadian System and Performance Deficit During the Period of Transition: I. East-West Flight." *OAM Report No. AM 65-28.* (1965).
5. HAUTY, G. T., and T. ADAMS. "Phase Shifts of the Human Circadian System and Performance Deficit During the Period of Transition: II. West-East Flight." *OAM Report No. AM 65-29.* (1965).
6. HAUTY, G. T., and T. ADAMS. "Phase Shifts of the Human Circadian System and Performance Deficit During the Period of Transition: III. North-South Flight." *OAM Report No. AM 65-30.* (1965).