

AD/A-006 389

MEASURED EFFECTS OF SQUARE-WAVE MODULATED RF FIELDS
(450 AND 3100 MHz) ON CARDIAC PACEMAKERS

SCHOOL OF AEROSPACE MEDICINE

DECEMBER 1974

DISTRIBUTED BY:

NTIS

National Technical Information Service
U. S. DEPARTMENT OF COMMERCE

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER SAM-TR-74-51	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER AD/A-006389
4. TITLE (and Subtitle) MEASURED EFFECTS OF SQUARE-WAVE MODULATED RF FIELDS (450 AND 3100 MHz) ON CARDIAC PACEMAKERS		5. TYPE OF REPORT & PERIOD COVERED Final Report January - June 1974
7. AUTHOR(s) William D. Hurt, M.S.; John C. Mitchell, B.S.; Terry O. Steiner, Staff Sergeant, USAF		6. PERFORMING ORG. REPORT NUMBER
9. PERFORMING ORGANIZATION NAME AND ADDRESS USAF School of Aerospace Medicine (RAP) Aerospace Medical Division (AFSC) Brooks Air Force Base, Texas 78235		8. CONTRACT OR GRANT NUMBER(s)
11. CONTROLLING OFFICE NAME AND ADDRESS USAF School of Aerospace Medicine (RAP) Aerospace Medical Division (AFSC) Brooks Air Force Base, Texas 78235		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 62202F 77570146
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		12. REPORT DATE December 1974
		13. NUMBER OF PAGES 37
		15. SECURITY CLASS. (of this report) Unclassified
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Approved for public release; distribution unlimited.		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES Reproduced by NATIONAL TECHNICAL INFORMATION SERVICE U.S. Department of Commerce Springfield VA 22151		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Cardiac pacemakers Electromagnetic interference and pacemakers Radiofrequency radiation effects on pacemakers Microwave radiation effects on pacemakers		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) Tests were performed to measure the effect of pulsed 450 and 3100 MHz RF radiation on cardiac pacemakers. All models were tested in both a free-field and a simulated-implant configuration and were continuously monitored during testing. Most of the models exhibited some type of electromagnetic interference under some conditions of the tests, although five recent, different models were unaffected under all conditions of these tests.		



DD FORM 1 JAN 73 1473

EDITION OF 1 NOV 65 IS OBSOLETE

PRICES SUBJECT TO CHANGE
UNCLASSIFIED
SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

ACE-33000 for	
NTIS	White Section ☒
U.S.	DoD Section ☒
ORAL	☐
JUSTIFICATION	
BY	
DISTRIBUTION/AVAILABILITY CODES	
Dist.	AVAIL. and/or SPECIAL

NOTICES

This final report was submitted by personnel of the Radiation Physics Branch, Radiobiology Division, USAF School of Aerospace Medicine, Aerospace Medical Division, AFSC, Brooks Air Force Base, Texas, under job order 7757-01-46.

When U.S. Government drawings, specifications, or other data are used for any purpose other than a definitely related Government procurement operation, the Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data is not to be regarded by implication or otherwise, as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

This report has been reviewed and cleared for open publication and/or public release by the appropriate Office of Information (OI) in accordance with AFR 190-17 and DODD 5230.9. There is no objection to unlimited distribution of this report to the public at large, or by DDC to the National Technical Information Service (NTIS).

This technical report has been reviewed and is approved for publication.

William D. Hurt

WILLIAM D. HURT, M.S.
Project Scientist

Evan R. Golera

EVAN R. GOLERA, Colonel, USAF, MC
Commander

CONTENTS

	<u>Page</u>
INTRODUCTION	3
TEST PROCEDURES	4
TEST RESULTS	5
CONCLUSIONS	17
BIBLIOGRAPHY	19
ABBREVIATIONS AND ACRONYMS	35

Figures and Tables

Figure No.

1. Sample pacemaker test population	6
2. Plexiglas, pacemaker test stand and saline phantom	8
3. Test equipment for pacemaker response (block diagram)	9
4. Attenuation of 3100 MHz EMR by saline solution as measured by a cavity-back spiral antenna	15
5. Relative 450 MHz EMI thresholds vs. pulse width for various pacemakers	16
6. Relative 3100 MHz EMI thresholds vs. pulse width for various pacemakers	18

Table No.

1. Cardiac pacemaker nomenclature and number of units tested	22
2. Pacemaker EMI thresholds	24
3. Free-field pacemaker EMI thresholds	28
4. Simulated-implant pacemaker EMI thresholds	32
5. Pacemaker EMI attenuation in saline solution	34

MEASURED EFFECTS OF SQUARE-WAVE MODULATED RF FIELDS (450 AND 3100 MHz) ON CARDIAC PACEMAKERS

INTRODUCTION

The potential hazard from the interaction of radiofrequency (RF) electromagnetic radiation and cardiac pacemakers has been identified through tests conducted by personnel at the USAF School of Aerospace Medicine (USAFSAM) during the past three years. Such tests defined the type and extent of interference possible, and established the relative electromagnetic radiation interference (EMI) sensitivities among the pacemakers marketed or available at each point in time (5, 6, 11, 12, 13, 14, 17, 21).

In spite of the fact that many of the earlier model pacemakers and some currently marketed devices still have adverse effect thresholds below 10 volts per meter (V/m), it has been apparent from the beginning of the pacemaker testing program that designing a demand type pacemaker with good EMI characteristics--without sacrifice of other functional aspects--was technically feasible. Hence, in May 1973, USAFSAM personnel prepared and presented to the Food and Drug Administration a recommendation that manufacturers design and qualify their pacemakers to function properly at an E-field level of 200 V/m (rms), in the frequency range 200 - 500 MHz, using a square-wave pulse at a pulse repetition rate (PRR) of 5 pulses per second (pps) with a 1 - 10 millisecond (msec) pulse width. It is recognized that 200 V/m is the maximum E-field level associated with a 10 mW/cm² continuous wave (CW) emission, and that pulsed fields could be much higher than 200 V/m while staying below 10 mW/cm² (average power density). However, if all marketed pacemakers would function properly in a pulsed 200 V/m field, the potential EMI problem areas would be essentially eliminated.

By early 1974, an overall improvement became apparent in the EMI characteristics of pacemakers being marketed, and a new test program was initiated at USAFSAM to evaluate the significance of this trend.

EDITOR'S NOTE: The principal abbreviations and acronyms in this report are listed and briefly defined on p. 35.

This program was to include laboratory tests at radiofrequencies of 27 MHz, 450 MHz, and 3100 MHz as well as field tests around numerous high-power RF emitters.

TEST PROCEDURES

The first of these tests was conducted by USAFSAM personnel at the Georgia Institute of Technology (GIT) Engineering Experiment Station (Atlanta, Georgia), 18 - 29 March 1974. Here, 72 pacemakers representing 10 manufacturers and 24 different designs (Fig. 1 and Table 1) were tested in an anechoic chamber in square-wave modulated 450 MHz and 3100 MHz RF radiation fields. The 450 MHz fields were circularly polarized with electric field (E-field) levels up to 292 V/m. The ranges of pulse width and repetition rate used were 1 microsecond (μ sec) to 1 msec and 2 - 50 pps, respectively. The 3100 MHz fields were vertically polarized with levels up to 320 V/m (rms) for a pulse-width range of 10 - 120 μ sec at 7 - 400 pps.

Both free-field and simulated-implant configurations were investigated for the purpose of determining the shielding factor afforded by implantation. The effect of pulse-width and repetition rate on pacemaker response was studied. A cursory study of the effect of different pacemakers leads on interference thresholds was also accomplished.

When tested, the pacemakers were positioned in the far-field region of the anechoic chamber on the center line of the radiation device. For the free-field configuration: the pacemakers and leads were mounted on a Plexiglas stand (Fig. 2). For the simulated-implant configuration: the Plexiglas stand was so placed in the phantom (20 x 30 x 30 cm with 0.15-cm wall thickness), filled with 0.03 molar saline solution, that the pacemaker was 1 cm from the phantom wall facing the incident radiation.

The pacemaker response was recorded via a telemetry system which was designed to present the pacemaker with a load comparable to that produced by the heart and to provide as much isolation of the pacemaker as possible. The load network was mounted on a subminiature audio jack to which the pacemaker leads were attached with "flea clips." A light-emitting diode (LED) was mounted in a mating plug;

EDITOR'S NOTE: All tables are grouped at the close of this report.

and when the pacemaker fired, approximately one-half of the pacer output current passed through the LED, causing it to flash during the pulse. The LED was optically coupled to a 20-ft light pipe which was terminated by a photoresistor in a voltage divider circuit. The output of the voltage divider was ac coupled into an ECG amplifier (Mennen Greatbatch Model 621), the output of which was fed to one channel of a two-channel strip-chart recorder for a permanent record and to a computing counter (Hewlett-Packard, model #5360A) which constituted a real-time pacemaker rate monitor (Fig. 3). The E-field was monitored by an antenna positioned above and behind the pacemaker test point, and was recorded on the second channel of the strip-chart recorder.

The E-field was controlled by means of a set of attenuators in-line between the transmitter output and radiating device. The calibration was insured by maintaining a constant transmitter output power.

The E-field levels to which the pacemakers were exposed were measured independently by GIT personnel and by personnel from the AF Communication Service (1839 EIGp, Keesler AFB, Biloxi, Miss.). In conjunction with a standard gain dipole for the 450 MHz field and a pyramidal horn for the 3100 MHz field measurements, a power meter (Hewlett-Packard, model 432A) was used. All field measurements were within 0.6 decibel (dB). At 3100 MHz, a cavity-back spiral antenna (Transco, model 9C15100) was used for measuring the attenuation as a function of depth in 0.03 molar saline solution as well as the attenuation of different proposed phantom materials.

TEST RESULTS

Among cardiac pacemakers (of the fixed rate type and the synchronous or R-wave inhibited types), the latter are most likely to be affected by pulsed EM radiation because these use a sensing circuit to control the pacing mode (either demand, synchronous, or fixed-rate) and/or rate. The Cordis models 133C6, 133C7, and 164A were the only synchronous pacemakers tested. The 133C6 and 133C7 have a limiting circuit designed to prevent the pacemaker rate from exceeding a predetermined rate of 140 beats per minute (bpm). The 164A also has a circuit design, which limits the pacemaker synchronous rate, as well as a noise-sensing circuit which causes the pacemaker to revert to a fixed rate when EMI is detected. The Cordis omni models (162C and 164A) were tested at 70 bpm. For R-wave inhibited demand pacemakers, the sensing circuit reverts the pacemaker to a fixed rate when R-wave mocking EMI pulses come in at a rate greater than that for which the manufacturer's design provided. If the EMI rate is less than the designed rate, the pacemaker will interpret it as signals from the normally functioning heart, and will inhibit.




Figure 1. Sample pacemaker test population.

Top row: Stimtech 3821; G.E. A2075A; Medcor 3-70A

Middle row: Amer. Opt. 281003, and 281143;
Biotronik IDP-44

Bottom row: Medtronic 5842, and 5942

(Continued on facing page---)

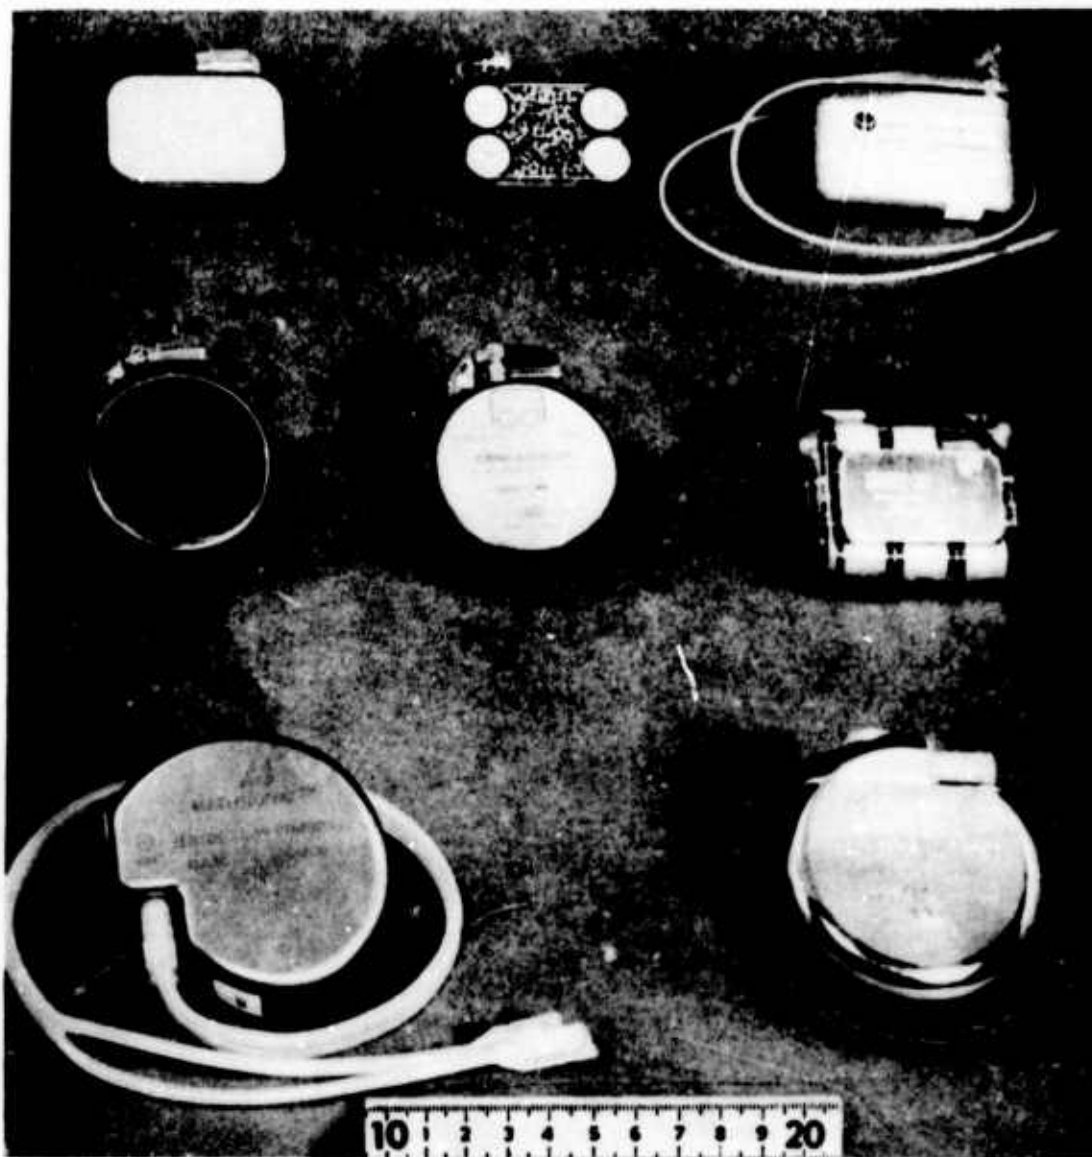

(Cont'd. from facing page--Figure 1. Sample pacemaker test population.)

Top row: Starr-Edwards 8116, and 8114; Pacemaker BD-101

Middle row: Cordis 162C, and 164A; Vitatron MIP-40-RT

Bottom row: Medtronic 5944, and 9000.

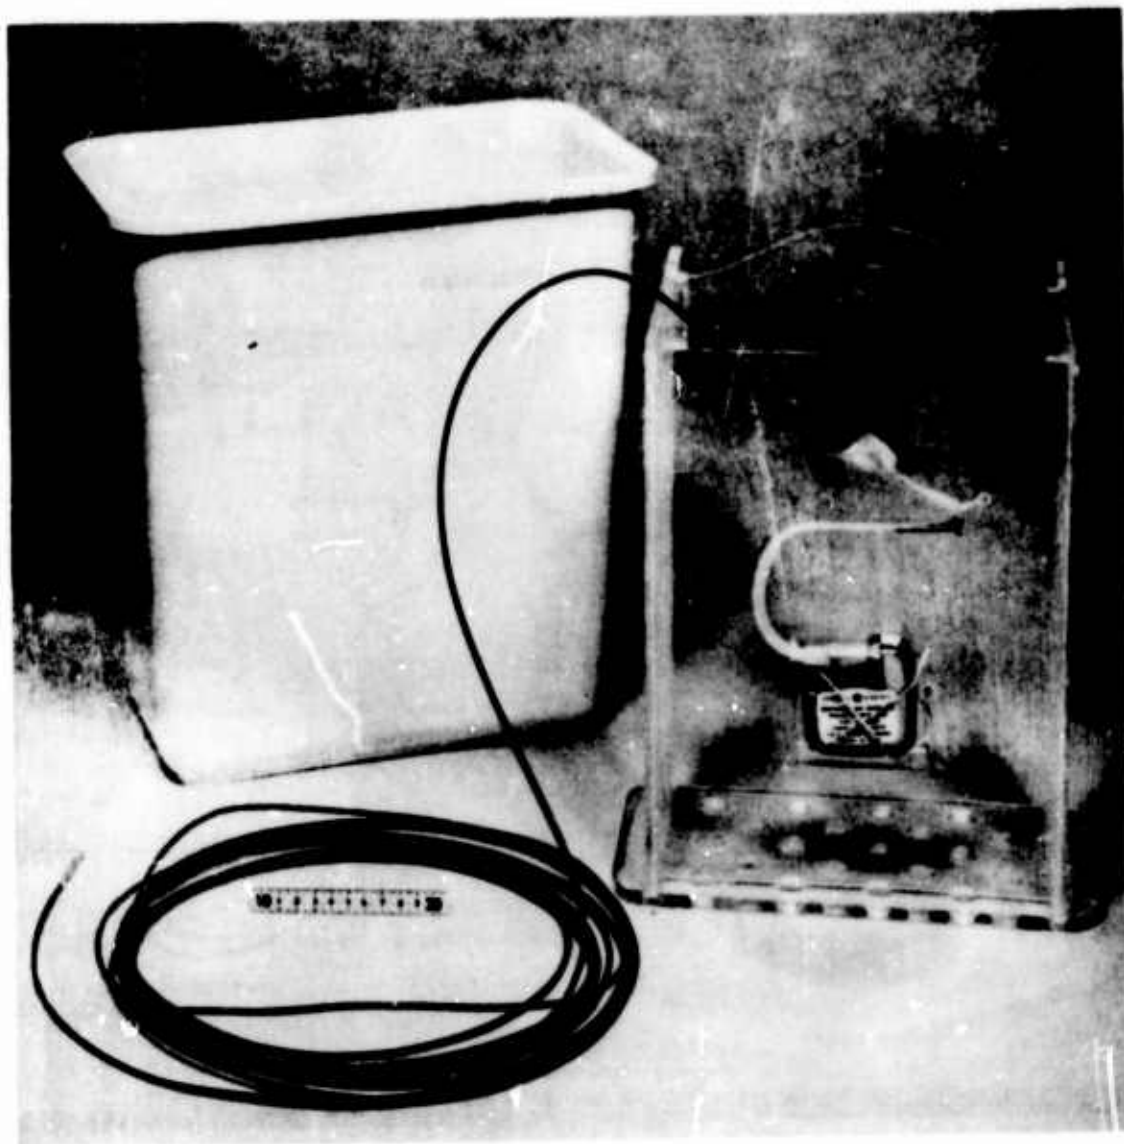


Figure 2. Plexiglas, pacemaker test stand and saline phantom.

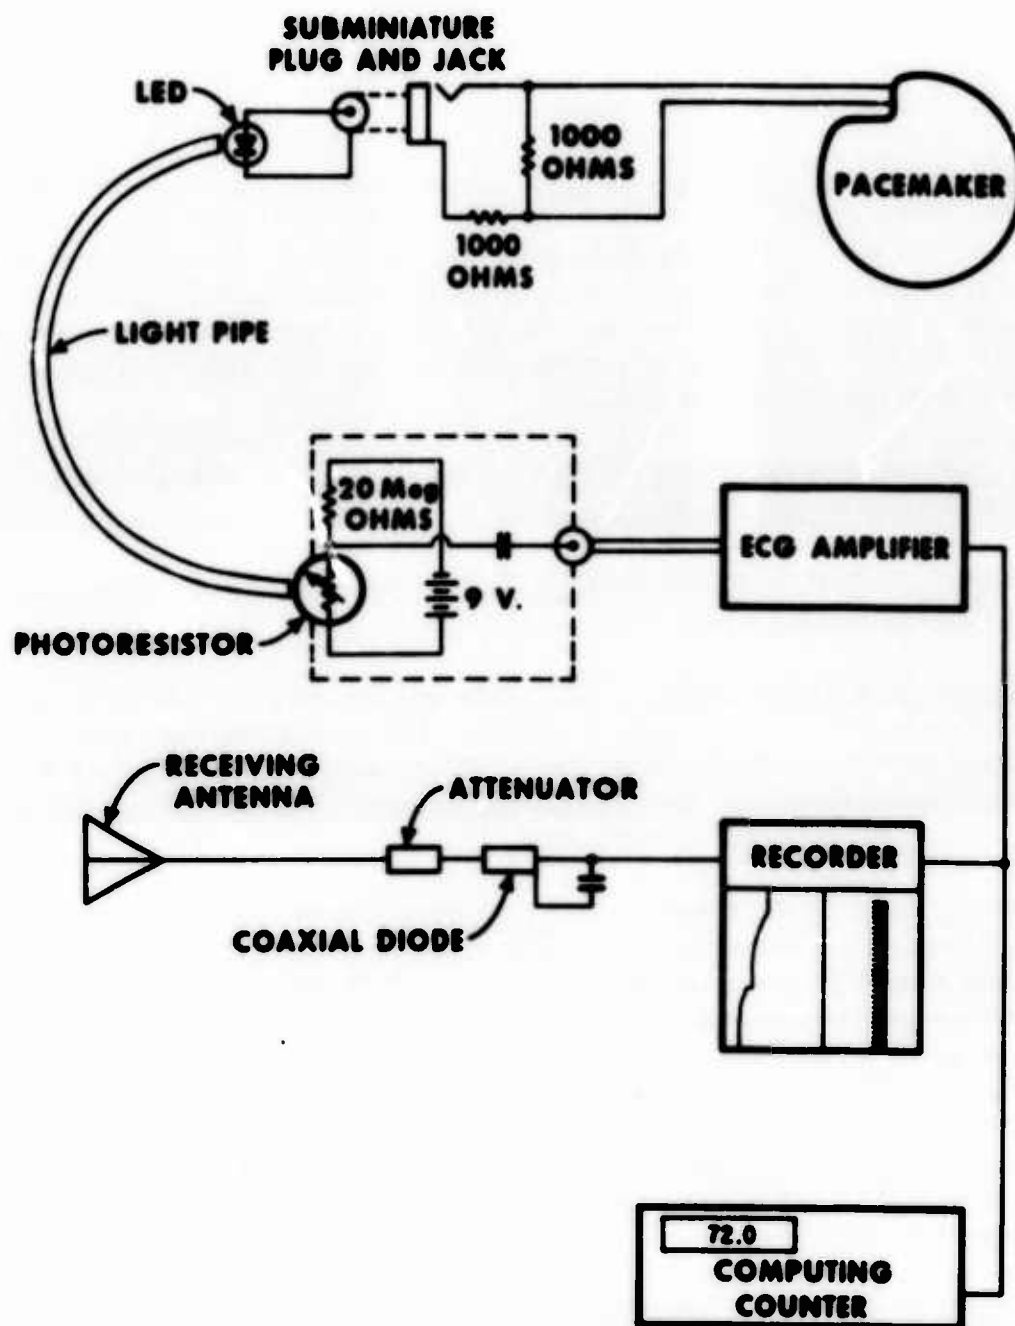


Figure 3. Test equipment for pacemaker response (block diagram).

The following pages of this report present a model-by-model description of the responses of the pacemakers to both 450 and 3100 MHz radiation. The response to PRR is the same at both frequencies, except for thresholds (as noted) and other indicated differences. The thresholds noted are generally those of the most sensitive pacemaker (out of the so-called 'identical' devices tested).

American Optical Model 281003--This model pacemaker reverted to a fixed rate between 65 and 80 bpm for a PRR ≥ 40 pps, and cut off at 20 pps and below when the threshold was reached. The thresholds at 450 MHz were 7 V/m in the free-field configuration and 13 V/m in the simulated-implant configuration. At 3100 MHz, the thresholds were 77 V/m for the free-field configuration and greater than 320 V/m for the simulated-implant configuration.

American Optical Model 281013--This model was affected in a manner similar to the 281003.

American Optical Model 281143 (Predicta)--No effects were observed under all conditions tested.

Biotronik Model IDP-44--This model pacemaker cut off at 2 and 4 pps, and reverted to fixed rate for PRRs ≥ 10 pps at the threshold. The free-field threshold at 450 MHz was 40 V/m, while the simulated-implant threshold was 141 V/m. One pacemaker was not affected at 450 MHz, while none were affected at 3100 MHz.

Cordis Model 133C6 and 133C7 (Atracor)--Since this model pacemaker is atrial synchronous, it has no fixed rate as such, but is designed to maintain a rate below 140 bpm. After the EMI threshold was reached, the pacemaker rate increased with increasing E-field. The pacemaker rate can exceed 120 bpm for some PRR values and/or some E-fields. The EMI threshold at 450 MHz was 17 V/m in the free-field configuration and 85 V/m in the simulated-implant configuration. The maximum rate was 172 bpm at 40 pps. At 3100 MHz, the EMI threshold was 43 V/m in the free-field configuration and 141 V/m in the simulated-implant configuration.

Cordis Model 143E7 (Stanicor)--This model pacemaker reverted to fixed-rate mode (70-85 bpm) for PRRs of 20 pps and greater when the E-field threshold was reached. The pacemaker cut off at 10 pps at the threshold. The threshold at 450 MHz was 10 V/m in the free-field configuration and 15 V/m in the simulated-implant configuration. At 3100 MHz, the threshold was 36 V/m for the free-field configuration and 141 V/m for the simulated-implant configuration.

Cordis Model 162C (Omni-Stanikor)--This model pacemaker reverted to a fixed-rate mode (equal to the demand rate) at PRRs above 20 pps at the threshold, and cut off at 10 pps and below. At 450 MHz, the threshold was 6 V/m for the free-field configuration, and 8 V/m for the simulated-implant configuration. At 3100 MHz, the threshold was 229 V/m for the free-field configuration, and 302 V/m in the simulated-implant configuration.

Cordis Model 164A (Omni-Atrikor)--This pacemaker is an atrial synchronous pacemaker which, unlike models 133C6 and 133C7, reverts to a fixed rate (equal to the demand rate) when interference becomes severe. The threshold level was somewhat dependent on PRR (decreasing with decreasing PRR) at 3100 MHz. The threshold at 450 MHz was 4 V/m for free-field configuration and 13 V/m for the simulated-implant configuration. At 3100 MHz, the threshold was 116 V/m for the free-field configuration and 320 V/m in the simulated-implant configuration for PRRs below 100 pps--while the pacemaker was not affected between 100 pps and 400 pps.

General Electric Model A2072D--This model pacemaker exhibited a rate increase with increasing E-field. After the E-field was increased above the threshold level, the pacemaker would cut off at 2 pps and revert to its fixed rate mode at 10 pps and above. The RF interference apparently affected the timing circuitry, causing both the demand and fixed rates to increase. The threshold at 450 MHz was 8 V/m in the free-field configuration and 29 V/m in the simulated-implant configuration. The thresholds at 3100 MHz were 77 V/m in the free-field configuration and >320 V/m in the simulated-implant configuration.

General Electric Model A2075A (Sentry)--At 450 MHz, the pacemaker cut off at the threshold at 2 pps, and increased in rate at the threshold at 10 pps and above. The threshold was 10 V/m free-field and 23 V/m in the simulated-implant configuration. This model was not seriously affected in the free-field configuration at 3100 MHz (demand rate increased to 86 bpm at 302 V/m), and was unaffected for simulated-implant configuration at this frequency.

Medcor Model 3-70A--At 450 MHz, this pacemaker cut off at 2 pps at the threshold. At 10 pps and above, it reverted to fixed rate, then cut off at a high E-field. The free-field threshold was 13 V/m, and the simulated-implant was 29 V/m with a high level cutoff at 141 V/m. At 3100 MHz, this model exhibited an increasing fixed rate with increasing E-field above the threshold (60-102 V/m). At 320 V/m, the rates were generally above 146 bpm. In the phantom, the rate did not exceed 72 bpm.

Medtronic Model 5842--At the threshold, this model reverted to a fixed rate of operation (45-55 bpm) at 100 pps and above, and cut off at 20 pps and below. At 40 pps, pacemakers of this type either cut off or went into fixed rate at the threshold. At 450 MHz, the pacemakers generally tracked the PRR at a high E-field level (114 V/m shielded). The thresholds at 450 MHz were 2 - 5 V/m for the free-field configuration, and 12 V/m for the simulated-implant configuration. At 3100 MHz, the free-field thresholds ranged from 40 - 100 V/m, and the simulated-implant threshold was >320 V/m.

Medtronic Model 5942--This model reacted in a manner similar to model 5842, except that no tracking was observed. The 450 MHz thresholds were 2 V/m free-field and 12 V/m for the simulated-implant configuration. The thresholds at 3100 MHz were 88 - >320 V/m for the free-field configuration, and greater than 320 V/m for the simulated-implant configuration.

Medtronic Model 5943--This pacemaker cut off for PRRs of 20 pps and below, and went into fixed rate (45 - 66 bpm) at PRRs of 40 pps and above for E-fields above the threshold. At 450 MHz, the pacemaker tracked the PRR at 114 V/m in the free-field configuration. The free-field threshold at 450 MHz was 6 V/m; and 19 V/m, in simulated-implant configuration. At 3100 MHz, the free-field threshold was 77 V/m; and >320 V/m, in simulated-implant.

Medtronic Model 5944--This model reverted to a fixed rate mode (44 - 52 bpm) at PRRs of 20 pps and above, and cut off for 10 pps and below. At 450 MHz, the free-field threshold was 6 V/m and the simulated-implant threshold was 19 V/m. At 3100 MHz, the free-field threshold ranged from 129 to 302 V/m and the simulated-implant threshold was greater than 320 V/m.

Medtronic Model 5950--No effects were observed under conditions tested. [Note: This model was a preproduction prototype pacemaker design.]

Medtronic Model 5951--No effects were observed under conditions tested. [Note: This model was a preproduction prototype pacemaker design.]

Medtronic Model 9000 (Nuclear)--This model pacemaker cut off at the threshold at 20, 10, and 2 pps. At 40 pps and above, it reverted to fixed rate at the threshold. The free-field threshold at 450 MHz was 1 V/m, and the simulated-implant threshold was 7 V/m. At 3100 MHz,

the free-field threshold was 52 V/m for one pacemaker (the other two were unaffected up to 320 V/m). The pacemaker was not affected in the simulated-implant configuration up to 320 V/m at 3100 MHz.

Pacesetter Model BD-101 (Rechargeable)--No effects were observed under conditions tested.

Starr-Edwards Model 8114--This model pacemaker cut off at the threshold below 10 pps. At PRRs of 20 pps and above, the pacemaker reverted to fixed rate at the threshold. The E-field threshold at 450 MHz was 33 V/m free-field, and 23 V/m in the simulated-implant configuration. This relationship between free-field and simulated-implant thresholds was not reasonable and was, therefore, thought to be due to variability in the pacemaker EMI response. At 3100 MHz, the free-field threshold was 60 V/m, and the simulated-implant threshold was 204 V/m.

Starr-Edwards Model 8116--No effects were observed under conditions tested.

Stimtech Model 3821--This model showed a great deal of variability in response from pacemaker to pacemaker. At 450 MHz, this model pacemaker cut off at the threshold at 2 pps. At 10 pps, the pacemaker would either cut off or revert to a fixed-rate mode at the threshold. At 20 pps, the pacemaker would revert to fixed rate at the threshold. One pacemaker of this model was unaffected at this frequency. The thresholds were 46 V/m in the free-field configuration and 107 V/m in the simulated-implant configuration. At 3100 MHz, one pacemaker was not affected to the limits of the tests. Another was unaffected from 400 to 100 pps, but cut off at 320 V/m at PRRs from 10 to 40 pps. A third cut off at PRRs of 40 pps and below at 302 V/m, but went to fixed rate at 100 pps and above. The oldest pacemaker of this model reverted to fixed rate at a threshold of 158 V/m in the free-field configuration for PRRs between 400 pps and 100 pps. From 40 to 10 pps, this pacemaker cut off at the threshold. This model was not affected in the simulated-implant configuration at 3100 MHz.

Vitatron Model MIP-40-RT--At 450 MHz, this model cut off at the threshold at 2 pps and 10 pps. At 20 pps and 40 pps, this model reverted to fixed rate at the threshold, but had a cut-off threshold at 243 V/m in the simulated-implant configuration. The free-field configuration threshold was 40 V/m, and the simulated-implant configuration threshold was 93 V/m. At 3100 MHz, as the E-field was increased above the threshold, the pacing rate (for all PRRs) increased to between 270 bpm

and approximately 2000 bpm. The threshold was 178 V/m in the free-field configuration, and the rate exceeded 120 bpm near 229 V/m. This model was unaffected in the simulated-implant configuration at 3100 MHz.

The pacemaker free-field and simulated-implant threshold data for 450 MHz and 3100 MHz are presented in Tables 2 - 4. The double entries indicate the insignificant and significant interference thresholds for those pacers which demonstrated both for the same PRR. A significant effect is defined as a pacemaker rate which falls below 50 bpm or exceeds 120 bpm as a direct result of RF radiation interference.

Measured with a cavity-back spiral antenna at 3100 MHz was the attenuation of: two different thicknesses of Plexiglas (1/8 in. and 1/4 in.); 1.5 in. of ethafoam coated on the inside with epoxy waterproofing; and 1.5 mm of polyethylene. These materials were considered for use as phantoms. The ethafoam and polyethylene contributed no measurable attenuation. The attenuation due to 1/8 in. and 1/4 in. of Plexiglas was 0 dB and 0.2 dB, respectively.

The attenuation for several depths of 0.03 molar saline solution was also investigated with the cavity-back spiral antenna at 3100 MHz. The results are presented in Figure 4. Table 5 contains attenuation factors derived from the free-field and simulated-implant pacemaker threshold data for 450 MHz and 3100 MHz. The variability is not believed to be indicative of anything except a seemingly inherent spread in EMI thresholds. Reproducibility of threshold data on any one pacer can vary by 6 dB. To eliminate as many variables as possible, however, the pacemakers used for the attenuation study remained on the Plexiglas plate and, as much as possible, undisturbed after the free-field test while being transferred to the phantom for the simulated-implant test. The only PRRs used in the acquisition of these data were 2 pps at 450 MHz, and 7 pps at 3100 MHz. Based on these data and the antenna measurements, the attenuation afforded by implantation at 3100 MHz is expected to be approximately 5 (14 dB). The average of the 450 MHz attenuation data gives an estimated implantation shielding factor of approximately 3 (10 dB).

The effect of pulse width and repetition rate on the pacemaker EMI threshold was investigated. At 450 MHz, thresholds were measured for pulse widths between 1 μ sec and 1 msec at 2 pps and 50 pps (Fig. 5). The curves are parabolic least square fits to the data normalized to the 1 msec points. Each curve generally represents data from more than one pacemaker, i. e., the data from the G.E. model A2075A and Medcor model 3-70A are represented by one curve, as are: the A.O. models 281003 and 281013; the Stimtech model 3821 and Vitatron model MIP-40-RT;

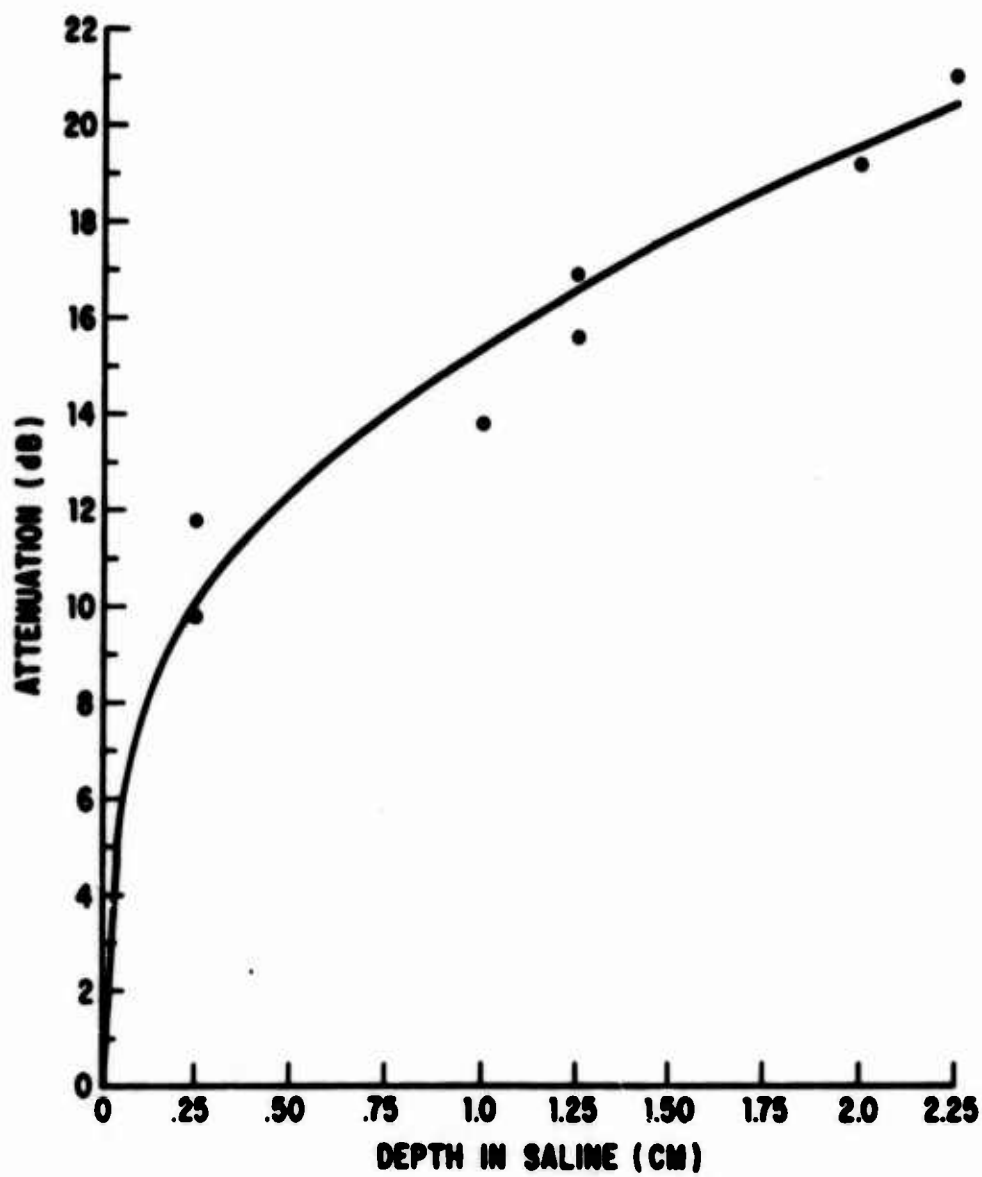


Figure 4. Attenuation of 3100 MHz EMR by saline solution as measured by a cavity-back spiral antenna.

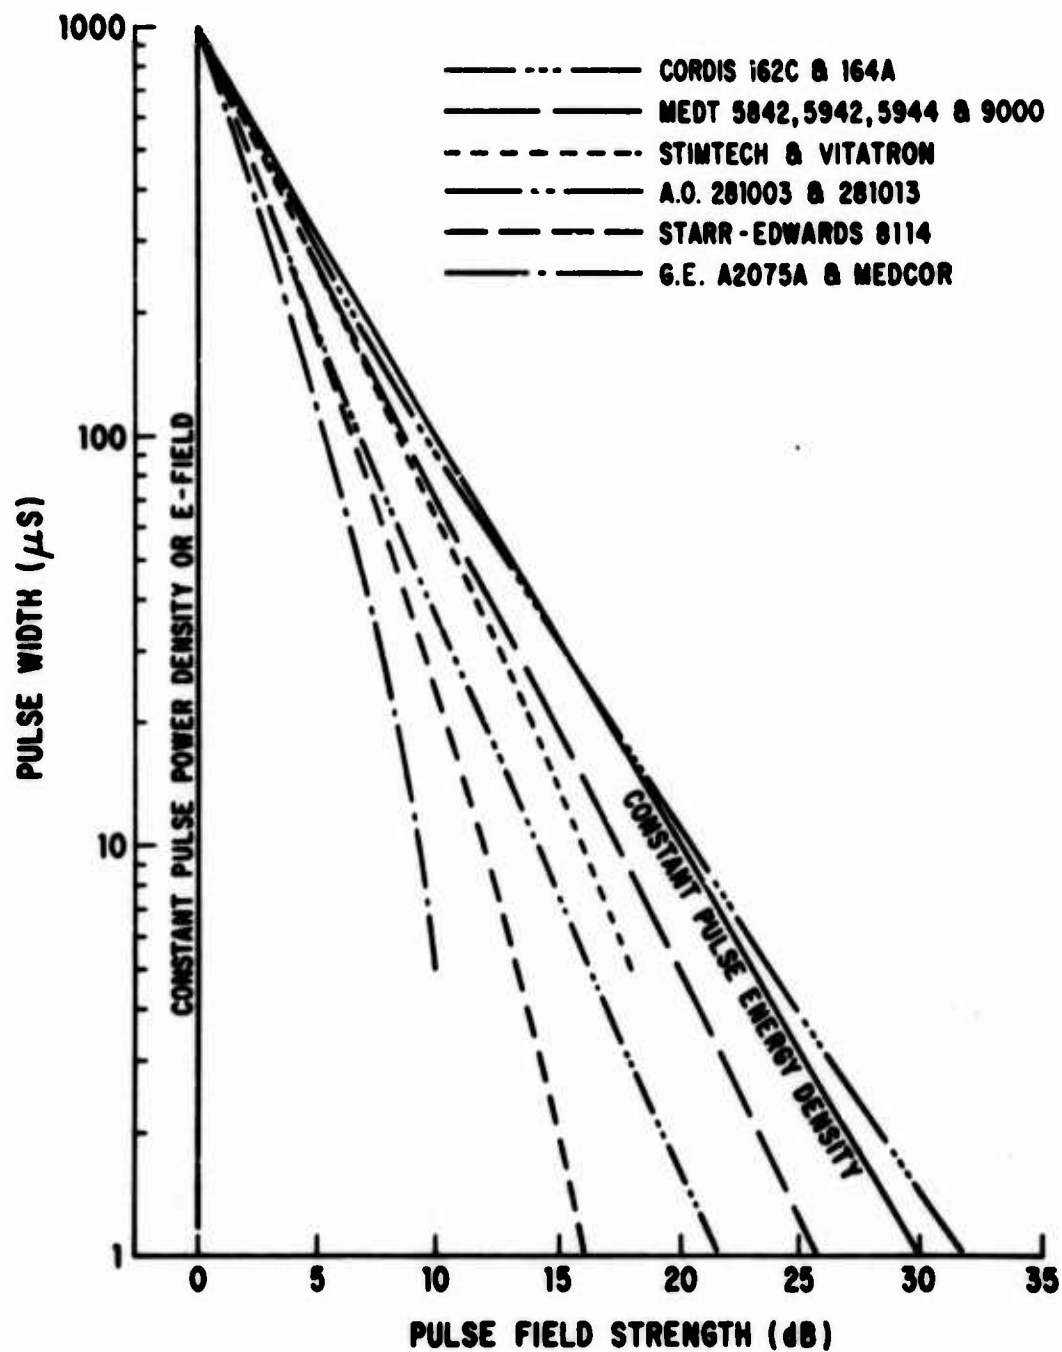


Figure 5. Relative 450 MHz EMI thresholds vs. pulse width for various pacemakers.

Medtronic models 5842, 5942, 5944, and 9000; and Cordis models 162C and 164A. One curve is based only on Starr-Edwards model 8114 data. There was no significant difference between the 2 pps and 50 pps data. The constant pulse energy density curve shows the relation between pulse width and the product of power density during the pulse and pulse width (energy density). These data demonstrate that the E-field threshold is inversely proportional to pulse width.

For 3100 MHz, a pulse-width range of 10 - 120 μ sec for 7 pps and 400 pps was investigated (Fig. 6). The data were normalized to the 120 μ sec points. Data from the Cordis models 133C7 and 164A are represented by one curve; from the A.O. model 281003, by another curve; from the Medtronic models 5842, 5942, 5944, and 9000 and the G.E. model A2072D (7 pps), by a third curve; and from the G.E. model A2072D (400 pps), by another curve. The G.E. model A2072D was the only pacemaker which demonstrated a significant difference in relationship between threshold and pulse width for different PRRs. The 3100 MHz data also demonstrated that the E-field threshold is inversely proportional to pulse width.

A cursory evaluation of the effect of leads was also made. For instance, the data presented for the Medtronic and A.O. pacemakers were taken using the Medtronic model 6914 epicardial leads. Switching to the model 5818 endocardial leads appears to raise the E-field thresholds somewhat for the Medtronic pacemakers, while the A.O. pacemakers thresholds remained the same for both leads.

CONCLUSIONS

These tests indicate an improvement in EMI characteristics of the more recent models of cardiac pacemakers (A.O. model 281143, Cordis models 162C and 164A, G.E. model A2075A, Medtronic model 5944, Pacemaker model BD-101, and Starr-Edwards model 8116) over their predecessors. This improvement reflects the abilities of manufacturers to solve the potential interference problems.

The data show that shielding factors of approximately 3 (10 dB) at 450 MHz and approximately 5 (14 dB) at 3100 MHz can be expected for EMI thresholds from the free-field to the implanted situation. These tests also showed that the EMI thresholds are inversely proportional to pulse width.

The comparison of the Medtronic leads, models 5818 and 6914, indicated that at 450 MHz the model 5818 might afford a slight reduction

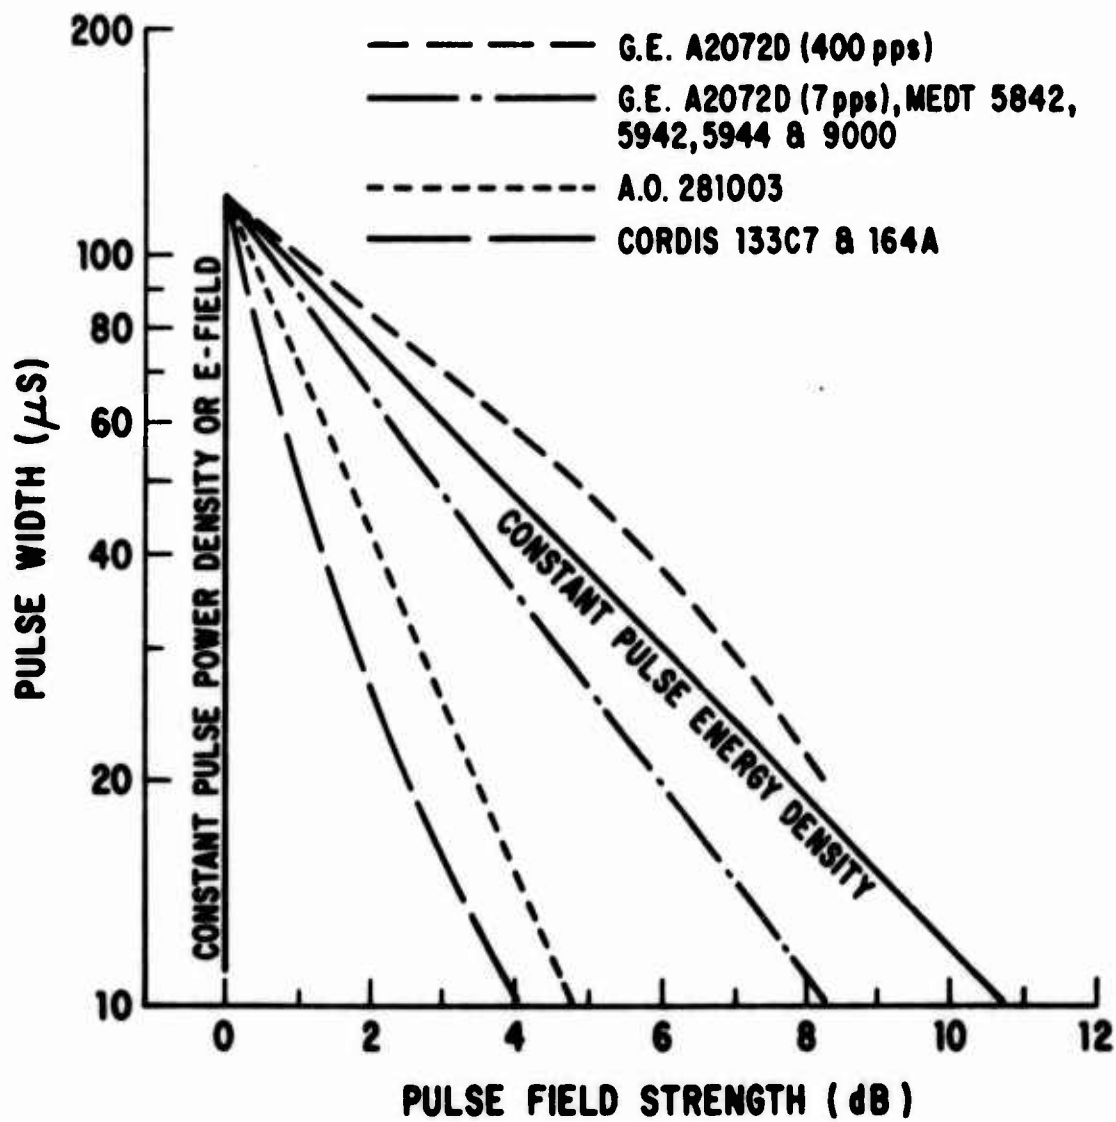


Figure 6. Relative 3100 MHz EMI thresholds vs. pulse width for various pacemakers.

in EMI sensitivity over the model 6914 (~ 5 dB). However, no difference was noted at 3100 MHz.

At 450 MHz, three models (the A. O. model 281143, Pacemaker model BD-101 and Starr-Edwards model 8116) were not affected at 200 V/m in the simulated-implant tests. Three other models (the Biotronik model IDP-44, Cordis model 133C7, and G. E. model A2072D) demonstrated no serious effects at 200 V/m for PRRs greater than 10 pps. All other pacemakers tested were significantly affected at E-field values below 200 V/m and PRRs greater than 10 pps. At the 3100 MHz frequency using 120 μ sec pulse width, none of the pacemakers tested under simulated-implant conditions were seriously affected at an E-field level of 200 V/m.

Subsequent tests to higher E-field levels would probably serve to establish the relative EMI thresholds for those pacemakers not affected at the limit of these tests.

BIBLIOGRAPHY

1. Crystal, R. G., J. A. Kastor, and R. W. Desantis. Inhibition of discharge of an external demand pacemaker by an electric razor. *Am J Cardiol* 27:695-697 (1971).
2. D'Cunha, G. F., et al. Syncopal attacks arising from erratic demand pacemaker function in the vicinity of a television transmitter. *Am J Cardiol* 31:789-791 (1973).
3. Escher, J. W., B. Parker, and S. Furman. Influence of alternating magnetic fields on triggered pacemakers. Supplement II, to *Circulation* XLIV:162 (1971).
4. Furman, S., et al. The influence of electromagnetic environment on the performance of artificial cardiac pacemakers. *Ann Thorac Surg* 6:90 (1968).
5. Hurt, W. D. Cardiac pacemaker electromagnetic interference (3050 MHz). SAM-TR-72-36, Dec. 1972.
6. Hurt, W. D. Effects of electromagnetic interference (2450 MHz) on cardiac pacemakers. SAM-TR-73-40, Dec. 1973.

7. King, G. R., et al. Effect of microwave oven on implanted cardiac pacemaker. JAMA 212:1213 (1970).
8. Kohler, F. P., and C. C. MacKinney. Cardiac pacemakers in electrosurgery. JAMA 193:855 (1965).
9. Meibon, J., and J. Anderson. Inhibition of demand pacemaker by leakage current from electrocardiographic recorder. Brit Heart J 33:326 (1971).
10. Michaelson, S. M., and A. J. Moss. Environmental influences on implanted cardiac pacemakers. JAMA 216:2006 (1971).
11. Mitchell, J. C., et al. Electromagnetic compatibility of cardiac pacemakers. Presented at the 1972 IEEE International Electromagnetic Compatibility Symposium, Arlington Heights, Ill.; and published in the Symposium Record, July 1972.
12. Mitchell, J. C., et al. Empirical studies of cardiac pacemaker interference. Aerosp Med 189 - 195 (Feb. 1974).
13. Mitchell, J. C., W. D. Hurt, and T. O. Steiner. Special problems of general public exposure to RF radiation. Presented at the Aerospace Medical Association Meeting, Washington, D. C., May 1974.
14. Mitchell, J. C., W. D. Hurt, and T. O. Steiner. EMC design effectiveness in electronic medical prosthetic devices. Proceedings of the Seventh Rochester International Conference on Environmental Toxicity, Fundamental and Applied Aspects of Non-Ionizing Radiation, 5 - 7 June 1974, University of Rochester, New York.
15. Parker, B., S. Furman, and D. Escher. Input signals to pacemakers in a hospital environment. Ann NY Acad Sci 167:823 (1969).
16. Pickers, B. A., and M. J. Goldberg. Inhibition of a demand pacemaker and interference with monitoring equipment by radiofrequency transmissions. Br Med J 2:504 (1969).
17. Rustan, P. L., W. D. Hurt, and J. C. Mitchell. Microwave oven interference with cardiac pacemakers. Med Instrum 7(3):185-188 (May - Aug. 1973).

18. Sanchez, S. A. When you transmit, you can turn off a pacemaker. QST 53 (Mar. 1973).
19. Smyth, N. P. D., et al. The pacemaker patient and the electromagnetic environment. JAMA 227(12):1412 (1974).
20. Sowton, E., K. Gray, and T. Preston. Electrical interference in noncompetitive pacemakers. Br Heart J 32:626 (1970).
21. Walter, W. H., III, et al. Cardiac pulse generators and electromagnetic interference. JAMA 224:1628-1631 (1973).

TABLE 1. CARDIAC PACEMAKER NOMENCLATURE AND NUMBER OF UNITS TESTED

Manufacturer	Model No.	No. of units tested	Nomenclature
American Optical	281003	3	Bipolar Cardio-Care Demand Pacemaker (R-wave Inhibited)
	281013	2	Monopolar Cardio-Care Demand Pacemaker (R-wave Inhibited)
	281143	3	Bipolar Predicta Demand Pacemaker (R-wave Inhibited)
Biotronik	IDP-44	4	R-wave Inhibited Unipolar Demand Pacemaker
Cordis	13306	1	P-wave Synchronous Cardiac Pacemaker
	13307	2	P-wave Synchronous Cardiac Pacemaker
	143E7	1	R-wave Inhibited Standby Cardiac Pacemaker
	162C	3	Programmable R-wave Inhibited Standby Cardiac Pacemaker
	164A	3	Programmable P-wave Synchronous Cardiac Pacemaker
General Electric	A20720	2	Standby (Ventricular Inhibited) Pulse Generator
	A2075A	3	Sentry Ventricular Inhibited Pulse Generator
Medcor	3-70A	3	Demand (R-inhibited) Pacemaker
Medtronic	5842	10	Ventricular Inhibited Bipolar Pulse Generator
	5942	9	Ventricular Inhibited Bipolar Pulse Generator
	5943	1	Ventricular Inhibited Unipolar Pulse Generator

TABLE 1 (Cont'd.)

Manufacturer	Model No.	No. of units tested	Nomenclature
Medtronic	5944	3	Ventricular Inhibited Bipolar Pulse Generator
	5950 ^a	1	Ventricular Inhibited Bipolar Pulse Generator
	5951 ^a	1	Ventricular Inhibited Unipolar Pulse Generator
	9000	3	Ventricular Inhibited Bipolar Pulse Generator
Pacesetter	BD-101	3	Rechargeable Demand Pacemaker
Starr-Edwards	8114	1	Ventricular Tracking Standby Pulse Generator
	8116	3	Ventricular Tracking Standby Pulse Generator
Stimtech	3821	4	R-wave Inhibited Demand Pacemaker
Vitatron	MIP-40-RT	3	On Demand Unipolar R-wave Blocked Pacemaker

^a Pre-production prototype pacemaker designs.

TABLE 2. PACE-MAKER EMI THRESHOLDS

Manufacturer	Model No.	Serial No.	Threshold values, 450 MHz									
			Free-field			Pulse repetition rate (pps)						
			2	50		Simulated-implant						
			V/m(bpm)	V/m(bpm)		2	10	20	40	50		
American Optical	281003	11591	7(0)			13(0)	15(0)	15(0)	15(71) ^a 243(0) ^a			
	281013	42545	6(0)	6(71)		26(0)	26(0)	26(0)	26(71)			
	281143	27322 27560 27312	>292 ^b			>292 >292 >292			>292 >292 >292			
	10P-44	61034 61035 61443	40(0)			141(0) 178(0) >292	141(82) 178(82) >292	141(82)				
Cordis	133C7	2352	17(122)			35(122)			35(75) 141(172)			
	143E7	11575	10(0)			15(0)	15(0)	15(76) 243(0)	15(74)			
162C		342 4246 5296	8(0) 10(0)	6(69)		8(0) 15(0)	9(0)	9(68) 15(69) 12(67)	15(69) 12(67)			
	164A	118 284 286	4(83)	4(69)		21(126) 13(107) 85(124)	17(69) 13(69) 85(69)	17(69)				

^a Throughout Table 2, double entries indicate the existence of both insignificant and significant thresholds.^b Such entries indicate that pacemaker not affected to limit of test.

TABLE 2 (Cont'd)

Manufacturer	Model No.	Serial No.	Threshold values, 450 MHz									
			Free-field					Simulated-implant				
			2	50	2	10	20	40	50	Pulse repetition rate (pps)		
			V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)			
General Electric	A20720	891930	8(0)		29(0)	29(71)						
						207(122)						
		937015	10(0)	15(78)	51(0)	51(78)						
		937147			23(0)	141(125)						
Medcor	3-70A	937164			36(0)	141(125)						
						36(67)						
		2015	13(0)	17(69)	29(0)	33(69)	33(71)	33(69)	33(69)			
		3753			33(0)	141(0)	141(0)	141(0)	141(0)			
Medtronic	5842	3754			58(0)	141(0)						
						58(71)						
		3700123	5(0)	3(0)	15(0)							
		3700154										
	5942	3700158			13(0)							
		37004597	3(0)	2(51)	12(0)							
		3700660										
		3729624										

TABLE 2 (Cont'd)

Manufacturer	Model No.	Serial No.	Threshold values, 450 Mhz									
			Free-field			Pulse repetition rate (pps)						
			2 V/m(bpm)	50 V/m(bpm)		2 V/m(bpm)	10 V/m(bpm)	20 V/m(bpm)	40 V/m(bpm)	50 V/m(bpm)		
Medtronic	5943	1L1282N	6(0)			23(0)		19(0)	19(47)			
	5944	3G20824 3G20877 3G20891	6(0)	5(43)		26(0)	19(0) 26(0) 33(0)	19(43) 26(42) 33(42)	19(43)			
	5950	3XX2022 <u>£</u>	>292			>292			>292			
	5951	3XX2025 <u>£</u>	>292			>292			>292			
	9000	3R00001 3R00003 3R00004	1(0)	.7(41)		21(0)	10(0) 10(0) 10(0)	17(0) 17(0) 7(0)	21(45) 17(37) 7(48)			
Pacesetter	BD-101	1196KC 13951D 1404ND	>292			>292 >292 >292			>292 >292 >292			
	8114	4399	33(0)	33(65)		23(0)	26(65)	26(65)				
	8116	ELX15514 ELX15518 ELX15520	>292			>292 >292 >292			>292 >292 >292			

£ Pre-production prototype pacemaker designs.

TABLE 2 (Cont'd)

Manufacturer	Model No.	Serial No.	Threshold values, 450 Hz									
			Free-field		Pulse repetition rate (pps)							
			2	50	Simulated-impedant							
			V/m(bnm)	V/m(bnm)	2	10	20	40	50			
Stimtech	3821	H38030	46(0)	46(107)	107(0)	114(0)	114(107)					
		J38015			>292		>292					
		J38016			114(0)	114(67)						
Vitatron	HIP-40-RT	0505	40(0)	141(72)	141(0)	141(74)	207(81)	141(72)				
		0507			93(0)	243(0)	243(0)	243(0)				
					93(0)	92(70)	85(69)	114(70)				
		5146			93(0)	243(0)	114(72)	243(0)				
						107(0)	243(0)					

TABLE 3. FREE-FIELD PACEMAKER EMI THRESHOLDS

			Threshold values, 3100 MHz Pulse repetition rate (prs)						
Manufacturer	Model no.	Serial No.	7 V/m(bpm)	10 V/m(hpm)	20 V/m(hpm)	40 V/m(bpm)	100 V/m(bpm)	200 V/m(bpm)	400 V/m(bpm)
American Optical	281003	11591	159(0)	141(0)	141(0)	88(70)	129(75)	129(75)	141(72)
		A6124		71(0)	71(0)	88(69)	77(75)	71(77)	77(75)
		AG995		229(0)	129(71) ^a 229(0) ^a	129(71)	141(72)	141(73)	141(74)
	281013	A2202		77(0)	71(0)	33(71)	57(72)	57(74)	52(72)
		A2545	77(0)	52(0)	57(0)	64(70)	29(75)	43(77)	52(76)
						282(0)			
Biotronik	281143	27322		>320 ^b	>320		>320		>320
		27560		>320	>320		>320		>320
		27312		>320	>320		>320		>320
		55038		>320	>320	>320	>320	>320	>320
		61034		>320	>320	>320	>320	>320	>320
	IDP-44	61035		>320	>320	>320	>320	>320	>320
		61443		>320	>320	>320	>320	>320	>320
Cordis	13306 13307	2210		204(86)	116(62)	116(64)	102(64)	64(64)	88(63)
		2352	36(105)	43(118)	43(117)	43(104)	43(83)	43(73)	102(87)
		2958		71(117) 266(123)	71(101) 229(148)	71(103) 248(159)	71(80)	204(126)	71(75) 229(124)
	143E7	11575		40(0)	40(76)	40(76)	36(76)	40(76)	43(76)

^a Throughout Table 3, double entries indicate the existence of both insignificant and significant thresholds.^b Such entries indicate that pacemaker not affected to limit of test.

TABLE 3 (Cont'd)

Manufacturer	Model No.	Serial No.	Threshold values, 3100 MHz									
			Pulse repetition rate (pps)									
			7	10	20	40	100	200	400			
			V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)			
Cordis	162C	342	302(0)	302(69)	302(69)	302(69)	320(69)	320	>320			
		4246	>320	>320	>320	>320	>320	>320	>320			
		529C	229(14)	248(54)	248(57)	248(57)	266(67)	302(67)	302			
	164A	118	159(69)	159(69)	159(69)	159(69)	178(69)	178(69)	204(69)			
		284	141(70)	141(70)	141(70)	141(70)	141(70)	141(70)	178(70)			
		286	116(70)	116(70)	116(70)	129(70)	129(70)	129(70)	141(70)			
General Electric	A2072D	888012	204(88)	229(93)	229(93)	266(105)	266(104)	248(100)	255(100)			
		891930	77(71)	102(71)	102(72)	116(72)	159(77)	159(77)	141(75)			
			248(201)	248(205)	248(205)	248(217)	266(240)	248(158)	266(153)			
	A2075A	937015	>320	>320	>320	>320	>320	>320	>320			
		937147	>320	>320	>320	>320	>320	>320	>320			
		937164	302(86)	>320	>320	320(76)	>320	>320	>320			
Medcor	3-70A	2015	77(70)	77(70)	77(70)	77(71)	77(72)	77(73)	77(74)			
		3753	60(71)	60(71)	60(71)	248(121)	266(126)	266(121)	266(126)			
		3754	302(147)	266(133)	266(133)	266(132)	266(130)	266(129)	266(123)			
Medtronic	5842		102(71)	102(71)	102(71)	102(71)	102(71)	102(72)	102(72)			
			266(150)	266(151)	266(151)	266(142)	266(138)	266(129)	282(150)			
		03851KK	47(0)	43(0)	43(0)	43(52)	43(53)	43(54)	43(54)			
		16669KK	102(0)	102(0)	102(0)	204(0)	178(0)	159(0)	159(0)			
						102(53)	102(54)	102(54)	89(52)			
						229(0)	229(0)	229(0)	204(0)			

TABLE 3 (Cont'd)

Manufacturer	Model No.	Serial No.	Threshold values, 3100 MHz Pulse repetition rate (pps)							
			7 V/m(bpm)	10 V/m(bpm)	20 V/m(bpm)	40 V/m(bpm)	100 V/m(bpm)	200 V/m(bpm)	400 V/m(bpm)	
Medtronic	5842	2100520		47(0)	40(0)	40(47)	40(49)	40(53)	40(52)	
		2100522		57(0)	52(0)	52(45) 204(0)	52(47)	52(49)	52(49)	
		2100815		47(0)	43(0)	43(48) 302(0) 71(44)	43(48) 266(0) 71(47)	43(49) 248(0) 71(49)	43(50) 248(0) 77(52)	
		2100981		71(0)	71(0)	229(0)	36(53)	40(59)	36(55)	
		2102202		36(0)	36(0)	36(0)	52(50)	52(51)	52(50)	
		3100123	71(0)	52(0)	52(0)	52(0)	52(51)	52(54)	52(53)	
		3100154		52(0)	52(0)	33(32)	33(54)	33(54)	33(54)	
		3100158	33(0)	33(0)	33(0)	129(0)				
	5942	1K19384		229(0)	229(0)	229(55)	229(55)	229(55)	229(55)	
		1K33732		141(0)	141(0)	141(55)	141(55)	141(55)	141(55)	
		1K39359		302(0)	302(0)	282(47)	282(47)	302(50)	302(58)	
		2K18159		159(0)	159(0)	159(0)	159(52)	159(52)	159(52)	
		3K04222		>320	>320	>320	>320	>320	>320	
		3K04597	159(0)	88(0)	88(0)	88(0)	88(49)	88(49)	88(49)	
		3K18607		>320	>320	>320	>320	>320	>320	
		3K20660	159(0)	159(0)	159(0)	159(0)	141(48)	141(48)	141(48)	
		3K29624		282(0)	282(0)	302(0)	302(49)	282(49)	242(49)	
	5943	1L1282N	77(0)	102(0)	88(0)	88(47)	88(47)	88(47)	60(48)	

TABLE 3 (Cont'd)

Manufacturer	Model No.	Serial No.	Threshold values, 3100 MHz							
			Pulse repetition rate (pps)							
			7	10	20	40	100	200	400	
			V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	
Medtronic	5944	3C20824	248(0)	266(0)	266(48)	266(48)	266(48)	266(48)	266(48)	
		3C20877	129(0)	178(0)	178(50)	178(50)	178(50)	178(50)	178(50)	
		3C20881	302(0)	302(0)	302(46)	302(46)	302(46)	302(46)	302(46)	
5950	3XX2022	3XX2022	>320	>320	>320	>320	>320	>320	>320	
		3XX2025	>320	>320	>320	>320	>320	>320	>320	
9000	3R00001	3R00001	71(0)	57(0)	57(0)	52(44)	57(50)	57(50)	57(51)	
		3R00003	>320	>320	>320	>320	>320	>320	>320	
		3R00004	>320	>320	>320	>320	>320	>320	>320	
Pacesetter	BD-101	1196KC	>320	>320	>320	>320	>320	>320	>320	
		1395ND	>320	>320	>320	>320	>320	>320	>320	
		1404ND	>320	>320	>320	>320	>320	>320	>320	
Starr-Edwards	8114	4399	88(0)	60(0)	60(65)	60(65)	60(65)	60(65)	60(65)	
		ELX15514	>320	>320	>320	>320	>320	>320	>320	
		ELX15518	>320	>320	>320	>320	>320	>320	>320	
Stimtech	3821	CA-88	178(0)	178(0)	178(0)	178(0)	159(107)	159(107)	178(107)	
		H38030	>320	>320	>320	>320	>320	>320	>320	
		J38015	302(0)	302(0)	302(0)	302(0)	302(107)	302(107)	302(107)	
Vitatron	HIP-40-RT	J38016	320(0)	320(0)	320(0)	320(0)	>320	>320	>320	
		0505	204(85)	204(86)	204(84)	224(84)	204(86)	204(86)	204(77)	
		0507	302(375)	302(375)	302(375)	302(375)	229(124)	229(124)	266(148)	
5146	5146	5146	178(75)	178(75)	178(75)	178(75)	178(75)	178(75)	102(68)	
		5146	229(150)	229(149)	229(161)	229(156)	229(156)	229(156)	320(118)	

— Pre-production prototype pacemaker designs.

TABLE 4. SIMULATED-IMPLANT PACEMAKER EMI THRESHOLDS

Manufacturer	Model No.	Serial No.	Threshold values, 3100 Hz					
			Pulse repetition rate (pps)					
			7	20	40	100	400	
			V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	
American Optical	281003	11591	>320 ^a	>320	>320	>320	>320	
	281013	A2545	>320	320(0)	>320	>320	>320	
	281143	27560	>320	>320	>320	>320	>320	
Biotronik	IDP-44	61035	>320	>320	>320	>320	>320	
	133C7	2352	141(105)	141(110)		>320	>320	
Cordis	143E7	11575	282(7)	302(76)		141(73)	141(72)	
	162C	5296	302(0)	320(67)		>320	>320	
	164A	286	320(104)	320(72)		>320	>320	
General Electric	A20720	891930	>320	>320		>320	>320	
	A2075A	937147	>320	>320		>320	>320	
Hedcor	3-70A	3753	116(71)	116(71)		129(71)	129(71)	
Hedtronic	5842	3400123	>320	>320		>320	>320	
		3400158	>320	>320		>320	>320	

^a Such entries indicate that pacemaker not affected to limit of test.

TABLE 4 (Cont'd)

Manufacturer	Model No.	Serial No.	Threshold values, 3100 MHz				
			Pulse repetition rate (pps)				
			7	20	40	100	400
			V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)	V/m(bpm)
Medtronic	5942	3K04597	>320	>320	>320	>320	>320
		3K20660	>320				
	5943	1L12821	>320	>320		>320	>320
		3C20824	>320		>320		
	5944	3C20877	>320	>320		>320	>320
		3XX2022 2	>320	>320		>320	>320
	5951	3XX2025 0	>320	>320		>320	>320
		9000	>320	>320	>320	>320	>320
	Pacesetter	BG-101	>320	>320		>320	>320
		8114	204(0)	204(65)		229(65)	248(65)
Starr-Edwards	8116	ELX15518	>320	>320		>320	>320
		3821	>320	>320		>320	>320
Stimtech							
Vitatron	MIP-40-RT	5146	>320	>320		>320	>320

b Pre-production prototype pacemaker designs.

TABLE 5. PACEMAKER EMI ATTENUATION IN SALINE SOLUTION

Manufacturer	Model No.	Attenuation (dB)	
		450 MHz	3100 MHz
American Optical	281003	5.1	
	281013	13.1	>12.3
Biotronik	IDP-44	11.0	
Cordis	133C7	14.2	11.0
	143E7	3.2	
	162C	3.2	
	164A	15.3	9.9
General Electric	A20720	10.8	12.3
	A2075A	13.9	
Medcor	3-73A	6.9	
Medtronic	5842	8.9	>19.8
	5942	11.0	> 6.1
	5943	11.1	>12.3
	5944	12.3	> 2.2
	9000	25.3	>13.1
Starr-Edwards	8114	-3.2	11.2
Stimtech	3821	7.3	
Vitatron	MIP-40-RT	11.0	

ABBREVIATIONS AND ACRONYMS

ac	alternating current
bpm	beats per minute
cm	centimeter(s)
CW	continuous wave
dB	decibel(s)
ECG	electrocardiographic
E-field	electric field strength (V/m)
EMI	electromagnetic radiation interference
EMP	electromagnetic radiation
GIT	Georgia Institute of Technology
kHz	kilohertz
LED	light-emitting diode
MHz	megahertz
min	minute(s)
μ sec	microsecond(s)
msec	millisecond(s)
mW	milliwatt(s)
pps	pulse(s) per second
PRR	pulse repetition rate
RF	radiofrequency
rms	root mean square
sec	second(s)
V/m	volt(s) per meter