

AD-A066 709


NAVAL MEDICAL RESEARCH INST BETHESDA MD
A CLOSED-LOOP GAS ANALYZING SYSTEM. (U)
1978 H C LANGWORTHY, C R FLYNN
NMRI-78-79

F/6 6/11

UNCLASSIFIED

NL

1 of 1
AD
A066709

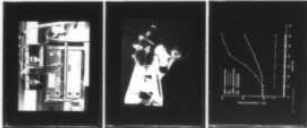

END
DATE
FILMED
5-79
DDC


9

LEVEL

14

**NAVAL MEDICAL RESEARCH INSTITUTE
BETHESDA, MARYLAND**

AD AO 66709

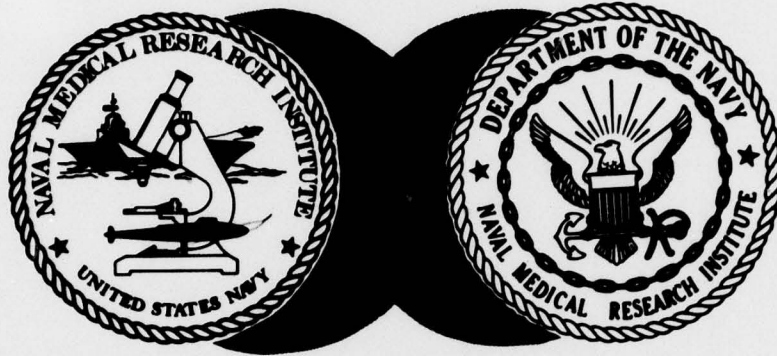

DDC
RECEIVED
MAR 30 1979

AA^C

DDC FILE COPY

78-79
A CLOSED-LOOP GAS ANALYZING SYSTEM
H.C. Langworthy and C.R. Flynn

W. F. Miner, CAPT, MC, USN

Commanding Officer

Naval Medical Research Institute

NAVAL MEDICAL RESEARCH AND DEVELOPMENT COMMAND

This document has been approved for public release and sale; its distribution is unlimited.

79 03 30 054

ACKNOWLEDGMENTS

Naval Medical Research and Development Command, Research Task No. M0099.PN003.3030. The opinions and assertions contained herein are the private ones of the authors and are not to be construed as official or reflecting the views of the Navy Department or the Naval Service at large.

This joint report covers work by the Departments of Hyperbaric Medicine and Physiology and Behavioral Sciences. We wish to acknowledge the invaluable assistance of the Naval Medical Research Institute personnel, especially the contributions made by C.K. Thompson and M.A. Page, who served as subjects. To M.M. Matzen and E.S. Grunewald appreciation for editorial assistance.

Address correspondence pertaining to this report to H.C. Langworthy, Department of Hyperbaric Medicine and Physiology, Naval Medical Research Institute, Bethesda, MD 20014.

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM	
1. REPORT NUMBER ① 14 NMRI-78-79	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER	
4. TITLE (and Subtitle) ② A CLOSED-LOOP GAS ANALYZING SYSTEM	5. TYPE OF REPORT & PERIOD COVERED ③ Medical Research Progress Report	6. PERFORMING ORG. REPORT NUMBER	
		7. AUTHOR(s) ④ H. C./Langworthy C. R./Flynn	
8. CONTRACT OR GRANT NUMBER(s) ⑤ MDD99PN		9. PERFORMING ORGANIZATION NAME AND ADDRESS Naval Medical Research Institute Bethesda, Maryland 20014	
10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS ⑥ MDD99.PN.003/3030 Report No. 2		11. CONTROLLING OFFICE NAME AND ADDRESS Naval Medical Research & Development Command Bethesda, Maryland 20014	
12. REPORT DATE ⑦ 11/1978		13. NUMBER OF PAGES 13	
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office) Bureau of Medicine & Surgery Department of the Navy Washington, D.C. 20372 ⑧ 12 15p.		15. SECURITY CLASS. (of this report) UNCLASSIFIED	
15a. DECLASSIFICATION/DOWNGRADING SCHEDULE		16. DISTRIBUTION STATEMENT (of this Report) approved for public release and sale; distribution unlimited 63713 N	
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)			
18. SUPPLEMENTARY NOTES			
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Gas analyzing; oxygen; carbon dioxide; one-atmosphere diving system.			
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) A closed-loop gas analyzing system was developed for monitoring concentrations of oxygen and carbon dioxide in the one-atmosphere diving system, "JIM." The gas-analyzing system ensures against loss of gas from a fixed gas volume and affords the option of monitoring the gas concentrations either in the operator's mask or in the cabin. JIM can be monitored by this system either in the laboratory or when submerged at shallow depths.			

DD FORM 1 JAN 73 1473

EDITION OF 1 NOV 65 IS OBSOLETE
S/N 0102-LF-014-6601

UNCLASSIFIED
SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

249 650

29 03 30 054
Gur

TABLE OF CONTENTS

	Page No.
Acknowledgments.....	on back of front cover
Abstract.....	1
Introduction.....	1
Methods and Materials.....	1
The system.....	1-2
Data collection.....	3
Results and Discussion.....	2-3
Conclusions.....	3
Appendix.....	4

List of Figures

	Appendix Page No.
Fig. 1. Block Diagram.....	5
Fig. 2. Penetrator.....	6
Fig. 3. Mask showing sample pickup.....	7
Fig. 4. Sample pickup valve.....	8
Fig. 5. Gas analyzers.....	9
Fig. 6. JIM in stand.....	10
Fig. 7. Gas concentrations.....	11

ACCESSION for	
NTIS	Wire Section <input checked="" type="checkbox"/>
DDC	Buff Section <input type="checkbox"/>
UNANNOUNCED	<input type="checkbox"/>
JUSTIFICATION	
BY	
DISTRIBUTION/AVAILABILITY CODES	
or SPECIAL	
A	

A CLOSED-LOOP GAS ANALYZING SYSTEM

Abstract

A closed-loop gas analyzing system was developed for monitoring concentrations of oxygen and carbon dioxide in the one-atmosphere diving system, "JIM." The gas-analyzing system ensures against loss of gas from a fixed gas volume and affords the option of monitoring the gas concentrations either in the operator's mask or in the cabin. JIM can be monitored by this system either in the laboratory or when submerged at shallow depths.

Index Terms: Gas analyzing; oxygen; carbon dioxide; one-atmosphere diving system.

INTRODUCTION

During evaluation of life-support requirements for JIM, a one-atmosphere diving system, the Naval Medical Research Institute designed and developed a closed-loop gas analyzing system. The system was needed for determining the oxygen and carbon dioxide concentrations in JIM's cabin and in the oral nasal mask worn by the operator. Essentially, JIM has a fixed volume of gas, because the available oxygen in the cabin is metabolized by the operator and oxygen is added by an oxygen makeup system that maintains the desired concentration of 21%. The carbon dioxide generated by the operator is absorbed in cannisters filled with baralyme, which are located on both the exhalation and inhalation sides of the mask.

The JIM operator relies upon a Draeger^R analyzer, which records oxygen concentrations, and a cabin pressure indicator, which shows increases in carbon dioxide. This method is adequate for operational dives, but does not provide sufficient information on gas concentrations for an in-depth evaluation of the life-support system.

METHODS AND MATERIALS

The System

The closed-loop gas analyzing system developed consists of two lengths of 3/16th o.d. Tygon^R flexible plastic tubing, which channels the gas flowing from the JIM cabin through the monitoring instruments back to the cabin (see block diagram, *Fig. 1; figures are in the Appendix). Tygon tubing was put inside a 40-foot length of hose that served as a carrier and protector; the hose was secured to JIM by a stainless steel hose adapter (manufactured in-house) that penetrated JIM's hull. The surface end of the hose around the Tygon tubes was potted with clear RTV #118 General Electric silicone rubber (Fig. 2); thus, gas leakage was prevented between JIM's cabin and the surface environment.

* Forty feet of hose allows for future shallow submerged testing.

In the JIM system there are two pickup locations for sample gas. One is located in the oral nasal mask (Fig. 3); the other is located in the cabin at the operator's chest level. The two pickup tubes are connected to a Luer two-way valve, which is controlled by the JIM operator (Fig. 4). When the Luer valve is in line with the pickup tube in the oral nasal mask, the operator's inspired and expired oxygen and carbon dioxide concentrations are monitored. When the Luer valve is in line with the pickup tube for the cabin, the oxygen and carbon dioxide concentrations in the cabin are monitored.

Data Collection

The concentration of oxygen is measured with an OM-11 Beckman oxygen analyzer; the concentration of carbon dioxide is measured with an LB-2 Beckman analyzer (Fig. 5). The microcatheter pump in each instrument provides the flow and direction of the gases within the closed loop. For data collection the analyzers are connected to a dual-channel recorder.

During the laboratory testing phase, the JIM system was held in a vertical position and supported by a stand (Fig. 6). The JIM operator was at rest in a standing position throughout the test. The controls for the life-support system were set up for a routine wet working dive; the oxygen was delivered at approximately 1.5 liters/minute.

RESULTS AND DISCUSSION

The lengths of the Tygon tubing through which the test gases flowed were too long to provide an accurate breath-by-breath measurement of carbon dioxide and oxygen. Although the respiration rates could be counted from the chart tracings, some inhalation and exhalation gas mixing took place both in the oral nasal mask and in the tubing. Therefore, the values shown in Fig. 7 represent the highest concentrations of carbon dioxide and oxygen recorded at each exhalation point. Also shown in Fig. 7 are the carbon dioxide and oxygen concentrations in the cabin at the operator's chest level.

Cabin thermal conditions dictated that 1 h was the optimum amount of time that an operator could remain inside JIM during dry laboratory testing. The heat generated by the absorbent cannisters along with the body heat given off by the operator increased the cabin temperature from 78° F to 86° F. Under actual diving conditions, the heat would contribute to the thermal comfort of the operator.

At the end of the 1-h testing period:

- Concentrations of oxygen in the cabin exhibited a slow, steady increase from 20.8% to 29.8%; concentrations of oxygen in the oral nasal mask increased from 19.9% to 42.9%. These increases were a result of the 1.5 liter/minute oxygen injection rate set for the average wet working dive.

● Carbon dioxide concentrations in the cabin increased from 0.3% to 0.32% during the 1-h testing period. The carbon dioxide concentrations in the oral nasal mask reached a low of 4.1% and a high of 4.8%, with a mean of 4.45%.

The accuracy of measurements during the testing period was ensured by calibration of both analyzers immediately before and immediately after the testing period.


CONCLUSIONS

The closed-loop gas analyzing system developed for evaluating JIM's breathing system has proved to be an invaluable tool. Throughout the testing with JIM, continuous accurate monitoring of oxygen and carbon dioxide concentrations was possible. This method of gas monitoring did not interfere with the operator's normal activities, and it should not interfere with JIM's mobility during wet, shallow dives. The system is compact and portable; it should work well in field conditions that can supply AC power for the Beckman instruments.

We anticipate that the closed-loop gas analyzing system will be useful in future evaluations of one-atmosphere diving systems and that it will contribute to life-support technology.


APPENDIX

Figures Relating to Report

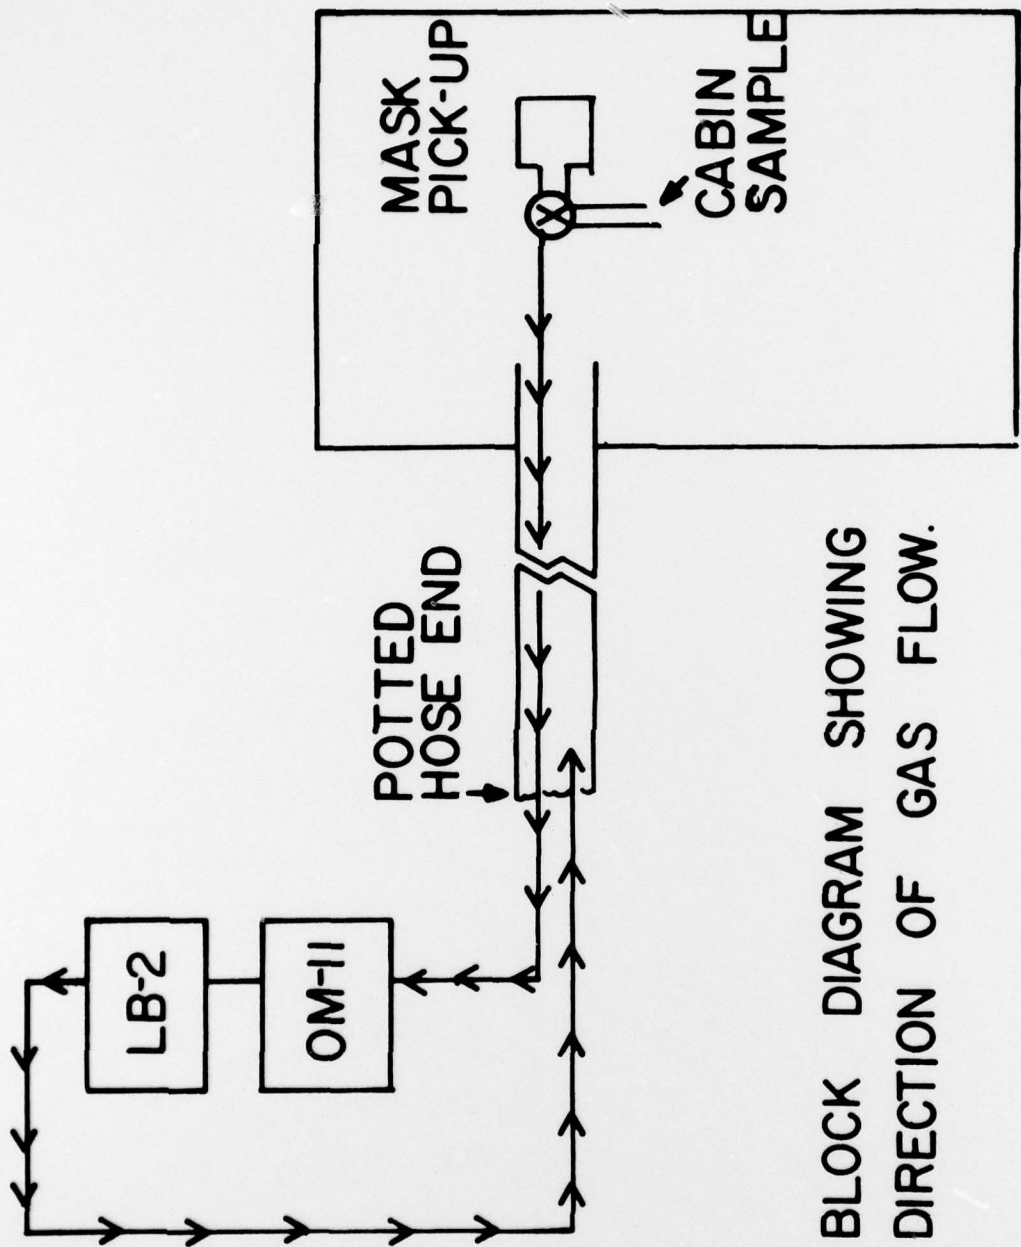

BLOCK DIAGRAM SHOWING
DIRECTION OF GAS FLOW.

Fig. 1. Block diagram.

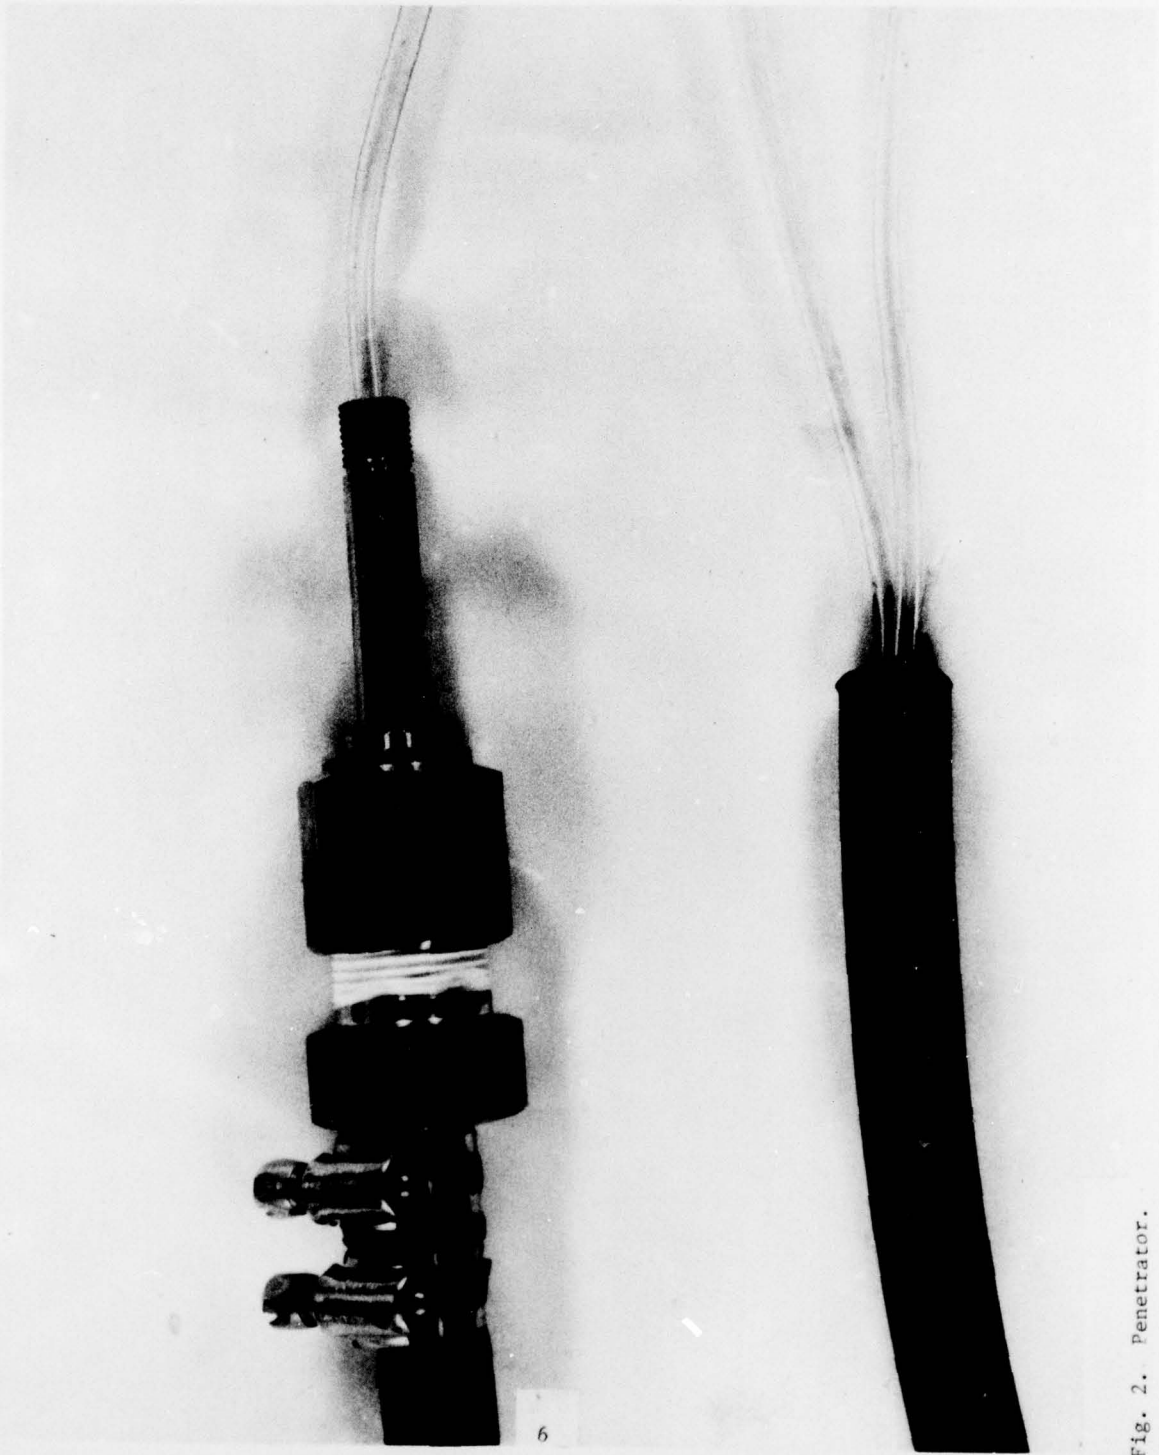

6

Fig. 2. Penetrator.

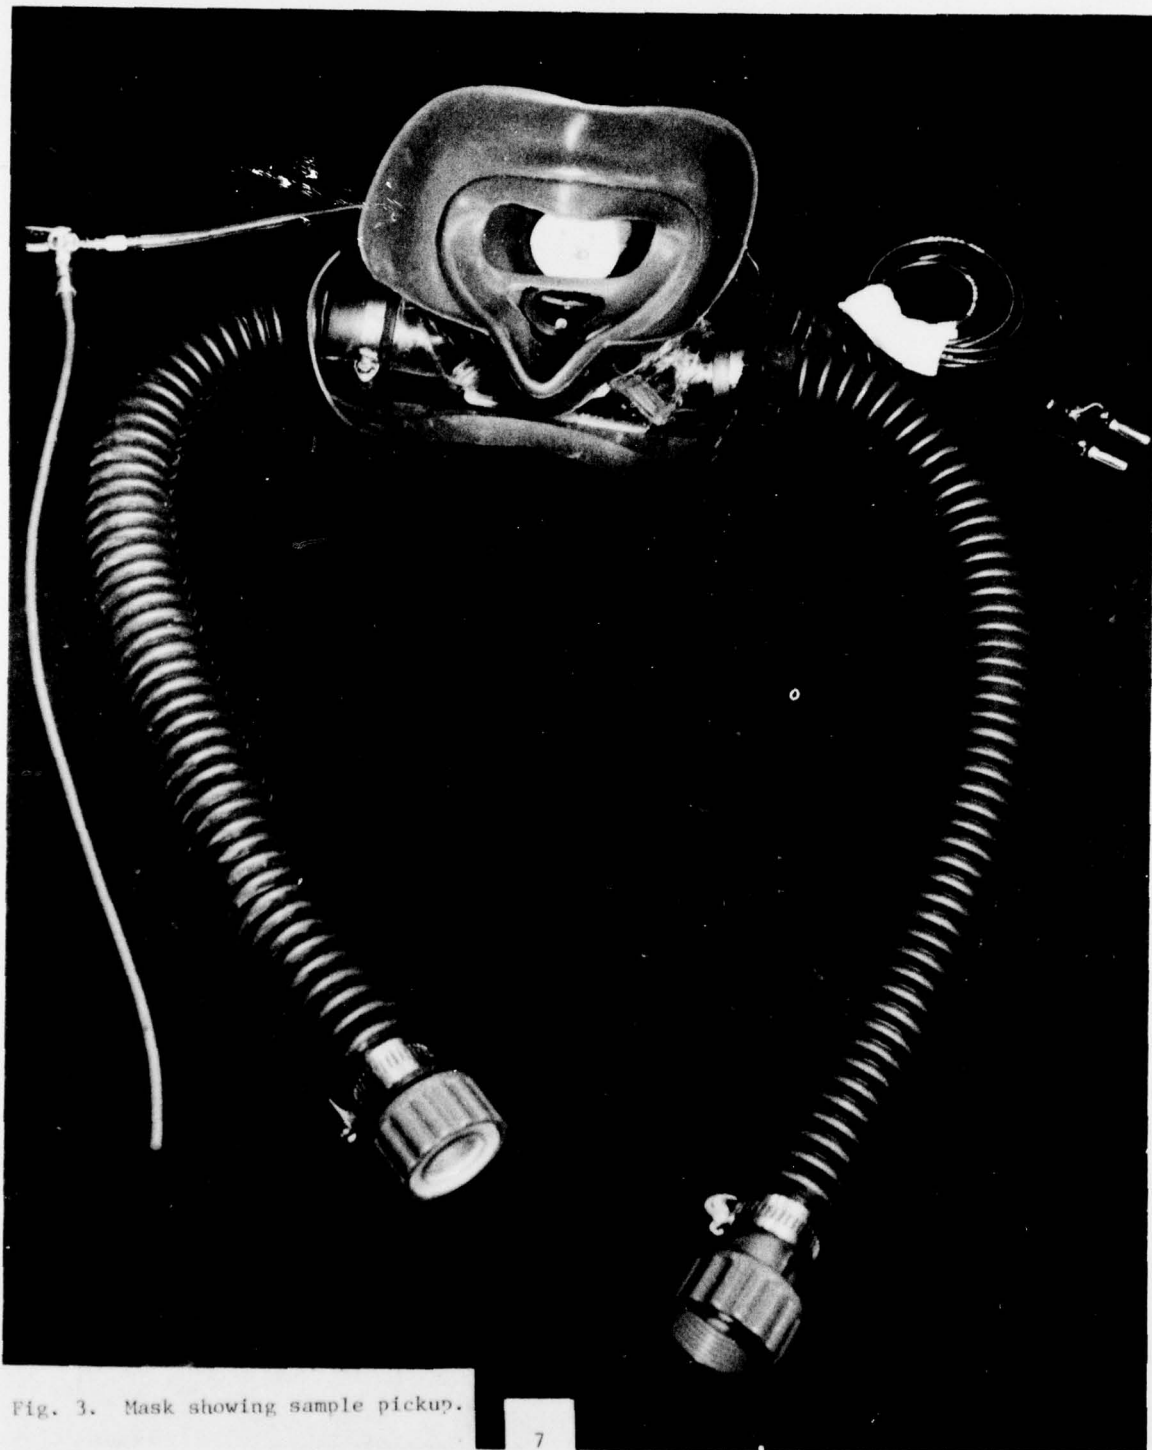


Fig. 3. Mask showing sample pickup.



Fig. 4. Sample pickup valve.



Fig. 5. Gas analyzers.

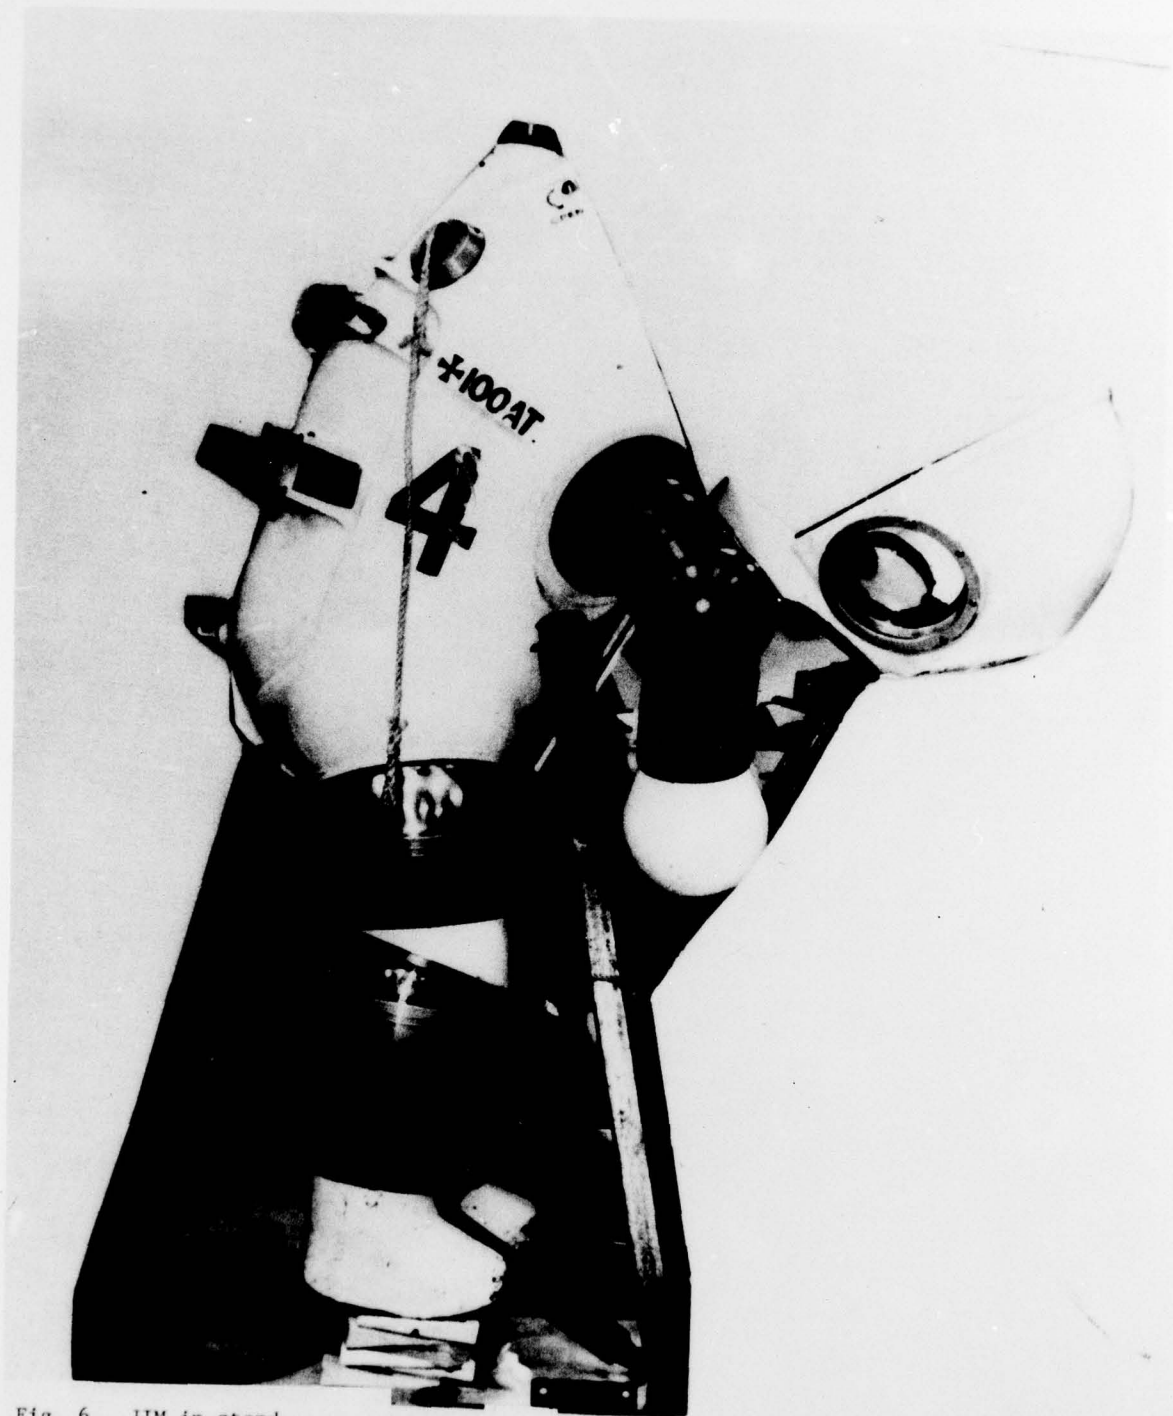


Fig. 6. JIM in stand.

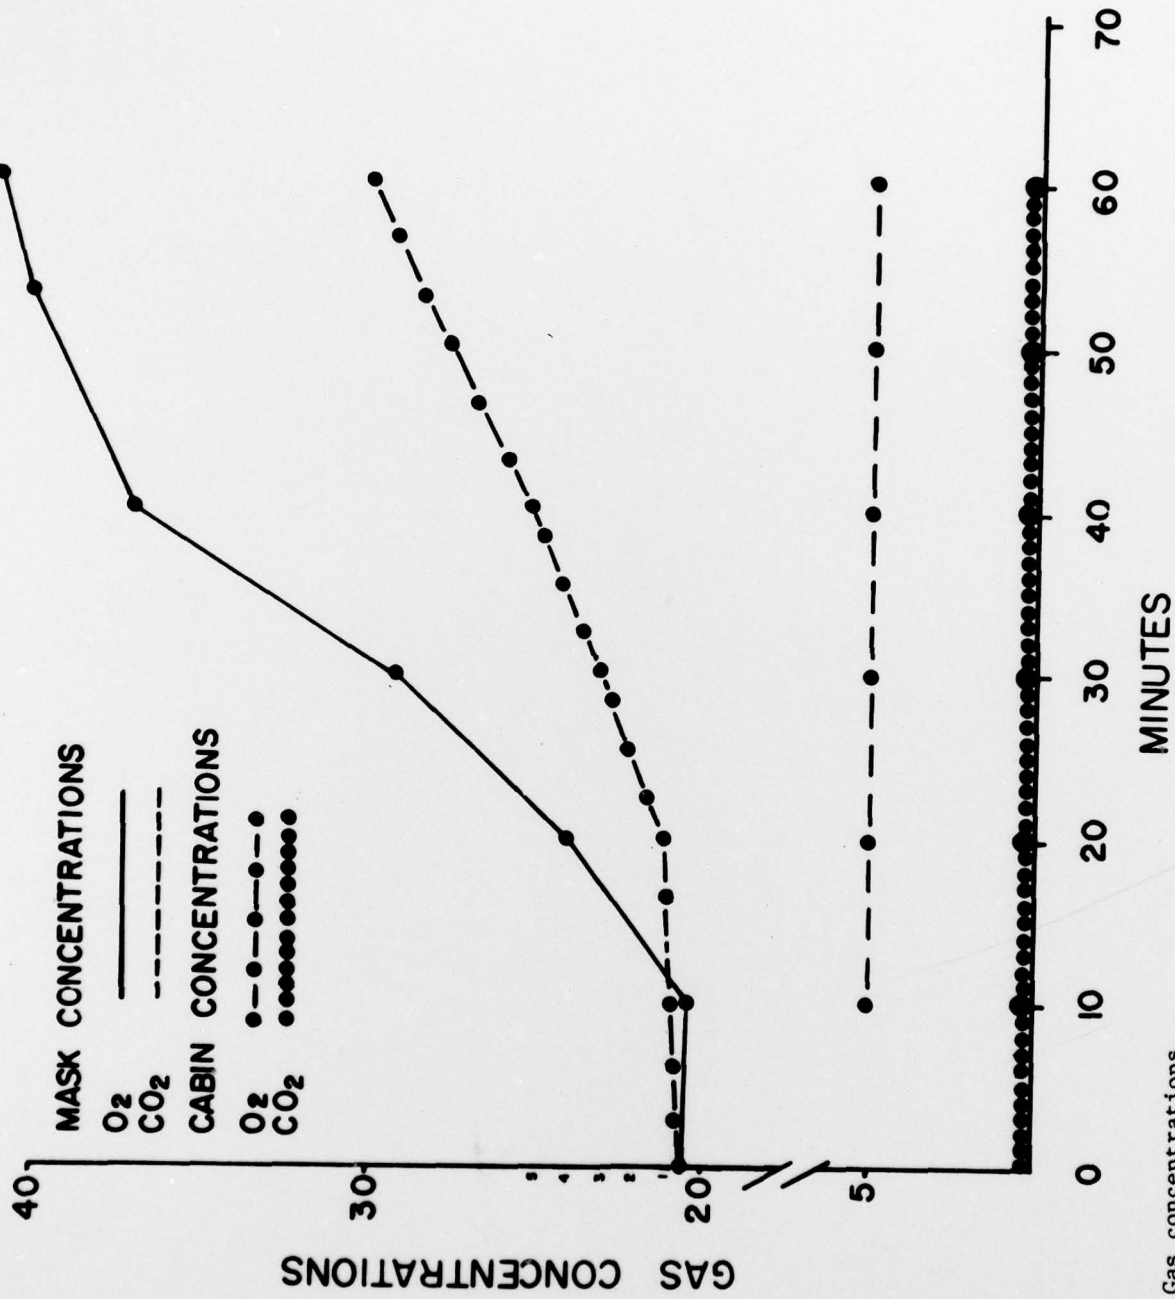


Fig. 7. Gas concentrations.