

AD-A087 039

MASSACHUSETTS INST OF TECH CAMBRIDGE  
EFFECT OF INFRARED LASER RADIATION ON BIOLOGICAL SYSTEMS.(U)  
JUN 73 G W PRATT

F/6 6/18

DADA17-72-C-2101

NL

UNCLASSIFIED


1-2  
a  
b  
c



ENG  
77  
9400  
6712

*CONT*

1 OF 2  
AD-  
A087039

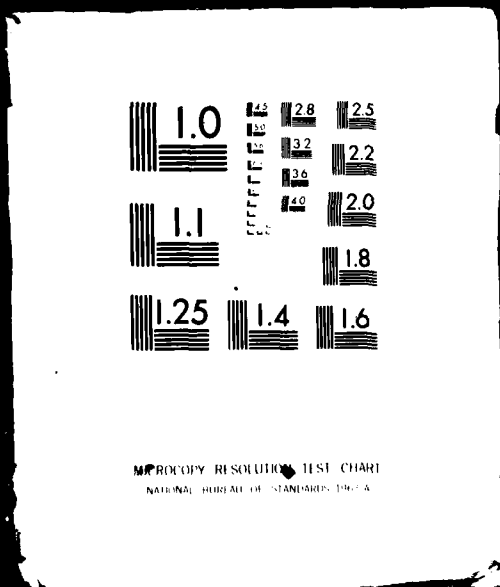

12 AD \_\_\_\_\_

EFFECT OF INFRARED LASER RADIATION  
ON BIOLOGICAL SYSTEMS

FINAL REPORT

by

GEROGE W. PRATT

LEVEL *11*

DTIC  
ELECT  
JUL 22 1980  
C

JUNE 1973

Supported by

U.S. Army Medical Research and Development Command  
Fort Detrick, Frederick, Maryland 21701

Contract No. DADA 17-72-C-2101

Massachusetts Institute of Technology  
Cambridge, Massachusetts 02139

DOD DISTRIBUTION STATEMENT

Approved for public release;  
distribution unlimited

The findings in this report are not to be construed as an  
official Department of the Army position unless so designated  
by other authorized documents.

ADA 087039

DDC FILE COPY

80 7 21

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER	2. GOVT ACCESSION NO. <b>AD-A097039</b>	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) <b>EFFECT OF INFRARED LASER RADIATION ON BIOLOGICAL SYSTEMS</b>	5. AUTHOR(s) <b>George W. Pratt, Jr</b>	6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s)	8. CONTRACT OR GRANT NUMBER(s) <b>DADA17-72-C-2101</b>	9. DATE OF REPORT & PERIOD COVERED <b>Final rept. Mar 1972 - May 1973</b>
9. PERFORMING ORGANIZATION NAME AND ADDRESS <b>Massachusetts Institute of Technology Cambridge, MA 01239</b>	10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS <b>62110A/3A062110821/00.013</b>	11. CONTROLLING OFFICE NAME AND ADDRESS <b>US Army Medical Research and Development Command Fort Detrick Frederick, Maryland 21701</b>
11. CONTROLLING OFFICE NAME AND ADDRESS	12. REPORT DATE <b>June 1973</b>	13. NUMBER OF PAGES <b>13</b>
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office) <b>12-14</b>	15. SECURITY CLASS. (of this report) <b>Unclassified</b>	16. DISTRIBUTION STATEMENT (of this Report) <b>Approved for public release; distribution unlimited</b>
16. DISTRIBUTION STATEMENT (of this Report)	17. SECURITY CLASS. (of this report)	17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)	18. DECLASSIFICATION/DOWNGRADING SCHEDULE	18. SUPPLEMENTARY NOTES
18. SUPPLEMENTARY NOTES	19. KEY WORDS (Continue on reverse side if necessary and identify by block number) <b>Lasers in Medicine Laser Sterilization Infrared Radiation of Biological Systems</b>	19. KEY WORDS (Continue on reverse side if necessary and identify by block number)
19. KEY WORDS (Continue on reverse side if necessary and identify by block number)	20. ABSTRACT (Continue on reverse side if necessary and identify by block number) <b>A low power CO<sub>2</sub> laser has been used to kill a spore preparation of Bacillus Subtilis. The CO<sub>2</sub> laser has been found to be very effective in deactivating these spores. A 65 watt/cm<sup>2</sup> beam reduced the dry live spore population by 3 orders of magnitude in 0.4 seconds as compared to a reduction by one order of magnitude after 60 seconds exposure (150 times as long) to pressurized steam at 130°C. A possible explanation of the high efficiency of laser sterilization may be deactivation by resonant absorption of infrared energy at 10.6 μ. Experi- ments discussing selected damage in proteins are presented.</b>	20. ABSTRACT (Continue on reverse side if necessary and identify by block number)

## INTRODUCTION

This is the "Final Scientific Report" under Contract No. DADA17-72-C-2101. The title of the contract was "Effect of Infrared Laser Radiation on Biological Systems."

## EXPERIMENTAL RESULTS

The first experiments were carried out using a very heat resistant dry spore preparation of Bacillus Subtilis. These spores were initially spread on Al substrates because metals, such as Al, reflect virtually all of the incident CO<sub>2</sub> laser radiation up to very high incident powers. These spores have a decimal reduction time D (that time required to reduce the number of viable organism to 1/10<sup>th</sup> of the original value) of approximately 60 seconds in pressurized steam at 130°C. In a 65 watt/cm<sup>2</sup> laser beam the spore population was reduced by 3 orders of magnitude in 0.4 sec for dry spores and by 5 orders of magnitude for spores with an active water coefficient of 0.8. This is shown in Fig. 1.

The spores are inactivated so rapidly in the CO<sub>2</sub> beam that it is not necessary to disperse them on a metal substrate. A 20 watt/cm<sup>2</sup> beam pulse for 1/20<sup>th</sup> of a second delivers one joule to the target. If all of this energy were absorbed by a paper substrate 10<sup>-2</sup> cm thick and 1 cm<sup>2</sup> area, the temperature would rise only by 50°C which is well below the rise necessary for ignition. The same energy delivered to a 10 μ thick spore layer would raise the temperature of these spores by roughly 500°C. Assuming approximately equal densities and specific heats the temperature rise of a surface layer  $\delta T_L$  of thickness  $t_1$  on a substrate of thickness  $t_s$  is in a very rough approximation

given by

$$\delta T_L = \frac{c_s}{c_1} \delta T_s$$

Approved For	By
DTIC Channel	Distribution
Unannounced	Availability Codes
Justification	Avail and/or Special
	Dist
	A

where  $T_s$  is the temperature rise of the substrate. Experiments carried out where the spore layer was spread over cellulose acetate paper showed that 1/25<sup>th</sup> of a second pulse at the 20 watt operating level completely destroyed the spore activity, but made no visible change in the paper substrate. This result is of considerable practical importance. It means that surface contamination can be rendered sterile on materials that are quite sensitive to heat and which cannot be sterilized using ordinary techniques eg. steam. The list of such materials is extensive including sutures, plastic and rubber catheters, dressings, etc. In addition many materials are unsuitable for radiosterilization with  $\gamma$  rays. Glass, darkness and some rubber and plastics deteriorate mechanically. Metallic instruments, vessels, etc. reflect most of the infrared energy until incident power levels in the  $K_w/cm^2$  range are attained. Organisms on the metal surface would, however, absorb the laser energy and be destroyed. The CO<sub>2</sub> and CO lasers offer the very attractive feature of sterilization of metallic surfaces in seconds rather than customary times of several minutes. Flash sterilization of foodstuffs is a further application again where surface contamination is involved.

Similar experiments have been carried out using Streptococcus faecium. The deactivation obtained in 60 seconds in the CO<sub>2</sub> beam was the equivalent to that produced by a radiation dose of 2.5 M rad. This requires 500

minutes from the MIT  $\gamma$ -ray source.

An interesting question is what is the nature of the "heating" process in a laser pulse of the order of  $10^{-2}$  seconds duration if all the energy absorbed were taken up by specific vibrational modes of the irradiated molecules? Certainly  $10^{-2}$  sec is enormously long compared to vibrational periods and to probable molecular relaxation times. One can estimate the molecular relaxation times from the infrared line widths. A line width of  $50 \text{ cm}^{-1}$  in a  $1000 \text{ cm}^{-1}$  line corresponds to a relaxation time of  $1.2 \times 10^{-13}$  sec. Therefore, energy absorbed in a given molecular vibrational mode is rapidly dispersed through the excitation spectrum. A 20 watt beam pulsed for  $1/20^{\text{th}}$  of a second delivers  $5 \times 10^{19}$  photons to a target area of  $1 \text{ cm}^2$ . This is approximately  $10^5$  quanta per absorbing bond per second. The deviation from the average number of quanta of vibrational excitation in a specific absorbing mode is roughly

$$\frac{n - n_0}{\tau} = 10^5 .$$

With  $\tau \sim 1.2 \times 10^{-13}$  sec we see that  $n - n_0$  is essentially zero. At  $10.6 \mu$  each photon carries 0.117 ev and 20 of these photons would be required to break a normal covalent bond. However, a typical hydrogen bond has a binding energy of 0.1 ev. Consequently at these low radiation levels from the  $\text{CO}_2$  laser it is almost certain that molecular alterations will be due to disruption of hydrogen bonds effecting total or partial denaturation.

The estimate above pictures individual molecules with an absorbing mode treated as a damped oscillator whose line width is described by a relaxation time  $\tau$ , which is typically  $10^{-12}$  sec long. Temperature is not well defined at times as short as this. In order to invoke reaction kinetics and heat flow equations enough time must elapse for the transfer of energy between molecules. This is the thermal relaxation time  $\tau_h$  and is related to the thermal conductivity. Typical values are  $10^{-6} - 10^{-7}$  seconds. Hayes and Wolbarsht<sup>1</sup> point out that laser pulses short compared to  $\tau_h$  heat up the target before the energy can be conducted away as heat. The temperature rise in

$$\Delta T = FE_{\text{abs}}/C$$

where C is the heat capacity of the target particle,  $E_{\text{abs}}$  the absorbed energy, and F the fraction of the absorbed energy available for heating. F is given by Hayes and Wolbarsht as

$$F = \frac{\tau_h}{\tau_e} (1 - e^{-\tau_e/\tau_h})$$

where  $\tau_e$  is the exposure time. In order to convey some feeling for the numbers involved in heat flow we quote a result of Vassiliadis<sup>2</sup> that a melanin granule  $1 \mu$  in diameter with an initial temperature rise  $\Delta T$  cools to  $1/e$  of  $\Delta T$  (after the radiation is shut off) in  $4 \times 10^{-7}$  seconds.

---

<sup>1</sup>J.R. Hayes and M.L. Wolbarsht, "Laser Applications in Medicine and Biology", Vol 1, Chapter IX, Plenum Press, ed., by M.L. Wolbarsht, New York, (1971).

<sup>2</sup>A. Vassiliadis, Loc. Cit. Chapter VI.

The extent of bond breaking due to heating is described by reaction kinetics. The equilibrium constant  $K_{eq}$  for a given bond is

$$K_{eq} = \frac{[\text{number of intact bonds}]}{[\text{number of broken bonds}]}$$

and is related to the bond strength  $\Delta G$  by

$$K_{eq} = e^{-\Delta G/RT}$$

A  $\Delta G$  typical of a hydrogen bond is  $-2.726$  K cal/mole and it leads to the following ratio as a function of temperature:

T°C	$K_{eq}$
500	5.6
300	9.8
100	30
25	100 .

A  $\Delta G$  of  $-27.26$  K cal/mole is representative of a covalent bond strength and gives a  $K_{eq}$  of  $10^{7.5}$  at  $500^\circ\text{C}$ . Thus heating a biomaterial to only  $300^\circ\text{C}$  breaks 10% of the hydrogen bonds but only one covalent bond in 30 million even at  $500^\circ\text{C}$ .

It has been stressed above that the infrared laser allows one to deliver large amounts of energy at a specific frequency and over a time domain ranging from cw to pulses of  $10^{-12}$  sec duration. A key question is

whether or not this energy can indeed be directed into specific bonds in a protein or nucleic acid. If this is successful it will then be a question of whether controlled molecular changes can be brought about. When the exposure time is long compared to intra-molecular relaxation times, then a given vibrational mode will leak away its excitation energy. The heat energy may be somewhat confined in the molecular structure but will more probably feed energy into all of the molecular vibrational and rotational modes. Therefore, the exposure time would seem to be confined to periods of less than  $10^{-9}$  seconds if only one particular bond is to be affected. An exposure time between the intra and inter molecular relaxation time will heat the exposed material so rapidly that the heat cannot escape. This will lead to the maximum temperature rise for a given energy input. One concludes then that sterilization will be most effectively accomplished under these conditions.

A step towards the development of pulse techniques has been taken by a Senior Thesis student, Marshall Schorin.<sup>3</sup> Simple proteins, polyglycine and phenylalanylglycine were pressed in KBr pellets. The infrared transmission spectrum was run on the pellet which was then exposed to pulsed  $\text{CO}_2$  radiation and the transmission spectrum run again. Exposure times were long eg.  $10^{-1}$  sec. Therefore, the laser had to act essentially as a heater. Changes in the transmission spectrum of these materials was

---

<sup>3</sup>M. Schorin, Senior Thesis Dept. of Electrical Engineering, MIT (1971).

observed and it differed for different parts of the spectrum. No identification has been made of which particular vibrational modes were most affected. Shorin's results are shown in Figures 2, 3, and 4. The main significance of Shorin's results is that he has established a useful technique that can be applied to higher power, shorter duration pulses.

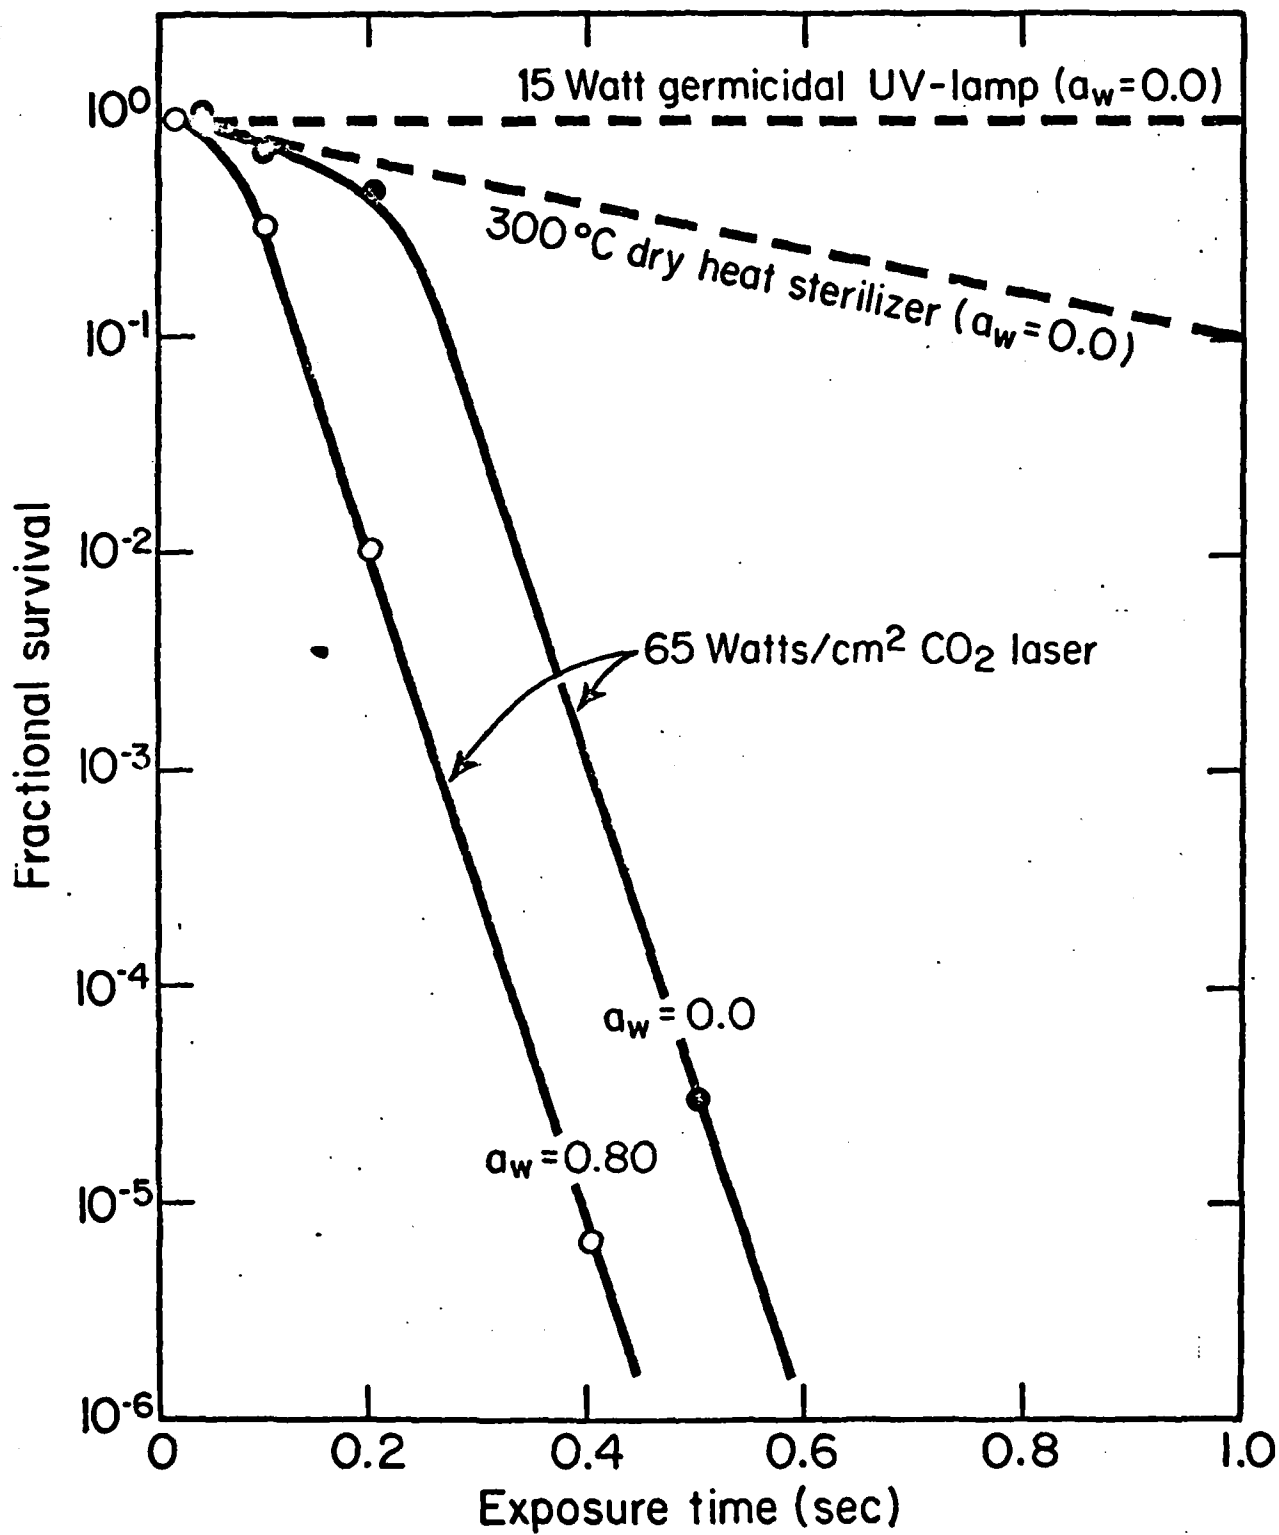


Fig. 1.

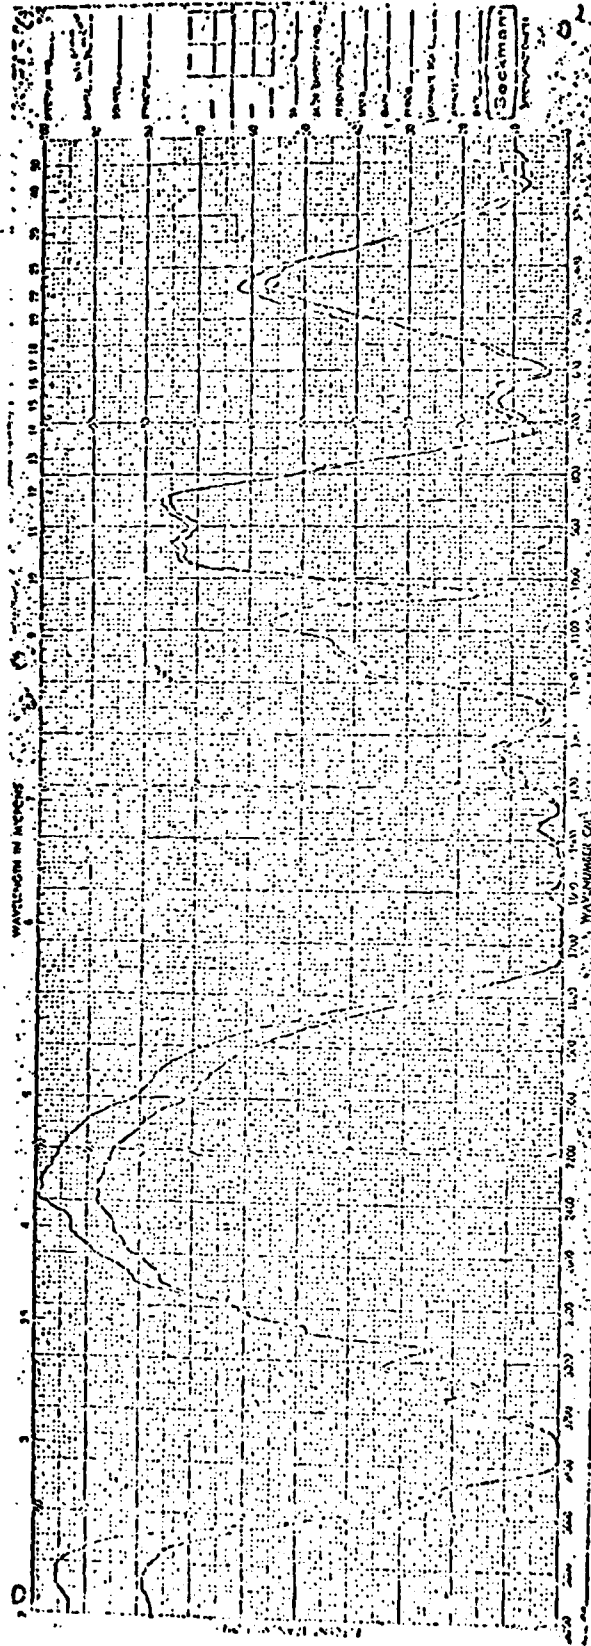


Fig. 2 This graph shows the difference between polyglycine unexposed (broken line) and exposed for a short time only (0.2 sec. @ 60 W.) (solid line).

THIS PAGE IS BEST QUALITY PRACTICABLE  
FROM COPY FURNISHED TO DDC

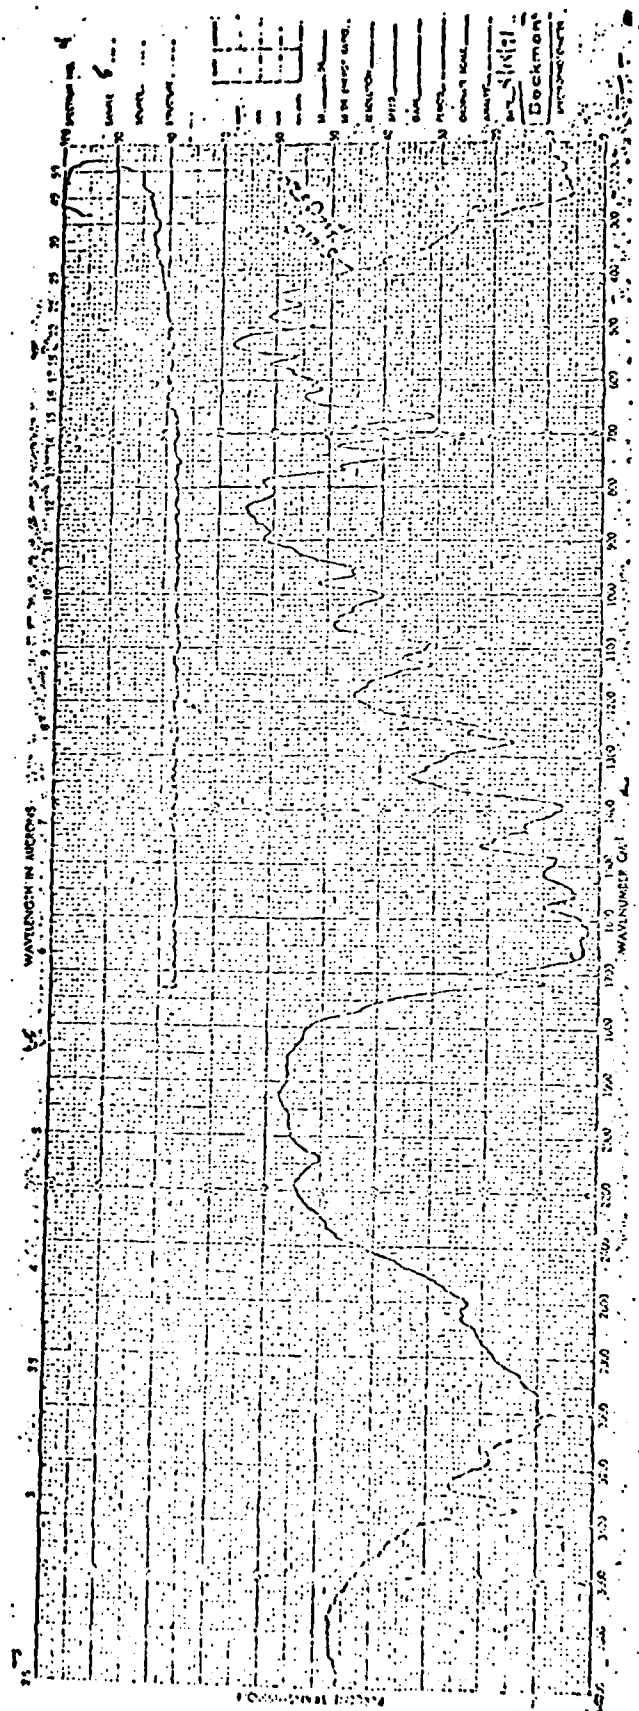


Fig. 3 Phenylalanylglycine after small exposure (0.1 sec. @ 52 W.). (The top (incomplete) trace was used to check the level of the spectrophotometer; ignore it.)

THIS PAGE IS BEST QUALITY PRACTICABLE FROM COPY FURNISHED TO DDC

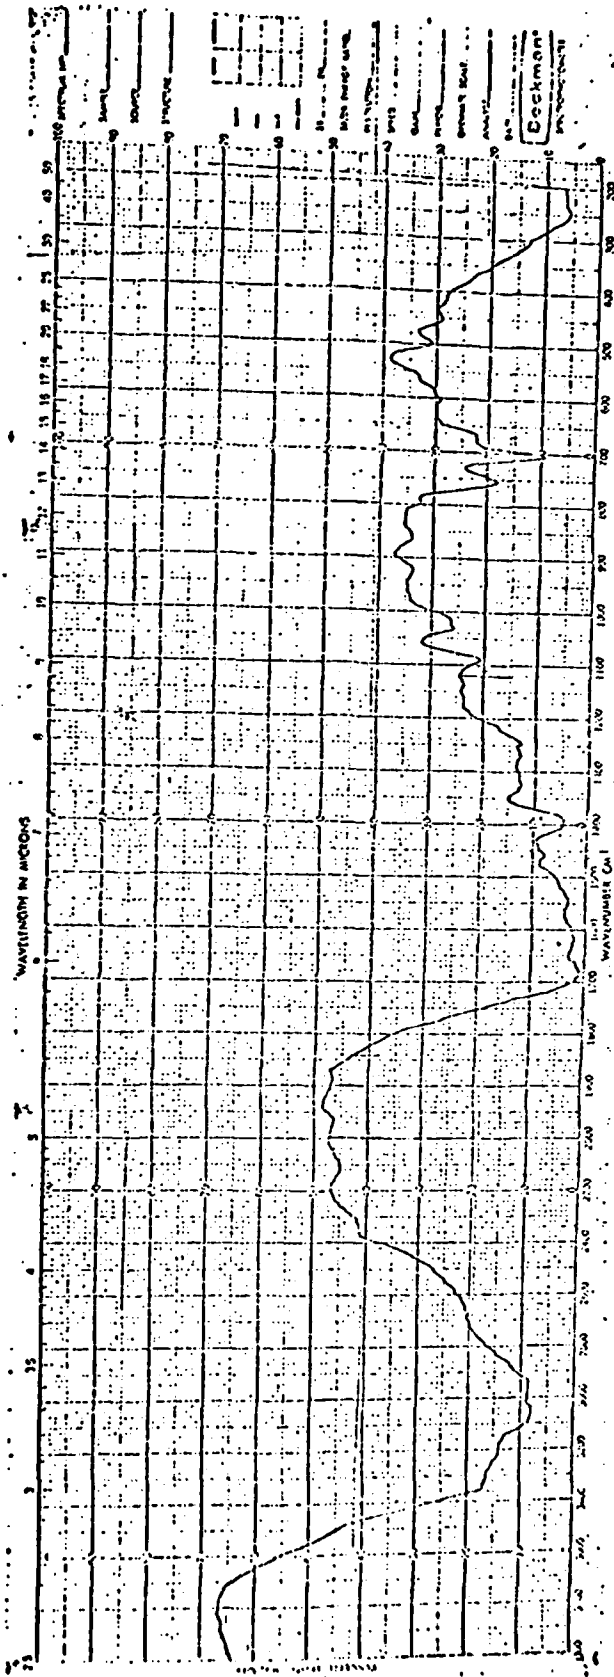


Fig. 4 . This graph was the first one to indicate a change in spectrum after irradiation. It is phenylalanyl glycine exposed for 0.5 sec. @ 60 W.

**THIS PAGE IS BEST QUALITY PRACTICABLE**  
FROM COPY FURNISHED TO DDC

DISTRIBUTION LIST

4 copies

HQDA (SGRD-SI)  
Fort Detrick  
Frederick, MD. 21701

12 copies

Defense Technical Information Center (DTIC)  
ATTN: DTIC-DDA  
Cameron Station  
Alexandria, Virginia 22314

1 copy

Dean  
School of Medicine  
Uniformed Services University of the  
Health Sciences  
4301 Jones Bridge Road  
Bethesda, Maryland 20014

1 copy

Superintendent  
Academy of Health Sciences, US Army  
ATTN: AHS-COM  
Fort Sam Houston, Texas 78234

4 copies

Commander  
Letterman Army Institute  
of Research (LAIR) Bldg. 1110  
ATTN: Dr. J. Ryan Neville  
Presidio of San Francisco, CA 94129

END

DATE  
FILMED

9-7-80

DTIC

IN

AD-A087 039

MASSACHUSETTS INST OF TECH CAMBRIDGE

F/6 6/18

EFFECT OF INFRARED LASER RADIATION ON BIOLOGICAL SYSTEMS.(U)

JUN 73 6 W PRATT

DADA17-72-C-2101

NL

UNCLASSIFIED

2  
612

2  
3  
612  
INFORMATION

INFORMATION

INFORMATION


END  
DATE  
FILMED  
10-80  
DTIC

551F1E1

2 OF 2

AD

A087039

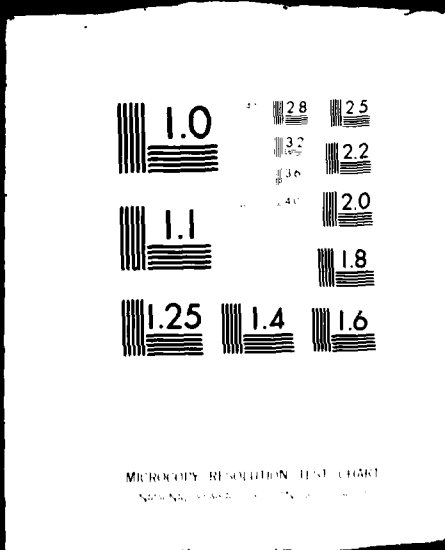

**SUPPLEMENTARY**

**INFORMATION**

AD A687039

EFFECT OF INFRARED LASER RADIATION  
ON BIOLOGICAL SYSTEMS

FINAL REPORT

by

~~GEORGE~~ W. PRATT

JUNE 1973

Supported by

U.S. Army Medical Research and Development Command  
Fort Detrick, Frederick, Maryland 21701

Contract No. DADA 17-72-C-2101

Massachusetts Institute of Technology  
Cambridge, Massachusetts 02139

DOD DISTRIBUTION STATEMENT

Approved for public release;  
distribution unlimited

The findings in this report are not to be construed as an  
official Department of the Army position unless so designated  
by other authorized documents.

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) EFFECT OF INFRARED LASER RADIATION ON BIOLOGICAL SYSTEMS		5. TYPE OF REPORT & PERIOD COVERED Final March 1972 - May 1973
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) George W. Pratt, Jr.		8. CONTRACT OR GRANT NUMBER(s) DADA17-72-C-2101
9. PERFORMING ORGANIZATION NAME AND ADDRESS Massachusetts Institute of Technology Cambridge, MA 01239		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 62110A.3A062110821.00.013
11. CONTROLLING OFFICE NAME AND ADDRESS US Army Medical Research and Development Command Fort Detrick Frederick, Maryland 21701		12. REPORT DATE June 1973
		13. NUMBER OF PAGES 13
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) Unclassified
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report)  Approved for public release; distribution unlimited		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Lasers in Medicine Laser Sterilization Infrared Radiation of Biological Systems		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) A low power CO <sub>2</sub> laser has been used to kill a spore preparation of <i>Bacillus Subtilis</i> . The CO <sub>2</sub> laser has been found to be very effective in deactivating these spores. A 65 watt/cm <sup>2</sup> beam reduced the dry live spore population by 3 orders of magnitude in 0.4 seconds as compared to a reduction by one order of magnitude after 60 seconds exposure (150 times as long) to pressurized steam at 130°C. A possible explanation of the high efficiency of laser sterilization may be deactivation by resonant absorption of infrared energy at 10.6 μ. Experiments discussing selected damage in proteins are presented.		

END