

AD-A116 433

PURDUE UNIV LAFAYETTE IN DEPT OF CHEMISTRY
AN AUTOMATED HANGING MERCURY DROP ELECTRODE.(U)
MAY 82 W A BYERS, S P PERONE

F/6 7/4

UNCLASSIFIED

TR-26

N00014-75-C-0874

NL

1 of 1
AD-A116 433



END
DATE
FILMED
8-82
DTIC

12

AD A116438

OFFICE OF NAVAL RESEARCH
Contract No. N00014-75-C-0874
Task No. NR 051-552
TECHNICAL REPORT NO. 26

An Automated Hanging Mercury Drop Electrode

by

W. Arthur Byers^(a) and S. P. Perone^{*(b)}

Department of Chemistry
Purdue University
W. Lafayette, IN 47907

Prepared for Publication in

Analytical Chemistry

May, 1982

Production in whole or in part is permitted for
any purpose of the United States Government.

Approved for Public Release; Distribution Unlimited

(a) Present address: Westinghouse Electric Corporation
1310 Beulah Road
Pittsburgh, PA 15235

(b) Present address: Chemistry & Materials Science Department
Lawrence Livermore National Laboratory
P.O. Box 808, L-326
Livermore, California 94550

DTIC
ELECTE
JUL 6 1982
S D
D

88 07 06 091

DTIC FILE COPY

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER Technical Report No. 26	2. GOVT ACCESSION NO. AD-A116 438	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) An Automated Hanging Mercury Drop Electrode		5. TYPE OF REPORT & PERIOD COVERED Interim
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) W. Arthur Byers and S. P. Perone		8. CONTRACT OR GRANT NUMBER(s) N00014-75-C-0874
9. PERFORMING ORGANIZATION NAME AND ADDRESS Purdue University Department of Chemistry W. Lafayette, IN 47907		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS NR 051-552
11. CONTROLLING OFFICE NAME AND ADDRESS Materials Science Division Office of Naval Research Arlington, VA 22217		12. REPORT DATE May, 1982
		13. NUMBER OF PAGES 4
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) Unclassified
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Approved for Public Release, Distribution Unlimited		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		Accession For NTIS GRA&I ☒ DTIC TAB ☐ Unannounced ☐ Justification
18. SUPPLEMENTARY NOTES Submitted for publication in <u>Analytical Chemistry</u>		By Distribution/ Availability Codes Dist <u>A</u>
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) electrochemistry mercury electrode automated analysis		
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) This paper describes the construction of an automated static mercury drop electrode dispenser. It can be constructed from readily available materials, requires little maintenance, is easy to fill, and dispenses very reproducibly.		

DD FORM 1473

1 JAN 73

EDITION OF 1 NOV 68 IS OBSOLETE
S/N 0102-014-6601

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

AN AUTOMATED HANGING MERCURY DROP ELECTRODE

by

W. Arthur Byers and S. P. Perone*

Automatic production of a constant area mercury drop has presented considerable problems in the past. Stepper motor driven electrodes of the microburet variety have been used with some success, but frequent filling of the electrode is required. Use of a slowly dropping mercury electrode to approximate a stationary drop eliminates the filling problem, but the very narrow capillary bore leads to frequent clogging and irreproducibility. In addition, long drop times needed for stripping and short drop times necessary to avoid adsorption effects are not possible.

Princeton Applied Research has recently marketed an instrument called the "static mercury drop electrode" which overcomes the previously mentioned disadvantages by valving the flow of mercury through a wide bore capillary (1, 2). The mercury is allowed to flow for a few hundred milliseconds until the drop has grown to the desired size. The drop growth is then terminated by a solenoid controlled polyurethane seal which plugs the mercury reservoir end of the capillary. Electrical connection is made by a tin oxide coating on the surface of the electrode.

This paper presents a static mercury drop electrode which can be constructed from materials readily available in most laboratories. The electrode requires little maintenance, is easy to fill, and dispenses very reproducibly.

The accompanying figure shows the basic construction of the electrode. In this design, a sharpened stainless steel wire is pulled in and out of a wide bore capillary by a 6 V solenoid to valve the mercury flow. The capillary is

.006 inches internal diameter and has been blown out at the end so that the wire is guided to the orifice. A microburet HMDE capillary can be used if the reservoir section is removed.

The wire is sharpened to a fine point which extends 1 mm into the capillary beyond where the capillary and the wire first make contact. A thin layer of electroplated gold improves the wetting of the wire by the mercury resulting in a good electrical connection.

The wire is sealed into a glass plunger with epoxy. The plunger is housed by a slightly larger glass tube which also contains the mercury. This larger tube is connected by Tygon tubing to the capillary. The connection is made rigid by yet another glass tube which fits over the Tygon tubing. This arrangement allows easy replacement of the capillary.

A 6 V continuous duty solenoid lifts the plunger a distance of 2 mm and can be activated by a computer controlled relay from 0.1 to 0.6 seconds to form various drop sizes. Drop mass varies linearly with solenoid activation time from 1 to 16 milligrams. The standard deviation of the drop mass is 0.1 milligram. After the necessary electrochemical measurements are made, a solenoid drop knocker strikes the electrode to dislodge the drop.

The electrode described here has been in use for 12 months. During that time the only maintenance required has been an occasional cleaning of the capillary tip. This can be done by activating the solenoid and applying a vacuum to the capillary tip. The rush of mercury through the capillary removes any clogs.

References


1. William M. Peterson, American Laboratory, 11, 69 (1979).
2. A. M. Bond, J. Electroanal. Chem., 118, 381 (1981).

Credit

This work supported by the Office of Naval Research.

List of Figures

Figure 1. Schematic Description of Automated Hanging Mercury
Drop Electrode

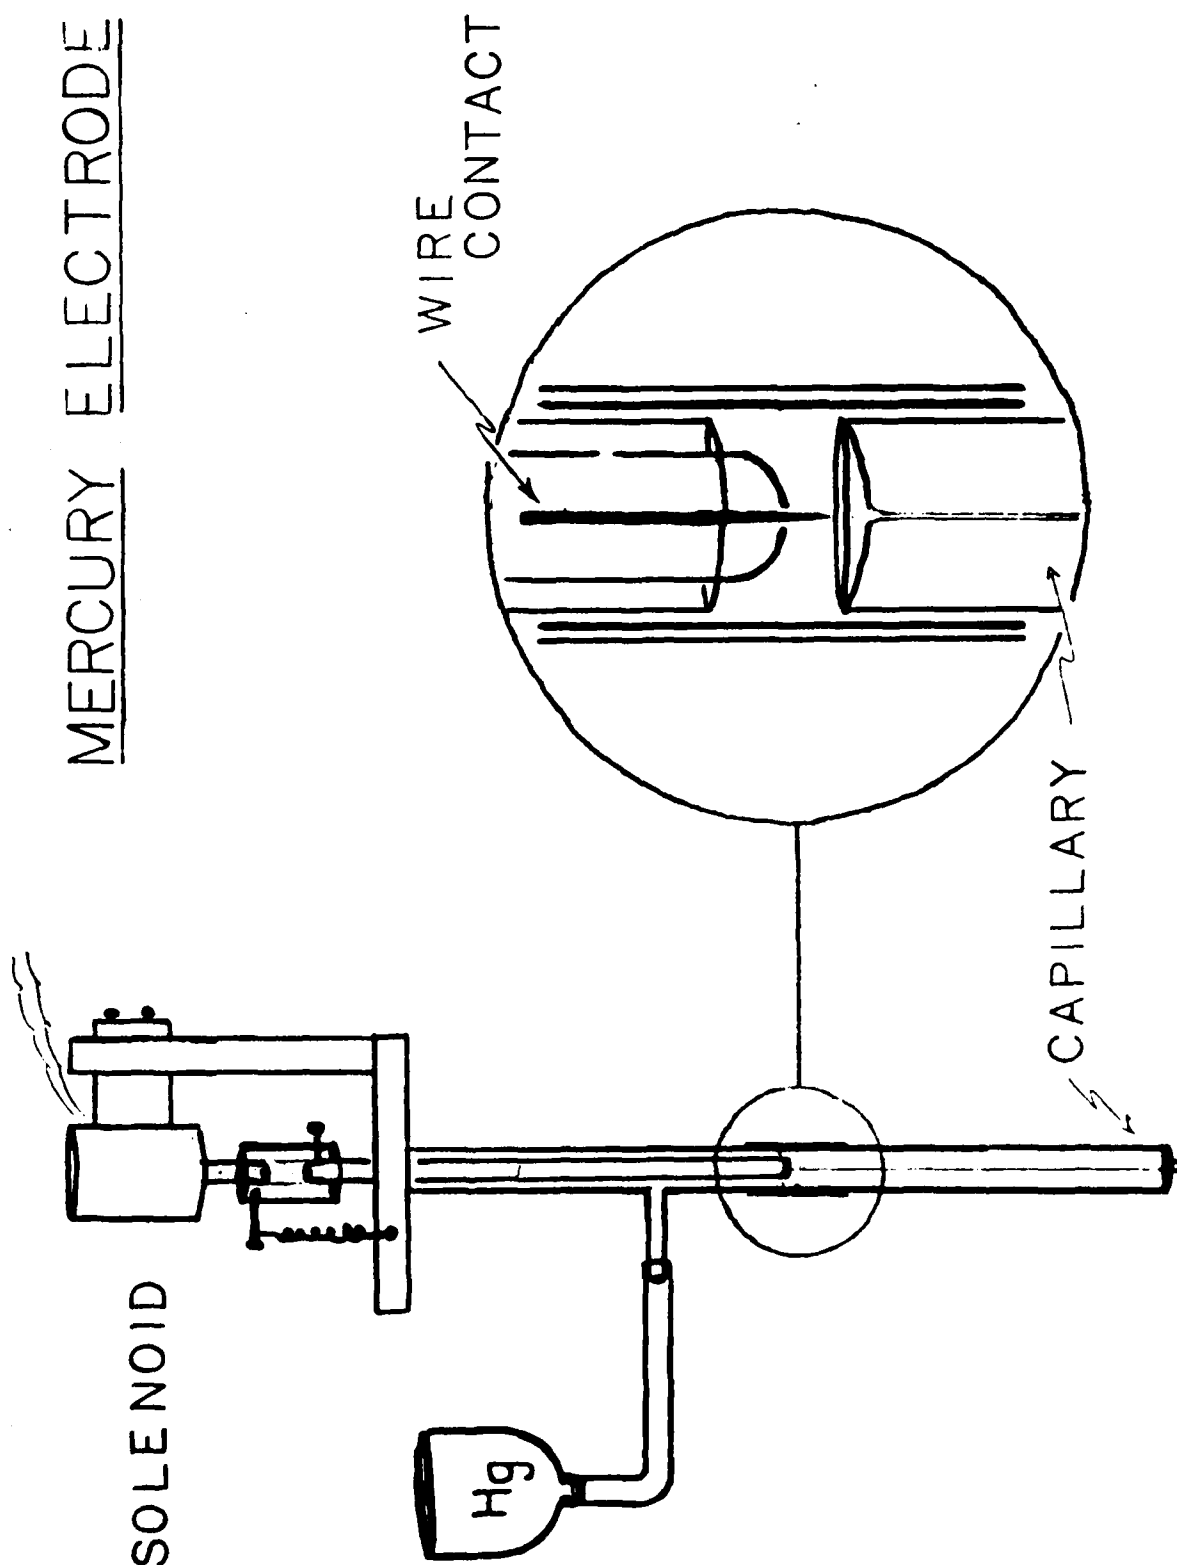

TECHNICAL REPORT DISTRIBUTION LIST, GEN

	<u>No. Copies</u>		<u>No. Copies</u>
Office of Naval Research Attn: Code 472 800 North Quincy Street Arlington, Virginia 22217	2	U.S. Army Research Office Attn: CRD-AA-IP P.O. Box 1211 Research Triangle Park, N.C. 27709	1
ONR Branch Office Attn: Dr. George Sandoz 536 So. Clark Street Chicago, Illinois 60605	1	Naval Ocean Systems Center Attn: Mr. Joe McCartney San Diego, California 92152	1
ONR Branch Office Attn: Scientific Dept. 715 Broadway New York, New York 10003	1	Naval Weapons Center Attn: Dr. A. B. Amster, Chemistry Division China Lake, California 93555	1
ONR Branch Office 1030 East Green Street Pasadena, California 91106	1	Naval Civil Engineering Laboratory Attn: Dr. R. W. Drisko Port Hueneme, California 93401	1
ONR Branch Office Attn: Dr. L. H. Peebles Building 114, Section D 666 Summer Street Boston, Massachusetts 02210	1	Department of Physics & Chemistry Naval Postgraduate School Monterey, California 93940	1
Director, Naval Research Laboratory Attn: Code 6100 Washington, D.C. 20390	1	Dr. A. L. Slafkosky Scientific Advisor Commandant of the Marine Corps (Code RD-1) Washington, D.C. 20380	1
The Assist Secretary of the Navy (R,E&S) Department of the Navy Room 4E736, Pentagon Washington, D.C. 20350	1	Office of Naval Research Attn: Dr. Richard S. Miller 800 N. Quincy Street Arlington, Virginia 22217	1
Commander, Naval Air Systems Command Attn: Code 310C (H. Rosenwasser) Department of the Navy Washington, D.C. 20360	1	Naval Ship Research and Development Center Attn: Dr. G. Bosmajian, Applied Chemistry Division Annapolis, Maryland 21401	1
Defense Documentation Center Building 5, Cameron Station Alexandria, Virginia 22314	12	Naval Ocean Systems Center Attn: Dr. S. Yamamoto, Marine Sciences Division San Diego, California 91232	1
Dr. Fred Saalfeld Chemistry Division Naval Research Laboratory Washington, D.C. 20375	1	Mr. John Boyle Materials Branch Naval Ship Engineering Center Philadelphia, Pennsylvania 19112	1

TECHNICAL REPORT DISTRIBUTION LIST, GEN

No.
Copies

Dr. Rudolph J. Marcus
Office of Naval Research
Scientific Liaison Group
American Embassy
APO San Francisco 96503

1

Mr. James Kelley
DTNSRDC Code 2803
Annapolis, Maryland 21402

1

TECHNICAL REPORT DISTRIBUTION LIST, 051C

	<u>No. Copies</u>		<u>No. Copies</u>
Dr. M. B. Denton Department of Chemistry University of Arizona Tucson, Arizona 85721	1	Dr. A. Zirino Naval Undersea Center San Diego, California 92132	1
Dr. R. A. Osteryoung Department of Chemistry State University of New York at Buffalo Buffalo, New York 14214	1	Dr. John Duffin United States Naval Postgraduate School Monterey, California 93940	1
Dr. B. R. Kowalski Department of Chemistry University of Washington Seattle, Washington 98105	1	Dr. G. M. Hieftje Department of Chemistry Indiana University Bloomington, Indiana 47401	1
Dr. D. L. Venezky Naval Research Laboratory Code 6130 Washington, D.C. 20375	1	Dr. Victor L. Rehn Naval Weapons Center Code 3813 China Lake, California 93555	1
Dr. H. Freiser Department of Chemistry University of Arizona Tucson, Arizona 85721	1	Dr. Christie G. Enke Michigan State University Department of Chemistry East Lansing, Michigan 48824	1
Dr. Fred Saalfeld Naval Research Laboratory Code 6110 Washington, D.C. 20375	1	Dr. Kent Eisentraut, MBT Air Force Materials Laboratory Wright-Patterson AFB, Ohio 45433	1
Dr. H. Chernoff Department of Mathematics Massachusetts Institute of Technology Cambridge, Massachusetts 02139	1	Walter G. Cox, Code 3632 Naval Underwater Systems Center Building 148 Newport, Rhode Island 02840	1
Dr. K. Wilson Department of Chemistry University of California, San Diego La Jolla, California 92037	1	Dr. George Morrison Department of Chemistry Cornell University Ithaca, New York 14850	1
		Dr. Isiah M. Warner Department of Chemistry Texas A&M University College Station, Texas 77840	1