

Insert list  
Name of author  
Number of pages

Classification

Security Classification

18 JUN 1982

DEVENUTO & ZEGNA

①

AD A117319

FIELD PRODUCTION OF PURIFIED STERILE WATER FROM AVAILABLE WATER SOURCES BY USING A PORTABLE APPARATUS (U)

\*FRANK DEVENUTO, PH.D.  
ANGELO ZEGNA

LETTERMAN ARMY INSTITUTE OF RESEARCH  
PRESIDIO OF SAN FRANCISCO, CA 94129

The development of portable equipment for the production of pure water from fresh pond, sea water, or other sources is important for military requirements in field situations. Also, it is necessary for many civilian activities whenever pure water is not available. The criteria for purity are influenced by the intended use of the water. Lake water which could be considered pure for swimming may not be suitable for drinking, and municipal water found pure for drinking is not considered pure for pharmaceutical preparations or for clinical use. The American Chemical Society, the American Society for Testing Materials, and the College of American Pathologists have specified various parameters for the purity of water. However, each of these agencies has proposed different standards (1), which apply for different purposes, and therefore, do not represent a uniform guide.

According to the criteria of the United States Pharmacopeia (USP) (2), sterile water for injection is a clear, colorless, odorless liquid; it is sterile without addition of antimicrobial agent or other substances, is pyrogen-free, and has a total solids content of 2 to 4 mg percent. In the usual urban environment, sterile water for injection is readily available; however, in field situations or in areas remote from supply sources, the procurement of purified water could present logistic difficulties. The problems associated with transportation, storage, and supply of large quantities of pure sterile water can be overcome by its production in situ by using any available source of water which is purified by a simple inexpensive process. Purified, injectable water may be needed in military field situations as a diluent for pharmaceutical formulations, for preparation of sterile saline solutions, for reconstitution of lyophilized hemoglobin for fluid therapy (3-5), for solubilization of preservatives to be added to human blood for prolongation of its shelf life (6), for preparation of solutions for the rejuvenation of outdated red blood cells (7) or for other purposes.

DTC FILE COPY

DTIC  
classification

DTIC  
ELECTE  
JUL 20 1982  
S D  
B

DISTRIBUTION STATEMENT A  
Approved for public release  
Distribution Unlimited

82 07 19 284

Insert last  
name of author  
or(s) here



Security  
Classification

Start here  
for all  
pages

DEVENTIO & ZEGNA

title of

The data presented here represent the results of the evaluation of a portable, compact, single unit apparatus used for the purification of sea water, pond water, and human urine, and the production of purified water that appears to satisfy the criteria for USP grade water for injection except for slightly higher content of total solids. Human urine was used in these studies to evaluate the potential of the purification process in extreme situations, such as a desert environment, where urine might be the only available source of water.

is first  
page type  
title of  
paper here

### PURIFICATION OF WATER BY A PORTABLE APPARATUS

author  
title of  
paper here

Three different sources of water were used for purification. Sea water was collected from the Marina at Fort Baker, California in the San Francisco Bay Area. Pond water was taken from the lagoon in the front of the Palace of Fine Arts in San Francisco. Pooled human urine was collected during a 24-hr period from several male laboratory workers. The apparatus used for the purification of water from the three different sources is manufactured by Allied Water Corporation, San Francisco, California. This portable SweetWater™ System, Model 200, enclosed in a fiberglass case, measures 45.7 x 78.7 cm, has a weight of 62 kg, and an output of 757 liters of water per day. The system is equipped with a water pump which, in the set-up used for these experiments, pumps the source water through three serial filters made of pure bleached cotton, cellulose, and activated carbon, then through a reverse osmosis purifier consisting of an acetate micropore filter, followed by a filter of activated carbon, a source of ultraviolet light, and finally, through an outlet provided with a sampling device. A

title of

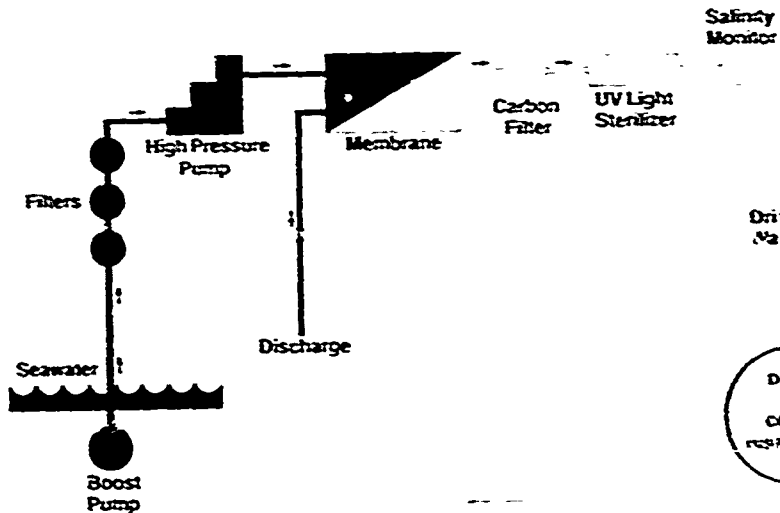


Fig. 1. Flow diagram of water purification process.

Security  
Classification

Accession For		
NTIS GRA&I		<input checked="" type="checkbox"/>
DTIC TAB		<input type="checkbox"/>
Unannounced		<input type="checkbox"/>
Justification:		
DTIC	By	
COPY	Distribution/	
RESPECTED	Availability Codes	
	Avail and/or	
Dist	Special	
A		

Insert last  
name of au-  
thor(s) here

→ DEVENUTO & ZECNA

Start here  
for all

ages

After the  
first

7 first

page type

Title of

paper here

Author

Classification

City, State

First line

→ flow diagram of the water purification process is shown in Figure 1. In some experiments, a millipore Twin-90 sterile 0.22  $\mu$  filter was connected to the outlet system prior to collection of purified water to remove bacterial contamination.

The acetate micropore filter incorporated in the reverse osmosis purifier lasts for two years or longer if properly maintained. It is continuously rinsed by water pumped into the apparatus, thus preventing the accumulation of particulate matter on the filter. The three serial filters placed before the reverse osmosis purifier and the activated carbon filter which follows remain effective for a period of time dependent on the impurities present in the water source used. Purification of sea water in a continuous operation requires replacement or regeneration after one week for the first-in-line filter and after two weeks for the other filters in order to obtain purified water of consistent high quality. The apparatus is portable, and can be used anywhere water is needed as long as a water supply of some source is available. It can be modified to use different power sources such as a combustion engine or even manpower.

### RESULTS

The ion content of the water samples from sea water, fresh pond water, and human urine before and after purification are shown in Table I. The

TABLE I  
ION CONTENT\* BEFORE AND AFTER WATER PURIFICATION

	USP	SEA		POND		URINE	
		Before	After	Before	After	Before	After
Na (mg/dl) <sup>†</sup>	0.0	1,023.05	16.39	19.54	1.15	188.52	2.30
K (mg/dl) <sup>†</sup>	0.0	39.10	0.73	2.35	0.39	174.00	1.17
Ca (mg/dl) <sup>†</sup>	0.2	22.80	0.31	2.65	0.05	8.30	0.30
Mg (mg/dl) <sup>†</sup>	0.59	14.70	0.25	1.12	0.00	4.52	0.35
Cl (mg/dl) <sup>†</sup>	0.0	1,730.11	13.26	9.08	0.00	5.67	1.06
P (mg/dl) <sup>†</sup>	0.0	0.0	0.0	0.95	0.20	105.20	0.30

\*Values of 0.0 represent levels below the limits of detection, which in mg/dl are: 1.1 for Na, 0.08 for K, 0.9 for Cl and 0.05 for Ca, Mg, and P.

<sup>†</sup>ppm = data in Table x 10

1-2

Classification

1-2

1-2

1-2

1-2

1-2

1-2

1-2

1-2

1-2

1-2

1-2

SIAM Security Classification

Insert last  
line of sum-  
mary here



→ DEVENUTO & ZEGNA

Start here  
for all

ages  
after the  
first

In first  
page type  
title of  
paper here

→ analysis of a sample of USP water is also included in this Table for comparison. Sea water with a high Na and Cl content, as expected, is purified to the extent that, with a single passage through the purification system, more than 98% of Na and more than 99% of Cl are removed. Na, K, and P, which are present in elevated amounts in human urine, are also reduced by the purification procedure to 1 to 2% of the initial value. All other ions indicated in the Table are reduced considerably independently of the source of water used. The detection limits of the methods used are indicated in Table I.

lines  
of  
text

→ Table II shows the metal content in the water samples before and after purification. In some samples the metal content before purification was below the limit of sensitivity of the assay (Table II). However, in those

first line

TABLE II  
METAL CONTENT BEFORE AND AFTER WATER PURIFICATION

	USP	SEA		POND		URINE	
		Before	After	Before	After	Before	After
Cu (ppm)	<0.06	<0.06	<0.06	<0.05	<0.06	0.71	<0.06
Fe (ppm)	<0.11	0.38	<0.11	<0.11	<0.11	0.34	<0.11
Mn (ppm)	<0.05	0.07	<0.05	<0.05	<0.06	<0.06	<0.06
Zn (ppm)	0.024	0.059	0.02	0.043	<0.011	0.526	0.066

instances where significant amounts were present, removal was achieved by the purification procedure, except for zinc in the urine sample where a decrease of 87.5% was observed.

Conductivity, electrical resistance, osmolality, and pH of the water samples before and after purification are shown in Table III. With a considerable decrease of ion content, as observed in Table I, a corresponding decrease in electrical conductance and parallel increase in electrical resistance was obtained, as expected. The decrease in osmolality after purification also reflects the removal of osmotic material from the water of different sources. The difference observed in the pH of pond water before and after purification may indicate loss of CO<sub>2</sub> dissolved in fresh pond water and/or removal of other alkaline material.

In Table IV, the spectrophotometric absorbance between 220 and 650 nm is indicative of the presence of organic or pigmented material with light

CONFIDENTIAL  
Classification  
mark

Insert last  
name of au-  
thor(s) here

→ DEVENUTO & ZEGNA

Start here  
for all

pages

after the  
first

In first  
page type

title of  
paper here

Author

Affiliation,  
City, State

First line

STAMP Security  
Classification  
here

TABLE III  
CONDUCTIVITY, ELECTRICAL RESISTANCE, OSMOLALITY, AND pH  
BEFORE AND AFTER WATER PURIFICATION

	USP	SEA		POND		URINE	
		Before	After	Before	After	Before	After
Conductivity (mhos)	2.8	37,000	750	1,000	29	11,000	200
Electrical Resistance (ohms)	400,000	30	1,400	1,000	37,000	95	5,200
Osmolality (mOsm/kg)	1	925	15	18	3	426	33
pH	7.45	7.20	7.60	9.2	6.30	6.45	6.25

TABLE IV  
ABSORBANCE, FLOURESCENCE, TOTAL PROTEIN, AND TOTAL  
MATTER BEFORE AND AFTER WATER PURIFICATION

	USP	SEA		POND		URINE	
		Before	After	Before	After	Before	After
Absorbance (220-650nm)	0.0	0.0	0.0	220-280nm	0.0	280nm	0.0
Flourescence (In 340/465 <sup>*</sup> )	0.0	16.5	0.0	>100	0.0	>100	0.0
Total Protein (g/dl)	—	—	—	—	—	0.15	0.0
Total Matter (g/dl)	0.003	4.05	0.034	0.17	0.007	3.02	0.20

\*Intensity units at 340nm excitation and 465nm emission.

absorbing characteristics in the ultraviolet or visible region. Pond water showed absorbance in the 220 to 280 nm region and uring at 280 nm before purification. After purification, the light absorbing material was removed since no absorbance was observed. Significant fluorecence was measured in sea water, and to a greater extent, in pond water and urine before purification. However, this fluorecence was not present in samples of purified water. No significant amounts of protein could be detected in the sea or pond water; the protein content determined in the urine sample was absent after the process of purification. The residue remaining after evaporation of 50 ml of water from the three different sources before and after purification is shown quantitatively in Table IV and is illustrated in Figure 2 (for sea water), Figure 3 (for pond water), and Figure 4 (for human urine).

Figure 5 depicts the results of the gas chromatographic analysis of samples of sea water and urine before and after purification and of a

Stamp

Classification

Stamp

Stamp

Stamp

Stamp

Stamp

Stamp

Stamp

ns of last  
one of sur-  
er water

DEVENUTO & ZEGNA

Start here  
for all

→  
→  
→

a first  
age type  
title of  
paper here

→  
→  
→  
→

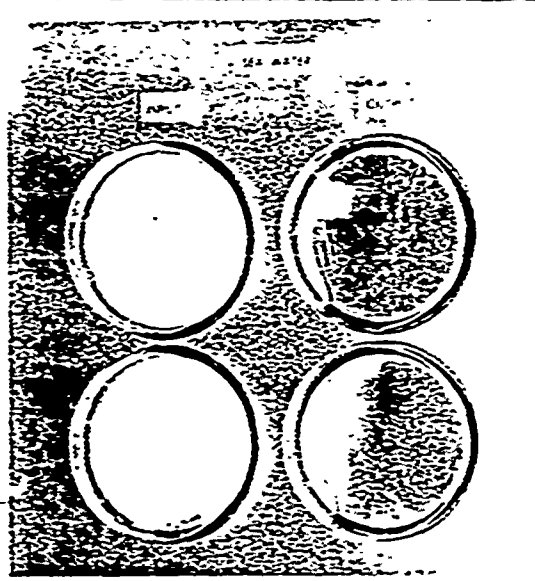


Fig. 2. Residue after evaporation of water from 50 ml sea water before and after purification. In duplicate.



Fig. 3. Residue after evaporation of water from 50 ml fresh pond water before and after purification. In duplicate.

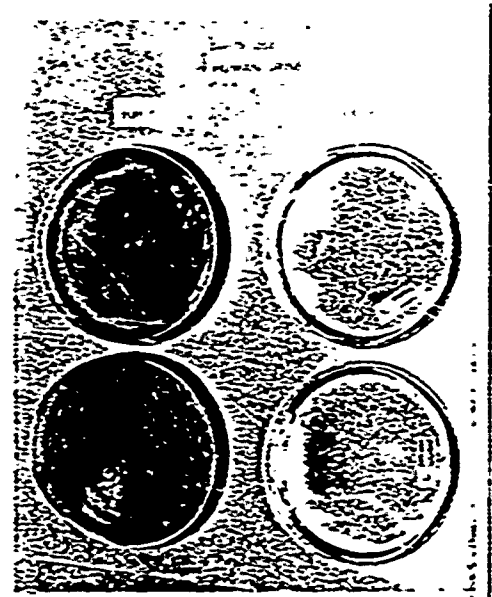


Fig. 4. Residue after evaporation of water from 50 ml human urine before and after purification. In duplicate.

Insert last  
name of au-  
thor(s) here

DEVENUTO & ZEGNA

Start here  
for all  
pages  
after the  
first

a first  
page type  
title of  
paper here

Author  
of Institu-  
tion, State

First line

GAS CHROMATOGRAPHY

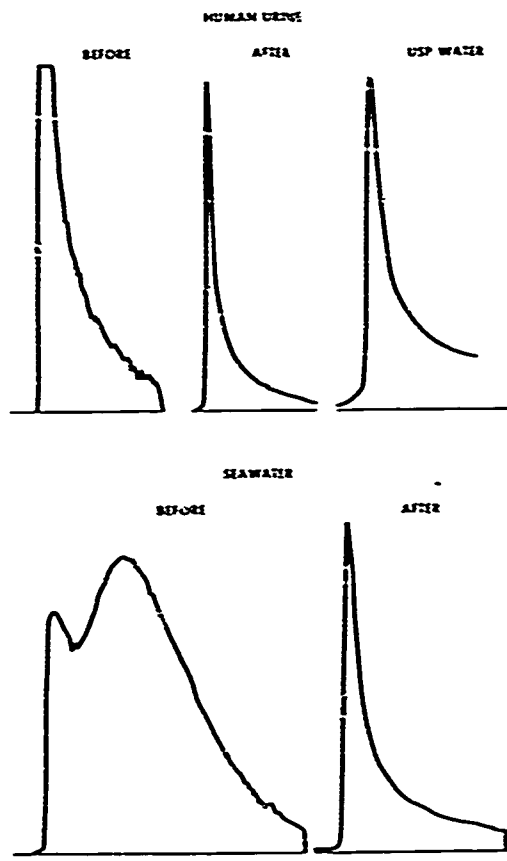


Fig. 5. Gas chromatographic analysis of sea water and human urine before and after purification. A pattern of sample of USP water is also illustrated. The ordinate indicates the frequency signals of the chromatographic detector and the abscissa the retention time of the gas products.

sample of USP water. Sea water or urine, prior to purification, shows patterns indicative of the presence of several impurities, but after purification the pattern is similar to that obtained with USP water. Purified water obtained from the three different sources appears as a clear, colorless, odorless liquid.

All the data obtained in Tables I to IV and Figures 2 to 5 are essentially the same with or without addition of the Twin-90, 0.22  $\mu$  millipore filter prior to collection of the purified samples. The addition of this sterile filter, however, has a remarkable effect on the bacteriological

SECRET  
Classification

STAMP Security  
Classification  
here

insert last  
name of author  
(short) here

→ DEVENUTO & ZEGNA

Start here  
for all  
pages  
from the  
first

in first  
page type  
title of  
paper here

author  
affiliation  
city, state

first line

TABLE V  
BACTERIAL ANALYSIS. COLONY FORMING UNITS PER ML.

	Before Purification	After Purification	
		Without Twin-90	With Twin-90
Sea Water	1.1*	1.2**	0.0
Pond Water	4.5 x 10 <sup>3</sup> ***	3.1 x 10 <sup>3</sup> ***	0.0
Urine	3.0 x 10 <sup>4</sup> †	1.2†	0.0

Bacteria Identified:

\*Klebsiella pneumoniae, Enterobacter aerocolerans, Serratia liquefaciens

\*\*Enterobacter aerocolerans and Serratia liquefaciens

\*\*\*Proteus

†Bacillus, Escherichia coli, Pseudomonas aeruginosa, Pseudomonas fluorescens, Proteus mirabilis, Enterobacter aerocolerans

‡Pseudomonas

TABLE VI  
DETECTION OF PYRENEIC BACTERIAL ENDOTOXIN BEFORE AND  
AFTER WATER PURIFICATION

	Concentration	Reaction		Result
		Duplicate	Result	
positive control	50.0 µg/ml	+	+	positive
(E. coli endotoxin)	0.5	+	+	positive
	0.1	+	+	positive
	0.05	=	=	positive
	0.025	-	-	negative
	0.0125	-	-	negative
	0.006	-	-	negative
Control (DW water)		-	-	negative
Sea water (before)		=	=	positive
	(after, without Twin-90)	=	=	positive
	(after, with Twin-90)	-	-	negative
Pond water (before)		+	+	positive
	(after, without Twin-90)	=	=	positive
	(after, with Twin-90)	-	-	negative
Urine (before)		+	+	positive
	(after, without Twin-90)	=	=	positive
	(after, with Twin-90)	-	-	negative

STAMP

Security  
Classification  
Information

Classification

insert last  
page of un-  
reported part



→ DEVENUTO & ZEGNA

Start here  
for all

pages →

assays. The results of these tests are shown in Table V. Water obtained from the three different sources is contaminated by different bacteria with very heavy contamination observed in pond water and urine. Purification without addition of the sterile filter shows little or no effect on the elimination of bacterial contamination from sea or pond water, although bacteria present in human urine are considerably reduced. However, the addition of the sterile filter prior to collection of water assures absence of bacterial contamination in the purified water.

Table VI →

shows the results of the detection of pyrogenic bacterial endotoxin in samples of water before and after purification. The limit of sensitivity of the test is indicated by data of the positive control, represented by *Escherichia coli* endotoxin; this limit is reached at a concentration of 0.05 ng/ml. Based on earlier assays, a pyrogenic response was obtained in rabbits at a concentration of 0.5 ng/ml. Prior to purification, water from the three different sources gave a positive reaction which is present also in purified water samples obtained without addition of a sterile filter. However, all the water samples collected after filtration through the sterile filter show a negative reaction, indicating removal of pyrogenic bacterial endotoxin. A negative reaction was observed also in the USP control water sample.

### CONCLUSIONS

The data obtained in our studies demonstrate that the purification system used satisfies all criteria for USP grade injectable water, except one: the limits of total solids. However, the purified water is non-pyrogenic, clear, colorless, odorless, and it is sterilized without addition of antimicrobial agents or other substances. The ion, metal content, and organic material present in human urine, pond water, and sea water are reduced considerably or completely removed by a single passage through the system. Although the total solids in the purified water exceed the limit of 2 to 4 mg% established for USP water, sodium and chlorine ions represent 96% and 64% of the total solids present in water purified from sea water and urine, respectively. However, these ions are generally added (900 mg sodium chloride per 100 ml) in order to make isotonic water for injection. The results indicate also that organic substances, with spectrophotometric absorption in the ultraviolet and visible regions, fluorescent compounds and protein material present in the water source are removed by the purification process. It is important to emphasize that this purification system, as presently available, will not manufacture water completely sterile and free of pyrogenic bacterial endotoxins, but requires the addition of a small porosity, sterile, in-line filter to produce water without bacterial contamination.

It appears that the reverse osmosis process is efficient in the production of purified water and it has been utilized for the preparation of

USP  
Classification  
Date

insert  
me of  
start here  
for all  
page type  
title of  
paper here

DEVENUTO & ZEGNA

drinking water in a desalinization project (8). The system evaluated in these studies represents a multipurpose water purification process which could be useful in many non-military applications such as disaster sites where sources of water are contaminated, at construction sites, off-shore drilling platforms, on commercial and pleasure boats, and other activities where pure water is needed but not available.

REFERENCES

1. Dharan M: Standards and methods to obtain reagent grade water. Lab Manag 16:39-42, 1978.
2. The United States Pharmacopeia, USF Convention, Inc., Rockville, MD, 19th revision, p. 540, 1975.
3. DeVenuto F, Moores WY, Zegna AI, Busse KR: Total and partial blood exchange in the rat with hemoglobin prepared by crystallization. Transfusion 17:555-562, 1977.
4. DeVenuto F, Zegna AI, Busse KR: Lyophilization of crystalline hemoglobin solution and exchange transfusions with lyophilized-reconstituted hemoglobin. Surg Gynecol Obstet 148:69-75, 1979.
5. DeVenuto F, Zuck TF, Zegna AI, Moores WY: Characteristics of stroma-free hemoglobin prepared by crystallization. J Lab Clin Med 89:509-516, 1977.
6. Moore GL, Ledford ME, Brummell MR, Brooks DE: The potential use of dihydroxyacetone for improved 2,3-DPG maintenance in red cell storage. Transfusion 20:24-31, 1980.
7. Valeri CR, Zaroulis CG: Rejuvenation and freezing of outdated stored human red cells. N Engl J Med 287:1307-1313, 1972.
8. Schnitt, RP: Military requirements for water supply. First Desalination Congress of the American Continent 1:1-8 (V-2), 1976.

120  
120  
120  
120  
120  
120  
120  
120  
120  
120

Insert last  
name of au-  
thor(s) here

DEVENUTO AND ZEGNA

Type TITLE  
here

\*TITLE: Field Production of Purified Sterile Water From Available  
Water Sources by Using a Portable Apparatus (U)

\*FRANK DEVENUTO, Ph.D., ANGELO I. ZEGNA  
Letterman Army Institute of Research  
Presidio of San Francisco, CA 94129

\*ABSTRACT:

first line

In a normal urban environment, sterile water for injection is readily available; however, in field situations or in areas remote from supply sources, the procurement of purified water could present logistic difficulties. A 60 kg, compact, self-contained, portable water purification apparatus, adapted with a sterile micropore filter, has been evaluated for purification of sea water, pond water, or human urine. The process is based on the reverse osmosis procedure and can use various power sources. The results indicate that polluted water can be purified by a single passage through the system, as demonstrated by considerable reduction of ions (>1 percent), and complete elimination of metal content and organic matter present in the source of water. The water obtained is clear, colorless, odorless, non-pyrogenic, is made sterile without addition of antimicrobial agents or other substances, and appears to satisfy the criteria for USP grade water for injection except for the limits on total solids. The residual solids are sodium and chloride ions which are common constituents of parenteral solutions. This purification process can be used anywhere water is needed as long as a water supply from some source is available. It represents a multipurpose water purification system which is capable of meeting the medical needs of the military in its various fields of operation, and could also be very useful in many non-medical situations.

\*BIOGRAPHY:

start  
ere

\*PRESENT ASSIGNMENT: Supervisory Research Chemist, Letterman Army  
Institute of Research

start  
ere

\*PAST EXPERIENCE: Research Chemist, Chief Section, Division Director,  
U.S. Army Medical Research Laboratory, Fort Knox, Kentucky, 1953-1974.

start  
ere

\*DEGREES HELD: Ph.D., Organic-Biological Chemistry, University of  
Rome, Rome, Italy, 1951.