

12

# DEVELOPMENT OF THE CAPTURED FUELS TEST KIT

AD-A166 952

INTERIM REPORT  
BFLRF-No. 211 ✓

By

S.R. Westbrook  
L.L. Stavinoha  
J.M. Burkes  
J.G. Barbee  
L.L. Bundy

DTIC  
ELECTE  
MAY 08 1986  
S D

Belvoir Fuels and Lubricants Research Facility (SwRI)  
Southwest Research Institute  
San Antonio, Texas

and

W.R. Williams  
U.S. Army Belvoir Research, Development  
and Engineering Center  
Materials, Fuels and Lubricants Laboratory  
Fort Belvoir, Virginia

Contract No. DAAK70-85-C-0007

Approved for public release; distribution unlimited

December 1985

86 5 8 008

### **Disclaimers**

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorized documents.

Trade names cited in this report do not constitute an official endorsement or approval of the use of such commercial hardware or software.

### **DTIC Availability Notice**

Qualified requestors may obtain copies of this report from the Defense Technical Information Center, Cameron Station, Alexandria, Virginia 22314.

### **Disposition Instructions**

Destroy this report when no longer needed. Do not return it to the originator.

AD-A166952

# REPORT DOCUMENTATION PAGE

|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |       |                                                  |                                                                                                  |                                                                               |                                |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------|--------------------------------------------------|--------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------|--------------------------------|
| 1a. REPORT SECURITY CLASSIFICATION<br>Unclassified                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |       |                                                  | 1b. RESTRICTIV MARKINGS<br>None                                                                  |                                                                               |                                |
| 2a. SECURITY CLASSIFICATION AUTHORITY<br>N/A                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |       |                                                  | 3. DISTRIBUTION/AVAILABILITY OF REPORT<br>Approved for public release;<br>distribution unlimited |                                                                               |                                |
| 2b. DECLASSIFICATION/DOWNGRADING SCHEDULE                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |       |                                                  |                                                                                                  |                                                                               |                                |
| 4. PERFORMING ORGANIZATION REPORT NUMBER(S)<br><br>Interim Report BFLRF No. 211                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |       |                                                  | 5. MONITORING ORGANIZATION REPORT NUMBER(S)                                                      |                                                                               |                                |
| 6a. NAME OF PERFORMING ORGANIZATION<br>Belvoir Fuels and Lubricants<br>Research Facility (SwRI)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |       | 6b. OFFICE SYMBOL<br>(If applicable)             |                                                                                                  | 7a. NAME OF MONITORING ORGANIZATION                                           |                                |
| 6c. ADDRESS (City, State, and ZIP Code)<br>Southwest Research Institute<br>6220 Culebra Road<br>San Antonio, TX 78251                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |       |                                                  | 7b. ADDRESS (City, State, and ZIP Code)                                                          |                                                                               |                                |
| 8a. NAME OF FUNDING/SPONSORING<br>ORGANIZATION<br>Belvoir Research, Development<br>and Engineering Center                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |       | 8b. OFFICE SYMBOL<br>(If applicable)<br>STRBE-VF |                                                                                                  | 9. PROCUREMENT INSTRUMENT IDENTIFICATION NUMBER<br><br>DAAK70-C-85-0007; WD 8 |                                |
| 8c. ADDRESS (City, State, and ZIP Code)<br><br>Ft. Belvoir, VA 22060-5606                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |       |                                                  | 10. SOURCE OF FINDING NUMBERS                                                                    |                                                                               |                                |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |       |                                                  | PROGRAM<br>ELEMENT NO.<br>62733                                                                  | PROJECT<br>NO. 1L762733<br>AH20                                               | WORK UNIT<br>ACCESSION NO.     |
| 11. TITLE (Include Security Classification)<br><br>Development of the Captured Fuels Test Kit (U)                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |       |                                                  |                                                                                                  |                                                                               |                                |
| 12. PERSONAL AUTHOR(S)<br>Westbrook, S.R.; Stavinoha, L.L.; Burkes, J.M.; Barbee, J.G.; Bundy, L.L.; and Williams, W.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |       |                                                  |                                                                                                  |                                                                               |                                |
| 13a. TYPE OF REPORT<br>Interim                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |       | 13b. TIME COVERED<br>FROM May 85 TO Jan 86       |                                                                                                  | 14. DATE OF REPORT (Year, Month, Day)<br>1986 January                         |                                |
| 15. PAGE COUNT<br>32                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |       |                                                  |                                                                                                  |                                                                               |                                |
| 16. SUPPLEMENTARY NOTATION                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |       |                                                  |                                                                                                  |                                                                               |                                |
| 17. COSATI CODES                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |       |                                                  | 18. SUBJECT TERMS (Continue on reverse if necessary and identify by block number)                |                                                                               |                                |
| FIELD                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     | GROUP | SUB-GROUP                                        | Field Test, Test Kit, Viscosity, Density, Fuel                                                   |                                                                               |                                |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |       |                                                  |                                                                                                  |                                                                               |                                |
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |       |                                                  |                                                                                                  |                                                                               |                                |
| 19. ABSTRACT (Continue on reverse if necessary and identify by block number)<br><br>This report details development of a portable test kit to allow an unskilled operator to quickly judge the usability of an undocumented fuel source in a compression ignition engine and in turbine-powered ground equipment. The test kit provides a means to measure a fuel's visual appearance, density, and viscosity. Cutoff limits were chosen for each of these parameters based on justifiable criteria. Novel approaches for rolling ball viscometer reference tubes, a density indicator, and temperature compensation for the density test were developed. |       |                                                  |                                                                                                  |                                                                               |                                |
| 20. DISTRIBUTION/AVAILABILITY OF ABSTRACT<br><input checked="" type="checkbox"/> UNCLASSIFIED/UNLIMITED <input type="checkbox"/> SAME AS RPT. <input type="checkbox"/> DTIC USERS                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |       |                                                  | 21. ABSTRACT SECURITY CLASSIFICATION<br>Unclassified                                             |                                                                               |                                |
| 22a. NAME OF RESPONSIBLE INDIVIDUAL<br>Mr. F.W. Schaekel                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |       |                                                  | 22b. TELEPHONE (Include Area Code)<br>(703) 664-3576                                             |                                                                               | 22c. OFFICE SYMBOL<br>STRBE-VF |

## FOREWORD

This work was conducted at the Belvoir Fuels and Lubricants Research Facility (SwRI) located at Southwest Research Institute (SwRI), San Antonio, TX, under Contract No. DAAK70-85-C-0007 during the period May 1985 through January 1986. The work was funded by the U.S. Army Belvoir Research, Development and Engineering Center, Ft. Belvoir, VA, with Mr. F.W. Schaekel (STRBE-VF) as the Contracting Officer's representative and Mr. M.E. LePera, Chief of Fuels and Lubricants Division (STRBE-VF), as the project technical monitor.

|                    |                                            |
|--------------------|--------------------------------------------|
| Accession For      |                                            |
| NTIS CRA&I         | <input checked="checked" type="checkbox"/> |
| DTIC TAB           | <input type="checkbox"/>                   |
| Unannounced        | <input type="checkbox"/>                   |
| Justification      |                                            |
| By                 |                                            |
| Distribution /     |                                            |
| Availability Codes |                                            |
| Dist               | Avail and/or Special                       |
| A-1                |                                            |



## ACKNOWLEDGEMENTS

The helpful assistance of MSgt Carstens, U.S. Army TRADOC/Quartermaster School, Ft. Lee, VA, in the conceptualization of the Captured Fuels Test Kit is gratefully acknowledged. The dedicated technical support of Belvoir Fuels and Lubricants Research Facility (SwRI) staff members C. Nystrom, D. Munoz, E. Lyons, D. Patterson, M. Lara, J. Cantu, C. Sturrock, L. Pierce, and J. Pryor is recognized in the successful completion of this program.

## TABLE OF CONTENTS

| <u>Section</u>                                                     | <u>Page</u> |
|--------------------------------------------------------------------|-------------|
| I. INTRODUCTION AND BACKGROUND .....                               | 5           |
| II. DESIGN GOALS FOR THE CFTK .....                                | 5           |
| III. CHOICE OF FUEL PARAMETERS TO BE MEASURED BY THE<br>CFTK ..... | 6           |
| IV. PRELIMINARY DESIGN CONCEPTS .....                              | 8           |
| A. Density .....                                                   | 8           |
| 1. Calibrated Spheres .....                                        | 9           |
| 2. Hydrometer .....                                                | 9           |
| 3. Buoyant Pointer .....                                           | 9           |
| B. Viscosity .....                                                 | 9           |
| 1. Calibrated Orifice .....                                        | 10          |
| 2. Falling Ball .....                                              | 11          |
| C. Visual Appearance (Clean and Bright) .....                      | 12          |
| 1. White Beaker .....                                              | 12          |
| 2. Comparator .....                                                | 12          |
| V. EVOLUTION OF THE CURRENT CFTK .....                             | 13          |
| A. Density Test .....                                              | 13          |
| B. Viscosity Test .....                                            | 17          |
| C. Visual Appearance .....                                         | 26          |
| VI. CFTK CONFIGURATION .....                                       | 27          |
| VII. CARRYING CASE .....                                           | 29          |
| VIII. QUALITY ASSURANCE TESTING .....                              | 29          |
| IX. CONCLUSIONS AND RECOMMENDATIONS .....                          | 32          |

## LIST OF ILLUSTRATIONS

| <u>Figure</u> |                                                                                                                                                                | <u>Page</u> |
|---------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------|
| 1             | Viscosity of Gasoline and Diesel Fuel Blends .....                                                                                                             | 8           |
| 2             | Approach for Using Calibrated Spheres to Measure Density .....                                                                                                 | 9           |
| 3             | Calibrated Orifice Versus Actual Viscosity .....                                                                                                               | 11          |
| 4             | Approach for Using Comparator for Visual Appearance .....                                                                                                      | 13          |
| 5             | Final Design of CFTK Density Pointer .....                                                                                                                     | 15          |
| 6             | Diagram of CFTK Viscosity Test .....                                                                                                                           | 18          |
| 7             | Viscosity Reference Tube .....                                                                                                                                 | 19          |
| 8             | Photograph of a Series of Diesel Fuel Samples Containing<br>10 Vol% Deionized Water (Samples 1-7) and the Indicated<br>Quantity of Surfactant (1-7 Vol%) ..... | 26          |
| 9             | Exploded View of the Final CFTK Configuration .....                                                                                                            | 28          |

## LIST OF TABLES

| <u>Table</u> |                                                                                                                                                                   | <u>Page</u> |
|--------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------|
| 1            | Specification Determination of Minimum and Maximum Limits<br>for Captured Fuel Test Kit .....                                                                     | 7           |
| 2            | Calibrated Orifice Flow Times and Kinematic Viscosity at<br>Various Temperatures .....                                                                            | 10          |
| 3            | Density Changes at Various Temperatures as Calculated<br>From ASTM D 1298, Density at 15°C .....                                                                  | 16          |
| 4            | Falling Ball Method at Various Tilts and Temperatures Using<br>Low Viscosity Reference Fuel .....                                                                 | 21          |
| 5            | Falling Ball Method at Various Tilts and Temperatures Using<br>High Viscosity Reference Fuel .....                                                                | 21          |
| 6            | Falling Ball Method at Various Tilts and Temperatures Using<br>1.09 cSt Viscosity Fuel .....                                                                      | 22          |
| 7            | Falling Ball Method Using Various Test Fuels .....                                                                                                                | 23          |
| 8            | Falling Ball Method at Various Tilts and Temperatures Using<br>0.97 cSt Viscosity Fuel .....                                                                      | 23          |
| 9            | Falling Ball Method at Various Tilts and Temperatures Using<br>2.2 cSt Viscosity Fuel .....                                                                       | 24          |
| 10           | Falling Ball Method at Various Tilts and Temperatures Using<br>3.2 cSt Viscosity Fuel .....                                                                       | 24          |
| 11           | Fall Times for Balls of Various Densities and Various Fall<br>Lengths .....                                                                                       | 25          |
| 12           | Results of Quality Assurance Testing of Six CFTK<br>Prototypes With Iso-Octane<br>Results of Quality Assurance Testing of Six CFTK<br>Prototypes With 85/15 ..... | 30          |
| 14           | Results of Quality Assurance Testing of Six CFTK<br>Prototypes With Diesel Control .....                                                                          | 31          |
| 15           | Results of Quality Assurance Testing of Six CFTK<br>Prototypes With 35/65 .....                                                                                   | 31          |

## I. INTRODUCTION AND BACKGROUND

A simple fuel tester is required to enable isolated combat units to identify field expedient fuels for use in ground combat vehicles. The current systems of petroleum testing kits, sets, and laboratories are either too complex or too large to be deployed and used by combat vehicle crewmen. As a result, there exists a need to provide a highly portable, simplistic device which the combat crewman can quickly use to determine fuel type and relative quality. Since the Army's turbine-powered ground equipment are highly fuel tolerant, it was concluded that any emergency or field-expedient fuel determined by the Captured Fuels Test Kit (CFTK) to be suitable for use in Army diesel engines would also be suitable for use in the turbine-powered ground equipment.

This CFTK will provide measurable increases in reliability when evaluating field expedient petroleum fuels.

## II. DESIGN GOALS FOR THE CFTK TESTER

In view of the stringent requirements for battlefield conditions, the following design concepts were incorporated:

- One person operation
- Compact, portable
- No electronic components
- No external power source required
- Minimum training time, easy to use
- Generally free from potential operating problems
- Maintenance free
- Require no calibration
- Rugged, droppable
- Must not leak fuel
- Does not allow dirt inside density/viscosity tester since debris can interfere with close tolerances in sample viscosity tube
- Operational in temperature range of 0°C to 40°C
- Able to use while wearing MOPP gear



- Requires fuel sample size of 500 mL or less
- Total test duration time not to exceed 5 minutes
- Uses only fuel-resistant materials for tester components
- Compatible with all hydrocarbon fuels
- No logistical support
- Minimum time to fill and drain
- Minimum shelf life of 10 years

### III. CHOICE OF FUEL PARAMETERS TO BE MEASURED BY THE CFTK

Ideally, the CFTK would be designed to provide a measure of the performance of a given fuel, in a compression-ignition engine, such as cetane number. However, tests for cetane number, or even calculated cetane index, do not meet the requirements placed on this test kit (i.e., field portable, quick, easy, no logistical support required, etc.) using current technology. Density, viscosity, and visual appearance were selected as the parameters to be measured since they do meet simple operational requirements. These parameters are not necessarily good predictors of overall fuel performance, but were judged to be acceptable screening tools since there are some density and viscosity differences between the various types of fuels (i.e., diesel, gasoline, JP-4, etc.). Additionally, within limits, the more dense and more viscous a petroleum fuel is, the better it tends to be as a compression-ignition engine fuel. In general, cetane number increases with density.

The pass/fail limits for the CFTK were selected based on the use of fuel specification tables for specific properties (when available) for a fuel. Other fuel data incorporated in the determination came from an earlier technical report\*: "Emergency Fuels Technology." These data were averaged and utilized as an estimate of a fuel's maximum and minimum limits.

As can be seen in Table I, the lower density cutoff (0.78 kg/L) represents a compromise of the minimum and maximum values for the various fuels shown in

---

\* Bowden, J.N. and Stavinoha, L., "Emergency Fuels Technology," Interim Report AFLRL No. 155, AD A125275, prepared under Contract No. DAAK70-80-C-0001, June 1982.

**TABLE 1. SPECIFICATION DETERMINATION OF MINIMUM AND  
MAXIMUM TEST LIMITS FOR CAPTURED FUELS TEST KIT**

|             | Density, D 1298, kg/L at<br>15°C (estimated value) |         | Kinematic Viscosity, D 445 at<br>40°C, cSt (estimated value) |        |
|-------------|----------------------------------------------------|---------|--------------------------------------------------------------|--------|
|             | Min                                                | Max     | Min                                                          | Max    |
| DF-1        | (0.786)                                            | (0.829) | 1.3                                                          | 2.9    |
| DF-2        | (0.809)                                            | (0.878) | 1.9                                                          | 4.1    |
| OCONUS DF-2 | 0.815                                              | 0.860   | 1.3*                                                         | 5.3*   |
| JP-8        | 0.775                                              | 0.840   | 1.08                                                         | -      |
| JP-4        | 0.751                                              | 0.802   | (0.75)                                                       | (0.82) |
| Gasoline    | (0.720)                                            | (0.750) | 0.5**                                                        | -      |
| Jet A       | 0.775                                              | 0.840   | (1.1)                                                        | (1.7)  |
| Burner Oil  | -                                                  | 0.875   | 2.0                                                          | 3.6    |
| DF-A        | -                                                  | -       | 1.1                                                          | 2.4    |

\* Calculated from limits of 1.8 to 9.5 cSt at 20°C.

\*\* Determined at BFLRF as average viscosity.

Table 1. The initial lower viscosity range was set at 1.1 cSt at 40°C in an attempt to include all DF-A, JP-8, and Jet A procurable fuels as suitable fuels. However, a 50/50 blend of gasoline and a high viscosity diesel fuel can also produce a viscosity of 1.1 cSt or greater at 40°C, and this fuel is not acceptable for compression-ignition engines.

Figure 1 is a plot of gasoline composition in a gasoline/diesel fuel blend versus calculated viscosity. The curve shown could be considered a worst-case example since the viscosity of the diesel fuel is assumed to be 5.3 cSt at 40°C (F-54, DF-2 upper viscosity limit). Even at 50-percent gasoline, the viscosity of the blend is within the lower limits for JP-8, Jet A, and DF-A. The lower viscosity reference liquid is currently set at 1.3 cSt at 40°C. This limit has the potential to eliminate several acceptable fuels, but is necessary to eliminate a blend/mixture that would not be usable within the context of a field expedient or emergency fuel.

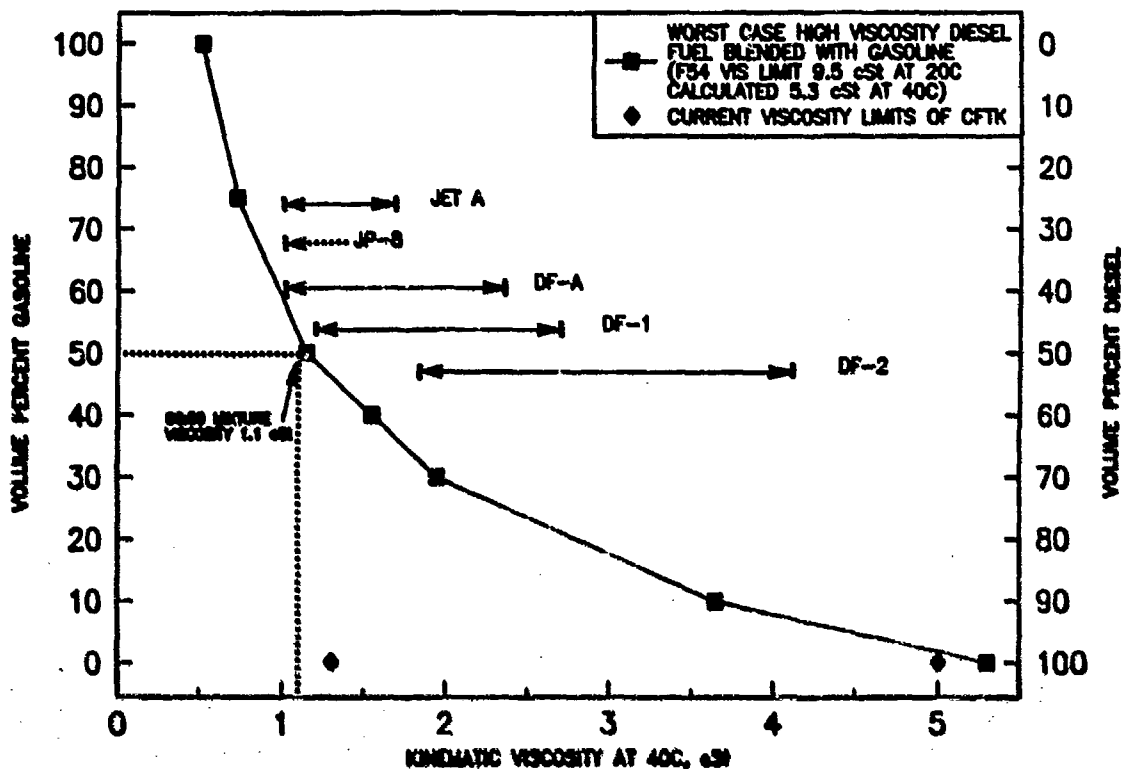


FIGURE 1. VISCOSITY OF GASOLINE AND DIESEL FUEL BLENDS

#### IV. PRELIMINARY DESIGN CONCEPTS

##### A. Density

Several methods to determine density were considered and evaluated. The most promising methods appeared to be calibrated spheres of varying density which would sink or float in the test fluid (a configuration for this approach is depicted in Figure 2), conventional hydrometer-type evaluation of density, or a buoyant pointer that would rotate in the test fluid as fluid densities varied.

### 1. Calibrated Spheres

Calibrated spheres were determined to be unsuitable due to the difficulty of procuring spheres made from fuel resistant materials in the proper density ranges and desired physical size. It was also judged that temperature compensation would possibly be more of a problem with this approach.

### 2. Hydrometer

Testing with a hydrometer indicated that it is a suitable approach. The hydrometer proved to be accurate and relatively easy to compensate for temperature. The only major problems identified with the hydrometer approach is that the hydrometer is sensitive to breakage if dropped and would have to be secured within its sample tube when not in use.

### 3. Buoyant Pointer

The buoyant pointer approach (based on Patent Nos. 4,136,551 and 4,236,405) was selected as the most promising approach since it allowed a compact final design, and would possibly be relatively simple to compensate for temperature variations.

### B. Viscosity

Two approaches were considered and tested for obtaining viscosity measurements.

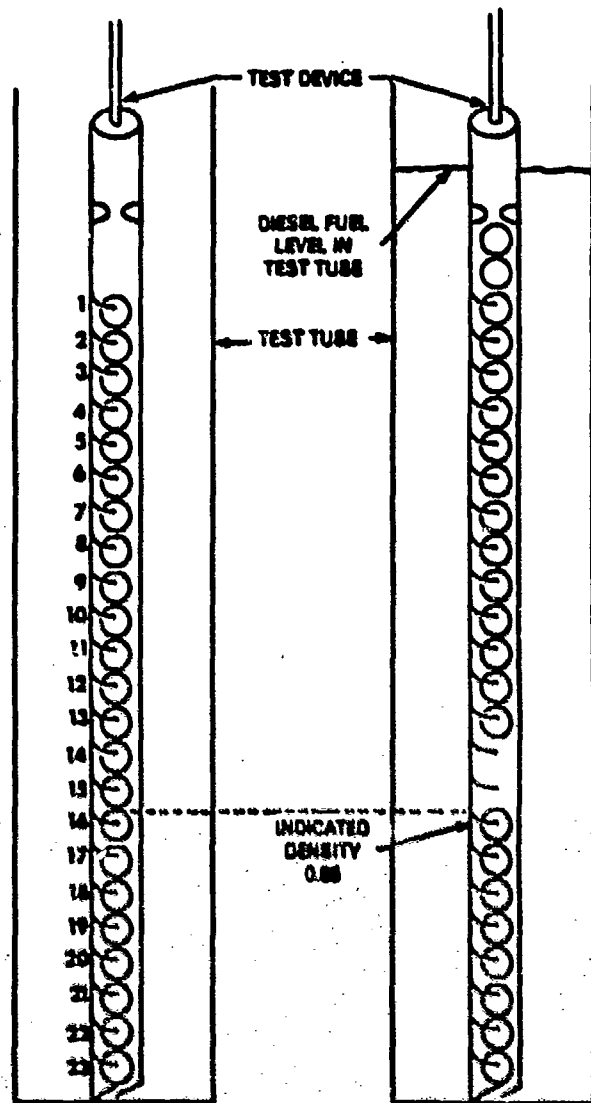


FIGURE 2. APPROACH FOR USING CALIBRATED SPHERES TO MEASURE DENSITY

# 1. Calibrated Orifice

A calibrated orifice was used to determine viscosity by measuring the time period required for a fixed volume to flow through the orifice. Variations in viscosity were observed as corresponding variations in time of flow during the test. The results of tests with the calibrated orifice are given in Table 2 and plotted in Figure 3. The data obtained using this approach show excellent correlation with a variety of fluids when compared to the known viscosity of the test fluids. While viable as a measuring technique, this method is too complex an approach for the ease of operation which was desirable for the test kit since test results would require temperature compensation using a conversion table. Additionally, a mechanical timer (of sufficient accuracy and durability) to measure the testing interval, a required component, was not readily available.

**TABLE 2. CALIBRATED ORIFICE FLOW TIMES AND  
KINEMATIC VISCOSITY AT VARIOUS TEMPERATURES**

| Fuel Type<br>AL-Code Number                             | MOGAS<br><u>14445-G</u> | Stoddard<br>Solvent<br><u>14364-F</u> | Jet A<br><u>14366-F</u> | Cat 1-H<br><u>14365-F</u> |
|---------------------------------------------------------|-------------------------|---------------------------------------|-------------------------|---------------------------|
| <u>0°C</u>                                              |                         |                                       |                         |                           |
| Kinematic Viscosity, D 445, cSt                         | 0.77                    | 1.75*                                 | 3.20*                   | 10.0*                     |
| Calibrated Orifice Flow Time for<br>30 mL Fuel, Seconds | 54.1                    | 87.5                                  | 119.2                   | 361.8                     |
| <u>24°C</u>                                             |                         |                                       |                         |                           |
| Kinematic Viscosity, D 445, cSt                         | 0.63                    | 1.25                                  | 1.76                    | 5.15                      |
| Calibrated Orifice Flow Time for<br>30 mL Fuel, Seconds | 52.9                    | 78.0                                  | 98.0                    | 257.0                     |
| <u>40°C</u>                                             |                         |                                       |                         |                           |
| Kinematic Viscosity, D 445, cSt                         | 0.52*                   | 0.97                                  | 1.20                    | 3.23                      |
| Calibrated Orifice Flow Time for<br>30 mL Fuel, Seconds | 42.8                    | 67.5                                  | 82.4                    | 178.8                     |

\* Calculated from viscosity chart.

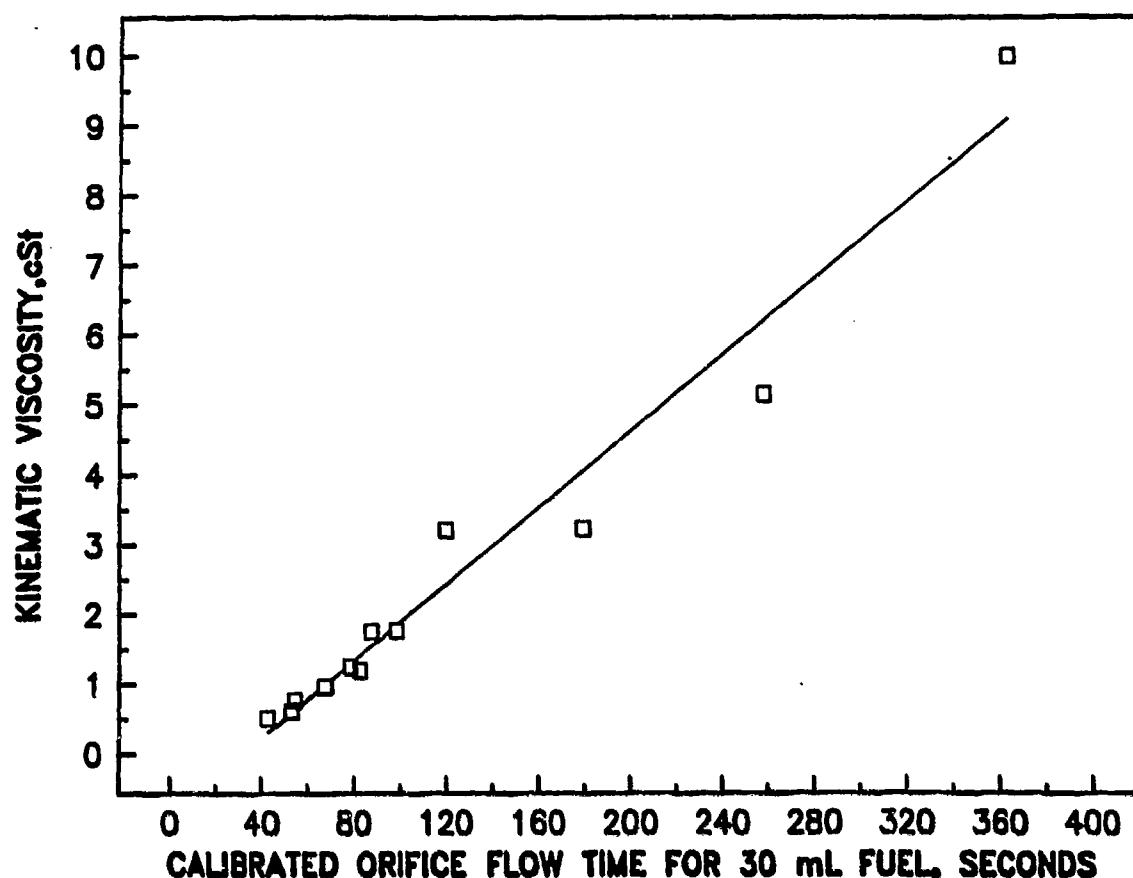


FIGURE 3. CALIBRATED ORIFICE VERSUS ACTUAL VISCOSITY

## 2. Falling Ball

The calibrated orifice method was abandoned in favor of the falling ball test, which was much simpler to use and was self compensating for temperature variations if reference materials were also incorporated. This method utilizes a glass tube containing a small ball. The tube is filled with the test fluid and aligned vertically, parallel to identical tubes that are filled with reference fluids representing upper and lower viscosity cutoff limits. When all tubes are simultaneously inverted, the sequence in which the balls reach the bottoms of their tubes indicates if the sample's viscosity is within the desired range.

Temperature compensation is automatically obtained with this approach by surrounding the outside surfaces of all the tubes with test fuel. This allows the tubes to reach temperature equilibrium after a relatively short residence time (approximately 1 minute). The biggest difficulty with this method was the requirement

that the reference viscosity fluids be sealed in the tubes. An approach for sealing the tubes and maintaining them without a vapor space over the temperature range of 0° to 40°C was reduced to practice (Patent Disclosure No. 1716, dated 22 January 1986).


C. Visual Appearance (Clean and Bright)

1. White Beaker

The initial approach for determining the visual appearance of the fuel was to pour a volume of the fuel into a small beaker with a white bottom. The operator would then look at the bottom of the beaker through the fuel, to see if there are any contaminants in the fuel. This approach proved to be unsatisfactory for several reasons. While this method is sufficient for detecting large particles in the fuel, it is not adequately sensitive to small particles. This method is also not as sensitive to cloudiness in the fuel caused by suspended water. Additionally, if the test fuel is relatively dark in color, the appearance of contamination or water droplets in the bottom of the beaker may be obscured. If required to conduct the examination under low light conditions, there is no way that the operator could use a light source (such as a flashlight) to make the examination. Based on these shortcomings with this method, it was judged that a visual comparator would be a more acceptable approach.

2. Comparator

The visual comparator (similar to the one pictured in Figure 4) solves the problems associated with the white beaker approach. It should be noted, however, that visual appearance is not readily quantified. Although efforts have been made to provide a simple, useful visual appearance test, the visual comparator continues to be subjective in nature and more of a "clear and bright" test rather than a "clean and bright" test.

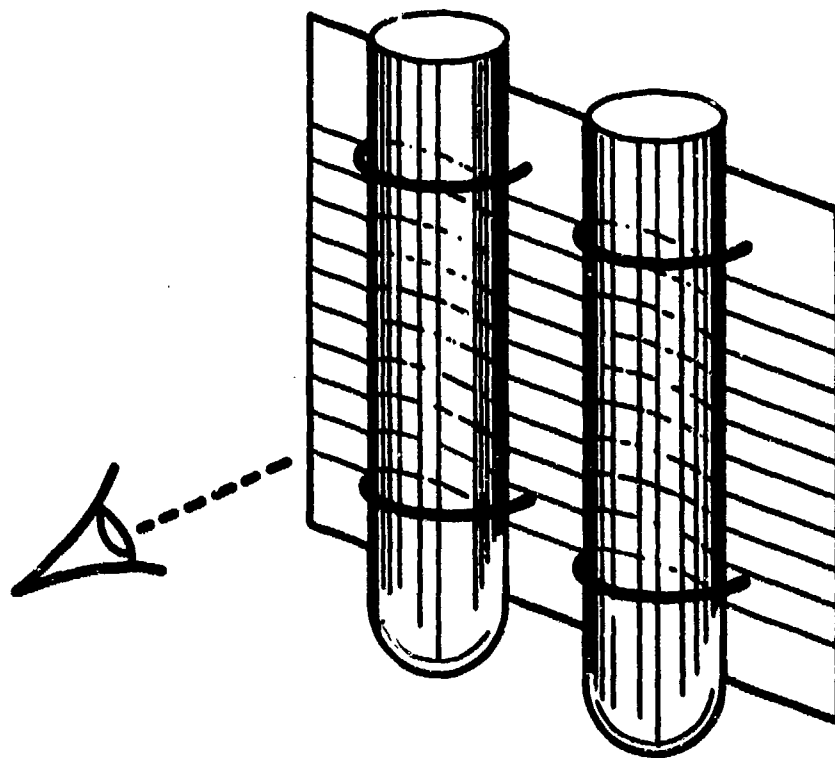

**FIGURE 4. APPROACH FOR USING COMPARATOR FOR VISUAL APPEARANCE**

## **V. EVOLUTION OF THE CURRENT CFTK**

### **A. Density Test**

The buoyant pointer approach to fluid density determination utilizes a mass which can rotate about a fixed pivot point. The mass is asymmetrically distributed around the pivot location which causes the center of buoyancy to be at a location offset to the pivot point. If the assembly is placed in a fluid, the weight distribution is altered due to the offset center of buoyancy and the assembly rotates about the pivot point to seek a new equilibrium position where the forces are balanced. Higher density fluids create more buoyant forces than lower density fluids, thus the higher the density of the fluid the greater the rotation of the assembly. The geometry of the asymmetrical weight distribution and the density of the pointer material affect the range and sensitivity of response.




The maximum rotation that can be produced by this interplay of forces is  $180^{\circ}$  and the greatest sensitivity is encountered near the  $90^{\circ}$  rotation point.

Since the purpose of the density test is to determine if a fuel is below a defined density limit, and  $90^{\circ}$  rotation is the most sensitive zone for the instrument, it became apparent that the final design should be "fine tuned" to produce  $90^{\circ}$  rotation when submerged in a fluid whose density is at the assigned lower cutoff limit (0.78 kg/L was selected as the density cutoff) for go/no-go testing of fuel density requirements.

Several designs for the density tester were empirically evaluated, modified, and refined. The first design tested was a disc of acrylic plastic with a pivot at its center. The mass distribution of the disc was then made asymmetrical by drilling holes in one half of the disc, and the counterbalance pointer was inserted into the edge of the disc near the drilled holes. This design did function in the manner expected but sensitivity proved to be insufficient. The same design was modified by reducing the thickness of the plastic disc to reduce inertial effects and the pivot design was improved to reduce friction. These modifications improved response, but sensitivity was still considered marginal. Experiments with other asymmetric geometries led to a final design which consisted of a pie-shaped wedge of plastic on one side of the pivot connected to a narrow strip of plastic on the opposite side of the pivot which contains the counterbalance pointer (see Figure 5). With this design, sensitivity and range were sufficiently improved to satisfy the design requirements when tested under laboratory conditions with various fluid and temperature combinations. (This improvement may have also been achievable by making the entire pointer mechanism buoyant in the range of densities being tested. This would have necessitated extensive testing for which no time could be allotted.)

Implementation of this approach was accomplished by using acrylic plastic for the buoyant mass with the bulk of its weight suspended on one side of the pivot point. Figure 5 is a drawing of the final design of the pointer. A counterbalance of stainless steel rod was inserted into the plastic on the opposite side of the pivot point. This steel rod serves as an indicating pointer as well as functioning as a counterbalance weight. When testing any of the experimental designs using this

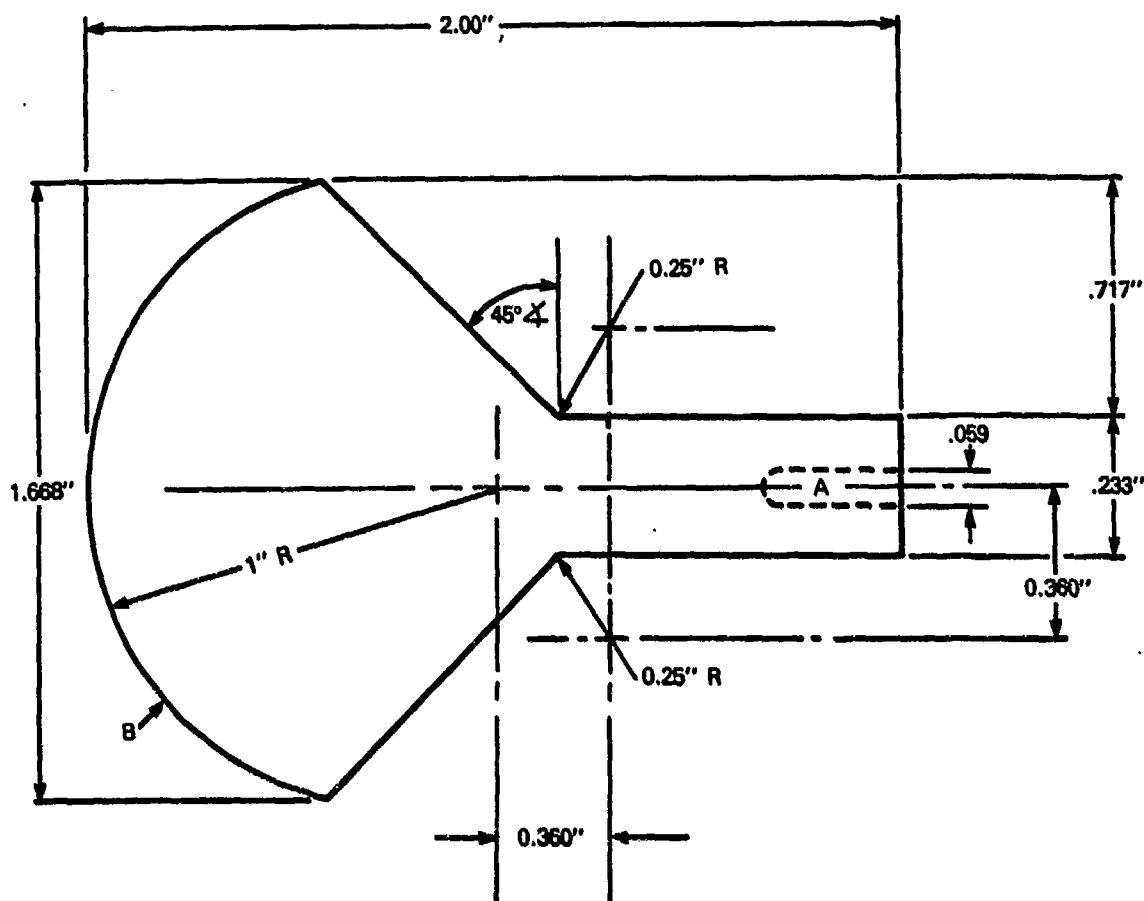

**FIGURE 5. FINAL DESIGN OF CFTK DENSITY POINTER**

approach, the length of the pointer was adjusted until its weight gave the proper counterbalancing effect, causing the pointer to float at  $90^\circ$  rotation when the assembly was submerged in fluid representing the cutoff limit for density ( $0.78 \text{ kg/L}$ ). This adjustment was made with the fluid at room temperature of about  $24^\circ\text{C}$  ( $75^\circ\text{F}$ ). In less dense fluids, the plastic sinks, causing the counterbalance pointer to rise. In denser fluids, the plastic is more buoyant, causing it to rise and the counterbalance pointer to sink.

Two major design requirements had to be achieved for this approach to be viable. The sensitivity of the responses must allow repeatable differentiation between the angular pointer position with the density reference fluid, as compared to the position achieved with less dense fluids. The second requirement is that the overall range of the pointer must be adjusted to ensure that, when the density of the cutoff limit reference fluid is altered by heating or cooling within the functional

temperature range of the tester, the angular variations of the pointer will be well within the range limits. When these requirements have been accomplished and the angular positions for the cutoff limit reference fluid established over the testing temperature range, the relative density of unknown fluids can be determined. In the tester, the density pointer will indicate a given level for the cutoff limit reference fluid. When testing an unknown fluid at that same temperature, if the pointer indicates a level higher than indicated for the reference fluid, then the questionable fluid is considered unacceptable.

As shown in Table 3, the density of a given fluid can experience a significant change over the temperature range of 0°C (32°F) to 38°C (100°F). Consequently, a simple means to temperature compensate the density tester was needed. One obvious method to accomplish this task is to generate a table containing a list of angular positions of the pointer determined for the cutoff limit reference fluid at all temperatures in the testing range. The angular position encountered with an unknown fluid at any temperature could then be compared to the position for the

**TABLE 3. DENSITY CHANGES AT VARIOUS TEMPERATURES AS  
CALCULATED FROM ASTM D 1298, DENSITY AT 15°C**

|                                | Density, kg/L<br>0°C (32°F) | Density, kg/L<br>15°C (59°F) | Density, kg/L<br>23°C (74°F) | Density, kg/L<br>38°C (100°F) |
|--------------------------------|-----------------------------|------------------------------|------------------------------|-------------------------------|
| 14364-F<br>Stoddard<br>Solvent | 0.785                       | 0.772                        | 0.765                        | 0.753                         |
| 14365-F<br>Cat 1-H             | 0.861                       | 0.851                        | 0.846                        | 0.838                         |
| 14366-F<br>Kerosene            | 0.807                       | 0.796                        | 0.790                        | 0.780                         |
| 14443-F<br>Burner Fuel         | 0.881                       | 0.871                        | 0.866                        | 0.857                         |
| 14446-F<br>JP-3                | 0.834                       | 0.823                        | 0.817                        | 0.807                         |
| 14447-F<br>JP-4                | 0.776                       | 0.763                        | 0.757                        | 0.744                         |

cutoff limit reference fluid at that temperature. This approach was rejected because it was felt to be too cumbersome. An alternate approach to temperature compensation would be for the center of gravity of the pointer to appropriately change with temperature. This could not be easily reduced to practice.


An effective and extremely simple means of temperature compensation was conceived and implemented. The angular position of the pointer was recorded with the cutoff limit reference fluid at  $38^{\circ}\text{C}$  ( $100^{\circ}\text{F}$ ),  $24^{\circ}\text{C}$  ( $75^{\circ}\text{F}$ ), and  $-12^{\circ}\text{C}$  ( $10^{\circ}\text{F}$ ). A small thermometer was then selected, and the locations of these temperature points on the thermometer were established. The thermometer was then positioned inside the unit's case at the proper height, angular displacement, and distance from the pivot point so that the position of the pointer at the corresponding temperatures would intersect these temperature locations on the thermometer's body. Once positioned in the critical location, the thermometer proved to track the angular position of the cutoff limit reference fluid over the entire temperature range of the instrument. The pointer would always intersect with the tip of the red thermometer fluid when testing the reference fluid, regardless of temperature.

When testing an unknown fluid, the thermometer reacts to the temperature of the unknown fluid and the tip of the red fluid in the thermometer indicates where the intersection would be for cutoff limit reference fluid at this temperature. If the unknown or test fluid causes the pointer to intersect the thermometer above the red fluid level, the fluid is less dense than the reference and unacceptable (no-go). If the pointer intersects the thermometer below the tip of the red fluid, the unknown or test fluid is more dense than the reference and acceptable (go).

#### B. Viscosity Test

The design approach selected for viscosity determination was to fabricate reference standards, containing fluids representing selected viscosity limits. The reference fluids were sealed into glass tubes which contained a small ball. This ball would fall through the fluid when the reference tube was inverted. In operation, a sample tube which also contained a small ball, would be filled with the unknown fluid, and the cell containing the sample and reference tubes was flooded

with the unknown fluid (see Figure 6). This allowed all of the tubes to reach temperature equilibrium after a short residence time. The cell was then inverted and the sequence in which the balls fell was used to determine if the unknown fluid's relative viscosity was within the preselected viscosity range.

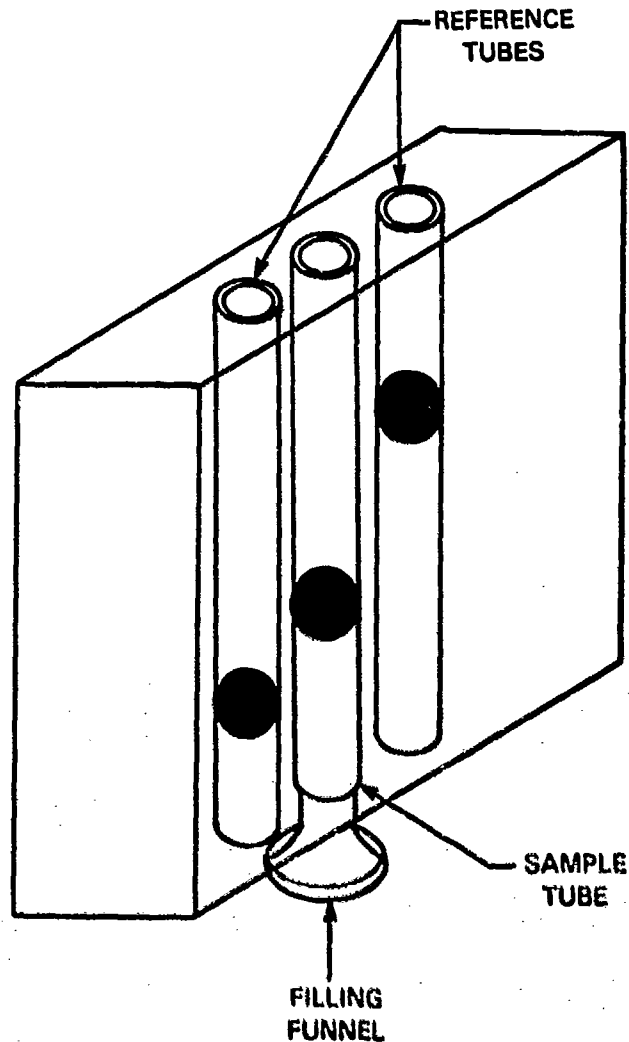

**FIGURE 6. DIAGRAM OF CFTK VISCOSITY TEST**  
(Showing Proper "GO" Ball Fall Sequence)


When the first prototype using this approach was tested, an operational problem was encountered with the reference tubes. Air bubbles in the tubes would sometimes become trapped under the ball, affecting its fall time. To overcome this problem, a means was required to completely fill the tubes, thus eliminating

all air bubbles. The pressure within the tube must also be sufficiently high to prevent the formation of vapor bubbles, and the tube must handle fluid volume changes from thermal expansion without breaking.

The approach used to accomplish these goals was to seal one end of each reference tube by melting the glass. The opposite end was then heated and slightly flared. The reference fluids were then cooled to near their freezing points to reduce their dissolved air content and to cause maximum contraction of the fluid. A ball was then placed in the glass tube and the tube was completely filled with the cold fluid, leaving a convex meniscus at the top of the flared tube end. A thin sheet of viton elastomer was then stretched over the flared end, taking care to exclude the introduction of air bubbles (see Figure 7). A viton O-ring was rolled over the flare to seal the viton membrane in place, and heat shrink tubing was applied to the O-ring to further aid in the sealing action. As the fluid warms and expands, the elastomer stretches, allowing the tube to accommodate the increased fluid volume. The stretched elastomer creates sufficient pressure within the tube to eliminate formation of vapor bubbles.

The long-term durability of this reference tube sealing technique can only be determined by observation of its behavior over a long-term time period. If any problem is encountered, it would probably be due to diffusion through the viton membrane over a long time period. An alternate approach, which would probably extend shelf life for the reference tubes, would be to use an expandable metal bellows in place of the elastomer. This bellows could be spring loaded to overcome the effects of vapor pressure and still accommodate thermal expansion of the fluid. This conceptual approach to extending shelf life of the reference tubes could not be fully evaluated within the time and manpower constraints of this program.

The elimination of air bubbles from the sample tube had to be accomplished in a different manner since neither end of the sample tube

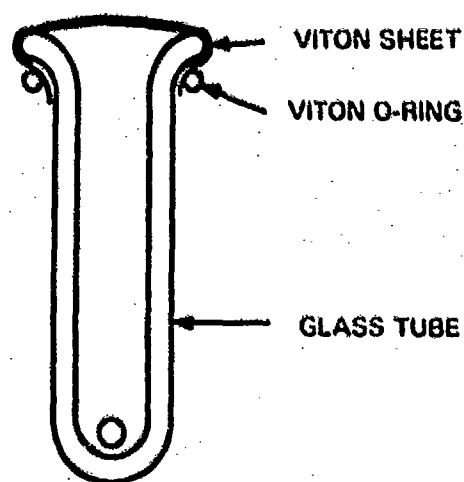

**FIGURE 7. VISCOSITY  
REFERENCE TUBE**

could be permanently sealed. It was determined, however, that at least one end of the sample tube had to be temporarily sealed during testing to be certain that the ball was falling through the fluid and not simply pushing the fluid out of the tube. The first approach tested utilized a check valve on one end of the tube with the other end of the tube open. When the cell containing the tubes was filled with sample fluid, the sample tube was expected to fill, with the check valve allowing the air to escape. When the tester was inverted, the check valve would seat, thus sealing the bottom of the tube while the ball fell. In practice, this approach worked poorly due to inconsistent seating of the gravity-operated check valve.

The problem was solved in the final design by incorporating a rotating closure which would seal off both the cell's fill port and the top of the viscosity sample tube after the cell and sample tube had been completely filled with fluid. This eliminated the air bubbles in the tube and provided a positive closure to the top of the sample tube, ensuring that, when inverted, the ball would fall toward the closed end. The closure could be rotated to open position to allow draining of the sample tube and cell in preparation for the next test or storage of the test cell.

Inconsistent fall times for reference tubes containing the same reference fluids was another problem encountered during testing of this design. The problem was traced to variation in diameter of the glass tubing that had been used. This was readily solved by purchasing precision bore tubing which gave more repeatable results in the final design.

Examples of laboratory tests using this final design are provided in Tables 4 through 10. Table 4 illustrates performance when the unit was tested with the same fluid that is contained in reference tube No. 1. Sample tube No. 2 should have identical fall times when compared to tube No. 1, and the fall time difference in seconds represents the variations encountered due to slight variations between the glass tubes or the balls.

Table 5 illustrates performance when the unit was tested with the same fluid that is contained in reference tube No. 3. In this case, sample tube No. 2 should have the same fall time as compared to tube No. 3, and the fall time difference represents the variations encountered.

**TABLE 4. FALLING BALL METHOD AT VARIOUS TILTS AND TEMPERATURES USING LOW VISCOSITY REFERENCE FUEL**

40% Isooctane, 60% Diesel Control AL-13883, and  
Viscosity at 40°C, 1.32 cSt

| Orientation of<br>Test Unit | Test<br>Temperature | Fall Time in Seconds |           |           | Fall Time Difference<br>Tube 2 - Tube 1<br>in Seconds |
|-----------------------------|---------------------|----------------------|-----------|-----------|-------------------------------------------------------|
|                             |                     | Tube<br>1            | Tube<br>2 | Tube<br>3 |                                                       |
| <u>0° Tilt</u>              | 0°C ( 32°F)         | 16.6                 | 15.5      | 73.8      | -1.1                                                  |
|                             | 23°C ( 73°F)        | 13.5                 | 12.1      | 41.5      | -1.4                                                  |
|                             | 38°C (100°F)        | 12.6                 | 11.7      | 27.3      | -0.9                                                  |
| <u>15° Left Tilt</u>        | 0°C ( 32°F)         | 13.9                 | 12.7      | 122.7     | -1.2                                                  |
|                             | 23°C ( 73°F)        | 9.8                  | 9.3       | 50.3      | -0.5                                                  |
|                             | 38°C (100°F)        | 8.5                  | 8.0       | 32.4      | -0.5                                                  |
| <u>15° Right Tilt</u>       | 0°C ( 32°F)         | 13.5                 | 12.7      | 128.3     | -0.8                                                  |
|                             | 23°C ( 73°F)        | 9.8                  | 9.4       | 50.1      | -0.4                                                  |
|                             | 38°C (100°F)        | 8.4                  | 7.6       | 31.8      | -0.8                                                  |
| <u>30° Left Tilt</u>        | 0°C ( 32°F)         | 14.0                 | 13.2      | 105.8     | -0.8                                                  |
|                             | 23°C ( 73°F)        | 11.2                 | 10.4      | 55.7      | -0.8                                                  |
|                             | 38°C (100°F)        | 9.4                  | 9.1       | 36.5      | -0.3                                                  |
| <u>30° Right Tilt</u>       | 0°C ( 32°F)         | 13.2                 | 12.4      | 101.4     | -0.8                                                  |
|                             | 23°C ( 73°F)        | 10.9                 | 10.1      | 54.9      | -0.8                                                  |
|                             | 38°C (100°F)        | 9.4                  | 9.0       | 36.7      | -0.4                                                  |

**TABLE 5. FALLING BALL METHOD AT VARIOUS TILTS AND TEMPERATURES USING HIGH VISCOSITY REFERENCE FUEL**

35% Mineral Oil AL-14607-L, 65% Diesel Control AL-13883-F,  
and Viscosity at 40°C, 5.05 cSt

| Orientation of<br>Test Unit | Test<br>Temperature | Fall Time in Seconds |           |           | Fall Time Difference<br>Tube 2 - Tube 1<br>in Seconds |
|-----------------------------|---------------------|----------------------|-----------|-----------|-------------------------------------------------------|
|                             |                     | Tube<br>1            | Tube<br>2 | Tube<br>3 |                                                       |
| <u>0° Tilt</u>              | 0°C ( 32°F)         | 16.7                 | 76.3      | 77.8      | +1.5                                                  |
|                             | 23°C ( 73°F)        | 14.7                 | 40.8      | 42.6      | +1.8                                                  |
|                             | 38°C (100°F)        | 12.0                 | 27.6      | 27.3      | -0.3                                                  |
| <u>15° Left Tilt</u>        | 0°C ( 32°F)         | 12.1                 | 91.3      | 90.1      | -1.2                                                  |
|                             | 23°C ( 73°F)        | 9.9                  | 49.9      | 50.3      | +0.4                                                  |
|                             | 38°C (100°F)        | 8.7                  | 32.7      | 33.3      | +0.6                                                  |
| <u>15° Right Tilt</u>       | 0°C ( 32°F)         | 11.6                 | 57.4      | 57.5      | +0.1                                                  |
|                             | 23°C ( 73°F)        | 9.4                  | 49.6      | 49.9      | +0.3                                                  |
|                             | 38°C (100°F)        | 8.5                  | 34.4      | 33.7      | -0.7                                                  |
| <u>30° Left Tilt</u>        | 0°C ( 32°F)         | 13.4                 | 99.9      | 97.5      | -2.4                                                  |
|                             | 23°C ( 73°F)        | 10.7                 | 54.9      | 55.6      | +0.7                                                  |
|                             | 38°C (100°F)        | 9.6                  | 38.0      | 38.6      | +0.6                                                  |
| <u>30° Right Tilt</u>       | 0°C ( 32°F)         | 13.4                 | 100.8     | 100.8     | 0.0                                                   |
|                             | 23°C ( 73°F)        | 10.7                 | 54.3      | 55.4      | +1.1                                                  |
|                             | 38°C (100°F)        |                      | 9.6       | *         | *                                                     |

\* Not Determined.



In generating the test information contained in Tables 4 and 5, the unit was operated at various temperatures and angular tilts of the device as shown in the tables. The effects of temperature and tilt angle proved to be insignificant when the tubes are compared to each other at the same temperature and tilt angle.

Tables 6 through 10 represent the results obtained with fuels or blends covering a wide range of viscosities. As shown in these tables, the fall sequence of the balls conformed to the expected results in all cases. The test fluids that were within the viscosity limits all produced a 1, 2, 3 fall sequence. Fluids outside the acceptable limit did not produce this sequence of fall.

**TABLE 6. FALLING BALL METHOD AT VARIOUS  
TILTS AND TEMPERATURES**

85% Stoddard Solvent AL-14364-F, 15% Diesel  
Control AL-13883-F, and Viscosity  
at 40°C, 1.09 cSt

| <u>Orientation of<br/>Test Unit</u> | <u>Test<br/>Temperature</u> | <u>Fall Time in Seconds</u> |                   |                   | <u>Ball-<br/>Fall<br/>Order</u> | <u>Correct</u> |
|-------------------------------------|-----------------------------|-----------------------------|-------------------|-------------------|---------------------------------|----------------|
|                                     |                             | <u>Tube<br/>1</u>           | <u>Tube<br/>2</u> | <u>Tube<br/>3</u> |                                 |                |
| <u>0° Tilt</u>                      | 0°C ( 32°F)                 | 17.5                        | 13.6              | 91.6              | 2-1-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 13.3                        | 10.6              | 43.0              | 2-1-3                           | Yes            |
|                                     | 38°C (100°F)                | 12.4                        | 9.5               | 28.3              | 2-1-3                           | Yes            |
| <u>15° Left Tilt</u>                | 0°C ( 32°F)                 | 13.7                        | 10.0              | 122.4             | 2-1-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 9.8                         | 7.6               | 52.3              | 2-1-3                           | Yes            |
|                                     | 38°C (100°F)                | 8.5                         | 6.6               | 34.6              | 2-1-3                           | Yes            |
| <u>15° Right Tilt</u>               | 0°C ( 32°F)                 | 12.9                        | 9.7               | 127.6             | 2-1-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 8.7                         | 7.6               | 51.9              | 2-1-3                           | Yes            |
|                                     | 38°C (100°F)                | 8.5                         | 5.8               | 34.5              | 2-1-3                           | Yes            |
| <u>30° Left Tilt</u>                | 0°C ( 32°F)                 | 15.2                        | 11.2              | 133.2             | 2-1-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 11.0                        | 8.3               | 57.6              | 2-1-3                           | Yes            |
|                                     | 38°C (100°F)                | 9.7                         | 7.5               | 38.6              | 2-1-3                           | Yes            |
| <u>30° Right Tilt</u>               | 0°C ( 32°F)                 | 13.9                        | 10.3              | 117.9             | 2-1-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 10.6                        | 8.1               | 56.7              | 2-1-3                           | Yes            |
|                                     | 38°C (100°F)                | 9.3                         | 7.3               | 38.6              | 2-1-3                           | Yes            |

**TABLE 7. FALLING BALL METHOD USING VARIOUS TEST FUELS**

| <u>Orientation of<br/>Test Unit</u>                       | <u>Test<br/>Temperature</u> | <u>Fall Time in Seconds</u> |             |             | <u>Ball-<br/>Fall<br/>Order</u> | <u>Correct</u> |
|-----------------------------------------------------------|-----------------------------|-----------------------------|-------------|-------------|---------------------------------|----------------|
|                                                           |                             | <u>Tube</u>                 | <u>Tube</u> | <u>Tube</u> |                                 |                |
|                                                           |                             | <u>1</u>                    | <u>2</u>    | <u>3</u>    |                                 |                |
| <u>Kerosene AL-14366-F and Viscosity at 40°C, 1.2 cSt</u> |                             |                             |             |             |                                 |                |
| <u>0° Tilt</u>                                            | 23°C ( 73°F)                | 14.0                        | 12.6        | 42.5        | 2-1-3                           | Yes            |
| <u>JP-8 AL-14446-T and Viscosity at 40°C, 1.27 cSt</u>    |                             |                             |             |             |                                 |                |
| <u>0° Tilt</u>                                            | 23°C ( 73°F)                | 14.7                        | 13.4        | 44.8        | 2-1-3                           | Yes            |
| <u>JP-4 AL-14447-T and Viscosity at 40°C, 0.8 cSt</u>     |                             |                             |             |             |                                 |                |
| <u>0° Tilt</u>                                            | 23°C ( 73°F)                | 15.0                        | 7.4         | 42.4        | 2-1-3                           | Yes            |

**TABLE 8. FALLING BALL METHOD AT VARIOUS  
TILTS AND TEMPERATURES**

Stoddard Solvent AL-14364-F and Viscosity  
at 40°C, 0.97 cSt

| <u>Orientation of<br/>Test Unit</u> | <u>Test<br/>Temperature</u> | <u>Fall Time in Seconds</u> |             |             | <u>Ball-<br/>Fall<br/>Order</u> | <u>Correct</u> |
|-------------------------------------|-----------------------------|-----------------------------|-------------|-------------|---------------------------------|----------------|
|                                     |                             | <u>Tube</u>                 | <u>Tube</u> | <u>Tube</u> |                                 |                |
|                                     |                             | <u>1</u>                    | <u>2</u>    | <u>3</u>    |                                 |                |
| <u>0° Tilt</u>                      | 0°C ( 32°F)                 | 15.9                        | 11.4        | 78.1        | 2-1-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 12.2                        | 8.7         | 43.3        | 2-1-3                           | Yes            |
| <u>15° Left Tilt</u>                | 0°C ( 32°F)                 | 11.8                        | 7.5         | 88.7        | 2-1-3                           | Yes            |
| <u>15° Right Tilt</u>               | 0°C ( 32°F)                 | 11.5                        | 7.4         | 97.4        | 2-1-3                           | Yes            |
| <u>30° Left Tilt</u>                | 0°C ( 32°F)                 | 15.5                        | 9.1         | 130.3       | 2-1-3                           | Yes            |
| <u>30° Right Tilt</u>               | 0°C ( 32°F)                 | 14.4                        | 8.9         | 136.0       | 2-1-3                           | Yes            |

**TABLE 9. FALLING BALL METHOD AT VARIOUS  
TILTS AND TEMPERATURES**

Burner Fuel AL-14443-F and Viscosity  
at 40°C, 2.2 cSt

| <u>Orientation of<br/>Test Unit</u> | <u>Test<br/>Temperature</u> | <u>Fall Time in Seconds</u> |                   |                   | <u>Ball-<br/>Fall<br/>Order</u> | <u>Correct</u> |
|-------------------------------------|-----------------------------|-----------------------------|-------------------|-------------------|---------------------------------|----------------|
|                                     |                             | <u>Tube<br/>1</u>           | <u>Tube<br/>2</u> | <u>Tube<br/>3</u> |                                 |                |
| <u>0° Tilt</u>                      | 0°C ( 32°F)                 | 15.2                        | 20.6              | 60.3              | 1-2-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 12.9                        | 16.5              | 42.7              | 1-2-3                           | Yes            |
| <u>15° Left Tilt</u>                | 0°C ( 32°F)                 | 10.8                        | 24.6              | 70.2              | 1-2-3                           | Yes            |
| <u>15° Right Tilt</u>               | 0°C ( 32°F)                 | 12.6                        | 33.3              | 118.1             | 1-2-3                           | Yes            |
| <u>30° Left Tilt</u>                | 0°C ( 32°F)                 | 16.0                        | 41.9              | 142.6             | 1-2-3                           | Yes            |
| <u>30° Right Tilt</u>               | 0°C ( 32°F)                 | 15.1                        | 41.1              | 156.4             | 1-2-3                           | Yes            |

**TABLE 10. FALLING BALL METHOD AT VARIOUS  
TILTS AND TEMPERATURES**

Cat 1-H AL-14365-F and Viscosity  
at 40°C, 3.2 cSt

| <u>Orientation of<br/>Test Unit</u> | <u>Test<br/>Temperature</u> | <u>Fall Time in Seconds</u> |                   |                   | <u>Ball-<br/>Fall<br/>Order</u> | <u>Correct</u> |
|-------------------------------------|-----------------------------|-----------------------------|-------------------|-------------------|---------------------------------|----------------|
|                                     |                             | <u>Tube<br/>1</u>           | <u>Tube<br/>2</u> | <u>Tube<br/>3</u> |                                 |                |
| <u>0° Tilt</u>                      | 0°C ( 32°F)                 | 11.6                        | 38.5              | 75.9              | 1-2-3                           | Yes            |
|                                     | 23°C ( 73°F)                | 13.4                        | 23.8              | 42.9              | 1-2-3                           | Yes            |
| <u>15° Left Tilt</u>                | 0°C ( 32°F)                 | 11.6                        | 42.7              | 81.8              | 1-2-3                           | Yes            |
| <u>15° Right Tilt</u>               | 0°C ( 32°F)                 | 11.1                        | 41.0              | 79.3              | 1-2-3                           | Yes            |
| <u>30° Left Tilt</u>                | 0°C ( 32°F)                 | 12.5                        | 45.9              | 87.3              | 1-2-3                           | Yes            |
| <u>30° Right Tilt</u>               | 0°C ( 32°F)                 | 11.7                        | 43.8              | 85.7              | 1-2-3                           | Yes            |

In the final version of the viscosity tester, the balls fall 3.5 inches. This distance was selected as a convenient distance in order to keep the overall size of the tester small. The balls are made of polytetrafluoroethylene (PTFE). PTFE was selected because it is inert and because its density is low enough to produce a reasonably short fall time during a 3.5-inch fall. When problems were encountered with contamination interfering with the fall of the sample ball, experiments were conducted to determine if a heavier ball (one that is less susceptible to contamination) would be preferable. Balls made of aluminum and bronze were tested for fall times at 3, 6, and 9-inch falls. Test fuels with viscosities of 1.3 cSt and 5.0 cSt at 40°C were used for these evaluations. These data are presented in Table 11. Note that results for bronze in each case show a relatively small difference in fall times between the 1.3 and 5.0 cSt extremes; as such, bronze was judged to be an unacceptable alternative. A 3-inch fall with the aluminum is the only option that yields results roughly equivalent to the previously selected 3-inch fall with PTFE. However, after the filter screen was installed in the filler cap, the problems with contamination subsided.

**TABLE 11. FALL TIMES FOR BALLS OF VARIOUS DENSITIES  
AND VARIOUS FALL LENGTHS**

| Ball                             | Fall Time in Seconds |         |            |         |            |         |
|----------------------------------|----------------------|---------|------------|---------|------------|---------|
|                                  | 3-in. Fall           |         | 6-in. Fall |         | 9-in. Fall |         |
|                                  | 1.3 cSt              | 5.0 cSt | 1.3 cSt    | 5.0 cSt | 1.3 cSt    | 5.0 cSt |
| PTFE<br>(Density = 2.3 kg/L)     | 10.6                 | 37.8    | 22.4       | 68.6    | 39.6       | 10.6    |
| Aluminum<br>(Density = 2.7 kg/L) | 9.4                  | 29.6    | 19.6       | 59.5    | 29.3       | 94.4    |
| Bronze<br>(Density = 7.5 kg/L)   | 1.5                  | 6.7     | 3.4        | 13.5    | 5.5        | 17.8    |

The final prototype viscosity tester utilizes a three-tube (one sample and two reference tubes) approach to measure viscosity. During the initial stages of development of the viscosity test, evaluations of a two-tube approach were also conducted. Under the two-tube (one sample and one reference tube) approach, the reference tube contains a fluid of a known given viscosity. The sample tube is


filled with the unknown fluid and the two tubes are inverted. The test can either be configured such that when the reference ball hits bottom, the sample ball must be in a green zone or the converse to this. The evaluations conducted gave inconsistent results across the temperature range of 0°C to 38°C. This approach may still be feasible with the proper selection of balls and reference fluid.

### C. Visual Appearance

The initial concept of a visual appearance test was to use a white beaker. This was to serve as a convenient pouring vessel as well as a visual test. This approach was discarded since it is difficult to see through a dark fuel to check for water or other contamination at the bottom of the beaker.

The visual comparator was then considered as this enables one to use a visual standard for comparison. It is also possible to shine a light through a clear comparator for a better view of possible contamination.

As can be seen in Figure 8, a series of lines behind the fuel sample can be used to enable a decision to be made about the clarity of the sample. There are lines on the comparator to permit a comparison. Since all the walls of the comparator are transparent, particulate contamination can be readily seen.

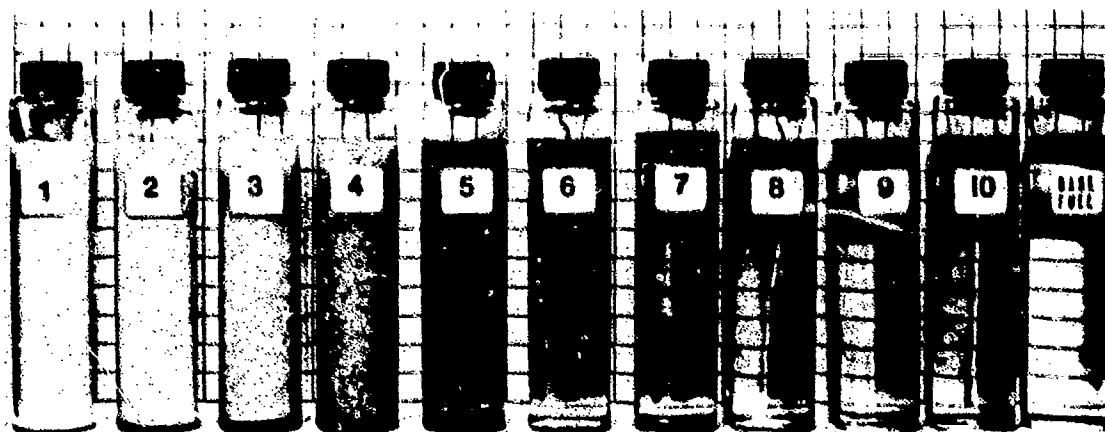

**FIGURE 8. PHOTOGRAPH OF A SERIES OF DIESEL FUEL SAMPLES  
CONTAINING 10 VOL% DEIONIZED WATER (SAMPLES 1-7) AND  
THE INDICATED QUANTITY OF SURFACTANT (1-7 VOL%)  
(Neat Base Fuel is Included for Comparison)**

## VI. CFTK CONFIGURATION


The CFTK incorporates all three of the testers in one housing. An exploded view of the final configuration is shown in Figure 9. This seemed the most efficient and simple approach for the user. Due to the sensitivity of the density and viscosity testers to small amounts of contamination, a filter screen with pores of approximately 100 micrometers was installed in the cap of the tester to prevent particles from interfering with the tests.

The initial cap design for the tester had two holes in the cap; one as a fill hole and one as a vent for the viscosity sample tube. These two holes were plugged with individual rubber stoppers. Three problems were discovered with this cap design; the stoppers were difficult to handle with gloves on, there was a tendency for air bubbles to collect in the viscosity sample tube, and filling and emptying the tester was difficult and messy. In the second prototype, the area around the two holes was machined to form a recess and a pouring spout was incorporated. Also, the two stoppers were secured into a single holder to improve ease of handling. These changes solved the problems of the air bubbles and the handling of the stoppers. There was also some improvement in the filling and emptying of the tester; however, the tester was now awkward to hold and required constant pressure on the stoppers to avoid leaks. To eliminate all of these problems, a new cap was designed. This new cap has a funnel (with an integral filter screen) for filling and emptying. This funnel also aided in the elimination of air bubbles in the sample viscosity tube. The new cap also has a positive twist closure to prevent fuel leakage. To further reduce the filling and emptying times, additional vents were installed in the cap, the top, and the bottom of the tester (see Figure 9, items 4 and 22). The vents in the top and bottom are spring-loaded valves and operate only when depressed by the user.

Since the density test requires that the tester be level during testing, a level indicator was incorporated in the tester. The level indicator consists of a pendulum/pointer and a dot and is in close proximity to the densitometer pointer for ease in viewing. When the tip of the pointer and the dot are aligned, the tester is level. No such provisions were made for the viscosity tester since experimentation showed that the viscosity test is not as sensitive to being out of level.

# **KEY**

1. Filter Screen
2. Filling Funnel
3. Vent
4. Vent for Faster Filling
5. Top Assembly
6. Side Assembly
7. Density Test Face Plate
8. Level Indicator
9. Thermometer for Temp. Compensation
10. Rotating GO/NO-GO Range Indicator
11. Retaining Cap
12. Pin
13. PEM Nut
14. Adjustable Screw
15. Density Pointer
16. Pointer Axle
17. Chamber Dividing Wall
18. Visual Appearance Tester
19. High End Viscosity Standard
20. Viscosity Sample Tube
21. Low End Viscosity Standard
22. Vent for Faster Emptying
23. Bottom Piece
24. Viscosity Test Face Plate

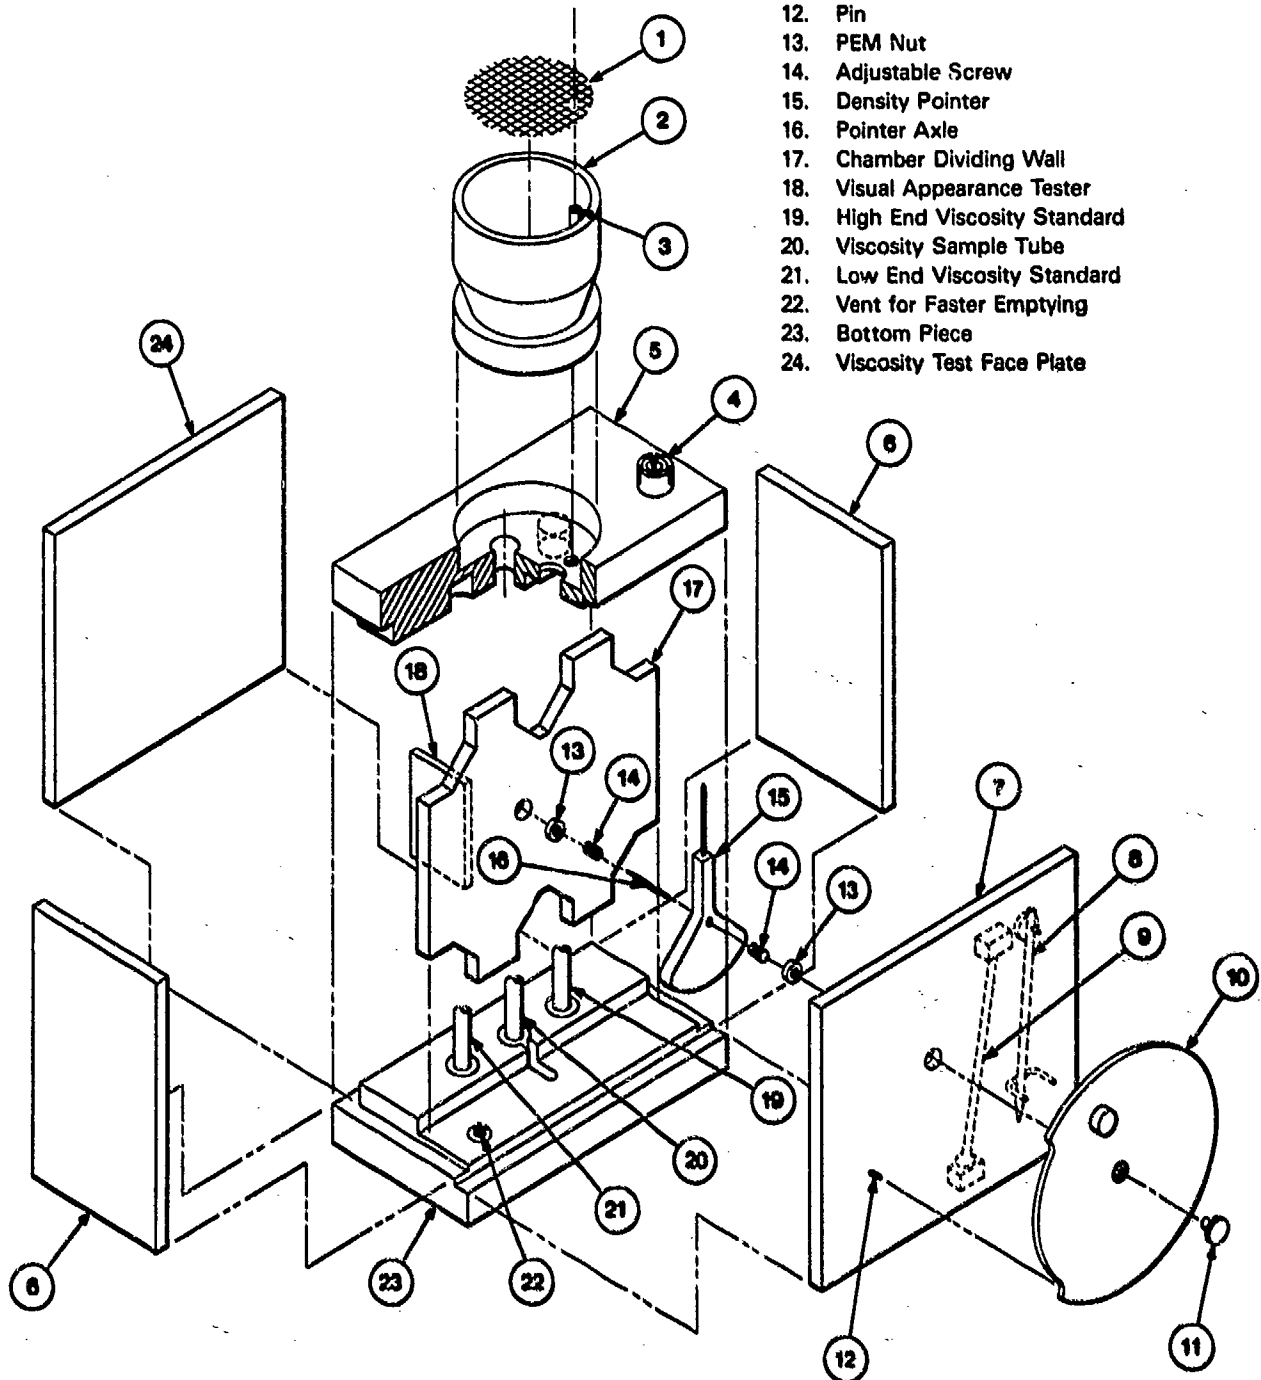

**FIGURE 9. EXPLODED VIEW OF FINAL CFTK CONFIGURATION**

## VII. CARRYING CASE

The carrying case for the CFTK measures 15 cm x 27 cm x 17 cm. Contained in the carrying case is the combined visual appearance/density/viscosity tester, a sampling hose, and a beaker to aid in sampling and testing. The case is made of fuel-resistant, shatter-resistant plastic and has a positive (cam lock) closure. The inside of the case contains a fuel-resistant foam for shock cushioning.

## VIII. QUALITY ASSURANCE TESTING

To ensure that the six prototypes were operating identically, each of the testers was tested with the same four fluids. These fluids are as follows:

| <u>Fuel</u>                                 | <u>Density, kg/L, 15°C</u> | <u>Viscosity, cSt, 40°C</u> |
|---------------------------------------------|----------------------------|-----------------------------|
| Iso-Octane                                  | 0.697                      | 0.60                        |
| 85% Stoddard Solvent/<br>15% Diesel Control | 0.775                      | 1.09                        |
| Reference Diesel                            | 0.847                      | 2.49                        |
| 35% Mineral Oil/<br>65% Diesel Control      | 0.850                      | 5.05                        |

The results of this testing are given in Tables 12 through 15.



**TABLE 12. RESULTS OF QUALITY ASSURANCE TESTING OF  
SIX CFTK PROTOTYPES WITH ISO-OCTANE**

| <u>Test Unit No.</u> | <u>86-101</u>                                                                               | <u>86-102</u> | <u>86-103</u> | <u>86-104</u> | <u>86-105</u> | <u>86-106</u> |
|----------------------|---------------------------------------------------------------------------------------------|---------------|---------------|---------------|---------------|---------------|
| <b>0°C</b>           |                                                                                             |               |               |               |               |               |
| Fill Time, seconds   | 12                                                                                          | 15            | 15            | 15            | 21            | 22            |
| Empty Time, seconds  | 17                                                                                          | 23            | 25            | 24            | 36            | 29            |
| Density, P/F         | F                                                                                           | F             | F             | F             | F             | F             |
| Degrees Displacement | 165                                                                                         | 170           | 169           | 169           | 168           | 168           |
| Viscosity Fall Order | 2-1-3                                                                                       | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         |
| <b>25°C</b>          |                                                                                             |               |               |               |               |               |
| Fill Time, seconds   | 15                                                                                          | 20            | 19            | 17            | 18            | 12            |
| Empty Time, seconds  | 15                                                                                          | 22            | 25            | 20            | 39            | 19            |
| Density, P/F         | F                                                                                           | F             | F             | F             | F             | F             |
| Degrees Displacement | 168                                                                                         | 170           | 169           | 168           | 168           | 168           |
| Viscosity Fall Order | 2-1-3                                                                                       | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         |
| <b>38°C</b>          |                                                                                             |               |               |               |               |               |
| Fill Time, seconds   |                                                                                             |               |               |               |               |               |
| Empty Time, seconds  | These tests were not conducted because of possible safety hazards from heating the solvent. |               |               |               |               |               |
| Density, P/F         |                                                                                             |               |               |               |               |               |
| Degrees Displacement |                                                                                             |               |               |               |               |               |
| Viscosity Fall Order |                                                                                             |               |               |               |               |               |

**TABLE 13. RESULTS OF QUALITY ASSURANCE TESTING OF  
SIX CFTK PROTOTYPES WITH 85/15**

| <u>Test Unit No.</u> | <u>86-101</u> | <u>86-102</u> | <u>86-103</u> | <u>86-104</u> | <u>86-105</u> | <u>86-106</u> |
|----------------------|---------------|---------------|---------------|---------------|---------------|---------------|
| <b>0°C</b>           |               |               |               |               |               |               |
| Fill Time, seconds   | 16            | 14            | 22            | 13            | 31            | 18            |
| Empty Time, seconds  | 18            | 22            | 18            | 18            | 37            | 20            |
| Density, P/F         | P             | P             | Cutoff        | P             | Cutoff        | Cutoff        |
| Degrees Displacement | 55            | 45            | 56            | 48            | 50            | 58            |
| Viscosity Fall Order | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         |
| <b>25°C</b>          |               |               |               |               |               |               |
| Fill Time, seconds   | 18            | 13            | 15            | 15            | 14            | 14            |
| Empty Time, seconds  | 18            | 13            | 17            | 18            | 50            | 17            |
| Density, P/F         | Cutoff        | Cutoff        | Cutoff        | P             | Cutoff        | Cutoff        |
| Degrees Displacement | 92            | 95            | 96            | 98            | 95            | 98            |
| Viscosity Fall Order | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         |
| <b>38°C</b>          |               |               |               |               |               |               |
| Fill Time, seconds   | 15            | 14            | 15            | 13            | 36            | 21            |
| Empty Time, seconds  | 18            | 32            | 17            | 17            | 30            | 22            |
| Density, P/F         | *             | *             | Cutoff        | *             | Cutoff        | Cutoff        |
| Degrees Displacement | 110           | 110           | 112           | 112           | 115           | 100           |
| Viscosity Fall Order | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         | 2-1-3         |

\* Just in red zone.

**TABLE 14. RESULTS OF QUALITY ASSURANCE TESTING OF  
SIX CFTK PROTOTYPES WITH DIESEL CONTROL**

| <u>Test Unit No.</u> | <u>86-101</u> | <u>86-102</u> | <u>86-103</u> | <u>86-104</u> | <u>86-105</u> | <u>86-106</u> |
|----------------------|---------------|---------------|---------------|---------------|---------------|---------------|
| <b>0°C</b>           |               |               |               |               |               |               |
| Fill Time, seconds   | 38            | 23            | 25            | 50            | 45            | 56            |
| Empty Time, seconds  | 16            | 22            | 22            | 22            | 25            | 18            |
| Density, P/F         | P             | P             | P             | P             | P             | P             |
| Degrees Displacement | 15            | 12            | 11            | 10            | 10            | 10            |
| Viscosity Fall Order | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         |
| <b>25°C</b>          |               |               |               |               |               |               |
| Fill Time, seconds   | 16            | 20            | 23            | 15            | 17            | 18            |
| Empty Time, seconds  | 16            | 22            | 22            | 19            | 15            | 18            |
| Density, P/F         | P             | P             | P             | P             | P             | P             |
| Degrees Displacement | 15            | 12            | 13            | 15            | 15            | 15            |
| Viscosity Fall Order | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         |
| <b>38°C</b>          |               |               |               |               |               |               |
| Fill Time, seconds   | 16            | 15            | 18            | 20            | 20            | 19            |
| Empty Time, seconds  | 18            | 17            | 17            | 17            | 18            | 19            |
| Density, P/F         | P             | P             | P             | P             | P             | P             |
| Degrees Displacement | 15            | 15            | 15            | 15            | 15            | 15            |
| Viscosity Fall Order | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         |

**TABLE 15. RESULTS OF QUALITY ASSURANCE TESTING OF  
SIX CFTK PROTOTYPES WITH 35/65**

| <u>Test Unit No.</u> | <u>86-101</u> | <u>86-102</u> | <u>86-103</u> | <u>86-104</u> | <u>86-105</u> | <u>86-106</u> |
|----------------------|---------------|---------------|---------------|---------------|---------------|---------------|
| <b>0°C</b>           |               |               |               |               |               |               |
| Fill Time, seconds   | 180           | 120           | 150           | 120           | 180           | 180           |
| Empty Time, seconds  | 20            | 30            | 37            | 35            | 25            | 25            |
| Density, P/F         | P             | P             | P             | P             | P             | P             |
| Degrees Displacement | 10            | 10            | 10            | 10            | 10            | 10            |
| Viscosity Fall Order | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         |
| <b>25°C</b>          |               |               |               |               |               |               |
| Fill Time, seconds   | 20            | 30            | 33            | 35            | 36            | 36            |
| Empty Time, seconds  | 20            | 22            | 21            | 22            | 24            | 23            |
| Density, P/F         | P             | P             | P             | P             | P             | P             |
| Degrees Displacement | 10            | 15            | 15            | 15            | 15            | 15            |
| Viscosity Fall Order | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         |
| <b>38°C</b>          |               |               |               |               |               |               |
| Fill Time, seconds   | 15            | 22            | 25            | 26            | 59            | 56            |
| Empty Time, seconds  | 20            | 20            | 20            | 19            | 47            | 19            |
| Density, P/F         | P             | P             | P             | P             | P             | P             |
| Degrees Displacement | 10            | 12            | 10            | 11            | 10            | 10            |
| Viscosity Fall Order | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         | 1-2-3         |

## **IX. CONCLUSIONS AND RECOMMENDATIONS**

A tester has been developed which will allow an unskilled operator to predict with reasonable probability if an undocumented fuel is potentially usable in Army compression-ignition engines and turbine-powered ground equipment. The reliability/confidence level of the tester to predict usability in a compression-ignition engine is yet to be determined in a separate program.

Density and viscosity cutoff limits were selected based on justifiable criteria. However, further testing and verification, especially in conjunction with engine tests, are required to establish the best limits.

The visual appearance test in the tester is not quantitative. There is not a simple, quantitative visual appearance test known at this time. This remains the most subjective part of the tester.

As noted earlier, density and viscosity are not reliable predictors of the overall performance of a fuel in a compression-ignition engine. Because of this, there will probably be acceptable fuels that the tester will reject. Likewise, there is the possibility that some unacceptable fuels will not be rejected. The frequency of each of these occurrences will depend on where the cutoff limits are set. Obviously, it is more desirable to reject some acceptable fuels than to accept some unacceptable fuels. Additionally, the acceptability limits will vary with climate (environmental engine start and operate temperature) and with the sensitivity of particular engines. The ability of a surrogate engine to start and run on a fuel designated as acceptable by the CFTK could be established as final acceptance criteria.

After acceptance of the prototype tester, it will be necessary to develop approaches to simplify its manufacture as the current prototype is far too complex to manufacture at a reasonable cost.

# DISTRIBUTION LIST

DEPARTMENT OF DEFENSE  
DEFENSE TECHNICAL INFORMATION  
CTR  
CAMERON STATION  
ALEXANDRIA VA 22314 12

DEPARTMENT OF THE ARMY  
HG, DEPT OF ARMY  
ATTN: DALO-TSE (COL BLISS) 1  
DALO-TSZ-B (MR KOWALCZYK) 1  
DALO-AV 1  
DAMO-FDR (MAJ KNOX) 1  
DAMA-ARZ (DR CHURCH) 1  
DAMA-ART (LTC RINEHART) 1  
WASHINGTON DC 20310

CDR  
U.S. ARMY BELVOIR RESEARCH,  
DEVELOPMENT & ENGINEERING CTR  
ATTN: STRBE-VF 30  
STRBE-HP 2  
STRBE-FSH 1  
FORT BELVOIR VA 22060-5606

CDR  
US ARMY MATERIEL DEVEL &  
READINESS COMMAND  
ATTN: AMCLD (DR ODOM) 1  
AMCDE-SG 1  
AMCDE-SS 1  
AMCQA-E 1  
AMCSM-WST (LTC DACEY) 1  
AMCIP-P (MR HARVEY) 1  
5001 EISENHOWER AVE  
ALEXANDRIA VA 22333-0001

CDR  
US ARMY TANK-AUTOMOTIVE CMD  
ATTN: AMSTA-RG (MR WHELOCK) 1  
AMSTA-TSL (MR BURG) 1  
AMSTA-G 1  
AMSTA-MTC (MR GAGLIO), 1  
AMSTA-MC, AMSTA-MV 1  
AMSTA-UBP (MR MCCARTNEY) 1  
AMSTA-MLF (MR KELLER) 1  
WARREN MI 48397-5000

DIRECTOR  
US ARMY MATERIEL SYSTEMS  
ANALYSIS ACTIVITY  
ATTN: AMXSY-CM (MR NIEMEYER) 1  
AMXSY-CR 1  
ABERDEEN PROVING GROUND MD  
21005-5006

CDR  
US ARMY GENERAL MATERIAL &  
PETROLEUM ACTIVITY  
ATTN: STRGP-F (MR ASHBROOK) 1  
STRGP-FE, BLDG 85-3 1  
STRGP-FT 1  
NEW CUMBERLAND PA 17070-5008  
HQ, DEPT. OF ARMY  
ATTN: DAEN-DRM 1  
WASHINGTON DC 20310

CDR  
US ARMY RES & STDZN GROUP  
(EUROPE)  
ATTN: AMXSN-UK-RA (DR OERTEL) 1  
AMXSN-UK-SE (LTC NICHOLS) 1  
BOX 65  
FPO NEW YORK 09510

CDR  
US ARMY FORCES COMMAND  
ATTN: AFLG-REG 1  
AFLG-POP 1  
FORT MCPHERSON GA 30330  
CDR  
US ARMY ABERDEEN PROVING  
GROUND  
ATTN: STEAP-MT-U (MR DEAVER) 1  
ABERDEEN PROVING GROUND MD  
21005

CDR  
US ARMY YUMA PROVING GROUND  
ATTN: STEYP-MT-TL-M 1  
(MR DOEBBLER)  
YUMA AZ 85364-9130

PROJ MGR, BRADLEY FIGHTING  
VEHICLE SYS  
ATTN: AMCPM-FVS-M  
WARREN MI 48397

1

CDR  
105TH S & T BATTALION  
5TH INFANTRY DIV (MECH)  
FORT POLK LA 71459

1

PROG MGR, M113 FAMILY OF VEHICLES  
ATTN: AMCPM-M113-T  
WARREN MI 48397

1

CDR  
TOBYHANNA ARMY DEPOT  
ATTN: SDSTO-TP-S  
TOBYHANNA PA 18466

1

PROJ MGR, MOBILE ELECTRIC POWER  
ATTN: AMCPM-MEP-TM  
7500 BACKLICK ROAD  
SPRINGFIELD VA 22150

1

CDR  
US ARMY DEPOT SYSTEMS CMD  
ATTN: AMSDS-RM-EFO  
CHAMBERSBURG PA 17201

1

PROJ OFF, AMPHIBIOUS AND WATER  
CRAFT  
ATTN: AMCPM-AWC-R  
4300 GOODFELLOW BLVD  
ST LOUIS MO 63120

1

CDR  
US ARMY LEA  
ATTN: DALO-LEP  
DALO-LEI  
NEW CUMBERLAND ARMY DEPOT  
NEW CUMBERLAND PA 17070

1

1

CDR  
US ARMY EUROPE & SEVENTH ARMY  
ATTN: AEAGG-FMD  
AEAGD-TE  
APO NY 09403

1

1

HQ, EUROPEAN COMMAND  
ATTN: J4/7-LJPO (LTC LETTERIE)  
VAIHINGEN, GE  
APO NY 09128

1

CDR  
THEATER ARMY MATERIAL MGMT  
CENTER (200TH)-DPGM  
DIRECTORATE FOR PETROL MGMT  
ATTN: AEAGD-MMC-PT-Q  
APO NY 09052

1

CDR  
US ARMY GENERAL MATERIAL &  
PETROLEUM ACTIVITY  
ATTN: STRGP-FW (MR PRICE)  
BLDG 247, DEFENSE DEPOT TRACY  
TRACY CA 95376

1

CDR  
US ARMY RESEARCH OFC  
ATTN: SLCRO-ZC  
SLCRO-EG (DR MANN)  
SLCRO-CB (DR GHIRARDELLI)  
P O BOX 12211  
RSCH TRIANGLE PARK NC 27709-2211

1

1

1

PROJ MGR, LIGHT ARMORED VEHICLES  
ATTN: AMCPM-LA-E  
WARREN MI 48397

1

PROG MGR, TACTICAL VEHICLE  
ATTN: AMCPM-TV  
WARREN MI 48397

1

CDR  
US ARMY FOREIGN SCIENCE & TECH  
CENTER  
ATTN: AMXST-MT-1  
AMXST-BA  
FEDERAL BLDG  
CHARLOTTESVILLE VA 22901

1

1

CDR  
TRADOC COMBINED ARMS TEST  
ACTIVITY  
ATTN: ATCT-CA  
FORT HOOD TX 76544

1

CDR  
AMC MATERIEL READINESS SUPPORT  
ACTIVITY (MRSA)  
ATTN: AMXMD-MO (MR BROWN)  
LEXINGTON KY 40511-5101

1

PROJECT MANAGER, LIGHT COMBAT  
VEHICLES

ATTN: AMCPM-LCV-TC  
WARREN, MI 48397

1

HQ, US ARMY T&E COMMAND

ATTN: AMSTE-TO-O

AMSTE-CM-R-O

AMSTE-TE-T (MR RITONDO)

ABERDEEN PROVING GROUND MD  
21005-5006

1

1

1

CDR, US ARMY TROOP SUPPORT  
COMMAND

ATTN: AMSTR-ME

AMSTR-S

AMSTRE-E

4300 GOODFELLOW BLVD  
ST LOUIS MO 63120-1798

1

1

1

TRADOC LIAISON OFFICE

ATTN: ATFE-LO-AV

4300 GOODFELLOW BLVD  
ST LOUIS MO 63120-1798

1

HQ

US ARMY TRAINING & DOCTRINE CMD

ATTN: ATCD-SL-5 (MAJ JONES)

FORT MONROE VA 23651-5000

1

CDR

US ARMY NATICK RES & DEV LAB

ATTN: STRNA-YE (MR KAPLAN)

STRNA-U

NATICK MA 01760-5000

1

1

CDR

US ARMY TRANSPORTATION SCHOOL

ATTN: ATSP-CD-MS (MR HARNET)

FORT EUSTIS VA 23604-5000

1

PROJ MGR, PATRIOT PROJ OFFICE

ATTN: AMCPM-MD-T-C

U.S. ARMY MISSILE COMMAND

REDSTONE ARSENAL AL 35898

1

CDR

US ARMY QUARTERMASTER SCHOOL

ATTN: ATSM-CD

ATSM-TD

ATSM-PFS

ASTM-DTN

FORT LEE VA 23801

1

1

1

1

HQ, US ARMY ARMOR CENTER AND  
FORT KNOX

ATTN: ATSB-CD

FORT KNOX KY 40121

1

CDR

101ST AIRBORNE DIV (AASLT)

ATTN: AFZB-KE-J

AFSB-KE-DMMC

FORT CAMPBELL KY 42223

1

1

CDR

US ARMY WESTERN COMMAND

ATTN: APLG-TR

FORT SCHAFER HI 96858

1

CDR

COMBINED ARMS COMBAT  
DEVELOPMENT ACTIVITY

ATTN: ATZL-CAT-E

ATZL-CAT-A

ATZL-TIE (MR DODSON)

FORT LEAVENWORTH KA 66027-5300

1

1

1

CDR

US ARMY LOGISTICS CTR

ATTN: ATCL-MS (MR A MARSHALL)

ATCL-C

FORT LEE VA 23801-6000

1

1

PROJECT MANAGER

PETROLEUM & WATER LOGISTICS

ATTN: AMCPM-PWS

4300 GOODFELLOW BLVD

ST LOUIS MO 63120-1798

1

CDR

US ARMY FIELD ARTILLERY SCHOOL

ATTN: ATSF-CD

FORT SILL OK 73503-5600

1

CDR

US ARMY ENGINEER SCHOOL

ATTN: ATZA-TSM-G

ATZA-CDM

ATZA-CDD

FORT BELVOIR VA 22060-5606

1

1

1

CDR

US ARMY INFANTRY SCHOOL

ATTN: ATSH-CD-MS-M

FORT BENNING GA 31905-5400

1

CDR  
MILITARY TRAFFIC MANAGEMENT  
COMMAND  
ATTN: MT-SA (MR DOWD)  
WASHINGTON DC 20315

1

DIR  
US ARMY MATERIALS & MECHANICS  
RESEARCH CENTER  
ATTN: SLCMT-M  
SLCMT-O  
WATERTOWN MA 02172-2796

1

1

PROG MGR, TANK SYSTEMS  
ATTN: AMCPM-MIEI-SM  
AMCPM-M60  
WARREN MI 48397

1

1

CDR  
US ARMY ARMOR & ENGINEER BOARD  
ATTN: ATZK-AE-AR  
ATZK-AE-LT  
FORT KNOX KY 40121

1

1

CDR  
6TH MATERIEL MANAGEMENT CENTER  
19TH SUPPORT BRIGADE  
APO SAN FRANCISCO 96212-0172

1

CHIEF, U.S. ARMY LOGISTICS  
ASSISTANCE OFFICE, FORSCOM  
ATTN: AMXLA-FO (MR PITTMAN)  
FT MCPHERSON GA 30330

1

CDR  
US ARMY SAFETY CENTER  
ATTN: PESD-SSD (MR BUCHAN)  
FORT RUCKER AL 36362

1

U.S. ARMY DEVELOPMENT AND  
EMPLOYMENT AGENCY  
ATTN: MODE-FDD-CSSB  
(MAJ GROSSMAN)  
FORT LEWIS WA 98433-5000

1

CDR  
U.S. ARMY LABORATORY COMMAND  
ATTN: AMSLC-TP (DR GONANO)  
ADELPHI MD 20783-1145

1

## DEPARTMENT OF THE NAVY

COMMANDING GENERAL  
US MARINE CORPS DEVELOPMENT  
& EDUCATION COMMAND  
ATTN: DO74 (LTC WOODHEAD)  
QUANTICO VA 22134

1