

AD-A193 554

A PERIMETRIST'S GUIDE FOR OPTIC DISC VISUAL FIELD

1/1

SCREENING: THE ARMY-D. (U) SCHOOL OF AEROSPACE

MEDICINE BROOKS AFB TX D W CARLSON ET AL. FEB 88


UNCLASSIFIED

USAFSAM-TP-87-4

F/O 6/5

NL



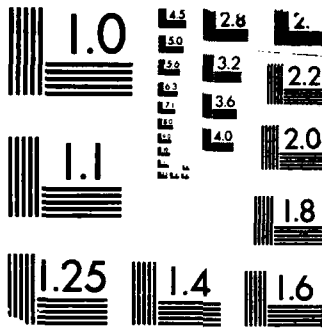

MICROCOPY RESOLUTION TEST CHART
NBS-1963-A

ANALYSIS OF THE EFFECTS OF OPTICALLY ACTIVE SUBSTANCES ON THE SPINNING OF ANISOTROPIC POLYMER SOLUTIONS

AD-A193 554

**DR. W. G. GIBSON, Captain, USAF, MC
L. S. GIBSON, Major, USAF, MC**

February 1968

Final Technical Report in Support of AFOSR Grant AF49(604)-01-0001

AD-A193 554

AFOSR-TR-68-001



NOTICES

This progress report was submitted by personnel of the Ophthalmology Branch, Medical Sciences Division, USAF School of Aerospace Medicine, Human Factors Division, AFSC, Brooks Air Force Base, Texas, under job order 7755-

When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely Government-related procurement, the United States Government incurs no responsibility or any obligation whatsoever. The fact that the Government may have formulated or in any way supplied the said drawings, specifications, or other data, is not to be construed by implication, or otherwise in any manner construed, as conveying the title or any other patent or proprietary right or as conveying any right of permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

The Office of Public Affairs has reviewed this report, and it is available to the National Technical Information Service, where it will be available to the general public, including foreign nationals.


This report has been reviewed and is approved for publication.



DEAN W. CARLSON, Captain, USAF, MC
Project Scientist



ROBERT S. QUINN, JR., Colonel, USAF, MC
Supervisor

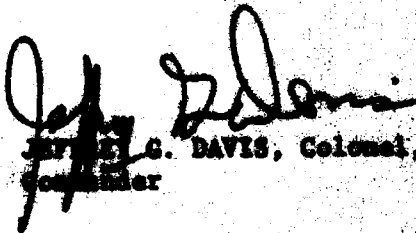

JEFFREY C. DAVIS, Colonel, USAF, MC
Commander

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE

ADA193554

REPORT DOCUMENTATION PAGE				Form Approved OMB No. 0704-0188			
1a. REPORT SECURITY CLASSIFICATION Unclassified			1b. RESTRICTIVE MARKINGS				
2a. SECURITY CLASSIFICATION AUTHORITY			3. DISTRIBUTION / AVAILABILITY OF REPORT Approved for public release; distribution is unlimited.				
2b. DECLASSIFICATION / DOWNGRADING SCHEDULE			5. MONITORING ORGANIZATION REPORT NUMBER(S)				
4. PERFORMING ORGANIZATION REPORT NUMBER(S) USAFSAM-TP-87-4			7a. NAME OF MONITORING ORGANIZATION				
6a. NAME OF PERFORMING ORGANIZATION USAF School of Aerospace Medicine		6b. OFFICE SYMBOL (If applicable) USAFSAM/NGOC		7b. ADDRESS (City, State, and ZIP Code)			
6c. ADDRESS (City, State, and ZIP Code) Human Systems Division (AFSC) Brooks Air Force Base, TX 78235-5301			9. PROCUREMENT INSTRUMENT IDENTIFICATION NUMBER				
8a. NAME OF FUNDING / SPONSORING ORGANIZATION USAF School of Aerospace Medicine		8b. OFFICE SYMBOL (If applicable) USAFSAM/NGOC		10. SOURCE OF FUNDING NUMBERS			
8c. ADDRESS (City, State, and ZIP Code) Human Systems Division (AFSC) Brooks Air Force Base, TX 78235-5301			PROGRAM ELEMENT NO. 62202F	PROJECT NO. 7755	TASK NO 24	WORK UNIT ACCESSION NO. 02	
11. TITLE (Include Security Classification) A Perimetrist's Guide for Optic Disc Visual Field Screening: The Armaly - Drance Method							
12. PERSONAL AUTHOR(S) Carlson, Dean W.; Tychsen, Lawrence							
13a. TYPE OF REPORT Progress		13b. TIME COVERED FROM 87/02 TO 87/12		14. DATE OF REPORT (Year, Month, Day) 1988, February		15. PAGE COUNT 14	
16. SUPPLEMENTARY NOTATION							
17. COSATI CODES			18. SUBJECT TERMS (Continue on reverse if necessary and identify by block number)				
FIELD 06	GROUP 05	SUB-GROUP	Armaly-Drance method, Goldman Visual Field, Glaucoma Visual Field, Screening Visual Field, Perimetry, Perimetrist				
19. ABSTRACT (Continue on reverse if necessary and identify by block number) Disc-related defects constitute over 90% of field defects found in typical outpatient clinical population--e.g., ischemic neuropathy, optic neuritis, glaucoma. This handout is designed for anyone who uses a Goldman Visual Field Perimeter. It describes an efficient standardized screening examination that, when mastered, should take the ophthalmologist, ophthalmology resident, and experienced or inexperienced ophthalmic technician only 5 to 10 minutes per eye to perform. The technique, developed by Armaly and modified by Drance, is a combination of kinetic and suprathreshold static perimetry. Detection of disc-related field defects has been shown to improve to 95% after a single day of instruction in the Armaly-Drance method.							
20. DISTRIBUTION / AVAILABILITY OF ABSTRACT <input checked="" type="checkbox"/> UNCLASSIFIED/UNLIMITED <input type="checkbox"/> SAME AS RPT. <input type="checkbox"/> DTIC USERS				21. ABSTRACT SECURITY CLASSIFICATION Unclassified			
22a. NAME OF RESPONSIBLE INDIVIDUAL Dean W. Carlson, Capt. USAF, MC				22b. TELEPHONE (Include Area Code) (512) 536-3258		22c. OFFICE SYMBOL USAFSAM/NGOC	

A PERIMETRIST'S GUIDE FOR OPTIC DISC VISUAL FIELD SCREENING :
THE ARMALY - DRANCE METHOD

INTRODUCTION

Disc-related defects constitute over 90% of field defects found in a typical outpatient clinic population--e.g., ischemic neuropathy, optic neuritis, glaucoma.

This paper will teach anyone who uses a Goldman visual field perimeter to use it better. It describes an efficient standardized screening examination that, when mastered, should take the ophthalmologist, ophthalmology resident, and experienced or inexperienced ophthalmic technician only 5 to 10 min per eye to perform.

The technique, developed by Armaly (2) and modified by Drance (3), is a combination of kinetic and suprathreshold static perimetry.

While this is an accurate test, the quality of any visual field examination is only as good as the care taken by the perimetrist.

Detection of disc-related field defects has been shown to improve to 95% after a single day of instruction in the Armaly-Drance method.



Accession For	
DTIS GRA&I	<input checked="" type="checkbox"/>
DTIC TAB	<input type="checkbox"/>
Unannounced	<input type="checkbox"/>
Justification	
By _____	
Distribution/	
Availability Codes	
Dist	Avail and/or Special
A-1	

GENERAL CONSIDERATIONS

- Use the perimeter in a completely dark room, free from distractions. It must be calibrated each day before it is used.
- Explain the test clearly and firmly. Fixation must be stressed. The patient should be comfortable.
- Tell the patient to use "tapping" or other nonverbal signals. Do not let the patient talk.
- Start the examination with the best eye, if known.
- Use an accurate refraction. Correct for astigmatism greater than 0.75 diopters.
- Use the appropriate near addition for the central (25°) field. The following are estimates:

30-39 years old	+1.0 sph
40-44 years old	+1.5 sph
45-49 years old	+2.0 sph
50-54 years old	+2.5 sph
55-60 years old	+3.0 sph
Over 60 years	+3.5 sph

- Determine the correct lens to use by placing a near reading card in the bowl.
- Use narrow rim trial lenses if available. Touch the lenses to the patient's brow.
- Follow a systematic approach; but, at the same time, avoid getting into a rhythm.
- Rest after each 10 to 15 min of testing.
- Record all details of the examination, including the patient's name, examiner, date, pupillary size, corrections used, target size, etc. Also evaluate the patient's reliability. Without this vital information, your visual field is of little use to the patient or to the ophthalmologist.

STATIC PRESENTATIONS

- Avoid getting into a rhythm.
- Use presentations of 1 sec duration ("on-one thousand-off").
- Retest all misses.
- If missed twice, then record with an open circle.
- If missed three times, then search the area kinetically for the extent of the scotoma.

KINETIC PRESENTATIONS

- Pause after the initial presentation to make sure the patient can't see the target.
- Move the target at 4 degrees per second until it is seen ("line-one-thousand-two-one-thousand-line").
- Avoid following the horizontal and vertical meridians.

THE ARMALY - DRANCE METHOD

1. Determine a stimulus that is above threshold at 25°.

With the appropriate refractive add for near correction in position, place the target 15° above and below the temporal horizontal meridian at 25° from fixation (Fig. 1). If the target is not seen, then increase intensity (I 3e to I 4e) or size (I 4e to II 4e).

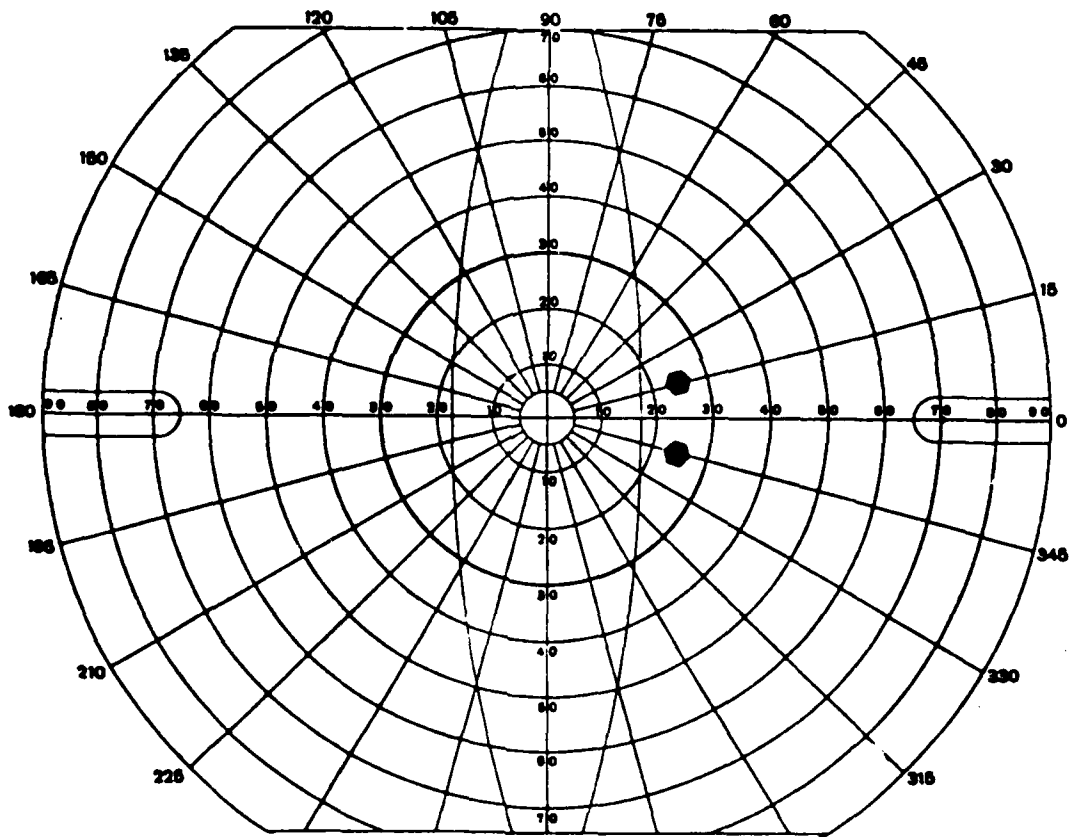


Figure 1

os. (00)

II. Map the blind spot.

Use the same stimulus and map the blind spot kinetically in eight directions (Fig. 2) to familiarize the patient with the test and also to detect enlargement of the blind spot.

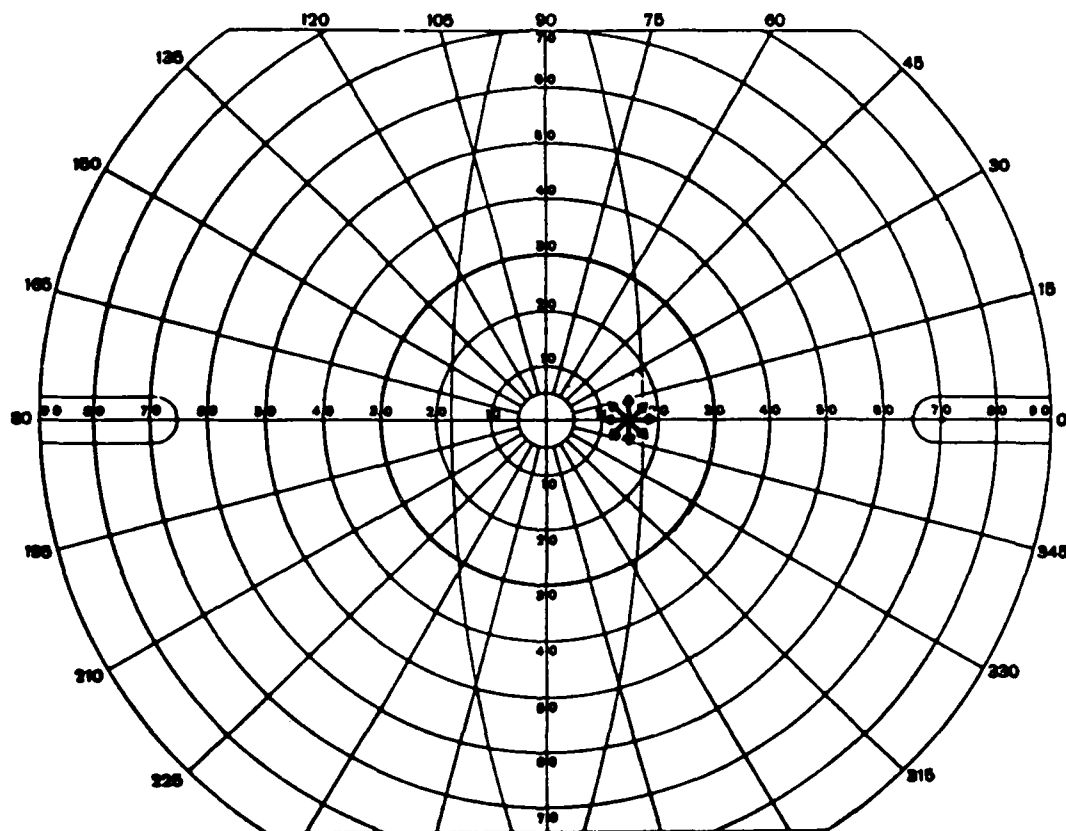


Figure 2

oa. (D)

III. Try to detect the four main defects.

1. Para-central scotomas (central, cecocentral, and arcuate)

Using the same stimulus, statically check at 5°, 10°, 15°, along each 15° meridian (Fig. 3). You will detect over 75% of the earliest visual field defects if you do this correctly.

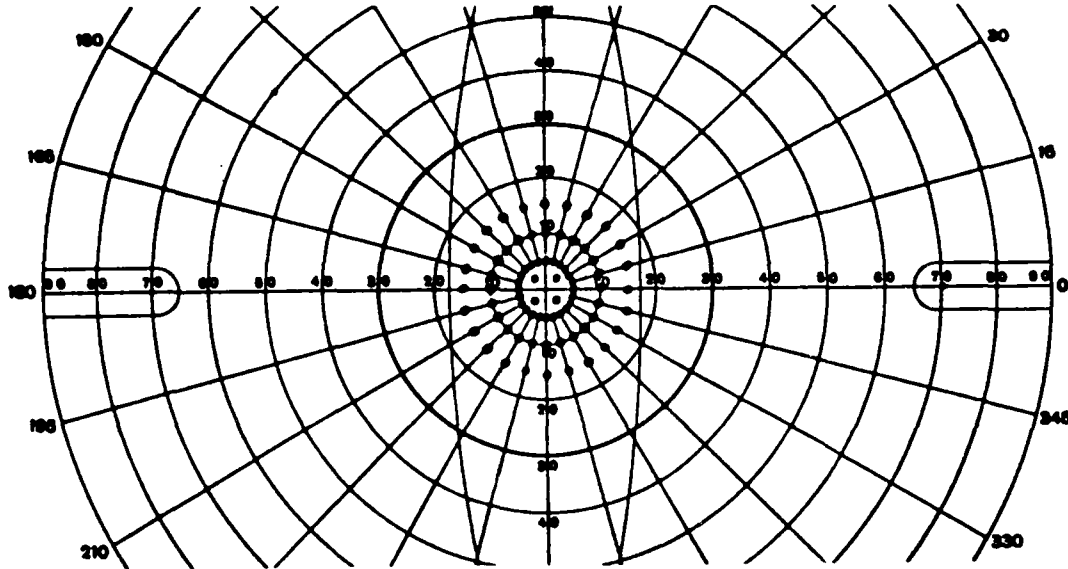


Figure 3

os. (50)

2. Nasal step in the central field

Again, use the same stimulus and determine kinetically the nasal isopter at 5°, 10°, 15°, and 30°, above and below the nasal horizontal meridian (Fig. 4).

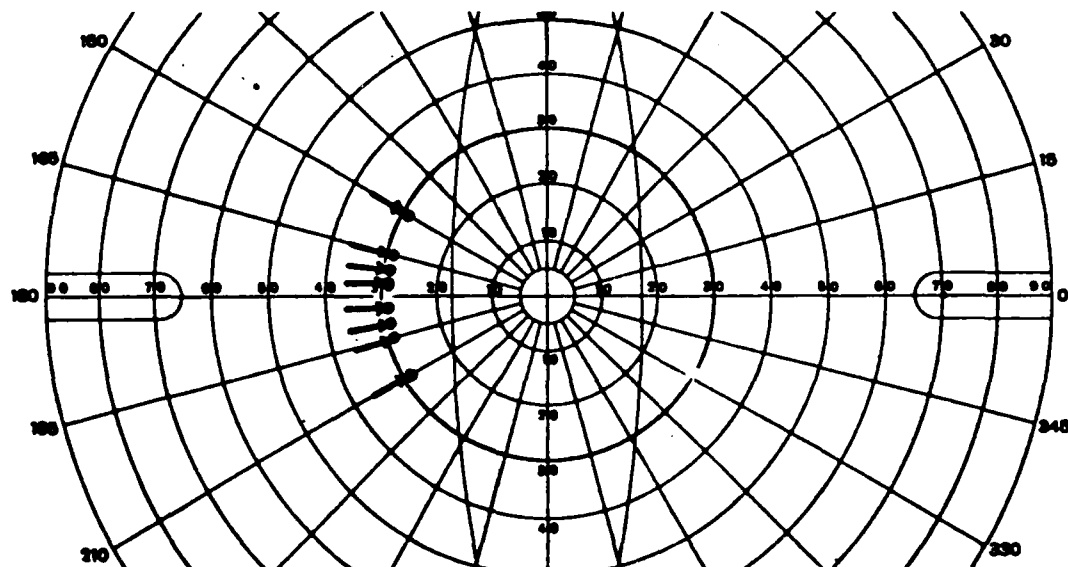


Figure 4

os. (50)

3. Nasal step in the peripheral field

Remove all corrective lenses. Place the I 4e target at 70° on the temporal side (Fig. 5). If not seen, then increase target size (II 4e, III 4e).

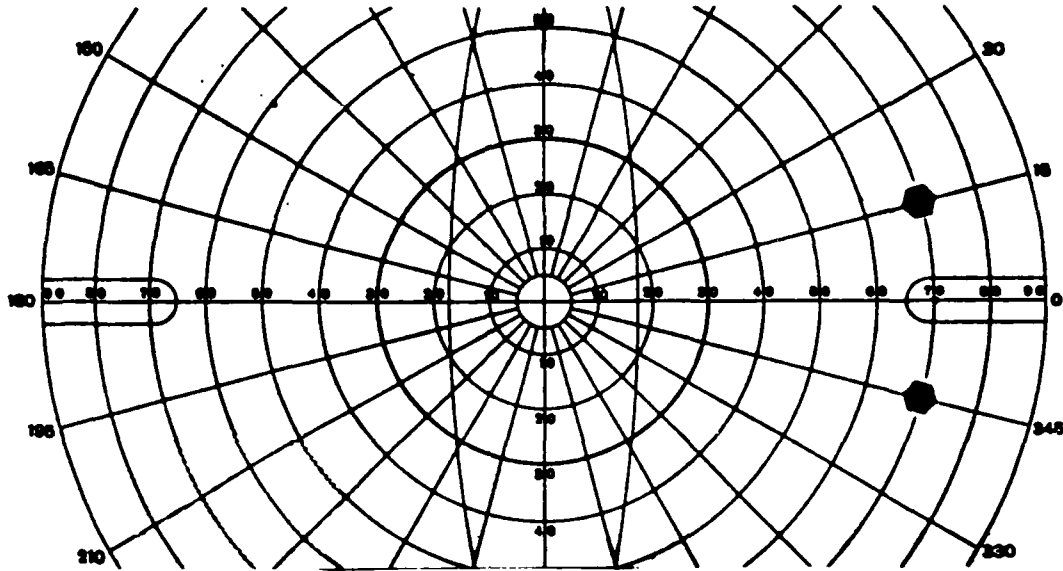


Figure 5

OS. (D)

Kinetically map the nasal isopter at 5°, 10°, 15°, and 30° above and below the nasal horizontal meridian (Fig. 6).

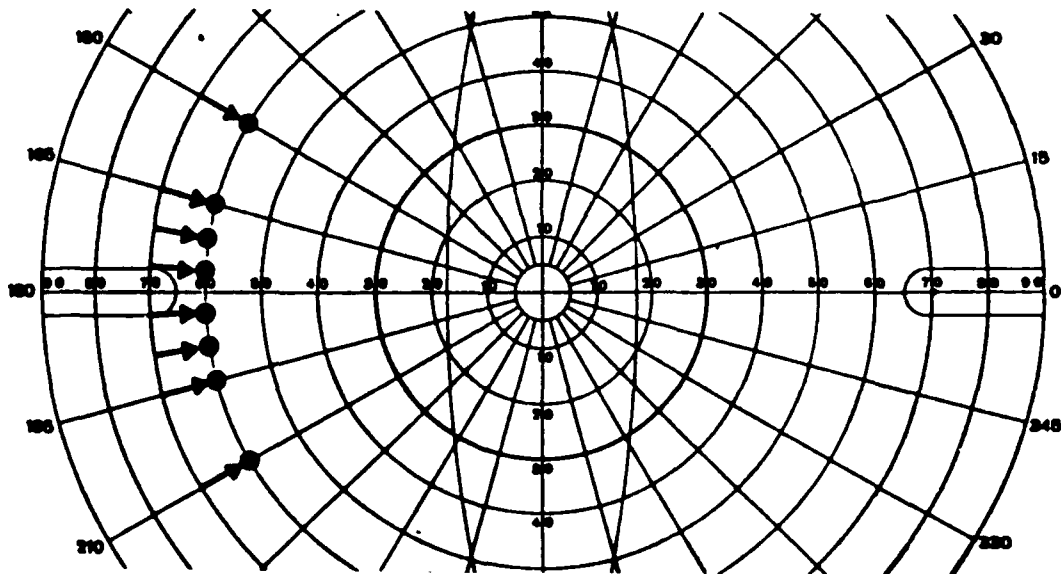


Figure 6

OS. (D)

4. Temporal sector defects

Use the same stimulus and kinetically search the temporal half of the visual field every 15° (Fig. 7). Then statically search within the temporal field for areas of depression.

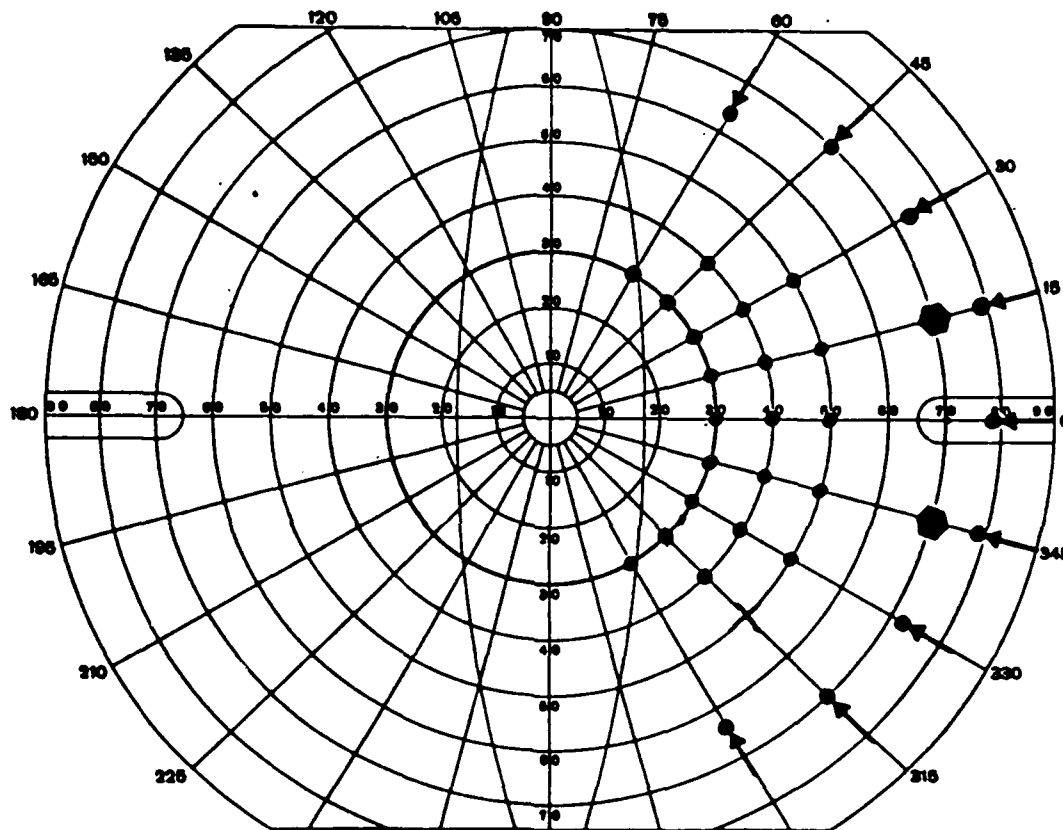


Figure 7

os. (50)

REFERENCES

1. Anderson, D.R. Testing the field of vision. St. Louis, C.V. Mosby Co, 1982.
2. Armaly, M.F. Ocular pressure and visual fields. Arch Ophthalmol 81:25-40(1969).
3. Drance, S.M. A modification of the Armaly visual field screening technique for glaucoma. Can J Ophthalmol 6:283-292(1971).
4. O'Connor, P.S. A perimetrist's guide for glaucoma visual field screening. USAF School of Aerospace Medicine, Brooks AFB, TX, Mar 1982.
5. Ophthalmology Basic and Clinical Science Course, Section 8. American Academy of Ophthalmology, San Francisco, CA, p 50, 1986.

END

DATE

FILMED

8-88

DTIC