

DTIC FILE COPY

2

BBM 00685

A convenient spectroscopic method
for the estimation of hemoglobin concentrations
in cell-free solutions

S.M. Snell and M.A. Marini

REPRINTED FROM:

AD-A201 384

A proven record of efficient handling and rapid
publication of research reports

DISTRIBUTION STATEMENT A

Approved for public release
Distribution Unlimited

DTIC
ELECTE
NOV 21 1988
S H D

88 11 21 36
ELSEVIER SCIENCE PUBLISHERS
BIOMEDICAL DIVISION

Journal of Biochemical and Biophysical Methods

managing editor C.F. CHIGNELL, Laboratory of Molecular Biophysics, National Institute of Environmental Health Sciences, Box 12233, Research Triangle Park, NC 27709 U.S.A.

associate managing editor S. HJERTEN, Institute of Biochemistry, Biomedical Centre, University of Uppsala, Box 576, S-751 23 Uppsala, Sweden

EDITORIAL BOARD

R.L.P. Adams (U.K.)
R.L. Berger (U.S.A.)
S. Beychok (U.S.A.)
O.J. Bjerrum (Denmark)
J. Chattopadhyaya (Sweden)
A. Chrambach (U.S.A.)
J.S. Cohen (U.S.A.)
L. De Maeyer (F.R.G.)
H. Hirai (Japan)
E.G. Janzen (Canada)

L.N. Johnson (U.K.)
H. Köster (F.R.G.)
A. Kuksis (Canada)
J.R. Lakowicz (U.S.A.)
A.H. Levy (U.S.A.)
Liang Chih-Chuan (People's Republic of China)
J.S. Miller (U.S.A.)
W. Müller (F.R.G.)
D.A. Peattie (U.S.A.)

Yu.A. Ovchinnikov (U.S.S.R.)
P.G. Righetti (Italy)
M.A.J. Rodgers (U.S.A.)
G. Schill (Sweden)
P. Todd (U.S.A.)
O. Vesterberg (Sweden)
D.F.H. Wallach (U.S.A.)
M. Wickek (Israel)
R.M. Winslow (U.S.A.)

Subscription information

The subscription price (1987) for Volumes 14 and 15 (2 volumes in 12 issues) is Dfl. 550.00 (US \$221.75); postage and handling included. The Dutch guilder price is definitive. The US \$ price is subject to exchange rate fluctuations and is therefore only given as a guide. Journals are sent by surface delivery to all countries, except the following countries where SAL airdelivery (Surface Airlifted Mail) is ensured: U.S.A., Canada, Japan, Australia, New Zealand, P.R. China, India, Israel, South Africa, Malaysia, Singapore, South Korea, Taiwan, Pakistan, Hong Kong, Brazil, Argentina, Mexico and Thailand. Airmail rates for other countries are available on request.

Subscription orders can only be entered by calendar year (Jan.-Dec.) and should be sent to: Elsevier Science Publishers B.V., Journals Department, P.O. Box 211, 1000 AE Amsterdam, The Netherlands. Telex 18582 ESPA NL, or any other subscription agent. Claims for missing issues should be made within three months of publication otherwise they cannot be honoured free of charge.

The Publishers reserve the right to issue additional volumes during the course of the year. Such volumes will be invoiced before publication and delivered on receipt of payment.

In the U.S.A. and Canada, for further information and personal subscriptions, contact: Elsevier Science Publishers, Journal Information Center, 52 Vanderbilt Avenue, New York, NY 10017. Tel. (212) 370-5520.

© 1987 Elsevier Science Publishers B.V. (Biomedical Division)

All rights reserved. No part of this publication may be reproduced, stored in a retrieval system or transmitted, in any form or by any means, electronic, mechanical, photocopying, recording or otherwise, without the prior written permission of the publisher, Elsevier Science Publishers B.V. (Biomedical Division), P.O. Box 15, 1000 RM Amsterdam, The Netherlands.

Submission of a paper to this journal entails the author's irrevocable and exclusive authorization of the publisher to collect any sums or considerations for copying or reproduction payable by third parties (as mentioned in article 17, paragraph 2 of the Dutch Copyright Act of 1912 and in the Royal Decree of June 20, 1974 (S. 351) pursuant to article 16b of the Dutch Copyright Act of 1912) and/or to act in or out of Court in connection therewith.

For an explanation of the code line at the bottom of each title page the reader is referred to page iv of the first issue of this volume.

Special regulations for readers in the U.S.A. This journal has been registered with the Copyright Clearance Center, Inc. Consent is given for copying of articles for personal or internal use, or for the personal or internal use of specific clients. This consent is given on the condition that the copier pays through the Center the per-copy fee stated in the code on the first page of each article for copying beyond that permitted by Sections 107 or 108 of the U.S. Copyright Law. The appropriate fee should be forwarded with a copy of the first page of the article to the Copyright Clearance Center, Inc., 27 Congress Street, Salem, MA 01970, U.S.A. If no code appears in an article the author has not given broad consent to copy and permission to copy must be obtained directly from the author. All articles published prior to 1980 may be copied for a per-copy fee of US \$2.25, also payable through the Center. This consent does not extend to other kinds of copying such as for general distribution, resale, advertising and promotion purposes, or for creating new collective works. Special written permission must be obtained from the publisher for such copying.

Special regulations for authors. Upon acceptance of an article by the journal, the author(s) will be asked to transfer copyright of the article to the publisher. This transfer will ensure the widest possible dissemination of information.

Printed in The Netherlands

2

BBM 00685

A convenient spectroscopic method for the estimation of hemoglobin concentrations in cell-free solutions

S.M. Snell and M.A. Marini

Letterman Army Institute of Research, Presidio of San Francisco, CA 94129-6800, U.S.A.

(Received 24 February 1988)

(Accepted 11 May 1988)

SELECTED
NOV 21 1988
H

Summary

Using a millimolar absorptivity of 7.12 ± 0.09 at 523 nm, it is possible to estimate the total concentration of hemoglobin in solutions containing oxyhemoglobin, deoxyhemoglobin and methemoglobin in any combination. This estimate is independent of the pH in the range 6.0-10.0 and will provide concentrations comparable to that obtained by the conventional and more precise use of cyanomethemoglobin. This methodology should be of value for the determination of extracellular hemoglobin in vivo, as a means for determining the vascular half-life of stroma-free hemoglobin based blood substitutes.

Key words: Methemoglobin spectrum; Isobestic point; pH dependency; Concentration estimation; Hemoglobin

Introduction

Hemoglobin concentrations are routinely estimated by conversion to the cyanomethemoglobin derivative [1] which is a stable derivative with a broad maximum centered at 540 nm and a millimolar absorptivity of 11.00 [2]. By this procedure, it is possible to determine the total hemoglobin content of solutions which contain mixtures of oxyhemoglobin, deoxyhemoglobin, methemoglobin and

Correspondence address: M.A. Marini, Letterman Army Institute of Research, Presidio of San Francisco, CA 94129-6800, U.S.A.

The opinions or assertions contained herein are the private views of the authors and are not to be construed as official or as reflecting the views of the Department of the Army or the Department of Defense (AR 360-5).

0165-022X/88/\$03.50 © 1988 Elsevier Science Publishers B.V. (Biomedical Division)

DISTRIBUTION STATEMENT A

Approved for public release;
Distribution Unlimited

carboxyhemoglobin with an error of less than 2%. Another minor component occasionally present is sulfohemoglobin which is not converted to the cyanomethemoglobin, but it causes little error since it is normally present in low concentration and it has a millimolar absorptivity of approximately 7 at 540 nm. It is also possible to approximate the hemoglobin concentration by using a millimolar absorptivity of 15.3 at 576 nm [3] on the basis that the major component of an aerated solution is composed mainly of oxyhemoglobin.

For the study of the metabolic fate of in vivo stroma-free hemoglobin, however, it can be anticipated that the solution would contain a mixture of oxy-, deoxy- and methemoglobin. Estimation of the total concentration by cyanomethemoglobin is awkward, and the estimation at 576 nm would be erroneous. This error would be further enhanced by the pH dependence of the methemoglobin spectra.

During a study of the formation of methemoglobin as a function of pH, it was observed that isobestic points or a narrow isobestic region occurred at 489, 523 and 616 nm. An isobestic point near 523 nm had also been observed by Kaplan [4] who used it to calculate the amount of methemoglobin in solutions of oxyhemoglobin. However, both oxy- and deoxyhemoglobin have pH independent absorbances at 523 nm which were identical to that of equal concentrations of methemoglobin. Since neither carboxy- nor sulfohemoglobin is expected to be formed in these studies, a convenient and rapid method for the estimation of total hemoglobin concentration was suggested.

Experimental

Stroma-free hemoglobin (pH 7.2, 10 μ S) was prepared from recently outdated human blood by the method of Rabiner et al. [5]. Oxygenated hemoglobin was used directly since no spectral change was observed after equilibration with water-saturated oxygen in a tonometer. The solutions for spectral analysis were prepared from a common stock of stroma-free hemoglobin (8 g/dl, with $A_{577\text{nm}} \approx 76$ determined on a 1:100 dilution at 1 cm lightpath) by passing 10 ml through a mixed-bed ion-exchange column of Bio-Rex RG 501-X8 (1.5 $\times$ 30 cm) and capturing it in a 50 ml volumetric flask. The ion free eluate ($< 5 \mu$ S) was diluted 1:10 with 0.11 M Tris-HCl, pH 7.4, and the spectra taken with a Cary-14 spectrophotometer equipped with an on-line data acquisition system (OLIS, Jefferson, GA). Spectra were obtained between 450 and 650 nm at intervals of 1 nm. Each spectrum was taken at least twice and averaged.


Deoxyhemoglobin was prepared from this solution by placing 4 ml in a tonometer (Instrumentation Lab. Inc., Lexington, MA) and equilibrating with water-saturated nitrogen at room temperature for 15 min. Samples were taken directly from the tonometer with a nitrogen-purged syringe and transferred to a nitrogen-purged teflon-stoppered cuvette and the spectra obtained. Sodium dithionite crystals were then added and the spectra again recorded. Occasionally there were slight alterations observed, and only those spectra which were essentially unchanged by the addition of dithionite were considered. Longer periods for the conversion to

Carboxyhemoglobin was prepared from the dilute deionized oxyhemoglobin by passing water-saturated carbon monoxide over a stirred solution at room temperature for periods up to 1 h. The solutions were transferred with a carbon monoxide-purged syringe into a carbon monoxide-purged teflon-stoppered cuvette and the spectrum recorded. Complete conversion to carboxyhemoglobin required longer times than that for conversion to deoxyhemoglobin so the spectra obtained were altered due to the differences in concentration. Adjustment of these spectra on the basis of the concentrations determined by the cyanomethemoglobin derivative gave a millimolar absorptivity of 10.1 at 523 nm.

Various mixtures of oxy- and methemoglobin were prepared from the column eluates (≈ 1 mM) and diluted 1 : 10 with 0.11 M Tris-HCl at the desired pH. These samples were at the same total concentration as those previously prepared, and the spectra, as well as the total concentration of hemoglobin in the solutions [1] and the methemoglobin concentration [6], were obtained. Methemoglobin was also estimated by an analysis of the spectra by a 200 point inversion matrix [7].

Spectra of methemoglobin as a function of pH from 6.1 to 10.22 at room temperature in 0.1 M Tris are shown in Fig. 1. The isobestic point or region at 523 nm has an absorption of 7.12 ± 0.09 for a millimolar concentration of methemoglobin. The values ranged from 7.09 to 7.42 and the higher values all occurred above pH 9.4. This increase is also present in the calculation of the ionization constant for the ionization of ferriheme (Fig. 2) and may be due to a general unfolding at elevated pH. The pK' calculated for a variety of wavelengths is 7.99 ± 0.08 using the curve-fitting algorithm, MLAB [8]. A pK' value of 8.14 had previously been reported for $\mu = 0.05$ at 20°C [9]. Brunori et al. [10] found $pK' = 8.05$ at 20°C and $\mu = 0.2$. The isobestic point at 523 nm may also be seen for the spectra of oxy- and deoxyhemoglobin (Fig. 3). The curves were obtained on

Codes
u/or

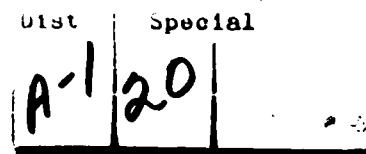

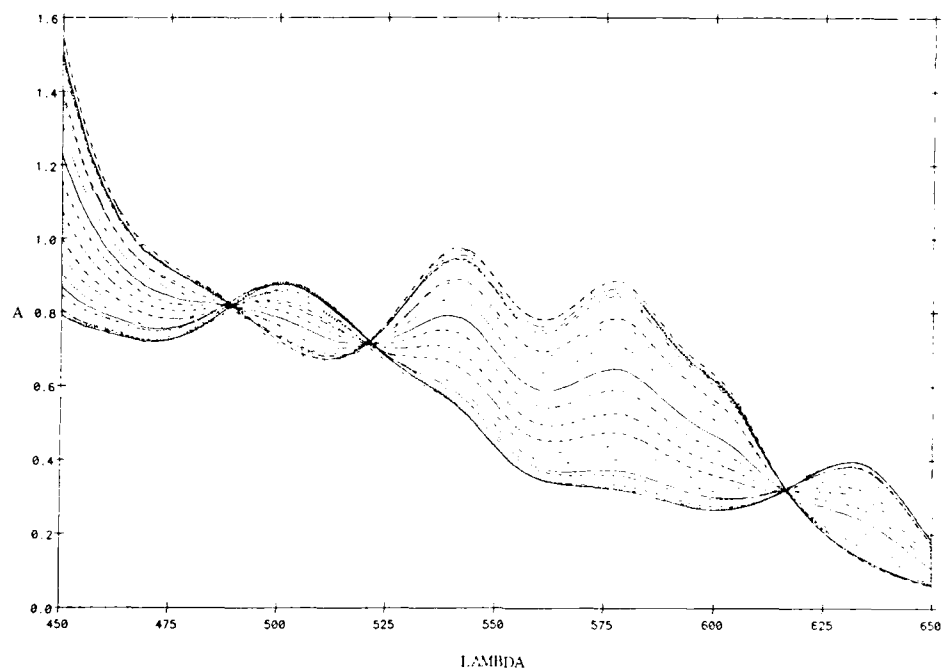


Fig. 1. Absorbance of methemoglobin as a function of pH. The lowest curve at 579 nm is that obtained at pH 6.1 in 0.1 M Tris-HCl. Subsequent spectra to pH 10.22 are those obtained at approximately 0.2 pH intervals. All the spectra were obtained at room temperature. The concentration of the samples was 0.1 mM.

TABLE 1

MILLIMOLAR ABSORPTIVITIES OF HEMOGLOBIN DERIVATIVES

Lambda	HbO ₂	SD	Hb	SD	MetHb	SD
450	15.88	0.10	14.57	0.20	9.87	0.05
460	10.88	0.05	5.37	0.17	8.58	0.10
470	8.15	0.03	3.58	0.13	7.96	0.09
480	6.55	0.03	3.42	0.11	7.95	0.10
490	5.63	0.03	3.73	0.09	8.37	0.12
500	5.10	0.03	4.42	0.08	8.59	0.13
510	4.85	0.04	5.47	0.07	8.12	0.11
520	6.03	0.04	6.58	0.07	7.38	0.06
530	10.48	0.04	8.16	0.11	6.97	0.11
540	14.22	0.02	10.67	0.16	6.72	0.20
550	11.57	0.05	13.03	0.11	5.55	0.17
560	8.58	0.04	13.06	0.11	4.57	0.16
570	11.89	0.06	11.39	0.09	4.63	0.21
580	13.70	0.07	9.13	0.18	4.67	0.22
590	3.64	0.10	6.76	0.05	3.95	0.06
600	0.86	0.06	3.65	0.06	3.45	0.10
610	0.38	0.05	1.97	0.05	3.21	0.10
620	0.22	0.05	1.41	0.04	3.30	0.09
630	0.15	0.05	1.18	0.05	3.48	0.10
640	0.11	0.05	1.04	0.04	2.90	0.09
650	0.08	0.05	0.96	0.04	1.57	0.06

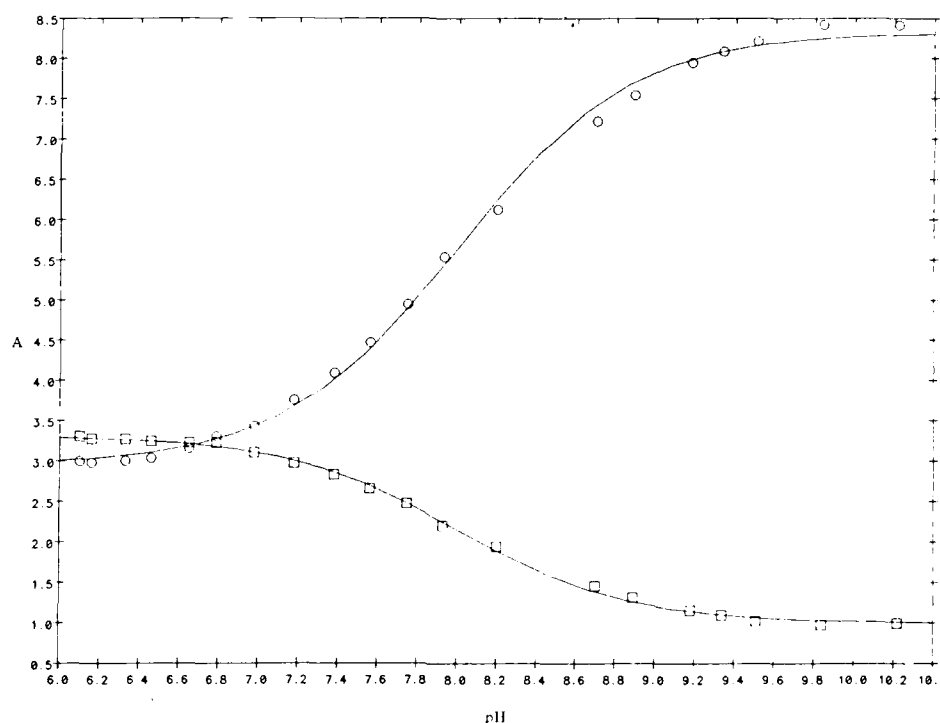


Fig. 2. The pH dependence of the spectra of methemoglobin. Points are the experimental values expressed as the millimolar absorptivity differences; the lines are calculated for a pK' of 7.99 for the ionization of ferriheme. The upper curve (circles) is obtained at 579 nm; the lower curve (squares) is that found at 639 nm.

solutions prepared by the volumetric procedures described. They may also be obtained by conversion of any concentration of hemoglobin using the millimolar absorptivities calculated from the absorption at 523 nm, or by the absorption of the cyanomethemoglobin at 540 nm using a millimolar absorptivity of 11.0 [3]. From a minimum of 17 separate spectra, the average absorptivities and the standard deviation were determined and are given in Table 1.

The millimolar absorptivity for HbO_2 found is somewhat below that of Van Assendelft [13], ϵ_{577} of 15.37. It is, however, somewhat higher than the values reported by Zijlstra et al. [14] for HbO_2 solutions of the concentration 0.05 mM which is comparable to those used in the present study (0.03–0.1 mM). They reported a millimolar absorptivity at 577 nm of 15.03 ± 0.27 compared to 15.22 ± 0.08 found here.

It is difficult to compare the spectra of methemoglobin found here with that given by Van Assendelft [13] inasmuch as he reported the spectra for the pH range 7.0–7.4 to be identical. The spectra shown in Fig. 3 indicate that the spectra are pH-dependent in this range. The values reported (Table 1) tend to fall between those of Van Assendelft [13] and Benesch et al. [12]. This variation is not due to the

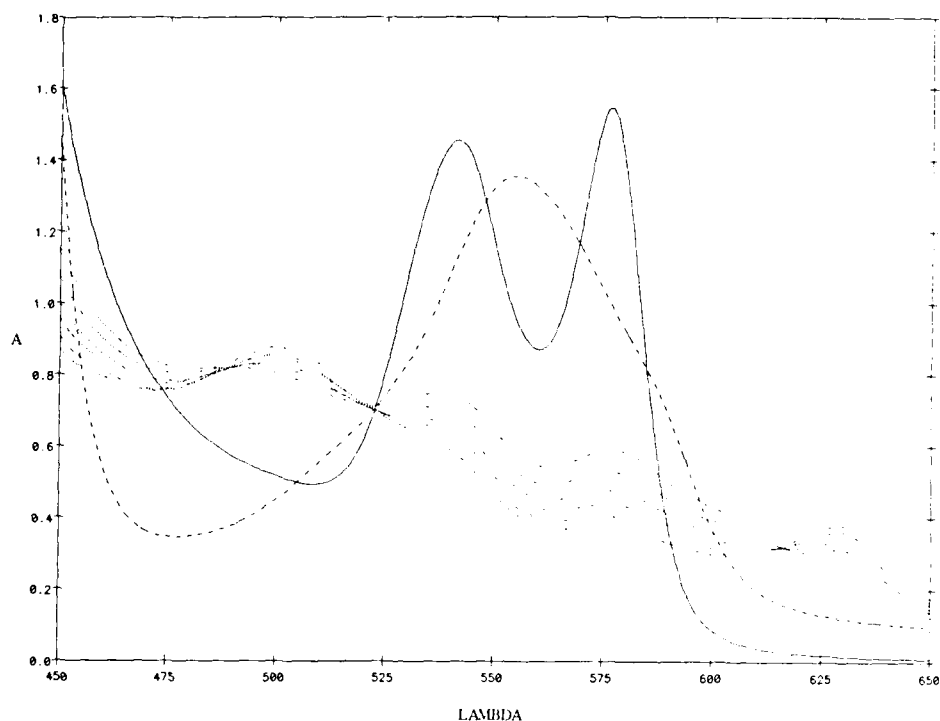


Fig. 3. Isobestic regions for the spectra of oxyhemoglobin (solid line), deoxyhemoglobin (dashed line) and methemoglobin. The methemoglobin spectra (dotted lines) are for pH 6.98 (lower curve at 575 nm) and pH 7.21, 7.41, 7.55 and 7.80, successively. The concentrations of the samples were prepared as discussed in the text to be 0.1 mM so that the millimolar absorptivities may be easily calculated.

nature of the buffers used inasmuch as spectra in phosphate buffers (0.1 M) for the pH values ranging from 6.0 to 8.0 are identical to those in 0.1 M Tris-HCl. Nor are the variations due to any differences in the methemoglobin structure caused by either ferricyanide or nitrite since these spectra are very nearly identical after passage through the mixed-bed resin when the slight reversion to oxyhemoglobin is considered. Nonetheless, because of the difficulty encountered in preparing a fully oxidized preparation that is also stripped of the oxidizing reagent, the spectra show a greater variation than either the oxy- or deoxyhemoglobin spectra. For deoxyhemoglobin, a millimolar absorptivity $\epsilon_{555\text{ nm}}$ of 13.35 ± 0.12 is found. This compares to $\epsilon = 13.29$ reported by Zwart et al. [15] but is higher than $\epsilon = 13.04$ reported by Van Assendelft [13] at the same wavelength.

A comparison of the estimation of hemoglobin concentration by the cyanomethemoglobin methodology and the use of the isobestic point at 523 nm is given in Table 2. Concentrations are calculated by:

$$\text{g/dl} = (A_{523\text{ nm}})(\text{dil})(1.611)/7.12 \quad (1)$$

where the factor 1.611 converts millimolar to gram per decilitre. Various concentra-

TABLE 2

COMPARISON OF HEMOGLOBIN CONCENTRATION BY DRABKIN'S AND BY THE ABSORPTION AT 523 nm

Hb (g/dl) (Drabkin's)	Hb (g/dl) ($A_{523\text{nm}}$)	MetHb (%)
0.93	1.01	4.50
0.93	1.01	11.10
1.36	1.37	4.22
1.46	1.54	4.40
1.61	1.60	1.40
1.76	1.76	8.49
2.00	2.00	5.40
7.77	7.85	1.70
7.91	7.85	100.00
8.02	7.93	10.82
9.33	9.35	0.64
9.62	9.63	100.00
9.88	9.71	1.66
13.60	13.33	9.10

tions of hemoglobin containing the fractions of methemoglobin shown were analyzed with very good agreement. Some of the lower concentration samples were exposed to water-saturated nitrogen for varying periods of time to provide some deoxyhemoglobin. The amount of deoxyhemoglobin present was not monitored.

TABLE 3

VARIATION OF THE HEMOGLOBIN CONCENTRATION BY ESTIMATION AT 523 nm^a

Absorption	Hb (g/dl)
0.6518	7.37
0.6531	7.39
0.6765	7.65
0.6775	7.66
0.6718	7.60
0.6933	7.84
0.6571	7.43
0.6896	7.80
0.7137	8.07
0.6848	7.75
0.6971	7.89
0.6961	7.87
0.6790	7.68
0.6946	7.86
0.6868	7.77
Mean 0.6841	7.74
SD 0.0166	0.19

^a The original hemoglobin solution contained 0.66% methemoglobin. Some samples were converted to methemoglobin by ferricyanide or nitrite, deionized, diluted and assayed. Others were converted partially to deoxyhemoglobin and assayed.

TABLE 4

ESTIMATION OF HEMOGLOBIN CONCENTRATION AT VARIOUS pH VALUES USING $A_{523\text{nm}}$

pH	$A_{523\text{nm}}$	Hb (g/dl)
5.96	0.8589	9.72
6.17	0.8788	9.94
6.44	0.8525	9.64
7.01	0.8631	9.76
7.21	0.8601	9.73
7.41	0.8621	9.75
7.55	0.8605	9.74
7.62	0.8529	9.65
7.80	0.8664	9.80
8.43	0.8672	9.81
8.83	0.8633	9.77
9.22	0.8668	9.81
9.59	0.8658	9.79
9.77	0.8655	9.79
9.95	0.8656	9.79
Mean	0.8630	9.76
SD	0.0060	0.07

Using a single sample of stroma-free hemoglobin, the concentrations shown in Table 3 are obtained. The range of concentrations is 7.37 to 8.07 g/dl which seems quite large. These same samples were assayed by the cyanomethemoglobin method which gave a range of 7.46 to 7.99 g/dl with an average of 7.83 ± 0.15 in substantial agreement with the average 7.74 ± 0.19 obtained using the isobestic absorption. This variation may be attributed to the manipulation of the samples during oxidation or deoxygenation and subsequent passage through the mixed-bed ion-exchange column. When a single sample of stroma-free hemoglobin prepared with 10% methemoglobin is analyzed as a function of pH, the values in Table 4 are obtained. The average is 9.76 ± 0.07 which is a better indication of the precision of the method.

It is quite important that the wavelength be precisely defined since the millimolar absorptivity for HbO_2 in this region is rising at 0.31/nm; Hb is rising at 0.12/nm, while that of methemoglobin is relatively flat, varying at $-0.04/\text{nm}$. Notwithstanding this difficulty, it would appear that the millimolar absorptivity at 523 nm is a convenient, precise and relatively simple measurement for estimating total hemoglobin concentrations of solutions consisting of oxy-, deoxy- and methemoglobin.

Simplified description of the method

Samples of hemoglobin solutions are read in a Cary-14 spectrophotometer at 523 nm. This reading is converted to the millimolar concentration by:

$$\text{mM(Hb)} = (A_{523\text{nm}})(\text{dil})/7.12$$

where 7.12 is the millimolar absorptivity for oxy-, deoxy- and methemoglobin at room temperature in 0.1 M ionic strength and in the pH range 6.0 to 10.

References

- 1 Van Kampen, E.J. and Zijlstra, W.G. (1961) *Clin. Chim. Acta* 6, 538-544
- 2 International Committee for Standardization in Haematology (1978) *J. Clin. Pathol.* 31, 139-143
- 3 Van Assendelft, O.W. and Zijlstra, W.G. (1975) *Anal. Biochem.* 69, 43-48
- 4 Kaplan, J.C. (1965) *Rev. Franc. Etudes Clin. Biol.* X, 856-859
- 5 Rabiner, S.F., Helbert, J.R., Lopas, H. and Friedman, L.H. (1967) *J. Exp. Med.* 126, 1127-1142
- 6 Evelyn, K. and Malloy, H. (1938) *J. Biol. Chem.* 126, 655-662
- 7 Snell, S.M., Shrager, R., Winslow, R.M. and Marini, M.A., in preparation
- 8 Knott, G.D. (1979) *Computer Prog. Biochem.* 10, 271-280
- 9 Beetstone, J.G. and Irvine, D.H. (1964) *J. Chem. Soc.* 5090-5095
- 10 Brunori, M., Amiconi, G., Antonini, E., Wyman, J., Zito, R. and Rossi Fanelli, A. (1968) *Biochim. Biophys. Acta* 154, 315-323
- 11 Drabkin, D.L. (1946) *J. Biol. Chem.* 164, 703-723
- 12 Benesch, R.E., Benesch, R. and Yung, S. (1973) *Anal. Biochem.* 55, 245-243
- 13 Van Assendelft, O.W. (1970) *Spectrometry of Haemoglobin Derivatives*, Royal van Gorcum, Assen, The Netherlands
- 14 Zijlstra, W.G., Buursma, A. and Zwart, A. (1983) *J. Appl. Physiol.* 54, 1287-1291
- 15 Zwart, A., Van Kampen, E.J. and Zijlstra, W.G. (1986) *Clin. Chem.* 32, 972-978

AIMS AND SCOPE

The *Journal of Biochemical and Biophysical Methods* will publish research papers dealing with the development of methods to solve biological problems. Articles may be concerned either with new methodology or with the significant modification of existing techniques. The scope of the Journal is broad encompassing all methodological aspects of biochemistry, biophysics and molecular biology. Although articles should be written in sufficient detail to allow easy verification they should also be intelligible to a broad scientific audience. In addition, the Journal will publish a section of short notes describing improvements in methods which, though significant, do not warrant a full-length research paper. Short review articles dealing with recent developments in a particular method or technique that are of interest to a broad scientific audience will also be published.

TYPES OF PAPERS

- (1) Full-length articles describing important new methods and significant developments in existing ones
 - (2) Short notes describing improvements in methods which, though significant, do not warrant full-length research papers
 - (3) Concise critical review articles on methods including their development, applicability and present status. These will initially be invited, but authors wishing to contribute to this section should send a proposal to one of the Managing Editors.
- Articles should be written in sufficient detail to allow easy verification and theoretical understanding and in a manner intelligible to a wide scientific audience.

Submission of a paper to the *Journal of Biochemical and Biophysical Methods* implies the transfer of copyright from the author to the Publisher and that it is not being submitted for publication elsewhere. Papers should be submitted to an appropriate editor, or to one of the Managing Editors if uncertain of to which Editorial Board member it should be sent.

INSTRUCTIONS TO AUTHORS

Manuscripts should be submitted to an appropriate editor (see inside front cover). In order to expedite publication, the original and three copies are required of both text and illustrations. Duplicates of photographs must be of the same standard as the originals. The manuscript should be typed with double spacing and wide margins on one side of the paper only and should be accompanied by a separate title page giving the authors' names and affiliations, as well as an address for correspondence. Words to be printed in italics should be underlined.

Full-length methodology articles should

- (a) be divided into sections (Summary, Introduction, Materials and Equipment, Methodology, Discussion, Simplified Description of the Method and its Applications);
- (b) contain a Summary not exceeding 200 words, at the beginning of the paper, followed by 3-6 key words;
- (c) not exceed 10 printed pages (approximately 18 typewritten pages) including the space required for figures. Longer papers will be considered, but may be subject to delayed publication;
- (d) contain a concluding paragraph which presents a simplified description of the method, its advantages and potential applications.

Full-length applications articles should

- (a) be divided into sections (Summary, Introduction, Materials, Methods and Equipments and Results, Discussion, Applications of Results to other areas);
- (b) & (c) as for methodology papers;
- (d) contain a concluding paragraph which presents a description of application of results to other biological disciplines.

Full-length reviews should be on methodological advances only, usually on invitation from a member of the Editorial Board.

Short notes should, in principle, not exceed 2000 words, contain only one figure but be adequately referenced.

Additional information: Authors are requested to submit together with their manuscript sufficient experimental results to substantiate the method described therein in order to facilitate critical and rapid refereeing. This information will be returned if requested.

References should be numbered singly in the order of citation in the text and listed in numerical sequence on a separate sheet. In the text they should be referred to by their numbers in square brackets in line with the rest of the text. First and last relevant page numbers are to be included in the reference list. The abbreviations of periodical titles should conform to those adopted by *Bibliographic Guide for Editors and Authors*, 1974, and in the list citation of periodicals [1], books [2] and multi-author books [3] should accord with the following examples:

1. Pipps, J.P. and Buchanan, J.M. (1977) *Biochim. Biophys. Acta* 247: 181-184.
2. Dixon, M. and Webb, E.C. (1964) *Enzymes*, 2nd edn., pp. 565-567. Longmans Green, London.
3. Brachet, J. (1967) *Comprehensive Biochemistry* (Florkin, M. and Stoltz, E.M., eds.), Vol. 28, pp. 23-54. Elsevier, Amsterdam.

Authors are urged to follow the instructions given in *Information for Contributors to Biochimica et Biophysica Acta*, which is available free of charge from: BBA Editorial Secretariat, P.O. Box 1345, 1000 BH Amsterdam, The Netherlands.

Tables should be typed double spaced on separate sheets, numbered consecutively with Arabic numerals, and only contain horizontal lines. A short descriptive title should appear above each table, with possible legend and footnotes (identified with a, b, c, etc.) below.

Figures should be line drawings in black ink or very sharp, well-contrasting prints on glossy paper suitable for immediate reproduction. Half-tone figures should be black and white, very sharp, well-contrasting and on glossy paper. Figures should be completely lettered, the size of the lettering being appropriate to that of the drawing, taking into account the necessary reduction in size. All legends should be typed double spaced on separate sheets. Tables, figures and photographs should be clearly marked on the reverse side with the number, author's name and orientation (top), using a soft pencil.

Proofs: proofreading will be performed by the Publisher. Authors may, however, specifically request proofs of their articles by including this request on the title page when the article is submitted. Proofs will only be supplied for the author to check for typesetting accuracy. No changes to the original manuscript will be allowed. The sending of proofs may cause a delay in publication.

Page charges will not be made.

Reprints may be ordered by filling in and returning to the Publishers the order form sent to the authors on acceptance of their paper. Fifty free reprints per contribution will be made available.

**A FREE SAMPLE COPY OF THE JOURNAL IS
AVAILABLE ON REQUEST ***

Free sample copies can be obtained from: Elsevier Science Publishers, Journals Department, P.O. Box 211, 1000 AE Amsterdam, The Netherlands. Tel. (020) 5803 911.

ORDER FORM

Send to your usual supplier or:

ELSEVIER SCIENCE PUBLISHERS,
P.O. Box 211, 1000 AE Amsterdam,
The Netherlands.

For further information and/or free specimen copy, write to:

In the U.S.A. and Canada:

Journal information center,
ELSEVIER SCIENCE PUBLISHERS,
52 Vanderbilt Avenue, New York, NY 10017,
U.S.A.

In the rest of the world, write to the Promotion Manager in Amsterdam.

JOURNAL OF BIOCHEMICAL AND BIOPHYSICAL METHODS

1987, Volumes 14-15 (2 volumes in 8 issues)

Please enter a subscription for 1987 at US\$ 221.75/Dfl. 550.00 including postage
and handling

ISSN 0165-022X

- ☐ Please send me a proforma invoice
☐ Please send me a free sample copy

Please bill my credit card:

- | | | | |
|---|-----------------------------------|---------------------------------|-----|
| ☐ MasterCard | ☐ Eurocard | ☐ Access | No. |
| ☐ American Express | | | No. |
| ☐ Visa | | | No. |

Card No.

Valid until

Name

Address

Postal Code

Date

Signature

The Dutch guilder price is definitive. US \$ prices are subject to exchange rate fluctuations.
Prices are excl. BTW for Dutch customers.

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE

REPORT DOCUMENTATION PAGE				Form Approved OMB No. 0704-0188	
1a. REPORT SECURITY CLASSIFICATION			1b. RESTRICTIVE MARKINGS		
2a. SECURITY CLASSIFICATION AUTHORITY			3. DISTRIBUTION/AVAILABILITY OF REPORT		
2b. DECLASSIFICATION/DOWNGRADING SCHEDULE			Approved for public release; distribution is unlimited.		
4. PERFORMING ORGANIZATION REPORT NUMBER(S)			5. MONITORING ORGANIZATION REPORT NUMBER(S)		
6a. NAME OF PERFORMING ORGANIZATION Letterman Army Institute of Research		6b. OFFICE SYMBOL (if applicable) SGRD-ULBR		7a. NAME OF MONITORING ORGANIZATION	
6c. ADDRESS (City, State, and ZIP Code) Presidio of San Francisco, CA 94129-6800			7b. ADDRESS (City, State, and ZIP Code)		
8a. NAME OF FUNDING/SPONSORING ORGANIZATION		8b. OFFICE SYMBOL (if applicable)		9. PROCUREMENT INSTRUMENT IDENTIFICATION NUMBER	
8c. ADDRESS (City, State, and ZIP Code)			10. SOURCE OF FUNDING NUMBERS		
			PROGRAM ELEMENT NO.	PROJECT NO.	TASK NO.
			WORK UNIT ACCESSION NO.		
11. TITLE (Include Security Classification) A convenient spectroscopic method for the estimation of hemoglobin concentrations					
12. PERSONAL AUTHOR(S) S. M. Snell and M. A. Marini					
13a. TYPE OF REPORT research		13b. TIME COVERED FROM 9/87 TO 1/88		14. DATE OF REPORT (Year, Month, Day) 1988 Jan 4	
15. PAGE COUNT 20					
16. SUPPLEMENTARY NOTATION Journal of Biochemical and Biophysical Methods 1988; 17: 25-34.					
17. COSATI CODES			18. SUBJECT TERMS (Continue on reverse if necessary and identify by block number)		
FIELD	GROUP	SUB-GROUP	methemoglobin spectra, isobestic points, pH dependency, estimation of Hb concentration		
19. ABSTRACT (Continue on reverse if necessary and identify by block number) Using a millimolar extinction coefficient of 7.12 at 523 nm, it is possible to estimate the total concentration of hemoglobin in solutions containing oxyhemoglobin, deoxyhemoglobin and methemoglobin in any combination. This estimate is independent of the pH in the range 6.0 to 10.0 and will provide concentrations comparable to that obtained by the conventional and more precise use of cyanomethemoglobin. This methodology should be of value for the determination of extracellular hemoglobin <u>in vivo</u> .					
20. DISTRIBUTION/AVAILABILITY OF ABSTRACT ☒ UNCLASSIFIED/UNLIMITED ☐ SAME AS RPT ☐ DTIC USERS			21. ABSTRACT SECURITY CLASSIFICATION unclassified		
22a. NAME OF RESPONSIBLE INDIVIDUAL Mario Marini			22b. TELEPHONE (Include Area Code) (415) 561-5875		22c. OFFICE SYMBOL

DD Form 1473, JUN 86

Previous editions are obsolete.

SECURITY CLASSIFICATION OF THIS PAGE
UNCLASSIFIED