

1000 1000
NBDL-88R001

FABRICATION AND APPLICATION OF A
STANDARDIZED T1/T2 MOUNT

Norman S. Gilbert, M.D., Stephen V. Mawn, M.D.,
Salvadore J. Guccione, Jr., Ph.D, Ferris E. Bolin

Naval Biodynamics Laboratory
Box 29407
New Orleans, LA 70189-0407

December 1988

AD-A208 328



DTIC
ELECTE
MAY 23 1989
S H D
cb

Approved for public release; distribution is unlimited.


Prepared for

Naval Medical Research and Development Command
Bethesda, MD 20014

REPORT DOCUMENTATION PAGE


1a REPORT SECURITY CLASSIFICATION Unclassified			1b RESTRICTIVE MARKINGS		
2a SECURITY CLASSIFICATION AUTHORITY			3 DISTRIBUTION/AVAILABILITY OF REPORT		
2b DECLASSIFICATION/DOWNGRADING SCHEDULE					
4 PERFORMING ORGANIZATION REPORT NUMBER(S) NBDL-88R001			5 MONITORING ORGANIZATION REPORT NUMBER(S)		
6a NAME OF PERFORMING ORGANIZATION Naval Biodynamics Laboratory		6b OFFICE SYMBOL (If applicable)	7a NAME OF MONITORING ORGANIZATION		
6c ADDRESS (City, State, and ZIP Code) P. O. Box 29407 New Orleans, LA 70189-0407			7b ADDRESS (City, State, and ZIP Code)		
8a NAME OF FUNDING SPONSORING ORGANIZATION Naval Medical Research and Development Center		8b OFFICE SYMBOL (If applicable)	9 PROCUREMENT INSTRUMENT IDENTIFICATION NUMBER		
8c ADDRESS (City, State, and ZIP Code) Naval Medical Command Building 1, Tower 12 Bethesda, MD 20814-5044			10. SOURCE OF FUNDING NUMBERS		
			PROGRAM ELEMENT NO 6321	PROJECT NO M0097	TASK NO .001
11 TITLE (Include Security Classification) Fabrication and Application of a Standardized T1/T2 Mount (Unclassified)					
12 PERSONAL AUTHOR(S) N. S. Gilbert, S. V. Mawn, S. J. Guccione, F. E. Bolin (Naval Biodynamics Laboratory)					
13a TYPE OF REPORT		13b TIME COVERED FROM _____ TO _____		14. DATE OF REPORT (Year, Month, Day) December 1988	
				15 PAGE COUNT 6	
16 SUPPLEMENTARY NOTATION					
17 COSATI CODES			18 SUBJECT TERMS (Continue on reverse if necessary and identify by block number)		
FIELD	GROUP	SUB-GROUP	acceleration, impact, cervical spine, kinematic measurements		
06	02				
19 ABSTRACT (Continue on reverse if necessary and identify by block number) Experimental impact forces which affect the cervical spine are accurately reflected at T1 and consequently can be measured there. Adventitious movement of an acceleration measuring system at T1 can distort data and thereby diminish the validity of conclusions drawn from that data. A standardized T1/T2 mount has been fabricated and used to improve the study of human response to experimental impact. Gross slippage has not been evident since adopting the new mount and strapping techniques.					
20 DISTRIBUTION/AVAILABILITY OF ABSTRACT ☒ UNCLASSIFIED/UNLIMITED ☐ SAME AS RPT ☐ DTIC USERS			21. ABSTRACT SECURITY CLASSIFICATION		
22a NAME OF RESPONSIBLE INDIVIDUAL JAMES F. PALMER, CDR, MSC, USN			22b TELEPHONE (Include Area Code) (504) 257-3922		22c OFFICE SYMBOL

Approved by



CDR James F. Palmer, MSC, USN
Chairman,
Scientific Review Committee

Released by



CAPT Douglas W. Call, MSC, USN
Commanding Officer

Naval Biodynamics Laboratory
P.O. Box 29407
New Orleans, LA 70189-0407

Approved for public release; distribution is unlimited.
Reproduction in whole or part is permitted for any purpose of the
United States Government.

The interpretations and opinions in this work are the
authors' and do not necessarily reflect the policy and views of
the Navy or other government agencies.

Volunteer subjects were recruited, evaluated, and employed in
accordance with the procedures specified in Department of Defense
Directive 3216.2, Secretary of the Navy Instruction 3900.39
series, and Bureau of Medicine and Surgery Instruction 3900.6
series. These instructions meet or exceed the provisions of
prevailing national and international guidelines.

The animals used in this work were handled in accordance with
the principles outlined in the "Guide for the Care and Use of
Laboratory Animals (National Institutes of Health Document No.
NIH 80-23)," established by the Institute of Laboratory Animal
Resources, National Research Council.

To be precise, trade names of products are cited. These
citations do not constitute endorsements of the products.

FABRICATION AND APPLICATION
OF A STANDARDIZED T1/T2 MOUNT

INTRODUCTION

Human response to impact is studied at the Naval Biodynamics Laboratory (NAVBIODYNLAB) using a horizontal accelerator which propels a restrained subject in a sled along an indoor track. Similar research using a vertical accelerator will begin in the near future at the Laboratory. Experimental impact forces which affect the cervical spine and head are accurately reflected at the subject's first thoracic vertebra (T1), and consequently can be measured there.

A system to measure acceleration at T1 has been developed which consists of: (1) an anatomical mount molded from each subject's cervicothoracic region; (2) a fixture which is fastened to the mount and held to the subject by straps; and (3) a plate carrying accelerometers and photo targets which is attached to the fixture. Unfortunately, kinematic measurements from this instrument package reflect not only T1 motion, but also any adventitious movement of the package.

Since the anatomical mount can not be rigidly attached to T1 (e.g., surgically attached to the spinous process of T1), there has been concern about whether the instrument package accurately follows T1 motion. Review of cinephotography has shown occasional package movement relative to T1 depending on the input force and the coupling between the package and the subject. Adventitious mount movement can create distortions in the force input/acceleration output relationship between T1 and the cervical spine and head. As a result, mathematical models designed to represent dynamic head and neck interaction and manikins which are based on this data may be less reliable in certain vectors.

Since beginning human impact experiments in 1973, the NAVBIODYNLAB staff has attempted to design an anatomical mount which minimizes adventitious movement. A shearless T1 mount which could be strapped to a specific and repeatable surface location on a subject's upper back was specially designed.¹ The goal was to design a mount which would follow T1 motion regardless of changes occurring in torso configuration and strap length during acceleration.

Procedures to apply the mount were outlined in detail in 1985.² Later, a study of the effect of mount slippage on various T1 acceleration components was completed.³ T1 accelerations were taken from a Hybrid III dummy with a rigidly attached mount and compared with one in which the mount was merely strapped. Minimal differences were seen in the X linear acceleration component (the primary driver of head motion), but all other components had spurious oscillations which indicated some motion relative to T1.

Since then, a series of seven human runs in the -X direction have been analyzed and spurious oscillations and/or spikes were



Dist Special

A-1

Codes
1/or

identified in some less significant components. Moreover, during a recent human +Z series, data analysis, film review, and pre- and post-run photographs of skin impressions made by the mount evidenced sporadic slippage.

Further measures, therefore, were indicated to control cervicothoracic mount slippage. A study comparing the dynamic responses of three different geometries showed that the best data reproducibility was exhibited by a mount overlying the spinous processes of both T1 and T2.⁴ The fabrication and application of a standardized T1/T2 mount is outlined below.

FABRICATION

Until 1976, the NAVBIODYNLAB's thoracic mounts were fabricated using traditional fiberglass techniques. An impression was lifted from a subject's spine with a mixture of dental plaster, chopped fiberglass strands, polyester resin, and a hardener. After this impression cured, a second one was taken from it as a positive form upon which a mount with excellent structural integrity and biofidelity was made. This method required a craftsman from outside the Laboratory and was eventually abandoned. In 1976, the Laboratory adopted a method which used fiberglass orthopedic cast material which hardened when exposed to ultraviolet light. Unfortunately, this fiberglass material became unavailable in 1985 and a new fabrication method was required.

The latest method, which is similar to the original three-step fiberglass technique, yields a thoracic mount of improved biofidelity by making a greater surface contact with the skin overlying T1 and T2. The new method can be divided into two procedures: modeling and construction.

A. Modeling

(1) Using a felt tip pen, mark the subject's skin overlying the spinous processes of C7, T1, and T2 (Figure 1). The spinous processes are best identified with the subject seated on a stool, head flexed, and arms hanging loosely at the sides.

(2) Apply a lubricant to aid in the separation of the impression from the subject's skin. Common hand lotion serves as a good releasing agent.

(3) Mix children's modeling clay and mineral oil in a ratio of one cubic inch of clay to one drop of oil.

(4) Press this mixture, in a container 4" long x 3" wide x 1/2" deep, over the area from C7 - T2. The entire area must be covered and adequate pressure must be applied (Figure 2).

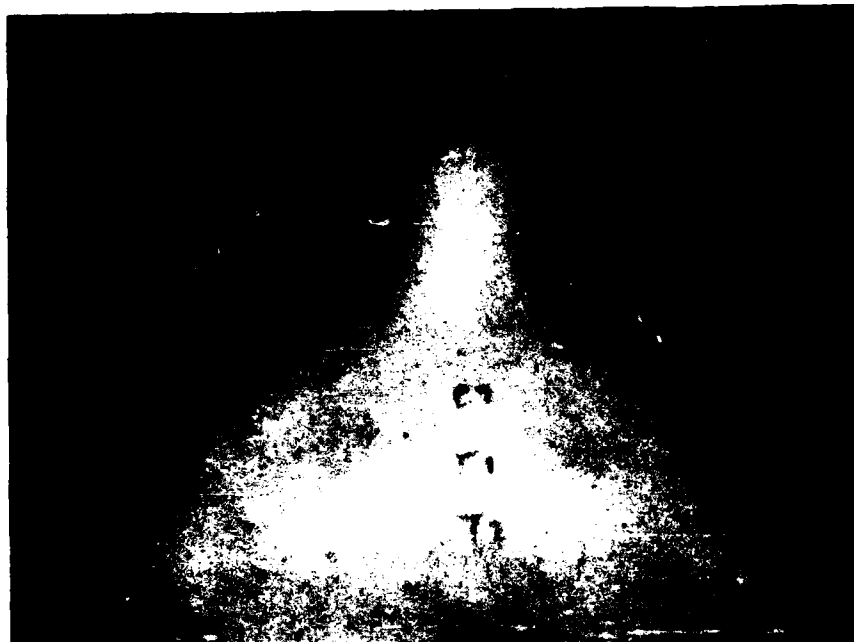


FIGURE 1 - Skin overlying subject's C7, T1, and T2 spinous processes appropriately marked for modeling.



FIGURE 2 - Impression being taken from subject's cervicothoracic region.

(5) Place the impression in a freezer for one hour.

(6) Remove the impression, in its container, from the freezer and fill the container to the top with Plaster of Paris. Allow the plaster to dry for approximately 24 hours.

B. Construction

(1) After the plaster model is dry, examine it for holes or bumps caused by the drying process. These defects should be filled or sanded to conform to the subject's surface anatomy.

(2) Thinly coat the surface to be fiberglassed with a standard mold releasing agent.

(3) After the releasing agent is dried, apply enough coats of white gelcoat (1 to 3) to the entire top surface (surface contacting the spinous processes) of the model to obtain a 1/32" thickness.

(4) When the gelcoat is cured, the mount can be constructed according to the dimensions in Figure 3.

APPLICATION

High speed cinephotography and data analysis of impact runs have indicated that the thoracic mount occasionally tends to move away from T1 upon abrupt neck flexion. This movement varies unpredictably between runs. In 1985, an experiment was conducted to determine if the movement resulted from variability in mount strapping tightness. The investigators found that excessive, inadequate, or uneven strap tightening resulted in a poor tracking of the mount to T1 motion. Therefore, developing a standard strapping procedure has been considered a crucial part controlling mount slippage.

Due to anatomical variation between subjects, a formal strapping procedure presents difficulty. Nonetheless, adherence to certain steps can minimize adventitious mount movement during a run.

(1) Before moving to the sled (and before attaching straps and instrumentation to the mount), position the T1/T2 mount properly on the subject's back. The spinous processes in the cervicothoracic region are best identified with the subject seated on a stool, head flexed, and arms hanging. Using a felt tip pen, trace an outline of the upper border of the mount onto the subject's skin. This mark will aid in placing the mount properly when the subject is on the sled.

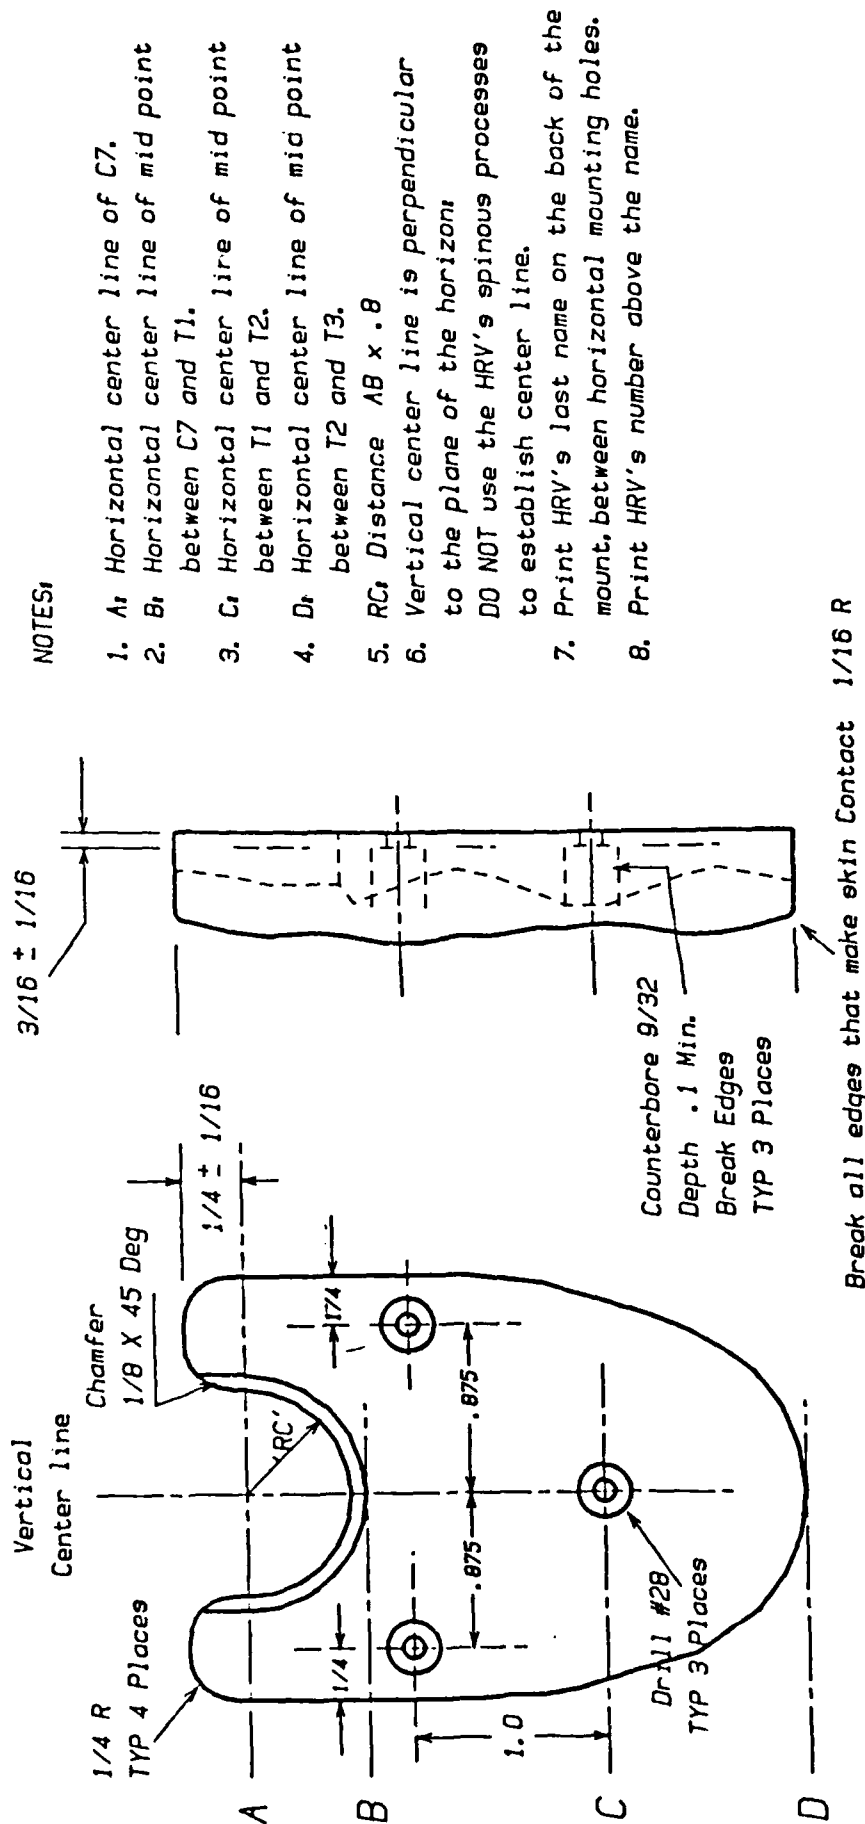


FIGURE 3 - Schematic drawing of standardized T1/T2 mount.

NOTES:

1. A, Horizontal center line of C7.
2. B, Horizontal center line of mid point between C7 and T1.
3. C, Horizontal center line of mid point between T1 and T2.
4. D, Horizontal center line of mid point between T2 and T3.
5. RC, Distance AB x .8
6. Vertical center line is perpendicular to the plane of the horizontal DO NOT use the HRV's spinous processes to establish center line.
7. Print HRV's last name on the back of the mount, between horizontal mounting holes.
8. Print HRV's number above the name.

All dimensions are shown in inches.

MATERIAL:

Unsaturated polyester resin

GENERAL DESCRIPTION:

The mount is formed from the T1/T2 spinous processes. It contains two colors of fiberglass. The white color is next to the skin, is 1/8-3/16 in. thick and contains two layers of 1/2 oz. fiberglass mat. The blue color is 1/4-5/16 in. thick with three layers of fiberglass mat. Fiberglass strands are rolled through-out both colors to increase strength.

TOLERANCES	NAVAL BIODYNAMICS LABORATORY	
DECIMAL	MICHAUD STATION	NEW ORLEANS LA
± .01 in.	SCALE	DRAWN BY R BLACK
FRACTIONAL	FULL	APPROVED BY
± 1/32 in.	TITLE	T1/T2 MOUNT
ANGULAR	DATE	DRAWING NUMBER
± N/A	4/27/88	A-065

(2) After the subject is in the sled's restraint system and has flexed his neck, place the T1/T2 mount into proper position. Hold the mount firmly in position and begin tightening all four straps. Continue to tighten the straps with the subject's neck in a neutral or slightly flexed position. The front straps should be substantially tighter than the rear ones when this step is completed.

(3) A simple check can be performed to assess the adequacy of the strapping. Pull the subject back into the seat with the restraints and ask him to flex his neck. If the T1/T2 mount does not pull away from the skin or otherwise alter its position, strapping is satisfactory. If the mount does pull away or change position, the restraints are released and step 2 is repeated.

CONCLUSION

Since adopting the standardized T1/T2 mount and strapping procedure, gross slippage as reflected by either distorted skin impressions or data with obvious artifacts has not been seen. Nevertheless, certain concerns have been expressed about the T1/T2 mount.

A criticism has been made that the T1/T2 mount measures T1/T2 motion rather than purely T1. A second objection has been raised that splinting by the mount may effect T1 motion itself. The benefit of reducing adventitious mount movement using an increased area of skin contact, however, greatly outweighs these potential disadvantages. Moreover, it is doubtful that a mathematical model will be developed which will require differentiating between T1 motion and T1/T2 motion.

REFERENCES

1. Muzzy III, W. H. and Becker, E. B., Shearless T-1 Instrumentation Mount, Proceedings of the Thirteenth Annual International Workshop on Human Subjects for Biomechanical Research, Arlington, Virginia, 1985, pp. 75-77.
2. Naval Biodynamics Laboratory, Memorandum by L. S. Lustick on Stability of T1 Mounts, New Orleans, LA, 25 September 1985.
3. Seaman, M. R., Hybrid III Hard Mount/Soft Mount on the Motion of T1 Instrumentation Packages, Task Number NB-TE-3782, Naval Biodynamics Laboratory, New Orleans, LA, September 1987.
4. Naval Biodynamics Laboratory, Memorandum by L. S. Lustick and J. M. Bartholomew on Measurement of Acceleration at T1, New Orleans, LA, 16 January 1981.