

4

**CHEMICAL
RESEARCH,
DEVELOPMENT &
ENGINEERING
CENTER**



CRDEC-TR-208

**VAPOR PRESSURE MEASUREMENT
WITH DIFFERENTIAL THERMAL ANALYSIS:
AN IMPROVEMENT IN THE METHOD**

**Donald Fielder
Ann Brozena**

RESEARCH DIRECTORATE

October 1990

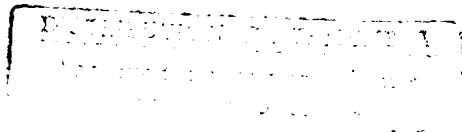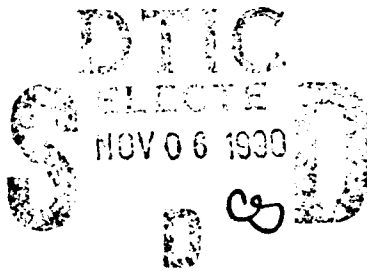

**U.S. ARMY
ARMAMENT
MUNITIONS
CHEMICAL COMMAND**

Aberdeen Proving Ground, Maryland 21010-5423

AD-A228 699

Disclaimer

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorizing documents.

Distribution Statement

Approved for public release; distribution is unlimited.

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE 1990 October	3. REPORT TYPE AND DATES COVERED Final, 88 Nov - 89 Feb	
4. TITLE AND SUBTITLE Vapor Pressure Measurement with Differential Thermal Analysis: An Improvement in the Method			5. FUNDING NUMBERS PR-1C162622A553I	
6. AUTHOR(S) Fielder, Donald, and Brozena, Ann				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) CDR, CRDEC, ATTN: SMCCR-RSC-P, APG, MD 21010-5423			8. PERFORMING ORGANIZATION REPORT NUMBER CRDEC-TR-208	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)			10. SPONSORING/MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution is unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) A method is described that extends the temperature range over which vapor pressure may be measured when using differential thermal analysis. The technique developed allows for measuring vapor pressure of pure liquids that boil below room temperature.				
14. SUBJECT TERMS Vapor pressure Differential thermal analysis Subambient			15. NUMBER OF PAGES 17	
Freon-113 DTA Freon-114 Quick Cool			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT UNCLASSIFIED	18. SECURITY CLASSIFICATION OF THIS PAGE UNCLASSIFIED	19. SECURITY CLASSIFICATION OF ABSTRACT UNCLASSIFIED	20. LIMITATION OF ABSTRACT UL	

Blank

PREFACE

The work described in this report was authorized under Project No. 1C162622A553I, CB Simulants, Survivability and Systems Science. This work was started in November 1988 and completed in February 1989.

The use of trade names or manufacturers' names in this report does not constitute an official endorsement of any commercial products. This report may not be cited for purposes of advertisement.

Reproduction of this document in whole or in part is prohibited except with permission of the Commander, U.S. Army Chemical Research, Development and Engineering Center, ATTN: SMCCR-SPS-T, Aberdeen Proving Ground, Maryland 21010-5423. However, the Defense Technical Information Center and the National Technical Information Service are authorized to reproduce the document for U.S. Government purposes.

This report has been approved for release to the public.



ACQUISITION	
NTIS	
CNC	
Under	
Justification	
By	
Distribution	
Availability	
Dist	Availability
A-1	

Blank

CONTENTS

	Page
1. INTRODUCTION	7
2. EXPERIMENTATION	7
2.1 Temperature Control	7
2.2 Sample Handling	8
3. DISCUSSION	8
4. CONCLUSIONS	13
LITERATURE CITED	17

LIST OF FIGURES AND TABLES

		Page
	Figures	
1	DTA Cell Block Self-Warming Curve	9
2	Vapor Pressure of Freon 113: Literature vs. Experimental	10
3	Vapor Pressure of Freon-114: Literature vs. Experimental	11
4	Boiling Thermogram for Freon-113	14
5	Boiling Thermogram for Freon-114	15

Tables

1	Vapor Pressure Data for Freon-113	12
2	Vapor Pressure Data for Freon-114	13

VAPOR PRESSURE MEASUREMENT WITH DIFFERENTIAL THERMAL ANALYSIS: AN IMPROVEMENT IN THE METHOD

1. INTRODUCTION

The use of differential thermal analysis (DTA) to measure vapor pressure of pure liquids has been described in the open literature by Vassallo and Harden,¹ Chiu,² Kemme and Kreps,³ and Krawetz and Torrog⁴ and internally by Belkin and Brown.⁵ Basically, all the references cite the same techniques and instrumentation. The DTA technique requires a small sample size (0.02 μ l/data point) and permits rapid determination of the entire vapor pressure versus temperature curve (ca. 10 min/data point) from 10 to 760 torr. For these reasons, the DTA method is frequently preferred over other techniques (e.g., the Knudsen effusion method or isoteniscope, which require a greater sample volume and are much more time consuming) that are used in the U.S. Army Chemical Research, Development and Engineering Center laboratories. The references cited above describe measurement of vapor pressures of compounds that boil above room temperature. The method described in this report extends the temperature range for measuring vapor pressure by DTA to the subambient region.

2. EXPERIMENTATION

A DuPont Model 9900 Thermal Analyzer (DuPont Company, Wilmington, DE) was used in these experiments. The basic setup has been described previously.^{1,3} The major differences between this procedure and those used by Vassallo and Harden¹ and Kemme and Kreps³ were the use of a computer to control data acquisition and the employment of a Quick Cool sample holder accessory (DuPont Company). The Quick Cool accessory is a Dewar flask designed to hold the sample cell block, which allows for rapid cool down of the cell block and for subambient operations through the use of liquid nitrogen. The instrument was calibrated using triple distilled, deionized water, Freon 113 (trifluorotrichloroethane) and Freon 114 (1,2-dichloro-1,1,2,2-tetrafluoroethane). The pressure readout device was a Wallace and Tiernan Type 187 absolute manometer (Wallace and Tiernan, Belleville, NJ) capable of reading to the nearest 0.1 mm Hg.

2.1 Temperature Control.

Prior to measuring vapor pressures at very low temperatures, the ability of the DTA to control the rate of

temperature increase was investigated. Kemme and Kreps³ had determined that 5 deg/min was the optimum heating rate for determining the boiling point. Therefore, it was critical that the cooled cell block did not self-warm at a faster rate. The cell block was cooled to -180 °C and allowed to self-warm. Figure 1 is a plot of the rate of temperature increase with time. The observed temperature rise was well below the desired 5-deg/min heating rate and, therefore, presented no problems.

2.2 Sample Handling.

To load samples that boil below room temperature into the glass capillaries that are placed in the sample cell block, special handling techniques were developed. The compounds that boil below room temperature are normally received in lecture bottles (LB) equipped with valves. The samples are transferred from the LB to a Reacti-Vial (Pierce Chemical Company, Rockford, IL) that is equipped with a screw cap containing a rubber septum. The vial is precooled to a temperature below the boiling point of the compound under study, and a portion of the sample is transferred from the LB to the vial. Once a sufficient amount of sample has been collected, the vial is capped. The sample in the vial will remain a liquid as long as the cap does not leak. Transferring the sample to the DTA glass capillary tube is accomplished by cooling the cell block with the capillary in place and transferring the proper amount of liquid using a precooled microsyringe.

3. DISCUSSION


The technique developed allows one to establish a complete vapor pressure-temperature curve (10-760 mm Hg) in less than 2 hr with a minimum of sample size. Plots of the vapor pressure versus temperature for Freons 113 and 114, respectively, are shown in Figures 2 and 3 where the symbols are experimental points, and the line is the calculated vapor pressure from the literature.^{6,7} Tables 1 and 2 show the experimental temperatures and pressures compared with the calculated literature temperature at each experimental pressure. The data clearly indicate that the technique is quite good, giving data that agrees quite well with published values.

Representative thermograms are shown in Figures 4 and 5 as an example of output from the system.

Sample: EMPTY CAPILLARY (SELF-WARMING)
Size: 0.0050 mg
Method: SELF-WARMING CURVE
Comment: Proportional Band = 60

DTA

File: WARM.02
Operator: ABL
Run Date: 04/01/88 11:24

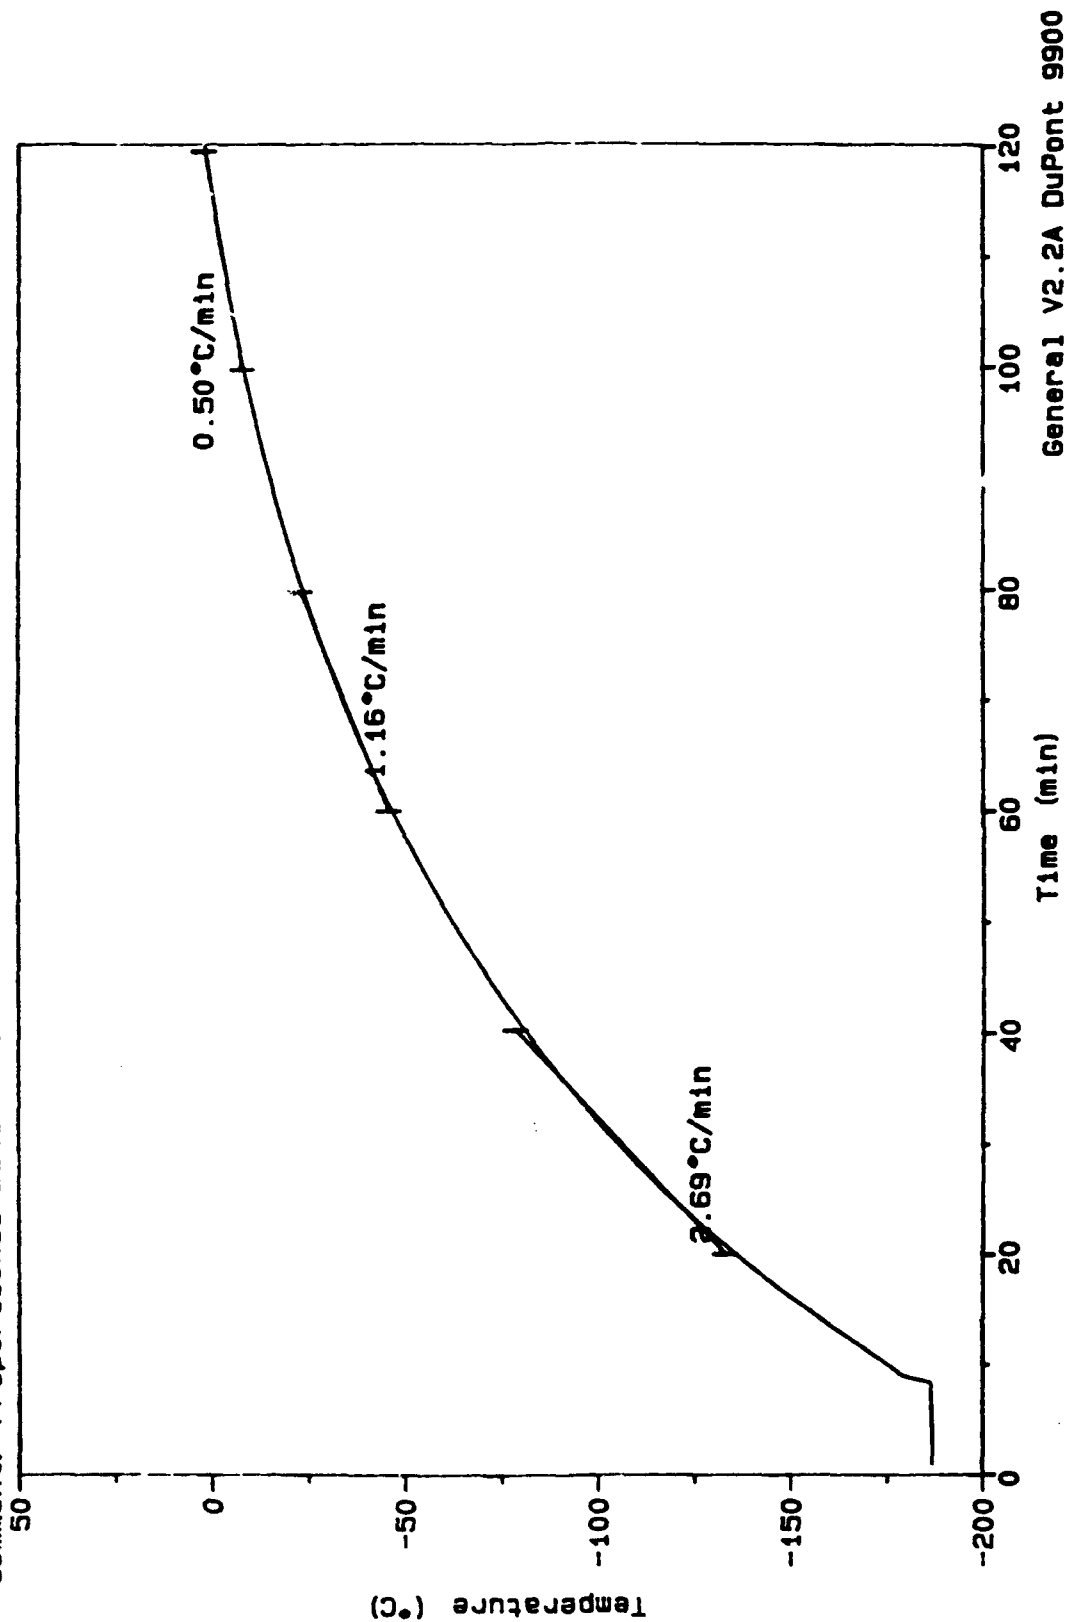

General V2.2A DuPont 9900

Figure 1. DTA Cell Block: Self-Warming Curve

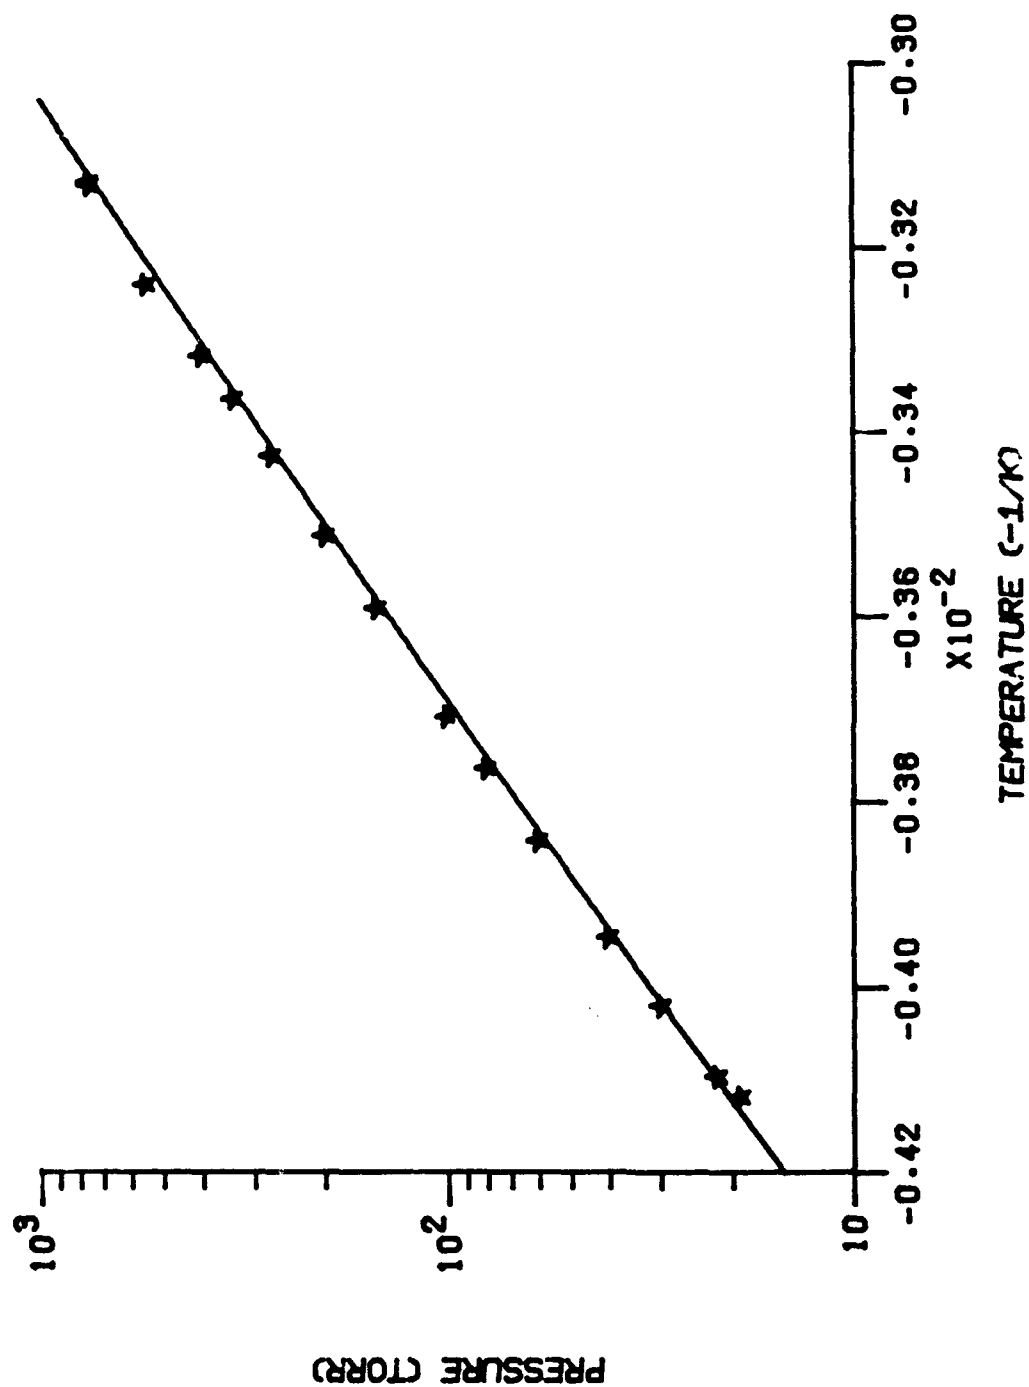


Figure 2. Vapor Pressure of Freon 113: Literature vs. Experimental

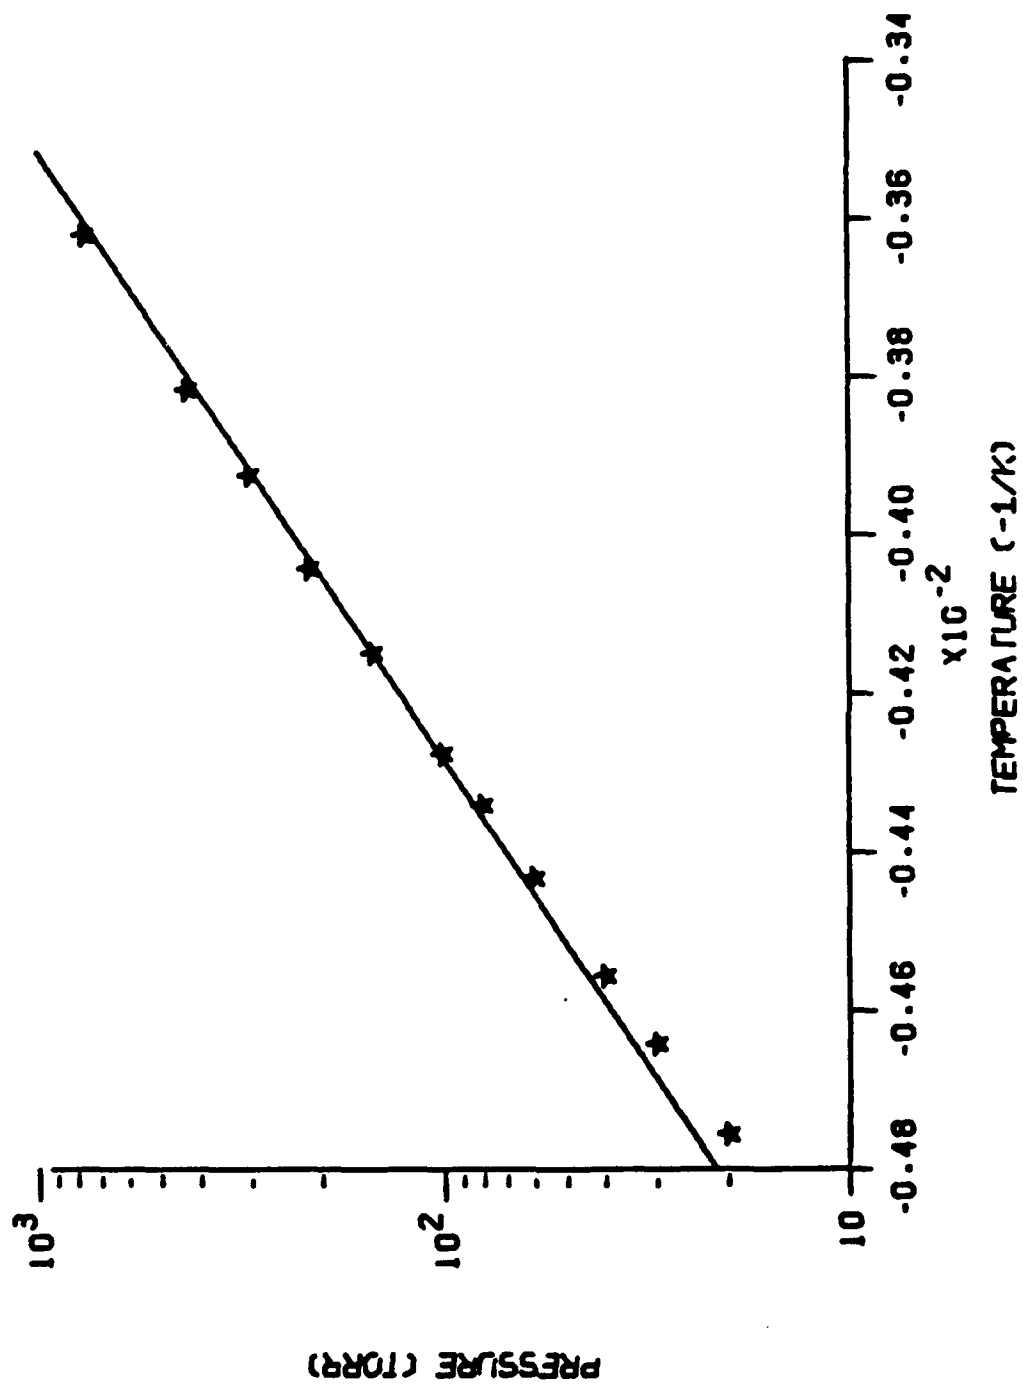


Figure 3. Vapor Pressure of Freon-114: Literature vs. Experimental

Table 1. Vapor Pressure Data for Freon-113

Temperature (°C)		Δt	Pressure (torr)
Experimental	Literature	(Lit - Exp)	
46.8	47.6	0.8	761.4
46.3	47.5	1.2	759.1
46.3	47.5	1.2	759.0
35.7	38.2	2.5	549.3
28.4	29.6	1.2	400.0
24.2	25.1	0.9	334.8
18.7	19.8	1.1	270.0
11.6	12.8	1.2	200.1
5.3	6.3	1.0	150.0
-3.4	-2.1	1.3	100.0
-7.4	-6.5	0.9	80.0
-12.8	-12.0	0.8	60.0
-19.7	-19.1	0.6	40.2
-24.3	-24.1	0.2	30.0
-29.0	-29.2	-0.2	21.9
-30.3	-31.3	-1.0	19.1

Table 2. Vapor Pressure Data for Freon-114

Temperature (°C)		Δt	Pressure (torr)
Experimental	Literature	(Lit - Exp)	
3.1	3.3	0.2	767.3
-11.2	-11.0	0.2	424.1
-18.4	-17.8	0.6	300.0
-25.8	-25.9	-0.1	213.2
-32.2	-32.2	0.0	149.2
-39.2	-39.7	-0.5	100.0
-42.8	-43.7	-0.9	80.0
-47.6	-48.6	-1.0	60.0
-53.6	-55.3	-1.7	40.0
-57.7	-59.7	-2.0	30.0
-62.8	-65.8	-3.0	19.9

4. CONCLUSIONS

A modified DTA technique for measuring vapor pressure has been shown to be a quick, easy method, requiring a very small sample. The use of a Quick Cool accessory extends the use of the method to subambient temperature region.

Sample: FREON 113
Size: 0.0500 mg
Method: INIT TEMP THEN RAMP

DTA

File: FREON.10
Operator: ABL
Run Date: 06/29/89 10:08

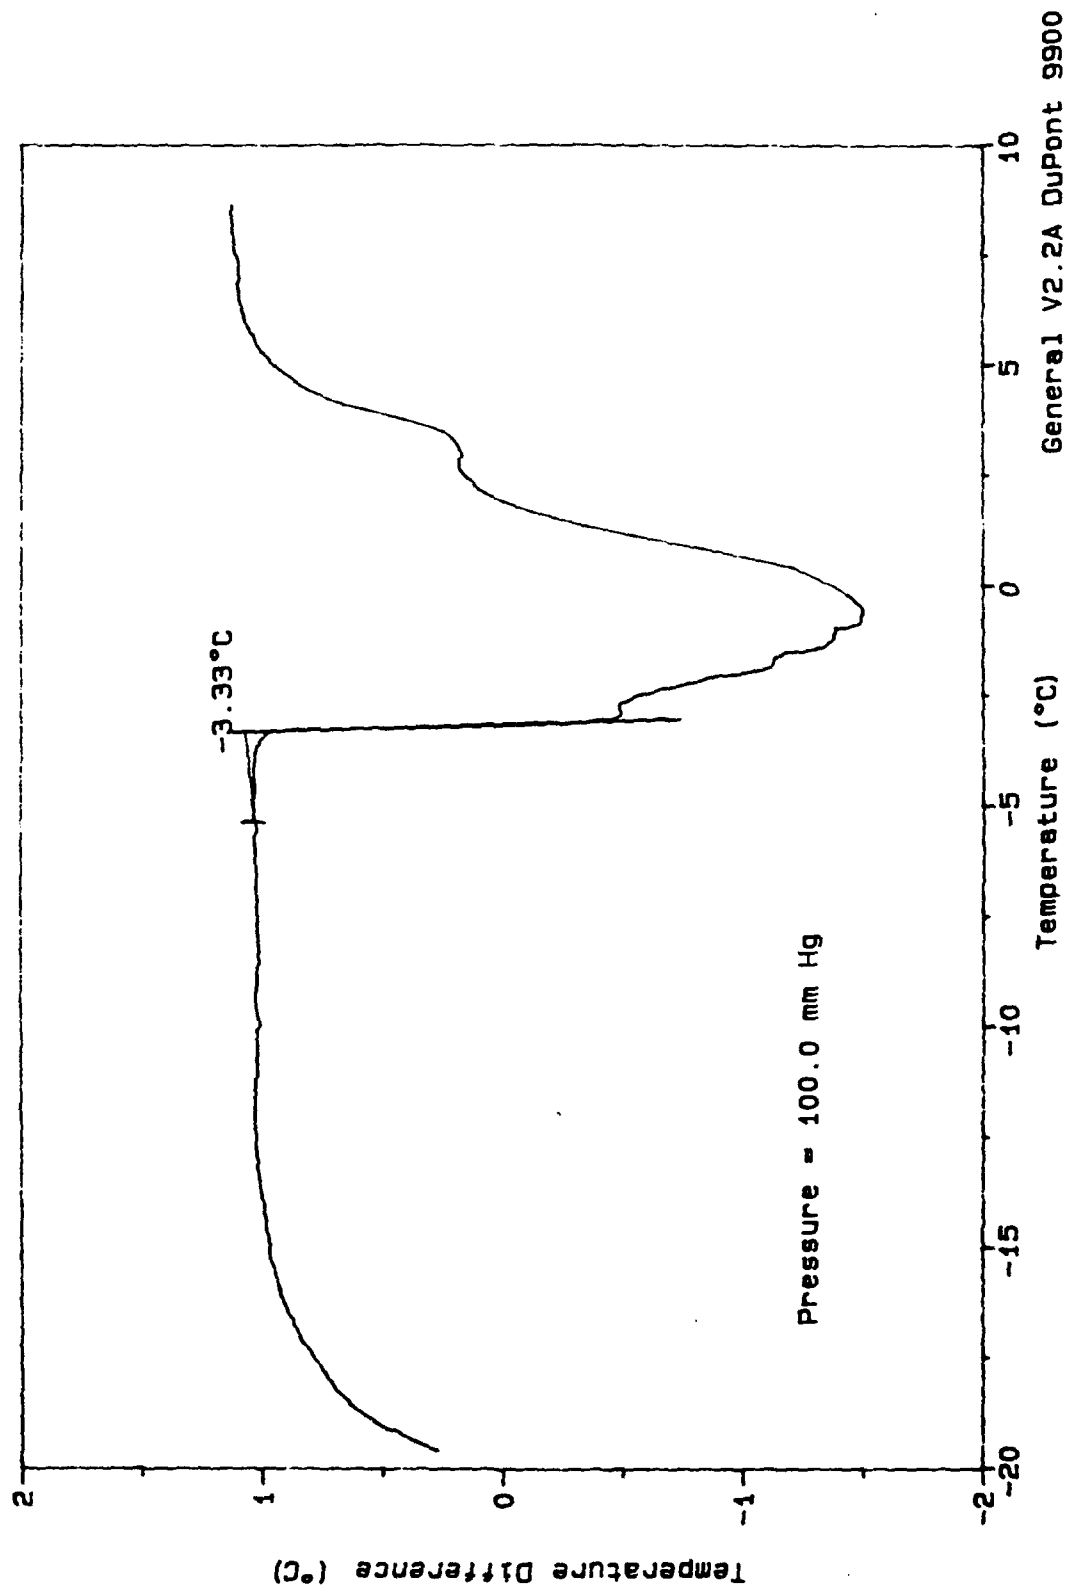


Figure 4. Boiling Thermogram for Freon-113

Sample: FREON 114
Size: 0.0500 mg
Method: INIT TEMP THEN RAMP

DTA

File: FREON14.04
Operator: ABL
Run Date: 06/30/89 11:15

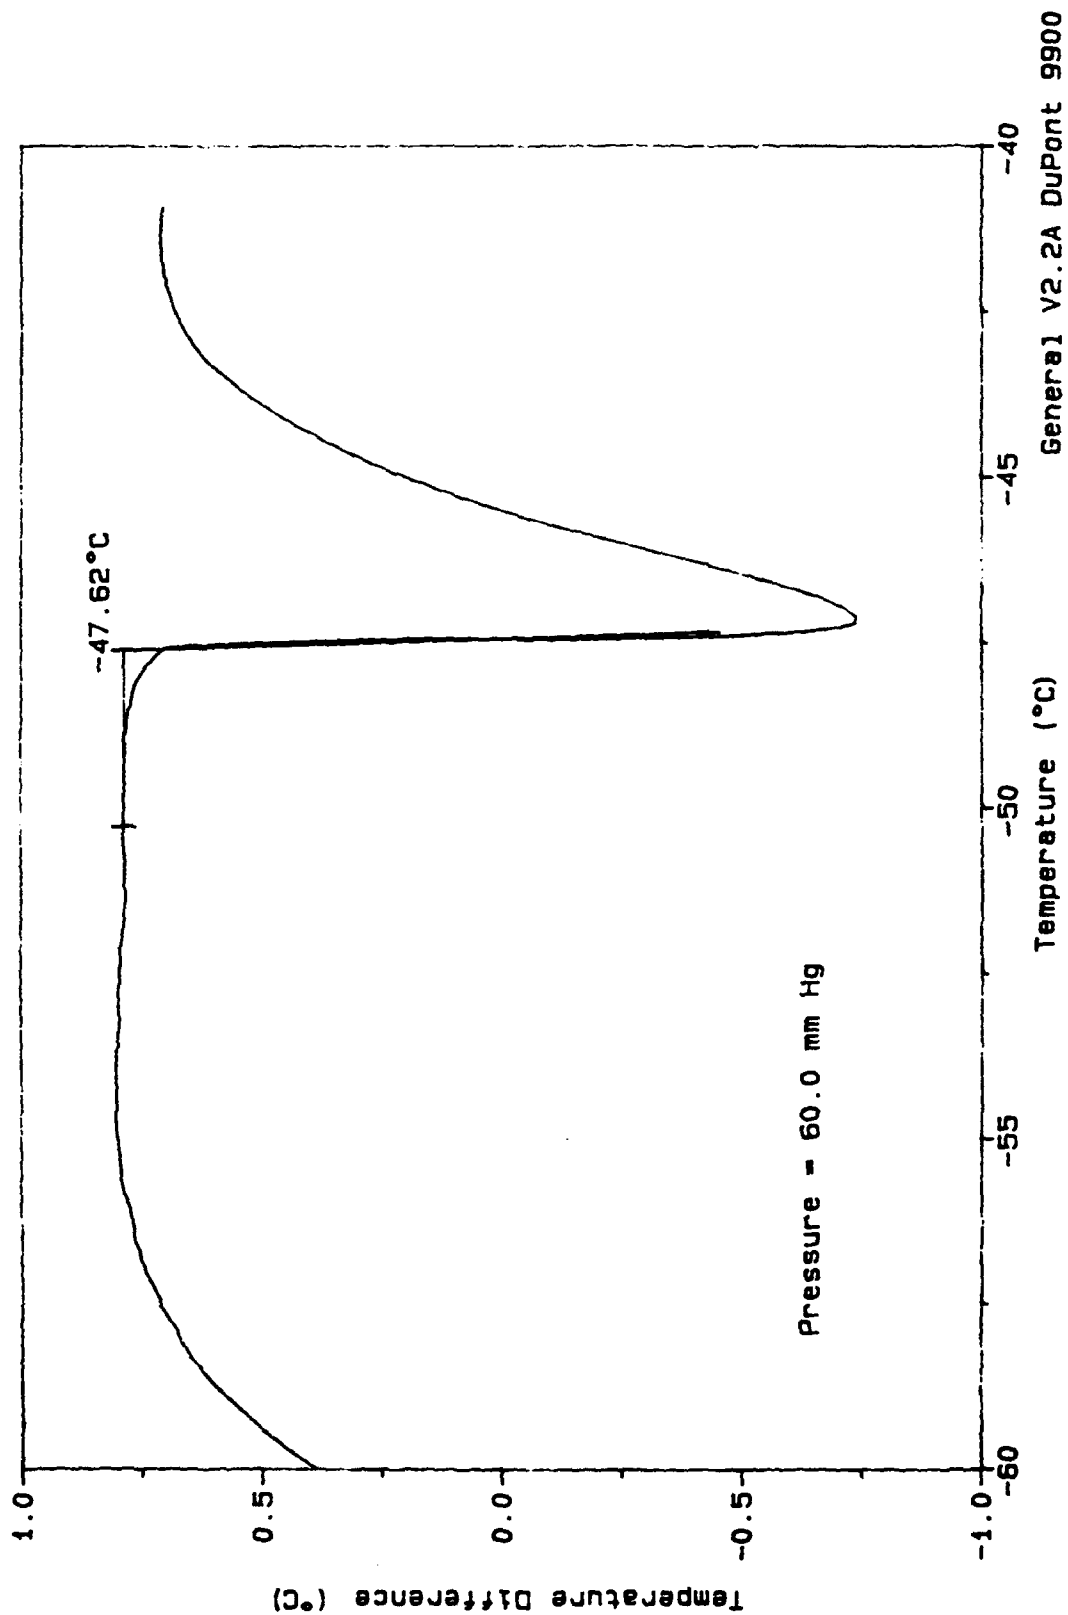


Figure 5. Boiling Thermogram for Freon-114

Blank

LITERATURE CITED

1. Vassallo, D.A., and Harden, J.C., "Precise Phase Transition Measurements of Organic Materials by Differential Thermal Analysis," Anal. Chem. Vol. 34, p 132 (1962).
2. Chiu, J., "Differential Thermal Analysis of Inorganic Compounds, Nitrates and Perchlorates of the Alkali and Alkaline Earth Groups and their Subgroups," Anal. Chem. Vol. 27, p 1102 (1955).
3. Kemme, H.R., and Kreps, S.I., "Vapor Pressure Determination by Differential Thermal Analysis," Anal. Chem. Vol. 41, p 1869 (1969).
4. Krawetz, A.A., and Torrog, T., "Determination of Vapor Pressure by Differential Thermal Analysis," Rev. Sci. Instrum. Vol. 33, p 1465 (1962).
5. Belkin, F., and Brown, H.A., Vapor Pressure Measurements of Some Chemical Agents Using Differential Thermal Analysis, Part III, EC-TR-75032, Edgewood Arsenal, Aberdeen Proving Ground, MD, June 1975, UNCLASSIFIED Report.
6. Hudlicky, M., "Chemistry of Organic Fluorine Compounds," In American Chemical Society Audio Course Manual, p 70, 1972.
7. Jordan, T.E., Vapor Pressure of Organic Compounds, p 70, Interscience Publishers, New York, NY, 1954.