


TNO Defence Research
AD-A266 291



TNO-report

FEL-93-A034

title

Description of an Infrared Zoomcollimator

author(s):

A.N. de Jong

date:

March 1993

TDCK RAPPORTCENTRALE

Frederikkazerne, gebouw 140
v/d Burchlaan 31 MPC 16A
TEL. : 070-3166394/6395
FAX. : (31) 070-3166202
Postbus 90701
2509 LS Den Haag

This document has been approved
for public release and sale; its
distribution is unlimited.

All rights reserved.

No part of this publication may be
reproduced and/or published by print,
photoprint, microfilm or any other means
without the previous written consent of
TNO.

In case this report was drafted on
instructions, the rights and obligations of
contracting parties are subject to either the
Standard Conditions for Research
Instructions given to TNO, or the relevant
agreement concluded between the
contracting parties.

Submitting the report for inspection to
parties who have a direct interest is
permitted.

TNO

Netherlands organization for
applied scientific research

TNO Defence Research consists of
the TNO Physics and Electronics Laboratory,
the TNO Prins Maurits Laboratory and the
TNO Institute for Perception

TNO Physics and Electronics
Laboratory

Dude Waasdorpweg 63
2597 AK The Hague
P.O. Box 90864
2509 JG The Hague
The Netherlands

Fax +31 70 328 09 61
Phone +31 70 326 42 21

classification

classified by : G. Zwiep

classification date : February 25, 1993

title

: ongerubriceerd

abstract

: ongerubriceerd

report text

: ongerubriceerd

no. of copies

: 37

no. of pages

: 13 (excluding RDP and distribution list)

no. of appendices

: -

All information which is classified according to
Dutch regulations shall be treated by the recipient in
the same way as classified information of
corresponding value in his own country. No part of
this information will be disclosed to any party.

The classification designation ONGERUBRICEERD
is equivalent to UNCLASSIFIED.




The Standard Conditions for Research Instructions
given to TNO, as filed at the Registry of the District Court
and the Chamber of Commerce in The Hague
shall apply to all instructions given to TNO

93-14793



TO
53-0295
8870-05 01

DISCLAIMER NOTICE

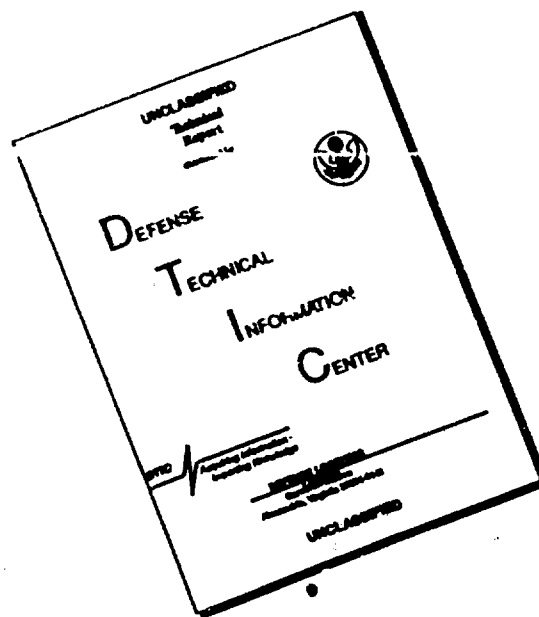

**THIS DOCUMENT IS BEST
QUALITY AVAILABLE. THE COPY
FURNISHED TO DTIC CONTAINED
A SIGNIFICANT NUMBER OF
PAGES WHICH DO NOT
REPRODUCE LEGIBLY.**

report no. : FEL-93-A034
title : Description of an Infrared Zoomcollimator

author(s) : A.N. de Jong
Institute : TNO Physics and Electronics Laboratory

date : March 1993
NDRO no. : A90KL654
no. in pow '93 : 716.1

Research supervised by : A.N. de Jong
Research carried out by : A.N. de Jong

ABSTRACT (ONGERUBRICEERD)

The performance of thermal imagers is generally tested by means of test targets, put in the focal plane of a collimator. For MRTD measurements bar targets are used with a certain frequency and variable temperature contrast. The zoomcollimator, described in this report provides a variable spatial frequency, which is more comparable to the range variation of a target in the terrain with certain size and temperature contrast. In the focal plane also a line source and a circular source with variable temperature contrast can be used, in order to measure the MRTD in an objective way conform the method, developed at TNO-FEL.

Accession For	
NTIS	TEASIS
DTIC	✓
INT	—
JGND	—
By	
Date	
Available in	
Dist	
A-1	

DTIC QUALITY INSPECTED 2

rapport no. : FEL-93-A034
titel : Beschrijving van een Infrarood Zoomcollimator

auteur(s) : ir. A.N. de Jong
instituut : Fysisch en Elektronisch Laboratorium TNO

datum : maart 1993
hdo-opdr.no. : A90KL654
no. in iwp '93 : 716.1

Onderzoek uitgevoerd o.l.v. : ir. A.N. de Jong
Onderzoek uitgevoerd door : ir. A.N. de Jong

SAMENVATTING (ONGERUBRICEERD)

De prestatie van warmtebeeldcamera's wordt over het algemeen gemeten met behulp van test-objecten welke in het brandvlak van een collimator worden geplaatst. Voor MRTD metingen worden balkenpatronen gebruikt met een bepaalde frequentie en variabel temperatuurcontrast. De zoomcollimator, beschreven in dit rapport voorziet in een variabele spatiële frequentie, welke meer vergelijkbaar is met de afstandvariatie tot een doel in het terrein met een zekere afmeting en temperatuurcontrast. Bij gebruik van een lijnbron en een circulaire bron met variabel temperatuurcontrast kan de MRTD op objectieve wijze worden gemeten conform een op FEL-TNO ontwikkelde methode.

CONTENTS

ABSTRACT	2
SAMENVATTING	3
1 INTRODUCTION	5
2 DESCRIPTION OF THE EQUIPMENT	7
3 EXAMPLES	11
4 CONCLUSIONS	12
5 REFERENCES	13

1 INTRODUCTION

The performance of a thermal imaging sensor is generally measured by using a collimator system with different kinds of targets in its focal plane. Because of the fact, that thermal imagers are dealing with 2 types of resolution: geometrical- and thermal resolution, two kinds of targets are used, one with variable spatial frequency information and one with temperature gradients.

The Minimum Resolvable Temperature Difference (MRTD) is a performance parameter, widely in use because of its capability to predict ranges, which is a combination of spatial and thermal resolution. It is a subjective parameter including the observer, who has to judge if a certain 4-bar pattern target can be distinguished at a certain temperature difference between bars and background (see e.g. ref [1] and [2]).

A complete MRTD measurement at a number of spatial frequencies and a number of observers is very time consuming. For this reason, a new method was developed, which excludes the observer from the direct measurement and replaces him by a model.

Furtheron the spatial resolution is measured by means of the system Line Spread Function (LSF), delivering the Modulation Transfer Function (MTF) and the Noise Equivalent Temperature Difference (NETD) (see ref [3]).

For this purpose a line source is used for the LSF and a circular source of certain size for geometry- and NETD measurement. The display is partly (about 1/5) projected onto a CCD camera of which the images are processed in a PC. Care is taken that all signals stay within the linear part of the dynamic range.

In order to further simplify the system, it was decided to build a portable collimator which can be used in the field. The collimating component was changed from reflective (30 cm aperture) to refractive (15 cm aperture) with the advantage that the imager pupil can be positioned closely to the collimator pupil.

Another idea was integrated into the new collimator concerning a zoom capability. This meant that the two targets (line and circle) can be kept for a variety of imagers with different fields of view. Furthermore, if the circle target is replaced by a 4-bar target, zooming in and out means variation of range, keeping the temperature difference constant.

In fig. 1 the classical method of subjective MRTD measurement is indicated at position A; at frequency f_0 , ΔT_0 is varied until the observer decides upon the limit of recognition.

At position B the temperature difference ΔT_1 is kept constant and the observer varies the spatial frequency, while the same target is kept, which is a great advantage. Target changing easily causes temperature instabilities and it cost more time.

The development of the zoomcollimator was carried out at TNO-FEL as a project with "basic funding". The work was carried out in 1992. The mechanical construction was realized by Jan ten Donkelaar and the electronics by Wim van Bommel and Marco Roos. The latter also provided the software for system control.

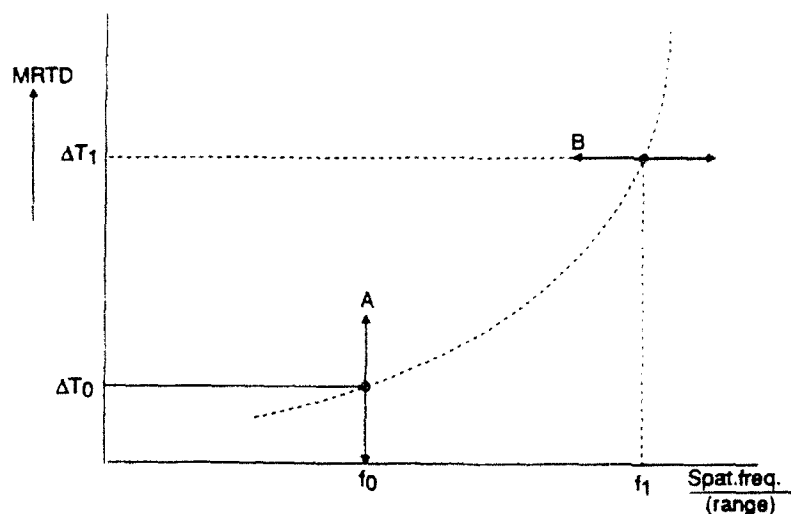


Fig. 1: Description of MRTD measurement

The negative lens L_2 provides compensation of spherical aberration for all focal lengths below $0,02 \cdot 10^{-5}$ mrad which is far below the diffraction limit (0,08 mrad for 10 μm).

The pupil is imaged at appropriate locations from F. The field of view of the collimator is for an unobscured pupil through all lenses for a full pupil diameter of 150 mm respectively $2,34^\circ$; $1,77^\circ$ and $0,52^\circ$ for the situations A, B and C. The limiting lenses are respectively the 2nd, the 3rd and the 4th lens. If the pupil goes down to 100 mm, the fields of view increase respectively $2,81^\circ$; $2,19^\circ$ and $1,25^\circ$. If some vignetting is allowed the fields of view will be greater.

The data for lenses L_2 and $L_3 (= L_4)$ are:

- L_2 :
- material: germanium; $n = 4,004$ ($= 9,2 \mu\text{m}$)
 - curvatures $R_1 = -223,08 \text{ mm}$ $R_2 = -869,00 \text{ mm}$
 - axial thickness 6,00 mm
 - focal length -100,61 mm
 - diameter 60 mm
- L_3, L_4 :
- material: germanium; $n = 4,004$
 - curvatures $R_1 = 325,76 \text{ mm}$ $R_2 = 478,71 \text{ mm}$
 - axial thickness 10,00 mm
 - focal length 323,54 mm (back focal length 316,08 mm)
 - diameter 110 mm

The paraxial positions for lens L_2 for situations A, B and C are:

- A: $S_3 = 150 \text{ mm}$ $S_3' = -588,88 \text{ mm}$ $S_4 = -594,88 \text{ mm}$ $S_4' = -305,44 \text{ mm}$ Magn = 2,020
distance P'-P = 449,44 mm
- B: $S_3 = 200 \text{ mm}$ $S_3' = -472,95 \text{ mm}$ $S_4 = -478,95 \text{ mm}$ $S_4' = 203,95 \text{ mm}$ Magn = 1,007
distance P''-P = 397,95 mm
- C: $S_3 = 300 \text{ mm}$ $S_3' = -395,16 \text{ mm}$ $S_4 = -401,16 \text{ mm}$ $S_4' = -153,28 \text{ mm}$ Magn = 0,503
distance P'-P = 447,28 mm

Lens L_3 is always at 316,08 mm from P'(P'').

All lenses are made of germanium, which implies chromatic aberrations of about 0,05 mm diameter. This is sufficiently below the diffraction limit if we limit the collimator between 8 and 12 μm .

Fig. 3 and fig. 4 give pictures of the complete collimator and of a close up of the zoom compartment. The lenses L_2 and L_3 are driven by means of servo motors with driving belts, mounted on the bottom side. Potentiometers provide position information. Electronic circuitry is mounted in the inside compartment, as shown in fig. 4.

The targets are mounted at the backside as plug in units. One unit is provided with a line source, tilted under about 10° from the vertical or horizontal. This wire is heated and has a diameter of 0,03 mm. The second unit is provided with a rectangular, circular or 4-bar source.

The system has 2 connectors, one to the zoomcompartment and one to the targets. The target compartment is provided with a peltier heated or cooled background. The heat is removed at the back side by free convection. The complete system can be mounted on a tripod by means of a standard mounting plate.

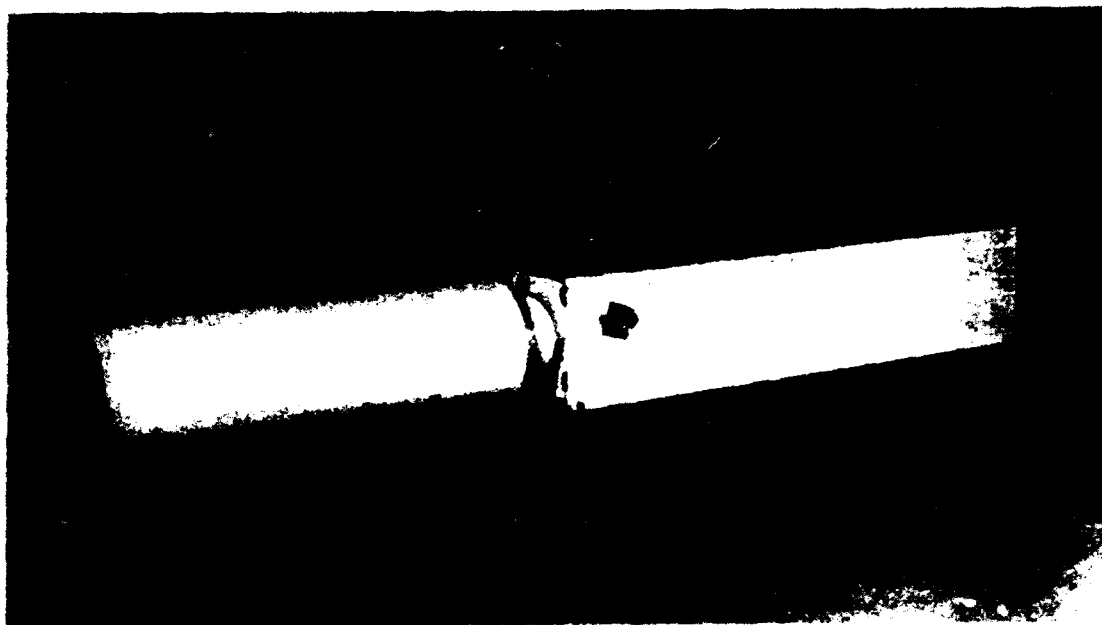


Fig. 3: Complete view of zoomcollimator

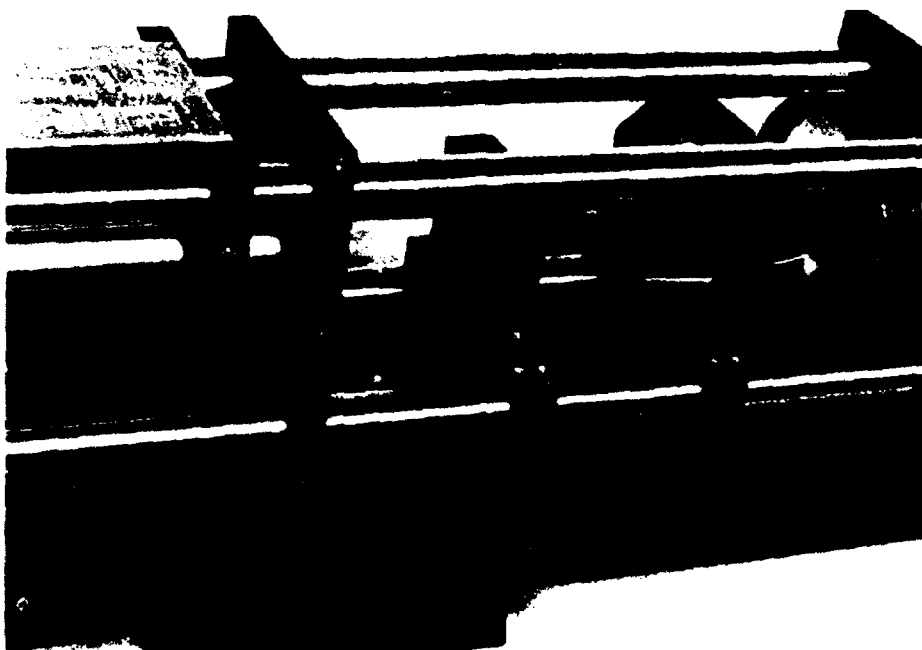


Fig. 4: Inside view of zoomcollimator with lenses L_2 , L_3 and L_4

3 EXAMPLES

Some examples of images, taken with an IR 18 infrared imager from Barr and Stroud, are shown in fig. 5 and fig. 6.

Fig. 5 shows the circular source for the 3 situations A, B and C. Fig. 6 shows the line source for the same situations. The total transmission of the 4 germanium lenses was measured to be 0.65. All lenses are provided with a single layer anti-reflection coating for a wavelength of $10\text{ }\mu\text{m}$. The heating and cooling of the background plate is going at sufficient speed to perform a subjective MRTD measurement. The read out of the temperature differences with Pt resistors was calibrated with a second calibrated source from Electro Optical Industries and a radiometer with sufficient resolution.

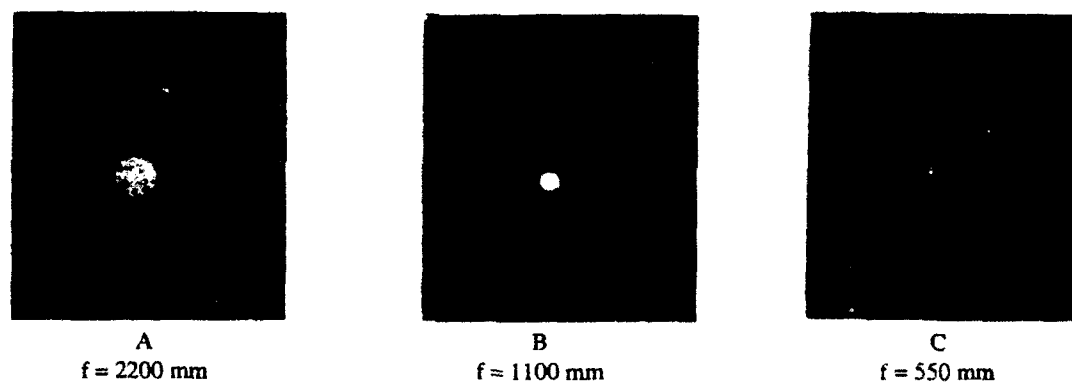


Fig. 5: Images of a circular source; $\Delta T = 6^\circ\text{C}$; Directly taken with IR 18 thermal imager

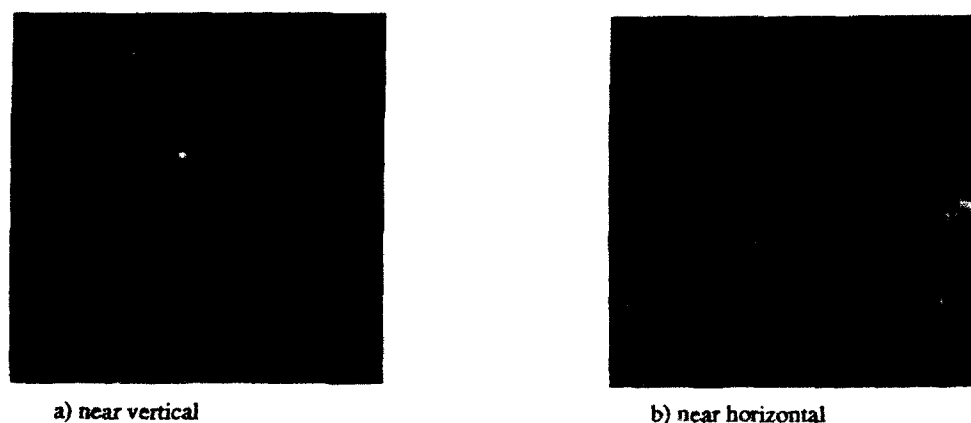


Fig. 6: Images of a tilted line source via CCD camera with 5 x magnification; Picture taken with IR 18 thermal imager

4 CONCLUSIONS

The development of an Infrared Zoomcollimator has been very successful. The instrument creates new possibilities to carry out faster, more repeatable and more accurate performance measurements of IR sensors, in the field, in the factory and in the laboratory. The most relevant system parameters like Signal Transfer Function, Modulation Transfer Function, Noise Equivalent Temperature Difference as well as Minimum Resolvable Temperature Difference and Noise Equivalent Irradiance can be measured, especially when data acquisition is done by means of a PC with frame grabber. By means of the zoom-capability of the collimator, the possibility has been created to measure directly the range at which a 4-bar target with given temperature difference can be recognized. The Physics and Electronics Laboratory, TNO-FEL is ready to provide quotations on the device.

5 REFERENCES

- [1] J.M. Lloyd, Thermal Imaging Systems
Plenum Press, New York (1975).
- [2] J.A. Ratches e.a. NVL Static Performance Model for Thermal Imaging Systems; US Army
ECDM 7043 (1975).
- [3] A.N. de Jong e.a. Fast and Objective MRTD measurement.
Report FEL-1988-24.

J. Bennema
(Divisional Head)

A.N. de Jong
(Author)

REPORT DOCUMENTATION PAGE

(MOD-NL)

1. DEFENSE REPORT NUMBER (MOD-NL)	2. RECIPIENT'S ACCESSION NUMBER	3. PERFORMING ORGANIZATION REPORT NUMBER
TD93-0295		FEL-93-A034

4. PROJECT/TASK/WORK UNIT NO.	5. CONTRACT NUMBER	6. REPORT DATE
22174	A90KL654	MARCH 1993

7. NUMBER OF PAGES	8. NUMBER OF REFERENCES	9. TYPE OF REPORT AND DATES COVERED
13 (EXCL. RDP & DISTRIBUTION LIST)	3	FINAL REPORT

10. TITLE AND SUBTITLE
DESCRIPTION OF AN INFRARED ZOOMCOLLIMATOR

11. AUTHOR(S)
A.N. DE JONG

12. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES)
TNO PHYSICS AND ELECTRONICS LABORATORY, P.O. BOX 96864, 2509 JG THE HAGUE
OUDERWAALSDORPERWEG 63, THE HAGUE, THE NETHERLANDS

13. SPONSORING/MONITORING AGENCY NAME(S)
DMKL

14. SUPPLEMENTARY NOTES
THE CLASSIFICATION DESIGNATION ONGERUBRICEERD IS EQUIVALENT TO UNCLASSIFIED.

15. ABSTRACT (MAXIMUM 200 WORDS, 1044 POSITIONS)

THE PERFORMANCE OF THERMAL IMAGERS IS GENERALLY TESTED BY MEANS OF TEST TARGETS, PUT IN THE FOCAL PLANE OF A COLLIMATOR. FOR MRTD MEASUREMENTS BAR TARGETS ARE USED WITH A CERTAIN FREQUENCY AND VARIABLE TEMPERATURE CONTRAST. THE ZOOMCOLLIMATOR, DESCRIBED IN THIS REPORT PROVIDES A VARIABLE SPATIAL FREQUENCY, WHICH IS MORE COMPARABLE TO THE RANGE VARIATION OF A TARGET IN THE TERRAIN WITH CERTAIN SIZE AND TEMPERATURE CONTRAST. IN THE FOCAL PLANE ALSO A LINE SOURCE AND A CIRCULAR SOURCE WITH VARIABLE TEMPERATURE CONTRAST CAN BE USED, IN ORDER TO MEASURE THE MRTD IN AN OBJECTIVE WAY CONFORM THE METHOD, DEVELOPED AT TNO-FEL.

16. DESCRIPTORS

PERFORMANCE

IDENTIFIERS

THERMAL IMAGERS
TEST EQUIPMENT
INFRARED COLLIMATOR

17a. SECURITY CLASSIFICATION
(OF REPORT)
ONGERUBRICEERD

17b. SECURITY CLASSIFICATION
(OF PAGE)
ONGERUBRICEERD

17c. SECURITY CLASSIFICATION
(OF ABSTRACT)
ONGERUBRICEERD

18. DISTRIBUTION/AVAILABILITY STATEMENT

UNLIMITED DISTRIBUTION

17d. SECURITY CLASSIFICATION
(OF TITLES)
ONGERUBRICEERD