

AL/DO-TP-1993-0025

AD-A268 400



**AUTOMATED DATA COLLECTION SYSTEM FOR THE TCM3
TRANSCUTANEOUS pO₂/pCO₂ MONITORING SYSTEM**

Roxanne Constable

DTIC
ELECTE
AUG 24 1993
S B D

OPERATIONS AND SUPPORT DIRECTORATE
TECHNICAL OPERATIONS DIVISION
2404 E Drive, Suite 1
Brooks Air Force Base, TX 78235-5112

August 1993

Final Technical Paper for Period January 1993 - June 1993

Approved for public release; distribution is unlimited.

240-3853

93 8 23 089

93-19596



AIR FORCE MATERIEL COMMAND
BROOKS AIR FORCE BASE, TEXAS

ARMSTRONG

LABORATORY

NOTICES

When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely Government-related procurement, the United States Government incurs no responsibility or any obligation whatsoever. The fact that the Government may have formulated or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication, or otherwise in any manner construed, as licensing the holder, or any other person or corporation; or as conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

The Office of Public Affairs has reviewed this paper, and it is releasable to the National Technical Information Service, where it will be available to the general public, including foreign nationals.

This paper has been reviewed and is approved for publication.


ROXANNE CONSTABLE
Project Engineer


JAMES R. DICKEY
Chief, Technical Operations Division

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE August 1993	3. REPORT TYPE AND DATES COVERED Final January 1993 - June 1993	
4. TITLE AND SUBTITLE Automated Data Collection System for the TCM3 Transcutaneous pO ₂ /pCO ₂ Monitoring System			5. FUNDING NUMBERS	
6. AUTHOR(S) Roxanne Constable				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Armstrong Laboratory (AFMC) Operations and Support Directorate Technical Operations Division 2404 E Drive, Suite 1 Brooks Air Force Base, TX 78235-5112			8. PERFORMING ORGANIZATION REPORT NUMBER AL/DO-TP-1993-0025	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)			10. SPONSORING/MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution is unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) The Hyperbaric Medicine Division of the Armstrong Laboratory (AL/AOHP) routinely uses the TCM3 Transcutaneous system for monitoring of patients and during research protocols. The monitor is used to measure the amount of oxygen/carbon dioxide at the skin surface. Up to 3 monitors may be utilized, and all data must be written down by hand at some interval. This method requires an individual to be watching the monitors at all times. If any further data analysis is to be performed, then the data must be entered into a computer by hand, or the manipulations are performed on paper. The purpose of this technical paper is to describe a data acquisition system designed to automate the collection and analysis of information processed by the TCM3 transcutaneous monitor. The hardware portion of the system is designed around a Macintosh II computer, and the software was written using LabVIEW 2.				
14. SUBJECT TERMS Data acquisition LabVIEW Medical Monitors			15. NUMBER OF PAGES 22	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT UL	

AUTOMATED DATA COLLECTION SYSTEM FOR THE TCM3 TRANSCUTANEOUS PO₂/PCO₂ MONITORING SYSTEM

INTRODUCTION

The Hyperbaric Medicine Division of the Armstrong Laboratory (AL/AOHP) routinely uses the TCM3 Transcutaneous system for monitoring of patients and during research protocols. The device is used to measure the amount of oxygen/carbon dioxide at the skin surface. Up to 3 monitors are utilized, and all data must be written down by hand at some interval. This method requires an individual to be watching the monitors at all times. This paper describes a simple system to automate the collection and analysis of this information. The system described here could easily be adapted to be used at any facility using this type of monitoring system.

METHODS

Hardware

There was an urgent need for the data acquisition system; therefore, the major goal was to design around equipment available in-house.

The TCM3 monitor provides output in analog and digital (RS-232) formats. To use the digital output, a separate serial port is required for each monitor connected to the data acquisition system. Most computers do not have 3 serial ports readily available, as they are also used to communicate with the mouse, printers, scanners, etc. Therefore, utilization of the analog output of the monitors was determined to be the best solution. An analog data acquisition board and a Macintosh computer of sufficient capability was available for use, resulting in the decision to proceed on this platform.

The hardware setup consisted of a Macintosh II computer with 10 Mb of memory, and a National Instruments NB-MIO-16H multi-purpose data acquisition board. This board has sufficient on-board gain for the analog signal sent by the TCM3; therefore, we did not need to amplify the signal before converting. Used in the single-ended mode, the board supplies 16 analog input channels. Only 3 channels were required to implement this system. Figure 1 is a block diagram describing the computer interface hardware connections. All interface cables were built in-house.

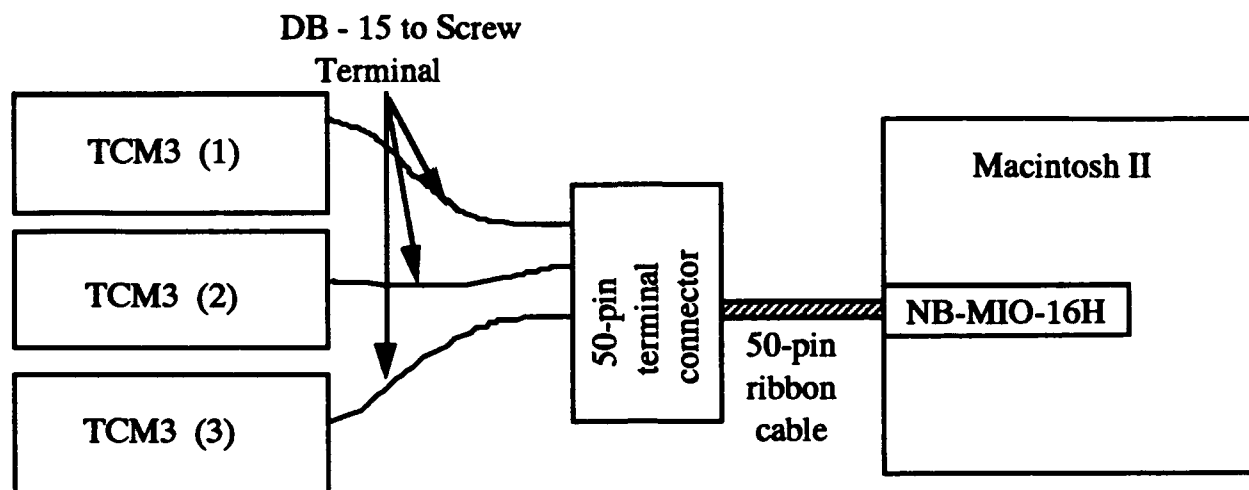



Figure 1. Cabling diagram for the TCM3 automated data collection system.

The cabling diagram included in the *Transcutaneous pO_2/pCO_2 Monitoring System User's Handbook* (1) was used. After extensive testing, we found that the data provided was not sufficient to build the cable correctly. Figure 2 shows the instructions provided and the additional information required to properly construct the cable. The cable must be plugged in before the device is turned on. If the cable is not plugged in when switched on, the device automatically defaults to digital output mode, and there is no way to change it back to the analog output mode without switching the power off, then back on.

Accession For		☒ ☐ ☐
NTIS GRA&I		
DTIC TAB		
Unannounced		
Justification		
By		
Distribution/		
Availability Codes		
Dist	Avail and/or Special	
A-1		

Analog recorder output:

Alarm, heat/temperature, tcpO₂, and tcpCO₂



Pin signals:

- 5 Alarm
- 8 Heat/Temperature
- 9 Tension (pO₂)
- 10 Tension (pCO₂)
- 15 Ground

***** NOT INCLUDED IN MANUAL *****

Pin 13 must be tied to pin 15

Figure 2. Cable pin-outs and other necessary cabling information.

Software

The software was written using LabVIEW 2 (2), an interactive programming environment developed by National Instruments. It is available for MS-DOS or Macintosh computer systems. This programming environment provides the drivers for the data acquisition boards, as well as tools to make the user interface easy to operate and interpret. The basic unit of LabVIEW is the Virtual Instrument (VI). A VI is a complete program which behaves as an instrument. Each instrument has its own front panel which consists of switches, knobs, and indicators. This panel serves as the interface between the user and the program, and can be made to nearly duplicate the operating panel of the actual instrument. Behind each front panel is a block diagram, which serves the same function of textual code in conventional languages. The block diagram is where other VI's and basic functions have been "wired" together to build the program. Each subVI (a VI used as a subroutine) has its own front panel of inputs and indicators which are controlled or read by the block diagram.

One of LabVIEW's major advantages is the ease with which VI's can be reused and/or adapted for use in many varied applications. LabVIEW forces the developer to use modular programming techniques

and provides an easy method for program documentation. The intuitiveness of LabVIEW VI's and their self-documentation features allow any user to adapt the VI for their application.

There were two separate programs written for this project. The first program (TCPO2MMON) reads in the data at user defined intervals, then plots the data on the screen and stores the data to disk at a user defined interval. The second program (Read and Graph) is used to review the data after the study has been completed, or the patient has completed his/her treatment. The program reads back the stored data and plots it on the computer screen. Although not currently implemented, LabVIEW supplies a wide range of data analysis routines which could be used to further analyze the data.

TCPO2MMON

The front panel for this program is shown in Figure 3. The system uses a color monitor which allows the indicators and trend lines to be color-coded. This feature is not evident in this figure. The diagram is included in the Appendix. Before starting the program, the user inputs how often data is to be collected, how often data is to be saved to the hard disk, and whether the devices are operating on full or half scale. The user then starts the program.

After start-up, the user is prompted to enter a filename under which to store the data. Following this prompt, another panel is displayed in which the user can enter subject data and other pertinent experimental data. This material is appended to the data file for later retrieval. Data collection begins after this information has been entered.

At the sampling interval, 10 samples are collected and averaged for each channel and returned as the data point. This feature helps to reduce noise which may be introduced, especially as the input signal voltage levels are low and thereby easily contaminated. The software is written to collect all of the data available from the TCM3 monitors. However, currently only the chest, leg, and foot oxygen data is being stored and displayed. The digital display is updated at the rate data is collected, and then the data is used to update the chart. This chart provides the researcher a graphical, real-time display of the data. The data is stored to the hard disk in ASCII text format. This feature allows the file to be opened by any spreadsheet, statistical, or word processing package.

At the end of the experiment, the user uses the mouse to "click" on the test complete switch. This feature suspends the data acquisition, and closes the data file. At this time, the user can begin the process over again using a different file name.

Front Panel

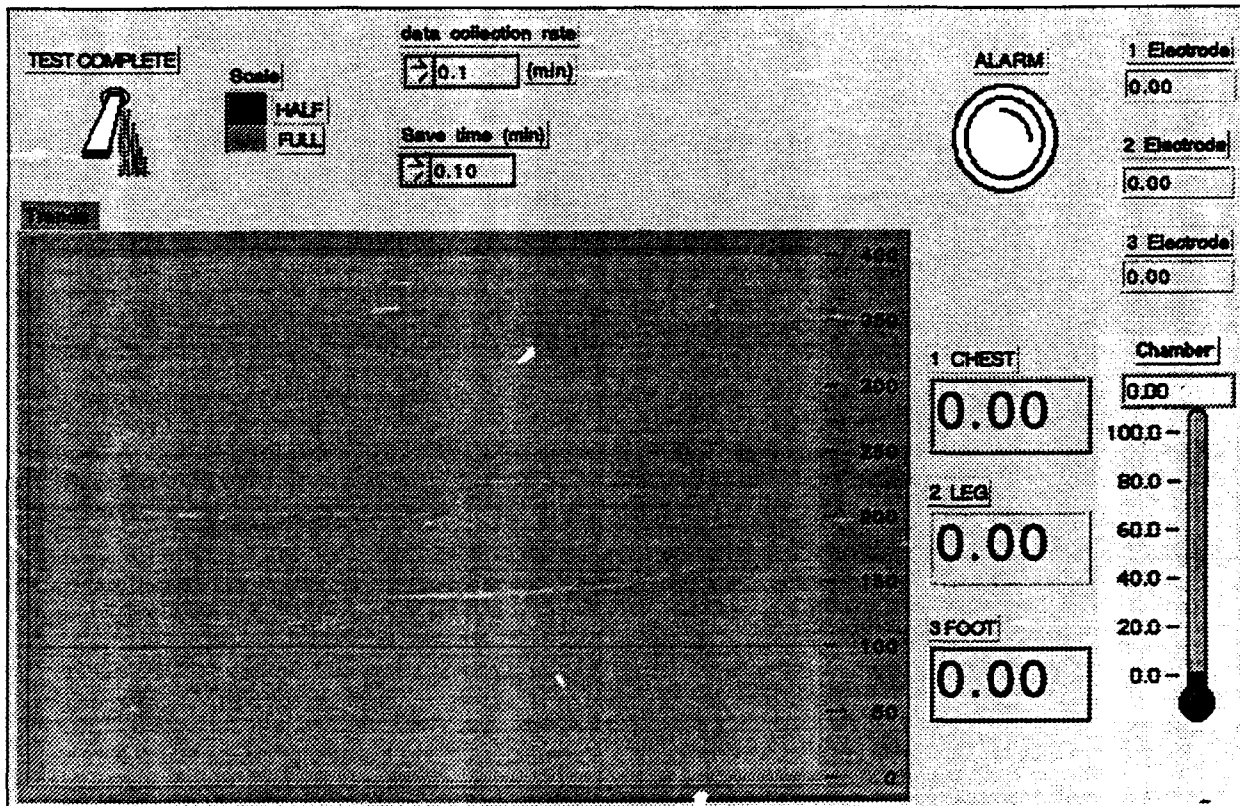


Figure 3. TCPO2MMON Front Panel.

Read & Graph

The front panel for this program is shown in Figure 4. The system uses a color monitor which allows the indicators and trend lines to be color-coded. This feature is not evident in this figure. The diagram is included in the Appendix.

After the program begins, the user is prompted for the name of the data file to read. Once this is entered, the data file is read in and displayed both numerically and graphically. The graph is expressed in terms of data v. time, allowing the user to analyze trends, slopes, etc.

Front Panel

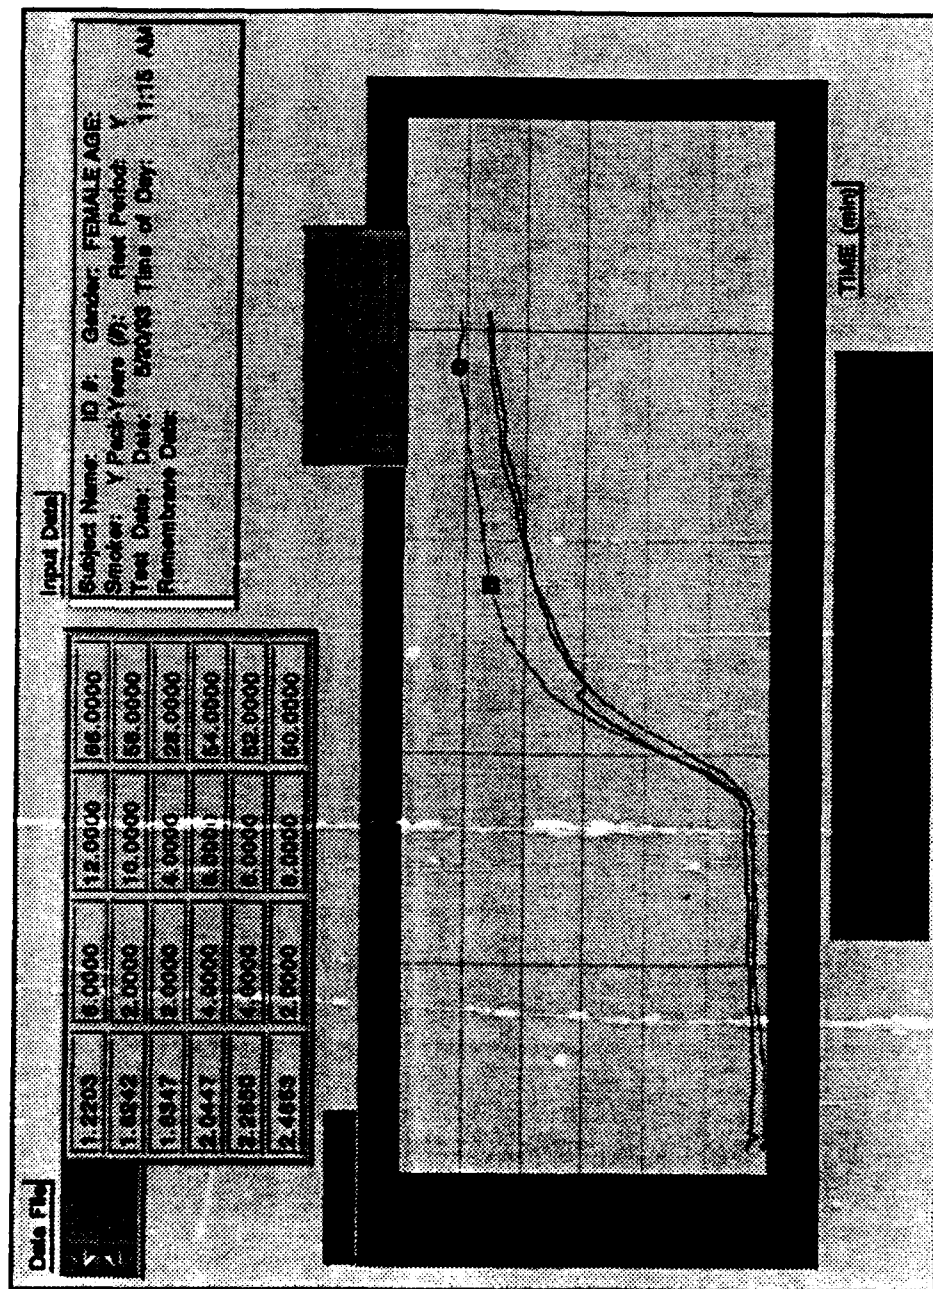


Figure 4. READ & GRAPH Front Panel.

RESULTS AND CONCLUSIONS

Using readily available tools, a powerful and user-friendly data acquisition system was developed for use by the Hyperbaric Medicine Division. The system reduces the need for additional personnel to be present during a study, and reduces the need for data to be recorded manually and then manually entered into a computer for analysis. The data is available in a convenient spreadsheet format which can then be printed out and kept with the patient's file for later reference.

With the availability of personal computers today, and software tools such as LabVIEW, data acquisition is no longer the difficult task that it was several years ago. Although not all problems can be solved as easily as this one, the payoff to the investigator can be significant time savings later in terms of recording, retrieving, and analyzing the data, even if the initial investment in time and equipment appears to be great.

REFERENCES

1. *Transcutaneous pO_2/pCO_2 Monitoring System User's Handbook*, Radiometer/Copenhagen, Edition D, January 1990.
2. *LabVIEW 2 User Manual*, National Instruments, Austin TX, July 1992.


APPENDIX

Block Diagrams for TCP02MMON and Read & Graph


TCPO2MMON
Thursday, May 27, 1993 2:19 PM

Front Panel

Page 1 ☐

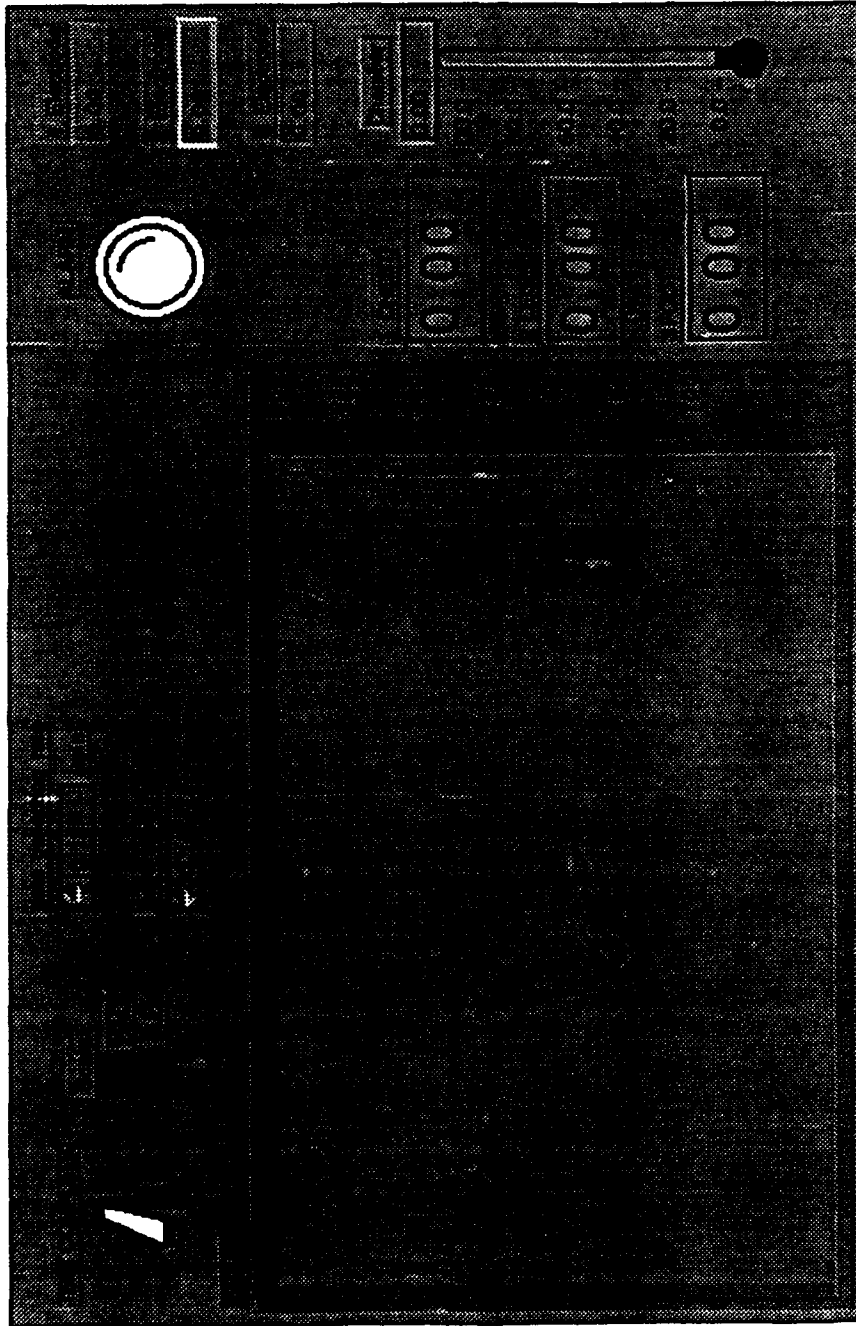

COPY AVAILABLE TO DTIC DOES NOT PERMIT FULLY LEGIBLE REPRODUCTION

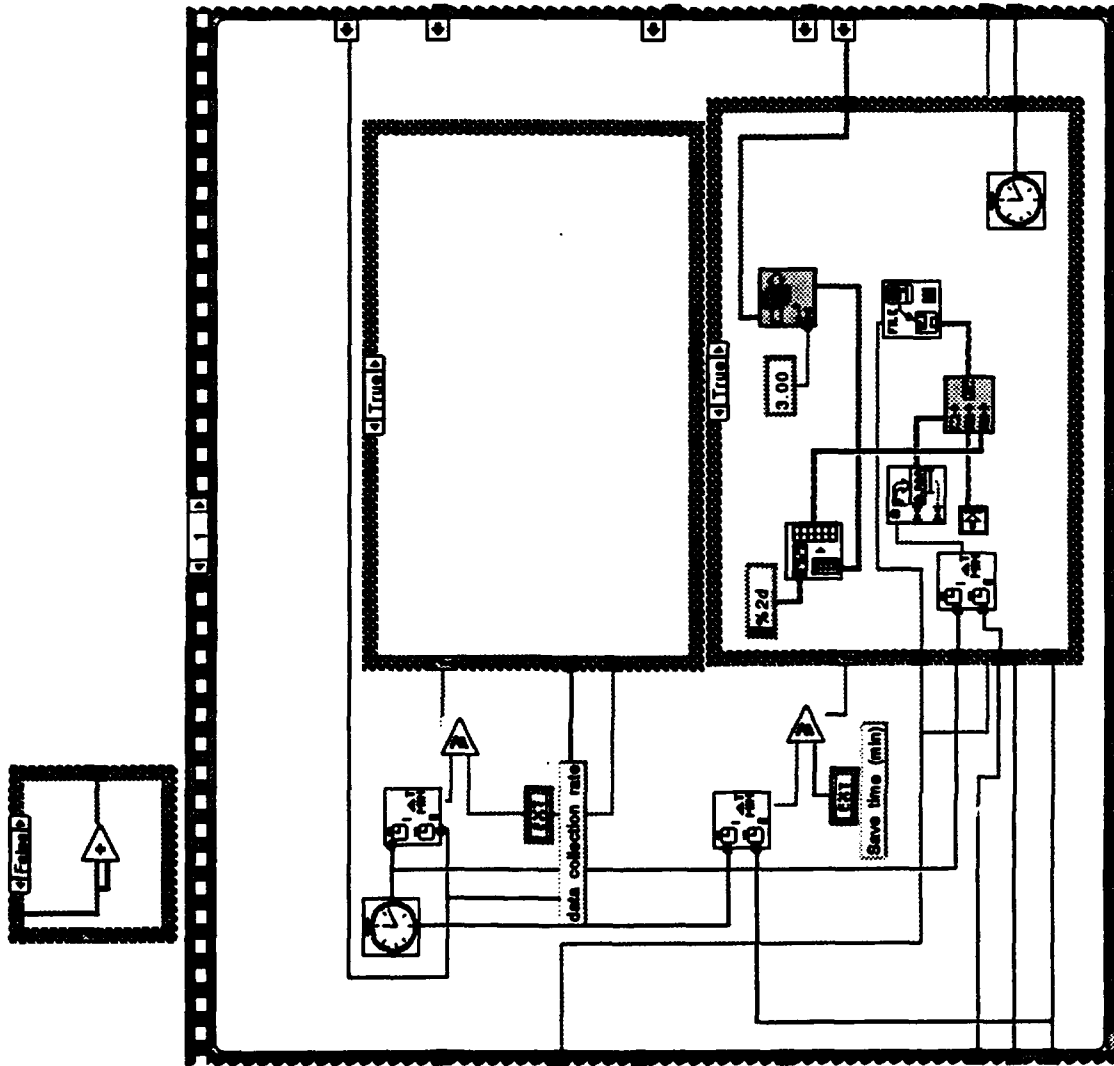

TCPO2AMMON
Thursday, May 27, 1983 2:19 PM

Page 3

