

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE	3. REPORT TYPE AND DATES COVERED FINAL REPORT 1 Apr 93 - 31 Mar 94		
4. TITLE AND SUBTITLE TIME-RESOLVED, HIGH-RESOLUTION, X-RAY MICROSCOPY OF IN-VITRO BIOLOGICAL AND LIFE SCIENCE SPECIMENS WITH THE AID OF LASER PLASMAS			5. FUNDING NUMBERS 61102F 2301/BS		
6. AUTHOR(S) Professor Martin Richardson					
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) University of Central Florida 4000 Central Florida Blvd Orlando, FL 32816-0150			8. PERFORMING ORGANIZATION REPORT NUMBER AFOSR-TR 94 0449		
9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES) AFOSR/HE 110 DUNCAN AVENUE SUITE B115 BOLLING AFB DC 20332-0001			10. SPONSORING / MONITORING AGENCY REPORT NUMBER F49620-93-1-0148		
11. SUPPLEMENTARY NOTES					
12a. DISTRIBUTION / AVAILABILITY STATEMENT APPROVED FOR PUBLIC RELEASE; DISTRIBUTION UNLIMITED					
13. ABSTRACT (Maximum 200 words) The intent of this contract was to help create an x-ray microscopy facility at the Laser Plasma Laboratory at CREOL specially dedicated to applications to biology. The hope of this contract was that, in setting up a dedicated facility here in the US, we might attract the collaboration of medical and biological researchers, and thereby demonstrate the usefulness of this form of x-ray analysis. Hopefully then further development of this approach could then be supported by research funds from the medical and biological sciences. We have been successful in this endeavor. We have established a facility for biological microscopy. This facility will soon be a dedicated facility to this activity. We have produced our own x-ray images of biological specimens. Most encouragingly, we have formed collaboration with several groups of biologists and medical scientists to exploit this technology further.					
14. SUBJECT TERMS			15. NUMBER OF PAGES		
			16. PRICE CODE		
17. SECURITY CLASSIFICATION OF REPORT UNCLASSIFIED			18. SECURITY CLASSIFICATION OF THIS PAGE UNCLASSIFIED	19. SECURITY CLASSIFICATION OF ABSTRACT UNCLASSIFIED	20. LIMITATION OF ABSTRACT UNCLASSIFIED

AD-A283 200

8001 Ym



UNIVERSITY OF CENTRAL FLORIDA

CREOL - CENTER FOR RESEARCH AND EDUCATION IN OPTICS AND LASERS

12424 Research Parkway, Suite 400, Orlando, Florida 32826 • Phone (407) 658-6800 • FAX (407) 658-6880

AFOSR-IR 94 0449

Approved for public release;
distribution unlimited.

Final Technical Report

**Time-resolved, high-resolution, x-ray
microscopy of *in-vitro* biological and life science
specimens with the aid of laser plasmas.**

Martin Richardson,
CREOL,
University of Central Florida,
Orlando, FL 32826
tel #407 658 6819
fax# 407 658 6880

Contract F49620-93-1-0148

Dr Howard Schlossberg,
Air Force Office of Research,
Bolling Air Force Base,
Washington, DC

94-25319
[Barcode] *SOP*

June 30th 1994

94 8 11 022

**Time-resolved, high-resolution, x-ray
microscopy of *in-vitro* biological and life science
specimens with the aid of laser plasmas**

As a final report for this one-year contract we submit a short summary of the success of this contract and as evidence of the technical output of this contract we submit copies of ~~three~~ ^{four} manuscripts which have been, or are in the process of being, published. These submissions satisfy the stated requirements of the contract.

The initial intent of this contract was to help create an x-ray microscopy facility at the Laser Plasma Laboratory at CREOL specially dedicated to applications to biology. This followed on work that we had initiated in Japan. The hope of this contract was that, in setting up a dedicated facility here in the US, we might attract the collaboration of medical and biological researchers, and thereby demonstrate the usefulness of this form of x-ray analysis. Hopefully then further development of this approach could then be supported by research funds from the medical and biological sciences.

We have been successful in this endeavor. We have established a facility for biological microscopy. This facility will soon be a dedicated facility to this activity. We have produced our own x-ray images of biological specimens. Most encouragingly, we have formed collaboration with several groups of biologists and medical scientists to exploit this technology further. Principal among these are

[a] Our Japanese collaborators. These include K. Shinohara from the Tokyo Metropolitan Institute of Medical Science, Y. Kinjo of the Tokyo Metropolitan Isotope

Research Center, and K. Tanaka of the Institute of Laser Engineering of the University of Osaka. CREOL has also established a separate collaboration agreement with ILE in the general area of laser plasmas. We are currently continuing our collaboration with these workers in the area of human chromosome studies.

[b] Our British collaborators. These include Dr Tony Stead from Royal Holloway College, University of London and Dr Robin Cotton from Oxford University. We are presently studying dry and wet samples of botanical cells such as crithidia with this group.

[c] Arnold Palmer Hospital for Children & Women Orlando, Florida. We are collaborating with Dr Jayshree Rajyaaguru in the study of bacteria such as p. cerpacia that presently have a high resistance to antibiotics. This structure changes under the stimulus of certain drugs. We are using x-ray microscopy to analyze the structural effect of these drugs.

[d] Orlando Regional Health Center, Orlando Florida. We are collaborating with Dr Jane Gibson in the study of fragile X syndrome in human chromosomes.

From the above, it is evident that we have begun to make meaningful outreach to medical and biological research groups, and that we are progressing toward our goal of having the progress of this technology driven by those who stand to benefit the most from it. We hope that in the future this will lead to funding support from agencies such as NIH and NCI and outside sponsorship.

For completeness, we include copies of three ^{four} publications that have so far been prepared under the tenure of this contract.

Accession For	
NTIS GRA&I	<input checked="" type="checkbox"/>
DTIC TAB	<input type="checkbox"/>
Unannounced	<input type="checkbox"/>
Justification	
By _____	
Distribution _____	
Availability Codes	
Dist	Avail and/or Special
A-1	

Pulsed x-ray microscopy of biological specimens with laser plasma sources.

Martin Richardson*, Kunio Shinohara[†], Kazuo A. Tanaka[‡],
Yasuhito Kinjo[†], Naomi Ikeda[‡] & Masataka Kado[‡].

* Center for Research in Electro-Optics & Lasers, University of Central Florida, Orlando, FL 32826, USA.

[†] Department of Radiation Research, Tokyo Metropolitan Institute of Medical Science, Bunkyo, Tokyo, 113, Japan.

[‡] Institute of Laser Engineering, Osaka University, Suita, Osaka, 565, Japan

[†] Radiation Biology Division, Tokyo Metropolitan Isotope Research Center, Setagaya, Tokyo, 158, Japan.

ABSTRACT

The development of a compact, affordable, high-resolution x-ray microscope will have a strong impact on the biological and medical sciences. We discuss the potential that pulsed, laser-plasma x-ray sources have to this development. Several approaches to the high-resolution analysis of dried and *in-vitro* biological specimens with laser-plasma sources are described. We discuss the details of the laser and plasma conditions required for optimum x-ray generation, and the various x-ray optical and x-ray electro-optical imaging systems which could be incorporated into a compact, laser-plasma x-ray microscope.

I. Introduction.

At the present time detailed high resolution analysis of sub-cellular biological and life science structures is most commonly performed by electron microscopy. It is well-known that while this technique can provide Angstrom resolution, it suffers from a small depth of field and the need to significantly treat the samples (drying, dyeing, sectioning, coating etc.) before analysis. X-ray microscopy in principle will avoid many of these limitations. While being limited to the resolution in the 100A range, it's ability to probe the internal structure of *in-vitro* assemblies provides biologists and life scientists the opportunity to observe complex features in their natural, even live state. Most x-ray microscope development has so far been made using large synchrotron sources. The latter limits x-ray microscopy to being primarily a limited research tool centered around a complex beam line located at a major synchrotron facility. The use of a laser-plasma x-ray source, however, makes plausible the development of a compact x-ray microscope having a size and cost comparable to a conventional electron microscope. The overall design of such a laser plasma-based x-ray microscope is illustrated in fig.1. One could envisage such a system being part of the standard analytical hardware available in major research and medical institutions. In this paper, we review the characteristics of laser-plasmas as they pertain to a microscope source, and discuss the various imaging technologies which can be incorporated into such a source. In the latter, we describe some new results obtained with both reflective optical microscopy and with high-resolution contact microscopy of dry and wet cellular structures. We also discuss the potential incorporation of high magnification electron-optical imaging systems into a compact x-ray microscope and the capability it will give for real-time imaging.

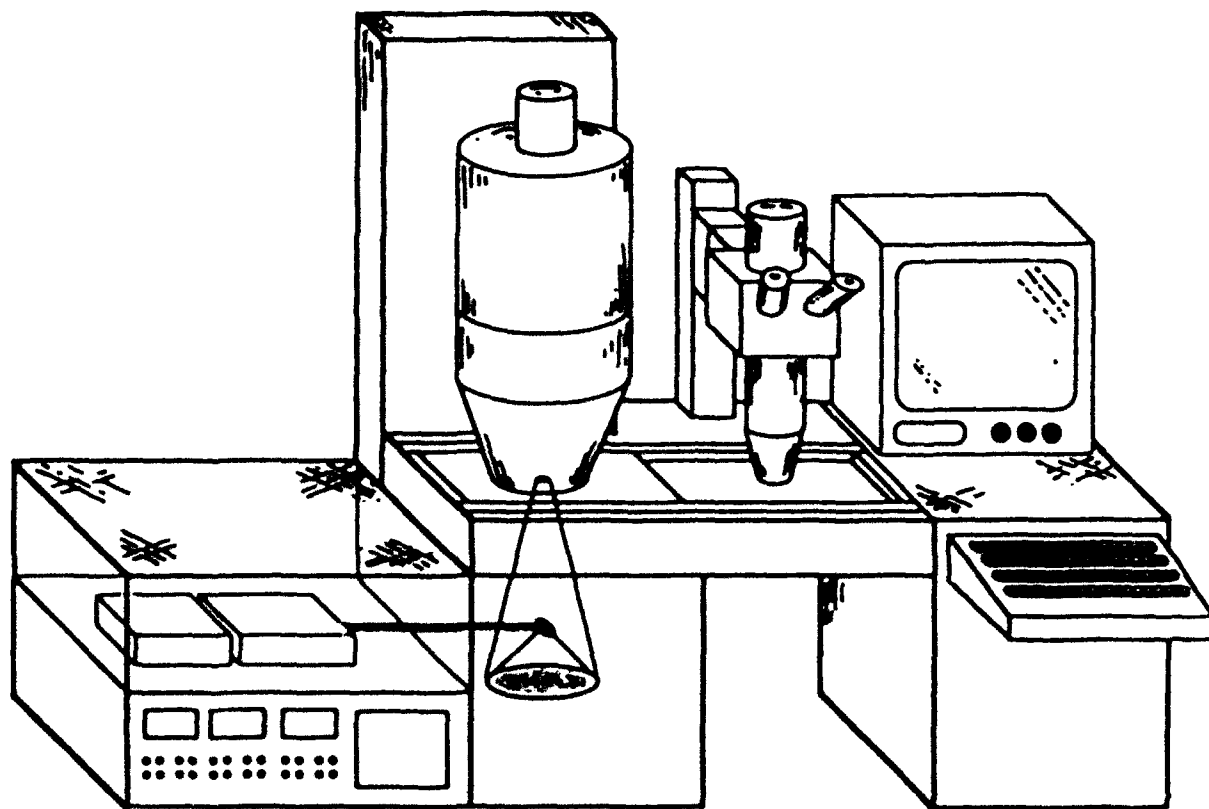


Fig.1. Design concept of a compact, stand-alone, laser-plasma x-ray microscope.

II. Advantages of a laser plasma source for x-ray microscopy of biological specimens.

The primary advantages of a laser plasma x-ray source stem from its compactness and flexibility. As has been previously mentioned, the spectral brightness of laser plasma x-ray sources can be comparable to the brightest available synchrotrons¹. Laser plasma x-ray sources have the advantage of being compact, moveable and tolerable of modest vacuum requirements. The x-ray emission spectrum of laser plasmas is rich in bright broad (Planckian) continuum emission and in narrow atomic emission lines, and can easily be varied to suit specific microscopy needs. Typical characteristics of the x-ray emission of laser plasmas are illustrated in fig.2. This selectivity in x-ray wavelength has a potential high dividend for x-ray microscopy in facilitating elemental analysis of features within biological structures by difference imaging with emission at two different wavelengths. Laser plasmas are point sources which can be highly reproducible, a requirement for precision x-ray optical systems having extremely high alignment specifications. Lastly pulsed laser plasmas introduce the time domain element into x-ray microscopy. Whereas exposure times for microscopy with synchrotrons are measured in seconds, laser plasmas can provide x-ray emission in pulses ranging from several nanoseconds duration to less than one picosecond. This introduces the possibility of capturing kinetic, chemical, or morphological changes in biological structures in time frames of interest to understanding complex biological processes. No other type of microscopy can offer this capability.

Many measurements of the x-ray emission from laser plasmas have been made in the spectral regions of interest for biological microscopy²⁻⁵, that is in the so-called 'water window' (2.3-4.4nm), and at other, element specific wavelengths. However these measurements have been made with laser and

target characteristics more germane to other applications of laser plasmas (such as laser fusion and x-ray laser generation). Moreover these studies have not had reason to consider the effects of plasma and particulate blowoff from the laser plasma, an important additional issue for microscopy, as it is for the use of laser-plasmas x-ray sources for lithography^{6,7}, where the integrity of expensive x-ray optics in close proximity to the target must be preserved. To the author's knowledge, no detailed laser-plasma design study has yet been made specifically to satisfy all the needs of pulsed x-ray microscopy.

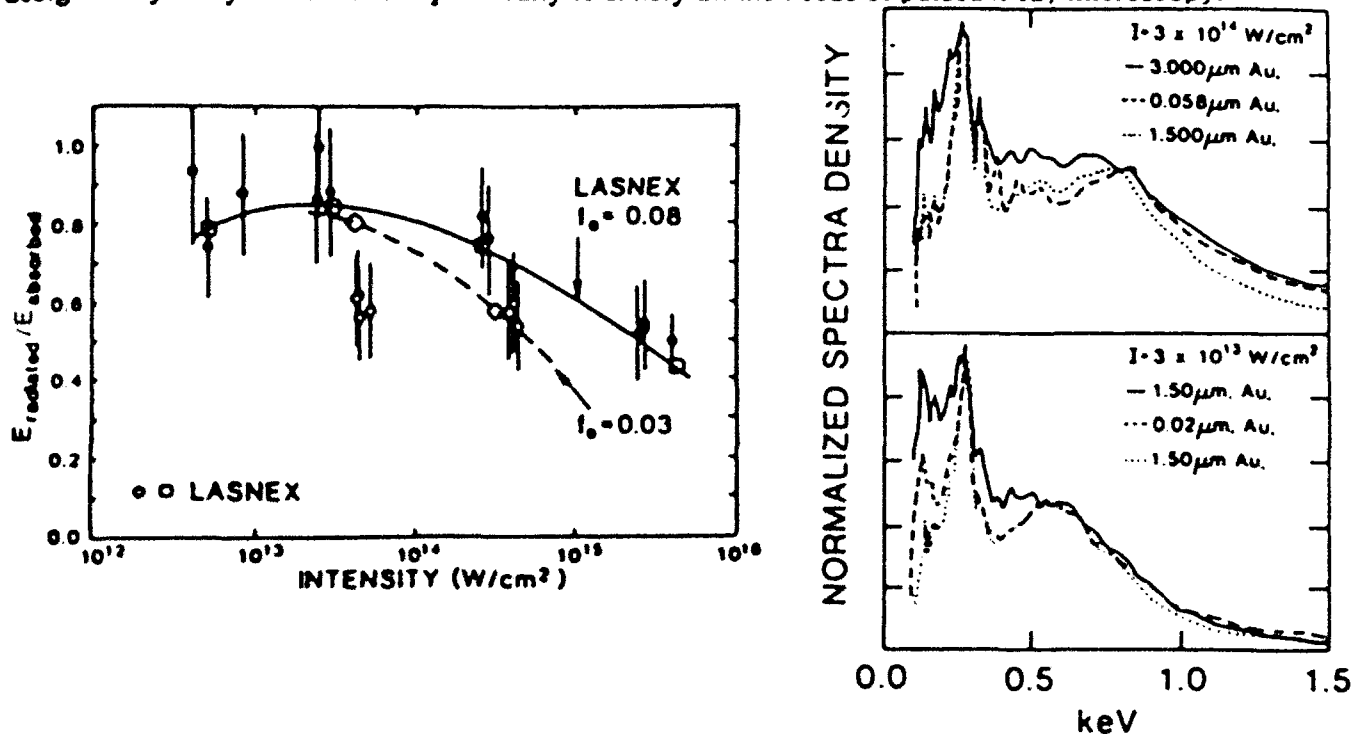


Fig.2. X-ray spectral characteristics of laser plasmas produced from Au targets. (a) shows the variation of x-ray conversion efficiency with laser intensity, and (b) indicates the variation of the x-ray spectrum with laser intensity. (from ref. 2)

III. X-ray optical requirements for a laser-plasma x-ray microscope.

In determining the specifications of x-ray optical components in a laser plasma-based x-ray microscope, we first establish the primary performance requirements of the overall system. We assume that the required resolution must be in the range of current imaging capabilities, $\sim 50\text{nm}$. This resolution, or better, has been demonstrated with Fresnel zone-plate imaging^{8,9}, contact imaging^{10,11}, and, at longer wavelengths, with normal incidence reflective optical imaging¹². Moreover we assume that the system must be capable of real-time image acquisition. Current advanced image array detectors have pixel sizes in the $6\mu\text{m}$ range. Assuming a minimum image contrast ratio of ~ 10 , this implies the need for an overall image magnification of $\sim 3 \times 10^3 - 10^4$. This level of image magnification cannot easily be met with x-ray optics alone. Although most x-ray microscopes today rely primarily on optical elements having modest image magnification and long-time image processing of an image recorded on resist, film, or through image scanning, we believe the optimum microscope will require real-time image acquisition and thus will incorporate a combination of x-ray image magnification and electron-optical image magnification. Such a system is shown schematically in fig. 3. The specimen to be analyzed will be irradiated with monochromatic radiation from the laser plasma source. This could be facilitated by either a normal incidence multilayer mirror collector or a zone-plate condenser. An image of the specimen in the backlit radiation is then created with either a Schwarzschild microscope or Fresnel lens with a magnification (20-50) commensurate with the cathode resolution capability of an electro-optical image magnifier such as an x-ray-sensitive zoomtube¹³ or an x-ray photoelectron microscope^{14,15}. A zoomtube having an image

magnification of 40-200 and a cathode resolution of $\sim 1\mu\text{m}$ has already been demonstrated¹³. Moreover, a photoelectron microscope having a resolution of $0.1\mu\text{m}$ and a magnification of 1000 should be developed in the near future¹⁶. At some loss in resolution, but with considerable gain in sensitivity and simplicity, the latter could be used in a simple contact or 'proximity' imaging mode.

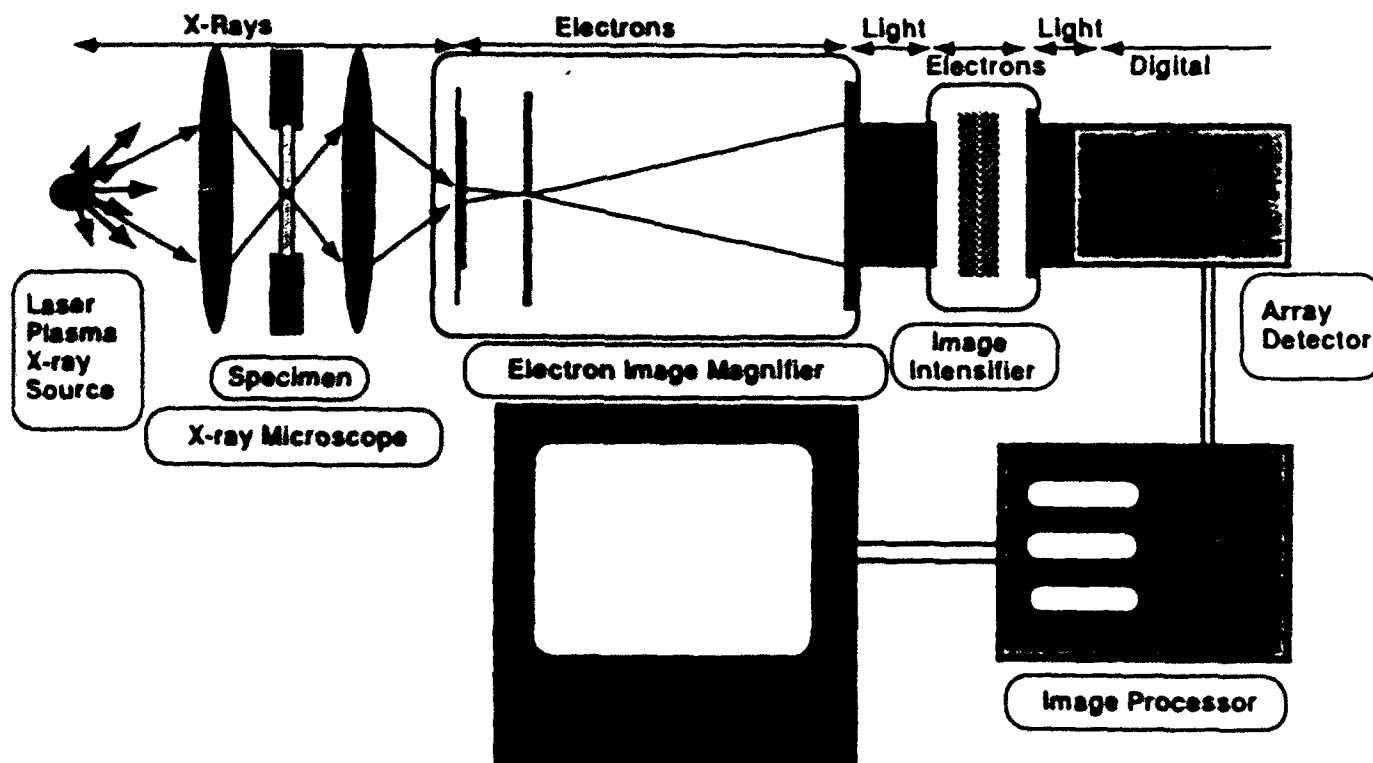


Fig.3 Possible structure of an x-ray - photoelectron-optical microscope.

We currently are investigating the practicality of two forms of x-ray imaging which could be incorporated into a laser plasma x-ray microscope of the type described above. In the first we investigate the limits of contact microscopy for analyzing *in-vitro* biological objects. In this investigation we study the effects of the x-radiation on the specimen, the degree to which the image contrast can be enhanced, and the resolution limits that can be achieved. In the second approach we examine the potential that Schwarzschild optics have in combination with laser-plasma x-ray sources for microscopy. We have made investigations with several Schwarzschild optics coated with x-ray multilayer coating with reflectivities centered at different wavelengths (4.42nm, 7nm and 17nm). We discuss the primary issues of resolution and contrast as well questions of practicality, stability and ease of use in so far as envisaging such an optic in a compact x-ray microscope system.

IV. High resolution contact imaging of *in-vitro* biological specimens.

Many previous studies of contact microscopy of biological and life science objects have been reported. Several different sources have been used¹⁷⁻²², including pulsed e-beam devices and synchrotrons, and a few recent investigations have been made with laser-plasma sources^{21,22}.

In the present studies small water specimen cells, $1-3\mu\text{m}$ thick, having a 100nm thick SiN window and backed with polymethylmethacrylate (PMMA) photoresist, fig.4(a), were used to contain stretched, live human chromosomes. They were irradiated with the x-rays generated by one pulse from a high power laser irradiating a planar Au target located 2cm away. The plasma was created on the target by 26J energy, 526nm wavelength, 1ns duration laser pulses with a focal spot intensity of $\sim 10^{13}\text{W}/\text{cm}^2$.

In this configuration a spherical W/C multilayer x-ray mirror²⁶ is used to focus 4.4nm wavelength x-rays onto the specimen cell. This approach should result in higher contrast images and in less radiation damage to the specimen from highly absorbed radiation from the x-ray source.

The principal limitation and disadvantage of this form of contact microscope is the complexity and delay involved in processing the x-ray image. This can be removed if contact microscopy could be integrated with a special form of x-ray-sensitive photoelectron microscope. Considerable progress has been made in the last few years in developing low energy photo-emission microscopes^{14,15}. The spatial resolution of these instruments can now reach below 100nm^{14,15}. The development of highly resolving transmission x-ray photocathodes having a spatial resolution in this range, and their incorporation with a similar electron-optical system to that used in a photo-emission microscope¹⁶, would provide this capability. Such a system could be used in combination with contact imaging to provide high magnification, real-time images of biological specimens.

V. Normal-incidence reflective x-ray optical microscopy.

An important component in the microscope design described above is the high-resolution x-ray objective. This can, in principle, be a reflective optic, using either grazing incidence optics or normal incidence, high-reflectivity, multilayer coatings, or a transmissive Fresnel lens. We have made considerable effort in the last few years to explore the potential of x-ray multilayer-coated Schwarzschild x-ray optical elements for high-resolution biological microscopy. It is well known that this approach to high-resolution microscopy presses the limits of x-ray mirror fabrication and efficient x-ray mirror design. A 120mm diameter, NA = 0.35, 15X Schwarzschild microscope coated with Ni/C multilayer mirrors for 7nm and having a measured resolution, limited by the recording film-grain size, of 0.5 μ m was developed by Kado et al^{27,28}, and separately Richardson et al²⁹ developed a smaller, 33mm diameter, NA = 0.28, 15X Schwarzschild microscope coated with a W/C multilayer mirror for 4.4nm, in the so-called 'water window' (2.5-4.4nm). In the present, we report a multilayer-coated Schwarzschild microscope for 17nm, of similar design to that in ref.28. In particular, we report it's application, for the first time with a laser plasma source to the imaging of biological specimens.

The biological specimens used in these studies were dried HeLa cells in their natural state. The cells were supported on a thin plastic membrane, and irradiated with x-rays from a laser plasma created from a thin Au target. These experiments were made with the setup shown in fig.6.

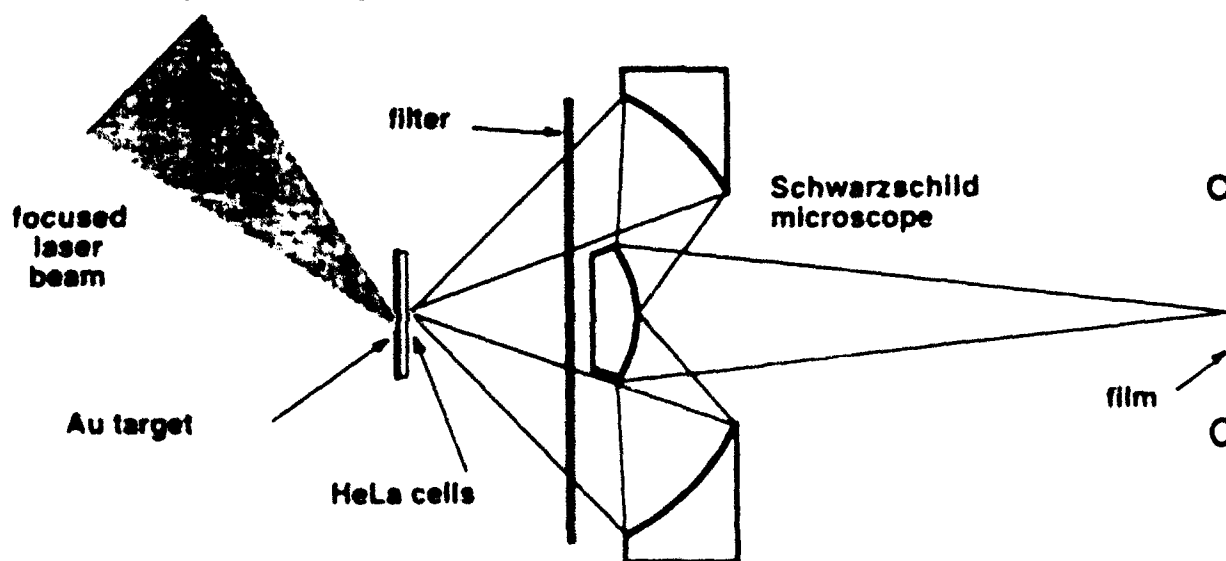


Fig.6. Experimental configuration for imaging x-ray microscopy of dried HeLa cells

The specimen cell was positioned at an angle of 45° to the normal to the target and the laser beam axis. The stretched chromosomes were prepared by the surface-spreading technique and whole-mounted directly on the PMMA photoresist.



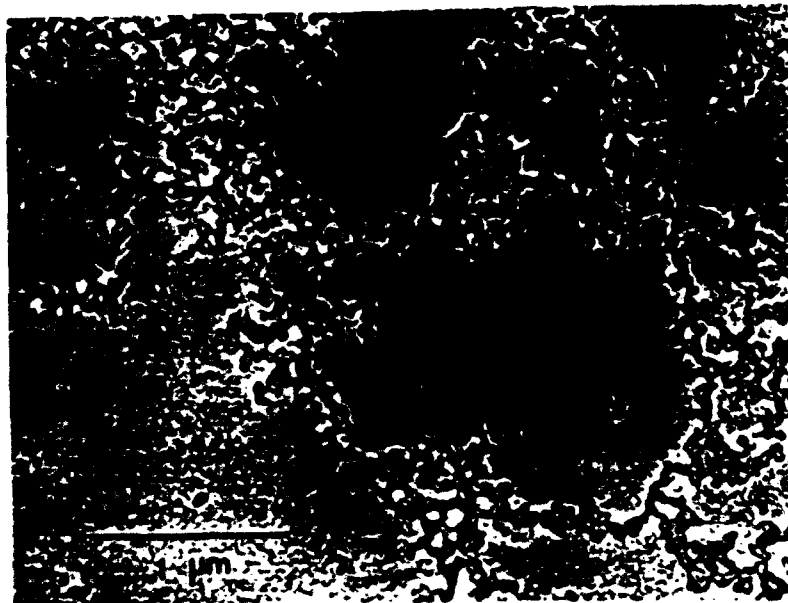


Fig.4. (a) Contact irradiation scheme. (b) Contact image of stretched in-vitro human chromosomes obtained with a single nanosecond burst of laser plasma x-rays.

After irradiation, the resist was developed by dissolving the damaged material in a mixture of methyl isobutyl ketone and isopropyl alcohol. Visualization of the three-dimensional morphology of the developed resist was then made by transmission electron microscopy of a thin ethylene replica of the resist made by plasma polymerization²³. This technique of analysis is described in more detail elsewhere²⁴. A typical image is shown in fig. 4(b). This shows details of the stretched in-vitro chromosome structure. Clearly visible are the superbead structure of chromatin fibrils, as described by Watanabe²⁵, composed of supertwisted DNA molecules. In fact the supertwisted DNA fiber, which has a dimension of $\sim 10\text{nm}$ can be seen connecting the superbeads. This image clearly demonstrates the capability of obtaining nanosecond-time-resolved x-ray images with a resolution down to the resolution limit of the resist, using a laser plasma. Although the TEM images of these chromosomes appears quite good, we believe the image contrast can be further improved. The x-rays used to irradiate the sample in these experiments possessed a broad spectral range, not optimized for maximum image contrast of the chromosomes. This will best be achieved with x-rays in the water window. To this end we are currently using 4.4nm wavelength x-rays from a laser plasma obtained as in the configuration shown in fig.5.

Fig.5.

Scheme for monochromatic, water-window contact x-ray microscopy.

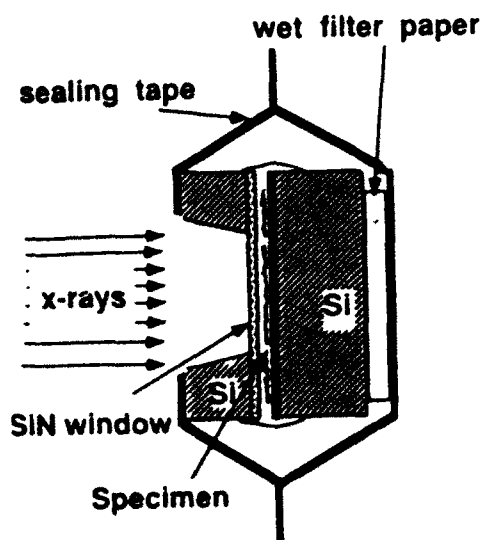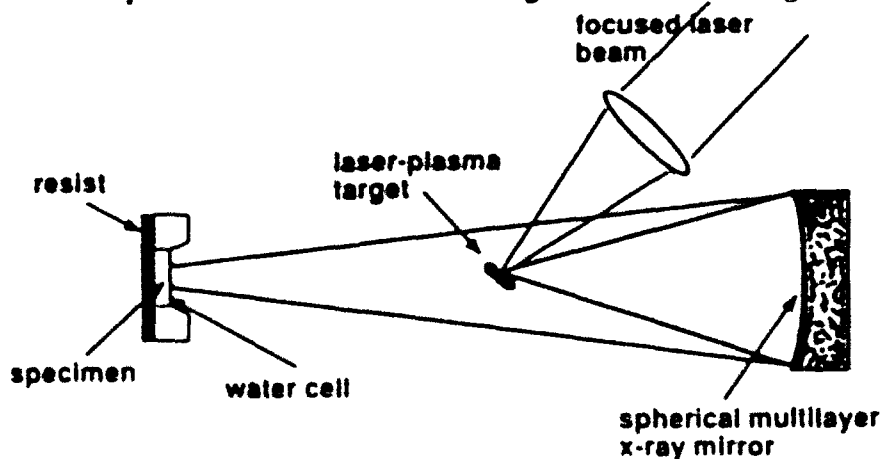

membrane supporting the HeLa cells was configured on a rectangular grid structure in direct contact with a 0.2 μ m thick Au laser plasma target, the whole assembly being positioned on a metallic washer accurate (1 μ m resolution) three-dimensional stepper motor-controlled target positioner in the center radiation vacuum chamber at 5×10^{-4} Torr. The grid structure was incorporated as an aid in placing the specimen to be in the correct position relative to the focus position of the irradiating laser, and the alignment of the Schwarzschild microscope to the specimen.

A precision method of alignment was vital to recording well-focused images of preselected regions of the HeLa cells distributed across the membrane. The position of the 200 μ m diameter laser spot was accurately registered on two CCD-recorded viewing systems attached to the target holder, in separate laser irradiation experiments with thin foil targets, in which the laser plasma produced a small $\sim 200\mu$ m diameter hole. This hole was then used to align the lateral position of the Schwarzschild microscope relative to the laser plasma x-ray source. The surrogate target was then aligned with the biological cell target, and aligned optically to the laser focus position. The axial position of the Schwarzschild microscope was then adjusted under vacuum by illuminating the grid and cell structure with white light and using a high-resolution CCD camera in the image plane of the microscope. Precise lateral motion of the target structure then permitted selection of the desired cell region for x-ray examination. The final x-ray image was recorded on Kodak 101 x-ray film, developed according to the calibration of Henke et al. A thin x-ray filter, (200nm Al on 300nm CH), was used to prevent visible light from the plasma from being detected. The duration of the x-ray emission is similar to the duration of the irradiating laser pulse (300ps). Thus the x-ray emission irradiates the sample before it is destroyed by the expanding laser plasma.

A typical single-shot x-ray image of dried HeLa cells recorded by the Schwarzschild microscope is shown in fig.7. The grid thickness and separation is 20 μ m and 100 μ m respectively. The individual, 10 μ m diameter HeLa cells are clearly visible, with a resolution of ~ 500 nm, limited by the grain size of film (5-7 μ m). Fig.8 shows the correlation between the optical image of a HeLa cell structure taken prior to irradiation with the resulting x-ray image of the same structure.

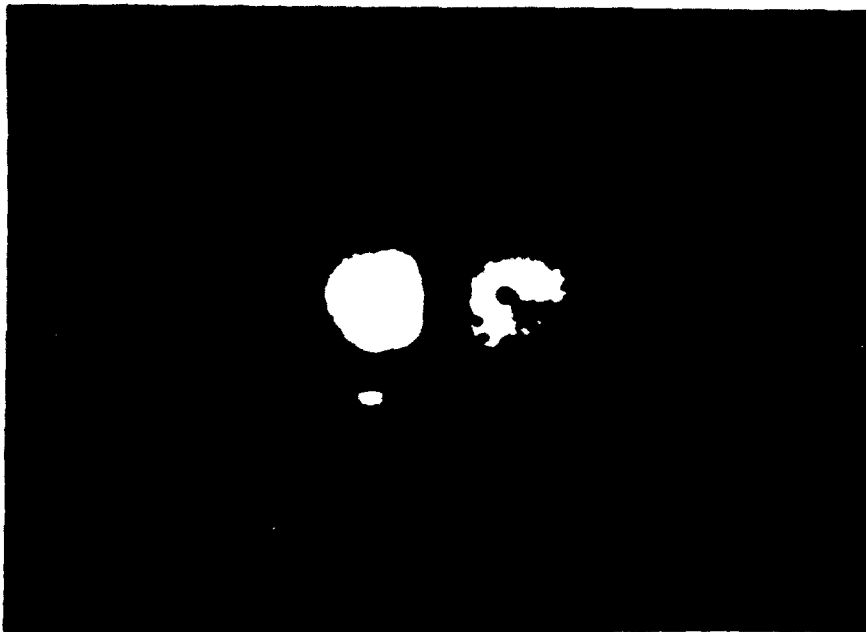


Fig. 7. X-ray image at 17nm of dried HeLa cells. Grid bar width 20 μ m, grid separation 100 μ m



Fig.8. Corresponding optical (a) and x-ray (b) images of dried HeLa cells.

These images of these biological structures are limited in resolution by the film used for image recording. This limitation will be removed in future experiments with the use of an x-ray sensitive, electron-optical zoomtube image magnifier and direct, real-time, image acquisition¹³. The full potential of this approach will then be realized.

VI. Summary.

We have presented a concept of a practical x-ray microscope based on a compact laser plasma x-ray source. In addition, we have summarized our progress in both contact and imaging x-ray microscopy of biological samples in their natural state. In the future we plan to use these approaches towards two near term objectives. Firstly these techniques will be used to survey a wider range of biological samples to demonstrate the usefulness of x-ray microscopy to biological, medical and life sciences. Secondly, we will continue to develop these and the other technologies mentioned in this paper that are required for the successful fabrication of a practical stand-alone x-ray microscope.

VII. References.

1. N.M. Ceglio, *J. X-Ray Sci. & Tech.* **1** 1 (1990)
2. P. D. Goldstone, S. R. Goldman, W. C. Mead, J. A. Cobble, G. Stradling, R. H. Day, A. Hauer, M. C. Richardson, R. S. Marjoribanks, P. A. Jaanimagi, R. L. Keck, F. J. Marshall, W. Seka, O. Barnouin, B. Yaakobi & S. A. Letzring. *Phys. Rev. Lett.* **59**, 56-59 (1987)
3. K. Eidmann & T. Kishimoto. *Appl. Phys. Lett.* **49**, 377 (1986)
4. R. Kodama, K. Okada, N. Ikeda, M. Mineo, K. A. Tanaka, T. Mochizuki & C. Yamanaka, *J. Appl. Phys.* **59**, 3050, (1986)
5. K. A. Tanaka, H. Aritome, T. Kanabe, M. Nakatsuka, T. Yamanaka & S. Nakai, *Proc SPIE*. **1140**, 350, (1989)
6. M. C. Richardson, W. T. Silfvast, H. Bender, A. Hanzo, V. Yanovsky, F. Jin & J. Thorpe, *Appl. Opt.* (to be published)
7. F. Bijkerk, E. L. Marnix, J. van der Wiel, E. C. I. Turcu, G. J. Tallents & D. Batani, *J. X-Ray Sci. & Tech.* **3**, 133, (1992)

- B. Niemann, X-ray Microscopy III (Ed A. G. Michette, G. R. Morrison & C. J. Buckley), Springer Verlag (Berlin), p142, (1992)
- W. Meyer-Ilse, P. A. Guttman, J. Thieme, D. Rudolph, G. Schmah, E. Anderson., P. Batson, D. Attwood, N. Iskander & D. Kern, X-ray Microscopy III (Ed. A. G. Michette, G. R. Morrison & C. J. Buckley), Springer Verlag (Berlin), p284, (1992)
10. K. Shinohara, X-Ray Microscopy in Biology and Medicine, (Ed. K. Shinohara, K. Yada, H. Kihara, & T. Saito) Publ. Springer Verlag, p203, (1990)
11. K. Shinohara, Y. Kinjo, M. C. Richardson, A. Ito, N. Morimoto, Y. Horiiko, M. Watanabe, K. Yada & K. A. Tanaka, Proc. SPIE 1741, (1992), this volume.
12. D. W. Berreman, J. E. Bjorkholm, L. Eichner, R. R. Freeman, T. E. Jewel, W. M. Mansfield, A. A. MacDowell, M. L. O'Malley, E. L. Raab, W. T. Silfvast, L. H. Szeto, D. M. Tennant, W. K. Waskiewicz, D. L. White, D. L. Windt, O. R. Wood II & J. H. Brunning, Opt. Lett. 15, 529 (1990)
13. K. Kinoshita, T. Matsumura, Y. Inagaki, N. Hirai, M. Sugiyama, H. Kihara, N. Watanabe, Y. Shimanuki & A. Yagashita, X-ray Microscopy III (Ed. A. G. Michette, G. R. Morrison & C. J. Buckley), Springer Verlag (Berlin), p335, (1992)
14. W. Engel, M. E. Kordes, H. H. Rotermund, S. Kubala & A. von Oetzen, Ultramicroscopy, 36, 148 (1991)
15. G. F. Rempfer, W. P. Skoczylas & O. H. Griffith, Ultramicroscopy, 36, 196 (1991)
16. T. Lucatorto & R. N. Watts (private communication)
17. R. Feder, E. Spiller, J. Topalian, A. N. Broers, W. Gudat, B. J. Panessa, Z. A. Zadnaisky & J. Sedat, Science 197, 259 (1977)
18. B. J. Panessa, G. Coleman, R. A. McCorkle & J. B. Warren, Ultramicroscopy, 5, 267 (1980)
19. R. Feder, V. Banton, D. Sayre, J. Costa, M. Baldini & B. Kim, Science, 227, 63 (1985)
20. Y. Kinjo, K. Shinohara, M. Watanabe, S. Kikuchi, K. Kobayashi & H. Maezawa, X-Ray Microscopy in Biology and Medicine, (Ed. K. Shinohara, K. Yada, H. Kihara, & T. Saito) publ. Springer Verlag, p243, (1990)
21. R. J. Rosser, K. G. Baldwin, R. Feder, D. Bassett, A. Coles & R. W. Eason, J. Microscopy, 138, 311 (1985)
22. P. C. Cheng, S. P. Newberry, H. G. Kim & M. D. Wittman, Eur. J. Cell Biol. 48, (Suppl. 25) 169 (1989)
23. K. Shinohara, H. Nakano, M. Watanabe, Y. Kinjo, S. Kikuchi, Y. Kagoshima, K. Kobayashi & H. Maezawa, X-Ray Microscopy II (Ed. D. Sayre, M. Howells, J. Kirz, & H. Rarback), p 429, Springer Verlag, Berlin, (1988)
24. K. Shinohara, H. Nakano, Y. Kinjo & M. Watanabe, J. Microscopy, 158, 335 (1990)
25. M. Watanabe Saibou (Cell) 18, 460, (1960)
26. The multilayer x-ray mirrors used in this experiment were fabricated by J. Underwood & J. Kortright of the Center for X-ray Optics at LBL.
27. M. Kado, K. A. Tanaka, R. Kodama, T. Yamanaka, K. Yamashita, M. Ohtani, S. Kitamoto and S. Nakai, Rev. of Laser Eng. (in Japanese), 18, 938, (1990)
28. M. Kado, K. A. Tanaka, R. Kodama, T. Yamanaka, S. Nakai, K. Yamashita, M. Ohtani and S. Kitamoto, Opt. Lett., 16, 109 (1991)
29. M. Richardson, W. Maixner, R. Sigel, J. Seely, C. Brown, J. Underwood and J. Kortright. 1990, (unpublished)

PROCEEDINGS REPRINT

 SPIE—The International Society for Optical Engineering

Reprinted from

Soft X-Ray Microscopy

19-21 July 1992
San Diego, California



Volume 1741

©1992 by the Society of Photo-Optical Instrumentation Engineers
Box 10, Bellingham, Washington 98227 USA. Telephone 206/676-3290.

Observation of human chromosome fibers in a water layer
by laser-plasma X-ray contact microscopy

Kunio Shinohara¹, Yasuhito Kinjo², Martin C. Richardson³, Atsushi Ito¹, Noboru Morimoto⁴, Yasuhiro Horiike⁴, Makoto Watanabe², Keiji Yada¹, and Kazuo A. Tanaka⁵

¹Department of Radiation Research, Tokyo Metropolitan Institute of Medical Science, Bunkyo-ku, Tokyo 113, Japan.

²Radiation Biology Division, Tokyo Metropolitan Isotope Research Center, Setagaya-ku, Tokyo 158, Japan.

³Center for Research in Electro-Optics and Lasers, University of Central Florida, 12424 Research Parkway, Orlando, Florida 32826, USA.

⁴Department of Engineering, Hiroshima University, Higashihiroshima-shi, Hiroshima 724, Japan.

⁵Institute of Laser Engineering, Osaka University, Suita-shi, Osaka 565, Japan.

ABSTRACT

Soft X-ray contact microscopy was applied to hydrated human chromosomes. Chromosomes of human lymphocytes were spread on a clean surface of distilled water, attached on a X-ray resist, polymethylmethacrylate (PMMA), immediately covered with silicon nitride window, and mounted in a simple hydrated chamber. The specimens were exposed to a single shot of laser-produced gold plasma X-rays (600 ps) in a vacuum chamber. The developed images were observed with transmission electron microscope using the replica method with a plasma polymerization-film in a glow discharge. The results show that we have imaged the complicated entanglement of chromosome fibers in a hydrated condition. The thickness was estimated as 10 nm in average of four narrow parts of these fibers. Particle like structures were observed in many places. The present results prove that hydrated biological specimen is observable with the contrast produced by their components themselves by soft X-ray microscopy at the resolution of 10 nm.

During this imaging exposure, however, silicon nitride (SiN) window was broken. We have studied the reason for this evidence and found that the energy absorbed by the SiN window or water layer was very high. The estimated temperature increase were 870-1470 °C for SiN and 43 °C for water layer. These results suggest that the temperature increase may be responsible for the breakage of SiN window.

1. INTRODUCTION

Application of soft X-ray microscopy to hydrated biological specimens has been demonstrated in recent years [1]. Accumulation of these results will present the new findings in biology.

Chromosomes are composed of DNA, an essential genetic material in life, and proteins. In addition, chromosome fibers have a unit structure called nucleosome, a disc-like structure of 11 nm in diameter and 5.5 nm in height. Nucleosomes are made of DNA and eight core proteins called histone. They are packed to form 30 nm chromatin fibers in a interphase cell and folded into chromosome at mitosis. During a cell cycle, nucleosomes are folded to form chromosomes for cell division and unfolded to 30 nm fibers and a single nucleosome for replication and transcription. Therefore, it is of great interest to understand this highly organized process of nucleosomes to form chromosomes and chromosome fibers, especially in situ. As a step to this goal, we have imaged dry nucleosomes in chromosome fibers in a previous paper [2]. In the present report, we have tried to observe hydrated chromosome and obtained the images of unfolded chromosome fibers. The thickness of the fibers was estimated as 10 nm in narrow parts, which means that we have imaged the size of nucleosomes and suggest that X-ray microscopy will give

us the new method to understand the detailed configuration of nucleosomes in chromosome fibers.

2. MATERIALS AND METHODS

Preparation of human chromosomes are as described elsewhere [3,4]. Briefly, chromosomes from mitotic human lymphocytes (RPMI 1788) were spread on a clean surface of distilled water and whole-mounted directly on a X-ray resist, polymethylmethacrylate (PMMA). The PMMA with a water droplet was immediately mounted in a simple hydrated specimen chamber [5]. The chamber was composed of silicon nitride window (0.25 mm x 0.25 mm; thickness, 0.4 μm) and PMMA supported by silicon bases (see, Fig. 7), and covered with a sticky tape (Scotch Sealing Tape #483). The thickness of water layer was 1-5 μm. The chamber was placed at the specimen-target distance of 28.8 mm and exposed to laser-produced gold plasma X-rays (laser wavelength, 527 nm; energy, 15.9 J) with a pulse length of 600 ps at Gekko IV, Institute of Laser Engineering, Osaka University [6]. Exposed specimens were treated as described previously [3]: (1) Removing the specimen from PMMA with sodium hypochlorite (chlorine concentration, 0.5%), (2) developing the PMMA with mixed solution of methylisobutylketone and isopropanol (3:1) for 250 s, and (3) observing with transmission electron microscope using the replica method with plasma polymerization-film in a glow discharge made of a mixture gas of ethylene and methane.

3. RESULTS AND DISCUSSION

3.1. Imaging chromosome fibers

Figure 1 shows an image of stretched part of human chromosome fibers. Since replica method was used for the observation of developed PMMA, white line surrounded by dark lines corresponds to X-ray image [2] in Fig. 1. Figure 2 shows the negative image of Fig. 1. Complicated entanglement of dark lines was observed in the whole area of Fig. 2. The image with weak contrast may be the image for the entangled chromosome fibers unfolded and dispersed from a chromosome, the remaining core part of which was imaged with clear contrast. Figure 3 shows another image of a remaining chromosome core and chromosome fibers. The negative image of Fig. 3 is shown in Fig. 4. The image shown in Figs. 3 and 4 may be the image of chromosome fibers sprung out from one chromosome core.

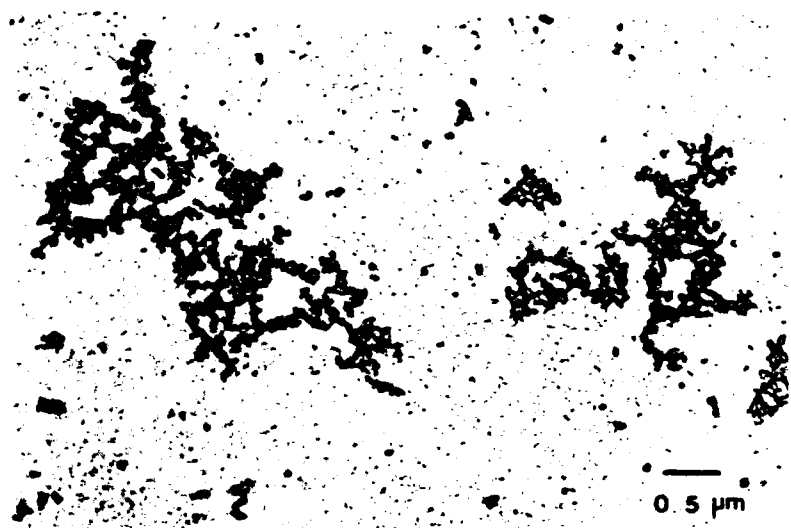


Fig. 1. X-ray image of entangled chromosome fibers with remaining core of chromosomes.



Fig. 2. Negative image of Fig. 1.

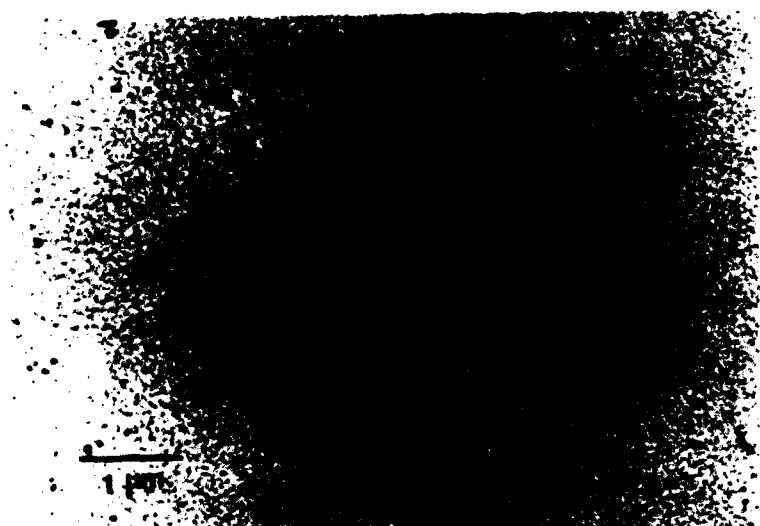


Fig. 3. Another image of entangled chromosome fibers with a remaining core of a chromosome.



Fig. 4. Negative image of Fig. 3.


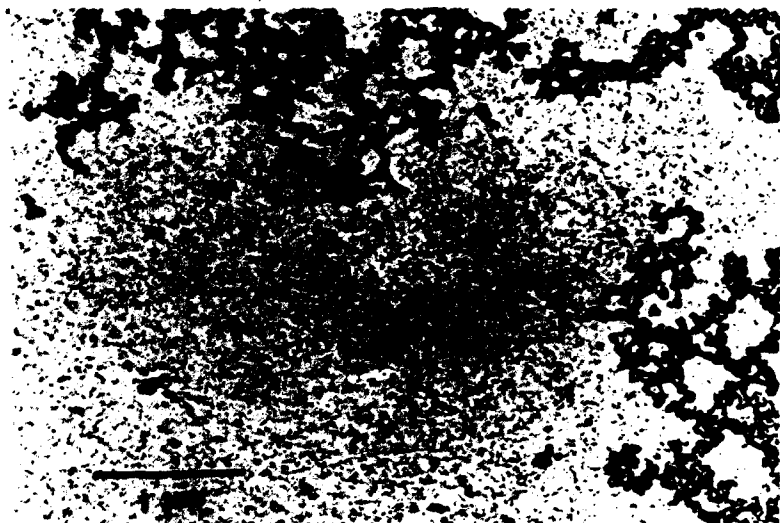


Fig. 5. Different image of an entangled chromosome fibers.



Fig. 6a. Enlarged image of a part of Fig. 5. (surrounded by a rectangle line)
6b. Illustration of a rectangle part of Fig. 6a.

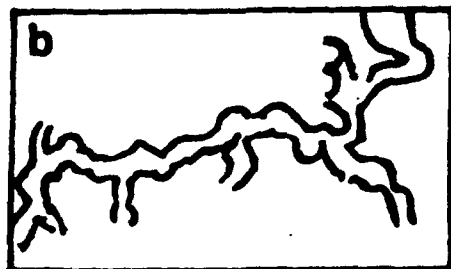

Different part of the image of chromosome fibers was shown in Fig. 5. The rectangle part surrounded by a line was enlarged and shown in Fig. 6a. Figure 6b illustrates a part of the image in Fig. 6a. The thickness of the four narrow parts of the image of a chromosome fiber shown by arrows were estimated as 9.9 nm, 9.9 nm, 9.5 nm, and 10.7 nm (10.0±0.5 nm in average). These narrow parts show particle shapes suggesting the image of nucleosomes.

The present results indicated that chromosome fibers and their unit structure, nucleosomes in a hydrated condition were observed by soft X-ray contact microscopy using pulsed (600 ps) laser-produced plasma X-rays with the contrast of their components and

suggest that soft X-ray microscopy will be a new method to study the structure of hydrated biological specimens at the resolution of as high as 10 nm.

3.2. X-ray spectra and the dose estimates

Figure 7 illustrates the exposure system. Laser (wavelength, 527 nm) was focused to a gold target. The X-rays emitted from the gold plasma show a broad spectrum with a peak wavelength of 6.2 nm [7]. The X-rays were, however, exposed to the specimen in water after passing through SiN window. Therefore, the actual spectrum of the exposed X-rays to the specimen should be changed from that of the source because of the absorption by the SiN window and water. We have estimated the X-ray spectra of various stages from level 0 to level 2 as shown in Fig. 7 with the following equation:

$$I = I_0 \exp(-\mu \cdot d) \dots \dots \dots (1)$$

where I_0 and I are X-ray fluences before and after the substance (i.e., SiN window, water, or water and a nucleosome), μ and d are the linear absorption coefficient and the thickness of the substance. Since μ is dependent on the energy of a photon (wavelength of X-rays), fluence I was calculated for each photon energy by the equation (1).

Figure 8 shows the spectra of the source (gold plasma; broken line), of the X-rays immediately after the 0.4 μm SiN window (level 1 in Fig. 7), and of the X-rays after passing through 1 μm water layer (level 2 without nucleosome in Fig. 7). Total photon flux (F) after the SiN window was estimated by the following equation:

$$F = \sum I_{E_i} \cdot \delta E_i = \sum [I_0 \cdot \exp(-\mu_{SiN} \cdot d_{SiN})]_{E_i} \cdot \delta E_i \dots (2)$$

where suffix E_i means the value at the photon energy of E_i . With the exposure condition for the Figs. 1-6 (laser energy, $E_L=15.9$ J; target-specimen distance=28.8 mm; thickness of SiN window $d_{SiN}=0.4$ μm), the total photon flux in the energy range of 0.114-1.254 keV (0.99 nm-10.9 nm) was estimated as 4.0×10^{14} photons/cm². Figure 9 shows the comparison of the spectrum of the X-rays after the water layer (1 μm) with that after the water (1 μm) and a long axis (11 nm in depth) of a nucleosome (level 2 of the case 2 in Fig. 7). The difference of these two spectra was shown in Fig. 10. This difference should cause the production of the image contrast of a nucleosome. The percent contribution to imaging a nucleosome of the wavelength of longer than 4.37 nm, 4.37-2.33 nm (water window), and shorter than 2.33 nm were 1.1%, 82.0%, and 16.9%, respectively. The results indicated that X-rays in water window were the main photons contributing to the contrast formation of a nucleosome in water.

The results were in good agreement with the expectation for X-ray microscopy of hydrated biological specimens. It should be noted, however,

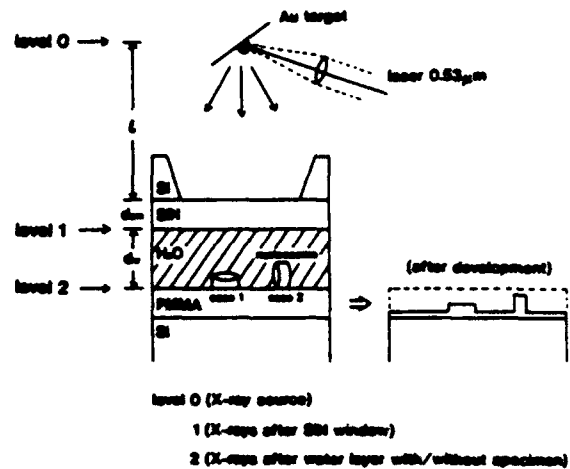


Fig. 7. Illustration of the experimental system.

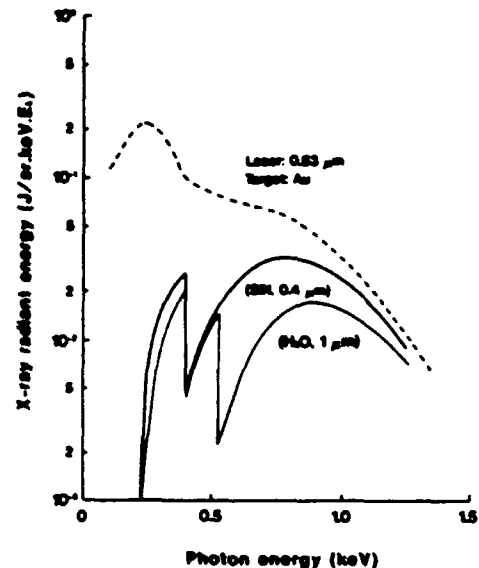


Fig. 8. X-ray spectra of a source, level 1 (after the SiN window, and level 2 (after the water layer).

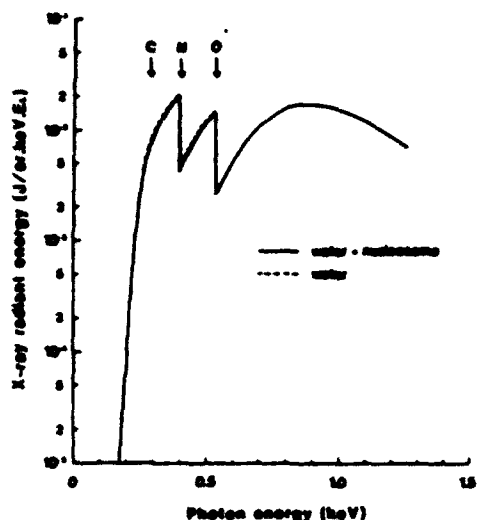


Fig. 9. X-ray spectra of level 2 (after the water with/without a nucleosome).

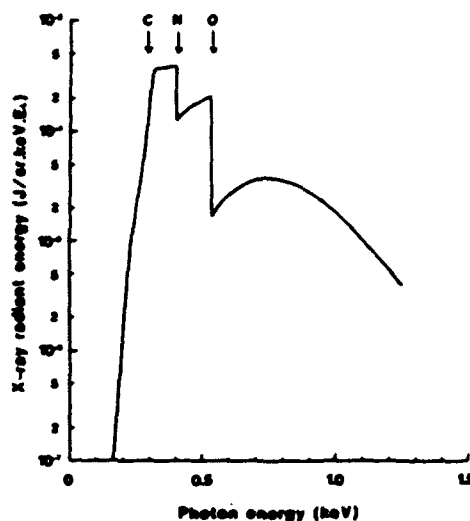


Fig. 10. Difference in X-ray spectrum after water layer with nucleosome from the spectrum after water layer alone.

that there existed a significant amount (16.9%) of contribution by X-rays shorter than 2.33 nm to the image contrast.

We have noticed that the SiN window was broken by a single shot of exposure. To study the cause for this evidence, we have estimated the energies absorbed by the SiN window and by the water with the following equations:

$$E_{SiN} = \sum [I_0 \cdot (1 - \exp(-\mu_{SiN} \cdot d_{SiN}))]_{E_1} \cdot \delta E_1 \quad \dots \dots \dots (3)$$

for SiN window and

$$E_{H_2O} = \sum [I' \cdot (1 - \exp(-\mu_{H_2O} \cdot d_{H_2O}))]_{E_1} \cdot \delta E_1 \quad \dots \dots \dots (4)$$

for water layer where I' is X-ray fluence after SiN window. In the present exposure condition for Figs. 1-6 (laser energy, $E_1=15.9$ J; target-specimen distance=28.8 mm; thickness of SiN window, $d_{SiN}=0.4$ μm), estimated energies were as follows:

$$E_{SiN} = 0.134 \text{ J/cm}^2 \text{ at } 0.4 \text{ μm SiN, and}$$

$$E_{H_2O} = 0.018 \text{ J/cm}^2 \text{ at } 1 \text{ μm H}_2\text{O.}$$

The results may correspond to the temperature increase (ΔT) for SiN window of,

$$\Delta T_{SiN} = 1470 \text{ }^\circ\text{C if we use } C_p = 99.89 \text{ J/K}\cdot\text{mol at } 25 \text{ }^\circ\text{C or}$$

$$= 869 \text{ }^\circ\text{C if we use } C_p = 169 \text{ J/K}\cdot\text{mol at } 727 \text{ }^\circ\text{C, and for water layer of,}$$

$$\Delta T_{H_2O} = 43 \text{ }^\circ\text{C}$$

where C_p is a molar heat at constant pressure assuming that there is no thermal loss during the exposure time of 600 ps. Therefore, the cause for the breakage of SiN window may be attributed to the temperature increase in SiN window and water in addition to the physical damage caused by plasma particles. The use of monochromatic X-rays in water window may reduce these temperature increase remarkably and prevent the breakage of SiN window.

4. CONCLUSION

Human chromosome fibers were observed in hydrated condition with a single shot of flush X-ray contact microscopy with a laser-produced gold plasma X-rays. The image showed the complicated entanglement of chromosome fibers unfolded and dispersed from a chromosome. The thickness of the narrow parts of unfolded chromosome fibers was estimated as 10 nm

corresponding to the size of a nucleosome. The present results prove that hydrated biological specimen is observable with the contrast produced by their components themselves by X-rays. The studies on the X-ray spectra of the imaging and the dose estimates indicated that there may be a big temperature increase in SiN window and recommended the use of monochromatic X-rays at the wavelength in water window for the imaging of nucleosomes, a unit structure of a chromosome.

5. REFERENCES

1. A. G. Michette, G. R. Morrison, and C. J. Buckley (Eds.), "X-Ray Microscopy III", Springer Series in Optical Sciences, Vol. 67, Springer-Verlag, Berlin, 1992.
2. K. Shinohara et al., "Fine structure of unstained human chromosome fibres dried with no fixative as observed by X-ray contact microscopy", J. Microscopy, 158, 335-342, 1990.
3. K. Shinohara et al., "X-ray contact microscopy of human chromosomes and human fibroblasts," in X-Ray Microscopy II, D. Sayre et al. Eds., Springer Series in Optical Sciences, Vol. 56, pp. 429-432, Springer-Verlag, Berlin, 1988.
4. K. Shinohara, "Observation of human chromosomes with soft X-ray contact microscopy", SPIE Proceedings, 1140, 196-200, 1989.
5. K. Shinohara et al., "A simple chamber for hydrated specimens in a vacuum and its application to X-ray contact microscopy with laser-produced plasma X-rays", in X-Ray Microscopy III, A. G. Michette, G. R. Morrison, and C. J. Buckley Eds., Springer Series in Optical Sciences, Vol. 67, pp. 347-349, Springer-Verlag, Berlin, 1992.
6. M. Richardson et al., "Pulsed X-ray microscopy of biological specimens with laser plasma sources", SPIE Proceedings, 1741, in press.
7. R. Kodama et al., "Soft X-ray emission from e_0 , $2e_0$, and $4e_0$ laser-produced plasmas", J. Appl. Phys., 59, 3050-3052, 1986.

Development of X-Ray microscopy systems based on laser plasma sources

Martin Richardson, Andrew Vasil'ev, Steven Grantham,
Kai Gabel, & Masataka Kado

Center for Research & Education in Optics & Lasers,
University of Central Florida, Orlando, FL 32826, USA.

ABSTRACT

We report progress in two areas of technology relevant to the development of high-resolution x-ray microscopy techniques based on laser plasma x-ray sources for the analysis of wet and dry biological specimens. The approach we discuss involves the use of ultrashort x-ray emission from a laser plasma source. Precision x-ray optics are used to collimate and filter this light onto the specimen. Imaging and image magnification are accomplished with a combination of x-ray and electron-optical systems. We discuss our progress towards establishing a flexible laser-plasma x-ray source for the development of biological imaging and contact microscopy, and progress we have made towards the development of an electro-optical imaging system having high magnification and spatial resolution.

1. Introduction.

X-ray microscopy in principle will avoid many of the limitations of present-day electron microscopy techniques for analyzing biological material. Principal among these are the small depth of field and the need to significantly treat samples (drying, dyeing, sectioning, coating etc.) before analysis. While being limited to the resolution in the 100Å range, the ability of x-ray microscopy to probe the internal structure of *in-vitro* assemblies provides biologists and life scientists the opportunity to observe complex features in their natural, even live state. Most x-ray microscope development has so far been made using large synchrotron sources. The latter limits x-ray microscopy to being primarily a limited research tool centered around a complex beam line located at a major synchrotron facility. The use of a laser-plasma x-ray source, however, makes plausible the development of a compact x-ray microscope having a size and cost comparable to a conventional electron microscope. We have previously discussed several approaches towards x-ray microscopy based on laser plasma x-ray sources¹. In this paper we describe progress we have made at the Laser Plasma Laboratory at CREOL towards constructing a flexible laser-plasma-based facility for the development of x-ray microscopy techniques, and the progress we have made in electron-optical image tube technology that will hasten the development a compact real-time imaging system for x-ray microscopy.


2. A laser-plasma x-ray source for the development of x-ray microscopy.

The primary advantages of a laser plasma x-ray source for x-ray microscopy system from it's compactness and flexibility. The spectral brightness of laser plasma x-ray sources can be comparable to the brightest available synchrotrons². Laser plasma x-ray sources have the advantage of being compact, moveable and tolerable of modest vacuum requirements. Compared to synchrotrons they are much cheaper to install and to operate. The x-ray emission spectrum of laser plasmas is rich in bright broad continuum emission and in narrow atomic emission lines,

and can easily be varied to suit specific microscopy needs. This selectivity in x-ray wavelength has a potential high dividend for x-ray microscopy in facilitating elemental analysis of features within biological structures by difference imaging with emission at two different wavelengths. Laser plasmas are point sources which can be highly reproducible, a requirement for precision x-ray optical systems having extremely high alignment specifications. Lastly pulsed laser plasmas introduce the time domain element into x-ray microscopy. Whereas exposure times for microscopy with synchrotrons are measured in seconds, laser plasmas can provide x-ray emission in pulses ranging from several nanoseconds duration to less than one picosecond. This introduces the possibility of capturing kinetic, chemical, or morphological changes in biological structures in time frames of interest to understanding complex biological processes. Moreover the influence of radiation damage on image reliability is avoided by using exposure times short enough to prevent the sample responding to the damaging radiations. No other source for x-ray microscopy can offer this capability.

Although many measurements of the x-ray emission from laser plasmas have been made in the spectral regions of interest for biological microscopy³⁻⁶, that is in the so-called 'water window' (2.3-4.4nm), and at other, element specific wavelengths., many of them have been made with laser and target characteristics more germane to other applications of laser plasmas. Moreover these studies have not had reason to consider the effects of plasma and particulate blowoff from the laser plasma, an important additional issue for microscopy, as it is for the use of laser-plasmas x-ray sources for lithography^{7,8} where the integrity of expensive x-ray optics in close proximity to the target must be preserved. At CREOL we have initiated a broad program of development of laser plasma x-ray sources for lithography and microscopy. This program includes addressing not only the efficient generation of x-ray emission at specific wavelengths, but also addressing the issues of target debris mitigation and inhibition, and the engineering issues associated with routine high repetition rate operation that are required for many of these applications. For x-ray microscopy of biological material, we have commenced a detailed study of optimum laser plasma conditions for constructing a source of x-rays in the water window and at shorter wavelengths. The laser system that we will use for these studies is shown in Fig. 1.

Fig.1. 700 MW solid state laser incorporating nonlinear wavefront correction by stimulated Brillouin scattering (SBS).

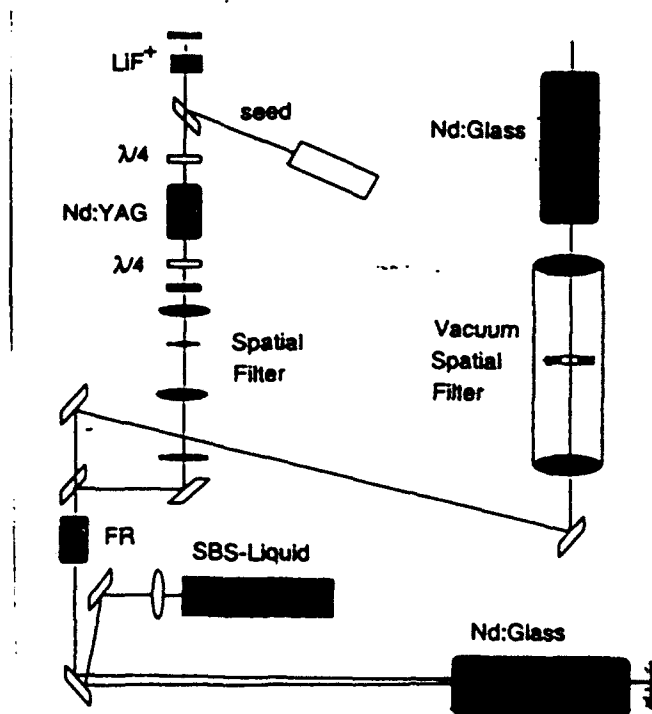

The laser incorporates an oscillator followed by several amplifier units in a fully imaged optical beamline. The Nd:YAG oscillator is Q-switched with a solid-state passive saturable absorber (LiF*)⁹, and is frequency injection locked with the output of a diode-pumped cw Nd:YAG laser. Its output consists of a 12 ns duration laser pulse in a diffraction limited beam of peak power 1 MW. The output of this laser is imaged-relayed through an air spatial filter to a four-pass amplifier which utilizes a Faraday rotator (FR) as the final output element. This amplifier stage also incorporates a phase-conjugation mirror which preserves the wavefront quality of the output of the oscillator as it passes through four consecutive passes of the 410 mm long Nd:glass amplifier. The 150 MW output of this amplifier is then relayed through a 1:1 vacuum spatial filter to a single-pass 16 mm diameter 410 mm long amplifier. The output of the laser has a peak power of up to 700 MW with a pulse duration of ~7 ns, the [pulse-shortening being due to the influence of of gain saturation and the nonlinearity of the phase conjugation mirror¹⁰

Experiments will be carried out in the experimental chamber shown in Fig.2. The laser beam is focused onto targets with a $f = 14$ cm focal length lens, producing intensities in the range $1 \times 10^{12} - 5 \times 10^{13}$ W/cm². Biological samples are exposed to x-rays from the target by encapsulating them in a hydrated cell of the type shown in Fig.2(b), situated 2 cm from the target. an array of x-ray diagnostic instrumentation including x-ray diodes, an x-ray crystal spectrograph, an x-ray pinhole camera and a flat field grating spectrograph is used to characterize the x-ray radiation.

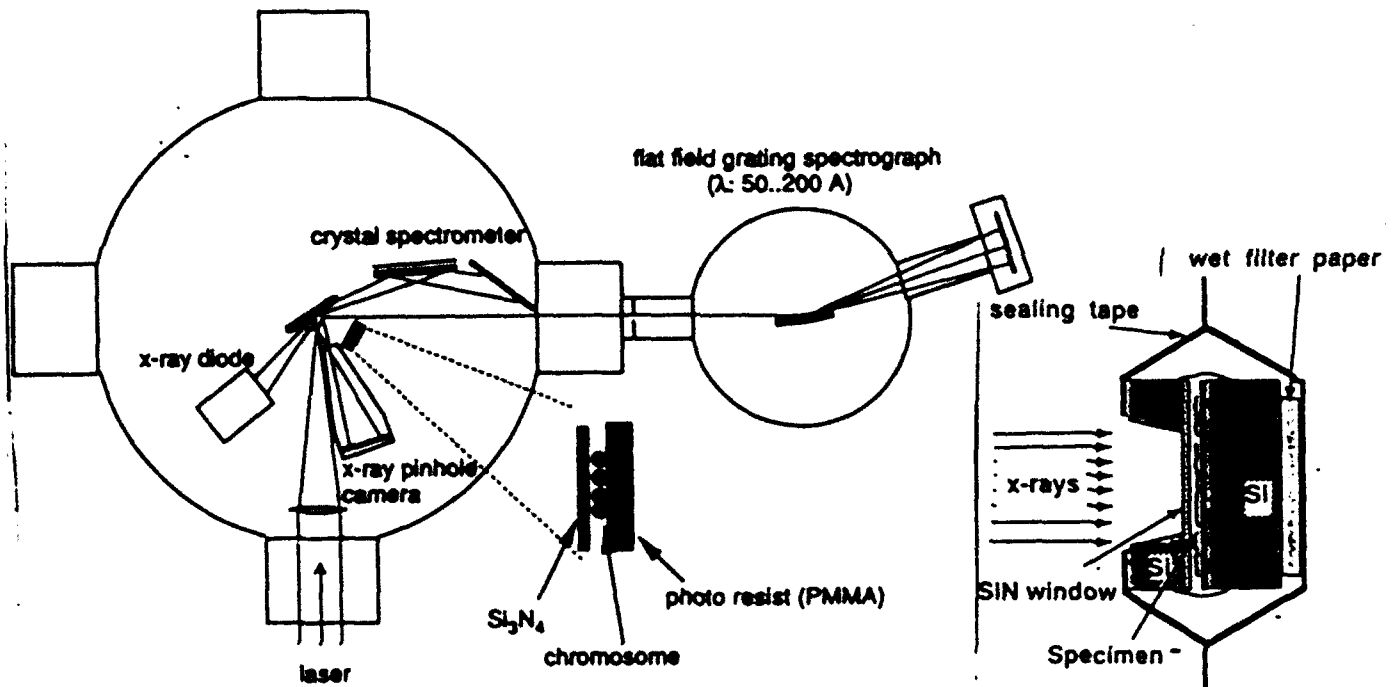


Fig.2. (a) Experimental set up used for initial biological x-ray microscopy experiments at CREOL. (b) Hydrated cell for exposing biological material for contact imaging.

3. A high resolution, high magnification electron-optical x-ray imaging system.

In determining the specifications of x-ray optical components in a laser plasma-based x-ray microscope, we first establish the primary performance requirements of the overall system. We assume that the required resolution must be in the range of current imaging capabilities, ~50nm. This resolution, or better, has been demonstrated with Fresnel zone-plate imaging^{11,12}, contact imaging^{13,14}, and, at longer wavelengths, with normal incidence reflective optical imaging¹⁵. Moreover we assume that the system must be capable of real-time image acquisition.

Current advanced image array detectors have pixel sizes in the $6\mu\text{m}$ range. Assuming a minimum image contrast ratio of ~ 10 , this implies the need for an overall image magnification of 10^3 - 10^4 . This level of image magnification cannot easily be met with x-ray optics alone. Although most x-ray microscopes today rely primarily on optical elements having modest image magnification and long-time image processing of an image recorded on resist, film, or through image scanning, the optimum microscope will require real-time image acquisition and thus will incorporate a combination of x-ray image magnification and electron-optical image magnification. Such a system is shown schematically in fig. 3. The specimen to be analyzed will be irradiated with monochromatic radiation from the laser plasma source. This could be facilitated by either a normal incidence multilayer mirror collector or a zone-plate condenser. An image of the specimen in the backlit radiation is then created with either a Schwarzschild microscope or Fresnel lens with a magnification (20-50) commensurate with the cathode resolution capability of an electron-optical image magnifier such as an x-ray-sensitive zoomtube¹⁶ or an x-ray photoelectron microscope^{17,18}. A zoomtube having an image magnification of 40-200 and a cathode resolution of $\sim 1\mu\text{m}$ has already been demonstrated¹⁶. Moreover, a photoelectron microscope having a resolution of $0.1\mu\text{m}$ and a magnification of 1200 should be developed in the near future¹⁹. At some loss in resolution, but with considerable gain in sensitivity and simplicity, the latter could be used in a simple contact or 'proximity' imaging mode.

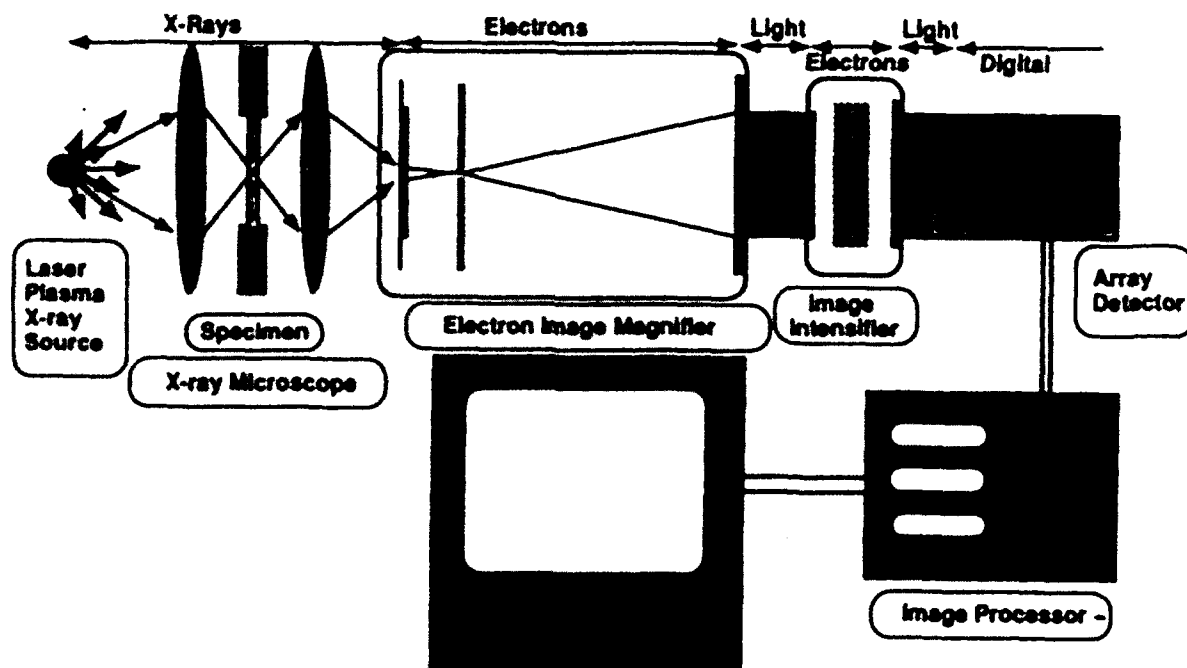


Fig.3 Possible structure of an x-ray - photoelectron-optical microscope.

An electron-optical image magnification tube of the type shown in Fig.3. is currently being built at the National Institute for Standards and Technology (NIST) for use with the SURF II synchrotron light source in a microscope for the observation of masks made for the optical alignments of soft x-ray lithography systems²⁰. We are participating in this development by developing the high resolution soft x-ray photocathodes required for this system. These photocathodes must resolve features of $0.1\mu\text{m}$ at a wavelength of 13.5nm . We have therefore assembled at the Laser Plasma Laboratory at CREOL a dedicated x-ray photocathode fabrication

facility for the development of efficient x-ray photocathodes for high resolution electron-optical systems. We have also tested some of these new types of photocathodes on a calibrated beamline of SURF II²¹. Fig.4 shows the photo-emissive yield in electrons/photon in the wavelength range adopted for the NIST Conversion Microscope for a number of photocathode materials.

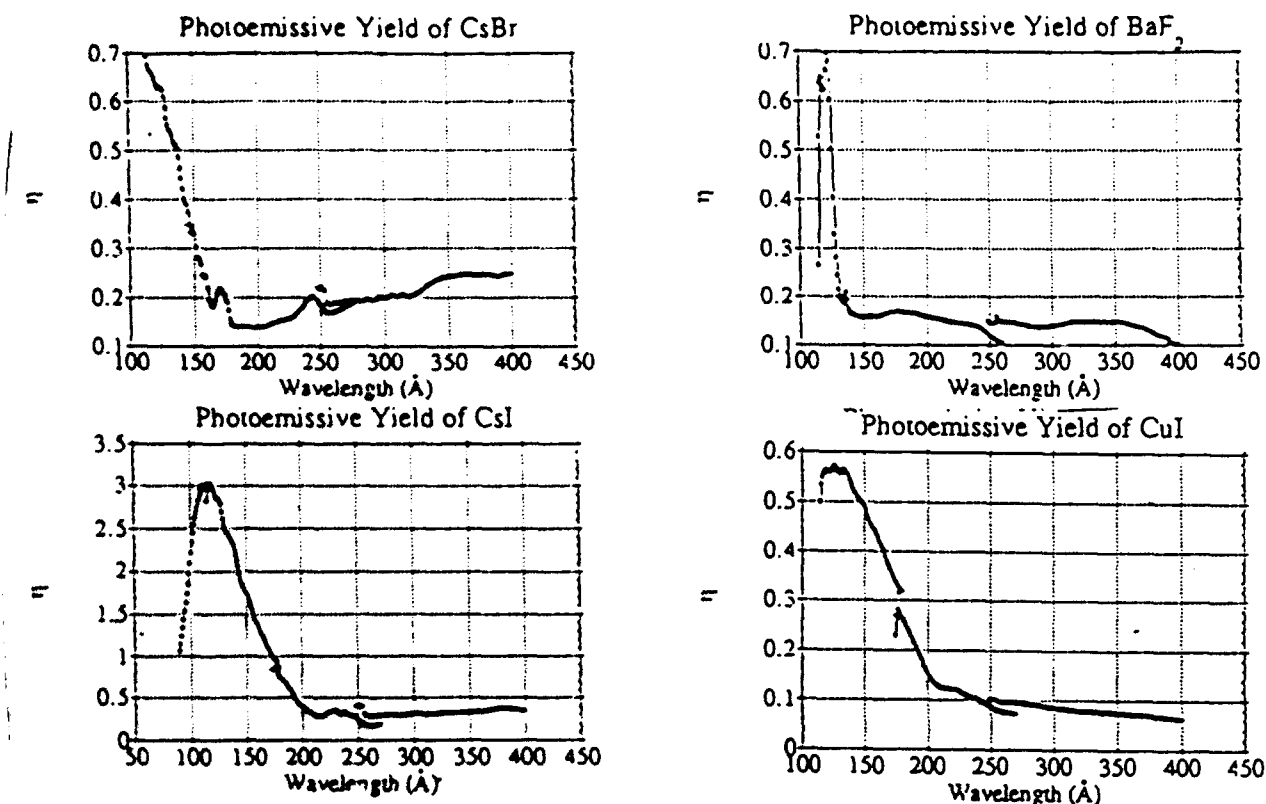


Fig. 4 Photoemissive yields of various photocathodes as measured on SURF II.

We intend to adapt the design of this electron-optical imaging system for applications to biological imaging. Although the electron optical imaging system will remain the same, we will develop new x-ray photocathodes for the water window and shorter wavelengths.

4. Summary

We have presented in this paper the progress we have made toward the development of x-ray microscope technology based on laser plasma point x-ray sources. We have established at the Laser Plasma Laboratory at CREOL a solid state laser system dedicated to the development of optimum point sources for biological x-ray microscopy. This source is currently being used to make progress in the use of contact microscopic techniques, and will also soon be used for advanced x-ray imaging systems incorporating multilayer coated Schwarzschild optics and high resolution zone plates. Towards the development of high resolution, high magnification electron-optical imaging systems for x-ray imaging applications we have established a dedicated x-ray photocathode fabrication facility and wish soon to adapt electron-optical designs of the soft x-ray conversion microscope at NIST for a similar instrument sensitive for x-rays in the water window and of shorter wavelength. These developments will bring closer the realization of a compact real-time x-ray imaging microscope for the biological and life sciences.

5. Acknowledgments

The authors wish to thank Prof. Karl Guenther of CREOL for his helpful support, and J. Darnell and P. Reese for their technical support. They also gratefully acknowledge the close collaboration of colleagues at NIST, especially Drs. T. Lucatorto, R. Watts, C. Tarrío and F. Pollack, and collaborations with Drs K. Shinohara and Y. Kinjo, and Prof. K. Tanaka.

This work was supported in part by US Air Force Office of Scientific Research under contract #F49620-93-1-0148. K. Gabel is supported in part by the Deutsche Forschungsgemeinschaft (DFG), and M. Kado is supported in part by the Japanese Society for the Promotion of Science.

6. References.

1. M. Richardson, K. Shinohara, K. Tanaka, Y. Kinjo, N. Ikeda & M. Kado, *Proc. SPIE* 1741, (1992)
2. N.M. Ceglio *J. X-Ray Sci. & Tech.* 1, 1 (1990)
3. P. D. Goldstone, S. R. Goldman, W. C. Mead, J. A. Cobble, G. Stradling, R. H. Day, A. Hauer, M. C. Richardson, R. S. Marjoribanks, P. A. Jaanimagi, R. L. Keck, F. J. Marshall, W. Seka, O. Barnouin, B. Yaakobi & S. A. Letzring. *Phys. Rev. Lett.* 59, 56-59 (1987)
4. K. Eidmann & T. Kishimoto, *Appl. Phys. Lett.* 49, 377 (1986)
5. R. Kodama, K. Okada, N. Ikeda, M. Mineo, K. A. Tanaka, T. Mochizuki & C. Yamanaka, *J. Appl. Phys.* 59, 3050, (1986)
6. K. A. Tanaka, H. Aritome, T. Kanabe, M. Nakatsuka, T. Yamanaka & S. Nakai, *Proc SPIE*. 1140, 350, (1989)
7. M. C. Richardson, W. T. Silfvast, H. Bender, A. Hanzo, V. Yanovsky, F. Jin & J. Thorpe, *Appl. Opt.* (to be published)
8. F. Bijkerk, E. L. Marnix, J. van der Wiel, E. C. I. Turcu, G. J. Tallents & D. Batani, *J. X-Ray Sci. & Tech.* 3, 133, (1992)
9. A. F. Vasi'ev, S. B. Gladin & V. E. Yashin, *Sov. J. Quant. Electr.* 21(5), 494, (1991)
10. A. F. Vasi'ev, V. V. Krainov & V. E. Yashin, *Sov. J. Quant. Electr.* 20(2), 140, (1990)
11. B. Niemann, *X-ray Microscopy III* (Ed A. G. Michette, G. R. Morrison & C. J. Buckley), Springer Verlag (Berlin), p142, (1992)
12. W. Meyer-Ilse, P. A. Guttmann, J. Thieme, D. Rudolph, G. Schmahl, E. Anderson,, P. Batson, D. Attwood, N. Iskander & D. Kern, *X-ray Microscopy III* (Ed. A. G. Michette, G. R. Morrison & C. J. Buckley), Springer Verlag (Berlin), p284, (1992)
13. K. Shinohara, *X-Ray Microscopy in Biology and Medicine*, (Ed. K. Shinohara, K. Yada, H. Kihara, & T. Saito) Publ. Springer Verlag, p203, (1990)
14. K. Shinohara, Y. Kinjo, M. C. Richardson, A. Ito, N. Morimoto, Y. Horiiko, M. Watanabe, K. Yada & K. A. Tanaka, *Proc. SPIE* 1741, (1992), this volume.
15. D. W. Berreman, J. E. Bjorkholm, L. Eichner, R. R. Freeman, T. E. Jewel, W. M. Mansfield, A. A. MacDowell, M. L. O'Malley, E. L. Raab, W. T. Silfvast, L. H. Szeto, D. M. Tennant, W. K. Waskiewicz, D. L. White, D. L. Windt, O. R. Wood II & J. H. Brunning, *Opt. Lett.* 15, 529 (1990)
16. K. Kinoshita, T. Matsumura, Y. Inagaki, N. Hirai, M. Sugiyama, H. Kihara, N. Watanabe, Y. Shimanuki & A. Yagashita, *X-ray Microscopy III* (Ed. A. G. Michette, G. R. Morrison & C. J. Buckley), Springer Verlag (Berlin), p335, (1992)
17. W. Engel, M. E. Kordesch, H. H. Rotermund, S. Kubala & A. von Oetzen, *Ultramicroscopy*, 36, 148 (1991)
18. G. F. Rempfer, W. P. Skoczylas & O. H. Griffith, *Ultramicroscopy*, 36, 196 (1991)
19. T. Lucatorto & R. N. Watts (private communication)
20. R. Watts (private communication)
21. S. Grantham, M Richardson, R. Watts, T. Lucatorto, C. Tarrío & F. Pollack, *Proc Spring Mtg. Mat. Res. Soc.* (1993). to be published.

Direct Imaging in a Water Layer of Human Chromosome Fibres Composed of Nucleosomes and Their Higher-Order Structures by Laser Plasma X-ray Contact Microscopy

Yasuhito Kinjo¹⁾, Kunio Shinohara²⁾, Atsushi Ito²⁾, Hisako Nakano²⁾, Makoto Watanabe¹⁾, Yasuhiro Horiike³⁾, Yukiko Kikuchi⁴⁾, Martin C. Richradson⁵⁾ and kazuo A. Tanaka⁶⁾

*Submitted to
Journal of Microscopy*

¹⁾ Radiation Biology Division, Tokyo Metropolitan Isotope Research Center, Setagaya, Tokyo 158, Japan, ²⁾ Department of Radiation Research, Tokyo Metropolitan Institute of Medical Science, Bunkyo, Tokyo 113, Japan, ³⁾ Department of Engineering, Hiroshima University, Higashi-Hiroshima, Hiroshima 724, Japan, ⁴⁾ Toshiba ULSI Research Center, Saiwai, Kawasaki 210, Japan, ⁵⁾ Center for Research in Electro-Optics and Lasers, University of Central Florida, Orlando, Florida 32826, U.S.A., and ⁶⁾ Department of Electro-magnetic Energy Engineering, Osaka University, Suita, Osaka 565, Japan

RUNNING TITLE: Imaging Hydrated Human Chromosome Fibres

KEY WORDS: laser-plasma X-rays, contact microscopy, hydrated human chromosome fibre, unfixed, unstained, nucleosome, superbead

ABSTRACT

X-ray contact microscopy with a 300 ps duration laser-plasma X-ray source has been used to image hydrated human chromosome fibres. Clearly imaged are individual nucleosomes and their higher order particles (superbeads), elementary chromatin fibrils of ~ 30 nm in diameter and their higher order fibres of various sizes up to ~ 120 nm in diameter. The results demonstrate that X-ray microscopy is now capable of opening a new path of investigation into the detailed structures of hydrated chromosome fibres in their natural state.

INTRODUCTION

Soft X-ray microscopy has many potential advantages over other microscopies for the visualization of thick, hydrated biological specimens in the resolution range 10-100 nm such as ① better resolution than optical microscopy and ② higher penetration depth than electron microscopy (Kirz and Sayre, 1980). These advantages have lead to an increasing effort in X-ray microscope development, particularly in the last few years. Several approaches to high resolution imaging are now being tried, and have already demonstrated the potential of this new microscopy in visualizing different biological structures. These include the observation of proteoglycan (Panessa *et al.*, 1981), myosin filaments (Panessa-Warren, 1984), living platelets (Feder *et al.*, 1985) sea urchin sperms (Tomie *et al.*, 1991) and human chromosomes (Shinohara *et al.*, 1992a) by contact microscopy, midge polytene chromosomes by imaging zone plate microscopy (Guttmann *et al.*, 1992), and bean chromosomes by scanning zone plate microscopy (Williams *et al.*, 1992). The latter two methods have not demonstrated sufficient resolution yet to reveal the fine structures of chromatin fibres including nucleosomes.

Observing fine structures of chromosome and chromatin as intact as possible in a hydrated state is important for better understanding their organization and functions *in situ*. These functions may play a key role in various cellular

control mechanisms such as cell cycle progress, differentiation, radiation sensitivities and cell death.

Eukaryotic chromosomes are composed of chromatin fibers which themselves consist of unit structures (Watanabe *et al.*, 1990), nucleosomes of 10-15 nm in diameter (Langmore and Wooley, 1975; Oudet *et al.*, 1975) and superbeads of 15-50 nm in diameter (Hozier *et al.*, 1977; Azorin *et al.*, 1982; Zentgraf and Franke, 1984). Bordas *et al.* (Bordas *et al.*, 1986) have shown that the native uncondensed chromatin fibre in solution has an outer diameter of ~30 nm using synchrotron radiation scattering analysis. Belmont *et al.* (Belmont *et al.*, 1987) have demonstrated that size hierarchy of discrete chromatin structural domains with cross-sectioned diameters of 120, 240, 400-500, and 800-1000 Å exist in mitotic chromosomes by the analyses of three dimensionally reconstructed electron microscopic images of isolated *Drosophila melanogaster* chromosomes. Nevertheless, the organization and functions of chromosomes or chromatin *in situ* have not been clarified yet.

In a previous publication (Shinohara *et al.*, 1990), we have described the first use of X-ray contact microscopy to observe the "beads-on-a-string" structures in human chromosome fibres. The chromosome fibres were as close to their natural state as possible. Namely, they were unstained without any fixative. However they were dried, and that the drying process in some way may have modified the fine structure of chromosome fibre. This possible limitation is overcome in the study of hydrated specimens.

For the observation of hydrated biological specimens at a high resolution the exposure time should be less than 1 ms to eliminate the image blurring caused by thermal diffusion and/or radiation damage (Shinohara and Ito, 1991; Ito and Shinohara, 1992). From this point of view a laser plasma X-ray source (Rosser *et al.*, 1985) is the most suitable for X-ray microscopy at the present time.

Laser-plasma X-ray sources have previously been used for a number of contact microscopy studies of biological specimens (Tomie *et al.*, 1991; Ford *et al.*,

1992; Cheng *et al.*, 1992) including our previous studies (Shinohara *et al.*, 1992a; Shinohara *et al.*, 1992b; Shinohara *et al.*, in press), in which natural hydrated human chromosome fibres were imaged with soft X-ray contact microscopy illuminated by a pulsed (300 ps), single burst of X-rays from a laser-plasma x-ray source. In the present work, we have precisely analysed the results obtained by the X-ray contact microscopy of human chromosome fibres in a water layer with laser produced plasma X-rays.

MATERIALS AND METHODS

Chromosome preparation in a hydrated specimen chamber

The chromosome specimens were prepared for X-ray imaging in the following way. Human lymphocytes (RPMI 1788) were incubated at 37 °C in RPMI 1640 medium supplemented with 10 % fetal bovine serum in the presence of 0.05 µg/ml colcemid for 16 hrs to accumulate mitotic cells. After centrifugation the cells pellet was placed on a clean surface of distilled water. At this moment the cells were broken, with the consequence that the chromosomes rapidly flowed out across a large surface area of the water. The chromosomes were then concentrated in density on the surface of the water by decreasing the surface area over which they could float. Finally, they were whole-mounted directly onto a thin layer of photoresist, polymethylmethacrylate (PMMA), supported on a 0.4 mm thick silicon wafer. The thickness of PMMA was 0.7 µm and the overall substrate size was about 7 mm × 7 mm.

The hydrated specimens without fixation and staining were then configured into a simple hydrated specimen chamber (Shinohara *et al.*, 1992b). This is shown schematically in Fig.1. This specimen chamber was assembled in the following way. After the hydrated chromosomes were mounted on the PMMA resist [Fig.1(a)], they were immediately covered with a thin (400 nm thick) SiN square (250 µm × 250 µm) window, ensuring that they were always maintained in a hydrated condition [Fig.1(b)]. The small SiN window had been chemically etched into a 0.4 mm thick Si wafer having approximate dimensions

of 7 mm × 7 mm. While still in a wet state, these two wafers were then press-fitted together using a torque gauge (1.2 kgf · cm) attached to a micrometer [Fig. 1 (c)]. Thus the chromosomes were encapsulated in a fully hydrated state. The excess water was removed with a piece of a filter paper, and the system was sealed with two pieces of adhesive tape (Scotch tape #483) as shown in Fig.1 (d). A small piece of wet filter paper was included on the rear of the specimen holder in order to verify that the specimen was still hydrated at the time of X-ray exposure. The final thickness of each water cell was in the 1-5 μm range, measured with an optical microscope. Specimen chambers constructed in this manner were found to be water-tight for many hours in a vacuum chamber.

X-ray exposure

The encapsulated human chromosomes were exposed to a single burst of X-rays from a laser-produced plasma. The plasma was created from solid Au targets by the focused second harmonic radiation (527 nm) converted from one beam of the four beam GEKKO IV Nd:glass laser system at the Institute of Laser Engineering at Osaka University. The 300 ps (FWHM) duration Gaussian output pulse of energy 26 J was focused in an evacuated target chamber (10^{-4} Torr) with a spot size of 100 μm in diameter on the Au target, providing an irradiating intensity of $\sim 10^{15}$ W/cm². The X-ray emission from Au targets under these irradiation conditions has been well-characterized (Kodama *et al.*, 1986). The specimen cell was situated 2 cm from the target at an angle of 25° to the laser axis and the target normal. Fig.2 shows the spectrum of X-ray flux from the plasma emitted in this direction and the spectrum of the X-rays irradiating the chromosomes taking account of the absorption of the SiN window (Henke *et al.*, 1982). The total photon flux irradiating the specimen was estimated to be $\sim 1.4 \cdot 10^{15}$ photons/cm² in the photon energy range of 250-1250 eV.

Development and Observation

After the exposure to the laser-plasma X-rays, the specimen chamber was

removed from the target chamber and was disassembled. The PMMA was then developed and teated in a procedure previously described (Shinohara *et al.*, 1986). Chromosomes were removed from the PMMA with sodium hypochlorite (chlorine concentration, 0.5%). Then the PMMA was developed with a mixture of metylisobutylketone and isopropanol. The three-dimensional topological representation in the PMMA of the absorption of the hydrated chromosome structure was then observed through the use of so-called "replica method" (Tanaka, 1983; Karasaki and Tanaka, 1984) and a transmission electron microscope(TEM). In the replica method the fine topological shape etched into the PMMA resist is transferred to a uniform-thickness film made of ethylene by plasma polymerization in a glow discharge. This structure can then be observed with a TEM.

RESULTS

Figs.3 and 4 show X-ray images of condensed chromosome fibres, and Figs.5 and 6 are images of partially decondensed chromosome fibres. The specimens were always in a hydrated condition during the exposure. In the replica method, the X-ray image from the TEM corresponds to the white lines covered with the black area(Shinohara *et a/.*, 1990). Pictures marked with letters b to f show enlarged images of the framed areas of the picture a in each figure. Usually the fibres were entangled three dimensionally in a complicated manner. However, wide variety of hierarchial organization of fibres and particles are observed: nucleosomes (arrowheads), superbeads (supranucleosomal particles; black arrows), superbeads clusters (white arrows), polynucleosome filaments (thin white arrows), " 30 nm" fibers (thick white arrows), and higher order fibres with the sizes of up to 100 nm or more in diameter (Large and thick white arrows). In most images of the higher order structures, nucleosomes are identified as components. In Fig. 3(b) and Figs. 6(c,e), superbeads and the clusters of them are apparently composed of multiple nucleosomes in a " moluroid organization (Zentgraf and Franke, 1984) " The mean diameters of

nucleosomes and superbeads at various portions were estimated to be 12.4 ± 1.8 (n=25) and 33.6 ± 8.3 (n=35) nm, respectively. The values correspond well with those estimated for dried specimens (Shinohara *et al.*, 1990). Series of nucleosomes are considered to be polynucleosome filaments (Figs. 3(c,d), 4(b) and 5(d)), though internucleosomal linker DNA (2 nm in diameter) is not identified because of resolution limit of the technique. 30nm fibres are seen in Figs. 3(d), 4(b), 5(c,e), and 6(b,d) where nucleosome- and/or superbead-sized particles are apparent. In one case (Fig.5(e)), the fibre is constructed with regularly arranged two parallel rows of nucleosomes (thick white arrow). Higher order fibres constructed with 30 nm fibres are seen in Figs.5(b) and 6(b,e). In Figs. 6(b,d), fibres with diameters of ≥ 30 nm coil helically into thicker (60-120 nm in diameter) fibres (framed by the rectangles and the illustrations of those fibres are shown in the column of each picture). Another example of a helical coil is observed in Fig.5(b). In this case, however, the fibre coils so tightly that it is hard to estimate the internal structures.

DISCUSSION

In the present study we have succeeded in observing fine structures of human chromosome fibres in a hydrated condition by X-ray contact microscopy with the aid of laser produced plasma X-rays. The data revealed wide variety of hierarchical organization of chromosome fibres, which are fundamentally compatible with previous data (Langmore and Wooley, 1975; Oudet *et al.*, 1975; Hozier *et al.*, 1977; Azorin *et al.*, 1982; Zentgraf and Franke, 1984; Bordas *et al.*, 1986; Belmont *et al.*, 1987; Shinohara *et al.*, 1990). One of those examples is "moruloid" organization of superbeads with nucleosomes which was reported by Zentgraf and Franke (Zentgraf and Franke, 1984) using conventional electron microscopy with fixation and staining. The present study presented the first example to demonstrate such structure of unfixed, unstained and hydrated chromosome fibres. Since the chromosome fibres were spread over the surface of

distilled water, there remains some uncertainty on the relationship between the present observation of the hierarchical organization of chromosome fibres and those of *in situ* natural structures for the following reasons: ① The surface tension may stretch some of the chromosomes from their natural state; ② Ionic environment at the preparation may modify the extent of packing tightness of nucleosomes into superbeads also from their natural state.

Nevertheless, it should be emphasized that the current technique used in this study is capable of observing wide variety of hierarchical organization of chromosome fibers neither fixed nor stained in a hydrated condition with the highest resolution of 10 nm. It has been discussed in detail elsewhere (Shinohara *et al.*, in press) that X-ray contact microscopy is applicable to image hydrated biological specimens at the resolution of 10 nm circumventing the possible factors of artefacts such as radiation damage, thermal diffusion, thermal expansion, temperature increase and the effect of free radicals produced in water.

In summary, we have shown that the direct imaging of wide variety of hierarchical organization in hydrated chromosome fibres is now possible with X-ray microscopy with the resolution up to 10 nm. This accomplishment will introduce a new form of high resolution imaging to biology. By accumulating data from images of condensed and decondensed chromatin fibres *in situ* in their natural state, much useful information can be obtained on the organization and on the regulation of the function of chromosomes. In addition, in the future, the use of coherent X-ray from pulsed X-ray lasers and X-ray holographic techniques will provide three dimensional images, from which detailed information on the higher configuration of nucleosomes can be obtained.

ACKNOWLEDGEMENTS

We would like to thank the invaluable technical assistances by T. Sakamoto, H. Sugio, and Y. Hagiwara to operate the GEKKO III beam system. One of the

authors (M. C. Richardson) was supported by the Japan Society for the Promotion of Science to conduct this study.

REFERENCES

- Azorin, F., Perez-Glau, L. & Subirana, J. A. (1982) Supranucleosomal organization of chromatin: electron microscopic visualization of long polynucleosomal chains. *Chromosoma*, 85, 251-260
- Belmont, A. S., Sedat, J. W. & Agard, D. A. (1987) A three-dimensional approach to mitotic chromosome structure : evidence for a complex hierarchical organization. *J. Cell Biol.* 105, 77-92
- Bordas, J., Perez-Grau, L., Koch, M. H. J., Vega, M. C. & Nave, C. (1986) The superstructure of chromatin and its condensation mechanism. I. Synchrotron radiation X-ray scattering results. *Eur. Biophys. J.* 13, 157-173
- Cheng, P. C., Kim, H. G. & Lin, T. H. (1992) The study of silica deposition in the leaf blade of *zea mays* L. by X-ray contact microradiography and confocal microscopy, X-Ray Microscopy III (ed. by A. Michette, G. Morrison, and C. Buckley) pp. 417-422. Springer Series in Optical Sciences Vol. 67, Springer-Verlag, Berlin Heidelberg
- Feder, R., Banton, V., Sayre, D., Costa, J., Baldini, M. & Kim, B. (1985) Direct imaging of live human platelets by flash X-ray microscopy. *Science*, 227, 63-64.
- Ford, T. W., Stead, A. D. & Page, A. M. (1992) Development of soft X-ray contact microscopy using laser-produced plasmas. X-Ray Microscopy III (ed. by A. Michette, G. Morrison, and C. Buckley), pp. 438-441. Springer Series in Optical Sciences Vol. 67, Springer-Verlag, Berlin Heidelberg
- Guttman, P., Schneider, G., Robert-Nicoud, M., Niemann, B., Rudolph, D., Thieme, J., Jovin, T. M. & Schmahl, G. (1992) X-ray microscopy investigations on polytene chromosomes isolated from salivary glands of *Chironomus thummi* larvae. X-Ray Microscopy III (ed. by A. Michette, G. Morrison, and C. Buckley), pp. 404-407. Springer Series in Optical Sciences Vol. 67, Springer-Verlag, Berlin Heidelberg
- Henke, B. L., Lee, P., Tanaka, T. J., Shimabukuro, R. L. & Fujikawa, B. K. (1982) Low-energy X-ray interaction coefficients: Photoabsorption, scattering, and reflection. *Atomic Data and Nuclear Data Tables*, 27, 1-144.

- Hozier, J., Renz, M. & Nehls, P. (1977) The chromosome fiber: evidence for an ordered superstructure of nucleosomes. *Chromosoma*, 62, 301-317
- Ito, A. & Shinohara, K. (1992) Image blurring by thermal diffusion in the observation of hydrated biomolecules with soft X-ray microscopy. *Cell Structure and Function* 17, 209-212.
- Karasaki, S. & Tanaka, A. (1984) Surface-replica cytochemistry as a tool for studying cell-surface enzyme activity : membrane ecto-ATPase localization in liver cell culture. *J. Electron Microsc. Tech.* 1, 289-298
- Kirz, J. & Sayre, D. (1980) Soft X-ray microscopy of biological specimens. *Synchrotron Radiation Research* (ed. by H. Winick and S. Doniach), pp. 277-322. Plenum Press, New York.
- Kodama, R., Ikeda, N., Mineo, M., Tanaka, K. A., Mochizuki, T. & Yamanaka, C. (1986) Soft X-ray emission from ω_0 , $2\omega_0$, and $4\omega_0$ laser-produced plasmas. *J. Appl. Phys.* 59, 3050-3052.
- Langmore, J. P. & Wooley, J. C. (1975) Chromatin architecture : investigation of a subunit of chromatin by dark field electron microscopy. *Proc. Natl. Acad. Sci. U. S. A.* 72, 2691-2695.
- Oudet, P., Gross-Bellard, M. & Chambon, P. (1975) Electron microscopic and biochemical evidence that chromatin structure is a repeating unit. *Cell*, 4, 281-300
- Panessa, B. J., McCorcle, R. A., Hoffman, P., Warren, J. B. & Coleman, G. (1981) Ultrastructure of hydrated proteoglycans using a pulsed plasma source. *Ultramicroscopy*, 6, 139-148.
- Panessa-Warren, B. J. (1984) Biological applications of X-ray contact microscopy. *X-Ray Microscopy* (ed. by G. Schmahl and D. Rudolph), pp. 268-278. Springer Series in Optical Sciences Vol. 43, Springer-Verlag, Berlin
- Rosser, R. J., Baldwin, K. G., Feder, R., Basset, D., Coles, A. & Eason, R. W. (1985) Soft X-ray contact microscopy with nanosecond exposure times. *J. Microsc.* 138, 311-319.
- Shinohara, K., Ito, A., Kinjo, Y., Watanabe, M., Kikuchi, K. & Tanaka, L. A. (1992a) A simple

- chamber for hydrated specimens in a vacuum and its application to X-ray contact microscopy with laser-produced plasma X-rays. *X-Ray Microscopy III*, (ed. by A. Michette, G. Morrison, and C. Buckley), pp. 347-349. Springer Series in Optical Sciences Vol. 67, Springer-Verlag, Berlin Heidelberg.
- Shinohara, K., Nakano H., Kinjo, Y. & Watanabe, M. (1990) Fine structure of unstained human chromosome fibres dried with no fixative as observed by X-ray contact microscopy. *J. Microsc.* 158, 335-342.
- Shinohara, K. & Ito, A. (1990) Radiation damage in soft X-ray microscopy of live mammalian cells. *J. Microsc.* 161, 463-472.
- Shinohara, K., Kinjo, Y., Richardson, M. C., Ito, A., Morimoto, N., Horiike, Y., Watanabe, M., Yada, K. & Tanaka, K. A. (1992b) Observation of human chromosome fibres in a water layer by laser-plasma X-ray contact microscopy. *SPIE Proceedings*, 1741, 386-392.
- Shinohara, K., Ito, A. & Kinjo, Y. (in press) X-ray microscopy of biological specimens with laser plasma X-rays. *SPIE Proceedings*, 2015.
- shinohara, K., Aoki, S., Yanagihara, M., Yagishita, A., Iguchi, Y. & Tanaka, A. (1986) A new approach to the observation of the resist in X-ray contact microscopy. *Photochem. Photobiol.* 44, 401-403
- Tanaka, A. (1983) A new replica method for electron microscopic studies with plasma polymerization-film in a glow discharge. *Seikagaku* (in Japanese), 55 1212-1219
- Tomie, T., Shimizu, H., Majima, T., Yamada, M., Kanayama, T., Kondo, H., Yano, M. & Ono, M. (1991) Three-dimensional readout of flash X-ray images of living sperm in water by atomic-force microscopy. *Science*, 252, 691-693.
- Watanabe, M., Kinjo, Y., & Shinohara, K. (1990) Observation of human chromosomes by X-ray microscopy in comparison with electron microscopy. *X-Ray Microscopy in Biology and Medicine* (ed. by K. Shinohara, K. Yada, H. Kihara, and T. Saito) pp. 295-304. Japan Scientific Societies Press, Tokyo/Springer-Verlag, Berlin.
- Williams, S., Jacobson, C., Kirz, J. Lamm, S & Van't Hoff J. (1992) Scanning transmission X-ray microscopy of hydrated mitotic chromosomes. *X-Ray*

Microscopy III (ed. by A.G. Michette, G.R. Morrison, and C. Buckley), pp. 408-412
Springer Series in Optical Sciences Vol. 67, Springer-Verlag, Berlin
Heidelberg.


Zentgraf, H. & Franke, W. (1984) Differences of Supernucleosomal Organization in
Different Kinds of Chromatin: Cell Type-Specific Globular Subunits
Containing Different Numbers of Nucleosomes. *J. Cell Sci.* 99, 272-286.

FIGURE LEGENDS


- Fig. 1. Experimental assembly of a simple hydrated chamber. The wet specimens isolated on a surface of distilled water were mounted on a layer of PMMA supported on a silicon wafer (a). The wet specimens were then covered with a SiN window (b) and press-fitted with a torque gauge (c). This wet assembly was then sealed with two pieces of adhesive tape, together with a piece of a wetted filter paper (d.).
- Fig. 2. Spectrum of the X-ray flux emitted from the laser produced plasma from Au target. The dotted line show the X-ray flux transmitted through the SiN window.
- Fig. 3. An X-ray image of a condensed chromosome fibre (a) and enlarged images of three specific regions identified by framed areas (b to d): b, a cluster of superbeads about 30 nm in diameter (white arrow) ; c, a polynucleosome filament in a series of nucleosomes (thin white arrow); and d, a 30 nm fibre constructed with a polynucleosome filament. Bars represent 1 μ m (a) and 100 nm (b-d), respectively.
- Fig. 4. Another example of a condensed chromosome fibre (a) and an enlarged image of a framed area (b): Polynucleosome filaments (thin white arrow) and a 30 nm fiber (short and thick white arrow) with tightly packed nucleosomes are evident. Bars represent 1 μ m (a) and 100 nm (b), respectively.
- Fig. 5. A partially decondensed chromosome fibre (a) and enlarged images of the framed areas (b to f): b, a higher order fibre (thick white arrow) with the size of 60-100 nm in diameter constructed with a helically coiling fibre; c, a knobby 30 nm fibre (small and thick white arrow) made up with superbeads ; d, a polynucleosome filament (thin white arrow); e, a 30 nm fibre with regularly arranged two rows of nucleosomes (white arrow), and f, a series of nucleosome and superbeads. Bars represent 1 μ m (a) and 100 nm (b-f), respectively.

Fig. 6. Another example of decondensed chromosome fibre (a) and the enlarged images of the framed areas (b to e): b, a higher order fibre (large white arrow) with a helically coiling 30 nm fibre (small white arrow); c. a cluster of superbeads (white arrow) ; d. a 30 nm fibre with tightly packed superbeads (small white arrow) and a higher order fibre of 60-120 nm in diameter (large and thick white arrow) made up with a coiling 30 nm fibre; and e, superbeads in a moruloid organization. Bars represent $1\mu\text{m}$ (a) and 100 nm (b-e), respectively.


a.

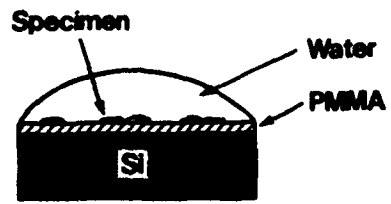

b.

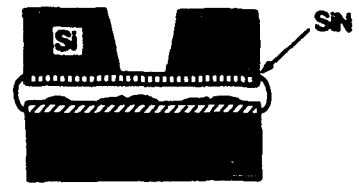

c.

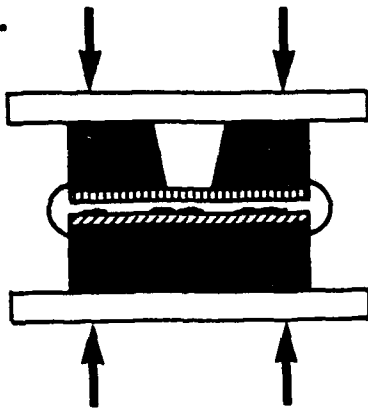

d.

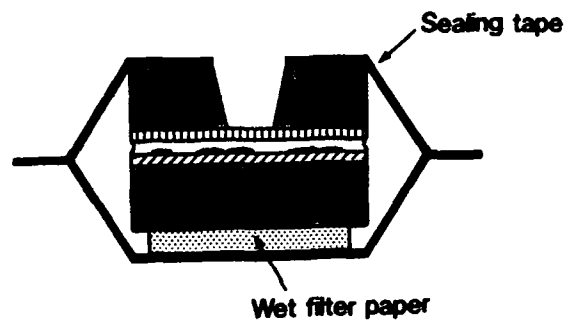


Fig.1

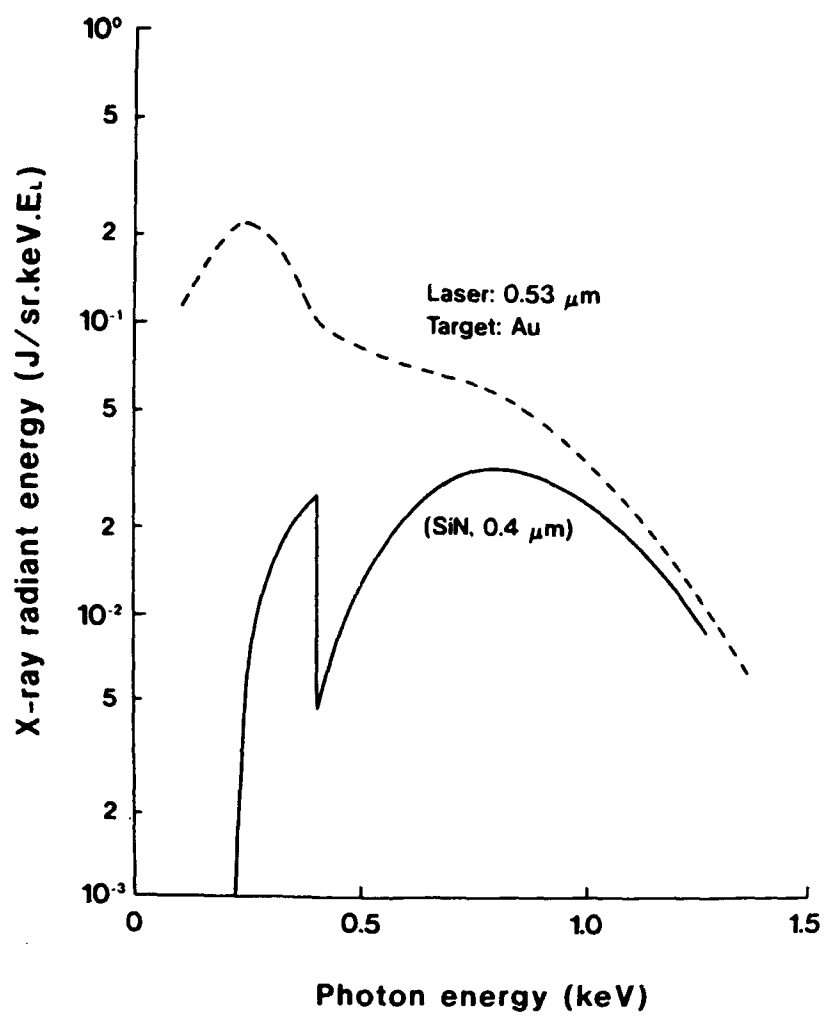


Fig. 2

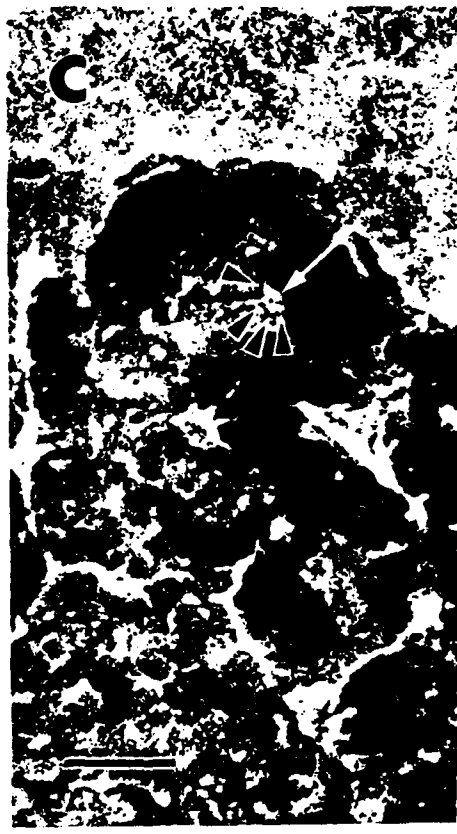
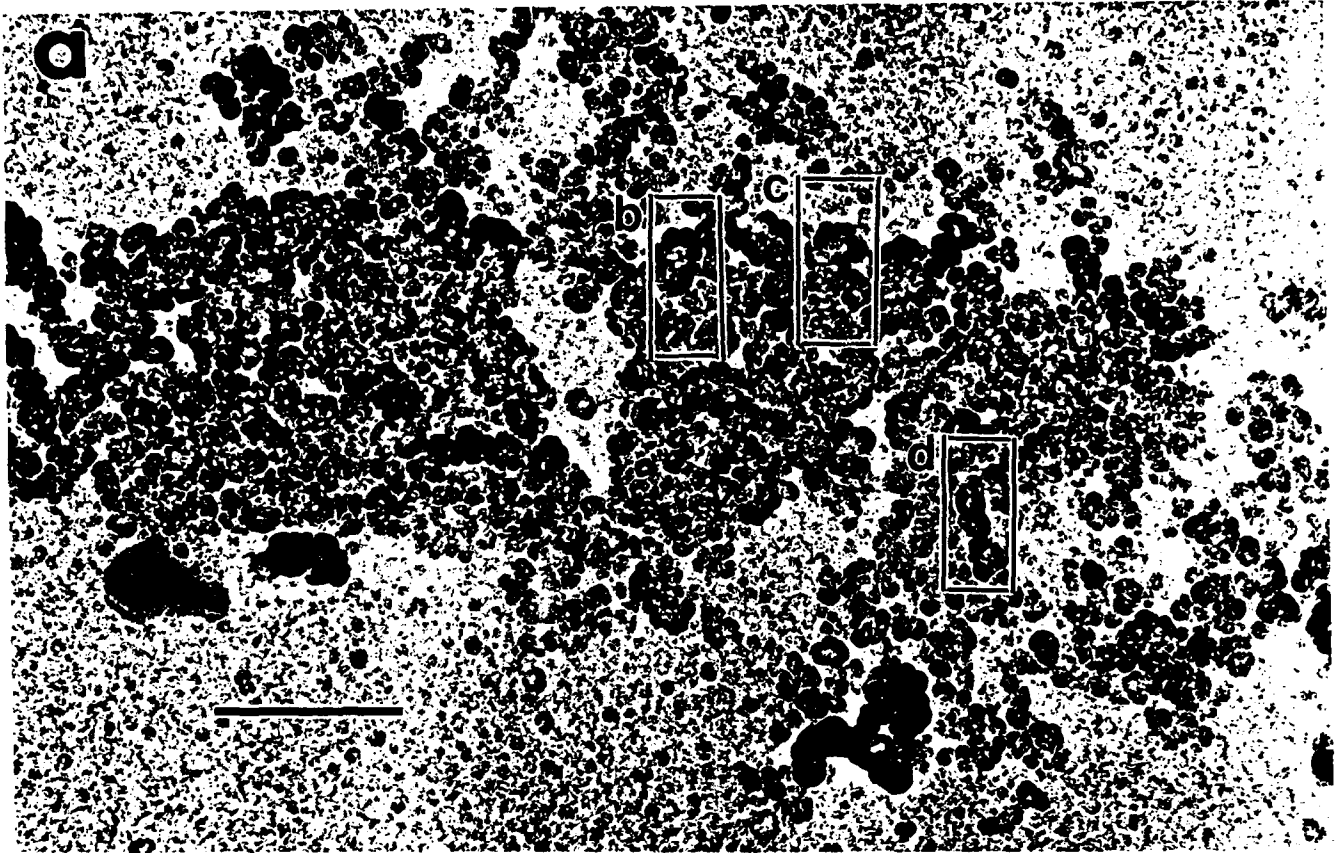


Fig. 3

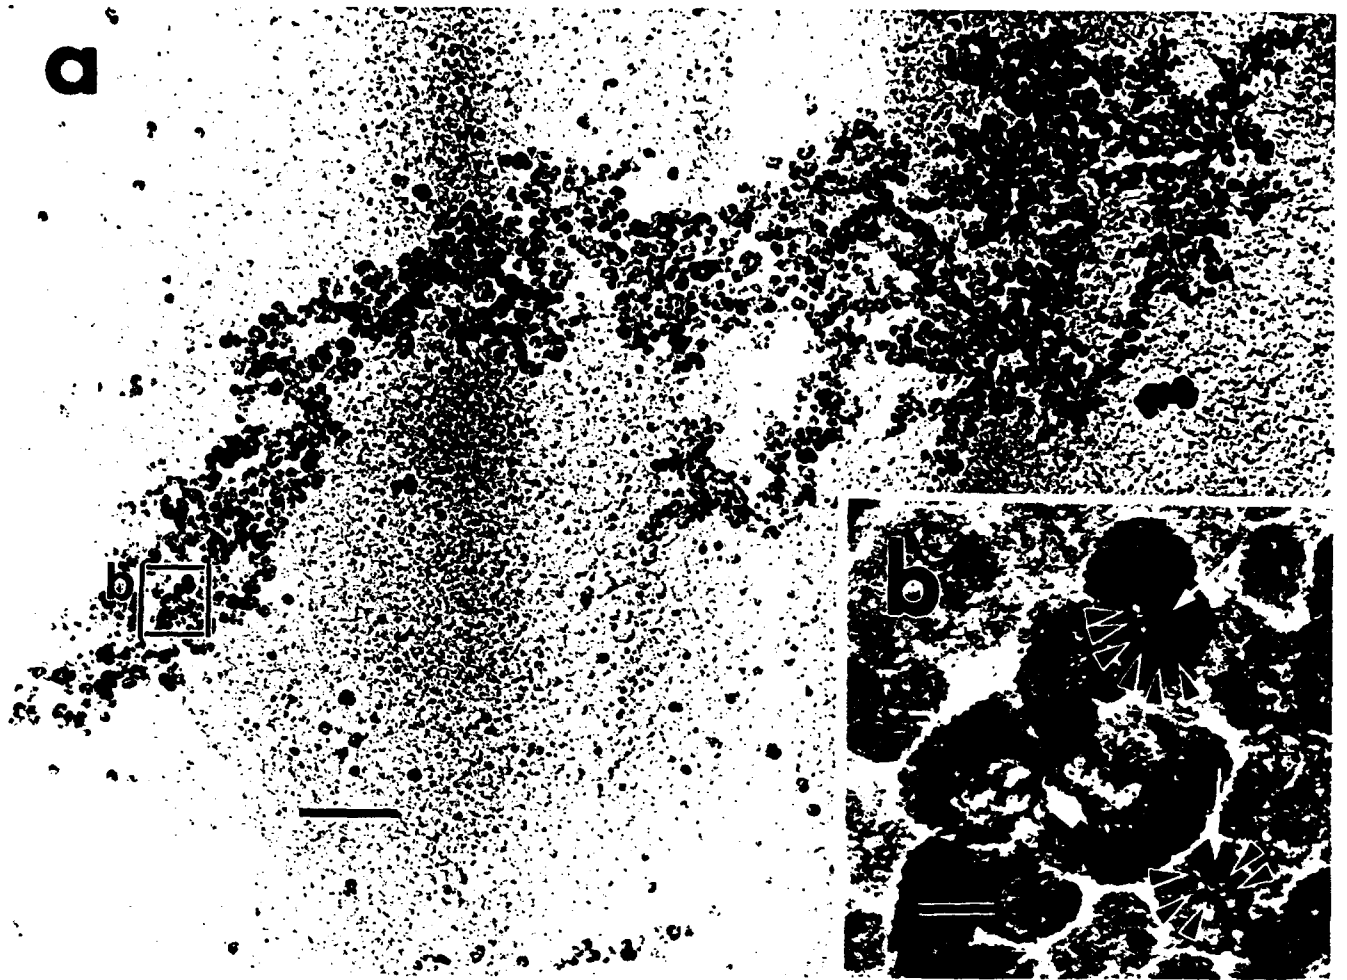


Fig. 4

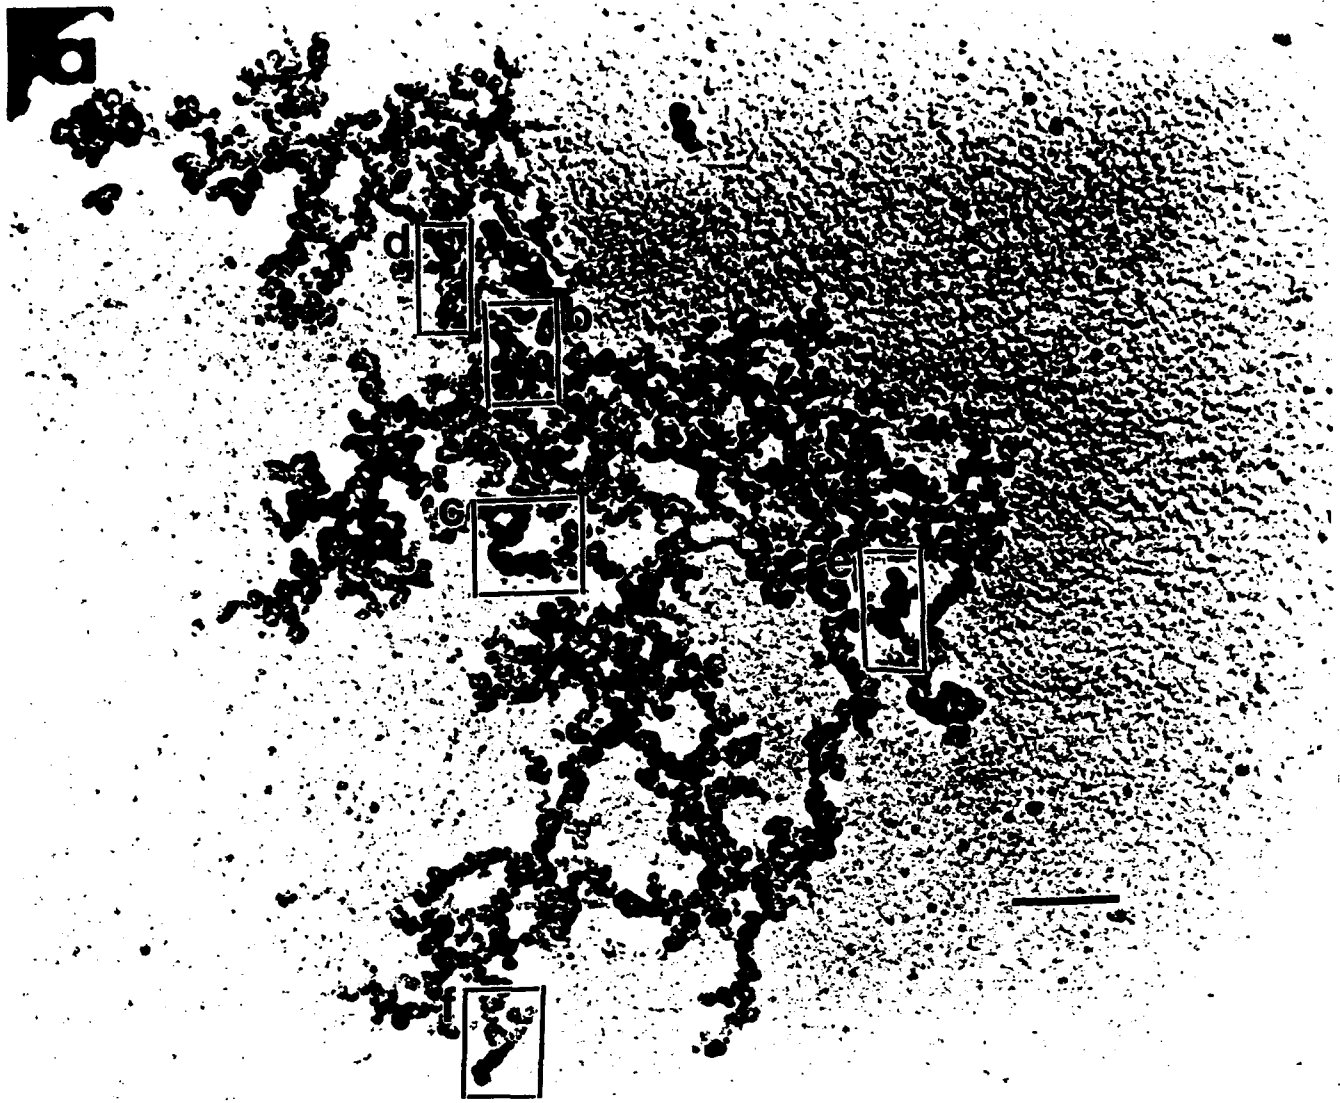


Fig. 5

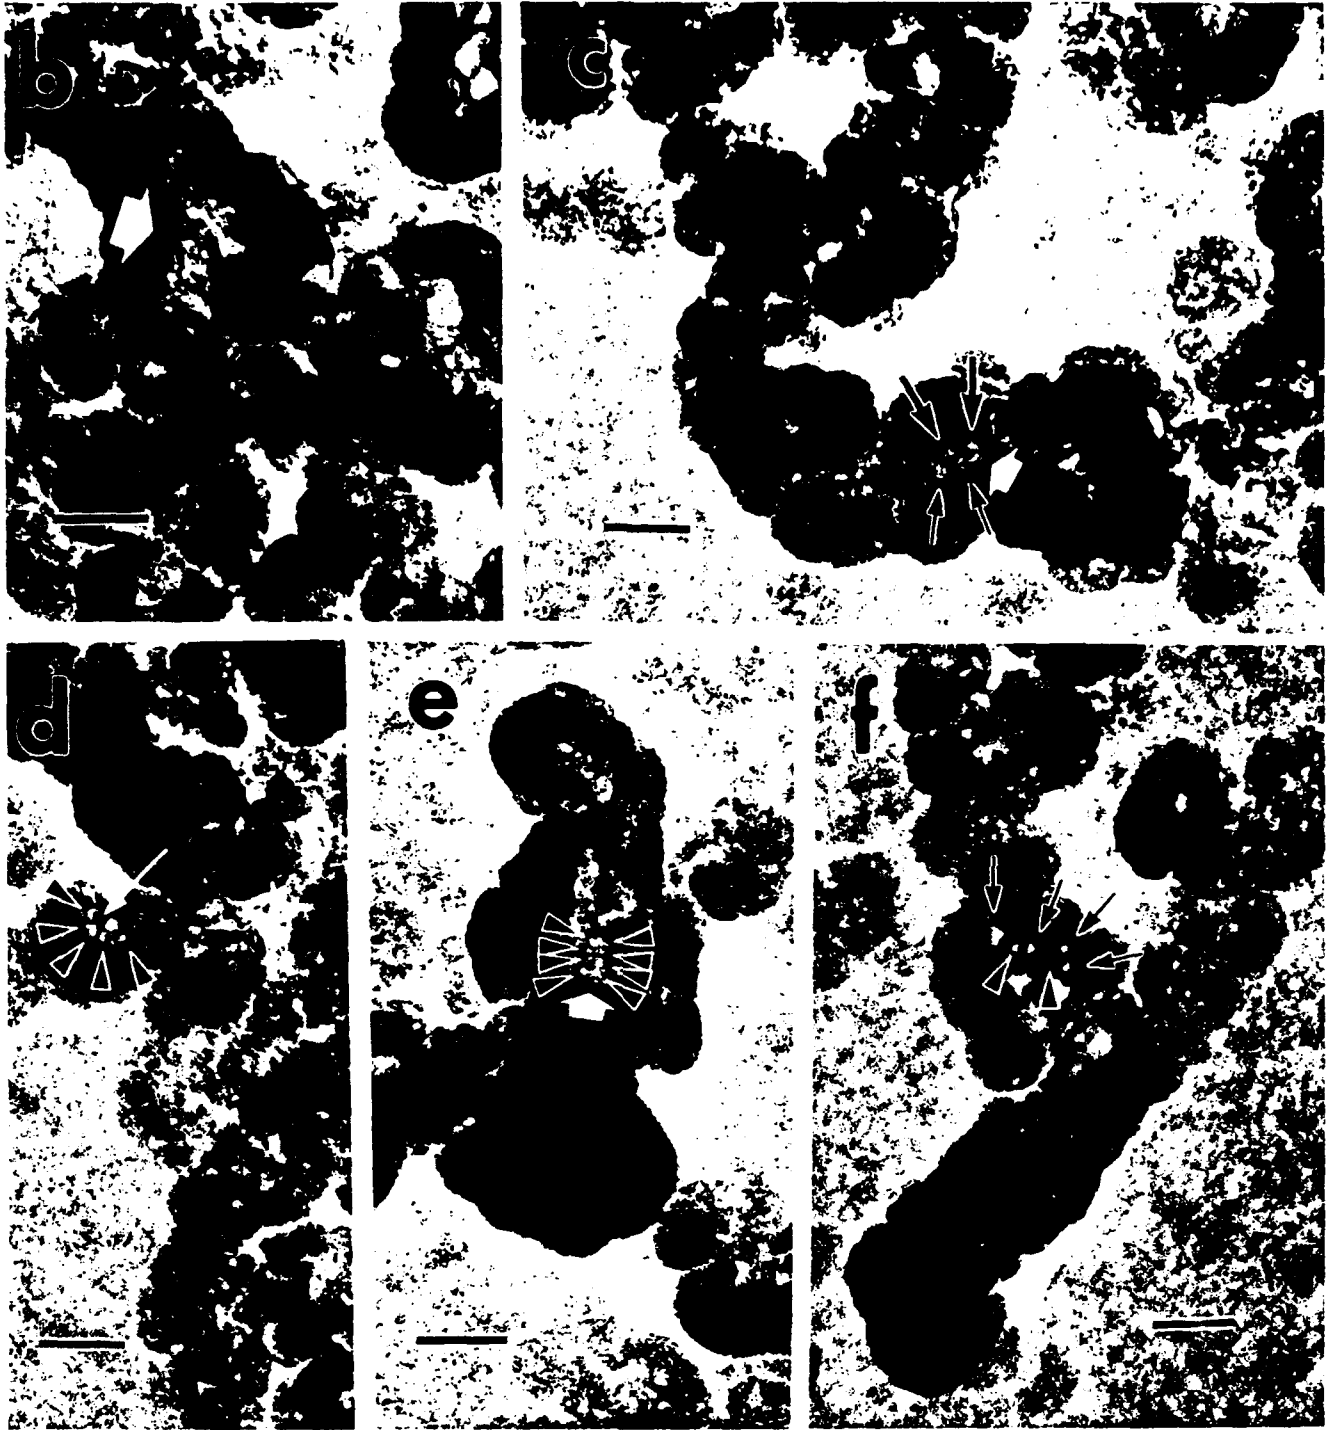


Fig. 5


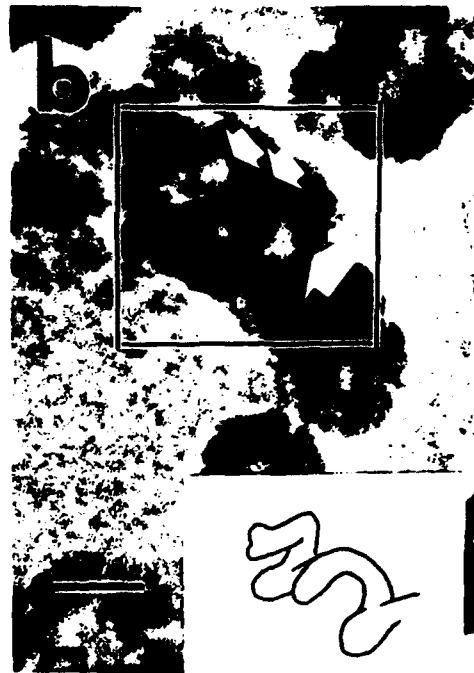
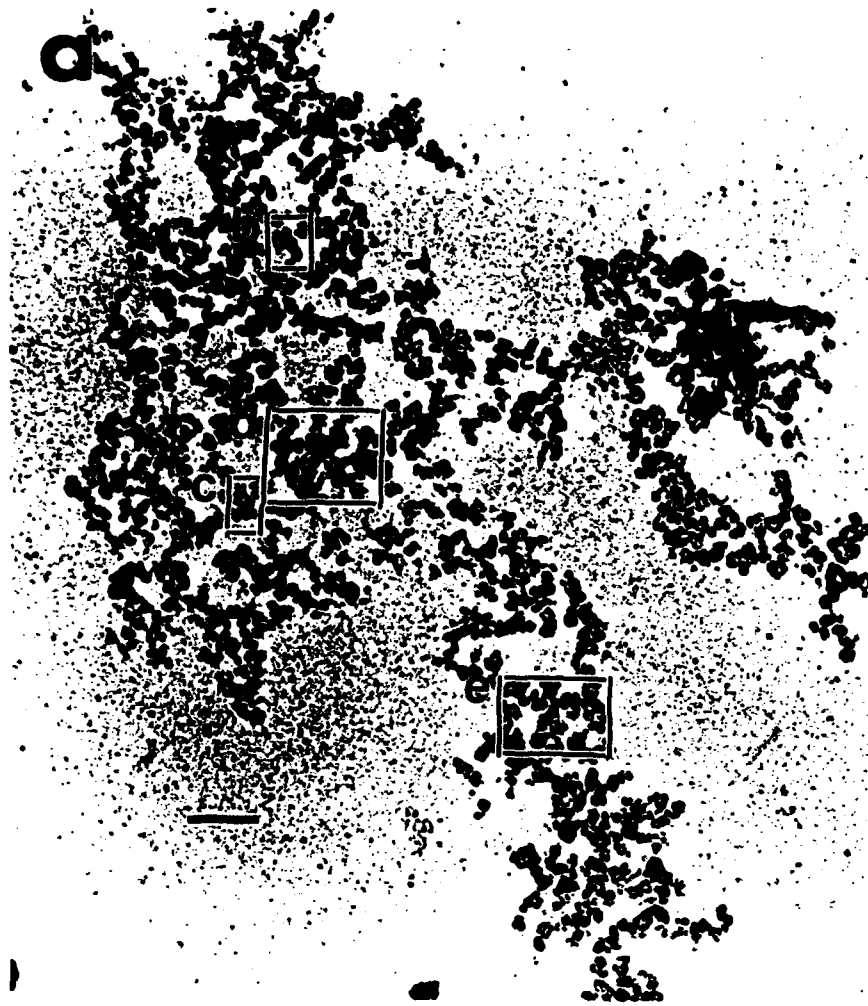


Fig. 6

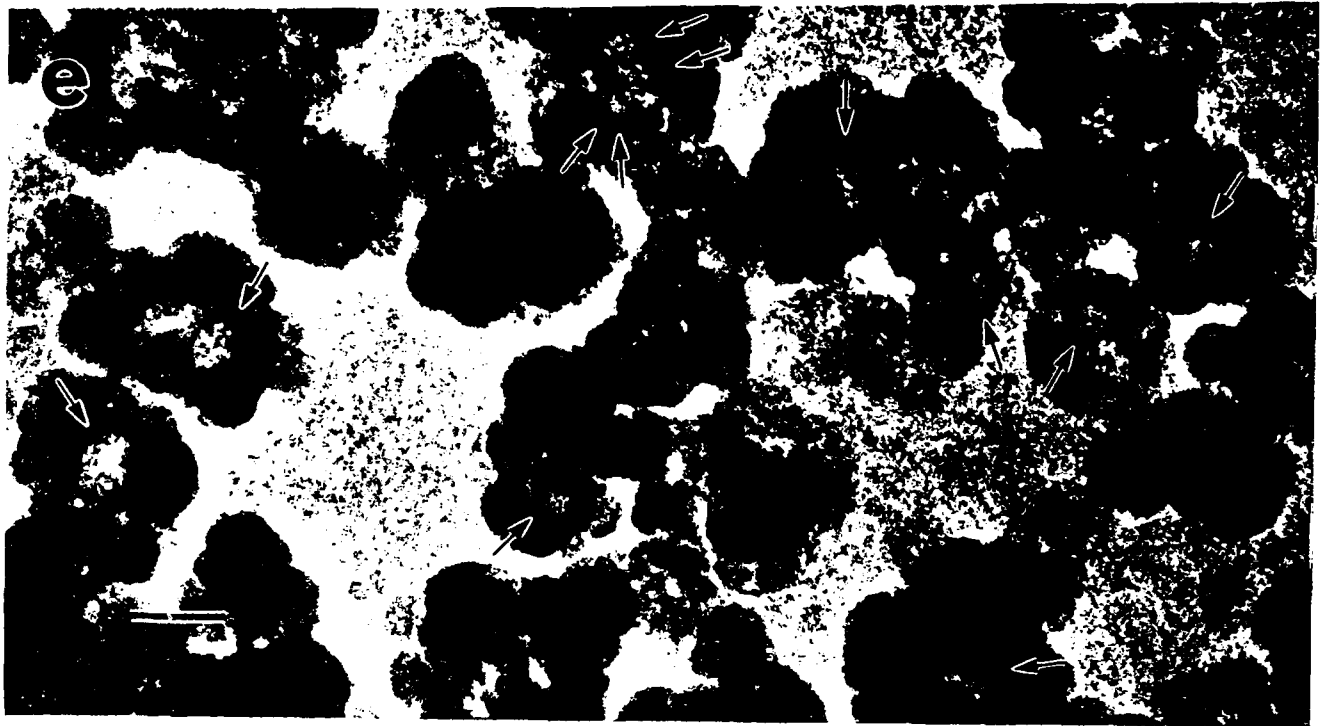


Fig. 6