


AL/CF-TR-1996-0054

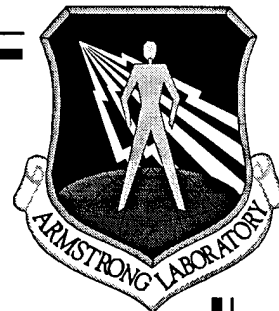

**DESIGN & DEVELOPMENT OF AN AIRWORTHY
MULTIPURPOSE 50 psi OXYGEN SYSTEM FOR TRANSPORTING
DECOMPRESSION SICKNESS PATIENTS**

Butch O. Blake, Technical Sergeant, USAF

DTIC QUALITY INSPECTED 2

**CREW SYSTEMS DIRECTORATE
Crew Technology Division
2504 Gillingham Drive, Suite 25
Brooks Air Force Base, TX 78235-5104**

May 1996

Final Technical Report for March 1995

Approved for public release; distribution is unlimited.


19960610 146

**AIR FORCE MATERIEL COMMAND
BROOKS AIR FORCE BASE, TEXAS**

**A
R
M
S
T
R
O
N
G**

**L
A
B
O
R
A
T
O
R
Y**

DISCLAIMER NOTICE

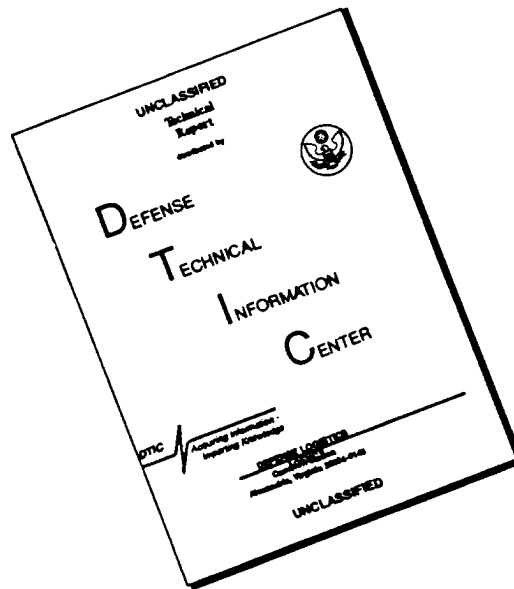

THIS DOCUMENT IS BEST QUALITY AVAILABLE. THE COPY FURNISHED TO DTIC CONTAINED A SIGNIFICANT NUMBER OF PAGES WHICH DO NOT REPRODUCE LEGIBLY.

NOTICES

This final technical report was submitted by personnel of the Systems Research Branch, Crew Technology Division, Armstrong Laboratory, AFMC, Brooks Air Force Base, Texas, under job order 7184-56-01.

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, expressed or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or usefulness of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency, contractor, or subcontractor thereof. The views and opinions of the authors expressed herein do not necessarily state or reflect those of the United States Government or any agency, contractor, or subcontractor thereof.

When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely Government-related procurement, the United States Government incurs no responsibility or any obligation whatsoever. The fact that the Government may have formulated or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication, or otherwise in any manner construed, as licensing the holder or any other person or corporation; or as conveying any rights or permission to manufacture, use or sell any patented invention that may in any way be related thereto.

The Office of Public Affairs has reviewed this report, and it is releasable to the National Technical Information Service, where it will be available to the general public, including foreign nationals.

This report has been reviewed and is approved for publication.



BLAKE, BUTCH O., TSgt, USAF
Aeromedical Research Technician



JACQUELINE D. HALE, Lt Col, USAF, NC
Chief, Aeromedical Research



JAMES P. DIXON, Colonel, USAF, BSC
Chief, Crew Technology Division

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)	2. REPORT DATE May 1996	3. REPORT TYPE AND DATES COVERED Final, March 1995	
4. TITLE AND SUBTITLE Design & Development of an Airworthy Multipurpose 50 psi Oxygen System for Transporting Decompression Sickness Patients		5. FUNDING NUMBERS PE: 62202F PR: 7184 TA: 56 WU: 01	
6. AUTHOR(S) BUTCH O. BLAKE, TSgt		8. PERFORMING ORGANIZATION REPORT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Systems Research Branch 2504 Gillingham Dr. STE 25 Brooks AFB TX 78235-5104		10. SPONSORING/MONITORING AGENCY REPORT NUMBER AL-CF-TR-1996-0054	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) Armstrong Laboratory (AFMC) Crew Systems Directorate Crew Technology Division 2504 Gillingham Dr. STE 25 Brooks AFB TX 78235-5104		11. SUPPLEMENTARY NOTES	
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distrobution unlimited.		12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) Davis Hyperbaric Laboratory, Brooks AFB TX requested Aeromedical Research to design and develop a 50 psi oxygen delivery system that could be used to transport decompression sickness patients aboard C-21 Learjets. With the help of an independant manufacturer's air ambulance life support unit having the required oxygen capacity could an interface oxygen system be built. Aeromedical Research staff members within the Systems Research Branch, considers the unit acceptable for use in the aeromedical evacuation environment.			
14. SUBJECT TERMS 50 psi Oxygen System Oxygen Delivery System Oxygen		medical equipment acceptable O2	Decompression Sickness Patients aircraft Airworthy
17. SECURITY CLASSIFICATION OF REPORT UNCLASSIFIED		15. NUMBER OF PAGES 18	
18. SECURITY CLASSIFICATION OF THIS PAGE UNCLASSIFIED		16. PRICE CODE	
19. SECURITY CLASSIFICATION OF ABSTRACT UNCLASSIFIED		20. LIMITATION OF ABSTRACT UL	

TABLE OF CONTENTS

BACKGROUND	1
DESCRIPTION	1
METHODS	4
Test Setup.....	4
Baseline Performance Assessment	4
Vibration	4
Altitude.....	5
Rapid Decompression	5
Environmental	5
RESULTS.....	5
Vibration	6
Altitude.....	6
Rapid Decompression	6
Environmental	6
RECOMMENDATIONS.....	6
CONCLUSION	7
REFERENCES	8
APPENDIX A.....	9

List of Figures

Figure 1. Exploded View of System (Labeled According to Description)	1
Figure 2. Complete System.	2
Figure 3. C1:MBU-5P1, C2:MBU-12P, D1:CRU60, D2:CRU8, & D3:PN 266-360.....	2
Figure 4. DCS O2 System with MBU-5P1 Mask.....	3
Figure 5. DCS O2 System with MBU-12P Mask.....	3

ACKNOWLEDGMENTS

I would like to thank all those who helped and advised during the development and evaluation of the Airworthy Multipurpose 50 psi Oxygen System for transporting Decompression Sickness patients. I would especially like to thank Lt Col Jacqueline Hale, 2Lt Kindra Edman, TSgt Allen Jones, SSgt Allen Gray, Mr. Ed Hade, Mr. Ronald Holden and Lt Col A. Penne, Clinical Coordinator, Hyperbaric Medicine Division.

DESIGN & DEVELOPMENT OF AN AIRWORTHY MULTIPURPOSE 50 psi OXYGEN SYSTEM FOR TRANSPORTING DECOMPRESSION SICKNESS PATIENTS

BACKGROUND

Hyperbaric Medicine Division requested Aeromedical Research design and develop a 50 psi oxygen delivery system which could be used for the transportation of decompression sickness (DCS) patients aboard the C-21 Learjet. The C-21 is a cost efficient aircraft supporting the regional aeromedical evacuation mission. Due to a need for an excessive quantity of oxygen to treat DCS patients enroute to medical care, the C-21 had not been a candidate for aeromedical transport. Airworthiness development and recent certification of an independent manufacturer's life support transport unit, containing it's own 50 psi oxygen source, expanded the C-21 capability. Still needed was a system to connect the transport unit's oxygen source to the patient while maintaining 100% oxygen at 50 psi pressure for a maximum expected two hour flight.

DESCRIPTION

The Multipurpose 50 psi Oxygen System was conceived and designed for transportation of Decompression Sickness (DCS) patients. All components are derived from existing government stock listed items. They include one each: A) Regulator, Chest Mounted, 100% oxygen, Positive Pressure, CRU-79P, B) Low Pressure Oxygen Hose, C) MBU-5P1 or 12P Aviator's mask, D) Connector to attach the O2 Regulator to Mask Hose, E) Hose, O2, Low Pressure, F) AN to 1/8" pipe thread nipple, G) 1/8" pipe thread to medical oxygen (O2) hose nipple, and H) either Puritan-Bennett or Schrader O2 adapter depending on outlet source.

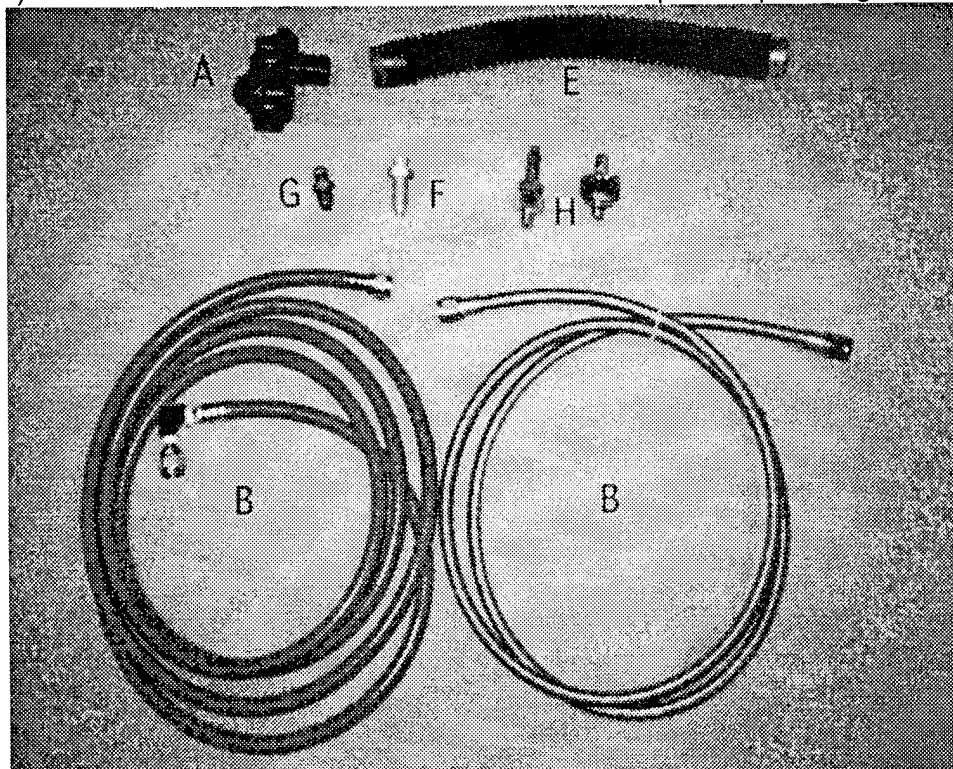


Figure 1. Exploded View of System (Labeled According to Description)

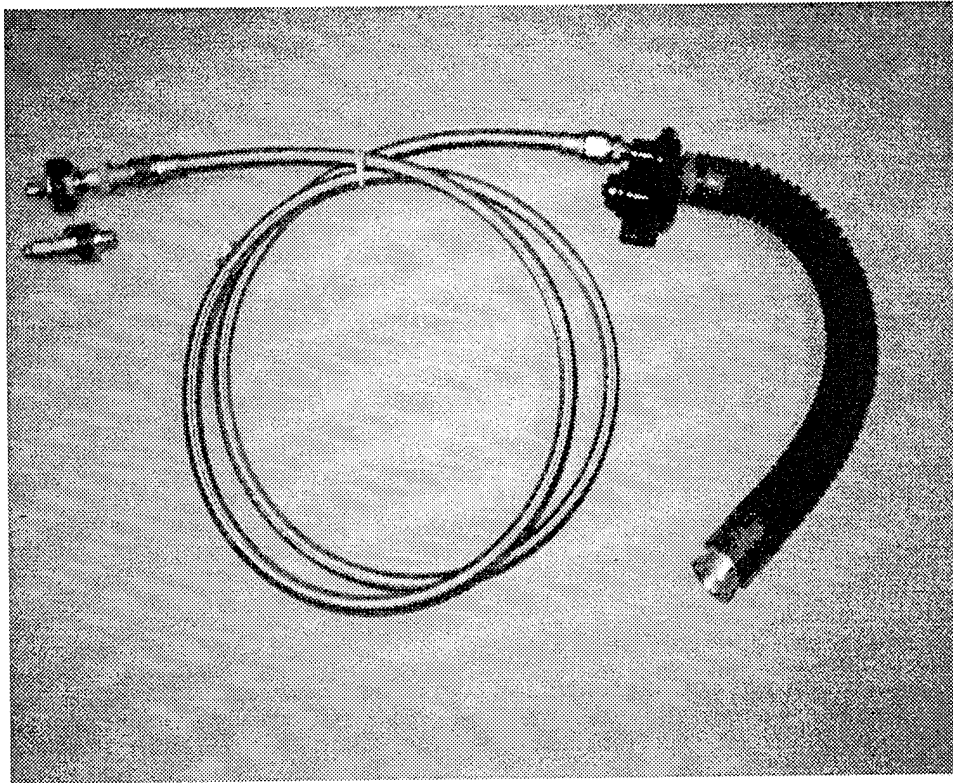


Figure 2. Complete System.

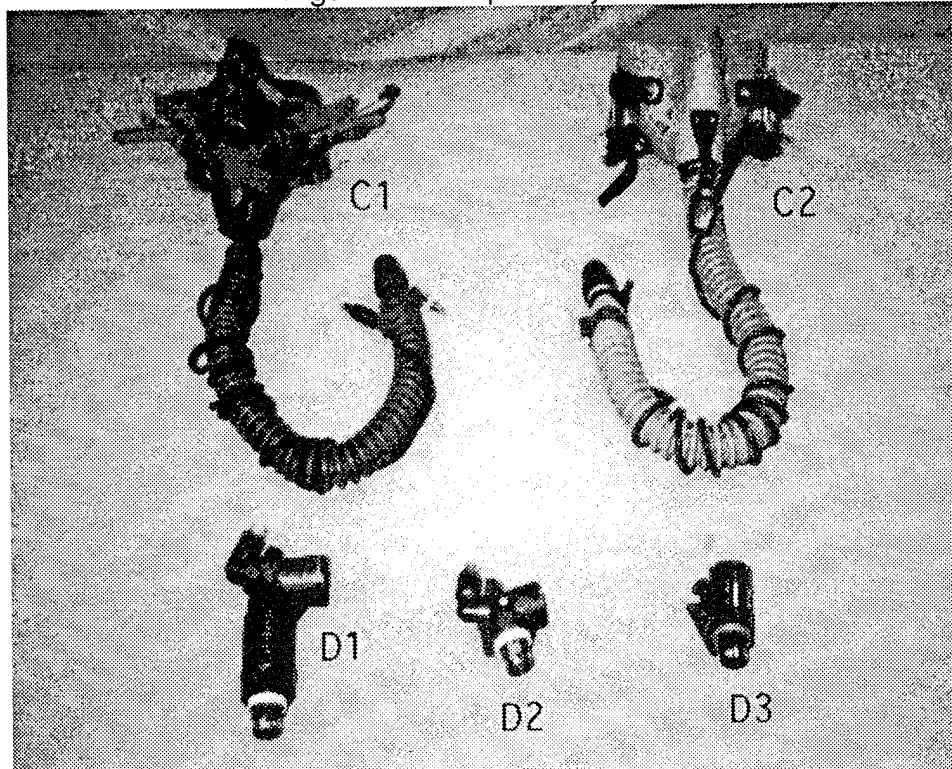


Figure 3. C1: MBU-5P1, C2: MBU-12P, D1: CRU60, D2: CRU8, & D3: PN 266-360

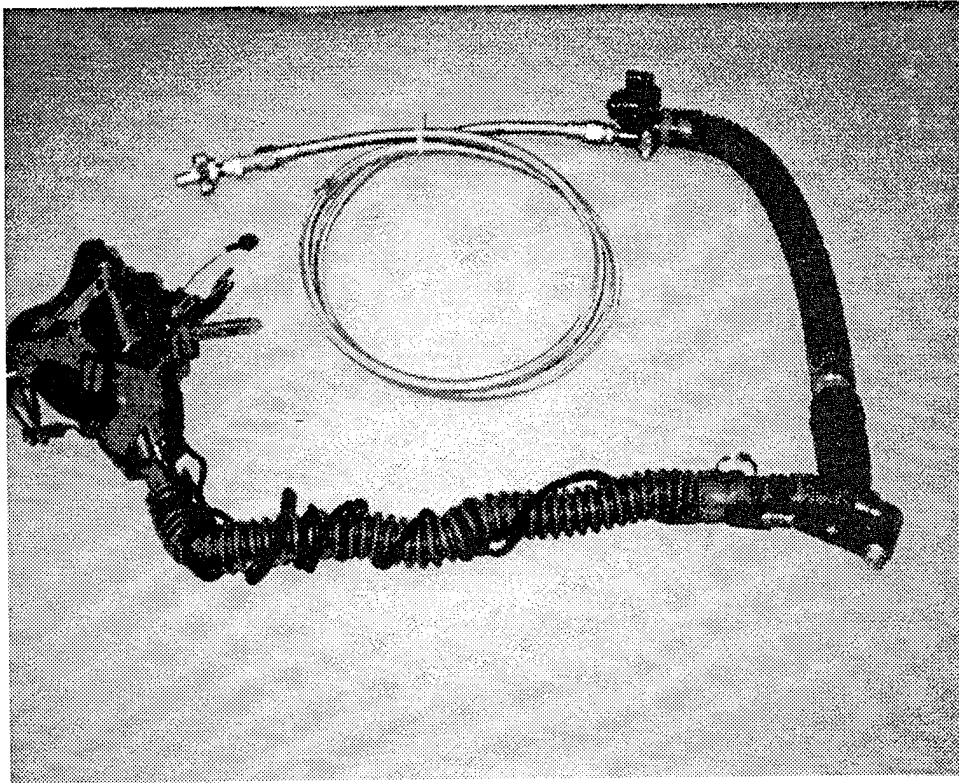


Figure 4. DCS O2 System with MBU-5P1 Mask

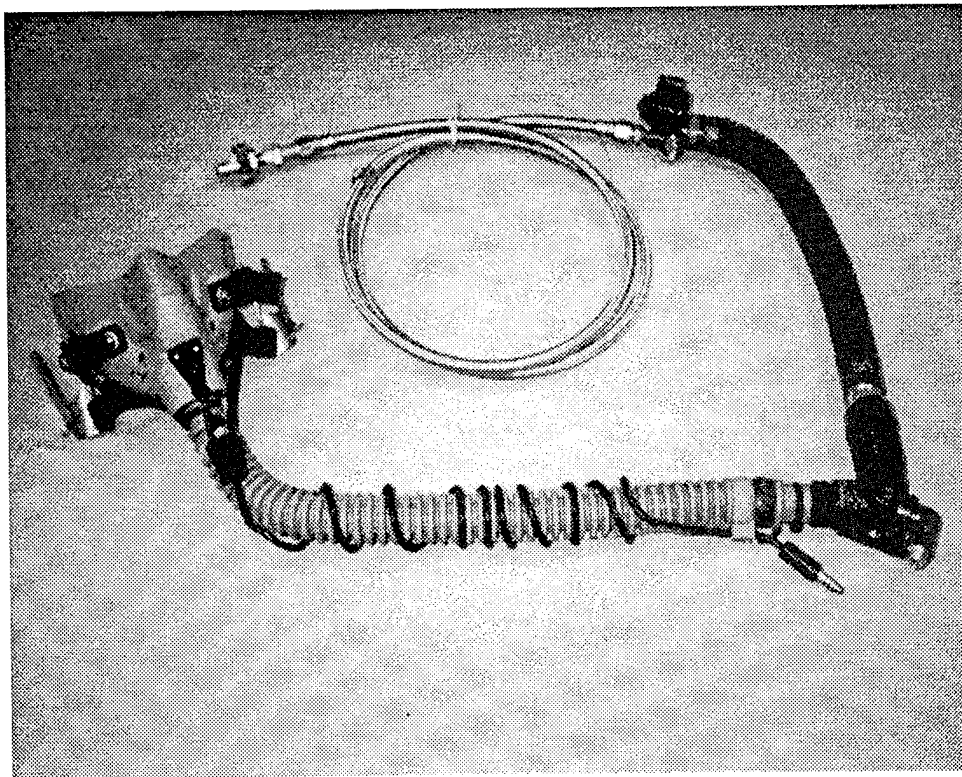


Figure 5. DCS O2 System with MBU-12P Mask

METHODS

Test methods and performance criteria were derived from various military standards (Reference List, 1-2), nationally recognized performance guidelines, Emergency Care Research Institute (ECRI), and Aeromedical Research Procedures Guide. Extensive testing on the regulator was conducted at Armstrong Laboratory for a Department of the Navy contract. The regulator is the critical device to the system that required extensive evaluation for its response to environmental conditions for aeromedical evacuation. Aeromedical Research analyzed these tests and conducted a baseline performance and gas consumption evaluation of the entire system.

Test Setup

The Multipurpose 50 psi Oxygen System will operate from a 50 Pounds psi oxygen (O₂) source. The low pressure O₂ hose fitted with a Puritan-Bennett adapter will be inserted into an O₂ outlet. The other end will be connected to a CRU 79P 100% oxygen, chest mounted, demand valve regulator. From the CRU 79, an Aviator's mask and breathing hose will be attached. The Aviator's mask will be fitted to a KRUG INTERNATIONAL breathing simulator. All tests involving environmental extremes, vibration, and altitude will be evaluated by Aeromedical Research personnel using the Aeromedical Research Procedures Guide and Military Specification MIL-R-81553B(AS) dated 17 Sept. 1992.

Baseline Performance Assessment

The purpose of the Baseline Performance Assessment (BPA) is to quantitatively measure and record the Multipurpose 50 psi Oxygen System's performance under standard ambient conditions before adverse testing. The BPA will then be used as a reference to measure subsequent performance. Initially it verifies specifications and checks for safe operation before testing. Specifically, the BPA includes the following:

Initial Inspection. Each component of the Multipurpose 50 psi Oxygen System was inspected for external damage and faulty manufacturing. Operational procedures were verified against military specification MIL-R-81553B(AS) dated 17 Sept. 1992, and the performance check procedures from the test plan, noted as follows.

Performance Checks. The following measurements taken during initial operation at standard ambient conditions served as a baseline for later comparison. A baseline test consists of connecting the system's low pressure oxygen hose to the 50 psi source and the aviator's mask to the KRUG INTERNATIONAL breathing simulator concurrently using a Biotek DPM III to assess the aviator mask pressure.

Vibration

Vibration evaluation is designed to determine an item's integrity, durability, and performance during worst case scenario vibrations. The Multipurpose 50 psi Oxygen

System was subjected to vibration tests in accordance with MIL-R-81553B(AS) to include, a vibration schedule for 9 hours (3 hours in each axis) at a frequency of 500 to 2500 to 500 cycles at a sweep rate of 15 minutes, and a double amplitude of 0.018 to 0.020 inch.

Altitude

The Multipurpose 50 psi Oxygen System regulator was assessed for evaluation of effects of reduced barometric pressure in accordance with MIL-R-81553B(AS). The parameters involve ascending from ground level to 50,000 feet for 50 cycles. Ascent rates will constitute 500 feet per second and descent rates of 1,000 feet per second.

Rapid Decompression

The purpose of this test was to approximate the stress that medical equipment is exposed to during normal, emergency, and accidental decompression. Although, rapid decompressions are uncommon in military transport aircraft, the effect of such an occurrence on a medical item could present a severe safety hazard to the patient, crew, or aircraft operations. The Multipurpose 50 psi Oxygen System regulator was subjected to One cycle from ground level to 50,000 feet returning to ground level in accordance with MIL-R-81553B(AS).

Environmental

Environmental test conditions for aeromedical evacuation medical equipment devices are tailored based on the aeromedical operational environment from MIL-STD-810E. However, testing for the Multipurpose 50 psi Oxygen Regulator was accomplished under MIL-R-81553B(AS). MIL-R-81553B(AS) exceeds parameters set forth in the Aeromedical Research Procedures Guide. The Procedure's Guide requires cold temperature of -40° C, and hot temperature of 60° C of 49° C. MIL-R-81553B(AS) evaluates cold temperature to -54° C and hot temperature to 71° C. Consequently, results from testing to MIL-R-81553B(AS) were accepted for airworthiness evaluation.

RESULTS

Testing was accomplished using MIL-R-81553(AS). Multiple tests were performed and data were evaluated against aeromedical evacuation requirements. Under the following conditions the Multipurpose 50 psi Oxygen System functioned as required and is therefore, considered an air worthy medical device capable of supplying 100% oxygen to decompression sickness patients.

Vibration

Aeromedical Research analyzed data from MIL-R-81553B(AS) evaluation of the Multipurpose 50 psi Oxygen System which indicated no adverse affects. Aeromedical Research found the device acceptable for use in the aeromedical evacuation environment.

Altitude

The altitude parameters used in MIL-R-81553B(AS) to test the regulator exceeded parameters outlined in the Aeromedical Research Procedures Guide. Aeromedical Research analyzed the data and determined the Multipurpose 50 psi Oxygen System functions as required at altitude and is acceptable for use on board aeromedical evacuation aircraft.

Rapid Decompression

The Multipurpose 50 psi Oxygen System regulator was exposed to limits higher in MIL-R-81553B(AS) testing than limits used by Aeromedical Research. Data analysis indicates the oxygen regulator remained functional during testing. The Multipurpose 50 psi Oxygen System is acceptable for use in the aeromedical evacuation environment.

Environmental

Under MIL-R-81553B(AS) the Multipurpose 50 psi Oxygen System regulator was evaluated to a higher level of environmental extremes than outlined in the aeromedical research procedure's guide. Data analysis indicates the oxygen regulator remained functional during testing. The Multipurpose 50 psi Oxygen System is deemed acceptable for use in USAF aircraft.

RECOMMENDATIONS

1. Do not use oil or any kind of petroleum products on or around this product.
2. Do not smoke or use combustibles around oxygen equipment.
3. Provide a carrying case to protect the system during handling, i.e. a USAF helmet bag.
4. Caution needs to be taken not to allow contaminants of any kind to be used on or about the oxygen regulator.

CONCLUSION

Overall, the Multipurpose 50 psi Oxygen System is considered airworthy. It operates within expected parameters when subjected to environmental extremes and simulated cabin altitude's, and does not produce a hazard to patient or crew during rapid decompression. A parts list is available in appendix A of this report.

REFERENCES

1. MIL-R-81553B(AS), Regulator, Chest Mounted, Oxygen, Positive Pressure, CRU-79/P
2. Emergency Care Research Institute (ECRI),
3. Aeromedical Research Procedures Guide, Internal Operating Instruction, Armstrong Laboratory, Systems Research Branch.

APPENDIX A

APPENDIX

DESIGN PLAN AND PARTS LIST FOR THE MULTIPURPOSE 50 PSI OXYGEN SYSTEM

<u>National Stock Number</u>	<u>Cost</u>	<u>Description</u>
1. 1660-01-008-8107	\$245.00	CRU-79/P Oxygen pressure regulator
2. 4720-01-142-0750	\$63.88	.Hose, Oxygen, low pressure
3. 4730-00-541-8297 (X2)	\$0.32	.Clamp, Hose, OD 1.062 min., 1.125 max.
4. 1660-00-730-2247	\$4.59	Straight connector
5. 4730-00-187-0088	\$0.61	Adapter, Straight, Pipe to Boss fitting or 1/8" Pipe to DISS fitting depending on type of low pressure hose you will be using (no number).
6. None	\$40.95	Green medical low pressure oxygen hose 72" in length.
7. None	\$14-25.00	Ohmeda or Puritan-Bennett adapter to connect to outlets in USAF ambulances and outlets on the Spectrum 2500 Air Ambulance Life Support system.
8. 1660-01-073-7595LS	<u>\$101.10</u>	MBU-12/P, Aviators Oxygen Mask
Total cost	\$490.84	

* The following items may also be substituted depending on cost and availability.

1. 1660-00-810-3225	\$53.00	MBU-5/P, Aviators Oxygen Mask
2. 4720-01-140-4381	\$257.03	.Hose assembly, Oxygen breathing, 72" in length