

AD A

REPORT NO T 97-8

**TELEMETRY PILL MEASUREMENT OF CORE TEMPERATURE
DURING ACTIVE HEATING AND COOLING**

**U S ARMY RESEARCH INSTITUTE
OF
ENVIRONMENTAL MEDICINE**

Natick, Massachusetts

JULY 1997



Approved for public release; distribution unlimited

FORM 8 (MAY 1982) UNCLASSIFIED

**UNITED STATES ARMY
MEDICAL RESEARCH AND MATERIEL COMMAND**

19970811 062

The opinions or assertions contained herein are the private views of the author(s) and are not to be construed as official or as reflecting the views of the Army or the Department of Defense.

Human subjects participated in these studies after giving their free and informed voluntary consent. Investigators adhered to AR 70-25 and USAMRMC Regulation 70-25 on the use of volunteers in research.

Citations of commercial organizations and trade names in this report do not constitute an official Department of the Army endorsement or approval of the products or services of these organizations.

DTIC AVAILABILITY NOTICE

Qualified requesters may obtain copies of this report from Commander, Defense Technical Information Center (DTIC) (formerly DDC), Cameron Station, Alexandria, Virginia 22314.

DISPOSITION INSTRUCTIONS

Destroy this report when no longer needed.

Do not return to the originator.

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)	2. REPORT DATE July, 1997	3. REPORT TYPE AND DATES COVERED Technical Report
----------------------------------	------------------------------	--

4. TITLE AND SUBTITLE Telemetry pill measurement of core temperature during active heating and cooling	5. FUNDING NUMBERS
---	--------------------

6. AUTHOR(S) Catherine O'Brien, Reed W. Hoyt, Mark J. Buller, John W. Castellani and Andrew J. Young

7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) U.S. Army Research Institute of Environmental Medicine Kansas Street Natick, MA 01760-5007	8. PERFORMING ORGANIZATION REPORT NUMBER
--	--

9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) Same as Block 7	10. SPONSORING/MONITORING AGENCY REPORT NUMBER
--	--

11. SUPPLEMENTARY NOTES

12a. DISTRIBUTION / AVAILABILITY STATEMENT Approved for public release; distribution is unlimited.	12b. DISTRIBUTION CODE
---	------------------------

13. ABSTRACT (Maximum 200 words)

The agreement between core temperature measurements obtained using an ingestible temperature pill telemetry system (T_{pill}) and rectal (T_{re}) and esophageal (T_{es}) thermocouples was compared under conditions of both increasing and decreasing body temperature. Nine subjects participated in four 3-h trials: cold (18°C) water rest (CWR); cold water exercise (CWE); warm (36°C) water rest (WWR); and warm water exercise (WWE). During exercise trials, subjects completed three bouts of 15-min rest, followed by 45-min exercise on a cycle ergometer at 50% of peak oxygen uptake. The temperature pill was taken 10-12 h before testing. Root mean squared deviation (RMSD) was calculated for each pair of measurements (T_{pill} vs. T_{re} , T_{pill} vs. T_{es} , T_{re} vs. T_{es}) for each trial. An RMSD of "0" indicates perfect agreement, and as RMSD increases, agreement worsens. On CWR, the RMSD for $T_{pill}-T_{es}$ (0.23 ± 0.04) was lower ($P<0.05$) than for $T_{pill}-T_{re}$ (0.43 ± 0.10) or $T_{re}-T_{es}$ (0.46 ± 0.09). There were no significant differences in RMSD between measurement pairs on any other trial (overall average RMSD= 0.26°C). These results suggest the telemetry pill system provides a valid measurement of core temperature during conditions of decreasing as well as increasing body temperature and during steady state.

14. SUBJECT TERMS Exercise, Heat, Cold, Ambulatory monitoring	15. NUMBER OF PAGES
	16. PRICE CODE

17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT
---	--	---	----------------------------

CONTENTS

LIST OF FIGURES.....	iv
LIST OF TABLES.....	iv
EXECUTIVE SUMMARY.....	1
INTRODUCTION.....	2
METHODS.....	3
RESULTS.....	7
DISCUSSION.....	11
REFERENCES.....	13
DISTRIBUTION LIST.....	14

LIST OF FIGURES

Figure 1. Cold Water Rest Trial. Core temperature measurements by rectal and esophageal thermocouple and telemetric temperature pill.....	8
Figure 2. Cold Water Exercise Trial. Core temperature measurements by rectal and esophageal thermocouple and telemetric temperature pill.....	8
Figure 3. Warm Water Rest Trial. Core temperature measurements by rectal and esophageal thermocouple and telemetric temperature pill.....	9
Figure 4. Warm Water Exercise Trial. Core temperature measurements by rectal and esophageal thermocouple and telemetric temperature pill.....	10

LIST OF TABLES

Table 1. Root mean squared deviation (RMSD) values ($\bar{X} \pm \text{SEM}$) for each pair of measurements on each trial.....	7
--	---

**TECHNICAL REPORT
NO.**

**TELEMETRY PILL MEASUREMENT OF CORE TEMPERATURE
DURING ACTIVE HEATING AND COOLING**

by

Catherine O'Brien, Reed W. Hoyt, Mark J. Buller
John W. Castellani and Andrew J. Young

July, 1997

Thermal and Mountain Medicine Division
U.S. Army Research Institute of Environmental Medicine
Natick, Massachusetts 01760-5007

EXECUTIVE SUMMARY

The purpose of this study was to compare the agreement between core temperature measurements obtained using an ingestible temperature pill telemetry system (T_{pill}) with those obtained from rectal (T_{re}) and esophageal (T_{es}) thermocouples under conditions of both increasing and decreasing body temperature. Nine subjects participated in four 3-h trials: cold (18°C) water rest (CWR); cold water exercise (CWE); warm (36°C) water rest (WWR); and warm water exercise (WWE). Subjects were immersed to the neck for each trial. During resting trials, subjects sat quietly. During exercise trials, subjects completed three bouts of 15-min rest, followed by 45-min exercise on a cycle ergometer at 50% of peak oxygen uptake. The temperature pill was taken 10-12 h before testing, after which the subjects fasted. The trials created conditions of constantly decreasing (CWR) or increasing (WWR) core temperature, as well as periods of oscillating core temperature (CWE and WWE). Root mean squared deviation (RMSD) was calculated for each pair of measurements (T_{pill} vs. T_{re} , T_{pill} vs. T_{es} , T_{re} vs. T_{es}) for each trial. An RMSD of "0" indicates perfect agreement, and as RMSD increases, agreement worsens. On CWR, the RMSD for $T_{\text{pill}}-T_{\text{es}}$ (0.23 ± 0.04) was lower ($P<0.05$) than for $T_{\text{pill}}-T_{\text{re}}$ (0.43 ± 0.10) or $T_{\text{re}}-T_{\text{es}}$ (0.46 ± 0.09). There were no significant differences in RMSD between measurement pairs on any other trial (overall average $\text{RMSD}=0.26^{\circ}\text{C}$). Telemetry pill temperature and response time tended to be intermediate between T_{re} and T_{es} . These results suggest the telemetry pill system provides a valid measurement of core temperature during conditions of decreasing as well as increasing body temperature and during steady state.

INTRODUCTION

Monitoring body core temperature unobtrusively in active subjects is difficult. Esophageal and rectal temperature, generally considered the most reliable and precise indices of core temperature (Sawka and Wenger, 1988), are invasive measurements and require a wire connection between the sensor and monitoring/recording device. Thus, these measurement methods are unsuitable for physiological monitoring of ambulatory, unrestrained subjects. For these applications, ingestible temperature sensors offer an acceptable alternative.

Ingestible temperature pill telemetry systems provide a valid measure of core temperature during rest and exercise in warm or neutral ambient conditions (Sparling et al., 1993; Kolka et al., 1993). However, the validity of the temperature pill measurements during cold exposure has not been demonstrated. Therefore, the aim of this study was to compare measurements obtained from an ingestible telemetric temperature pill with those from esophageal and rectal thermocouples during cold as well as hot conditions. The validity of the temperature pill measurement for monitoring core temperature was thus determined during conditions of decreasing as well as increasing body temperature.

METHODS

SUBJECTS

Nine healthy soldiers (four male, five female) participated in this study. The subjects had the following characteristics: age= 25 ± 2 yr; weight= 73 ± 3 kg; height= 166 ± 3 cm; peak oxygen uptake= 3.1 ± 0.4 l/min. All subjects voluntarily consented to participate after being informed of the purpose, procedures, and known risks of these experiments, which were approved by the appropriate institutional review boards. Female volunteers were screened for pregnancy, which was an exclusionary criterion. All soldiers were in compliance with the Army height and weight standards (males less than 22% fat; females less than 32% fat) (Department of the Army, 1986).

Peak oxygen uptake was determined using a continuous effort, progressive intensity stationary cycle ergometer protocol. After a brief warmup, subjects pedaled for 2 min at 60 rpm against zero resistance; thereafter, the power output was increased 30 W every 2 min until the subject was unable to continue in spite of verbal encouragement. Oxygen uptake, carbon dioxide output, and minute ventilation were measured continuously throughout. Peak oxygen uptake was defined as the highest oxygen uptake achieved. Heart rate, monitored using an electrocardiogram obtained from chest electrodes (CM-5 placement) and radio telemetered to an oscilloscope-cardiotachometer, was recorded at the end of each stage.

PROTOCOL

The study employed a repeated measures design in which each subject served as his/her own control. Each volunteer participated in four 3-h immersion trials: a) cold (18°C) water rest (CWR), to produce a continuous decrease in core temperature (T_c); b) cold water exercise (CWE), to produce an oscillation in T_c superimposed over a generally decreasing T_c ; c) warm (36°C) water rest (WWR), to produce a continuous increase in T_c ; and d) warm water exercise (WWE), to produce an oscillation in T_c superimposed over a generally increasing T_c . Exercise consisted of three repeated bouts of 15-min rest followed by 45-min cycling at 50% of the individual's peak oxygen uptake.

TELEMETRY PILL SYSTEM

The ingestible telemetric temperature system consisted of a commercial temperature pill, 2 cm in length x 1.2 cm diameter (CorTemp™, Human Technologies, Inc., St. Petersburg, FL), and a compact data receiver/logger (BBN Systems and Technologies, Cambridge, MA). The temperature pill consists of a temperature-sensitive quartz crystal oscillator with a silver oxide battery, encapsulated in epoxy and covered with silicone rubber. This sensor transmits a continuous, low-frequency radio wave which varies with temperature. This signal is received and stored by the data logger and later downloaded to a computer after completion of data collection.

A linear relationship exists between signal frequency and temperature. While the slope constant of this relationship is similar from pill to pill, the intercept varies. Although the pills are individually calibrated by the manufacturer, the accuracy and precision of the calibration of each pill was confirmed in our laboratory using the same data loggers as used in the experiments. An individual linear regression relationship of temperature-to-frequency was derived for each pill based on the frequency emitted after equilibration in a water bath at three temperatures (33°C, 37°C, 41°C). This regression equation was used to convert frequencies transmitted by the pill into temperature values. Each pill had a correlation coefficient between water bath temperature and frequency emitted greater than 0.999.

EXPERIMENTAL PROCEDURES

Subjects began fasting at 1900 h on the evening before each immersion test. The telemetric temperature pill was then ingested at 2000 h. Subjects were allowed to ingest as much water as necessary to swallow the pill, but thereafter refrained from food or fluid intake until arriving at the laboratory at 0700 h the next morning. After voiding and having their nude weight measured, they consumed 235 ml of a commercial meal-replacement beverage (Ensure, Ross Products Division, Abbott Laboratories, Columbus, OH). The rectal thermocouple was inserted 10 cm into the rectum; the esophageal thermocouple was inserted through the nose to the level of the heart, estimated as 1/4 of the subject's height. All thermocouples (copper-constantan,

Physitemp Instruments, Inc., Clifton, NJ) were tested prior to use to verify that they were accurate within $\pm 0.1^\circ\text{C}$. The trials all began at approximately 0800 h.

For the experiments, subjects sat with their legs extended on the pedals of a semirecumbent cycle ergometer modified for use in water. Fly-wheel resistance was adjusted by attaching fins of varying length to the flywheel, similar to the method employed by Shapiro et al. (Shapiro et al., 1981). The seat and back of the chair were constructed of stainless steel, perforated to facilitate water movement around the subject and minimize the formation of a still boundary layer. Subjects wore aquatic sport sandals, open at the top, toes, and sides, to protect the bottom of the feet during pedaling. The ergometer was mounted on a platform that could be raised and lowered in and out of a 30,000 l pool in which water was continuously circulated and temperature maintained within $\pm 0.1^\circ\text{C}$ of the desired temperature. The water level was adjusted to cover the subjects' shoulders while they were immersed. During the exercise trials, subjects rested for the first 15 min of each hour, then pedaled at a rate of 40 rpm for 45 min. This cycle was repeated three times, for a total of 3-h immersion. The resistance was adjusted to a predetermined setting designed to elicit an oxygen uptake equivalent to 50% of peak oxygen uptake. Heart rate was monitored continuously during immersion. Rectal and esophageal temperatures were measured and recorded every 30 sec throughout immersion using an automated data acquisition system. Pill temperature data were recorded every 15 sec throughout immersion by data loggers attached to a belt around the waist of the subject. Metabolic rate was measured from the 5th to the 10th minute and from the 50th to 55th minute of each hour of immersion. At the end of each hour of immersion subjects were allowed to drink 200 ml of water.

STATISTICAL ANALYSIS

To compare temperature pill measurements (T_{pill}) with the corresponding rectal (T_{re}) and esophageal (T_{es}) temperature measurements, the root mean square deviation (RMSD) between the corresponding time series temperature data every 30 seconds (T_{pill} vs. T_{re} ; T_{pill} vs. T_{es} ; T_{re} vs. T_{es}) was calculated for each subject on each trial as described by Haslam and Parsons (Haslam and Parsons, 1988). The RMSD provides an estimate of the agreement between two measures of a single parameter, in this

case, core temperature. Agreement is perfect when $RMSD=0$. To determine whether exercise and water temperature influenced the agreement between T_{pill} and T_{re} and T_{es} , the RMSD values were compared using a two-way (measurement x trial) repeated measures analysis of variance (ANOVA). ANOVA was also conducted to compare measurements over time during each trial. For this analysis, representative data at 10 min time points were used; i.e., 19 data points per trial. In addition, pre-immersion temperatures were compared by ANOVA. Post-hoc analysis of significant ($P<0.05$) main effects (i.e., significant differences between measurements) was by Tukey's HSD test. Data are presented as $mean\pm SEM$.

RESULTS


On three occasions, T_{pill} signal was not detected from a subject on the morning of the trial. In these instances, a new pill was ingested, and the trial postponed 1 hour. The T_{pill} data for these subjects were within two standard deviations of the mean T_{pill} from all other subjects, and were therefore included in the statistical analyses. At the end of each hour, coincident with when subjects were allowed to drink water, a transient decrease in T_{es} was always observed. For the data analysis, these data (the drinking-associated depression) were deleted, since they reflected the transient local cooling effect of water ingestion on the esophagus.

The RMSD ($\bar{X} \pm SEM$) for each measurement pair ($T_{pill} - T_{re}$, $T_{pill} - T_{es}$, $T_{re} - T_{es}$) on each trial is presented in Table 1. On CWR, the RMSD for $T_{pill} - T_{es}$ was lower ($P < 0.05$) than for $T_{pill} - T_{re}$ or $T_{re} - T_{es}$, as indicated by *. There were no other differences between measurement pairs or trials.


TABLE 1. Root Mean Squared Deviation ($^{\circ}C$)

	$T_{pill} - T_{re}$	$T_{pill} - T_{es}$	$T_{re} - T_{es}$
Cold Water Rest	0.43 \pm 0.10	0.23 \pm 0.04*	0.46 \pm 0.09
Cold Water Exercise	0.36 \pm 0.08	0.24 \pm 0.02	0.35 \pm 0.06
Warm Water Rest	0.15 \pm 0.03	0.25 \pm 0.05	0.17 \pm 0.02
Warm Water Exercise	0.22 \pm 0.06	0.26 \pm 0.03	0.30 \pm 0.03


Data at 10-min timepoints for CWR is shown in Figure 1. Pre-immersion T_{pill} did not differ from either T_{re} or T_{es} ; however, T_{re} was higher (0.2 \pm 0.1 $^{\circ}C$, $P < 0.05$) than T_{es} . Temperature fell continuously during CWR (T_{pill} , -0.6 \pm 0.1 $^{\circ}C$; T_{re} , -1.4 \pm 0.2 $^{\circ}C$; T_{es} , -0.4 \pm 0.1 $^{\circ}C$). During CWR, T_{pill} and T_{es} did not differ from each other, but both were higher ($P < 0.05$) than T_{re} .

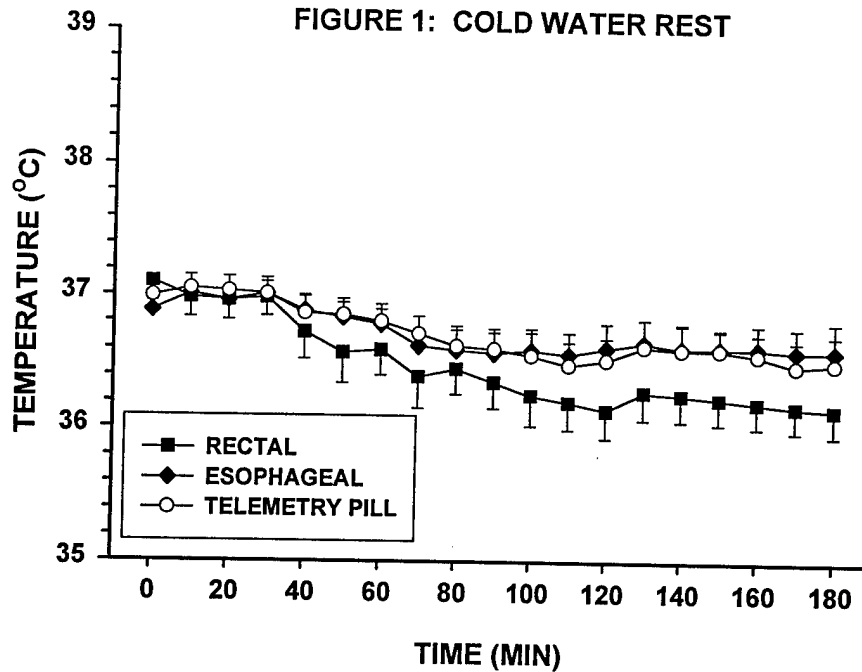

Data at 10-min timepoints for CWE is shown in Figure 2. Pre-immersion T_{pill} did not differ from either T_{re} or T_{es} ; however, T_{re} was higher ($0.3 \pm 0.1^\circ\text{C}$, $P < 0.05$) than T_{es} . The mean difference between highest and lowest temperature achieved during CWE was $1.2 \pm 0.1^\circ\text{C}$ for T_{pill} , $1.2 \pm 0.1^\circ\text{C}$ for T_{re} , and $1.4 \pm 0.1^\circ\text{C}$ for T_{es} . There were no differences between measurements across the trial.

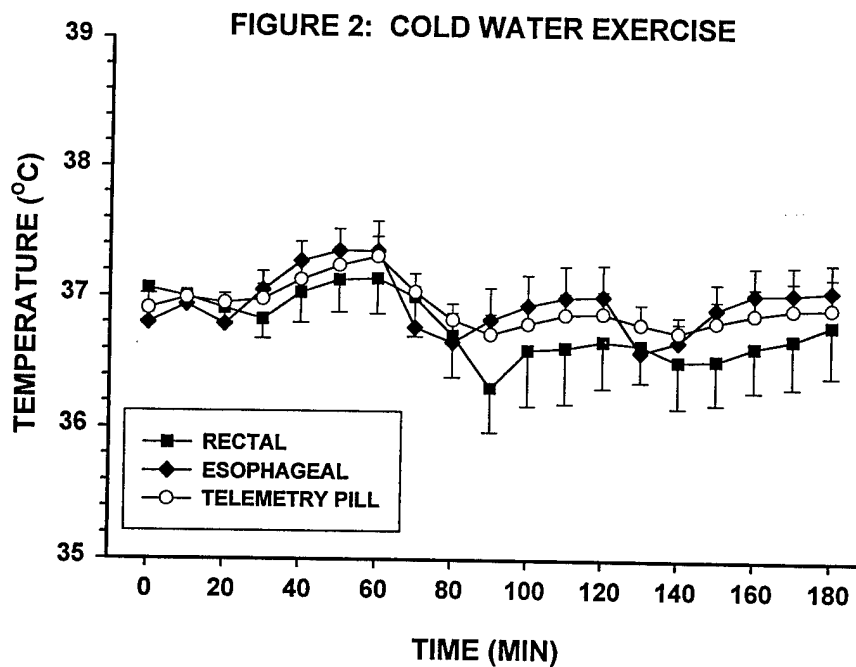


Data at 10-min timepoints for WWR is shown in Figure 3. Pre-immersion T_{es} was lower ($0.3 \pm 0.1^\circ\text{C}$, $P < 0.05$) than both T_{pill} and T_{re} , which did not differ. Temperature rose continuously during WWR (T_{pill} , $0.5 \pm 0.1^\circ\text{C}$; T_{re} , $0.3 \pm 0.1^\circ\text{C}$; T_{es} , $0.4 \pm 0.1^\circ\text{C}$). There was no difference between T_{pill} and T_{re} , but both were higher ($P < 0.05$) than T_{es} .

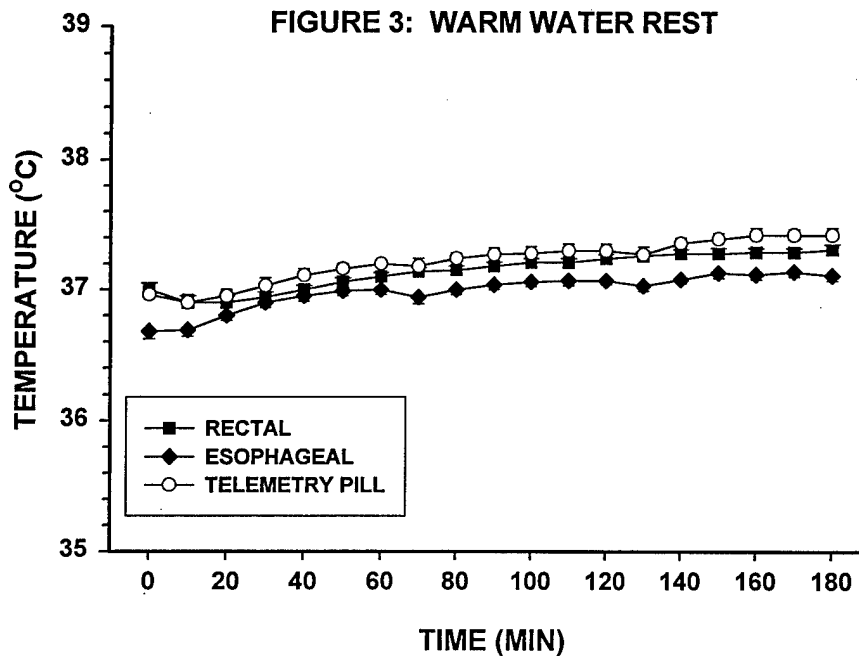

Data at 10-min timepoints for WWE is shown in Figure 4. Pre-immersion T_{pill} did not differ from T_{re} or T_{es} ; however, T_{re} was higher ($0.2 \pm 0.1^\circ\text{C}$, $P < 0.05$) than T_{es} . The mean difference for each subject between highest and lowest temperature achieved during WWE was $1.5 \pm 0.2^\circ\text{C}$ for T_{pill} , $1.4 \pm 0.2^\circ\text{C}$ for T_{re} , and $1.5 \pm 0.2^\circ\text{C}$ for T_{es} . On WWE, there was no difference between T_{pill} and T_{re} , but both were higher ($P < 0.05$) than T_{es} .

FIGURE 4: WARM WATER EXERCISE

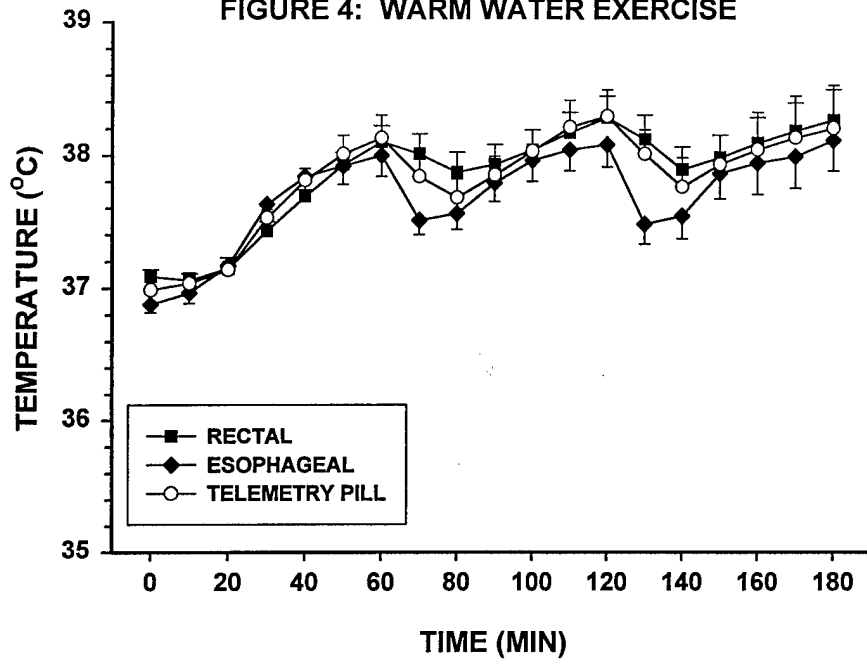

DISCUSSION

The purpose of this study was to extend previous findings demonstrating the validity of a telemetry pill for core temperature measurement in warm conditions by validating the pill system for measurement of core temperature in cold conditions. The trials successfully created the desired conditions of both rising and falling core temperature. During resting trials, a steady change in temperature occurred. The exercise trials showed a general change in temperature throughout the trial, with oscillations in temperature created by alternating rest and exercise.

Both T_{es} and T_{re} are widely accepted as valid measurements of core temperature, hence were used as standards against which T_{pill} is evaluated. Previous studies compared T_{pill} to T_{es} or T_{re} at selected discrete time points during rest or steady state exercise. However, a comparison of the measurements throughout an entire experimental period has never been reported. The root mean squared deviation used in our analysis does this by comparing each pair of measurements at all time points during the experiment to determine the overall mean deviation of one measurement relative to the other. This analysis demonstrated that the agreement between T_{pill} and T_{re} or T_{es} was similar to the agreement between T_{re} and T_{es} under all conditions studied. Thus, T_{pill} appears to be a valid method for measurement of core temperature in humans during conditions of both decreasing, as well as increasing, body temperature.

The advantages and limitations of differing sites and methodologies of measurements of human core temperature and the physiological mechanisms accounting for differences in the core temperature measured by those methodologies are considered in detail elsewhere (Sawka and Wenger, 1988). As others have reported (Kolka et al., 1993), we observed that T_{re} was generally higher than T_{es} , and that T_{pill} was typically intermediate. The exception to this was during the resting cold water trial. When seated at rest in cold water, subjects in this study displayed a lower T_{re} , compared to T_{pill} or T_{es} . This may reflect facilitated conductive heat loss from the subject's lower torso and limbs, as the subjects sat on a chair made of stainless steel, which has a higher heat transfer coefficient than water alone. During the warm water trials T_{es} was lower than T_{re} or T_{pill} , which may be due to a lower heat capacity of the esophagus, thus a closer reflection of blood temperature. These explanations are

speculative, but might suggest some considerations for selecting a measurement method.

The telemetry pill has been criticized as subject to variations in temperature that occur due to its movement through the gastrointestinal tract (Kolka et al., 1993; Livingstone et al., 1983). This effect was not evident during the 3-h trials in which temperature was monitored in this study. Since the subjects took the telemetry pill 12 h before the trial, versus 2-3 h in previous studies (Kolka et al., 1993), fluctuation in temperature as the pill passed through the stomach and past the liver (commonly cited as areas of temperature variability) may have been avoided. Temperature in the small and large intestines is probably more uniform than in the upper portion of the gastrointestinal tract. Further study of pill temperature variations over the entire time course of pill transit through the gastrointestinal tract is required to confirm this speculation. However, the magnitude of fluctuation attributed to pill movement, 0.2-0.3°C (Kolka et al., 1993), is not likely to be of physiological significance for many applications. In addition, while T_{es} and T_{re} have the benefit of a fixed anatomical position, these measurements are often not practical for assessing core temperature in studies involving large numbers of free-living, ambulatory test subjects. For those and other applications, a telemetry pill system is a valid alternative for assessing core temperature.

In summary, this study demonstrates that the ingestible temperature telemetry pill system provides a valid measurement of core temperature during both rest and exercise in cold as well as warm conditions. Further study, however, to better quantify the variation in core temperature measured by the pill as it transits the gastrointestinal tract is warranted. The pill system is particularly appropriate for monitoring core temperature in field environments where other techniques are not feasible.

REFERENCES

Department of the Army. The Army Weight Control Program. Washington, D.C., AR 600-9, 1986.

Haslam, R.A. and K.C. Parsons. An evaluation of computer based models that predict human responses to the thermal environment. ASHRAE Transactions, 94:1342-1360, 1988.

Kolka, M.A., M.D. Quigley, L.A. Blanchard, D.A. Toyota, and L.A. Stephenson. Validation of a temperature telemetry system during moderate and strenuous exercise. J Therm Biol, 18:203-210, 1993.

Livingstone, S.D., J. Grayson, J. Frim, C.L. Allen, and R.E. Limmer. Effect of cold exposure on various sites of core temperature measurements. J Appl Physiol, 54:1025-1031, 1983.

Sawka, M.N. and C.B. Wenger. Physiological responses to acute exercise-heat stress. In: Human Performance Physiology and Environmental Medicine at Terrestrial Extremes, K.B. Pandolf, M.N. Sawka, and R.R. Gonzalez (Eds.). Benchmark Press, Inc. Indianapolis, 1988, pp. 97-151.

Shapiro, Y., B.A. Avellini, M.M. Toner, and K.B. Pandolf. Modification of the Monark bicycle ergometer for underwater exercise. J Appl Physiol, 50:679-683, 1981.

Sparling, P.B., T.K. Snow, and M.L. Millard-Stafford. Monitoring core temperature during exercise: ingestible sensor vs. rectal thermistor. Aviat Space Environ Med, 64:760-763, 1993.

DISTRIBUTION LIST

2 Copies to:

Defense Technical Information Center
8725 John J. Kingman Road, STE 0944
Fort Belvoir, VA 22060-6218

Office of the Assistant Secretary of Defense (Health Affairs)
ATTN: Medical Readiness, Pentagon
Washington DC 20301-0103

Commander
US Army Medical Research and Materiel Command
ATTN: MCMR-OP
Fort Detrick MD 21702-5012

Commander
U.S. Army Medical Research and Materiel Command
ATTN: MCMR-PLC
Fort Detrick MD 21702-5012

Commander
U.S. Army Medical Research and Materiel Command
ATTN: MCMR-PLE
Fort Detrick MD 21702-5012

Commandant
Army Medical Department Center and School
ATTN: HSMC-FR, Bldg. 2840
Fort Sam Houston TX 78236

1 Copy to:

Deputy Director for Medical Readiness, Joint Chiefs of Staff, J4
ATTN: J4-MRD
4000 Joint Staff, Pentagon
Washington DC 20318-4000

HQDA
Assistant Secretary of the Army
(Research, Development and Acquisition)
ATTN: SARD-TM, Pentagon
Washington DC 20316-0103

HQDA
Office of the Surgeon General
Assistant Surgeon General
ATTN: DASG-RDZ/Executive Assistant Surgeon General
Room 3E368, Pentagon
Washington DC 20310-2300

HQDA
Office of the Surgeon General
ATTN: DASG-ZA
5109 Leesburg Pike
Falls Church VA 22041-3258

HQDA
Office of the Surgeon General
ATTN: DASG-DB
5109 Leesburg Pike
Falls Church VA 22041-3258

HQDA
Office of the Surgeon General
ATTN: DASG-MS
5109 Leesburg Pike
Falls Church VA 22041-3258

HQDA
Office of the Surgeon General
Preventive Medicine Consultant
ATTN: SGPS-PSP
5109 Leesburg Pike
Falls Church VA 22041-3258

Uniformed Services University of the Health Sciences
4301 Jones Bridge Road
Bethesda MD 20814-4799

Uniformed Services University of the Health Sciences
ATTN: Department of Preventative Medicine
4301 Jones Bridge Road
Bethesda MD 20814-4799

Commandant
Army Medical Department Center & School
ATTN: Chief Librarian Stimson Library
Bldg 2840, Room 106
Fort Sam Houston TX 78234-6100

Commandant
Army Medical Department Center & School
ATTN: Director of Combat Development
Fort Sam Houston TX 78234-6100

Commander
U.S. Army Aeromedical Research Laboratory
ATTN: MCMR-UAX-SI
Fort Rucker AL 36362-5292

Commander
U.S. Army Medical Research Institute of Chemical Defense
ATTN: MCMR-UVZ
Aberdeen Proving Ground MD 21010-5425

Commander
U.S. Army Medical Materiel Development Activity
ATTN: MCMR-UMZ
Fort Detrick MD 21702-5009

Commander
U.S. Army Institute of Surgical Research
ATTN: MCMR-USZ
Fort Sam Houston TX 78234-5012

Commander
U.S. Army Medical Research Institute of Infectious Diseases
ATTN: MCMR-UIZ-A
Fort Detrick MD 21702-5011

Director
Walter Reed Army Institute of Research
ATTN: MCMR-UWZ-C (Director for Research Management)
Washington DC 20307-5100

Commander
U.S. Army Soldier's Systems Command
ATTN: ANSSC-CG
Natick MA 01760-5000

Commander
U.S. Army Natick Research, Development & Engineering Center
ATTN: SSCNC-Z
Natick MA 01760-5000

Commander
U.S. Army Natick Research, Development & Engineering Center
ATTN: SSCNC-T
Natick MA 01760-5002

Commander
U.S. Army Natick Research, Development & Engineering Center
ATTN: SSCNC-S-IMI
Natick MA 01760-5040

Commander
U.S. Army Natick Research, Development & Engineering Center
ATTN: SSCNC-TM
U.S. Marine Corps Representative
Natick MA 01769-5004

Commander
U.S. Army Research Institute for Behavioral Sciences
5001 Eisenhower Avenue
Alexandria VA 22333-5600

Commander
U.S. Army Training and Doctrine Command
Office of the Surgeon
ATTN: ATMD
Fort Monroe VA 23651-5000

Commander
U.S. Army Center for Health Promotion and Preventative Medicine
Aberdeen Proving Ground MD 21010-5422

Director, Biological Sciences Division
Office of Naval Research - Code 141
800 N. Quincy Street
Arlington VA 22217

Commanding Officer
Naval Medical Research & Development Command
NNMC/Bldg 1
Bethesda MD 20889-5044

Commanding Officer
U.S. Navy Clothing & Textile Research Facility
ATTN: NCTRF-01, Bldg 86
Natick MA 01760-5000

Commanding Officer
Navy Environmental Health Center
2510 Walmer Avenue
Norfolk VA 23513-2617

Commanding Officer
Naval Aerospace Medical Institute (Code 32)
Naval Air Station
Pensacola FL 32508-5600

Commanding Officer
Naval Medical Research Institute
Bethesda MD 20889

Commanding Officer
Naval Health Research Center
P.O. Box 85122
San Diego CA 92138-9174

Commander
Armstrong Medical Research Laboratory
Wright-Patterson Air Force Base OH 45433

U.S. Airforce Aeromedical Library
Document Services Section
2511 Kennedy Circle
Brooks Air Force Base TX 78235-5122

Commander
USAF School of Aerospace Medicine
Brooks Air Force Base TX 78235-5000

Director
U.S. Army Research Laboratory
Human Research & Engineering Directorate
Aberdeen Proving Ground MD 21005-5001

Commander
U.S. Army Military History Institute
ATTN: Chief, Historical Reference Branch
Carlisle Barracks
Carlisle PA 17013-5008

U.S. Army Biomedical R&D Representative for Science
and Technology Center, Far East
ATTN: AMC-S&T, FE Unit 45015
APO AP 96343-5015

Director
Defence and Civil Institute of Environmental Medicine
1133 Sheppard Avenue W.
P.O. Box 200
Downsview, Ontario Canada M3M 3B9

Department of National Defence, CANADA
Defence Research Establishment Ottawa
ATTN: Head Physiology Group
Environmental Protection Section, Protective Sciences Division
Ottawa, Ontario Canada K1A 0Z4

Head, Environmental Physiology Section
Defence and Civil Institute of Environmental Medicine
1133 Sheppard Avenue W.
P.O. Box 200
Downsview, Ontario Canada M3M 3B9

National Defence Headquarters, CANADA
ATTN: Research and Development Branch
Human Performance Directorate
305 Rideau Street
Ottawa Ontario Canada K1A0K2