

ARMY RESEARCH LABORATORY



# Enhancing Biological Detection With Dendrimer-Based Immunosensors

by Amanda L. Jenkins, Kate K. Ong, and Ray Yin

ARL-TR-2593

September 2001

Approved for public release; distribution is unlimited.

20011120 036

# Army Research Laboratory

Aberdeen Proving Ground, MD 21005-5069

---

ARL-TR-2593

September 2001

---

## Enhancing Biological Detection With Dendrimer-Based Immunosensors

Amanda L. Jenkins, Kate K. Ong, and Ray Yin  
Weapons and Materials Research Directorate, ARL

---

Approved for public release; distribution is unlimited.

---

---

## Abstract

---

Dendrimers are highly branched, tree-like polymers that possess precise size and shape, as well as surface groups. Among them, polyamidoamine dendrimers are the most widely studied water-soluble/biocompatible dendritic macromolecules. Such dendrimers have been exploited for interesting applications in immunodiagnostics, magnetic resonance imaging, gene therapy, and drug delivery. This report introduces a new signal amplification strategy using dendrimers. While only one fluorescein group can be linked onto an antibody molecule, a large number of fluorophores can be attached to an antibody through a dendrimer linker molecule, thus forming a water-soluble fluorescein-dendrimer-antibody bioconjugate. Upon addition of the antigen, enhanced fluorescence signals are obtained when compared with the corresponding fluorescein-antibody analogs.

---

## Acknowledgments

---

We gratefully acknowledge Ms. Janet Jensen of the Joint Service Agent Water Monitor Program and Dr. H. Dupont Durst of the Edgewood Chemical and Biological Command for financial support of this project.

INTENTIONALLY LEFT BLANK.

---

## Contents

---

<b>Acknowledgments</b>	<b>iii</b>
<b>List of Figures</b>	<b>vii</b>
<b>List of Tables</b>	<b>ix</b>
<b>1. Introduction</b>	<b>1</b>
<b>2. Experimental</b>	<b>1</b>
2.1 Reagents.....	1
2.2 Sample Preparation.....	2
2.3 Instrumentation.....	2
<b>3. Results and Discussion</b>	<b>2</b>
3.1 Antibody-FITC Bioconjugate.....	2
3.2 Antibody-Dendrimer-FITC Bioconjugate.....	3
3.3 Dendrimer-FITC Bioconjugates.....	5
<b>4. Conclusions</b>	<b>7</b>
<b>5. References</b>	<b>9</b>
<b>Distribution List</b>	<b>11</b>
<b>Report Documentation Page</b>	<b>13</b>

INTENTIONALLY LEFT BLANK.

---

## List of Figures

---

Figure 1. Fluorescent microscopic images (40×) of antibody-fluorescein bioconjugates (a) without bot toxoid and (b) with bot toxoid.....	3
Figure 2. Fluorescent microscopic images (40×) of (a) PBS buffer and (b) bot toxoid. ....	4
Figure 3. Fluorescent microscopic images (40×) of antibody-dendrimer-fluorescein bioconjugate A (a) without bot toxoid and (b) with bot toxoid. ....	4
Figure 4. Fluorescent microscopic images (40×) of ab-dendrimer (B)-fluorescein conjugates (a) without bot toxoid and (b) with bot toxoid. ....	5
Figure 5. Upon reaction with antibody (red)-dendrimer (circle)-fluorescein (green) bioconjugate A and the bot toxoid (blue), highly crosslinked, dense immunoclusters formed immediately. ....	6

INTENTIONALLY LEFT BLANK.

---

## List of Tables

---

Table 1. Antibody-dendrimer-fluorescein ratios. ....	2
--	---

INTENTIONALLY LEFT BLANK.

---

## 1. Introduction

---

Immunoassays have been widely used in medical diagnostics and environmental sensing [1-4]. Such assays often involve an immunocomplex formation resulting from antibody (Ab)-antigen (Ag) binding reactions. This process, however, does not generate signals that can be readily visualized by the optical microscope. Therefore, a signal generator or a tag molecule (i.e., a fluorescent [Fl] dye) is conjugated onto antibodies for real-time imaging purposes [5]. The sensitivity of this assay often directly correlates with the dye density or the number of dye molecules per antibody. Higher dye density will result in better sensitivity. However, due to the hydrophobic nature of the fluorescent dyes, the attachment of multiple dye molecules onto an antibody often causes severe precipitation problems in buffer. Thus, the sensitivity enhancement based on multiple dye attachment is greatly limited.

On the other hand, polyamidoamine (PAMAM) dendrimers are multifunctional, water-soluble macromolecules that are capable of bearing multiple dyes and antibodies [6-7]. In this report, the fluorescent signals generated from antibody-fluorescein (Ab-Fl) and antibody-dendrimer-fluorescein (Ab-Den-Fl) conjugates, as well as their immunocomplexes with antigens, will be directly compared.

---

## 2. Experimental

---

### 2.1 Reagents

Polyamidoamine (PAMAM) dendrimers (generation 5, E5) were purchased from Dendritech, Inc., Midland, MI. Anti-bot (bot) toxin Fab and bot toxoid were obtained from the U. S. Army Edgewood Chemical and Biological Center, Aberdeen Proving Ground-Edgewood Area, MD. Fluorescein dye (FITC) was purchased from Sigma. Antibody-FITC, antibody-dendrimer-FITC (A and B), and dendrimer-FITC conjugates were prepared using procedures described previously [8]. The antibody bioconjugate samples were diluted in 10 mM phosphate buffered saline (PBS) pH 7.4 (Sigma Chemical, St. Louis, MO) to a final concentration of 100  $\mu\text{g}/\text{mL}$ . The dendrimer-FITC bioconjugate was diluted with 10-mM PBS to a final optical density of 0.6. The antigen (bot toxoid) was diluted to a concentration of 2.5  $\mu\text{g}/\text{mL}$  with 10-mM PBS.

## 2.2 Sample Preparation

Equal volume solutions of bioconjugate (i.e., 100 µg/mL) and bot toxoid (2.5 µg/mL) were mixed, and the resulting mixture was immediately transferred to a microscope slide cleaned with a solution of 0.5-M sodium hydroxide in 25% methanol prior to use. The formation of immunocomplexes was visualized through an optical microscope.

## 2.3 Instrumentation

Visualization was achieved using an Olympus BX40 (Opelco, Sterling, VA) optical microscope equipped with an epi-fluorescence attachment. The sample spots were excited with a xenon-mercury lamp using a 450-480 nm band pass filter recommended for FITC observation. All observations were made with a 40x objective, and images were captured using a charge-coupled device (CCD) camera (Optronics, Goleta, CA). The images were imported into Adobe Photoshop 5.0, whereby the sample brightness was based on luminosity measurements and the sample size was based on number of pixels. The pixel size was then converted into micron size using an NIST-traceable magnification reference standard (Geller Microanalytical Laboratory, MA) that was imaged under the same conditions as the sample.

---

## 3. Results and Discussion

---

A series of fluorescein-containing bioconjugates was utilized for this study. The ratios of antibody, dendrimer, and fluorescein in different bioconjugates are listed in Table 1.

Table 1. Antibody-dendrimer-fluorescein ratios.

Sample	Ratio of Ab-Den-FI
Antibody-FI	1: 0: 1
Antibody-Dendrimer-FI (A)	2: 1: 10
Antibody-Dendrimer-FI (A)	1: 1: 10
Dendrimer-FI	0: 1: 10

### 3.1 Antibody-FITC Bioconjugate

Antibody-FITC (Ab-FI) bioconjugates, as well as their immunocomplexes formed with bot toxoid, were directly imaged using a fluorescence microscope, as seen in Figure 1. Aggregates were observed in both cases. The former appeared to be more uniform in size and brightness, while the latter consisted of slightly larger and brighter spots. The luminosity reading obtained by Adobe Photoshop 5.0 measured 210 for the antibody-fluorescein bioconjugate and 233 for the aggregate.

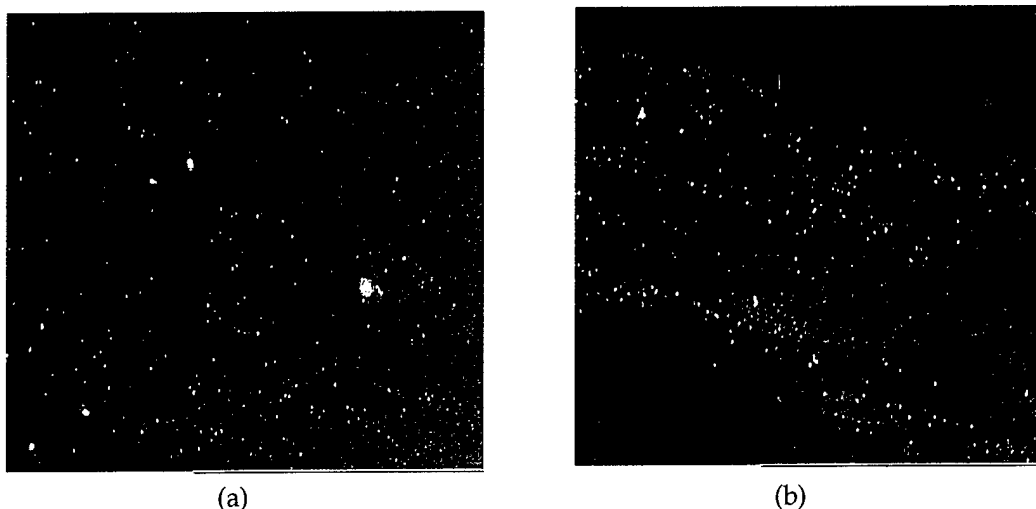


Figure 1. Fluorescent microscopic images (40 $\times$ ) of antibody-fluorescein bioconjugates (a) without bot toxoid and (b) with bot toxoid.

The stronger background observed in Figure 1(a) was not too surprising, since the introduction of FITC made the Ab-FI bioconjugates more hydrophobic. When dissolved in PBS buffer, these bioconjugates formed physical aggregates due to the hydrophobic association of the dye molecules. As a result, a micelle-like aggregate with fluorophores at its interior was produced. Such aggregates were very uniform in size, as seen in Figure 1(a). In the presence of bot toxoid, antibodies started to react with multivalent bot antigens, thus forming larger immuno clusters. As indicated in Figure 1(b), these clusters were approximately twofold larger than the physical aggregates. On the other hand, neither PBS buffer (a) nor bot toxoid (b) emitted observable fluorescence in this excitation range, as shown in Figure 2. This eliminated the possibility of background fluorescence and indicated that the larger, brighter spots indeed resulted from the immunocomplex formation.

### 3.2 Antibody-Dendrimer-FITC Bioconjugate

While maintaining the same ratio of the dendrimer and FITC, two paired samples, antibody-dendrimer-FITC (Ab-Den-FI) bioconjugate A and B, were prepared by varying the number of antibodies on a dendrimer. Ab-Den-FI bioconjugate A consisted of two antibody molecules per dendrimer, whereas Ab-Den-FI B only contained one antibody molecule per dendrimer. In the absence of bot toxoid, both bioconjugate A and B formed a uniform film, and no bright aggregate spots were observed, as shown in Figures 3(a) and 4(a). Upon addition of bot toxoid, larger immunoclusters immediately formed in both cases (Figures 3[b] and 4[b]). However, the clusters generated from bioconjugate A appeared noticeably larger and brighter with a luminosity reading of 260 (Figure 3[b]). The luminosity reading measured for bioconjugate B was 240. In both

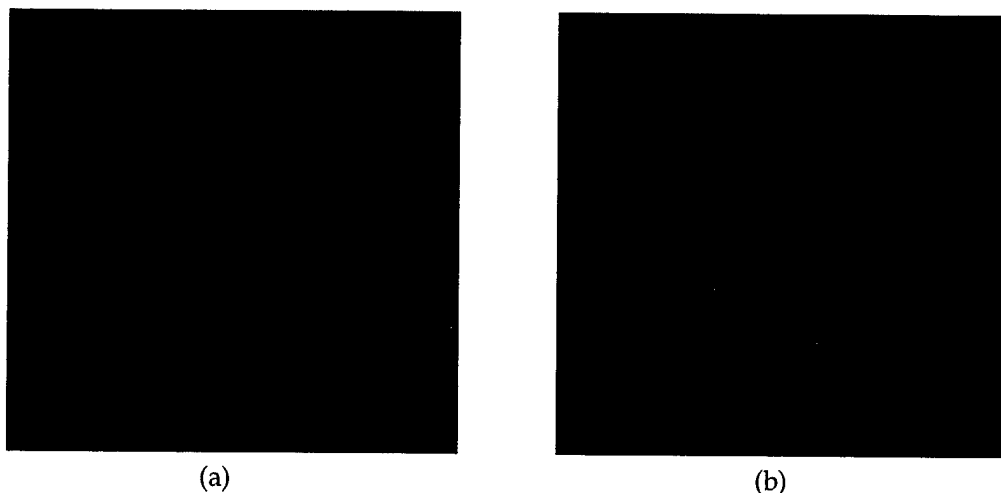


Figure 2. Fluorescent microscopic images (40 $\times$ ) of (a) PBS buffer and (b) bot toxoid.

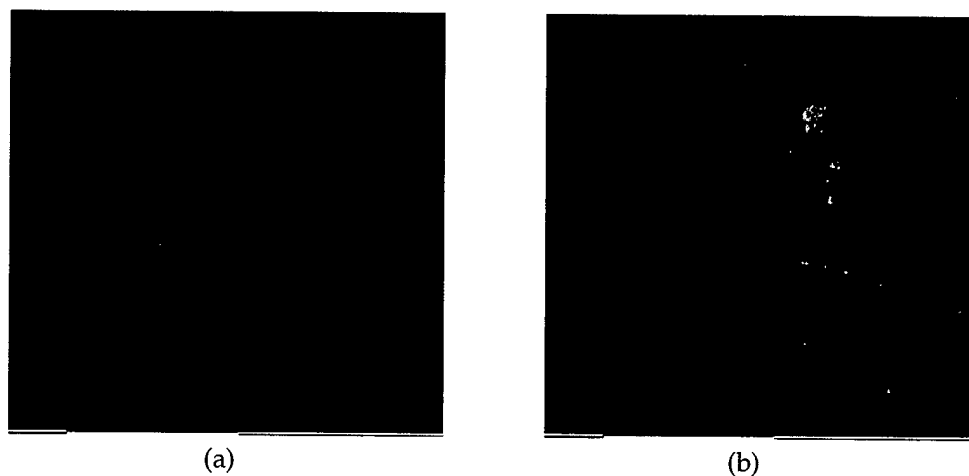


Figure 3. Fluorescent microscopic images (40 $\times$ ) of antibody-dendrimer-fluorescein bioconjugate A (a) without bot toxoid and (b) with bot toxoid.

cases, the intensity of the fluorescence signals from these clusters was significantly stronger than the corresponding Ab-FI bioconjugates (Figure 1[b]).

The cleaner background obtained from the Ab-Den-FI bioconjugates (A and B) suggested that dendrimers were better water-soluble linkers for hydrophobic dyes such as FITC. The addition of a dendrimer linker between organic dyes and antibodies apparently facilitated the dissociation of the physical aggregates or micelles present in the solution. Thus, no bright aggregated spots were observed (Figure 3[a]). Since bioconjugates A and B possessed the same number of FITC groups, the stronger fluorescence intensity observed with bioconjugate A (after

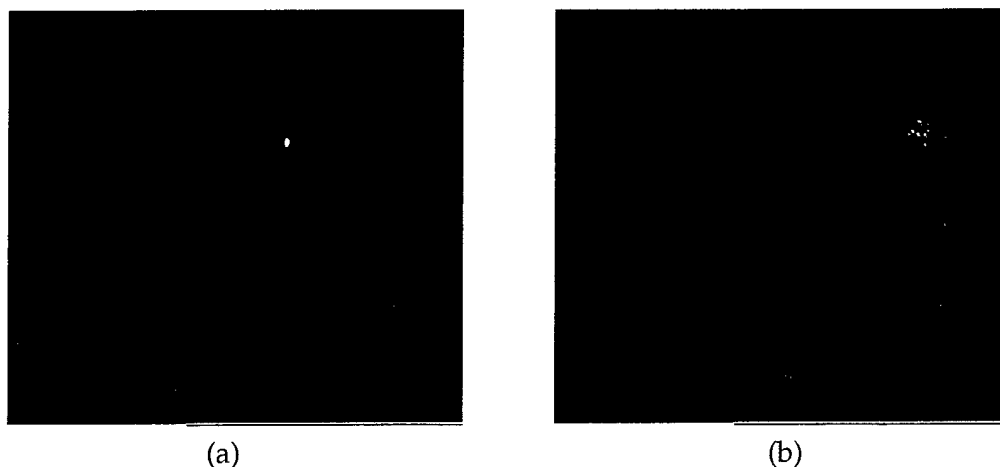


Figure 4. Fluorescent microscopic images (40 $\times$ ) of ab-dendrimer(B)-fluorescein conjugates (a) without bot toxoid and (b) with bot toxoid.

the addition of bot toxoid) was likely due to the presence of multiple antibodies within the bioconjugate. Typically, two antibody molecules were attached to each dendrimer in bioconjugate A; each bot toxoid exhibited multiple binding sites, highly crosslinked, dense immunoclusters that rapidly formed upon mixing (Figure 5). In contrast, only loose clusters were produced when mixing bioconjugate B with bot toxoid, resulting in much weaker fluorescent signals. The dendrimer linker not only enhanced the dye solubility in water, but also allowed multiple fluorescein and antibody attachment, thus greatly increasing the dye density on the antibody. As a result, the detection sensitivity was significantly enhanced. This was in sharp contrast with the conventional linkers that only allowed a single dye or receptor attachment and did not help to solubilize the resulting bioconjugates.

The bioconjugation process did not alter the antibody performance. Instead, signal enhancement was obtained from bioconjugates containing multiple dyes and antibodies.

### 3.3 Dendrimer-FITC Bioconjugates

To demonstrate the possibility of nonspecific binding occurrence, dendrimer-FITC bioconjugate samples were tested alone and in the presence of bot toxoid. The dendrimer-FITC bioconjugate itself fluoresced brightly; however, no aggregates were observed. When an equal volume solution of bot toxoid was added to the sample, no aggregates were observed.

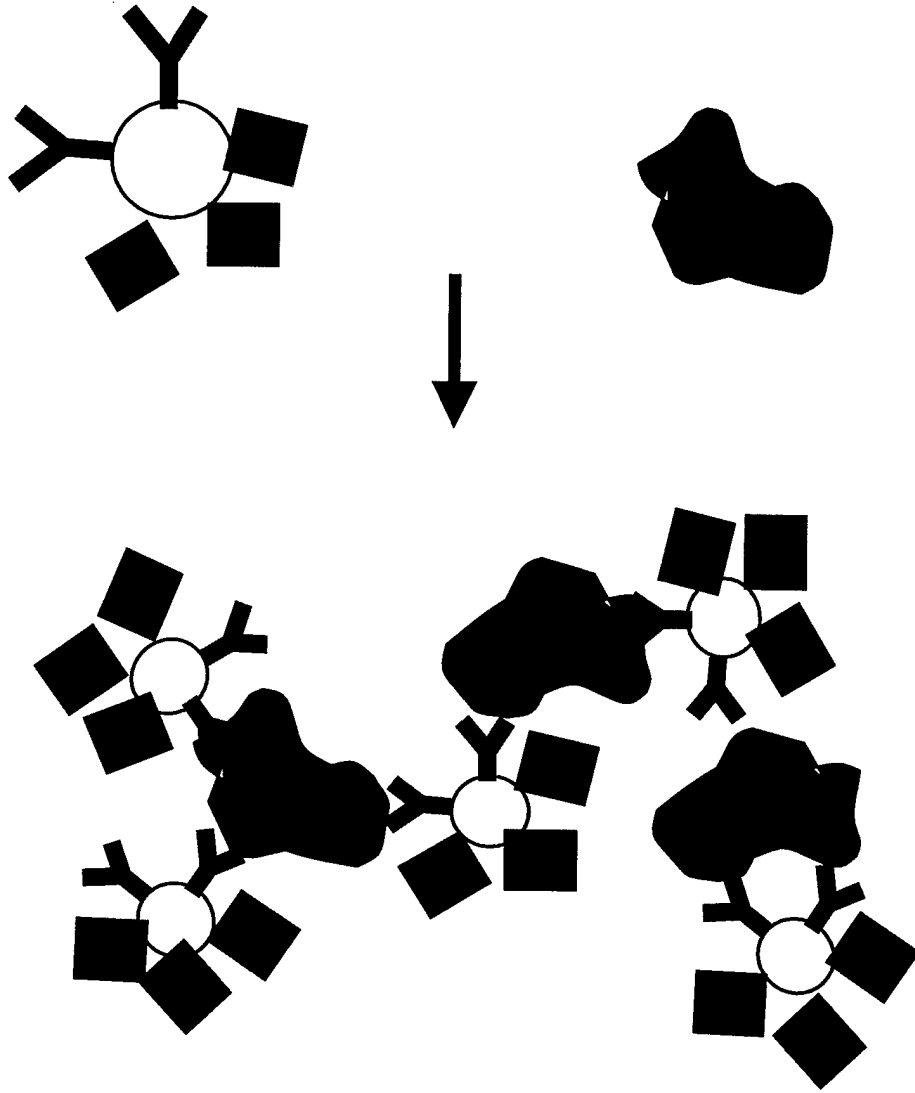


Figure 5. Upon reaction with antibody (red)-dendrimer (circle)-fluorescein (green) bioconjugate A and the bot toxin (blue), highly crosslinked, dense immunoclusters formed immediately.

This result suggested that in the absence of anti-bot toxin Fab, dendrimer-FITC conjugates alone were not capable of reacting or interacting with the bot toxin, as evidenced by the absence of immunoclusters. Therefore, the antibody-antigen reactions were the main cause for the formation of immunoclusters, and the nonspecific binding was not present between the dendrimer and the bot toxin.

---

## 4. Conclusions

---

Visualization of Ab-Den-FI bioconjugates as well as their immunoclusters has been successfully achieved using fluorescence microscopy. Using this technique, the immunoreactions between anti-bot-dendrimer-FITC bioconjugates and the bot toxoid can be directly studied and imaged in real time. Bioconjugates containing multiple dyes and antibodies tend to give more intense fluorescence signals, thus better assay sensitivity. Non-specific binding is not observed between the dendrimer-FITC bioconjugate and the bot toxoid. Multifunctional linkers such as dendrimers can be used as a general signal amplification strategy for immunoassays and other receptor-based assays.

INTENTIONALLY LEFT BLANK.

---

## 5. References

---

1. Price, C. P., and D. J. Newman (editors). *Principles and Practice of Immunoassay*. Second edition, New York: Stockton, 1997.
2. Harris, B. *TIBTECH*, vol. 17, p. 290, 1999.
3. Hermann, T. W. *Chem Anal*, vol. 42, p. 1, 1997.
4. Van Emon, J. M., and C. J. Gerlach. *Microbiol. Methods*, vol. 32, pp. 121-126, 1998.
5. Herman, B., and J. J. LeMasters, Editors. *Optical Microscopy: Emerging Methods and Applications*. New York: Academic Press, 1990.
6. Tomalia, D., A. M. Naylor, and W. A. Goddard III. *Angew Chem. Int. Ed. Engl*, vol. 29, pp. 138-144, 1990.
7. Frechet, J. M. J. *Science*, vol. 263, pp. 1710-1718, 1994.
8. Yoshitake, S., Y. Yamada, E. Ishikawa, and R. Masseyeff. *Eur. J. Biochem*, vol. 101, pp. 395-399, 1979.

INTENTIONALLY LEFT BLANK.

<u>NO. OF COPIES</u>	<u>ORGANIZATION</u>
2	DEFENSE TECHNICAL INFORMATION CENTER DTIC OCA 8725 JOHN J KINGMAN RD STE 0944 FT BELVOIR VA 22060-6218
1	HQDA DAMO FDT 400 ARMY PENTAGON WASHINGTON DC 20310-0460
1	OSD OUSD(A&T)/ODDR&E(R) DR R J TREW 3800 DEFENSE PENTAGON WASHINGTON DC 20301-3800
1	COMMANDING GENERAL US ARMY MATERIEL CMD AMCRDA TF 5001 EISENHOWER AVE ALEXANDRIA VA 22333-0001
1	INST FOR ADVNCD TCHNLGY THE UNIV OF TEXAS AT AUSTIN 3925 W BRAKER LN STE 400 AUSTIN TX 78759-5316
1	US MILITARY ACADEMY MATH SCI CTR EXCELLENCE MADN MATH THAYER HALL WEST POINT NY 10996-1786
1	DIRECTOR US ARMY RESEARCH LAB AMSRL D DR D SMITH 2800 POWDER MILL RD ADELPHI MD 20783-1197
1	DIRECTOR US ARMY RESEARCH LAB AMSRL CI AI R 2800 POWDER MILL RD ADELPHI MD 20783-1197

<u>NO. OF COPIES</u>	<u>ORGANIZATION</u>
3	DIRECTOR US ARMY RESEARCH LAB AMSRL CI LL 2800 POWDER MILL RD ADELPHI MD 20783-1197
3	DIRECTOR US ARMY RESEARCH LAB AMSRL CI IS T 2800 POWDER MILL RD ADELPHI MD 20783-1197
	<u>ABERDEEN PROVING GROUND</u>
2	DIR USARL AMSRL CI LP (BLDG 305)

NO. OF  
COPIES ORGANIZATION

3 US ARMY EDGEWOOD  
BIO CHEM CTR  
AMSSB RRT  
W LEOROP  
D DURST  
J JENSEN  
BLACKHAWK RD  
EDGEWOOD MD 21010

# REPORT DOCUMENTATION PAGE

Form Approved  
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project(0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE September 2001	3. REPORT TYPE AND DATES COVERED Summary, January 2000–March 2001	
4. TITLE AND SUBTITLE Enhancing Biological Detection With Dendrimer-Based Immunosensors			5. FUNDING NUMBERS 622105.AH84	
6. AUTHOR(S) Amanda L. Jenkins, Kate K. Ong, and Ray Yin				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) U.S. Army Research Laboratory ATTN: AMSRL-WM-MA Aberdeen Proving Ground, 21005-5069			8. PERFORMING ORGANIZATION REPORT NUMBER ARL-TR-2593	
9. SPONSORING/MONITORING AGENCY NAMES(S) AND ADDRESS(ES) Joint Service Agent Water Monitor Program (JSAWM) U.S. Army Edgewood Biological Chemical Center, AMSSB-RRT, Blackhawk Road, Edgewood, MD 21010			10. SPONSORING/MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution is unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) Dendrimers are highly branched, tree-like polymers that possess precise size and shape, as well as surface groups. Among them, polyamidoamine dendrimers are the most widely studied water-soluble/biocompatible dendritic macromolecules. Such dendrimers have been exploited for interesting applications in immunodiagnostics, magnetic resonance imaging, gene therapy, and drug delivery. This report introduces a new signal amplification strategy using dendrimers. While only one fluorescein group can be linked onto an antibody molecule, a large number of fluorophores can be attached to an antibody through a dendrimer linker molecule, thus forming a water-soluble fluorescein-dendrimer-antibody bioconjugate. Upon addition of the antigen, enhanced fluorescence signals are obtained when compared with the corresponding fluorescein-antibody analogs.				
14. SUBJECT TERMS dendrimers, fluorescence, immunosensors, antibodies			15. NUMBER OF PAGES 17	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT UNCLASSIFIED	18. SECURITY CLASSIFICATION OF THIS PAGE UNCLASSIFIED	19. SECURITY CLASSIFICATION OF ABSTRACT UNCLASSIFIED	20. LIMITATION OF ABSTRACT UL	

INTENTIONALLY LEFT BLANK.