

AD \_\_\_\_\_

Award Number: DAMD17-99-1-9374

TITLE: The CAD Method for Microcalcification Detection:  
Independent of Sensor and Resolution

PRINCIPAL INVESTIGATOR: Wei Qian, Ph.D.

CONTRACTING ORGANIZATION: University of South Florida  
Tampa, Florida 33620-7900

REPORT DATE: July 2001

TYPE OF REPORT: Annual Summary

PREPARED FOR: U.S. Army Medical Research and Materiel Command  
Fort Detrick, Maryland 21702-5012

DISTRIBUTION STATEMENT: Approved for Public Release;  
Distribution Unlimited

The views, opinions and/or findings contained in this report are those of the author(s) and should not be construed as an official Department of the Army position, policy or decision unless so designated by other documentation.

20011212 166

# REPORT DOCUMENTATION PAGE

Form Approved  
OMB No. 074-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing this collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503

1. AGENCY USE ONLY (Leave blank)	2. REPORT DATE July 2001	3. REPORT TYPE AND DATES COVERED Annual Summary (1 Jul 00 - 30 Jun 01)
----------------------------------	-----------------------------	---

4. TITLE AND SUBTITLE The CAD Method for Microcalcification Detection: Independent of Sensor and Resolution	5. FUNDING NUMBERS DAMD17-99-1-9374
--	--

6. AUTHOR(S) Wei Qian, Ph.D.
---------------------------------

7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) University of South Florida Tampa, Florida 33620-7900 E-Mail: qlanw@moffitt.usf.edu	8. PERFORMING ORGANIZATION REPORT NUMBER
---	--

9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES) U.S. Army Medical Research and Materiel Command Fort Detrick, Maryland 21702-5012	10. SPONSORING / MONITORING AGENCY REPORT NUMBER
---	--

11. SUPPLEMENTARY NOTES

12a. DISTRIBUTION / AVAILABILITY STATEMENT Approved for Public Release; Distribution Unlimited	12b. DISTRIBUTION CODE
---	------------------------

13. Abstract (Maximum 200 Words) (abstract should contain no proprietary or confidential information)

The aims of this work are to explore the feasibility of developing a *new class* of computer assisted diagnostic (CAD) methods for microcalcification cluster (MCC) detection for breast cancer screening using digital mammography. The objectives are to achieve: (a) improved CAD performance that is significantly more robust for large image databases, and (b) an *adaptive* CAD method that is independent of the digital sensor resolution and gray scale characteristics; for the first time.

The proposed method is novel in concept and is based on pioneering experience in development of adaptive CAD algorithms including linear wavelet transforms and non linear transforms for improved feature extraction, their implementation of filter banks that uniquely allow adaptive approaches, and experience in specialized multi-stage neural networks for detection of MCC's with different feature input strategies. The intent is to compare existing wavelet methods to the proposed new method and evaluate them for a *common case* data base using a state of the art direct digital detector and film (three digitizers)

14. SUBJECT TERMS digital mammography, computer-aided diagnosis	15. NUMBER OF PAGES 17
	16. PRICE CODE

17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT Unlimited
---	--	---	---

## Table of Contents

Cover.....	1
SF 298.....	2
Table of Contents.....	3
Introduction.....	4
Body.....	5-10
Key Research Accomplishments.....	10
Reportable Outcomes.....	10-11
Conclusions.....	11
References.....	11-14
Appendices.....	15-16

## Introduction:

The aims of this work are to explore the feasibility of developing a *new class* of computer assisted diagnostic (CAD) methods for microcalcification cluster (MCC) detection for breast cancer screening using digital mammography. The objectives are to achieve: (a) improved CAD performance that is significantly more robust for large image data bases, and (b) an *adaptive* CAD method that is independent of the digital sensor resolution and gray scale characteristics; for the first time. This report includes 2 sections, **(1). Summary of the work in first year, which includes data base collection and truth file establishment for different sensors, preprocessing for breast area segmentation, and basic algorithm design, (2). Algorithm design and optimization**, which includes a design of a successful MCCs detection system containing the design and optimization of all modules. The detail of our progress is summarized in our recent publications [1, 2, 3, 4, 5]. *A CAD method with improved and robust performance is required for both retrospective studies and an steps towards a more generalizable CAD method, which is critical for multi-center clinical trials.* The proposed method is novel in concept and is based on pioneering experience in development of adaptive CAD algorithms including linear wavelet transforms and non linear transforms for improved feature extraction, their implementation of filter banks that uniquely allow adaptive approaches, and experience in specialized multi-stage neural networks for detection of MCC's with different feature input strategies. The intent is to compare existing wavelet methods to the proposed new method and evaluate them for a *common case* database using a state of the art direct digital detector and film (three digitizers).

## BODY OF REPORT

### I. Summary of the work completed in the first year of the project

#### (a). *Data base collection and truth file establishment for three sensors*

In order to make the CAD algorithms for clinical use, the extensive tests of our algorithms are necessary for larger database from different digitizers with different resolutions. The films of the two sets of 200 views was digitized with two different digitizers: (a) a CCD-based system (ImageClear R3000, DBA Systems, Inc, Melbourne, FL) maximum resolution at 30  $\mu$ m and 16 bits and (b) a LUMISCAN 85 (Lumisys, Sunnyvale, CA) at maximum resolution, at 50  $\mu$ m, and 12 bits. Digitized images will be acquired at 50 microns with one set transformed to 100microns respectively. And another one set from direct digital mammography system from General Electric which was installed at the H. Lee Moffitt Cancer Center and Research Institute (MCCRI) at USF in June 1998. The direct digital images have a spatial resolution of 100  $\mu$ m and 12 bits per pixel.

#### (b). *Preprocessing for breast area segmentation*

Except a few digital mammogram images are with high quality, most of them suffer from more or less extrinsic signals such as images of edges of original X-ray pictures, or large bright regions caused by the cutting of them, various notes made by doctors, uneven illumination, blurred edges due to the exposure of pictures. Sometimes such extrinsic signals in the digital mammogram images may affect the detection result seriously. In the first year, we developed an algorithm to erase the extrinsic signals. They are helpful for the detection.

#### (c). *Basic algorithm design*

Basic algorithm design includes nonlinear bank filter design, implementation and segmentation algorithm design and testing. The nonlinear filter design is based on multiresolution techniques. In the first year of the project, we have tested 20 different segmentation algorithms on MCCs segmentation, such as Relaxation, Digital Desk - adaptive, Fuzzy sets, Otsu's method for grey level histograms, iterative selection, Johannsen Kapur method for using entropy, two histogram peaks, Minimum error and mean, Black percentage, Pun method for using entropy, two histogram peaks, etc.

### II. Algorithm Design and Optimization in the current funding year (second year)

#### (a). *Concise technical review for our research background*

A successful MCC detection scheme should consist of several modules aiming at solving different kinds of signal processing problems [7-11]. All published work can be grouped in the following five-step paradigm: (1) breast area segmentation and artifact elimination, (2) MCC structure and normal tissue enhancement, (3) suspicious MCC area segmentation or localization, (4) feature extraction and analysis of suspicious areas, and (5) suspicious area classification as normal or abnormal. Most of the work in the literature addressed only one subset of these procedures and some approaches reorganized these steps [10], [12], [13], [14-23]; *i.e. rather than a holistic approach in this work*. Efforts at enhancing microcalcification structures to refine digital visualization [24]-[26] can be also be incorporated in the above paradigm.

**Enhancement methods.** All the microcalcification enhancement methods can be considered as a simple matched filter or spot detector conducted either at only *single or multiple scales* [8], [10], [16]-[18], [24], [27]-[29]. These methods are generally not robust or generalizable for the work proposed here(C and N). The enhancement step is important to maintain high detection sensitivity and low FP rate.

**Segmentation methods.** The segmentation can be divided into: (a) global segmentation, which should be considered as suspicious microcalcification localization and mostly realized by simple empirical thresholding [8], [14]-[18], [28], and (b) local segmentation directed at keeping geometrical features of each microcalcification [8], [14]. The general criterion for global segmentation is to get a detection result, i.e., in most cases a set of segmented areas, with acceptable sensitivity and false positive distribution for further classifications. We proposed to take more advanced global and local segmentation method.

**Feature extraction.** In general, feature extraction methods can be divided into implicit approaches training with ROI's within a single image as inputs to a NN [9], [10], [13], [30]-[32] and explicit approaches using indexes calculated from segmented regions or group of regions( ROIs) [8], [12], [21], [23], [33], [34], [37]. *Implicit Features:* There are several problems with implicit feature extraction, i.e., difficulty in incorporating clinical knowledge into the classification and difficulty in deciding ROIs size. *Explicit features:* Their extraction suffers from the limitation of feature design procedures based on human observation and clinical knowledge, which may ignore certain useful visual information. *All the approaches in the literature use either implicit or explicit feature extraction scheme, and are not optimized in a combined way for MCC detection.* Some methods use very small sets of features. Some features are used only at single microcalcification level, instead of the cluster level. Studies aimed at discrimination of microcalcifications and similar normal tissues are rare and coarse [33]. *There does not exist an approach for using both advanced feature extraction methods and inter-projection reference information, the latter is used radiologists to interpret an abnormality in mammograms [35], [36].*

**Classifier Design.** Design of classifiers is closely related to the feature extraction. A successful system requires a nonlinear feature combination mechanism. More advanced NN techniques are preferable to linear discriminant analysis and rule-based methods [37], [32]. *Multistage based NN approaches, combining both explicit and implicit features at different stages should prove to be more robust than either only implicit or only explicit feature based approaches.*

**CAD parameter optimization.** Reported methods are all based iteratively changing CAD parameters, such as image preprocessing and segmentation parameters, and manually generating computed FROC curves; a very time consuming process. *We have recently developed a fully automatic method for this optimization, including parameter changes within a parameter range as opposed to fixed parameters for adaptive CAD methods, together with generation of computer FROC and ROC analysis curves. This is a highly efficient optimization method critical to meet the objectives of this proposal.*

*(b). Algorithm Design and Optimization for proposed project*

**1. Introduction.** The research efforts involve design and optimization of all CAD modules as illustrated in Fig 1. We first implemented a robust CAD module of breast segmentation, already developed, that is generalizable to different sensors, a modification of a reported method. We then focused on the design and optimization of nonlinear filter banks based methods for MCC enhancement. This should be optimized to maintain a high detection sensitivity and low false positive rate. A CAD module for MCC identification criteria, which is an extension of previous work [38], should be modified for more accurate cluster extraction from binary images. Extraction of explicit features (inter-projection) should be greatly emphasized and as extension of our work on implicit features. Existing multistage based NN methods will still be adopted and optimized by using input both implicit and explicit features at different stages.

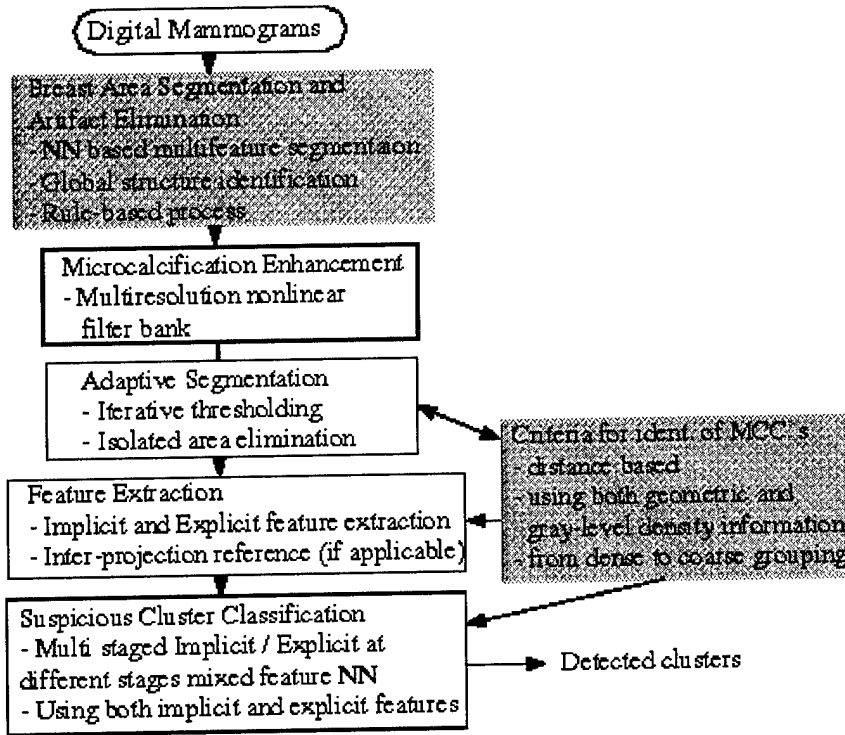


Fig.1. Block Diagram of the MCCs Detection System, Shaded areas have been fully completed. Preliminary progress has been made for all other CAD modules.

**2. Multiresolution microcalcification enhancement.** The basic structure of the proposed enhancement filter is similar to [29] and is shown in Fig.2a. The terminology for parameters is the same as [29]. The method is mathematically complex and is only briefly described here. Modifications proposed is the use of a multiresolution *nonlinear* filter bank, as shown in Fig. 2b., to replace a tree structured wavelet transform implemented on a linear filter bank, described in [29]. We have already done very preliminary testing of this method on simulated images and a representative mammographic image at 60 micron images, with a biopsy proven MCC's as shown in Fig 3, where details of microcalcifications were better preserved than using the 4 channel wavelet transform. *The feasibility of the method has been demonstrated.*




Fig.2a. Image enhancement scheme using hybrid adaptive multistage nonlinear filter (AMNF) and multiresolution nonlinear filter bank (NFB), where NFB is shown in Fig.2b.





Fig.2b. Multiresolution decomposition scheme with reconstruction using nonlinear filter bank (NFB).  $g_{NFB1}$  is the segmented results and  $g_{NFB2}(I, j)$  is the background image.




**Fig.3.** Representative result for MCCs segmentation of a subsection of a mammogram image ( $60 \mu\text{m}$  resolution ) containing 1 biopsy proven cluster; (a) Raw image, (b) and (c) 2 and 4 channel wavelet transform method respectively, and (d) preliminary data for non linear filter bank. Result in (b) and (c) do not fully delineate the cluster, preserve details of microcalcifications, or have too high FP detection rate. The method in (d) is not fully optimized and does not include all proposed CAD modules.

**3. Criteria for identification of clusters.** The measured performance of CAD methods for MCC detection is dependent on the specific criteria for identification of the “group of microclassifications” as a cluster. This has recently been addressed in a recent mammography workshop by Clarke and Nishakawa [6]. We proposed a distance-based area grouping method, instead of the commonly used kernel-based method, to avoid the problems of selection of kernel size and shape. We developed a method based on distance-based and from dense to coarse grouping strategy, this work has been submitted for publication and is attached [38]. Since we propose to evaluate the relative performance of the proposed adaptive CAD with a previously reported method[38], the impact of which criteria is not so critical.

**4. Adaptive Method for MCC Segmentation.** Segmentation methods generally used a fixed threshold for the full mammogram or an adaptive method to the full mammogram to segment MCCs. These methods are not optimum for FP reduction , especially for subtle MCCs. We propose to modify an existing method that is adaptive and iterative, where the criteria is unique. Preview methods generally focus on simple feature related criteria. The steps are as follows. First, segmented image is obtained for a given gray level threshold. If the clusters are larger than a geometrical criteria (i.e. fixed area:  $1.5 \times 1.5 \text{ cm}$ ) the threshold can be changed until the creterial is fully contained within this area. The process can be conducted in the inverse direction and the threshold adjustment step can be changed iteratively. This segmentation process directly eliminates the isolated areas. One solution to be investigated is to categorize image regions into several levels by a global segmentation. These regions may have some overlaps and the same adaptive MCC segmentation scheme can be used in all these regions. Since this segmentation scheme may control the FPs to manageable rate, the result obtained by adding segmented areas from different regions together may be suitable for further processing.

**5. Feature extraction.** This research step will mainly address explicit feature design and extraction. Implicit features, calculated within a single region of interest (ROI) as reported in the literature and used in our earlier work will be investigated, they include (1) microcalcification(s) area, (2) mean intensity, (3) deviation of intensity, (4) average edge gradient, (5) line-likeness, (6) contrast, and (7) number of MCC areas. They will be calculated from the original and enhanced image. We will also explore the use of generic algorithm(GA) for feature selection ranking but may defer most of this optimization step for the ROI proposal. The explicit features proposed include:

- extracting features from multiple domains, such as intensity, geometric.
- extracting both local features and global features, i.e., single calcification level, cluster level and more extended regional level.
- using multi-view reference information [35],( i.e., between CC view and ML view); statistical analysis combined with special case analysis, a specific-to-general philosophy.



*Fig.4. preliminary data for Inter-projection matching using pectoral muscle line as a proposed landmark. (a) and (b) are a CC view image and corresponding segmentation result and (c) and (d) are those for ML view. The true cluster is marked by a circle in each image. Dashed rulers in ML view images mark a wrong alignment direction for find relative positional correspondence. True cluster may possibly keep its distribution and shape patterns in two different views in which the breast was compressed differently during the imaging process. (Segmented areas are slightly dilated for rescaled presentation purpose.)*

**6. Correlation of Inter-projection features.** We will also explore inter-projection reference features, for suspicious cluster classification to improve detection sensitivity and reduce FP rate. The most difficult problem for using two-views (CC and ML) is the spatial matching between clusters. Since the breast is compressed, an exact alignment between two views may be impossible. In preliminary data we have found that the spatial correlation for two views along antero-posterior direction. As shown in Fig. 4, if the suspicious areas are found in upper parts of the views, the positional coherence should be approximately along Y-direction of images. Based on a feasible study over a considerable number of images, the Y-axis in CC view was found to correspond to the direction perpendicular to the pectoral muscle line in ML view; will play a key role in aligning the two views( Fig. 4). A matching procedure will be therefore proposed to match the set of clusters in one view as above using relaxation labeling techniques [39]. Additional explicit features will be explored such as similarity measurements between two clusters from the two views. They include : (1) Positional similarity, (2) Cluster size similarity, (3) Similarity of calcification number, (4) Similarity of average

calcification area, (5) Similarity of average intensity deviation within calcification areas, (6) Similarity of average elongation of calcification areas.

**7. Classifier design.** The classifier must combine both implicit and explicit features. To combine a considerable number of features is very difficult to realize in an analytical way and neural network methodologies have the advantages in dealing with this kind of nonlinear optimization problem through training procedures. Modifications to the NN design is required to address the great number of input nodes. A multistaged mixed feature neural network method is proposed based on our previous work for microcalcification detection [12], Kalman Filtering technique realized by the PI's group [12] will be used as a powerful tool for training a NN required for large number of input nodes and complex structures. The NN will have two stages to include input of implicit and explicit features at each stage, using previous experience in feed-forward NN's and backpropagation training as in [12].

### **Key Research Accomplishments**

- (1) Well done the whole system design and optimization.
- (2) Well done the enhancement module including multiresolution microcalcification cluster enhancement.
- (3) Well done the grouping criteria design for identification of microcalcification clusters.
- (4) Well done the adaptive method design for MCCs segmentation module.
- (5) Well done the feature extraction and analysis module including implicit feature and explicit features for digital mammograms.
- (6) Well done the correlation analysis for inter-projection features.
- (7) Well done the classification module design for classification of MCCs versus normal cases of mammograms.

### **Reportable Outcomes**

---Manuscripts, abstracts, presentations;

1. Wei Qian, Dansheng Song, Xuejun Sun, "Multistage statistical order with neural network for false positive reduction in full field digit mammography" on Nonlinear Signal and Image Processing June 3-6, 2001 Baltimore, USA
2. Wei Qian, Xuejun Sun, Dansheng Song, Robert A. Clark, "Digital mammography: Wavelet Transform and Kalman Filtering Neural Network in Mass Segmentation and Detection" Accepted by Academic Radiology, 2001
3. Wei Qian, Xuejun Sun, Dansheng Song, Robert A. Clark, "A Novel Hybrid Filter Architecture for Image Enhancement and Detection in Digital Mammography", Submitted to Computerized Medical Imaging and Graphics, 2001
4. L. Zhang, W. Qian, R.Sankar, D. Song, R.Clark, 'A New False Positive Reduction Method for MCCs Detection in Digital Mammography', International conference on acoustics speech, and signal processing May 7-11,2001 Salt Lake city, Utah

5. Dansheng Song, Wei Qian, Xuejun Sun, and Robert A Clark, "Neural Network for False Positive Reduction in Full Field Digital Mammography with Microcalcification Shape preservation," SPIE Multispectral Image Processing and Pattern Recognition, 22-24 Oct. 2001 Wuhan, China

**----- Degree obtained that are supported by this award ;**

Lin Zhang, got Master degree in March of 2001, He is currently working in CISCO Inc. in California.

Jie Lin, Working on Master degree, Will be finished in July of 2002.

**-----Funding applied for based on the work supported by this award;**

**Proposal Submitted to Agency: NIH, R01 on 02/01/21**  
A Telemammography Network for Underserved Area

**Proposal Submitted to Agency: U.S. Army Medical Research and Materiel Command DOD 2001 Breast Cancer Research Program**

1. Title: Telemedicine and Telemammography Using a Satellite Network for Remote Areas Including Oversea U.S. Military Bases
2. Title: Full Optimization of CAD System for Clinical Application
3. Title: A New CAD Scheme for the Detection of Tiny Mass Using Ipsilateral Multi-View Mammograms

## **Conclusion**

In the second year of the project, we successfully completed the design and optimization of our MCCs detection system which includes the following five-step paradigm: (1) breast area segmentation and artifact elimination, (2) MCC structure and normal tissue enhancement, (3) suspicious MCC area segmentation or localization, (4) feature extraction and analysis of suspicious areas, and (5) suspicious area classification as normal or abnormal. The full evaluation and further optimization is planned for the coming budget year.

## **Reference**

- [1] Wei Qian, Dansheng Song, Xuejun Sun, "Multistage statistical order with neural network for false positive reduction in full field digit mammography" on Nonlinear Signal and Image Processing June 3-6, 2001 Baltimore, USA
- [2] Wei Qian, Xuejun Sun, Dansheng Song, Robert A. Clark, "Digital mammography: Wavelet Transform and Kalman Filtering Neural Network in Mass Segmentation and Detection" Accepted by Academic Radiology, 2001

[3] Wei Qian, Xuejun Sun, Dansheng Song, Robert A. Clark, "A Novel Hybrid Filter Architecture for Image Enhancement and Detection in Digital Mammography", Submitted to Computerized Medical Imaging and Graphics, 2001

[4] L. Zhang, W. Qian, R.Sankar, D. Song, R.Clark, 'A New False Positive Reduction Method for MCCs Detection in Digital Mammography', International conference on acoustics speech, and signal processing May 7-11,2001 Salt Lake city, Utah

[5] Dansheng Song, Wei Qian, Xuejun Sun, and Robert A Clark, "Neural Network for False Positive Reduction in Full Field Digital Mammography with Microcalcification Shape preservation," SPIE Multispectral Image Processing and Pattern Recognition, 22-24 Oct. 2001 Wuhan, China

[6] Ascher etc. "Federal Multi-Agency Consortium on Imaging Technologies to Improve Women's Health, Technology Transfer Workshop on Breast Cancer Detection, Diagnosis, and Treatment", Co-chairs: L. Clarke and R. Nishikawa, Session 5B, Image Processing and Computer Assisted Diagnosis (CAD), Office of Woman's Health (OWH) Workshop on Digital Mammography, Washinton DC, June 1-2, 1997

[7] M.L. Giger." Computer-aided diagnosis. In Syllabus: A categorical course in physics. Technical Aspects of breast imaging", RSNA, 283-298,1993.

[8] H.P. Chan, Kunio Doi, Carl J. Vyborny, Kwok-Leung Lam, and Robert A. Schmidt. Computer-aided detection of microcalcifications in mammograms. Invest. Radiol., 23(9):664--671, September 1988.

[9] W. Zhang, K.Do, ML.Giger et al."An improved shift-invariant artificial neural network for computerized detection of clustered microcalcification in digital mammograms." Med Phys,23,595-601, Apr 1996.

[10] S.B. Lo, M. T. Freedman, J. J. Lin, et al," Preliminary study of computer-aided search for clustered microcalcification on mammograms.", Third International Workshop of Digital Mammography, Chicago, Illinois, June, 1996.

[11] R.M. Nishikawa, Y. Jiang, M.L. Giger, R.A. Schmidt, C.J. Vyborny, W. Zhang, J. Papaioannou, U. Bick, R. Nagel, D. Doi, "Performance of automated CAD Scheme for the detection and classification of clustered microcalcifications," in Digital Mammography, A.G. Gale et al., Ed., Elsevier Science B.V., 1994

[12] B. Zheng, W. Qian, and L. P. Clarke,"Digital Mammography:Mixed Feature Neural Network with Spectral Entropy Decision for Detection of Microcalcifications",IEEE, Trans.on Medical Imaging, Vol 15, No. 589-597,Oct.1996.

[13] H. P. Chan, S. B. Lo, B. Sahiner, et al. " Computer-aided detection of mammography microcalcifications: Pattern recognition with an artificial neural network." Med. Phys. 22(10), 1555-1567, Oct. 1995.

[14] D.H. Davis and D.R.Dance," Automatic computer detection of clustered calcification in digital mammograms," Phys. Med. Biol. 35, 1111-1118, 1990.

- [15] N. Karssemeijer, " Recognition of clustered microcalcifications using a random field model." Proc. SPIE 1905, 776-786, 1993.
- [16] F. Lefebvre, H. Benail et al, "Afractal approach to the segmentatin of microcalcifications in digital mammograms." Med. Phys. 22(4), April, 1995.
- [17] J.J. Heine, S.R. Deans, L.P. Clarke, " Multiresolution Statistical Analysis of High-Resolution Digital Mammograms", IEEE Trans. of Medical Imag. 503-515, 16(5), Oct. 1997.
- [18] R.N. Strickland and H.I. Hann, "Wavelet transforms for detecting microcalcifications in mammograms", IEEE Trans. of Medical Imag. 15(2), 1458-1473, 1996.
- [19] J. Dengler, S. Behrens, and J. F. Desaga, "Segmentation of Microcalcifications in Mammograms," IEEE Trans. MI, 12(4):634-642, 1993.
- [20] D. Rosen, B. Martin, M. Monheit, et al. "A bayesian Neural network to detect microcalcifications in digitized mammograms.", Third International Workshop of Digital Mammography, Chicago, Illinois, June, 1996.
- [21] S.A. Hojjatoleslami and J. Kittler, " Detection of clusters of microcalcifications using a K-nearest neighbor rule with locally optimum distance metric', Third International Workshop of Digital Mammography, Chicago, Illinois, June, 1996.
- [22] T. Netsch, " Detection of Microcalcification Clusters in Digital Mammograms: A Scale-Space Approach", Third International Workshop of Digital Mammography, Chicago, Illinois, June, 1996.
- [23] K.S. Woods, J.L. Solka, C.C. Priebe, C.E. amd Doss, K.W. Bowyer, and L.P. Clarke. Comarative evaluation of pattern recognition techniques for detection of microcalcifications. In Proc SPIE 1905, pages 841--852, 1993.
- [24] W. Qian, L. P. Clarke, M. Kallergi, B. Y. Zheng, P. Venugopal, R. A. Clark, M. L. Silbiger, "Application of Wavelet Transform for Image Enhancement in Medical Imaging," Intelligent Engineering Systems Through Artificial Neural Networks, ASME, vol. 4, 651-660, 1994.
- [25] W.M Morrow, R. B. Paranjape, R. M. Rangyyan, and J. E. L. Deaautels. "Region-based contrast enhancement of mammograms." IEEE Trans, Med. Imag. 11, 392-406, 1992.
- [26] J.K. Kim, J.M. Park, K.S. Song and H.W. Park, " Adaptive Mammographic Image Enhancement Using First Derivative and Local Statistics." IEEE Trans. of Medical Imag. 16(5), Oct. 1997.
- [27] W. Qian, L. P. Clarke, M. Kallergi, H. D. Li, R. P. Velthuizen, R. A. Clark, and M. L. Silbiger, "Tree-structured nonlinear filter and wavelet transform for microcalcification segmentation in mammography," Proc of the IS&T/SPIE Annual Symposium on Electronic Imaging, Science & Technology, San Jose, California, 1993.
- [28] W. Qian, L. P. Clarke et al., "Digital mammography: M-channel quadrature mirror filters for microcalcification extraction," Computerized Imaging and Graphics, Vol. 18, No. 5, pp 301-314, Sept./Oct., 1994.

[29] W. Qian, L. P. Clarke, M. Kallergi, B. Zheng, R. A. Clark, "Wavelet Transform for Computer Assisted Diagnosis (CAD) for Digital Mammography," IEEE Engineering in Medicine and Biology Magazine, Invited Paper, vol.14(5), 561-569, 1995.

[30] P. Sajda, C. D. Spence, J.C. Pearson, et al, " Integrating multi-resolution and contextual information for improved microcalcification detection in CAD", Third International Workshop of Digital Mammography, Chicago, Illinois, June, 1996.

[31] D. Wei, R.M. Nishikawa and K. Doi, " The Application of a Shift Invariant Neural Network for the Detection of Clustered Microcalcifications", Third International Workshop of Digital Mammography, Chicago, Illinois, June, 1996.

[32] S.B. Lo, H.P. Chan, J. Lin, H. Li, M.T. Freedman and S.K. Mun, "Artificial Convolution Neural Network for Medical Image Pattern Recognition," Neural Network, 8(7/8):1201-1214, 1995.

[33] Takehino Ema, Kunito Doi et al. "Image feature analysis and computer-aided diagnosis in mammography: Reduction of false-positive clustered microcalcification using local edge-gradient analysis", Med. Phys. 22(2), 161-169, Feb. 1995.

[34] C.S. Carman and G. Eliot, "Detecting calcification and calcification clusters in digitized mammograms," Third International Workshop of Digital Mammography, Chicago, Illinois, June, 1996.

[35] R.G. Blanks, S.M. Moss, M.G. Willis "A comparison of two view and one view in the detection of small invasive cancers: results from the National Health Service breast screening programme." J. Med. Screen, 3(4), 200-203, 1996.

[36] R.G. Blanks, S.M. Moss, M.G. Willis. "Use of two view mammography compared with one view in the detection of small invasive cancers: further results from the National Health Service breast screening programme." J. Med. Screen, 4(2), 98-101.

[37] Y. Wu, K. Doi, M.L. Giger, and R.M. Nishikawa. Computerized detection of clustered microcalcifications in digital mammograms: Applications of artificial neural networks. Medical Physics, 19:555--560, 1992.

[38] F. Mao, Y. Zhang, D. Song, W. Qian and L. P. Clarke, "An Improved Method of Individual Area Grouping for Microcalcification Detection in Digital Mammograms," Submitted to Medical Physics, 1998.

[39] P. Parent and S. Sucker, "Radial projection: an efficient update rule for relaxation labeling," IEEE Trans. PAMI, 11(8):886-889, 1989.

## Appendices

### Key Research Accomplishments

- (1) Well done the whole system design and optimization.
- (2) Well done the enhancement module including multiresolution microcalcification cluster enhancement.
- (3) Well done the grouping criteria design for identification of microcalcification clusters.
- (4) Well done the adaptive method design for MCCs segmentation module.
- (5) Well done the feature extraction and analysis module including implicit feature and explicit features for digital mammograms.
- (6) Well done the correlation analysis for inter-projection features.
- (7) Well done the classification module design for classification of MCCs versus normal cases of mammograms.

### Reportable Outcomes

---Manuscripts, abstracts, presentations;

1. Wei Qian, Dansheng Song, Xuejun Sun, "Multistage statistical order with neural network for false positive reduction in full field digit mammography" on Nonlinear Signal and Image Processing June 3-6, 2001 Baltimore, USA
2. Wei Qian, Xuejun Sun, Dansheng Song, Robert A. Clark, "Digital mammography: Wavelet Transform and Kalman Filtering Neural Network in Mass Segmentation and Detection" Accepted by Academic Radiology, 2001
3. Wei Qian, Xuejun Sun, Dansheng Song, Robert A. Clark, "A Novel Hybrid Filter Architecture for Image Enhancement and Detection in Digital Mammography", Submitted to Computerized Medical Imaging and Graphics, 2001
4. L. Zhang, W. Qian, R.Sankar, D. Song, R.Clark, 'A New False Positive Reduction Method for MCCs Detection in Digital Mammography', International conference on acoustics speech, and signal processing May 7-11,2001 Salt Lake city, Utah
5. Dansheng Song, Wei Qian, Xuejun Sun, and Robert A Clark, "Neural Network for False Positive Reduction in Full Field Digital Mammography with Microcalcification Shape preservation," SPIE Multispectral Image Processing and Pattern Recognition, 22-24 Oct. 2001 Wuhan, China

----- Degree obtained that are supported by this award ;

Lin Zhang, got Master degree in March of 2001, He is currently working in CISCO Inc. in California.

Jie Lin, Working on Master degree, Will be finished in July of 2002.

**-----Funding applied for based on the work supported by this award;**

**Proposal Submitted to Agency: NIH, R01 on 02/01/21**  
A Telemammography Network for Underserved Area

**Proposal Submitted to Agency: U.S. Army Medical Research and Materiel Command DOD 2001**  
Breast Cancer Research Program

1. Title: Telemedicine and Telemammography Using a Satellite Network for Remote Areas Including Oversea U.S. Military Bases
2. Title: Full Optimization of CAD System for Clinical Application
3. Title: A New CAD Scheme for the Detection of Tiny Mass Using Ipsilateral Multi-View Mammograms



# Academic RADIOLOGY

Stanley Baum, M.D.  
Editor-in-Chief

University of Pennsylvania, Department of Radiology  
3600 Science Center, Suite 370  
3600 Market Street, Philadelphia, PA 19104  
Tel: (215) 662-2028 Fax: (215) 662-6853  
academic-radiology@oasis.rad.upenn.edu

June 18, 2001

Wei Qian, Ph.D.  
Cancer Control Division  
Dept. of Interdisciplinary Oncology  
College of Medicine  
H. Lee Moffitt cancer Center and Research Institute  
12902 Magnolia Drive  
Tampa, FL 33612-9497

RE: Manuscript # 01-046

Dear Dr. Qian:

Thank you for submitting your revised manuscript, "Digital Mammography: Wavelet Transform and Kalman Filtering Neural Network in Mass Segmentation and Detection," to *Academic Radiology*. We are pleased to accept it for publication .

We anticipate that it will be published in 11/1/2001, though changes may occur which could alter this schedule. Your manuscript will be forwarded to the RSNA offices for copy editing and further processing. You will then receive "author queries" to review a few weeks later.

Although your manuscript has been accepted for publication, we are required to have on file a signed Publication Agreement for each submission. Please read and sign the enclosed form and return it to the editorial office at your earliest convenience.

Further correspondence may be made to the address above, or via electronic mail to us at [academic-radiology@oasis.rad.upenn.edu](mailto:academic-radiology@oasis.rad.upenn.edu). Please refer to manuscript number 01-046 when making inquiries.

Sincerely,

  
Stanley Baum, M.D.