

UNCLASSIFIED

ECBC

***FLUORIDE ION REGENERATION OF
CYCLOSARIN (GF) FROM MINIPIG
TISSUE AND FLUIDS FOLLOWING
WHOLE BODY GF MIOSIS LEVEL
VAPOR EXPOSURE***



Edgewood Chemical Biological Center
5183 Blackhawk Road, ATTN: AMSRD-ECB-RT-TT
Aberdeen Proving Ground, Maryland, USA 21010-5424

Email: edward.m.jakubowski@us.army.mil
Phone: (410) 436-8640
FAX: (410) 436-7129

UNCLASSIFIED

Report Documentation Page			Form Approved OMB No. 0704-0188		
Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.					
1. REPORT DATE 16 NOV 2004		2. REPORT TYPE N/A		3. DATES COVERED -	
4. TITLE AND SUBTITLE Fluoride Ion Regeneration Of Cyclosarin (Gf) From Minipig Tissue And Fluids Following Whole Body Gf Miosis Level Vapor Exposure				5a. CONTRACT NUMBER	
				5b. GRANT NUMBER	
				5c. PROGRAM ELEMENT NUMBER	
6. AUTHOR(S)				5d. PROJECT NUMBER	
				5e. TASK NUMBER	
				5f. WORK UNIT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Edgewood Chemical Biological Center 5183 Blackhawk Road, ATTN: AMSRD-ECB-RT-TT Aberdeen Proving Ground, Maryland, USA 21010-5424				8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)				10. SPONSOR/MONITOR'S ACRONYM(S)	
				11. SPONSOR/MONITOR'S REPORT NUMBER(S)	
12. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release, distribution unlimited					
13. SUPPLEMENTARY NOTES See also ADM001849, 2004 Scientific Conference on Chemical and Biological Defense Research. Held in Hunt Valley, Maryland on 15-17 November 2004., The original document contains color images.					
14. ABSTRACT					
15. SUBJECT TERMS					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT UU	18. NUMBER OF PAGES 24	19a. NAME OF RESPONSIBLE PERSON
a. REPORT unclassified	b. ABSTRACT unclassified	c. THIS PAGE unclassified			



ECBC

Authors

EM Jakubowski¹, JM McGuire², RA Evans², SW Hulet¹, DC Burnett¹, RA Way¹, BI Gaviola¹, JA Scotto¹, WT Muse¹, DB Miller¹, RJ Mioduszewski¹, SA Thomson¹.

¹Research and Technology Directorate, US Army
ECBC, APG-EA, Edgewood, MD 21010, USA;

²Geo-Centers, APG-EA, Edgewood, MD 21010,
USA.



ECBC

Introduction

Chemical warfare nerve agent biomarker methods:

- Cholinesterase activity,
- Nerve agent hydrolysis products,
- Fluoride ion regenerated alkyl methylphosphonofluoridate (G-agents)
 - human plasma,
 - red blood cells,
 - tissue

New analytical method:


- ammonia CI,
- a large volume injector (LVI) with Tenax[®] insert, and
- stable isotope ($^2\text{H}_{11}$ -GF) internal standard.



ECBC

Cyclosarin (GF)

UNCLASSIFIED

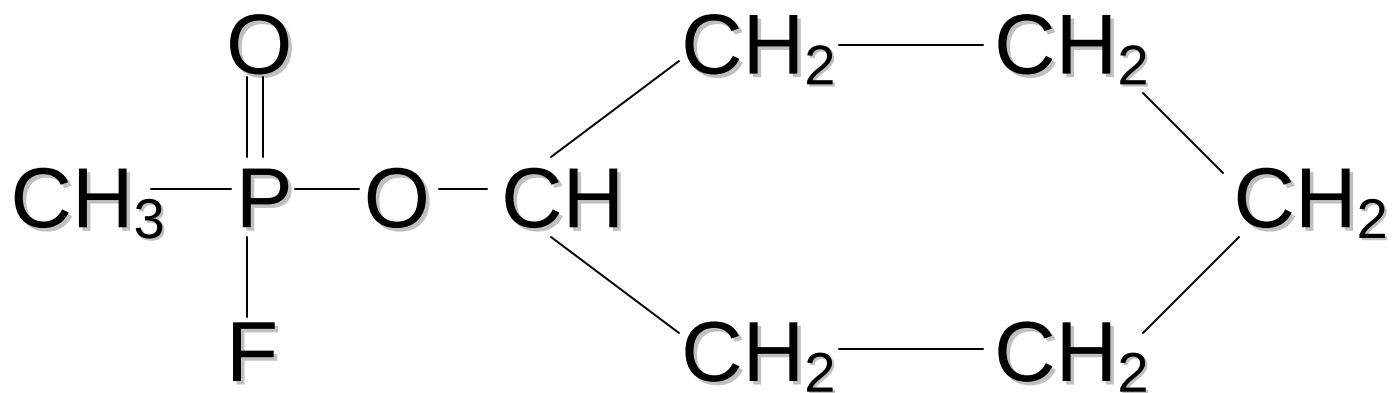

UNCLASSIFIED



ECBC

Objectives

- Develop method for GF exposed samples using GC-MS with positive ammonia chemical ionization and stable isotope standards.
- Explore performance characteristics including:
 - Column selection
 - optimizing LVI and oven parameters,
 - reportable range,
 - accuracy and precision,
 - detection limits.
- Spike animal whole blood/tissue at a series of GF levels
 - Analyze Recovery Data
- Analyze minipig samples after whole body GF exposure



ECBC

Experimental Methods: Materials

- GF : CASARM grade prepared and analyzed at ECBC and diluted with hexane or ethyl acetate.
- Deuterated GF ($^2\text{H}_{11}$): Synthesized at ECBC isotopic purity >99.9% by mass spectrometry
- C_{18} SPE cartridges: 200mg (Waters Associates, Millipore Corp., Milford, MA)
- Acetate buffer (pH=3.5)
- Potassium fluoride: 6 M
- Chemicals: All other chemicals were procured commercially at ACS reagent grade or higher.



ECBC

Minipig Blood Sample Collection

Inhalation Exposure Samples:


Whole blood from GF exposed minipigs was collected (with EDTA) via external jugular catheter allowing serial blood sample collection before, during, and after inhalation exposure.

Samples were centrifuged at 4400 rpm for 5 min. The resulting red blood cell pack and serum/plasma samples were analyzed for regenerated agent by the addition of acetate buffer and fluoride ion.



ECBC

Sample Process Flowchart

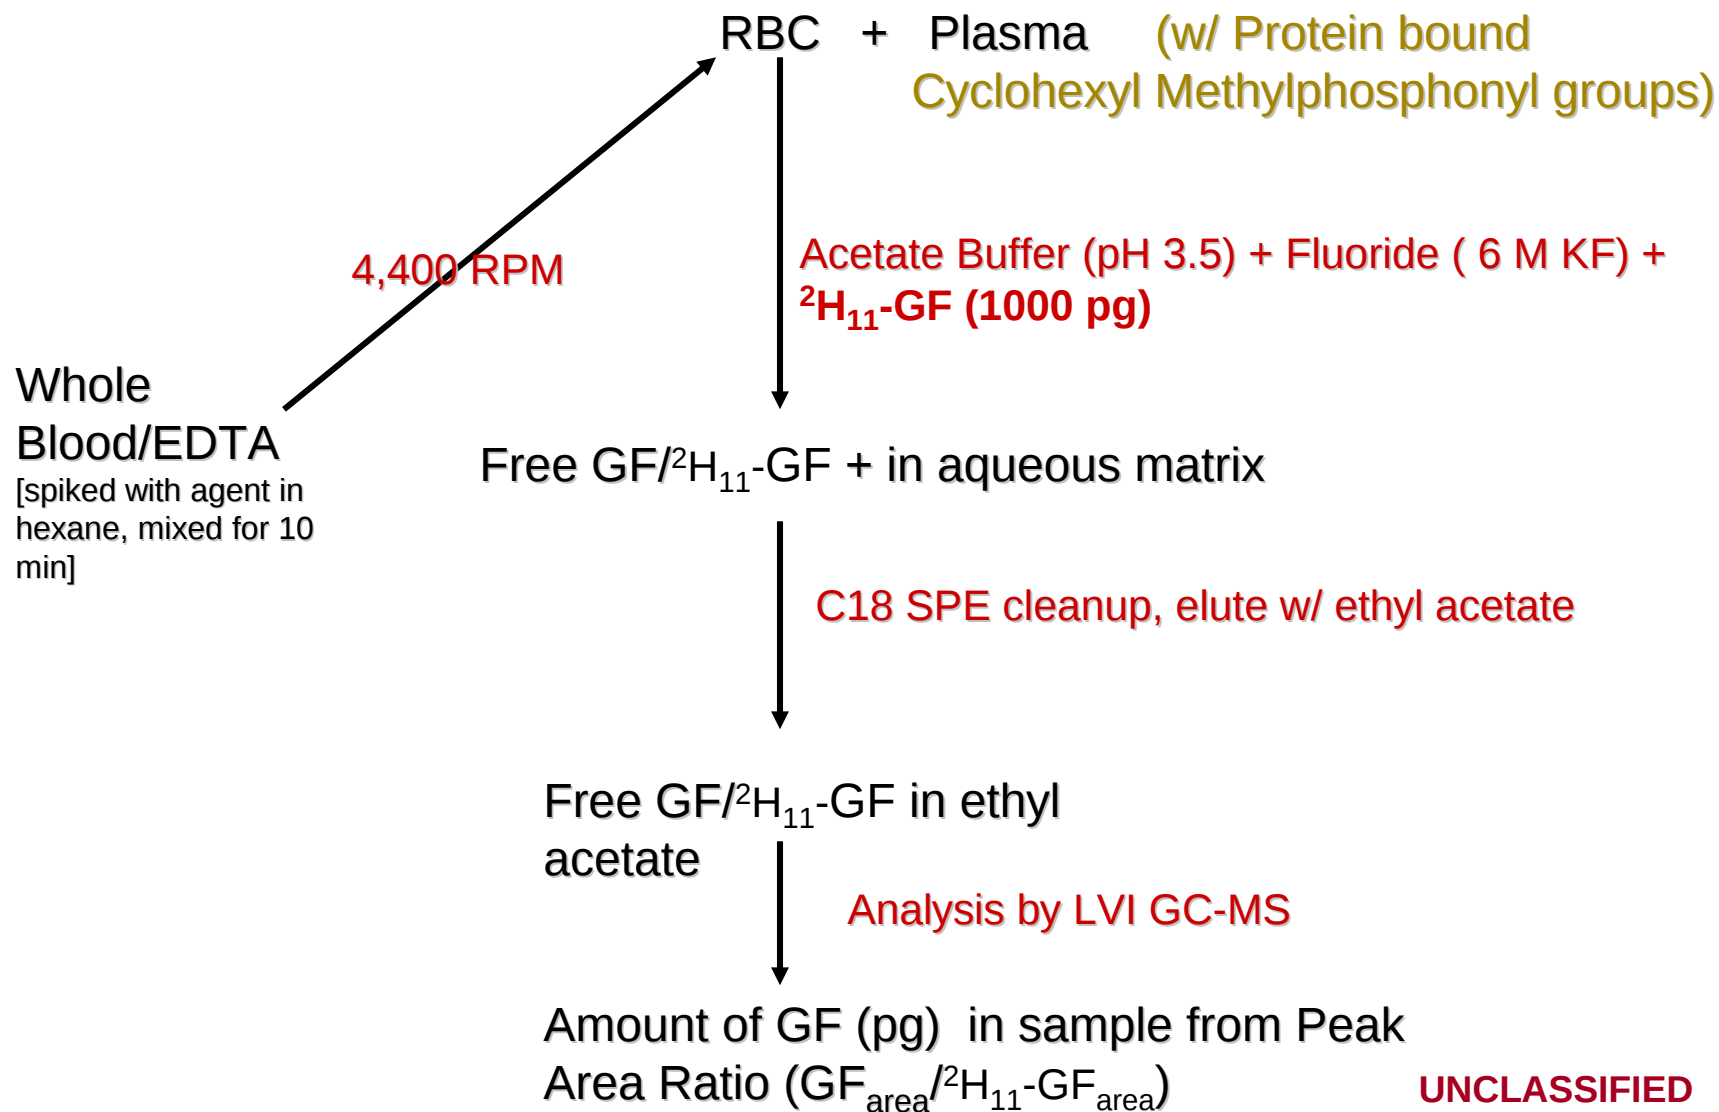



ECBC

Experimental Methods: Analysis

- **GC Model 6890** (Agilent Technologies, Wilmington, DE)
- **LVI Sample Introduction:** Agilent PTV: Inject 50 uL of extract, initial temp 0°C, initial time 5.1 min, final temp 260°C, rate 720°C/min, vent time 5.00 min, vent flow 300 mL/min, purge flow 50 mL/min, purge time 7.85 min.
- **GC Column:**
 - **14%-Cyanopropylphenyl 86%-Dimethylpolysiloxane:** 30 m x 0.32 mm x 1 µm film(Rtx-1701, Restek Inc., Bellefonte, PA)
- **GC Oven program:** Carrier He @ 3 mL/min (63 cm/sec),Temp Program: - 35°C(5.3 min) to 164°C @ 50°C/min to 178°C @ 2°C/min to 270°C(3 min) @ 50°C/min.
- **Detection:** MSD (Model 5973 MSD, Agilent Technologies, Wilmington, DE) SIM mode, ammonia CI, Source & Quad Temp 150°C
 - **GF ions:** Target-198.1 ([M+18]⁺) & Qualifier 215.2 ([M+35]⁺), Retention time 10.61 min
 - **Internal standard (²H₁₁-GF):**Target-209.1 ([M+18]⁺) & Qualifier 226.2 ([M+35]⁺), Retention time 10.53 min



Results and Discussion


- Positive ion NH_3 chemical ionization (CI) was chosen over CI using negative ion NH_3 , positive/negative ion CH_4 , or positive/negative ion isobutane.
 - NH_3 afforded better sensitivity than CH_4 or isobutane
 - Positive ion mode less sensitive to source conditions
- Ratio of $[\text{M}+18]^+ / [\text{M}+35]^+$ was used as tuning benchmark to set NH_3 pressure
- LVI flow rates and injector port purge times are critical parameters to optimize for each solvent and target analyte.
- Tenax packed injector port important.
- Detection limit was in the low picomole range.
- Calibration Curve Range 10-1000 pg on column (50 μL injection)
- Figure 1 is an overlay of five calibration curves from over a three week period.



ECBC

Figure 1. Calibration Curves

GF Calibration Curves

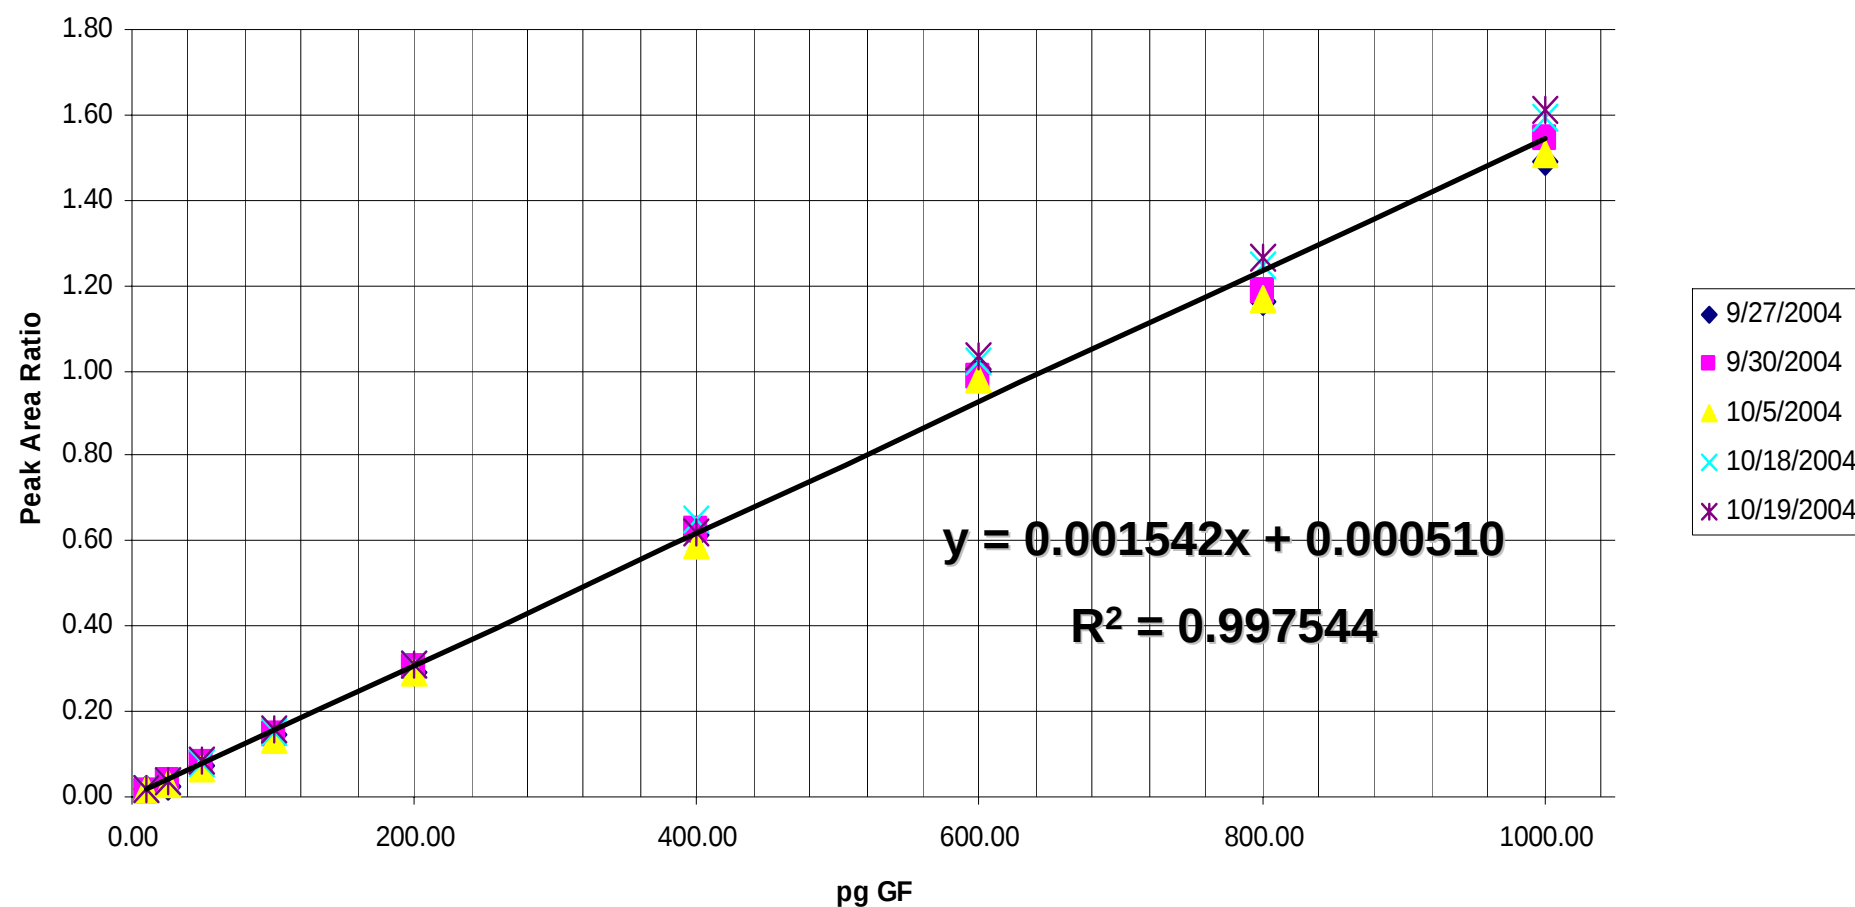



ECBC


Results and Discussion

- Peak-to-peak signal/noise at the lowest standard (10 pg) was over 100.
- Method can be used with blood or tissue samples.
- Figure 2 is a representative plot of lung tissue spiked with GF.
- Figure 3 is a representative plot of the regenerated GF (R-GF) from a minipig eye sample after whole body exposure to GF at 0.16 mg/m^3 for 10 min.
- Figure 4. minipig RBC Sample at 1500 min post exposure (0.16 mg/m^3 for 10 min).
- Figures 5-7 compare GF and GB uptake in the minipig.
- Figures 8 & 9 demonstrate late occurring peaks in R-GF profiles.
- Figures 10 compares R-GF and R-GB from tissue samples.
- Figure 11 presents the ratio of R-GF of Eye/RBC versus Ct
- Figure 12 shows that trends continue with near lethal exposures



Figure 2. GF lung tissue spike (100 pg)


Abundance

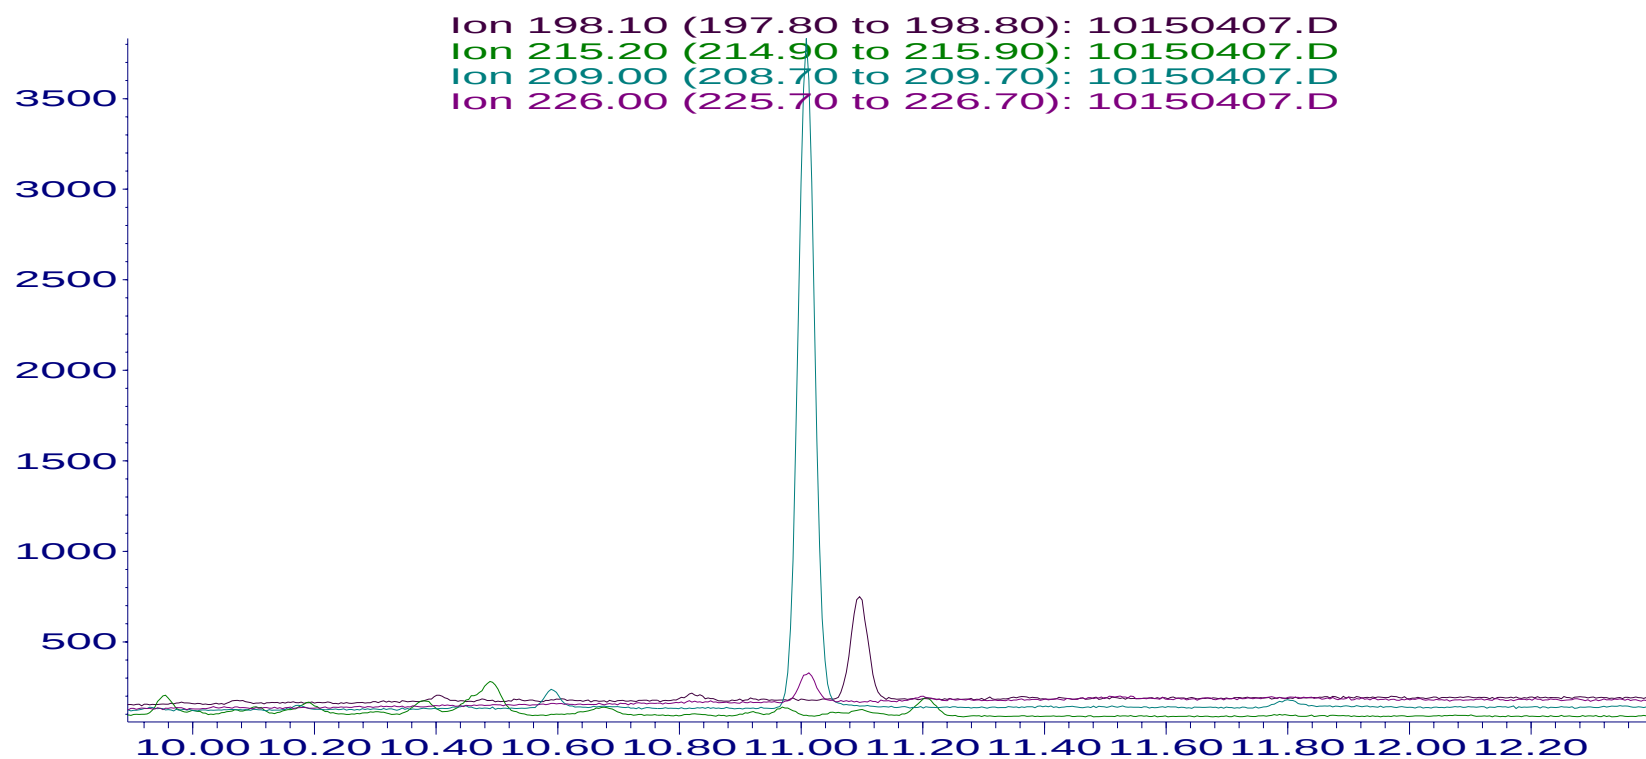

Time-->

Figure 3. Minipig Eye Tissue Sample Post Exposure (375 pg on column)

Abundance

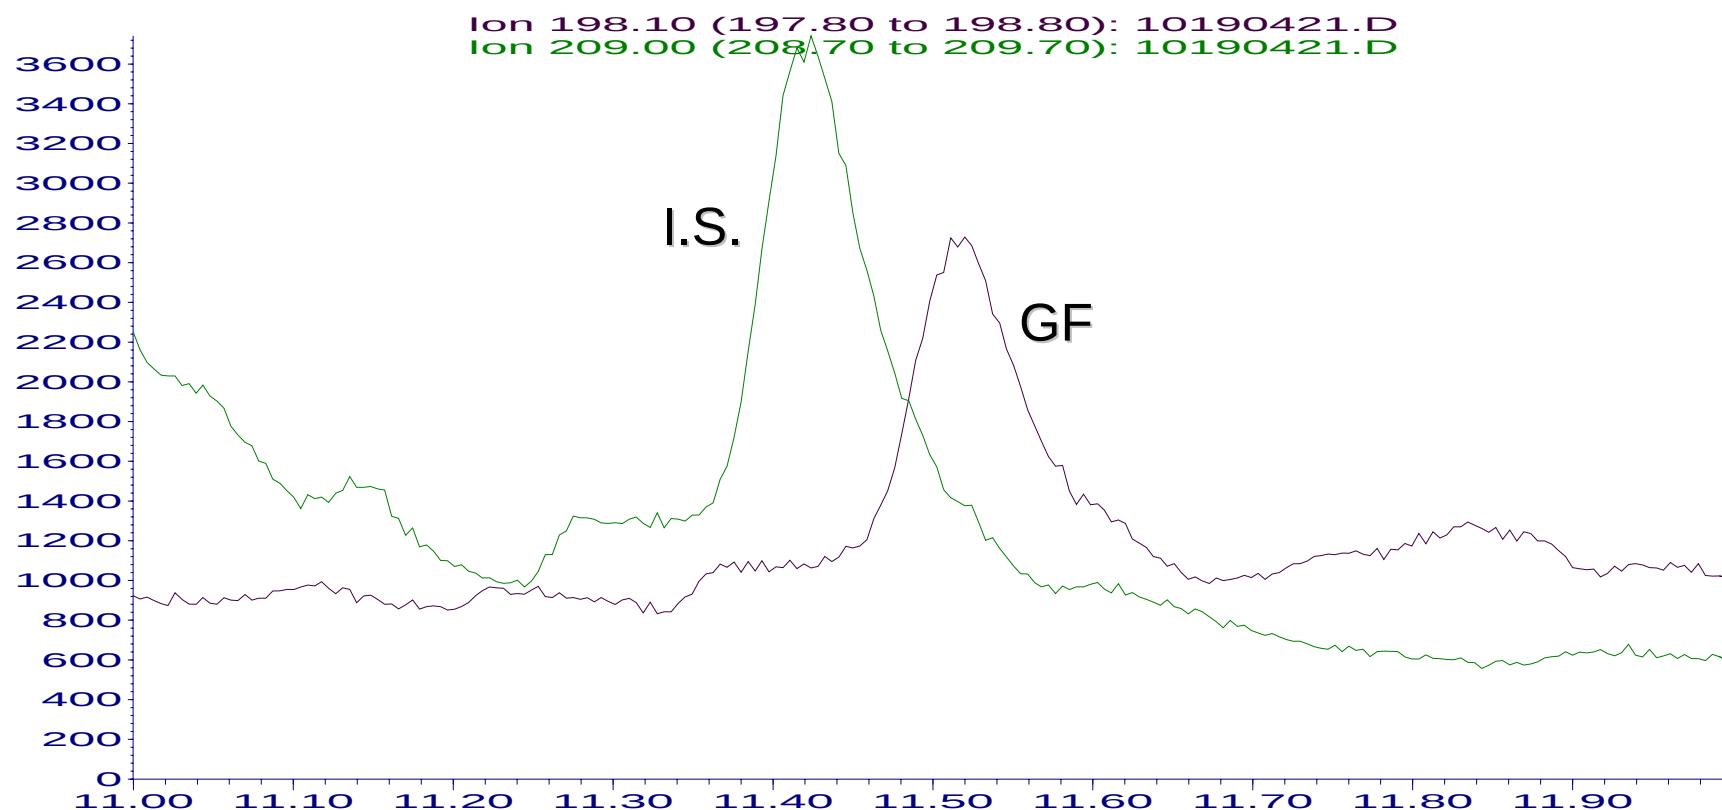

Time-->




ECBC

Figure 4. Minipig RBC Sample at 1500 min

Abundance

Ion 198.10 (197.80 to 198.80): 09150418.D
Ion 209.00 (208.70 to 209.70): 09150418.D

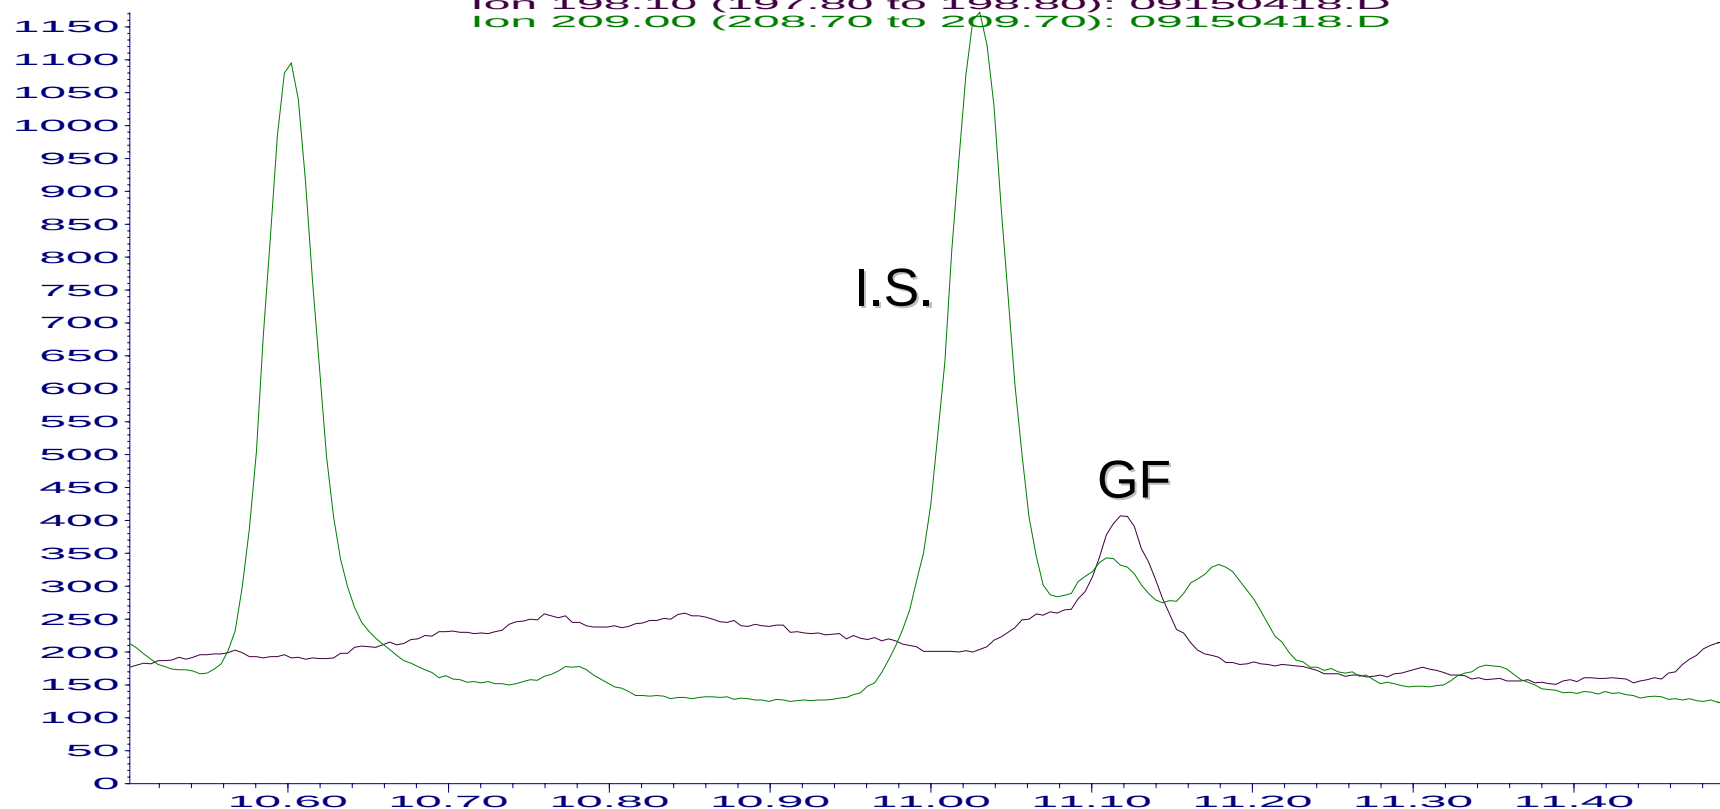


Time-->



Figure 5. GF vs GB Uptake in RBCs (ng/g)

#91:GF 0.22mg/m³(10 min)=2.2 Ct

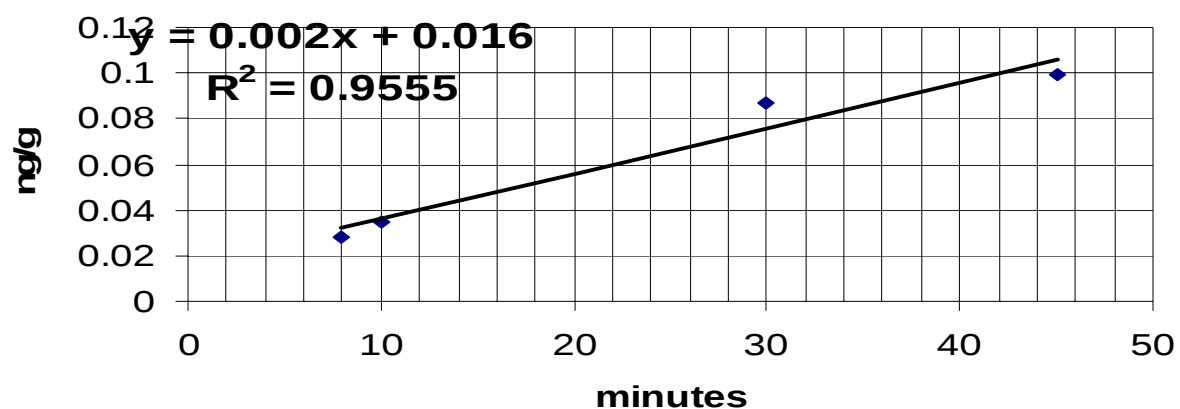

#35:GB 0.28mg/m³(10 min)= 2.8 Ct


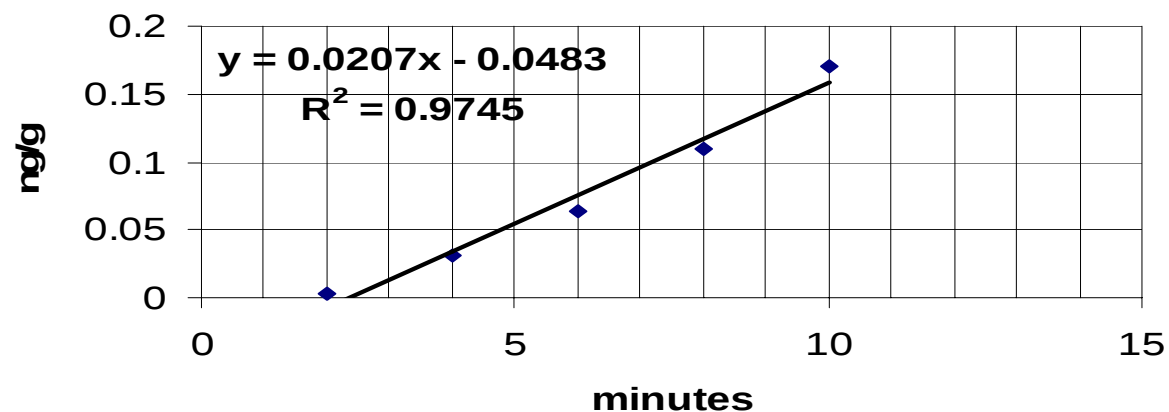



Figure 6. GF vs GB Uptake in RBCs (pmoles/g)

#91:GF 0.22mg/m³(10 min)=2.2 Ct

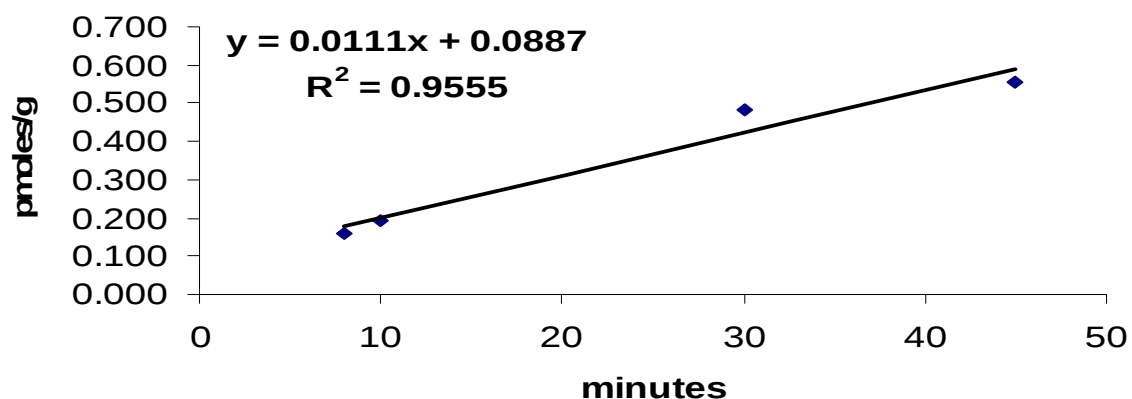

0.0122
mmoles(GF)/m³*t

#35:GB 0.28mg/m³(10 min)= 2.8 Ct

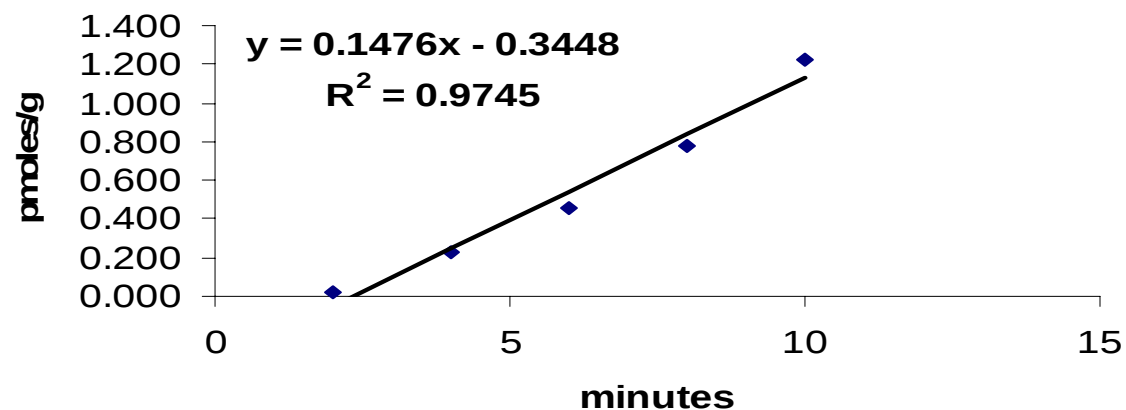


0.0200
mmoles(GB)/m³*t




Figure 7. R-GF vs R-GB from RBC, 24 Hr +

#91:GF 0.22mg/m³(10 min)=2.2 Ct

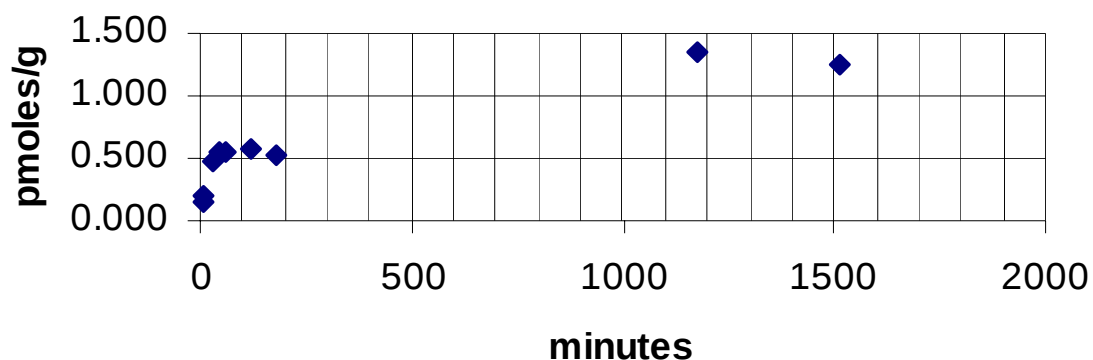

0.0122
mmoles(GF)/m³*t

#35:GB 0.28mg/m³(10 min)=2.8 Ct

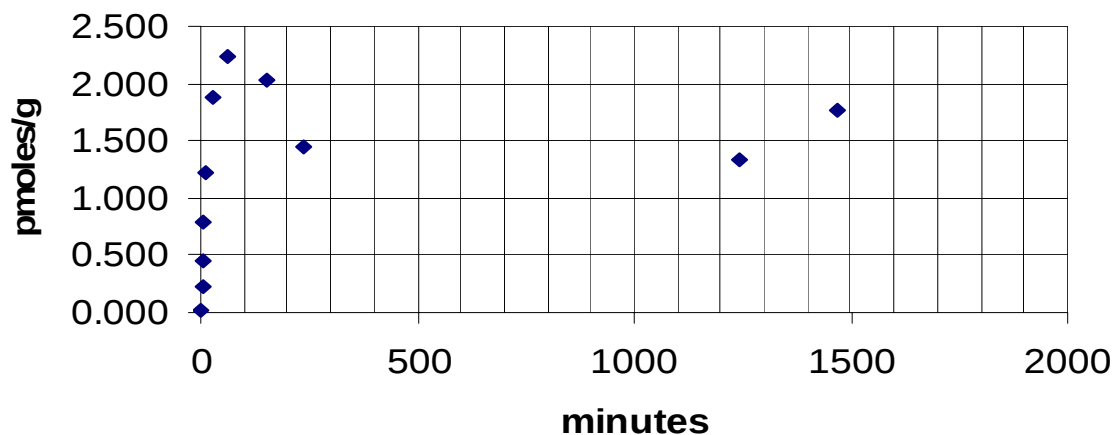


0.0200
mmoles(GB)/m³*t




ECBC

Figure 8. R-GF from Exposed Minipig

#122:GF 0.024mg/m³(180 min)=4.32 Ct
(0.0239 mmoles*min/m³)

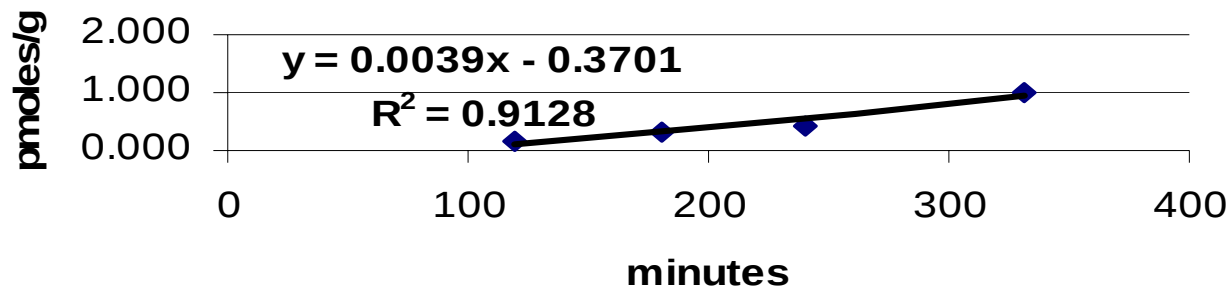

#122:GF 0.024mg/m³(180 min)=4.32 Ct
(0.0239 mmoles*min/m³)

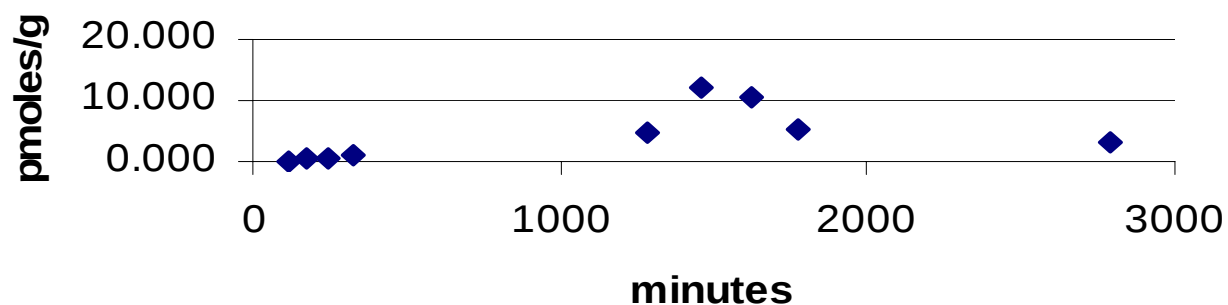





ECBC

Figure 9. R-GF Recovery Over Time

#115:GF 0.061mg/m³(60 min)= 3.66 Ct
(0.0203 mmoles*min/m³)

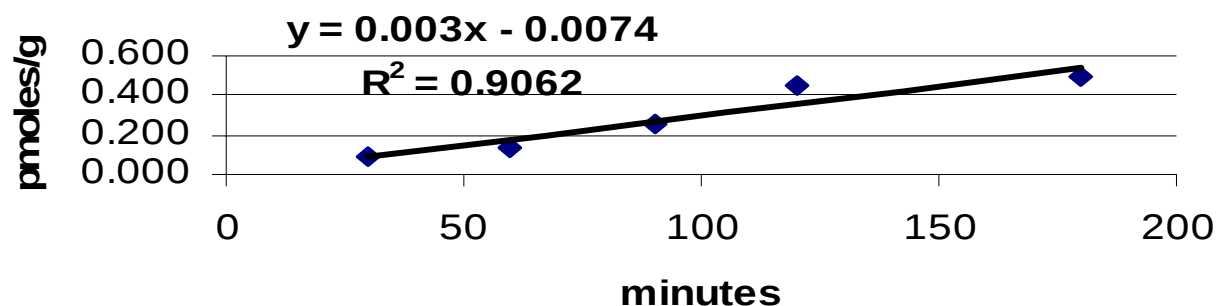

#115:GF 0.061mg/m³(60 min)= 3.66 Ct
(0.0203 mmoles*min/m³)

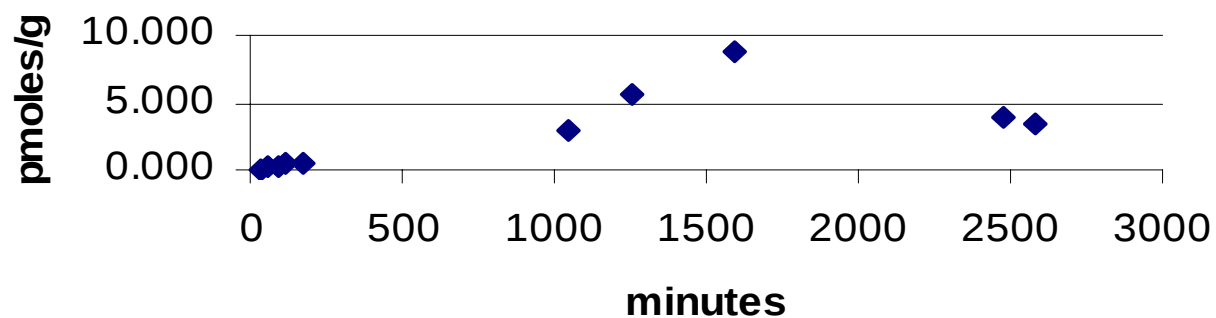



ECBC

Figure 10. R-GF from Tissue Samples


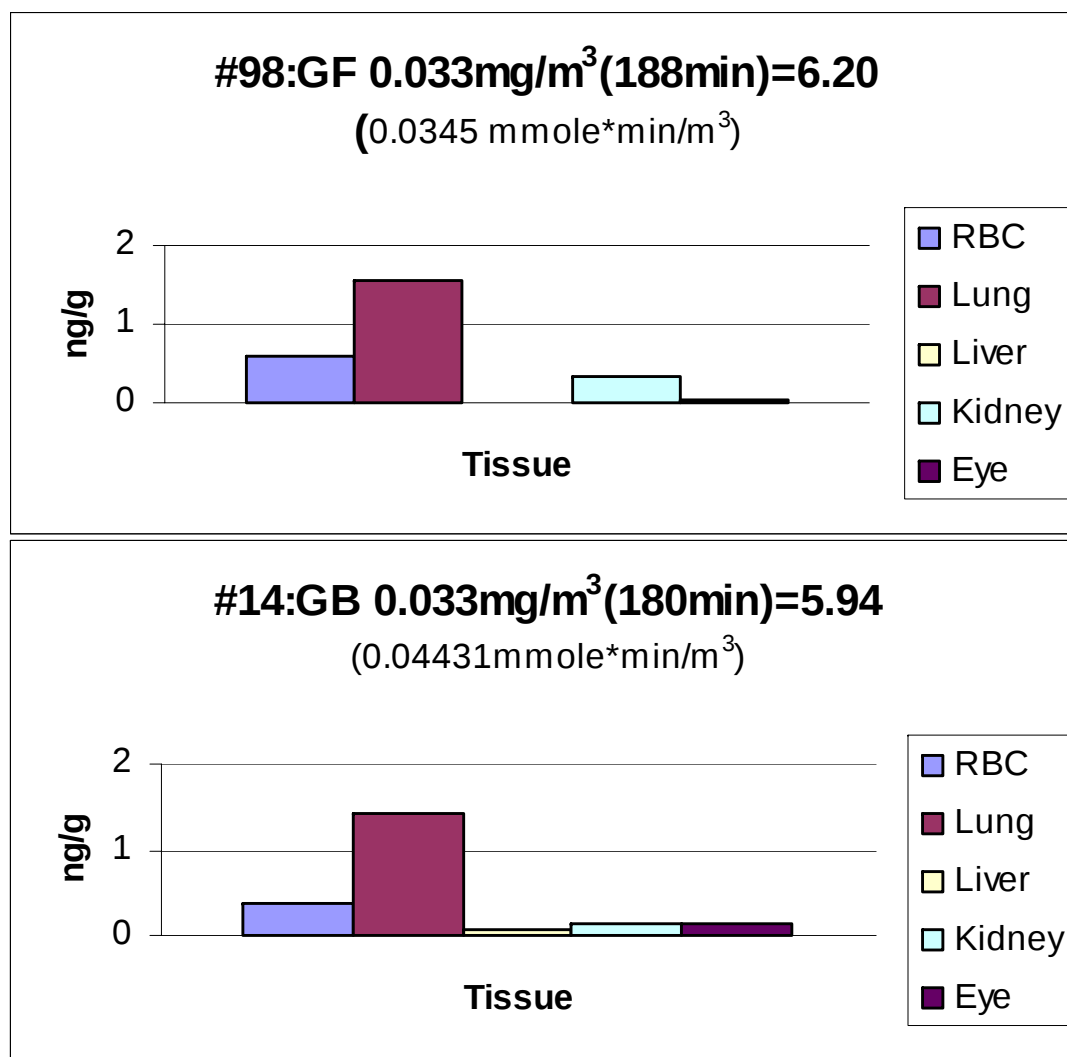





Figure 11. R-GF in Eye Tissue Relative to RBC



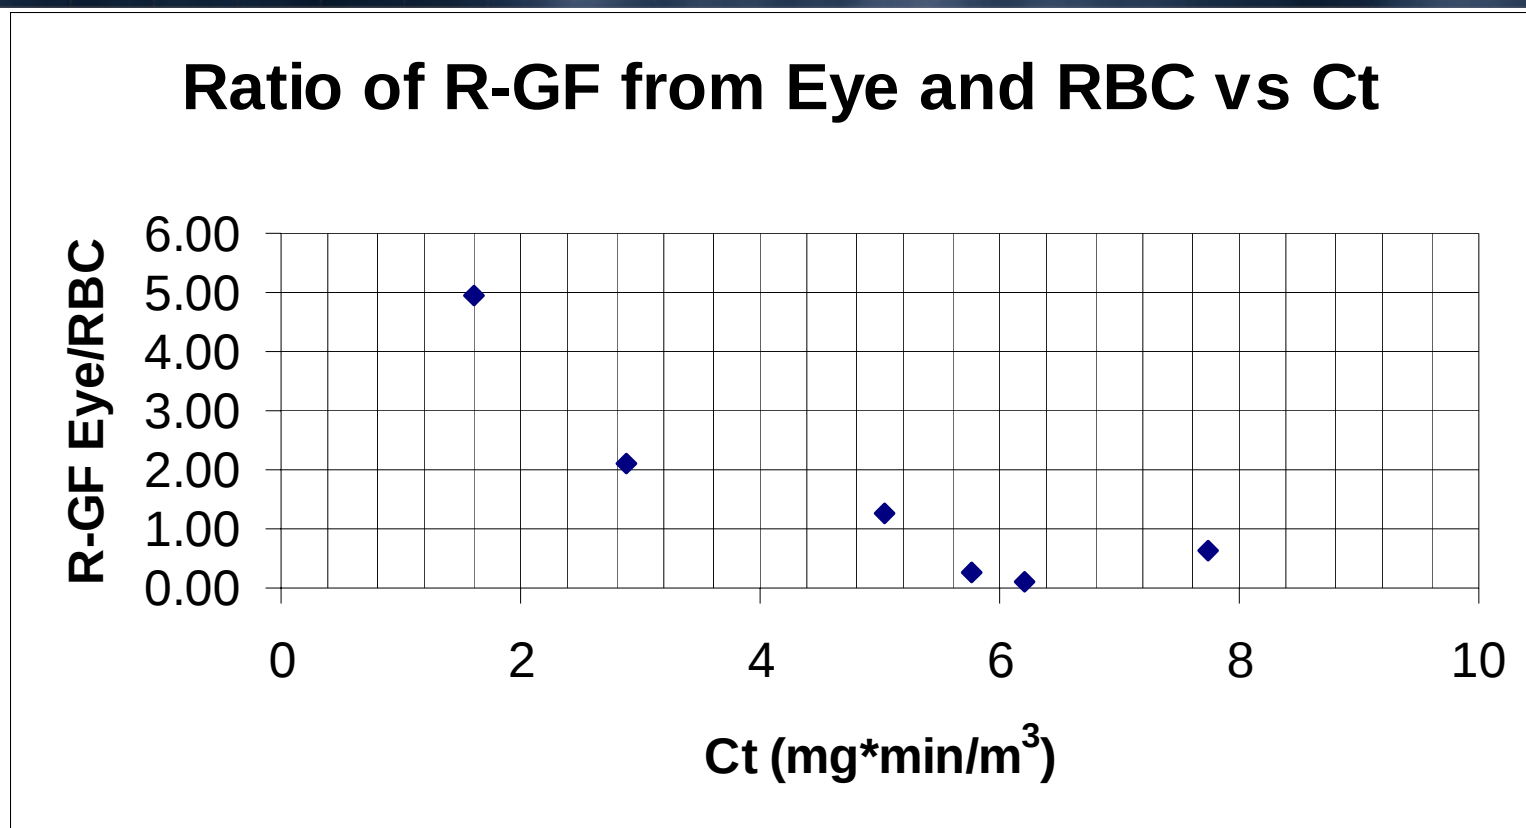

ECBC

Figure 12. R-GF at Near Lethal Exposure

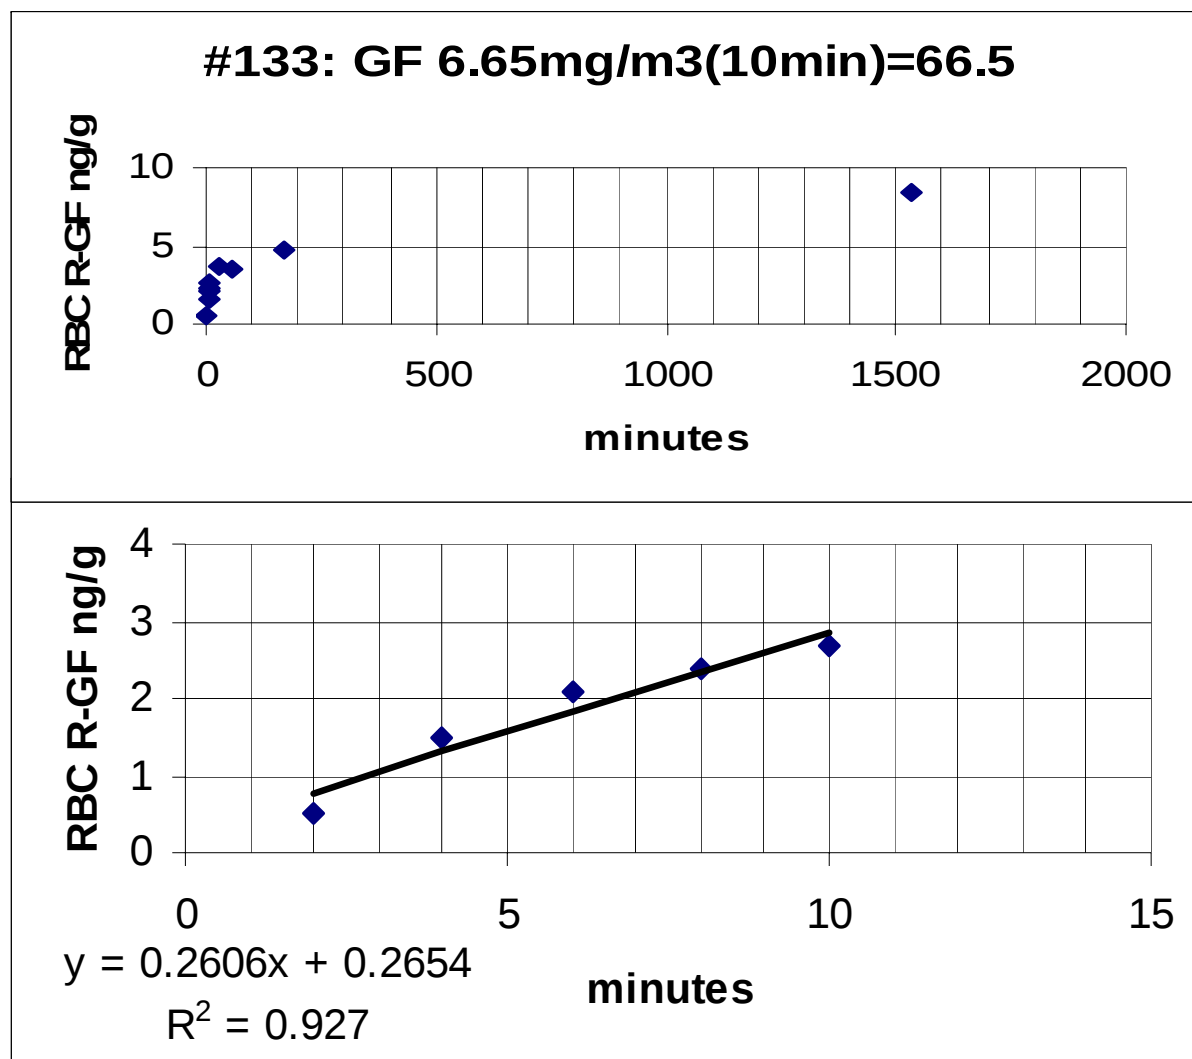



ECBC

Summary/Conclusions

- The isotope dilution LVI method is sensitive enough to quantify R-GF in blood and tissue after miosis level exposure
- Results indicated the ability to quantify GF down to ~400 pg/mL of extract despite the complexity of the matrix.
- Conditions that needed to be optimize for the LVI included injection volume, initial temperature, initial time, pressure, liner packing, and flow rate.
- The uptake of GF as reflected by R-GF levels appears to be much slower than GB.
- Maximum recovery of R-GF was ~24 hours after the beginning of the exposure for all levels of exposure to date. R-GB maximum is reached soon after exposure stops.