

USARIEM TECHNICAL REPORT T08-01

**DEMONSTRATION OF REAL-TIME PHYSIOLOGICAL STATUS MONITORING OF
ENCAPSULATED 1ST CIVIL SUPPORT TEAM – WEAPONS OF MASS
DESTRUCTION (CST-WMD) PERSONNEL**

Mark J. Buller
William J. Tharion
Anthony J. Karis
William R. Santee
Stephen P. Mullen
Laurie A. Blanchard
Reed W. Hoyt

Biophysics and Biomedical Modeling Division

October 2007

U.S. Army Research Institute of Environmental Medicine
Natick, MA 01760-5007

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.

1. AGENCY USE ONLY <i>(Leave blank)</i>	2. REPORT DATE October, 2007	3. REPORT TYPE AND DATES COVERED Technical Report	
4. TITLE AND SUBTITLE DEMONSTRATION OF REAL-TIME PHYSIOLOGICAL STATUS MONITORING OF ENCAPSULATED 1ST CIVIL SUPPORT TEAM - WEAPONS OF MASS DESTRUCTION (CST-WMD) PERSONNEL.		5. FUNDING NUMBERS	
6. AUTHOR(S) Mark J. Buller, William J. Tharion, Anthony J. Karis, William R. Santee, Stephen P. Mullen, Laurie A. Blanchard and Reed W. Hoyt		8. PERFORMING ORGANIZATION REPORT NUMBER T08-01	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Biophysics and Biomedical Modeling Division U.S. Army Research Institute of Environmental Medicine Building 42 - Kansas Street Natick, MA 01760		10. SPONSORING / MONITORING AGENCY REPORT NUMBER	
9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES) U.S. Army Medical Research and Materiel Command Fort Detrick, MD 21702		11. SUPPLEMENTARY NOTES	
12a. DISTRIBUTION / AVAILABILITY STATEMENT Approved for public release; distribution unlimited		12b. DISTRIBUTION CODE	
13. ABSTRACT <i>(Maximum 200 words)</i> Civil Support Teams -Weapons of Mass Destruction (CST-WMD) have a requirement for a medical monitoring telemetry system. This study demonstrated the Warfighter Physiological Status Monitoring (WPSM) system's capability in meeting those needs during a typical training exercise. CST-WMD Soldiers (n= 12) volunteered for this study. The Vital Sign Detection System (VSIDS) and hub were worn during 2 days of training. Remote monitoring took place with data transmitted to a base station laptop. Data was obtained every 15s. Mean data loss = $1.1 \pm 1.4\%$; 5% in the worst case. Most data were within physiologically reasonable bounds (98.7%). Respiration rate data was more variable and appeared to be less valid due to a firmware error. The VSIDS met the needs of CST-WMD for missions lasting < 8 hours. Skin irritation could be an issue for some individuals, especially for longer duration missions (> 8 hours). The graphical user interface (GUI) was adequate for CST-WMD medical monitoring purposes. In summary, currently WPSM system combined with commercial off-the-shelf radios met the CST-WMD medical monitoring needs.			
14. SUBJECT TERMS CBRN, Civil Support Team - Weapons of Mass Destruction, CST-WMD, Enclosed Space Training, First Responders, Medical Monitoring, Military Training, Personal Protective		15. NUMBER OF PAGES 62	
17. SECURITY CLASSIFICATION OF REPORT Unclassified		16. PRICE CODE	
18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT Unlimited	

DISCLAIMERS

The opinions or assertions contained herein are the private views of the author(s) and are not to be construed as official or as reflecting the views of the Army or Department of Defense.

Human subjects participated in these studies after giving their free and informed voluntary consent. Investigators adhered to AR 70-25 and USAMRMC Regulation 70-25 on the use of volunteers in research.

Citations of commercial organizations and trade names in this report do not constitute an official Department of the Army endorsement or approval of the products or services of these organizations.

Approved for public release; distribution unlimited.

TABLE OF CONTENTS

<u>Section</u>	<u>Page</u>
List of Figures.....	v
List of Tables.....	vi
Acknowledgments	vii
Executive Summary	1
Introduction	2
Methods	4
Volunteers	4
Training Event Description.....	4
Day 1: Concrete Tank Training Exercise	4
Day 2: Fire Training Site Exercise	5
Equipment	6
Physiological Monitoring	6
Environmental Monitoring	8
Measures.....	9
Heart and Respiration Rate Signal Quality	9
Skin Temperature Data Quality.....	10
Vital Sign Detection System (VSDS) Vital Sign Algorithm Performance	10
System Acceptability.....	10
Procedures	11
Statistical Analysis	11
Results	12
Meteorological Conditions	12
Physiological Monitoring	13
Heart Rate	16
Respiration Rate	16
Skin Temperature	16
Vital Sign Detection Algorithm	17
System Acceptability	17
Graphical User Interface Assessment	21

Map Screen Improvements.....	22
Squad Status Screen Improvements	23
Name List Screen Improvements.....	23
Individual Warfighter Status Screen Improvements	23
Team Screen Improvements.....	23
Medical Field Card Screen Improvements	23
Reference Center Screen Improvements.....	23
Discussion	23
Ability to Provide Remote Physiological Information.....	24
VSDS Acceptability.....	24
Usefulness of System to Medical Officer	25
Suitability of the Graphical User Interface (GUI).....	26
System Limitations and Planned Improvements.....	26
Conclusions.....	27
Specific Recommendations.....	27
References.....	29
Appendix A: CST-WMD Medical Working Group Medical Monitoring Telemetry System Requirement Document	31
Appendix B: WPSM System Acceptability Questionnaire.....	33
Appendix C: Medical System Computer Display Questionnaire.....	41
Appendix D: Time Series Data Plots	49

LIST OF FIGURES

<u>Figure</u>		<u>Page</u>
1	Warfighter Physiological Status Monitoring – Initial Capability system	3
2	Day 1 enclosed space training site	5
3	Day 2 enclosed space training site	5
4	Day 2 personal protective equipment	6
5	Graphical user interface display	8
6	Environmental monitoring equipment	9
7	Local meteorological conditions for training days 1 and 2	12
8	Day 1: Reinforced concrete enclosed space air temperature and relative humidity	13
9	Day 2: Metal enclosed space air temperature and relative humidity	13
10	Representative time series heart rate, respiration rate and skin temperature for one volunteer during Day 2 training	16
11	Data from a single volunteer from Day 1 training showing an example of an aberrant chest skin temperature reading, and extremely variable respiration rate data	17
12	Vital Sign Detection System (VSDS) overall comfort rating	19
13	Mid-back skin irritation caused by wearing the Vital Sign Detection System (VSDS) after four hours of training	20
14	Utility ratings of the Team List screen for CST-WMD personnel.	21

LIST OF TABLES

<u>Table</u>		<u>Page</u>
1	Physiological monitoring equipment used in the study (total weight ~ 1 kg).	7
2	Heart rate and respiration rates (overall group mean and SD, N = 8) and calculated acceptable ranges (minima and maxima) for heart rates and respiration rates (defined as laboratory values $\pm 2SD$).	10
3	Parameter variance thresholds based upon lab validation study activities for periods where heart rate is above or below 120 BPM	10
4	Heart and respiration rate data availability and data quality for each test period	14
5	Chest skin temperature quality and vital sign algorithm state by for each test period	15
6	Fit of the Vital Sign Detection System (VSDS) for various areas of the body	18
7	Tightness/looseness of the Vital Sign Detection System (VSDS) for various areas of the body	18
8	Comfort for the various parts of the Vital Sign Detection System (VSDS)	19
9	Source of negative comments regarding various parts of the VSDS	20
10	Suggested improvements to the Team List Screen	22
11	Ratings of the various concept screens that were previously developed from U.S. Army Medic feedback	22

ACKNOWLEDGMENTS

The authors thank the members of the 1st CST-WMD Massachusetts National Guard who made this technology demonstration possible.

EXECUTIVE SUMMARY

National Guard's Weapons of Mass Destruction Civil Support Teams (CST-WMD) have a requirement for a medical monitoring telemetry system to "assess status of downrange personnel" by observing "physiologic changes in vital signs and core temperature prior to collapse or loss of consciousness or death." The Warfighter Physiological Status Monitoring (WPSM) program has developed a wearable suite of sensors and algorithms to assess health state. In this study we demonstrated the WPSM – Initial Capability (WPSM-IC) system during a standard training exercise. We assessed the:

- Acceptability of a body-worn medical monitoring system to CST-WMD team members
- Ability to remotely provide physiological information to the command center
- Usefulness of the medical monitoring system to the CST-WMD medical officer in monitoring down-range team members' physiological state
- Acceptability of the graphical presentation of real-time physiological information to medical and/or command staff personnel.

Twelve male^{1st} CST-WMD Massachusetts National Guard members plus their medical officer who observed and monitored the training event, but didn't wear the medical monitoring system participated in this study. The Vital Sign Detection System (VSDS) and medical hub components of the WPSM-IC system were worn during several two to three hour enclosed-space training exercises performed over two days. Each exercise had one or more simulated casualties in a small enclosed space. In the first exercise, access to the enclosed spaces was constrained to approximately 30" diameter access holes. During each exercise, remote monitoring of six team members took place with data transmitted to a base station laptop for display on a graphical user interface (GUI). Meteorological and micro-meteorological conditions surrounding and within the enclosed training spaces were measured. Real time physiological information was provided every 15s for all team members fitted with a medical monitoring system throughout the training events. There was minimal loss of data (mean loss = $1.1 \pm 1.4\%$; 5% in the worst case). Most data were within physiologically reasonable bounds (98.7%). Heart rate and skin temperature data were similar to laboratory data collected using reference instrumentation. Respiration rate data was more variable and appeared to be less valid. The cause of this problem was detected to be a firmware error that has since been corrected. Information obtained from survey responses indicated the VSDS met the needs of CST-WMD missions, and could be used for real-time monitoring of CST-WMD personnel during missions lasting eight hours or less. Skin irritation could be an issue for some individuals, especially for longer duration missions (>8 hours). The simple GUI, which listed individual health status information, was found to be adequate for CST-WMD medical monitoring purposes. The currently available WPSM system, when combined with commercial off-the-shelf radios, was shown to meet most of the CST-WMD medical monitoring telemetry requirements as detailed by the national CST-WMD medical working group.

INTRODUCTION

National Guard Weapons of Mass Destruction Civil Support Teams (CST-WMD) were founded with the mission of responding rapidly to domestic chemical, biological, radiological, and nuclear (CBRN) threats. Response to CBRN threats often means that team members will be encapsulated within some level of personal protective equipment (PPE) ranging from Level C, similar to Military Operational Protective Posture (MOPP) IV, to Level A which requires encapsulation within an impermeable suit with the use of self-contained breathing apparatus (SCBA) or a re-breather (1). When encapsulated in various levels of CBRN protection, the ability of the human body to thermoregulate is reduced (2). With high or even moderate work rates, heat production can exceed the body's capacity for heat loss leading to heat illness and possible collapse. Thermal strain has also been suggested as a possible contributing factor in the sudden cardiac death of firefighters -- the leading cause of US firefighter deaths (3) -- where the cardiovascular system is stressed from the competing needs of thermoregulation and strenuous work (4).

Recognizing the need to monitor thermal/work strain when encapsulated, the National CST-WMD medical working group generated a requirements document for a medical monitoring telemetry system (See Appendix A). The problem they cited is that it is "Difficult to assess status of downrange personnel verbally. Most casualties demonstrate physiological changes in vital signs and core temperature prior to collapse or loss of consciousness/death." The requirement calls for a system that monitors core body temperature, heart rate and cardiac rhythm (electrocardiogram (ECG)), respiration rate, pulse oximetry, and ambient temperature remotely; and successfully transmits this data back to a medical officer. Except for pulse oximetry, USARIEM's Warfighter Physiological Status Monitoring – Initial Capability (WPSM-IC) system monitors the physiological parameters of interest to the CST-WMD medical working group.

The WPSM-IC system (Figure 1) (5, 6) provides physiological and health state information to Soldiers, medics, and commanders. This system is comprised of a medical hub which hosts a personal area network of physiologic and medical sensors and a number of algorithms. The algorithms, using personal characteristics and sensor data, estimate the state of the Warfighter in the following areas: thermal, hydration, sleep history, and life signs. Health state information, along with summarized physiologic data, is intended to be a tool that medics and/or commanders can use to assess the health and readiness of their Warfighters.

The WPSM-IC system was tested at the US Army Aberdeen Test Center's (ATC) Military Operations in Urban Terrain (MOUT) test facility (Aberdeen Proving Ground, MD) in June 2006. Periodically over two days, health state and physiologic parameters were telemetered from 9 volunteers back to a base station via commercial radio modems. The results of this initial field demonstration of the WPSM-IC system (7) suggest it could also be used to meet the medical telemetry needs of the CST-WMD.

Figure 1. Warfighter Physiological Status Monitoring – Initial Capability system



Components: 1. Notional display on a PDA device; 2. Medical Hub that manages the network of sensors, communications, algorithms, and models (Hidalgo Ltd, Cambridge UK; Mini Mitter / Respiration Inc., Bend OR); 3. Vital Sign Detection System (VSDS) chest belt measures heart rate, respiration rate, skin temperature, body posture, and activity; this device has received FDA 510k pre-market approval as a heart rate, respiration rate and skin temperature monitor (Equivital; Hidalgo Ltd, Cambridge UK); 4. Core temperature telemetry pill (FDA 510k certified) (Mini Mitter / Respiration Inc., Bend OR), 5. Prototype fluid intake monitor measures fluid consumed.; 6. Sleep Watch measures apparent sleep history (Precision Control Design, Ft. Walton Beach FL).

The objective of the present study was to demonstrate the performance of the VSDS and medical hub part of the WPSM – Initial Capability (WPSM-IC) system which measures heart rate, respiration rate, skin temperature, and body motion and body position (VSDS) and stores and readies the information for transmission over a radio network (medical hub). The other components of the WPSM-IC system, e.g. the sleep watch, fluid intake monitor, etc. (Figure 1) were not used. Testing was done in an operationally-relevant CST-WMD training environment. We assessed the:

- The acceptability of the body-worn system to CST-WMD team members
- The ability to remotely provide physiological information to the command center
- The usefulness of this monitoring system to the CST-WMD medical officer in monitoring down-range team members

- The acceptability of the graphical presentation of the real-time physiological information to the medical and/or command staff personnel.

Additionally, meteorological and micro-meteorological conditions surrounding and within the enclosed space training spaces were measured to provide the environmental context this test took place in.

METHODS

The functionality of this medical monitoring system was assessed during a regularly scheduled CST-WMD training event. During this training event, CST-WMD team members wore the WPSM-IC system VSDS and medical hub. Data were transmitted in real time to a base station computer. The base station computer had a graphical user interface (GUI) that presented real time data from all instrumented team members.

VOLUNTEERS

Twelve male team members from the Massachusetts National Guard 1st CST-WMD served as volunteers (age = 33.5 ± 6.9 yrs, height = 181.4 ± 6.1 cm, body weight = 89.9 ± 8.4 kg, two-mile run time = 15.75 ± 1.30 min). One additional volunteer was the medical officer who observed and monitored the training event but did not wear a monitoring system.

TRAINING EVENT DESCRIPTION

Monitoring systems were worn during portions of two days of enclosed space training. Each training scenario had one or more simulated casualties in a small enclosed space. Access to the enclosed space was through holes that were approximately 30" in diameter.


Day 1: Concrete Tank Training Exercise

This enclosed space consisted of two large septic tanks (Figure 2). The septic tanks were stacked vertically with a single casualty (simulated) in the bottom tank. Access to the casualty was through the two access holes in each tank. The upper tank was floorless – resting on top of a second tank allowing entry through the access hole (Figure 2, Panel B).

The training scenario was run twice, with six of the twelve volunteers participating in the morning and the remaining six in the afternoon. In each training session one volunteer served as a casualty with the remaining five serving as the rescue team. The training scenario did not have a CBRN component to it; therefore volunteers wore Battle Dress Uniform (BDU) pants and t-shirts. The goal of the exercise was to locate and extract the unconscious (simulated) casualty. Extraction of the casualty was achieved

through a rope lift mounted to a tripod above the top septic tank access hole (Figure 2, Panel A). This hole also served as the access and egress point for the rescue team.

Figure 2. Day 1 enclosed space training site

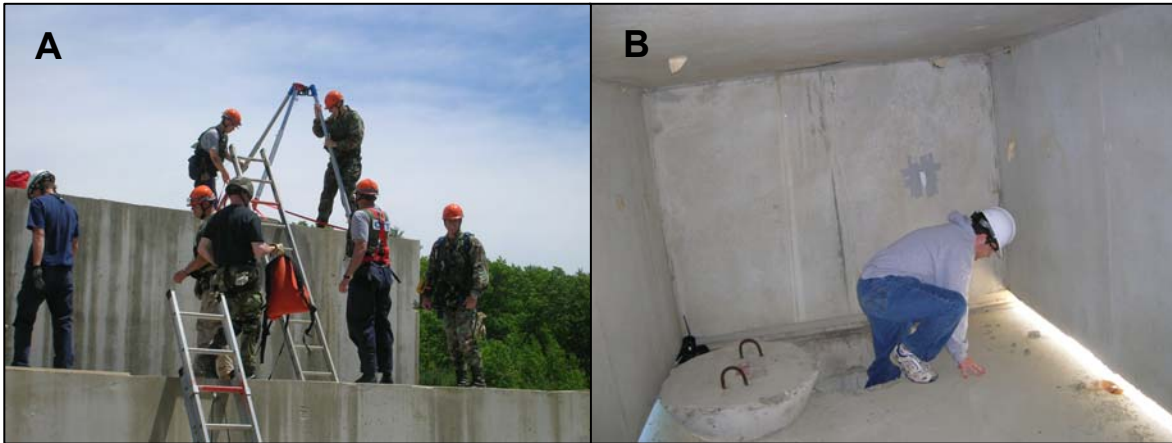

Panel A shows the two concrete septic tanks used for the enclosed space training. Panel B shows the entrance to the lower septic tank.

Day 2: Fire Training Site Exercise

The enclosed space for the second day of training consisted of two metal shipping containers converted into a fire training facility (Figure 3). Container windows and doors were shut during the exercise. Entrance to the structure was through an access hole located on the roof of the containers.

Figure 3. Day 2 enclosed space training site



The goal of second day of training was to locate and extract a number of unconscious casualties who had succumbed to a chemical agent (conditions were simulated, i.e., no one was unconscious and no chemical agents were used). Since a chemical agent was suspected in the training scenario, rescuers wore Level C personal protective equipment (PPE) with an external air supply (Figure 4). Rescuers climbed to the top of the containers via a ladder. Casualties were extracted by physically carrying

or dragging the casualties to the bottom of the access hole and then utilizing a rope lift to move the casualties through the access hole to the container roof top. Six of the twelve volunteers participated in the second day of training. Three volunteers served as casualties and the remaining three served as rescuers.

Figure 4. Day 2 personal protective equipment







EQUIPMENT

Physiological Monitoring

Each CST-WMD volunteer, except for the medical officer wore a physiological monitoring system consisting of the Vital Sign Detection System (VS DS) (http://www.hidalgo.co.uk/toplevel.htm?whatwedo_equivital.htm) (Hidalgo Ltd., Swavesey Cambridge, UK), hub components of the WPSM-IC system, and a commercial-off-the-shelf (COTS) radio with battery pack (Table 1).

The VS DS consists of a textile chest belt that supports a hard plastic sensor electronics module (SEM) that snaps into the center of the belt. The VS DS derives heart rate from the electrocardiogram (ECG), respiration rate from chest wall contraction and expansion, chest skin temperature by thermister; chest orientation (upright, supine face down, etc.) and physical activity patterns are derived from a three-dimensional accelerometer housed in the SEM. The VS DS has received Food and Drug Administration (FDA) 510K pre-market certification as a heart rate, respiration rate, and skin temperature monitor, and also provides an index of medical status (6) based upon the presence or absence of motion, heart rate, and respiration.

Table 1. Physiological monitoring equipment used in the study


Device	Manufacturer	Data type	Wt. (g)
 <p>Vital Sign Detection System (VSDS)</p>	<p>Equivital; Hidalgo Ltd., Swavesey Cambridge, UK</p>	<p>Heart Rate Respiration Rate Skin Temperature Body Position Activity/inactivity Vital Sign State</p>	193
 <p>WPSM Hub</p>	<p>Hidalgo Ltd., Swavesey Cambridge, UK</p>	<p>health state information (heart rate, respiration rate, temperature, activity/ inactivity) and system status (e.g., any error messages, battery charge)</p>	340
 <p>Off-Body Radio</p>	<p>Digi XTend RF Modem; Maxstream Inc., Lindon, Utah</p>	<p>Telemeters Hub data to base station PC</p>	208
 <p>Radio Battery</p>	<p>External Battery Pack (PM85-44)</p>	N/A	321

Total weight worn is ~ 1 kg). The COTS radio modems operate at 900 MHz using spread spectrum frequency hopping technology, and transmitted data every fifteen seconds from the Hub to a base station laptop computer. The radios were configured to allow simultaneous transmission of physiological data from six systems.

In this study the hub received data from the VSDS via Bluetooth™ radio frequency (RF) protocol, stored this information locally on a flash memory card, and exported the data to a long haul radio modem that transmitted the physiological data off-body to a command center.

Figure 5 shows the GUI used to present individual vital sign status, volunteer number, heart rate and trend, respiration rate and trend, chest skin temperature and trend, body/chest orientation, and time of last data update. These data, derived from each individual's physiological monitoring system outputs, were displayed in real-time for observation by study participants.

Figure 5. Graphical user interface display

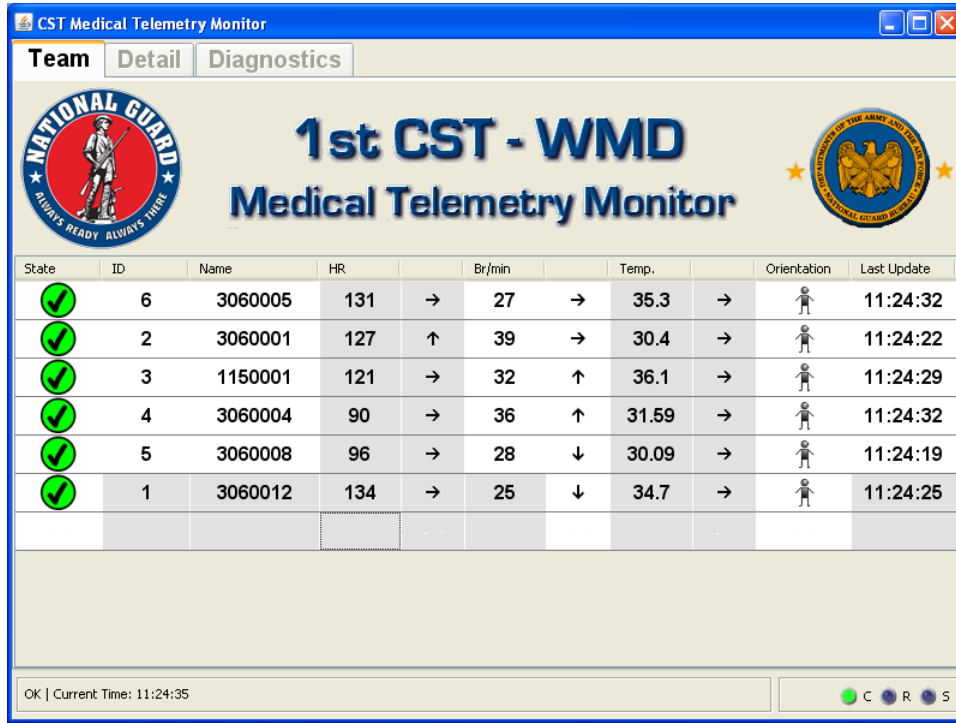

Environmental Monitoring

Two types of meteorological monitoring systems were used. The Campbell Scientific Inc. (Logan, UT) CR-10X weather station (Figure 6, Panel A) was used to record ambient weather conditions and was configured to measure wind speed, wind direction, humidity, air temperature, solar radiation, and ground surface temperature. Weather data were logged to onboard memory for later download. On the first day of training, weather data were also transmitted via a 100 mW 900 MHz spread spectrum radio (Digi XTend RS-232/RS-485 RF Modem, Maxstream Inc., Lindon, Utah) to a laptop computer for display and redundant logging. In addition, up to 16 HOBO® Pro v2 temperature/RH loggers (Onset Computer Corporation, Pocasset, MA) (Figure 6, Panel B) were used to record temperature and relative humidity in the enclosed spaces.

Figure 6. Environmental monitoring equipment

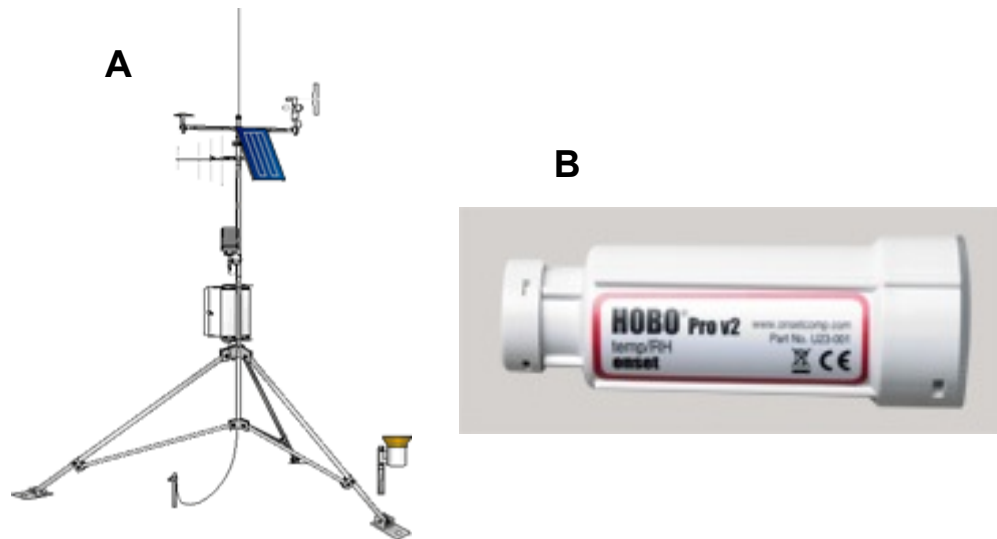


Figure 6A shows the Campbell Scientific Inc. (Logan, UT) CR-10X weather station. Figure 6B shows the HOBO® Pro v2 temperature/relative humidity (RH) logger (Onset Computer Corporation; Pocasset MA) which can log temperatures from -40 to $70^{\circ}\text{C} \pm 0.18^{\circ}\text{C}$ and RH between 0 - $100\% \pm 2.5\%$.

MEASURES

Heart and Respiration Rate Signal Quality

The medical monitoring system data was assessed by examining the availability and quality of its physiological information from six different systems as volunteers wore them during training. Quality of the heart rate and respiration rate data was assessed by examining how many reported values were within a physiologically reasonable range and had reasonable variance for the given activity. The physiologically reasonable ranges and variance used were derived from VSIDS laboratory validation study data (8).

The physiologically acceptable range was calculated for both heart and respiration rates in the following way. The minimum reasonable heart rate or respiratory rate was calculated as the minimum observed during sedentary sitting conditions minus two standard deviations (SD). Similarly, the maximum reasonable values were calculated as the maximum values observed during treadmill running (6 mph) plus two SDs. Rounded values, to the nearest integer, of the minimum and maximum rates were used. Table 2 shows VSIDS study data (8) for heart and respiration rate values for volunteers at rest (sitting) and during physical activity (running), and the corresponding range (minimum/maximum) used in the current data analysis. Table 3 shows the calculated bounds using the two-SD method described above. That is, when heart rates were below 120 BPM, the acceptable data variability was calculated as two-times the SD deviation in heart rate and respiratory rate measured during sitting. Similarly, when heart rates were above 120 BPM, the acceptable variability was set at 2 times the SD for heart rate and respiratory rate measured during running.

Table 2. Heart rate and respiration rates (overall group mean and SD, N = 8) and calculated acceptable ranges (minima and maxima) for heart rates and respiration rates (defined as laboratory values $\pm 2SD$)

	Sitting		Running		Range	
	Value	SD	Value	SD	Min	Max
Heart Rate ¹	74	6.6	153	15.7	61	184
Respiration Rate ¹	16	2.1	38	6.1	12	50

¹ Group mean and SD calculated by pooling data from all subjects for a given condition (sitting or running).

Table 3. Parameter variance thresholds based upon lab validation study activities for periods where heart rate is above or below 120 BPM

	Acceptable Heart Rate variability (2 × SD)	Acceptable Respiration Rate variability (2 × SD)
HR < 120 BPM	26	8
HR ≥ 120 BPM	62	24

Skin Temperature Data Quality

Skin temperatures with a rate of change ≥ 1 °C / min were defined as outliers, and noted. Skin temperature in the VSDS is measured by an insulated thermistor embedded in a cloth electrode that forms part of the VSDS chest strap. Consequently, the signal variance over time tends to be minimal. Rather than increased data variability, aberrant data tend to be extraneous, outlier data points.

VSDS Vital Sign Algorithm Performance

The VSDS incorporates a vital sign detection algorithm. This algorithm is designed to determine the absence of or grossly abnormal heart activity, respiration, or movement. The algorithm provides five outputs: green – “OK”, yellow – “look”, red – “look now”, gray – “absence of vital signs > 5 minutes, and blue – “unknown or fault” (6). In the present study, we anticipated only green or blue outputs since yellow, red, or gray outputs are usually associated with serious medical events. In this study, the analysis of VSDS algorithm output was limited to quantifying the number of false positives – that is; the number of times a state other than blue or green was output. The ratio of blue states to green states was also calculated.

System Acceptability

A questionnaire was used to assess the acceptability of the VSDS to the CST-WMD team members (Appendix B). Subjective ratings of the VSDS components were collected for fit, comfort, performance effects, physical impact, and overall acceptability. A variant of this survey was recently used to assess the form, fit, comfort, and

performance acceptability while performing a training exercise in an urban combat environment (5).

User comments regarding the utility and manner of presentation of real-time physiological information were also obtained using a questionnaire (Appendix C). The GUI used during this experiment was designed following recommendations from U.S. Army medics (9), with the exception that personal identifiers were not used.

PROCEDURES

Before the start of each day's training exercise, meteorological and micro-meteorological monitors were positioned near the training sites and set to log data. Physiological monitoring systems, except the VSDS, were pre-mounted to CST-WMD utility vests. When the volunteers arrived, they were fitted with a VSDS belt based upon chest size and the manufacturer's sizing chart. If a belt was too tight, an elastic extender was used to obtain the correct belt tension. A sensor electronics module (SEM) was turned on and snapped onto each volunteer's VSDS chest belt. The VSDS was deemed to be functioning when the device provided a pager-style triple buzz, and VSDS data reception at the base station laptop was confirmed. If no data was received at the base station, the VSDS and hub were reset.

Midway through the first day of training, when systems were exchanged between the first and second set of six volunteers, the VSDS belts were rinsed with water and left to dry for approximately one hour. At the end of each day, systems were retrieved from the volunteers. The VSDS belts were rinsed with water and left to air dry, and stored data were downloaded for subsequent analysis.

All volunteers were asked to view the base station GUI during their training exercise. After the training exercise, volunteers completed two surveys, one on GUI acceptability and one on the acceptability of the VSDS system itself.

STATISTICAL ANALYSIS


To examine whether average physiological parameters changed by training session, a single factor (training session) analysis of variance (ANOVA) was employed with level of significance set at $p < 0.05$. A Pearson's product-moment correlation coefficient was used to examine the level of association between selected variables. A two-tailed Student's independent samples t-test was used to examine differences between means from two groups where the level of significance was set at $p < 0.05$. Data are reported as mean \pm SD.

RESULTS

METEOROLOGICAL CONDITIONS

Figure 7 shows the air temperature, relative humidity, solar radiation, and wind speed for the two training exercises as measured by the Campbell Scientific CR-10X weather station. Day 2 was warmer and more humid than Day 1.

Figure 7. Local meteorological conditions for training days 1 and 2

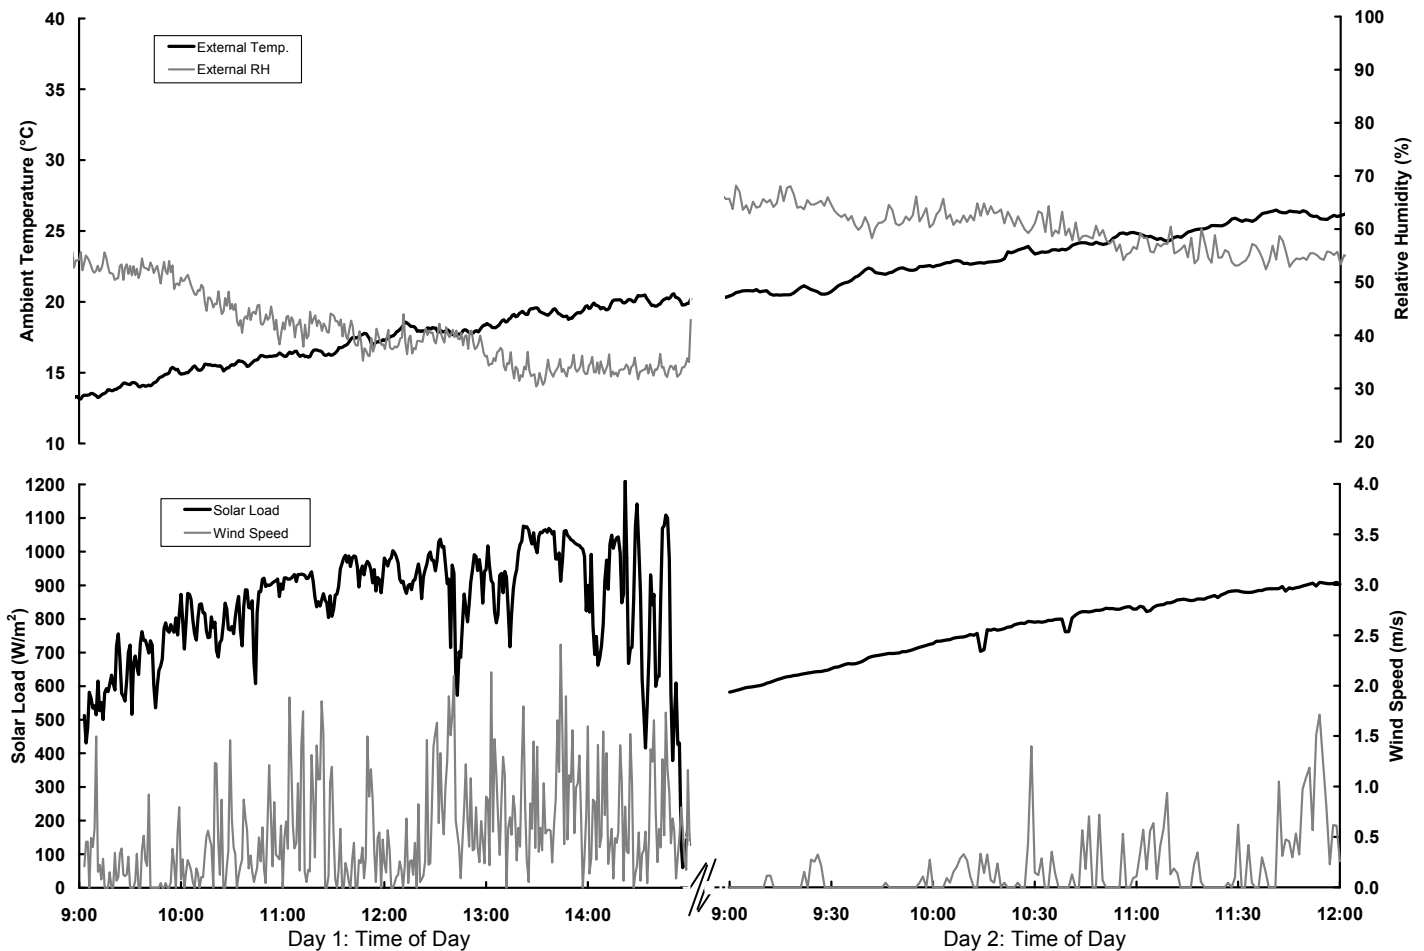

The enclosed space temperatures from the HOBO® Pro v2 monitors are presented for Day 1 in Figure 8 and for Day 2 in Figure 9. Compared to the metal containers used during Day 2 training, the micro-meteorological conditions in the concrete tanks on Day 1 were more stable, with temperatures from all sensors generally within 1.5 °C of each other. For the same tank location (north, south, or east) the upper concrete tank was warmer than the lower. Conversely relative humidity was higher in the lower tank compared to the upper. Temperatures within the concrete tanks were similar to external air temperature.

At the firefighter training site (metal containers), the temperatures near the east facing container walls were warmer than those near the interior walls or north or west-facing walls by as much as 10 °C. Relative humidity in the metal containers shows a reverse trend, lowest on east, higher on the other walls and interior wall - a trend related to the "relative" function as the same amount of moisture in warmer air is "drier". Temperatures in the metal containers were between 5 °C and 12 °C warmer than the external temperatures, at the hottest points reaching as high as 38.5 °C (101.3 °F).

Figure 8. Day 1: Reinforced concrete enclosed space air temperature and relative humidity


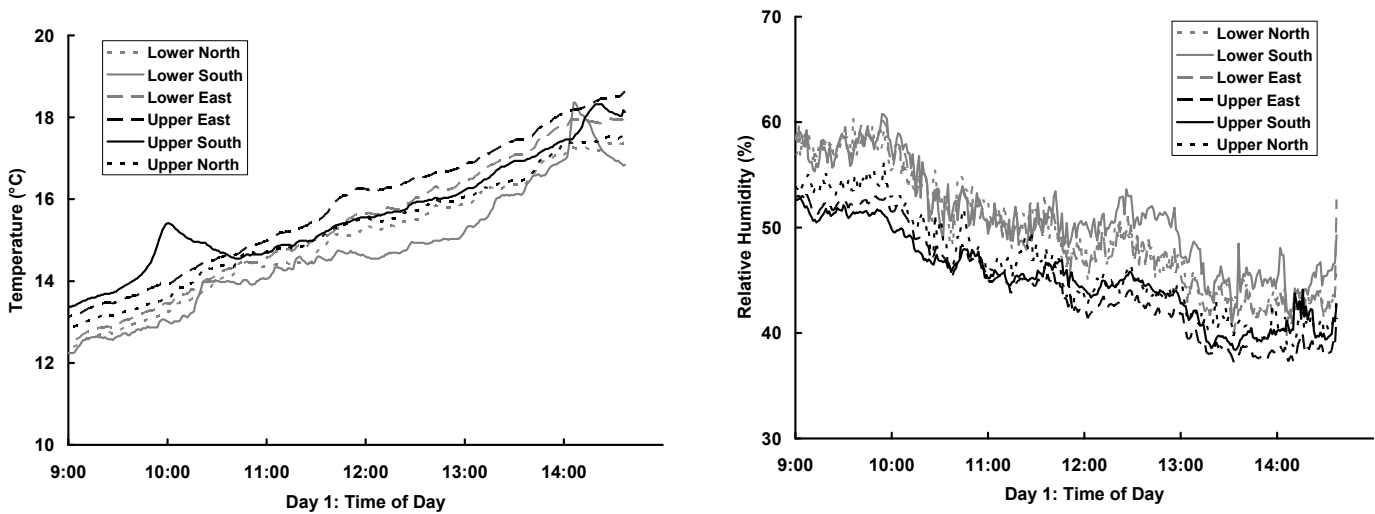


Figure 9. Day 2: Metal enclosed space air temperature and relative humidity

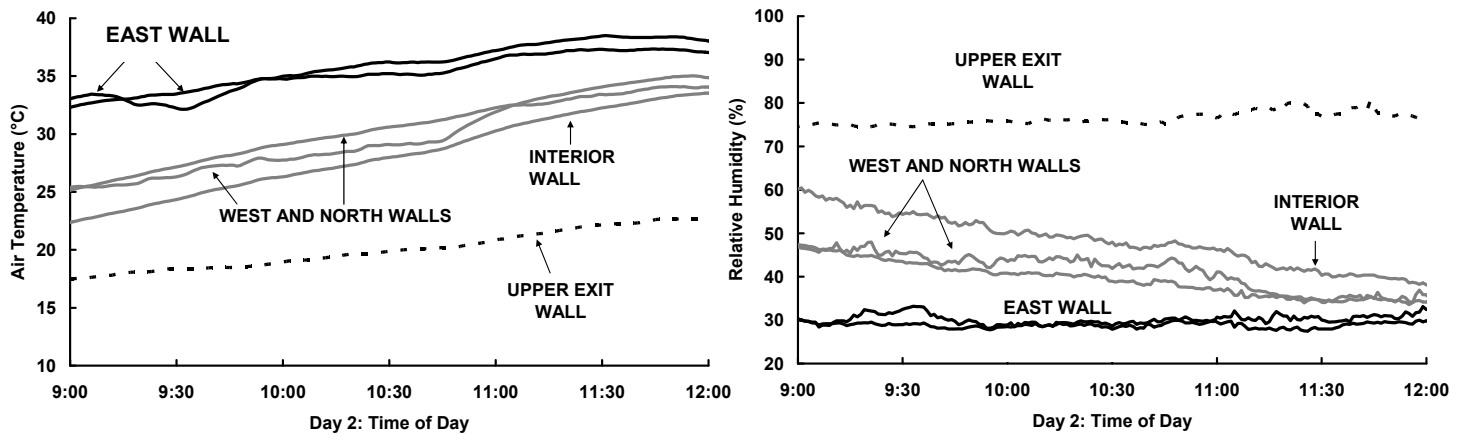

PHYSIOLOGICAL MONITORING

Data availability, and heart rate and respiration rate data quality are presented in Table 4 for each volunteer for each training session. Skin temperature data quality and vital sign detection algorithm performance are presented in Table 5. Overall, the VSIDS performed similarly across the three training sessions for all volunteers, with 98.9% of

expected data received at the base station. Plots of data for each system can be found in Appendix D. An example of the time series physiological data is presented in Figure 10.

Table 4. Heart and respiration rate data availability and data quality for each test period

Subj	Data Rec'd (%)	Heart Rate						Respiration Rate					
		Out of Range (%) ¹	Min (BPM)	Mean (BPM)	Max (BPM)	Large Var. (%) ²	Mean SD (BPM) ³	Out of Range (%) ¹	Min (Br/M)	Mean (Br/M)	Max (Br/M)	Large Var. (%) ²	Mean SD (Br/M) ³
Day 1 – Morning: Chase Precast (1015 – 1200 h)													
1	99.5	0.0	62	89	135	12.3	8	0.0	15	27	38	22.6	3
2	98.8	0.0	68	82	105	0.0	5	1.4	15	30	60	48.1	5
3	99.0	0.0	85	105	137	10.0	8	0.0	16	26	38	17.1	3
4	100.0	0.0	70	86	118	5.3	7	0.0	13	23	36	24.9	3
5	100.0	3.8	9	99	119	6.0	5	1.5	11	23	35	18.3	3
6	100.0	0.0	71	94	149	17.5	8	0.0	15	29	48	60.0	5
Mean	99.6	0.6	61	92	127	8.5	7	0.5	14	26	43	31.8	4
Day 1 – Afternoon: Chase Precast (1330 – 1420 h)													
7	100.0	0.0	72	92	141	8.5	8	0.0	16	27	42	48.5	4
8	100.0	0.0	72	86	117	7.5	6	0.0	15	26	40	35.5	4
9	100.0	0.0	83	99	129	2.5	6	0.0	19	29	42	46.0	4
10	100.0	1.0	42	100	127	8.5	7	0.5	7	25	34	17.5	3
11	100.0	0.0	91	120	146	6.3	10	0.6	8	28	37	21.1	4
12	97.0	0.0	64	89	126	14.5	9	3.5	11	28	57	76.0	6
Mean	99.5	0.2	71	98	131	8.0	8	0.8	12	27	42	40.8	4
Day 2: Firefighter Training Site (0930 – 1150 h)													
1	98.5	0.0	66	104	181	9.6	9	0.0	12	26	41	24.5	4
2	95.0	0.0	73	91	134	7.7	7	6.1	17	38	60	51.2	5
3	99.8	0.0	87	109	159	0.9	7	0.5	14	26	57	28.0	4
4	98.1	0.0	72	94	160	2.4	5	0.2	17	28	55	41.1	4
5	97.1	0.0	88	99	122	0.0	3	3.6	17	35	56	67.2	5
6	97.9	0.0	73	100	166	5.7	8	1.2	9	28	59	41.8	5
Mean	97.7	0.0	77	99	154	4.4	6	1.9	14	30	55	42.3	4
Grand Mean													
Mean	98.9	0.3	69	96	136	7.0	7	1.1	14	28	46	38.3	4

¹ Out of Range: heart rate or respiration rate was outside the range defined in Table 2

² Large Var.: large variability, that is, heart rate or respiration rate standard deviation exceeded pre-set standards.

³ Mean SD: mean of the standard deviations of 4 minute moving average.

Table 5. Chest skin temperature data quality and vital sign algorithm state for each test period


Sub	Chest Temperature					Vital Sign Algorithm ³				
	Min (°C)	Mean (°C)	Max (°C)	Mean dT/dt ¹	High Rate of Change (%) ²	Blue (%)	Green (%)	Yellow (%)	Red (%)	Gray (%)
Day 1 – Morning: Chase Precast (1015 – 1200 h)										
1	26.2	27.8	29.8	0.10	0.0	10.5	89.5	0	0	0
2	28.4	29.7	36.8	0.15	1.2	10.6	89.4	0	0	0
3	25.1	27.3	31.1	0.12	0.5	12.5	87.5	0	0	0
4	31.4	33.1	35.3	0.10	0.5	2.4	97.6	0	0	0
5	28.2	32.0	35.9	0.28	4.3	48.0	52.0	0	0	0
6	27.5	29.3	32.9	0.29	3.4	0.0	100.0	0	0	0
mean	27.8	29.9	33.6	0.17	1.6	14.0	86.0	0	0	0
Day 1 – Afternoon: Chase Precast (1330 – 1420 h)										
7	27.8	29.8	31.1	0.19	0.0	19.7	80.3	0	0	0
8	26.8	28.5	29.8	0.18	0.0	6.5	93.5	0	0	0
9	26.3	27.3	29.0	0.34	4.5	7.0	93.0	0	0	0
10	27.9	29.1	30.2	0.15	0.0	12.4	87.6	0	0	0
11	30.3	31.5	32.3	0.12	0.0	14.2	85.8	0	0	0
12	29.8	31.8	33.4	0.18	2.6	14.4	85.6	0	0	0
mean	28.2	29.7	31.0	0.19	1.2	12.4	87.6	0	0	0
Day 2: Firefighter Training Site (0930 – 1150 h)										
1	23.3	30.6	35.7	0.12	0.0	7.2	92.8	0	0	0
2	27.3	30.5	33.2	0.12	0.7	62.3	37.7	0	0	0
3	25.0	31.4	36.1	0.13	0.0	4.3	95.7	0	0	0
4	31.0	31.9	33.3	0.16	3.9	0.7	99.3	0	0	0
5	29.9	31.5	33.0	0.09	0.4	22.1	77.9	0	0	0
6	30.4	32.9	36.2	0.11	0.4	11.2	88.8	0	0	0
mean	27.8	31.4	34.6	0.12	0.9	18.0	82.0	0	0	0
Grand Mean										
mean	27.9	30.3	33.1	0.16	1.2	14.8	85.2	0	0	0

¹ Mean absolute rate of change of chest temperature (°C/Min)

² Percentage of data points where the rate of change exceeds 1.0 °C/Min

³ Vital Sign Algorithm: Blue = "Unknown or Fault", Green = "OK", Yellow = "Look", Red = "Look Now", and Gray = "Absence of vital signs for > 5 min"

Figure 10. Representative time series heart rate, respiration rate and skin temperature data for one volunteer during Day 2 training

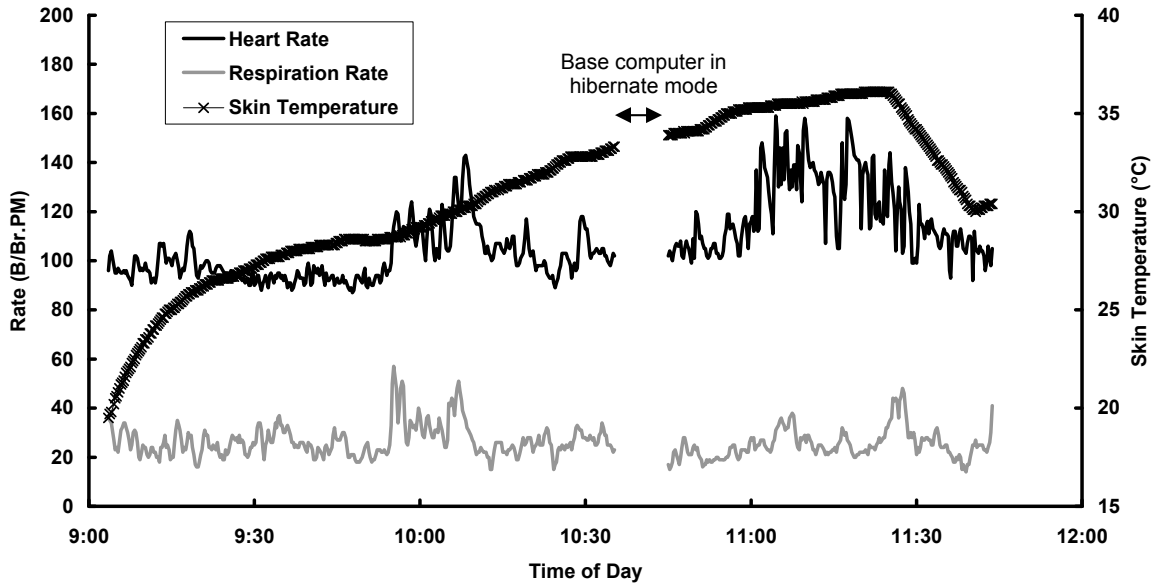

Heart Rate

Over the three training sessions, average HR did not vary significantly ($F = 0.98$, $df = 2$, $p = 0.40$). The number of HR data points outside of the physiologically reasonable range was $0.3 \pm 0.9\%$, and 0% for all but two volunteers. The percentage of data points where the surrounding data exhibited a large variance was also relatively modest (mean = $7.0 \pm 4.8\%$).

Respiration Rate


Over the three training sessions, average respiration rate did not vary significantly ($F = 1.98$, $df = 2$, $p = 0.17$). The number of respiration rate data points outside the physiologically reasonable range was modest ($1.1 \pm 1.7\%$). However, the percentage of data points exhibiting a large variance was $38.3 \pm 18.0\%$, with substantial differences between volunteers. For example 76% of the respiration rate data exceeded the acceptable, pre-established acceptable level of variability (Figure 11). For the first two training sessions, where standing was predominant, the average respiration rate (26.8 ± 2.3 Br/Min) was significantly ($t = 9.97$, $df = 18$, $P < 0.01$) higher than in the standing condition for the VSDS laboratory validation study (16.0 ± 2.1 Br/Min).

Skin Temperature

Average chest skin temperatures did not vary significantly over the three training sessions ($F = 1.88$, $df = 2$, $p = 0.19$). Chest skin temperature data changed gradually

(Figure 10), at an average rate of 0.16 °C per minute. Fewer than 2% of the skin temperature data points would be higher or lower than expected (Figure 11).

Figure 11. Data from a single volunteer from Day 1 training showing an example of an aberrant chest skin temperature reading, and excessively variable respiration rate data

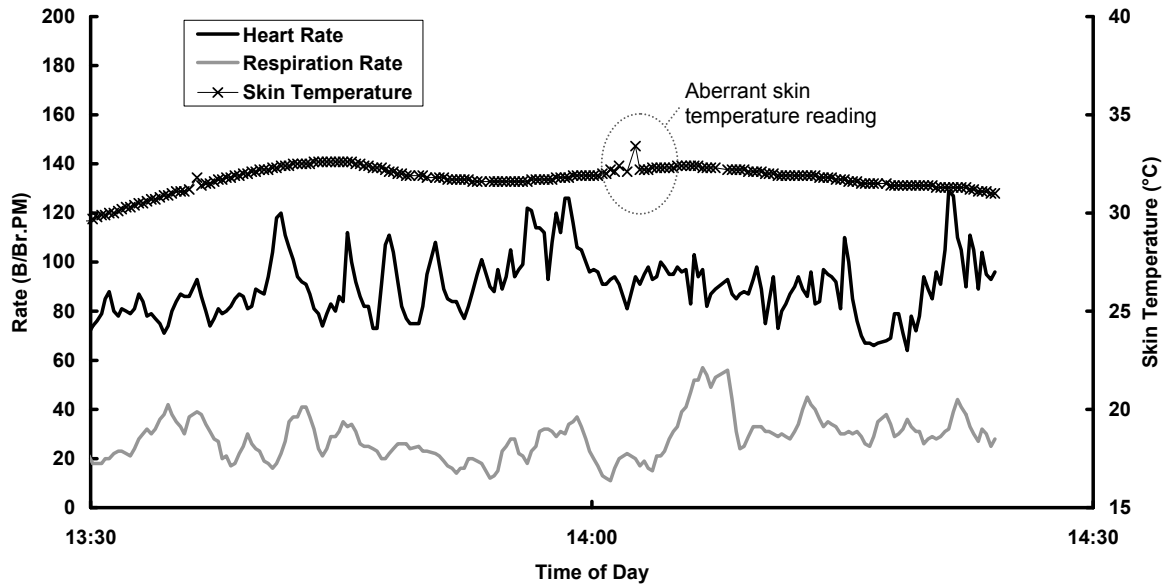

Vital Sign Detection Algorithm

Table 5 shows the VSDS algorithm outputs listing the percentage of time each state was given for each volunteer for each event. No false positives were output by the algorithm. The average percent of time a “blue” state was given varied across volunteers ($15 \pm 16\%$, median = 11%), with two volunteers receiving 48% and 62% blue state outputs. There was no correlation between the high respiration rate variance and the percentage of time a blue state was indicated ($r = 0.06$).

SYSTEM ACCEPTABILITY

Volunteers ($n = 12$) wore the VSDS for 4.0 ± 2.6 hours (range: 1 to 8 h). When they were asked if the system fit properly, 11 of 12 volunteers said it did. The one volunteer who found the system did not fit properly said that he needed a VSDS chest strap extender to achieve a correct fit. Ratings for fit by body area are summarized in Table 6. Table 7 tabulates whether the device was too tight or too loose by body area.

Table 6. Fit of the Vital Sign Detection System (VSDS) for various areas of the body

	Dislike Very Much	Dislike Moderately	Dislike Slightly	Neither Like nor Dislike	Like Slightly	Like Moderately	Like Very Much
Chest	0	0	1	1	2	5	3
Shoulders	0	0	0	2	0	7	3
Neck	1	0	0	1	0	7	3
Back	0	0	2	1	1	5	3
Overall	0	0	0	2	0	7	3

Table 7. Tightness/looseness of the Vital Sign Detection System (VSDS) for various areas of the body

	Very Tight	Moderately Tight	Slightly Tight	Neither Tight nor Loose	Slightly Loose	Moderately Loose	Very Loose
Chest	0	4	3	4	1	0	0
Shoulders	0	2	1	8	1	0	0
Neck	0	2	1	8	1	0	0
Back	0	1	4	6	1	0	0
Overall	0	1	4	5	1	0	1

With the exception of one individual, CST-WMD volunteers felt the VSDS was comfortable to wear. Figure 12 summarizes overall comfort ratings; while Table 8 summarizes comfort by the individual components of the VSDS (see VSDS component illustration in Appendix B, p. 35). With the exception of the chest strap adjustment fastener, the components were rated in the comfortable range. When volunteers who found the device uncomfortable in some way were asked if there was a specific activity when they experienced the discomfort, the three comments all dealt with the bulkiness of the device and its use in confined spaces. Comments offered were:

- “It pulled or compressed the chest.”
- “With tight spaces it rubs against my chest.”
- “With SCBA [self contained breathing apparatus], helmet, and gloves, we crawled through 30 inch or smaller tubes simulating confined space. The VSDS constricted movement. Pressured chest vest [i.e. we assume this means the hub and radio mounted on the volunteer’s webbing gear – author added comment] was more of a problem than VSDS though.”

Figure 12. Vital Sign Detection System (VS DS) overall comfort rating

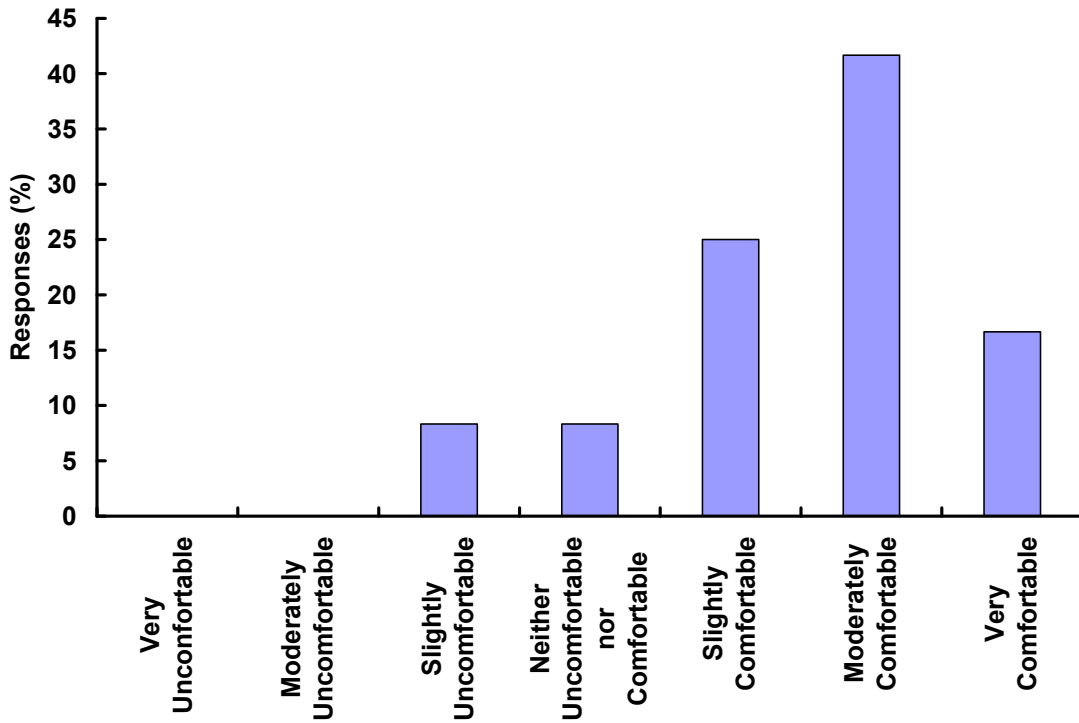


Table 8. Comfort of various parts of the Vital Sign Detection System (VS DS)

	Very Un-comfortable	Moderately Un-comfortable	Slightly Un-comfortable	Neither Un-Comfortable nor Comfortable	Slightly Comfortable	Moderately Comfortable	Very Comfortable
Electrodes	0	0	1	1	2	6	2
Water Proof Material	0	0	0	3	1	6	2
Central Belt Area	0	0	1	1	2	6	2
Belt Elastic	0	0	1	1	2	6	2
Belt Elastic Stitching	0	0	2	1	3	4	2
Shoulder Belt Adjuster	0	0	1	1	3	5	2
Adjustment Fastener	0	0	4	1	1	4	2

CST-WMD personnel were asked “Overall, from wearing the VS DS was there any negative impact on job performance? In response, 67% (8 of 12 volunteers) said there was no impact and the others (33%; 4 of 12 volunteers) said there was a slight negative impact on job performance. When specifically asked about how job performance was impacted in terms of ease of motion, ease of movement, and bending, 6, 5 and 4 individuals, respectively, stated that there was a slight negative impact on these activities from wearing the VS DS.

Two individuals cited that irritation of the skin on the back was a problem, with one individual specifically attributing the skin irritation to the adjustment fitting on the shoulder strap. Figure 13 is a photo of a test volunteer after wearing the VS DS showing

skin irritation on his back from the shoulder strap adjustment fitting. When asked if any of the VSIDS components had any negative impact, two individuals cited the shoulder strap adjustment fitting. Table 9 lists the VSIDS sub-components and the level of negative impact, if any. No systems broke during testing.

Figure 13. Mid-back skin irritation caused by wearing the Vital Sign Detection System (VSIDS) after four hours of training



Table 9. Sources of negative comments regarding various parts of the VSIDS

	Extreme Negative Impact	Very Negative Impact	Moderate Negative Impact	Slight Negative Impact	No Negative Impact
Electrodes	0	0	0	2	10
Water Proof Material	0	0	0	2	10
Central Belt Area	0	0	0	4	8
Belt Elastic	0	0	0	3	9
Belt Elastic Stitching	0	0	0	4	8
Shoulder Belt Adjuster	0	0	2	1	9
Adjustment Fastener	0	0	0	4	8
Overall VSIDS	0	0	0	4	8

When volunteers were asked if the VSIDS was acceptable, 92% (11 of 12) said it was. The one individual who found the VSIDS unacceptable said it was “because of the bulk of the chest piece.” When asked “If the system would help medics or medical officers identify medical emergencies sooner, would you wear the system?”, again all but one individual said they would. When volunteers were asked if they had any additional comments regarding the system, the following comments were provided:

- “I did not even notice I was wearing it; fit very well. I assume that I could wear it for 8 hours or more. I only wore it for about 1.5 hours.”

- “I would like if you could make the chest piece smaller and thinner. Other than that I like the idea.”
- “Smaller is better, lose the wires and build into a shirt.”
- “The only hindrance was in the vest with wiring. The actual monitor was fine to wear. More sensors would be good, covering other areas of the chest and back for detection.”

GRAPHICAL USER INTERFACE ASSESSMENT

Of the 13 volunteers, 12 observed the computer screen that showed data being displayed in real-time as CST-WMD personnel completed their training exercise. Eight volunteers observed the screen approximately 1-5 mins, three volunteers observed the screen approximately 5-10 mins, and 1 volunteer (the physician assistant) observed the screen for approximately 8 hours over 2 days of testing. The screen that was available to be viewed was the Team List Screen (Figure 5 above). Ten volunteers thought this screen provided enough information, while two volunteers thought it did not provide enough information. One volunteer wanted individual names displayed, and the other volunteer felt the respiration rate values were not valid. Figure 14 shows utility ratings of the Team List Screen for CST-WMD personnel. Table 10 lists improvements to Team List Screen suggested by the test volunteers.

Figure 14. Utility ratings of the Team List screen for CST-WMD personnel

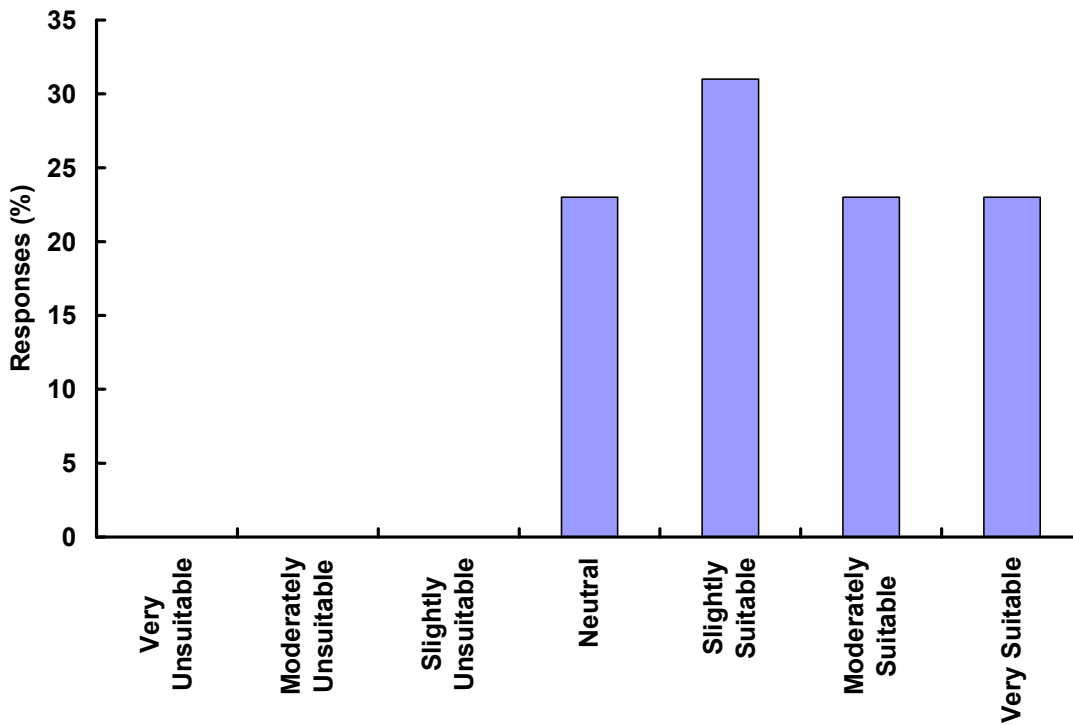


Table 10. Suggested improvements to the Team List Screen

Feature	N
List Individuals by Name	5
ECG Display	2
Blood Pressure	2
Temperature in both F and C	1
Color Code all Columns	1
Pulse Oximetry	1
Show Direction Person is Facing	1
Sort Individuals by Team Down Range	1
Show Accurate Time	1
Core Temperature	1
List Individuals Job Position	1
Do Not Have Automatic Screen Saver	1

Volunteers were also asked to provide feedback on GUI screens previously developed by U.S. Army medics (9) but not used in the present study (See appendix C). In addition to the twelve volunteers who wore the systems and the medical officer also completed this survey. Table 11 is a list of the various previously-developed concept screens and the “as is” ratings these screen concepts were given by the CST-WMD test volunteers. The highest rated screen was the Individual Warfighter Status screen with 77% of responses indicating moderately or very suitable ratings. All volunteers gave it better than a neutral rating. The lowest rated screen was the Squad Status screen with only 38% of volunteers giving it positive ratings and 31% of volunteers reporting it was slightly to very unsuitable for CST-WMD use.

Table 11. Ratings of the various concept screens that were previously developed from U.S. Army Medic feedback

Ratings	Concept GUI Screens Evaluated						
	Map Location	Squad Status	Name List	Individual Warfighter Status	Treat Administered	Medical Field Card	Reference Center
Very Unsuitable	1	1	0	0	1	1	1
Moderately Unsuitable	1	1	0	0	0	0	0
Slightly Unsuitable	0	2	0	0	0	0	0
Neutral	2	2	3	0	1	1	2
Slightly Suitable	2	2	4	3	2	3	3
Moderately Suitable	3	2	3	1	4	1	1
Very Suitable	4	3	3	9	5	7	6
% Favorable Responses to Concept	54%	38%	46%	77%	69%	62%	54%

Map Screen Improvements

The most frequently suggested improvements to the map screen would be to have buildings and streets represented on the map ($n = 6$) and a GPS reference on the

map ($n = 3$). Two individuals did not understand what the colored symbols on the map represented. The colored symbols represented the life-sign state of the Soldiers a medic is monitoring.

Squad Status Screen Improvements

The most frequent suggestion to improve the squad status screen was to change “squad status” to “entry team” and “back-up team” status ($n = 4$). Others commented that a legend was needed ($n = 1$) and an ability to track the location of teams in the building was needed ($n = 1$).

Name List Screen Improvements

Three improvements were suggested for the name list screen by one individual each: 1) the Ballistic Impact Detection System (BIDS) signal was not needed for CST-WMD personnel, 2) listing the type of PPE (personal protective equipment), and the amount of air remaining in the SCBA would be helpful, and 3) listing the distance from the cold zone (uncontaminated zone) would be useful.

Individual Warfighter Status Screen Improvements

Two improvements were suggested for the individual Warfighter screen by one individual each. One individual suggested doing away with the BIDS figure and replacing it with information on core temperature, EGG, and body orientation. The second individual suggested adding information of the patient’s duty position and section.

Treatment Screen Improvements

Two individuals suggested that injuries and treatments be more aligned with problems and treatments associated with a CBRN environment. Other comments regarding this screen were also provided, including “keep this screen”, “great”, and “good information page.”

Medical Field Card Screen Improvements

The only improvement suggested to this screen was to have the forms issued by first responders who work with the 1st CST-WMD, such as Massachusetts Emergency Medical Services. Other comments provided by one individual each regarding this screen was “awesome,” “good for medical use,” and “good to have an electronic copy on site in case the paper copy gets lost.”

Reference Center Screen Improvements

The only comment regarding improving this screen was that the language translator may not be necessary.

DISCUSSION

This study successfully demonstrated real-time physiological status monitoring of encapsulated 1st CST-WMD in an operationally-relevant field environment. The WPSM-IC VSDS, medical hub, COTS radio and COTS GPS systems were used. The

test and evaluation assessed the ability to acquire and transmit physiological information, acceptability of the system to CST-WMD personnel, usefulness of the physiological information to the medical officer, and suitability of GUI.

ABILITY TO PROVIDE REMOTE PHYSIOLOGICAL INFORMATION

The WPSM system, as configured with the VSIDS sensor system and the COTS radio telemetry, performed in a reliable and apparently valid fashion. The validity of the physiological data generated by the VSIDS was previously established in the laboratory (8) and as part of FDA 510k certification process. Real time physiological information was provided every 15 s for all team members fitted with a WPSM system over the course of the two training events with a minimal loss of data (mean data loss = 1.1%, ranging from 0% to 5%). Of the physiological data transmitted, almost all were within physiologically-reasonable bounds (98.7%). The quality of heart rate and skin temperature data was similar to the reference standard heart rate and skin temperature data collected during a VSIDS laboratory validation study (8). However, the respiration rate data was greater and more variable than measured during similar activities in the laboratory validation study. Upon closer analysis, the VSIDS firmware version (Semsoft4-0053.a90) was discovered to be an obsolete prototype version that had been used in error. Presumably, the poor performance of the respiration rate sensor can be attributed to this error. The same VSIDS devices, with updated respiration rate detection firmware, have since been demonstrated to perform as expected (10).

Although the vital sign detection algorithm generated no false positives, the number of “blue” or “unknown” states reported was unacceptably high. Given that a less-stable and less-accurate version of the respiration rate algorithm was running in the VSIDS, as discussed above, it is not surprising that there was a decreased confidence in the respiration rate data output by the algorithm. Furthermore, the nature of the vital sign detection algorithm is such that a single no-confidence event, e.g., out of bounds respiration rate, results in a three minute (15 data point) “blue state.” Thus, a modest number of anomalous data points can result in a protracted “blue” state. For example, for one volunteer the VSIDS did not exit the initial blue state for nearly two hours because the respiration rate confidence was not stable enough to allow a transition to a “green” state. Thus, the excessive number of “blue” state indications noted in this demonstration can reasonably be attributed to the errors in the respiration rate estimation associated with a firmware version error that has since been corrected.

VSIDS ACCEPTABILITY

The VSIDS was rated as acceptable by the majority of CST-WMD personnel in this study (92%). This is a substantial improvement over an evaluation of an earlier version of the VSIDS where only 38% of respondents reported the system to be acceptable for military field use (5). There are two primary explanations for the differences in acceptability. First, results from the previous study resulted in design changes to the VSIDS. These changes, which appear to have improved overall acceptability of the system, included the following:

- The center attachment area was reduced in size with the goal of reducing sweating and irritation in the chest area.
- The belt material in the front part of the VSDS was made softer and more breathable.
- The center piece of the belt where the SEM attaches was made more rigid to prevent the SEM from popping off of the belt. As a result, in the present study the SEM did not pop off at all, whereas in the previous study it occurred in 39% of the units (7).
- The large belt buckle in the back was replaced by small metal fasteners.

The second possible reason for improved acceptability was that in the current study volunteers only wore the device for an average of 4 hours with the longest wear time of 8 hours. In the previous study, volunteers were asked if the device was acceptable to wear for 8 hours or longer and wore the system for up to 120 hours of training over 7 days including one 24 hour sustained operation (5). Because of this difference and the small sample size, it is recommended that future testing with CST-WMD personnel include wearing the system for longer periods of time, include different types of training exercises, and include other CST-WMD units besides just the 1st CST-WMD to ensure the results can be generalized to the entire CST-WMD community.

One area that still needs improvement is to reduce the skin irritation associated with the shoulder belt adjuster and the adjustment fastener. Skin irritation in two individuals was reported after wearing the VSDS for less than 8 hours. Presumably, wearing the VSDS for longer periods of time would increase the severity of skin irritation or increase the frequency of those who may experience some skin irritation. Ideas for improvement offered by the test volunteers included building the system into a shirt, and making the chest piece smaller and thinner, although this last suggestion probably would not address the problem of skin irritation on the back.

When volunteers were asked if they would wear the system if it allowed medical personnel to better monitor their health state, 92% of volunteers said they would. This is comparable to the 89% of volunteers from a previous study who said they would wear that system as is if it would help medics save their life (5).

USEFULNESS OF SYSTEM TO MEDICAL OFFICER

The GUI used for this study would normally include multiple screens. However, only a Team List Screen was available for evaluation. The medical officer reported that he spent approximately 8 hours observing real-time physiological information. The medical officer suggested that having this information was a valuable supplement to the information he obtained from radio discussions with down-range personnel. The medical officer reinforced the usefulness of the system by suggesting that a PDA-based display of the real time data be used, so he could move around the incident site freely

but still be able to monitor the physiology status of his team without having to return to the base station display.

SUITABILITY OF THE GRAPHICAL USER INTERFACE (GUI)

A GUI concept for the medical monitoring system was previously developed with experienced infantry medics (9). CST-WMD personnel offered, in general, positive comments on these previously developed GUI designs. As shown in Table 11, only two of the seven previously developed screens received less than 50% favorable responses. The squad status screen was not appropriate in this study because CST-WMD personnel do not operate in squads. However, it was suggested that squad status be changed to entry and back-up of reconnaissance or survey teams. In addition, it was suggested the BIDS (ballistic impact detection system) icon be removed from the main screen since this function is not relevant to the CST-WMD mission. It was recommended that having a note on the level of PPE on the Name-List screen would be helpful since CST-WMD wear different levels of PPE that impose varying levels of thermal strain. CST-WMD personnel broadly approved of the appearance and content of Name-List/Team List Screen. Under operational use, the names of individuals would be displayed, in contrast to this technology demonstration where individuals' names were not displayed to maintain medical data confidentiality.

Nine of the 12 volunteers thought the Individual Warfighter Status screen was very suitable for their use, but that the BIDS icon should be deleted. Other suggestions included adding information on personnel's core temperature, ECG, and body orientation, duty position, and section. Overall, only small changes appear to be needed for the GUI to meet the needs of the CST-WMD community. However, this was the first study with this potential customer and a small sample was used. A follow-up study with other CST-WMD units is warranted.

SYSTEM LIMITATIONS AND PLANNED IMPROVEMENTS

The physiological monitoring equipment used in this field training exercise had multiple subcomponents. That is, the VSIDS, the hub, and a COTS radio with its battery pack. This bulk of equipment (4 boxes and connecting wires) could pose a problem for reliable continuous use in missions or during training, as noted in some of the user surveys. In addition, the COTS radio modems used to transmit the data back to a base station computer were adequate for this demonstration, but were operating near capacity and could not be readily scaled to use with larger groups. For example, when multiple repeaters were used to provide adequate radio coverage during the concrete tank portion of the training some repeater messages were lost. This indicates that adding more users could potentially stress the system to the point where radio messages could be lost entirely.

To address these limitations, a new VSIDS is being developed which will be able to receive other sensor data directly, eliminating the need for a medical hub. In addition, this new VSIDS will have the ability to (a) use core temperature (obtained from a thermometer pill) and heart rate data to calculate thermal/work strain or a

“Physiological Strain Index” (PSI) (11), and (b) through a newly developed algorithm predict core temperature of up to 20 minutes into the future with relative confidence levels (12). A number of commercial efforts are underway to improve data telemetry capabilities. Additional future work will concentrate on developing an integrated Thermal Injury Prevention System (TIPS), which will encompass mission planning tools such as the Heat Strain Decision Aid (HSDA) (13), real time monitoring with advanced sensors such as heat flux sensors (14), and novel algorithms to predict thermal state.

CONCLUSIONS

The physiological information displayed in real time was found to be useful in the monitoring of CST-WMD personnel. The physiological monitoring system provided reasonable data with almost 100% continuous monitoring of all participating team members. However, the respiration rate measurements were found to be in error (i.e., they were too high) because of a firmware error. Nevertheless, the relative change in respiration rates was seen as useful by the CST-WMD medical officer.

The VSDS, although relatively large to be worn routinely on the chest, was generally found to be satisfactory for CST-WMD missions, and useful for monitoring of CST-WMD personnel in real mission situations of eight hours or less. It is likely that skin irritation will remain an issue for some individuals, especially if required to wear the VSDS for longer than 8 hours.

The GUI previously developed for combat medics, listed each individual CST-WMD team member and their medical status. This GUI was found to provide adequate information regarding individual health status. However, an additional “drill down” screen providing individual physiological status trends and current individual status was desired as an additional capability. Specific recommendations that make the GUI screens more applicable to CST-WMD needs, such as having entry teams displayed instead of squads, and adding level of PPE, should also be considered.

The current WPSM VSDS was demonstrated to provide CST-WMD with the medical monitoring telemetry basic capabilities detailed in the national CST-WMD working group requirements. Ongoing improvements to the WPSM system will provide the CST-WMD with a viable system to begin medical monitoring during select missions.

SPECIFIC RECOMMENDATIONS

- Test and evaluate the new VSDS version capable of receiving and interpreting core thermometer pill data.
- The VSDS adjustment buckle should be further refined to avoid rubbing and irritation.

- The overall size of the VSIDS should be reduced to improve comfort and wear over an extended period of time.
- Confirm the functionality of the corrected respiration rate and vital signs detection algorithms.
- The WPSM display should be enhanced to include an individual's detail screen with time series data plots. The system should also be enhanced to allow the GUI to function on a PDA and receive health status message by wireless Ethernet (IEEE 802.11b/g). Future testing would include medical and/or command staff actually using the GUI on a preferred type of device (e.g., laptop computer, PDA, etc.).
- Software defined radio solutions should be identified that can reliably transfer digital data that can be readily accessed by third party applications. The radio should be capable of forming sophisticated short-range mesh networks and have the ability to link to repeaters for long range data transmission.
- Repeat testing with the enhanced equipment, a fully working GUI, with more volunteers, volunteers from different CST-WMD units, varying types of CST-WMD training exercises, and increasing the wear time of the system.

REFERENCES

1. Occupational Safety and Health Standards, Hazardous Materials, General description and discussion of the levels of protection and protective gear. U.S. Department of Labor Occupational Safety & Health Administration. Document Number: Standards – 29 CFR - 1910.120 App B. See http://www.osha.gov/pls/oshaweb/owadisp.show_document?p_table=STANDARDS&p_id=9767
2. Muza, S. R., L. E. Banderet, B. Cadarette. Protective uniforms for nuclear, biological and chemical warfare. In: *Medical Aspects of Harsh Environments*, edited by: K. B. Pandolf and R. E. Burr. Office of the Surgeon General, United States Army, Falls Church VA, Chapter 36, pp 1084 – 1127, 2001.
3. Fahy, R. F. and P. R. LeBlanc. *Firefighter Fatalities in the United States – 2005*. Quincy MA. Fire Analysis and Research Division, National Fire Protection Association. June 2006. See <http://www.nfpa.org>.
4. Smith, D. L., T. S. Manning and S. J. Petruzzello. Effect of strenuous live-fire drills on cardiovascular and psychological responses of recruit fire fighters. *Ergonomics*, 44(3): 244-254, 2001.
5. Tharion, W. J., M. J. Buller, A. J. Karis and S. P. Mullen. Acceptability of a wearable vital sign detection system. In: *Proceedings of the Human Factors Society 51st Annual Meeting*. Human Factors and Ergonomics Society, Santa Monica CA. Volume 51, p.1006-1010, 2007.
6. Buller M. J., R. W. Hoyt, J. S. Ames, W. A. Latzka, B. J. Freund. Enhancing Warfighter Readiness Through Situational Awareness – The Warfighter Physiologic Monitoring – Initial Capability. In: *11th International Conference on Human-Computer Interaction Proceedings*, Las Vegas, July 2005 (Augmented Cognition). Lawrence Erlbaum Associates, Inc (ISBN 0-8058-5807-5).
7. Tharion, W. J. *Executive summary of Aberdeen field test of the Warfighter Physiological Status Monitoring (WPSM) system with the Hidalgo Equivital™ Vital Sign Detection System (VSIDS)*. Natick, MA: U.S. Army Research Institute of Environmental Medicine, Memorandum for Record, 19 July 2006.
8. Tharion, W. J. *Reliability and Validity Test of the Hidalgo Equivital™ Vital Sign Detection System (VSIDS)*. Natick, MA: United States Army Research Institute of Environmental Medicine. Memorandum for Record, 14 June 2006.
9. Tharion, W.J. and S. Kaushik. *Graphical User Interface (GUI) for the Warfighter Physiological Status Monitoring (WPSM) System – U.S. Army Medic Recommendations*. Natick, MA: United States Army Research Institute of Environmental Medicine. Technical Report T-07-04. 2006.

10. Buller, M. J. and A. J. Karis. Heart rate and respiratory rate during fitness training, obstacle course runs, and mass casualty simulations - performance of two Warfighter Physiological Status Monitoring systems. Natick, MA: United States Army Research Institute of Environmental Medicine. Technical Report T-07-10. 2007.
11. Moran, D. S., A. Shitzer and K. B. Pandolf. A physiological strain index to evaluate heat stress. *Am J Physiol Regulatory Integrative Comp Physiol* 275:129-134, 1998.
12. Gribok, A., M. J. Buller, R. Hoyt and J. Reifman. Providing statistical measures of reliability for body core temperature predictions. In: *Proceedings of 29th International Conference of the IEEE Engineering in Medicine and Biology Society*, Lyons, France, 2007.
13. Blanchard, L. and W. Santee. *Comparison of USARIEM Heat Strain Decision Aid to Mobile Decision Aid and Standard Army Guidelines for Warm Weather Training*. Natick, MA: United States Army Research Institute of Environmental Medicine. Technical Report T-07-xx. 2007 (In preparation).
14. Gunga H. C. Wärmehaushalt und temperaturregulation. In: *Physiologie*. Edited by: Deetjen, P., E. J. Speckmann and J. Hescheler. München, Urban & Fischer 669-698, 2005.

APPENDIX A

National CST-WMD Medical Working Group Medical Monitoring Telemetry System Requirement Document. From Hoyt e-mail dated 2/21/07 this document title is 20070123.

CSTWG Submission Title: MEDICAL MONITORING TELEMETRY SYSTEM

Capability Addressed (From TDA Para 6):

6J: Provide, for assigned personnel only, preventive medicine, medical surveillance and EMT-level medical care.

6C: Determine the current contaminated area and assess current and potential hazards to personnel, animals and selected critical infrastructure features resulting from identified agent/substance presence.

Submission Sub-Group (OPS, COMMO, MED, SURVEY, LOG): MEDICAL

Action Officer POC: MAJ DAVID DOMINGUEZ / 1LT DAVID DIGREGORIO /
CPT EDWIN LEAVITT / LTC ROGER PRESZLER

Action Officer Unit: 95th CST / 1st CST / 32nd CST / 81st CST

Action Officer Email: david.dominguez1@us.army.mil / david.digregorio@us.army.mil /
edwin.leavitt@us.army.mil / roger.preszler@nd.ngb.army.mil

Action Officer Telephone: 510-750-3157 / 508-294-2741 / 443-845-6295 / 701-426-0753

Suggested Technical Working Group Lead (PTWG, TTWG, ETWG): ETWG

1. PROBLEM: Difficult to assess status of downrange personnel verbally. Most casualties demonstrate physiologic changes in vital signs and core temperature prior to collapse or loss of consciousness/death.

2. JUSTIFICATION: Proactive medical monitoring can decrease serious injuries and loss of operational strength/readiness by tracking changes and trends in vital signs/core temperatures and taking action before they become symptomatic and result in a medical emergency/"man-down" scenario.

3. SOLUTION CHARACTERISTICS: System characteristics need to have the following features/capabilities: AC/DC/Battery power; Ruggedized water resistant base station monitor and sensors capable of operating in harsh environments temperature of minus 20 up to 170 degrees. Base station requires audible and adjustable alarms. Able to tolerate humidity to 100%. Disposable oral capsule core temperature sensor; Disposable light weight heart rhythm sensor; Disposable light weight respiratory rate sensor; Disposable light weight oxymetry sensor; Ambient temperature sensor. Sensors need to be embedded into moisture wicking shirt. Wireless secure transmission of data in real-time, from sensors to monitoring station, with a distance capability of 2 miles over unobstructed open ground. Must be able to operate in confined space environment up to ½ mile; Must be able to monitor eight personnel simultaneously on a single receiving base station monitor; Must have data storage/trend graphing report capability. Must be portable as a set in a single pelican or other (rugged) type case. Must include service and technical support plan. Initial training upon fielding.

4. OPERATIONAL CONCEPT: Operated and monitored by medical personnel and employed (worn) by entry, backup and decon team personnel during level-A or B suit operations – total of eight simultaneously.

5. ORGANIZATIONAL CONCEPT: Equipment addition. Operated by medical personnel. Sensors worn by all personnel in level-A or Level-B suits.

6. PROCUREMENT OBJECTIVE: Each CST Team would require 2 base stations and any necessary signal repeaters. Also, would require multiple sets of disposable sensors per team.

7. SUPPORT REQUIREMENT: Would require maintenance, calibration, service and training support from manufacturer annually (at a minimum).

8. AVAILABILITY: Several COTS systems are currently available that meet some or most of the requirements, but fall short of some key requirements. **Specifically – Life shirt does not offer Cardiac rhythm monitoring or Core temperature. MiniMitter has research accomplished for cardiac rhythm sensor however needs to be incorporated into Transmitter information.**

9. RECOMMENDATION: Medical Telemetry systems need to be evaluated and tested on several CST teams in various climates and under extreme conditions (hot and cold), before fielding a system to the CST 's.

APPENDIX B

WPSM System Acceptability Questionnaire

Identification Number: _____



The Vital Sign Detection System (VSIDS) is a medical system that has been made to send life sign data to a medical station. The system measures breathing rate, heart rate, body position and activity. The VSIDS will allow a medical officer to identify any medical problems sooner.

The VSIDS that you have worn today is a new prototype. We would like to know your opinions about how you found wearing this device during your training exercise. By answering the questions below you will help us create a better product.

1. How long did you wear the VSIDS? _____ hours

Fit

2. Did the Vital Sign Detection System fit you properly?

Yes

No → If No: **2a.** Please explain why it did not fit you properly.


3. Using the following scale please rate how much you like or dislike the fit of the Vital Sign Detection System for the following areas:

	Dislike Very Much 1	Dislike Moderately 2	Dislike Slightly 3	Neither Like nor Dislike 4	Like Slightly 5	Like Moderately 6	Like Very Much 7
a. Overall	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
b. Chest	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
c. Shoulders	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
d. Neck	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
e. Back	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>

4. Using the following scale please rate, how tight or loose, the fit of the Vital Sign Detection System was for the following areas:

	Very Tight 1	Moderately Tight 2	Slightly Tight 3	Neither Tight nor Loose 4	Slightly Loose 5	Moderately Loose 6	Very Loose 7
a. Overall	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
b. Chest	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
c. Shoulders	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
d. Neck	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
e. Back	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>

Comfort

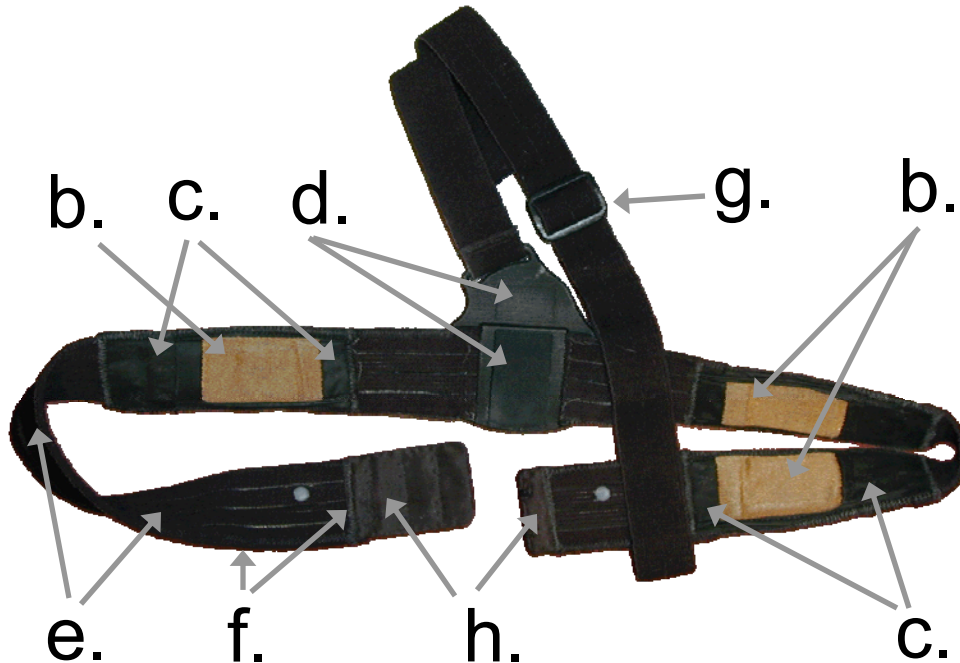

Please rate how comfortable or uncomfortable you found the VSDS during your training exercise. Rate the VSDS overall and for the individual parts of the belt listed for the question: *(Match the question letter to the belt area on the on the diagram above).*

5. COMFORT

	Very Uncomfortable	Moderately Uncomfortable	Slightly Uncomfortable	Neither Comfortable nor Uncomfortable	Slightly Comfortable	Moderately Comfortable	Very Comfortable
	1	2	3	4	5	6	7
a. Overall	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
b. Cloth Electrodes	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
c. Water Proof Material	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
d. Central Belt Area	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
e. Belt Elastic	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
f. Belt Elastic Stitching	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
g. Shoulder belt adjuster	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
h. Adjustment Fastener	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>

6. Was there a particular activity or activities during your training where you found the VSDS to be more uncomfortable?

No

Yes → If Yes:

6a. What was the activity?

6b. Please rate the overall comfort of the VSDS during this activity: _____ (*Use the comfort scale above*)

6c. Please describe the activity and how the VSDS was uncomfortable.

Activity 2:

6d. What was the activity?

6e. Please rate the overall comfort of the VSDS during this activity: _____ (*Use the comfort scale above*)

6f. Please describe the activity and how the VSDS was uncomfortable.

Performance

Please rate whether the VSDS had an impact on your overall job performance and for the other activities listed:

7. Performance Impact	Not Applicable	Extreme Negative Impact	Very Negative Impact	Moderate Negative Impact	Slight Negative Impact	No Negative Impact
		1	2	3	4	5
a. Overall impact on performance		<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
b. Ease of motion		<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
c. Ease of movement		<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
d. Rolling	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
e. Jumping	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
f. Landing	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
g. Running	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
h. Assuming a firing position	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
i. Bending	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>

Physical Impact

Impact Scale

Extreme Negative Impact	Very Negative Impact	Moderate Negative Impact	Slight Negative Impact	No Negative Impact
1	2	3	4	5

8. During your training did the VSDS cause any skin irritation, or other discomfort?


No


Yes → If Yes: **8a.** What was/were the problem/s?

8b. Please rate the overall negative impact of the problem/s: _____ (Use the impact scale above)

8c. Please describe the problem/s and how the VSDS caused it.

8d. Please indicate on the diagram below where the problem occurred.

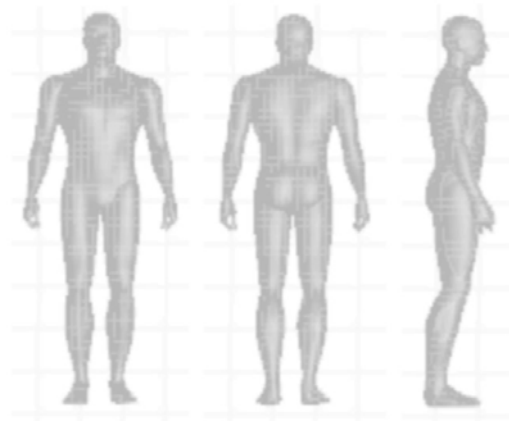

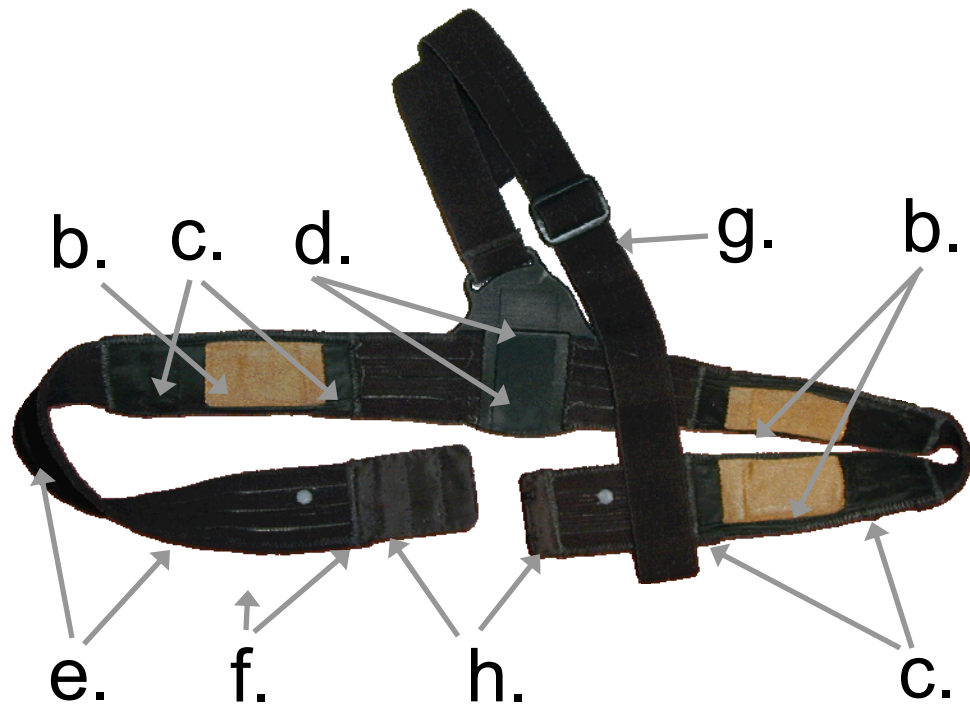

9. For each of the VSDS components listed below, please rate if there was any negative impact. (Match the question letter to the belt area on the on the diagram above).

	Extreme Negative Impact 1	Very Negative Impact 2	Moderate Negative Impact 3	Slight Negative Impact 4	No Negative Impact 5
a. Overall	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
b. Cloth Electrodes	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
c. Water Proof Material	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
d. Central Belt Area	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
e. Belt Elastic	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
f. Belt Elastic Stitching	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
g. Shoulder belt adjuster	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>
h. Adjustment Fastener	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>	<input type="radio"/>

Durability

10. Did the Vital Sign Detection System come apart or break?

No

Yes → If Yes:

10a. Please explain how the VSDS broke or came apart, and how you fixed the problem.

Acceptability

11. Is VSDS acceptable to wear for an extended period of eight hours or more?

Yes

No → If No:

11a. Please explain why the system is not acceptable.

12. If this system were able to help medics/medical officers identify medical emergencies sooner would you wear this system during missions?

Yes

No → If No:

12a. Please explain why you would not wear the system

If you have any other comments please feel free to write them below or on the back of this survey.

Thank You

APPENDIX C

Identification Number: _____

Civil Support Team – Weapons of Mass Destruction (CST-WMD)

Medical System Computer Display

Questionnaire

The medical telemetry system was designed to assess the medical status of downrange personnel, by presenting changes in vital signs and core temperature.

The medical computer display you saw today had two screens of information. The first screen (Team Screen) showed all CST-WMD personnel who were currently wearing a medical monitoring system. The second screen (Individual Screen) provided a more detailed view of an individual's medical information.

1. How long have you been in the CST-WMD? _____ years

2. What is your primary role in the CST-WMD? _____

3. Did you ONLY observe the display, or did you use the mouse and or keyboard to change something on the display?

- Observed ONLY
- Changed the display with the mouse or keyboard

4. How long did you observe or use the medical display?

- 1 – 5 Minutes
- 5 – 10 Minutes
- 10 – 20 Minutes
- 20 – 30 Minutes
- 30 – 45 Minutes
- 45 – 60 Minutes
- More than 60 Minutes
(please specify how long) _____ Hours, _____ Minutes

5. Which screens did you see or use? (check all that apply)

- Team Screen
- Individual Screen

Team Screen

6. Does the **Team Screen** provide enough information to identify personnel who may be getting into a dangerous medical condition?

Yes

No → If No:

6a. Please explain what information you would add.

7. Please list up to five things that could improve the **Team Screen** (feel free to add more points on the rear of this questionnaire).

a.

b.

c.

d.

e.

Individual Screen

8. Does the ***Individual Screen*** provide enough additional medical information about a CST-WMD member?

Yes

No → If No:

8a. Please explain what information you would add.

9. Please list up to five things that could improve the ***Individual Screen*** display (feel free to add more points on the rear of this questionnaire).

a.

b.

c.


d.

e.

Other Displays

We have worked with a number of U.S. Army medics to help define what types of screens would be most useful for displaying and using medical monitoring information for their particular jobs. For each of the following screens please rate how suitable or unsuitable each screen would be for a CST-WMD medical monitoring system.


10a. Map Location and Environmental Information

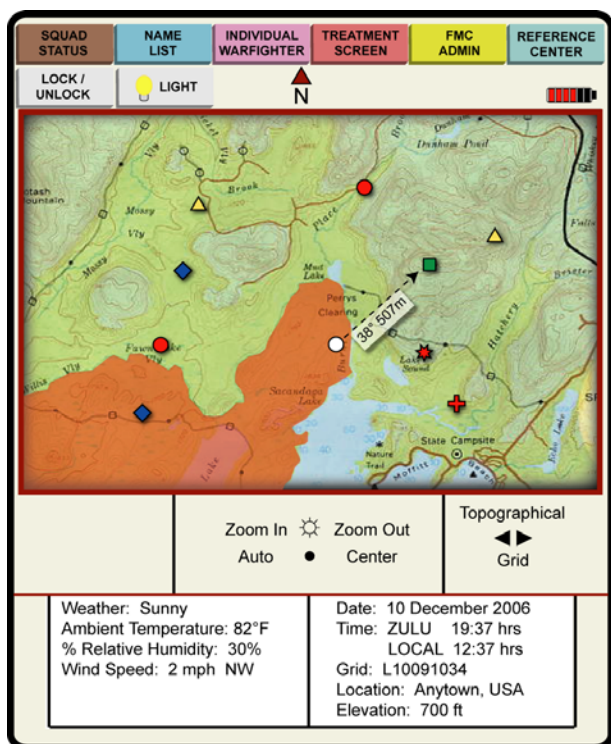

- Very Unsuitable (1)
- Moderately Unsuitable (2)
- Slightly Unsuitable (3)
- Neutral (4)
- Slightly Suitable (5)
- Moderately Suitable (6)
- Very Suitable (7)

10b. If applicable, describe how you would change this screen for CST use.

11a. Squad Status

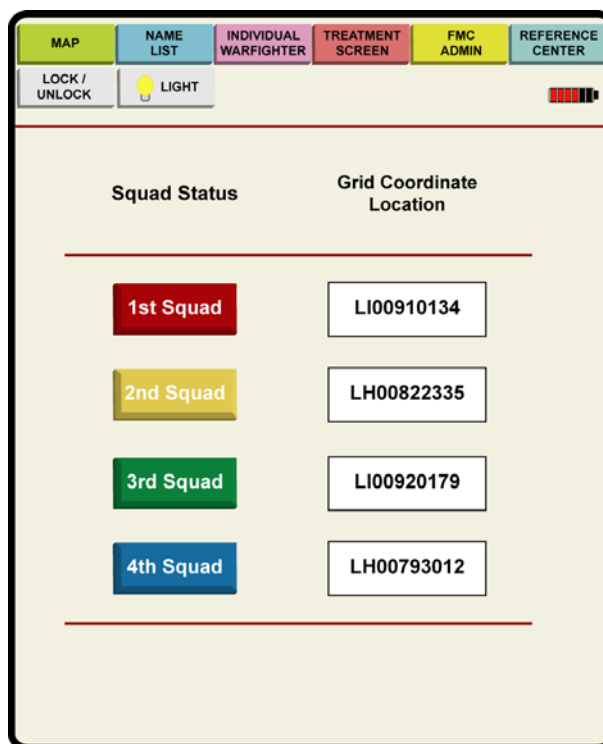

- Very Unsuitable (1)
- Moderately Unsuitable (2)
- Slightly Unsuitable (3)
- Neutral (4)
- Slightly Suitable (5)
- Moderately Suitable (6)
- Very Suitable (7)

11b. If applicable, describe how you would change this screen for CST use.

12a. Name List, Location, and Physiology

Soldier	BIDS	Distance Vehicle #	Grid Coordinate	HR	RR	T _c
▲ PVT Breen		620m	LI0910144	100	12	97
● PVT Brown		700m Veh # 81	LI0910121	165↑	7↓	96↓
★ PFC Fiske	●	440m	LI0910621	180↑	30↑	99
● SFC Gray		820m	LI0910533	99↑	12	97↓
■ LT Martinez		507m	LI0912624	75	12	99
★ SSG Price		710m	LI0910257	0	0	80
◆ SGT Thomas	—	800m	LI0911675	—	—	—
◆ SFC Tomlinson	—	900m	LI0910428	—	—	—

Fit to Fight: ■ x 1 ◆ x 2

- Very Unsuitable (1)
- Moderately Unsuitable (2)
- Slightly Unsuitable (3)
- Neutral (4)
- Slightly Suitable (5)
- Moderately Suitable (6)
- Very Suitable (7)

12b. If applicable, describe how you would change this screen for CST use.

13a. Individual Warfighter's physiological status

Rank: SSG
Age: 24
Name: Price, Brian

Gender: M
Battle Roster #: 44
Time: 1301

Heart Rate

Respiration Rate

911

- Very Unsuitable (1)
- Moderately Unsuitable (2)
- Slightly Unsuitable (3)
- Neutral (4)
- Slightly Suitable (5)
- Moderately Suitable (6)
- Very Suitable (7)

13b. If applicable, describe how you would change this screen for CST use.

16a. Reference Center



- Very Unsuitable (1)
- Moderately Unsuitable (2)
- Slightly Unsuitable (3)
- Neutral (4)
- Slightly Suitable (5)
- Moderately Suitable (6)
- Very Suitable (7)

16b. If applicable, describe how you would change this screen for CST use.


APPENDIX D


Heart rate, respiration rate, skin temperature, equipment temperature, and vital sign state time series data for Day 1 and Day 2 for each volunteer.

Vital sign state is plotted on the main Y – axis (left) with the following values:


Green	“OK”	=	0
Yellow	“Look”	=	4
Red	“Look Now”	=	8
Gray	“Absence of Vital Signs”	=	12
Blue	“Unknown / Fault”	=	16




Physiology Day 1- Morning, Chase Concrete

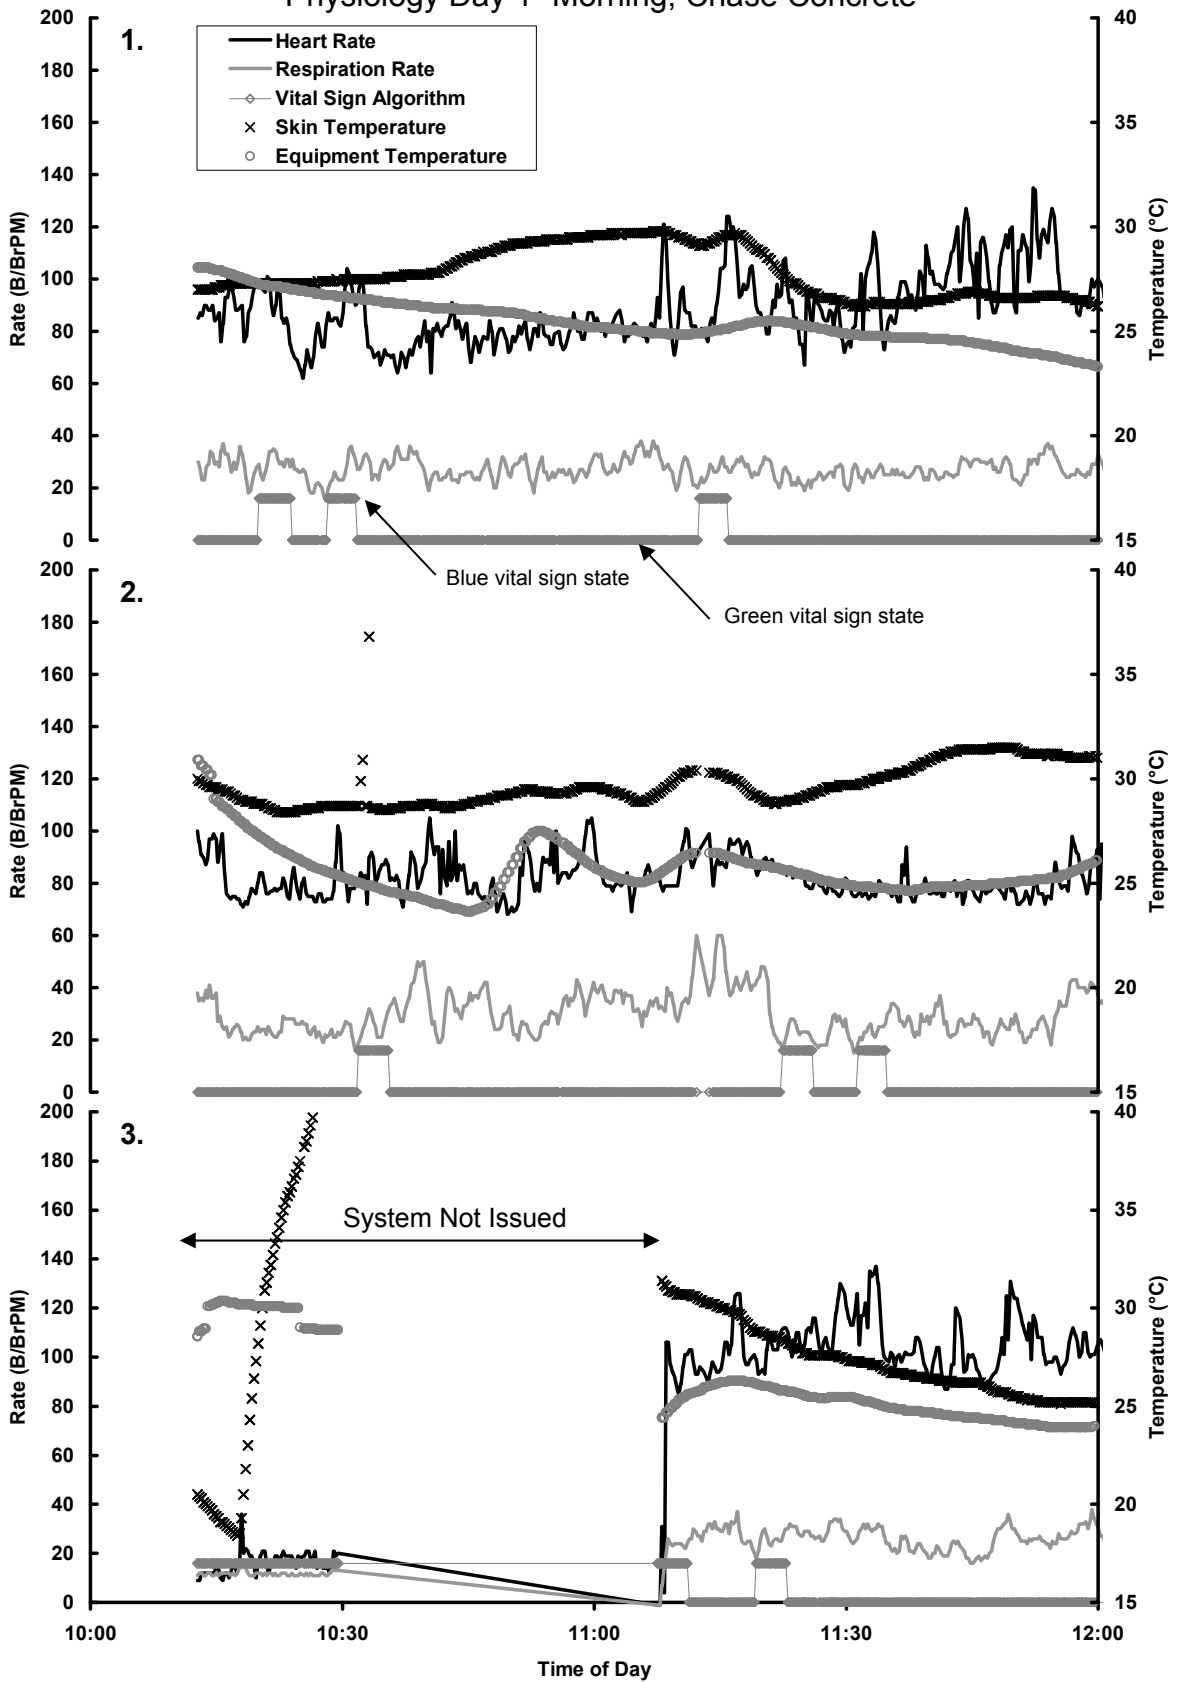

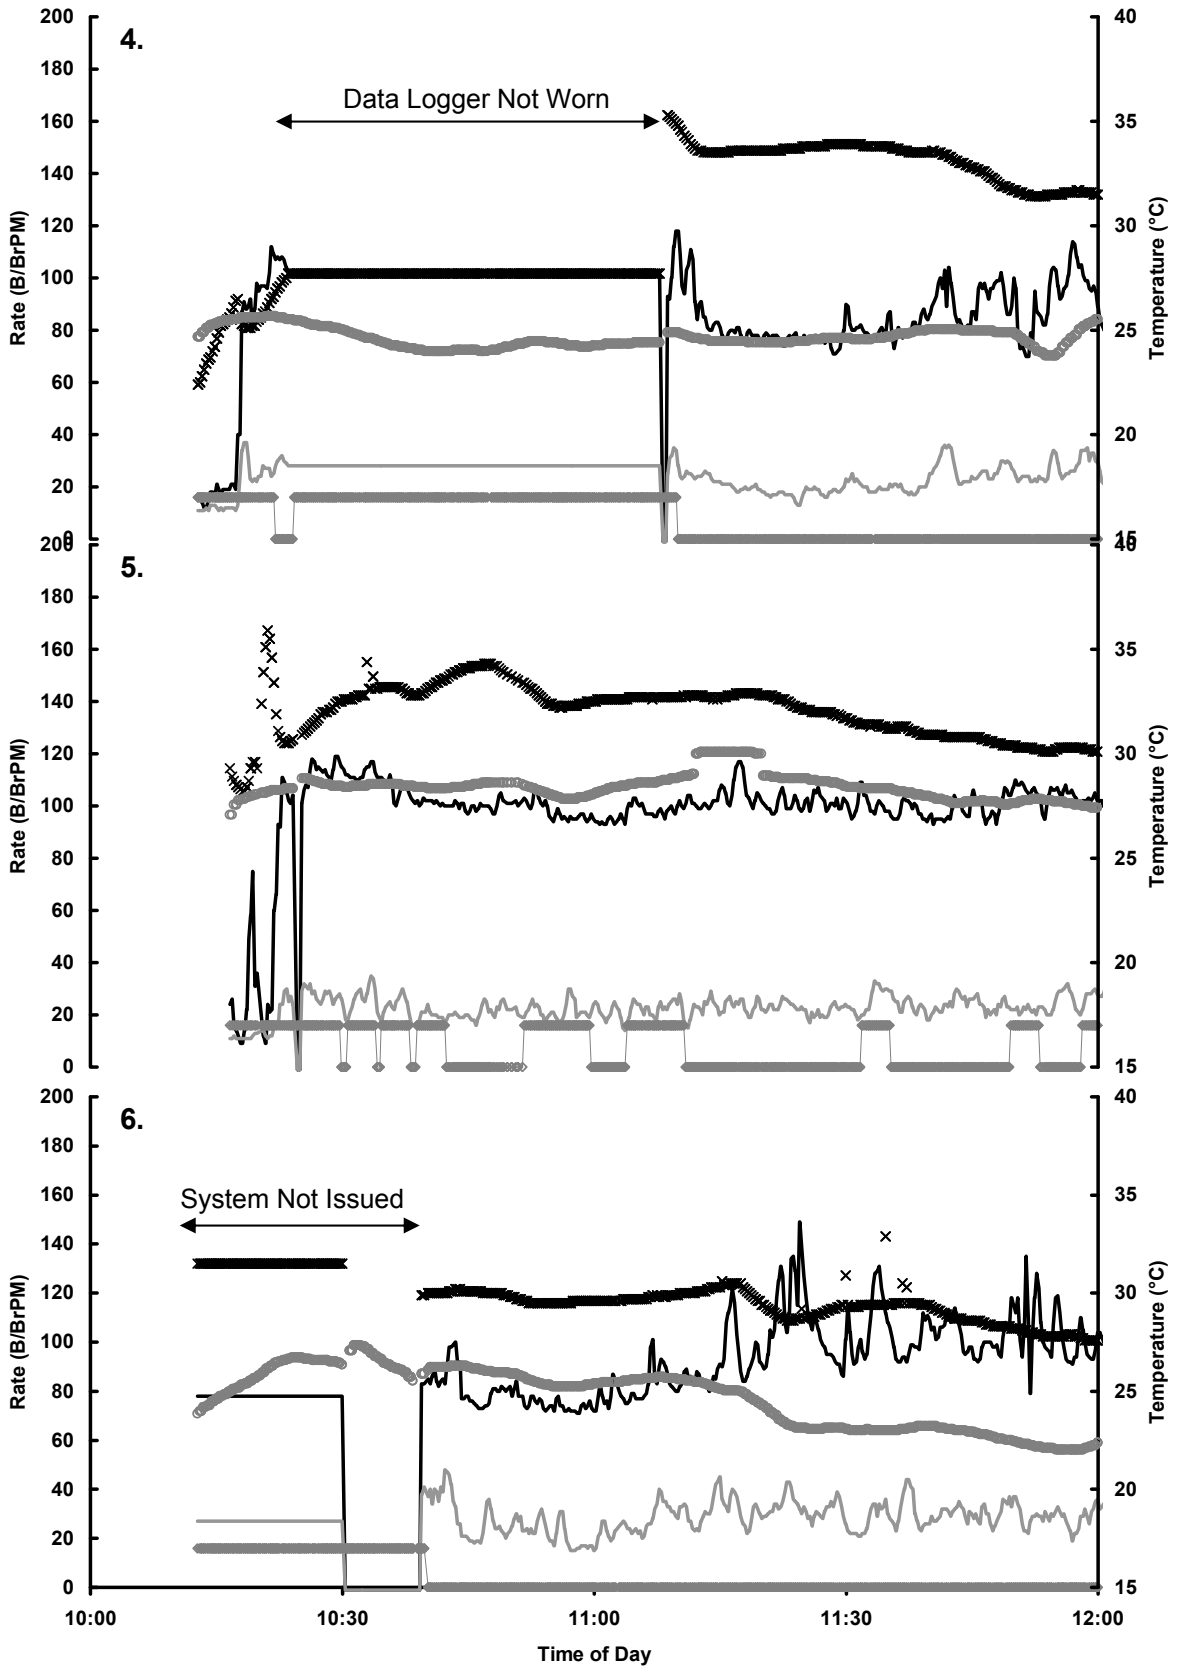

Physiology Day 1- Afternoon, Chase Concrete

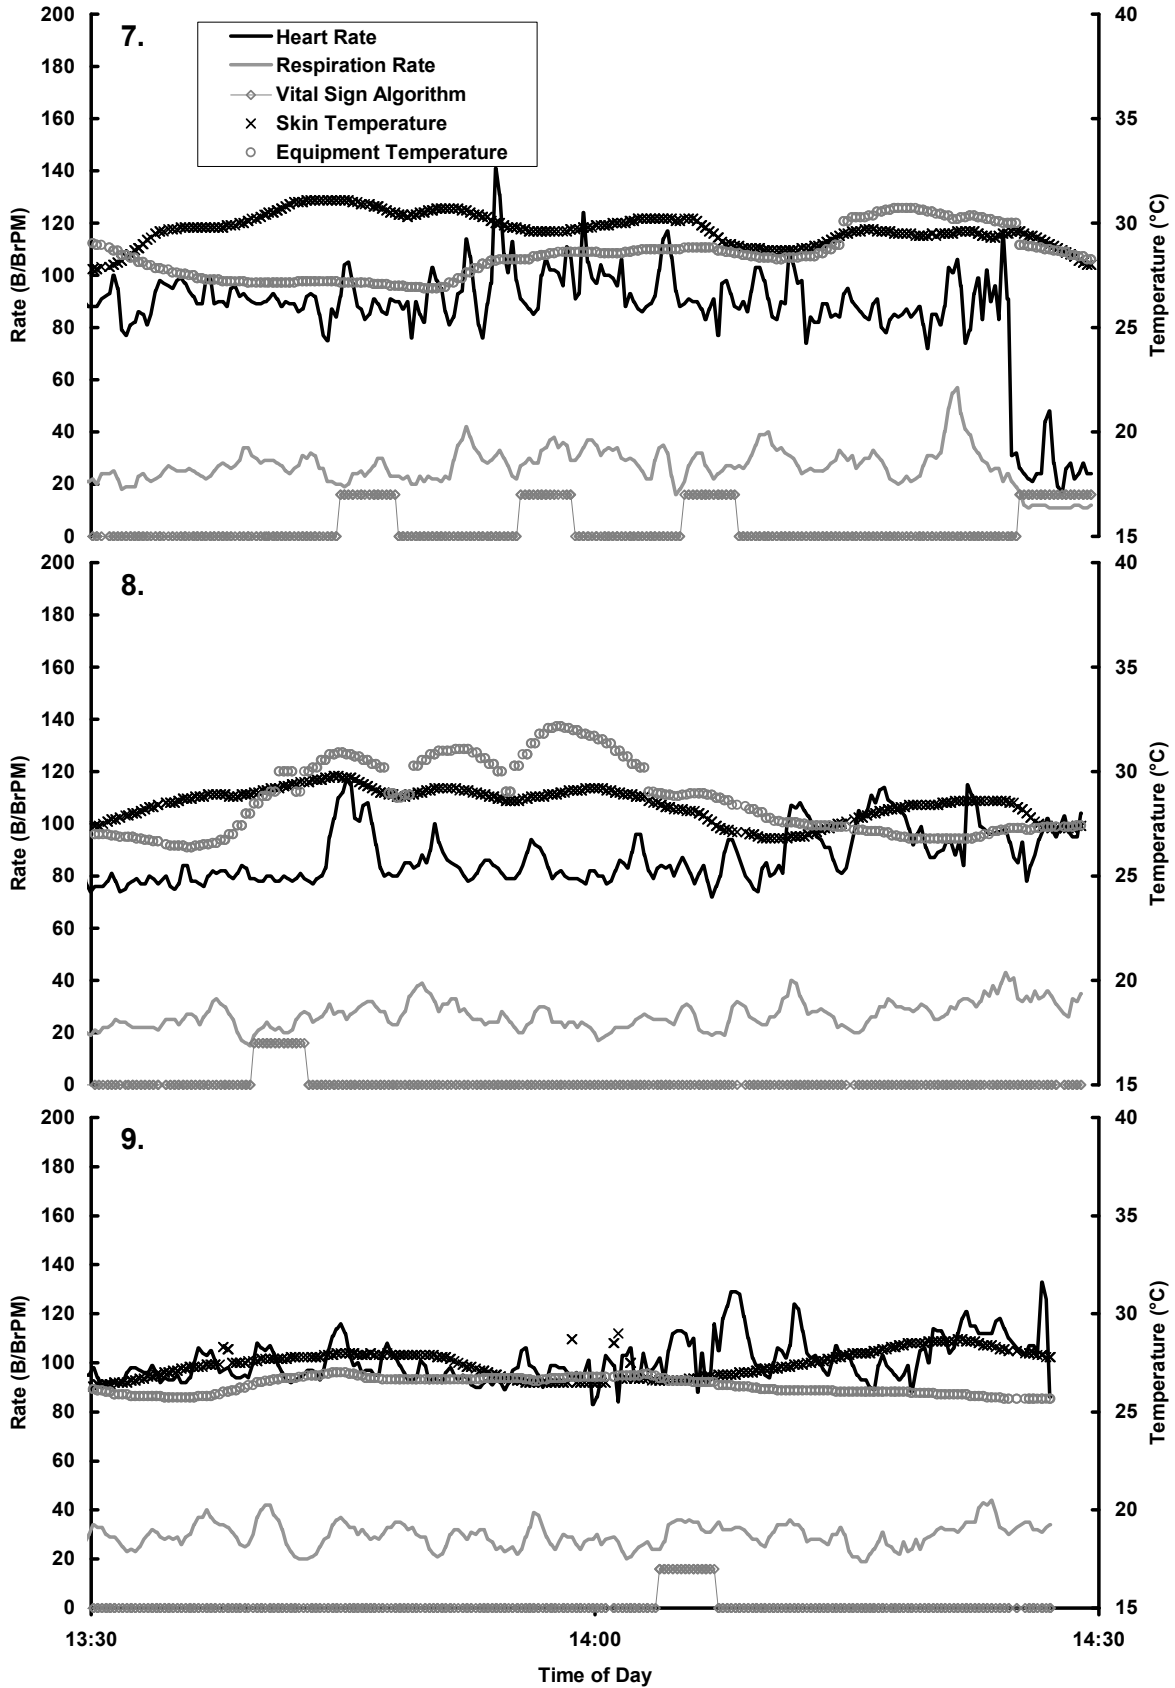

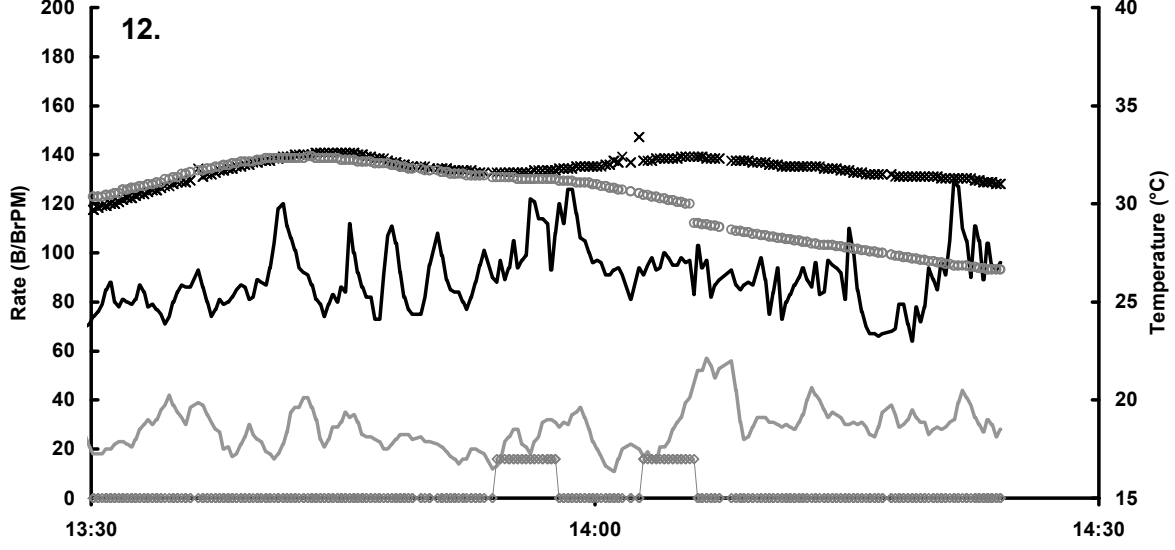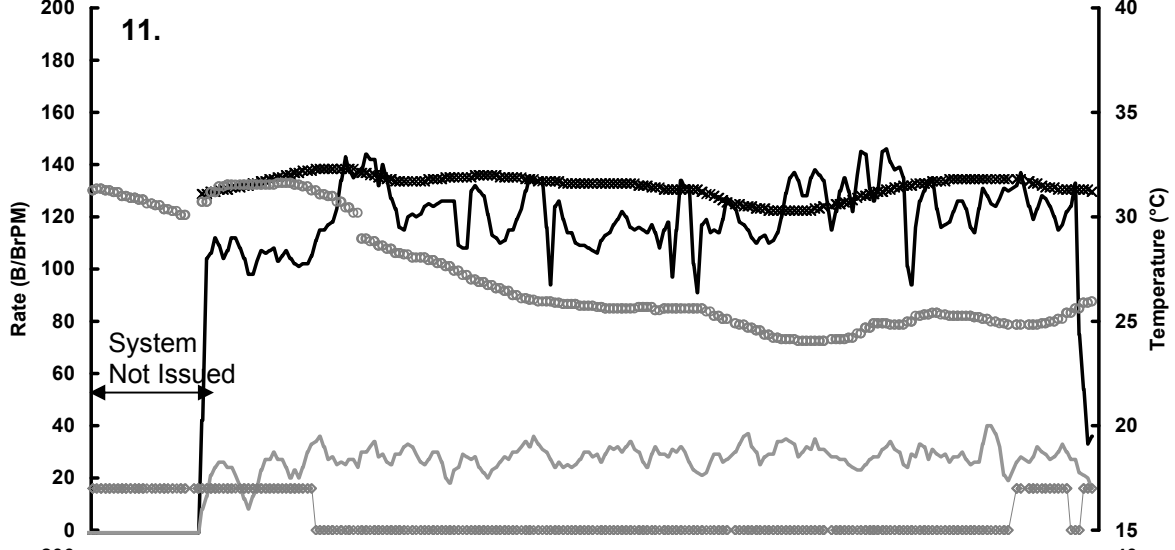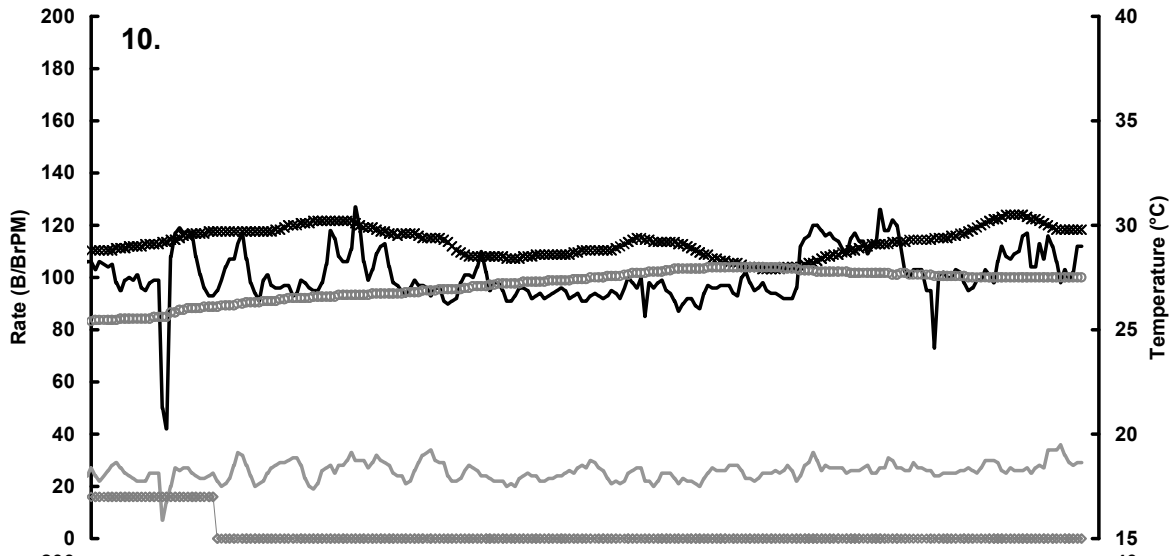

Physiology Day 2, Firefighter Academy

