



EDGEWOOD

CHEMICAL BIOLOGICAL CENTER

U.S. ARMY RESEARCH, DEVELOPMENT AND ENGINEERING COMMAND

ECBC-TR-816

RECOVERY OF VIRUS SAMPLES FROM VARIOUS SURFACES WITH THE INTEGRATED VIRUS DETECTION SYSTEM

Charles H. Wick

RESEARCH AND TECHNOLOGY DIRECTORATE

Patrick E. McCubbin



OptiMetrics, Inc.
Research & Engineering

OPTIMETRICS, INC.
Abingdon, MD 21009

June 2010

20100706064

Approved for public release;
distribution is unlimited.



ABERDEEN PROVING GROUND, MD 21010-5424

Disclaimer

The findings in this report are not to be construed as an official Department of the Army position unless so designated by other authorizing documents.

REPORT DOCUMENTATION PAGE

Form Approved
OMB No. 0704-0188

Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing this collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden to Department of Defense, Washington Headquarters Services, Directorate for Information Operations and Reports (0704-0188), 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to any penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number. PLEASE DO NOT RETURN YOUR FORM TO THE ABOVE ADDRESS.

1. REPORT DATE (DD-MM-YYYY) XX-06-2010		2. REPORT TYPE Final		3. DATES COVERED (From - To) Mar 2008 - May 2008										
4. TITLE AND SUBTITLE Recovery of Virus Samples from Various Surfaces with the Integrated Virus Detection System				5a. CONTRACT NUMBER										
				5b. GRANT NUMBER										
				5c. PROGRAM ELEMENT NUMBER										
6. AUTHOR(S) Wick, Charles H. (ECBC); and McCubbin, Patrick E. (OMI)				5d. PROJECT NUMBER None										
				5e. TASK NUMBER										
				5f. WORK UNIT NUMBER										
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) DIR, ECBC, ATTN: RBCB-DRD-D, APG, MD 21010-5424 OMI, 100 Walter Ward Boulevard., Abingdon, MD 21009				8. PERFORMING ORGANIZATION REPORT NUMBER ECBC-TR-816										
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)				10. SPONSOR/MONITOR'S ACRONYM(S)										
				11. SPONSOR/MONITOR'S REPORT NUMBER(S)										
12. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution is unlimited.														
13. SUPPLEMENTARY NOTES														
14. ABSTRACT Viruses are known to survive in environmental settings over various time periods. This study will show that certain viruses survive for a 24 h period, and certain viruses do not survive, depending on the substrate with which the viruses are in contact.														
15. SUBJECT TERMS <table border="0" style="width: 100%;"> <tr> <td>Virus detection</td> <td>Differential mobility analyzer</td> <td>Condensation particle counter</td> </tr> <tr> <td>Biological agents</td> <td>Electrospray</td> <td>Surface recovery</td> </tr> <tr> <td>Medical research</td> <td>Virus recovery</td> <td></td> </tr> </table>						Virus detection	Differential mobility analyzer	Condensation particle counter	Biological agents	Electrospray	Surface recovery	Medical research	Virus recovery	
Virus detection	Differential mobility analyzer	Condensation particle counter												
Biological agents	Electrospray	Surface recovery												
Medical research	Virus recovery													
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT	18. NUMBER OF PAGES	19a. NAME OF RESPONSIBLE PERSON									
a. REPORT	b. ABSTRACT	c. THIS PAGE			Sandra J. Johnson									
U	U	U	UL	15	19b. TELEPHONE NUMBER (include area code) (410) 436-2914									

Blank

PREFACE

The work described in this report was started in March 2008 and completed in May 2008.

The use of either trade or manufacturers' names in this report does not constitute an official endorsement of any commercial products. This report may not be cited for purposes of advertisement.

This report has been approved for public release. Registered users should request additional copies from the Defense Technical Information Center. Unregistered users should direct such requests to the National Technical Information Service.

Blank

CONTENTS

1.	INTRODUCTION	7
2.	IVDS DESCRIPTION	7
3.	EXPERIMENTAL SETUP.....	7
4.	RESULTS	8
5.	CONCLUSIONS.....	8
	LITERATURE CITED	15

FIGURES

1.	IVDS analyzer.....	9
2.	MS2 Live in LB stock solution.....	9
3.	MS2 plus TBSV stock solution	10
4.	MS2 recovery from stainless steel	10
5.	MS2 recovery from plastic.....	11
6.	MS2 recovery from ceramic	11
7.	MS2 recovery from lacquered wood.....	12
8.	MS2 recovery from glass slide	12
9.	MS2 TBSV recovery from stainless steel.....	13
10.	MS2 TBSV recovery from glass slide	13

TABLE

Virus application to surfaces.....	14
------------------------------------	----

RECOVERY OF VIRUS SAMPLES FROM VARIOUS SURFACES WITH THE INTEGRATED VIRUS DETECTION SYSTEM

1. INTRODUCTION

Viruses are known to survive in environmental settings [1, 2, 3] over various time periods. Certain viruses survive for a 24 h period, and certain viruses do not survive that long, depending on the substrate with which the viruses are in contact. This report will examine the recovery of virus samples from various surfaces. The viruses were placed on several surfaces and allowed to sit overnight. The sample areas were swabbed with a buffer solution and tested after 24 h.

2. IVDS DESCRIPTION

The virus recovery samples were analyzed using the Integrated Virus Detector System (IVDS). The detection stage of the IVDS consists of an electrospray unit to inject samples into the detector, a Differential Mobility Analyzer (DMA) and a Condensate Particle Counter (CPC), shown in Figure 1.

The electrospray unit subjects a conductive liquid to a strong electric field. The field produces a cone that emits a fine jet that then breaks up into small droplets and forms a fine plume. To eliminate the possibility of the breakdown (corona discharge) of the air in the plume, as caused by the high electric field, the spray tip is surrounded by a flow of CO₂, which will prevent corona discharge.

The DMA separates particles by their electrical mobility in air. The sample stream flows through a gap between a rod and a cylinder with an electrical potential between the two. Particle mobility, which is related to size and charge, will either pass particles through the DMA or impinge on the walls. With singly charged particles, which are generated by the electrospray, the mobility becomes a direct measure of the particle size.

In the CPC, the sample particles flow in tandem with a saturated working fluid of butanol. The nanosized particles initiate the condensation of the butanol, and the stream is then cooled. A standard optical counter can then count the butanol-condensed particles, and the results are displayed via the supplied software.

A complete description of the IVDS system, including the detector, can be found in several previous references [4, 5].

3. EXPERIMENTAL SETUP

Several viruses, MS2, a bacteriophage, and tomato bushy stunt virus (TBSV) were pipetted onto several surfaces overnight. The samples dried out in the 24 h time frame and were only visible due to the area being marked prior to samples being placed on the surfaces.

The sample volume for each application was 50 µl of the baseline sample. The baseline samples, an MS2 (sample Live LB, dilute 1:100 20 mM ammonium acetate) and MS2 plus TBSV were analyzed with the IVDS and are shown in Figures 2 and 3. The peak for the MS2 bacteriophage is shown at 24.1 nm, and the peak for TBSV is shown at 32.2 nm. At the end of the 24 h period, 50 µl of a 20 mM ammonium acetate solution was pipetted onto the virus spot and worked with a sterile cotton swab. The swab was placed into a closed tube with 500 µl of the 20 mM ammonium acetate solution, capped, and vortexed for 10-20 s. The sample was then analyzed with the IVDS.

Samples were applied to glass (microscope slide), stainless steel (balance plate), plastic (computer top-smooth), ceramic (stir plate surface at ambient temperature), and lacquered wood (meter stick). All sample areas were cleaned before application. The table shows the sample application.

4. RESULTS

MS2 was recovered and detected, at reduced levels, from the stainless steel (Figure 4), plastic (Figure 5), ceramic (Figure 6), and lacquered wood (Figure 7). The glass applications (Figure 8) were not conclusive for MS2 recovery and detection. The glass analysis with the IVDS had a very small peak at 24 nm, the size of MS2 measured with the IVDS. This peak was not distinguishable from the background and could not be labeled a positive detection. The other samples had distinguishable peaks above background.

TBSV was recovered and detected, at reduced levels, from the stainless steel (Figure 9) and glass sample (Figure 10). The IVDS showed distinguishable peaks above background

5. CONCLUSIONS

The virus samples, MS2 and TBSV, were applied to several surfaces and left at ambient temperature overnight in the laboratory. The samples were collected with cotton swabs and analyzed with the IVDS. The virus samples were recovered from all surfaces except for the MS2 application to the glass slide.



Figure 1. IVDS analyzer

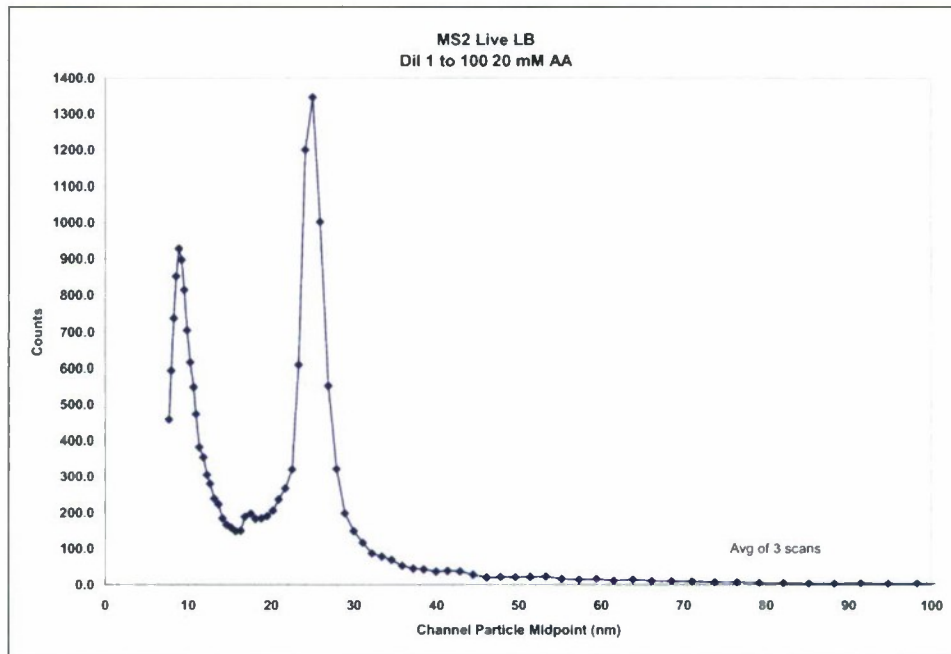


Figure 2. MS2 Live in LB stock solution

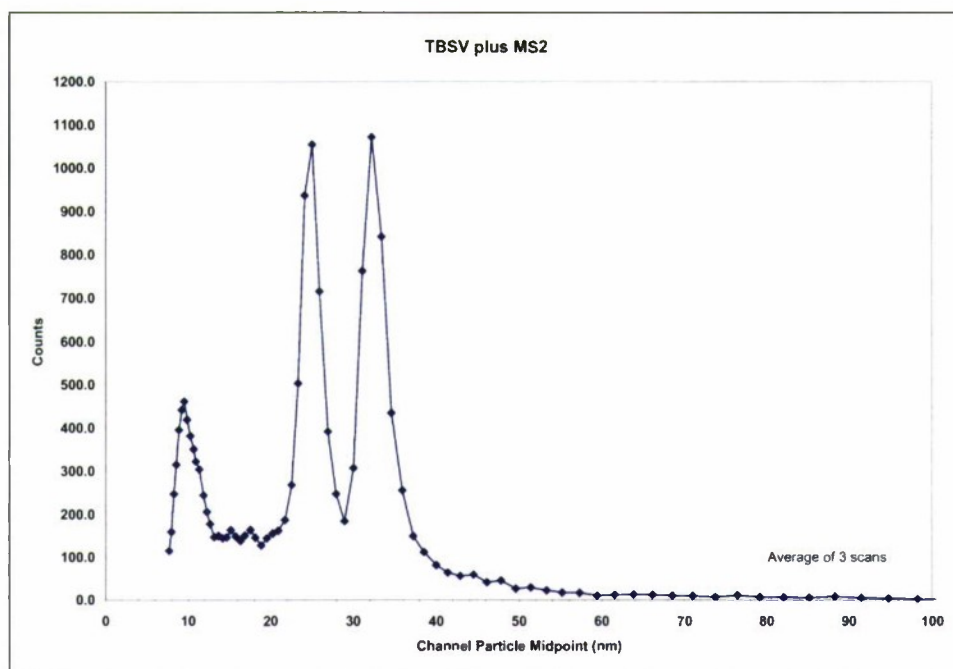


Figure 3. MS2 plus TBSV stock solution

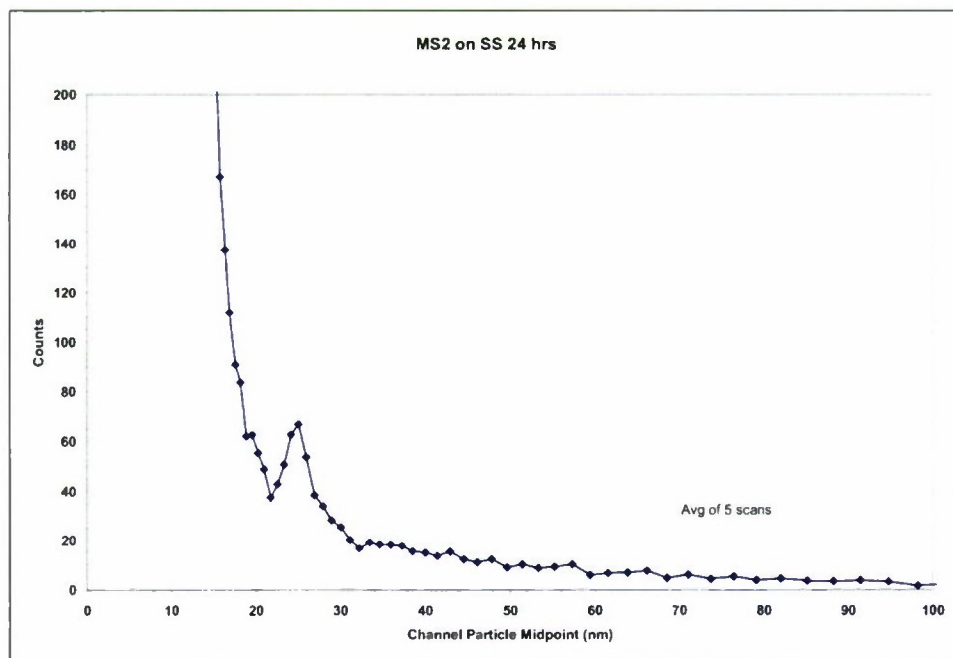


Figure 4. MS2 recovery from stainless steel

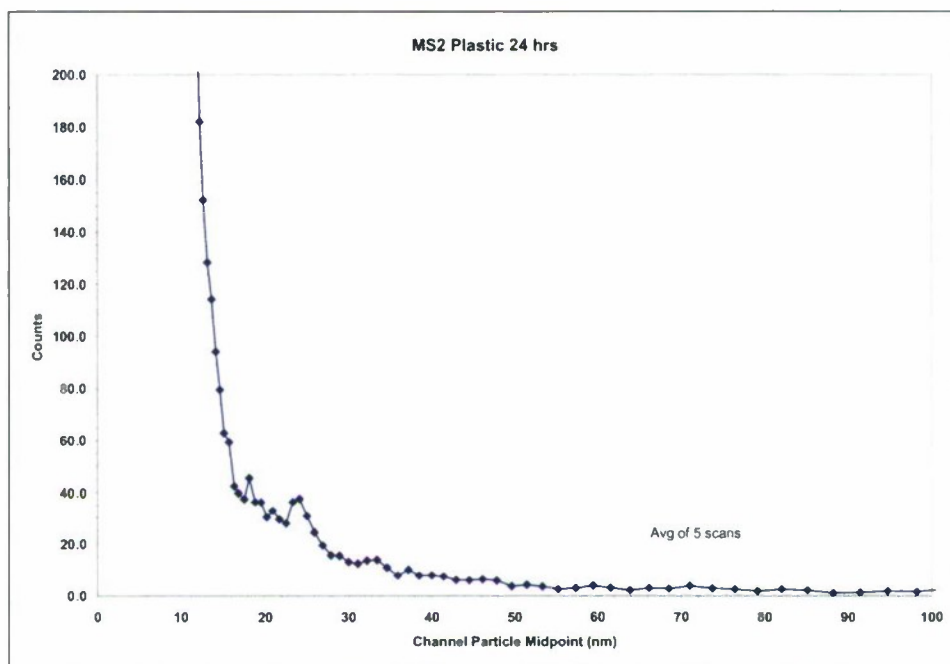


Figure 5. MS2 recovery from plastic

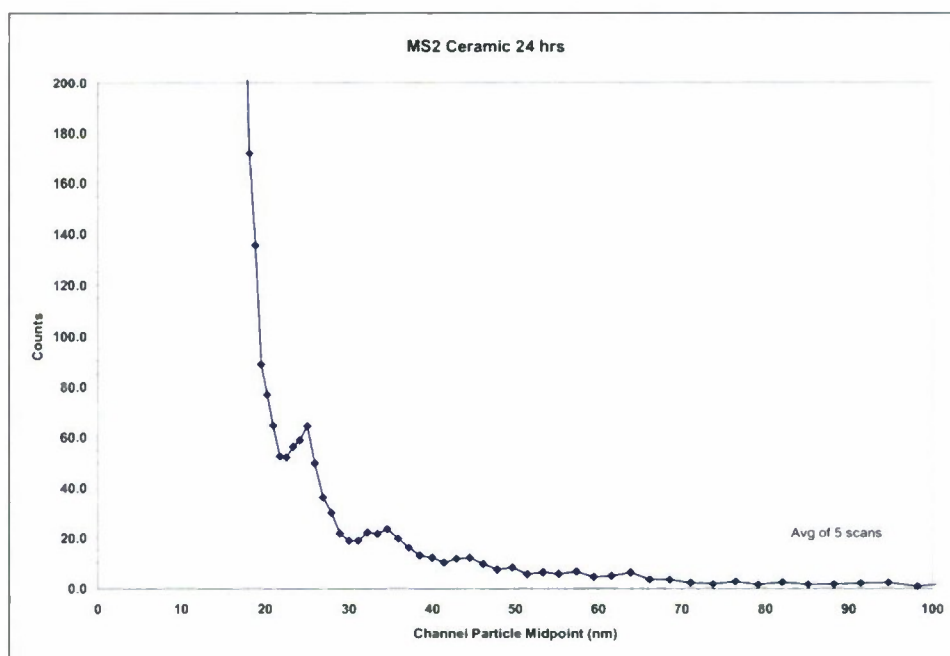


Figure 6. MS2 recovery from ceramic

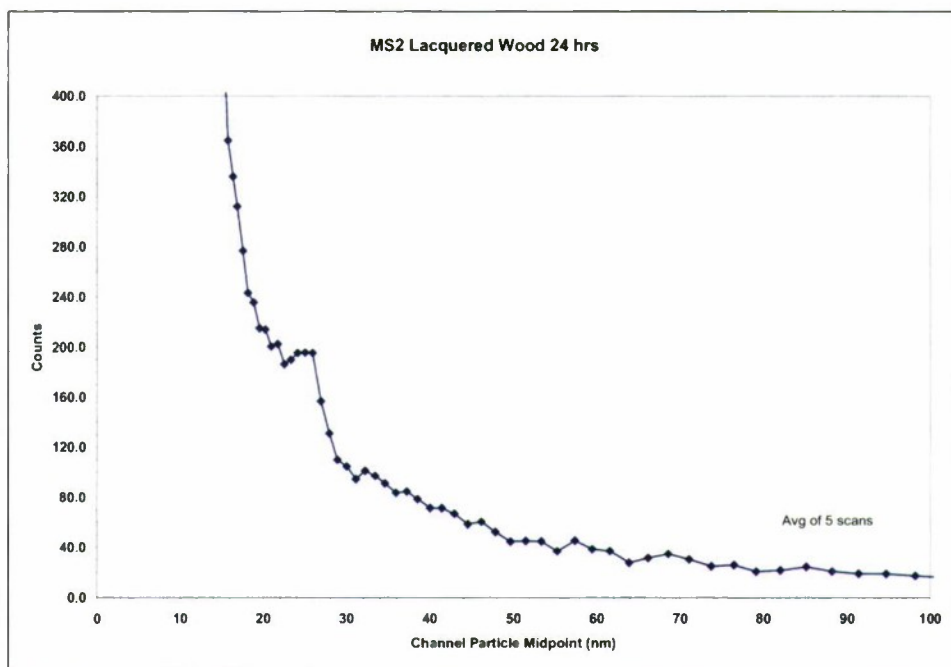


Figure 7. MS2 recovery from lacquered wood

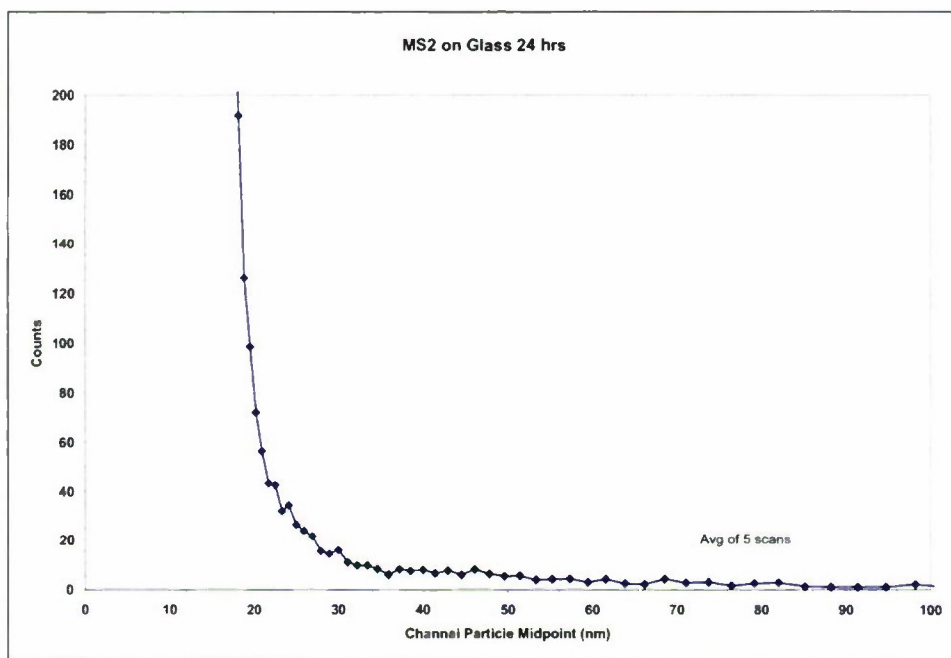


Figure 8. MS2 recovery from glass slide

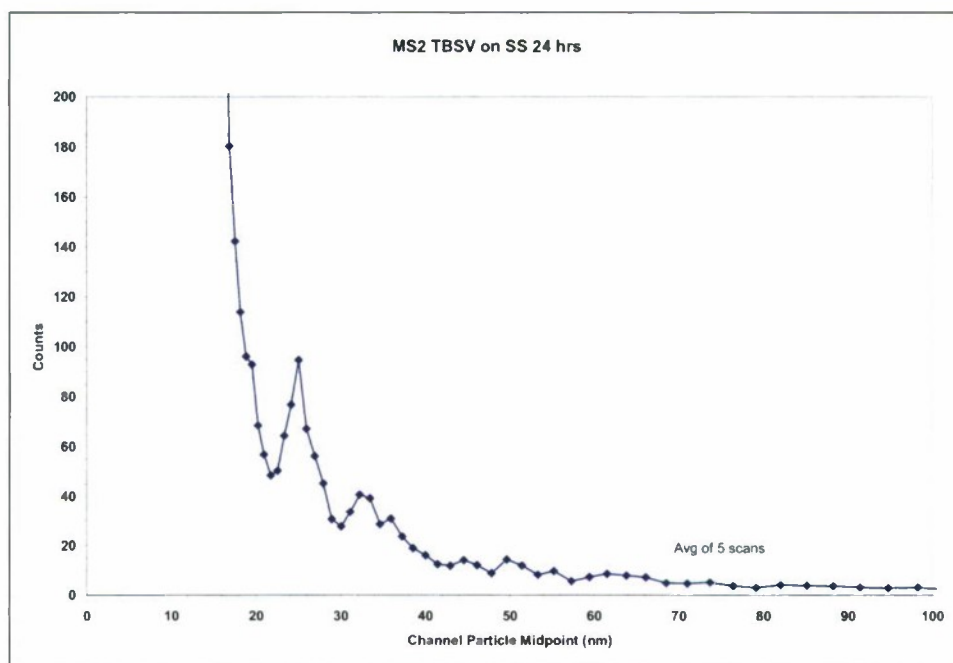


Figure 9. MS2 TBSV recovery from stainless steel

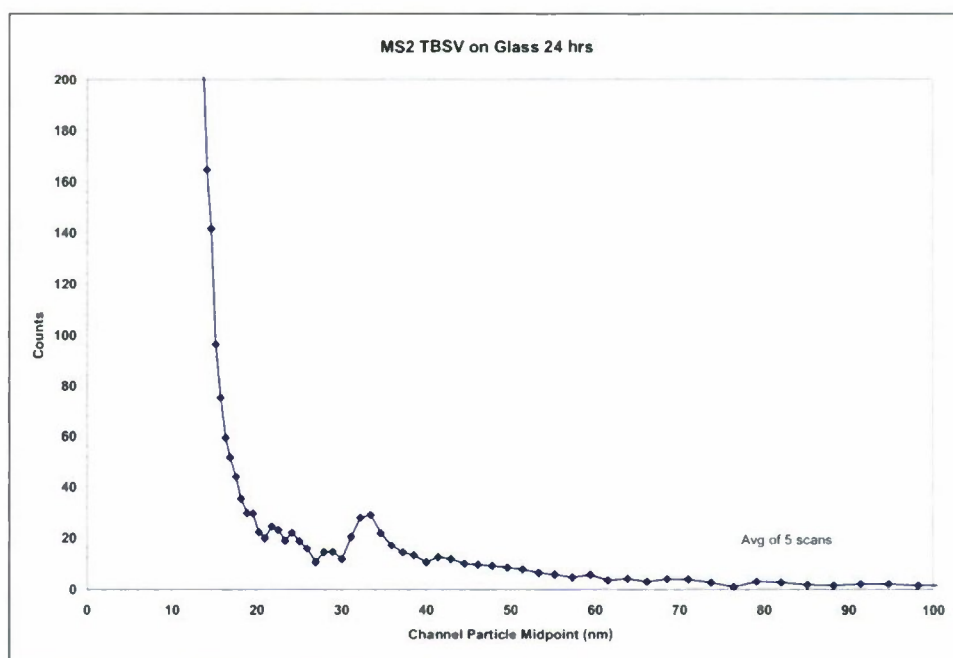


Figure 10. MS2 TBSV recovery from glass slide

Table. Virus application to surfaces

Virus sample	Surface	IVDS detection	
		MS2	TBSV
MS2 (Live in LB)	Glass	Not conclusive	n.a.
MS2 (Live in LB)	Stainless steel	Yes	n.a.
MS2 (Live in LB)	Plastic	Yes	n.a.
MS2 (Live in LB)	Ceramic	Yes	n.a.
MS2 (Live in LB)	Lacquered wood	Yes	n.a.
MS2 plus TBSV	Glass	Not conclusive	Yes
MS2 plus TBSV	Stainless steel	Yes	Yes

LITERATURE CITED

1. Wyn-Jones, A.P.; Sellwood, J. Enteric viruses in the aquatic environment. *J. Appl. Microbiol.* **2001**, *91*, 945-962.
2. Abad, F.X.; Pinto, R.M.; Bosch, A. Survival of Enteric Viruses on Environmental Fomites. *Appl. Environ. Microbiol.* **1994**, 3704-3710.
3. Tellier, R. Review of Aerosol Transmission of Influenza A Virus. *Emerging Infectious Diseases.* **2006**, *12* (11).
4. Wick, C.H.; Anderson, D.M.; McCubbin, P.E. *Characterization of the Integrated Virus Detection System (IVDS) Using MS-2 Bacteriophage*; ECBC-TR-018; U.S. Army Edgewood Chemical Biological Center: Aberdeen Proving Ground, MD, 1999; UNCLASSIFIED Report (AD-A364 117).
5. Wick, C.H.; McCubbin, P.E.; Birenzvice, A. *Detection and Identification of Viruses Using the Integrated Virus Detection System (IVDS)*; ECBC-TR-463; U.S. Army Edgewood Chemical Biological Center: Aberdeen Proving Ground, MD, 2005; UNCLASSIFIED Report (AD-A454 377).