

A D

Award Number: W81XWH-09-2-0069

TITLE: Corneal Protection for Burn Patients

PRINCIPAL INVESTIGATOR: Anthony Johnson MD

CONTRACTING ORGANIZATION:

The Henry M. Jackson Foundation for
the Advancement of Military
Medicine, Inc.

Bethesda MD, 20817

REPORT DATE: July 2013

TYPE OF REPORT: Annual report (revised)

PREPARED FOR: U.S. Army Medical Research and Materiel Command Fort Detrick, Maryland
21702-5012

DISTRIBUTION STATEMENT:

~ Approved for public release; distribution unlimited

The views, opinions and/or findings contained in this report are those of the author(s) and should not be construed as an official Department of the Army position, policy or decision unless so designated by other documentation.

REPORT DOCUMENTATION PAGE				Form Approved OMB No. 0704-0188	
Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing this collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden to Department of Defense, Washington Headquarters Services, Directorate for Information Operations and Reports (0704-0188), 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to any penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number. PLEASE DO NOT RETURN YOUR FORM TO THE ABOVE ADDRESS.					
1. REPORT DATE (DD-MM-YYYY) 1 July 2013		2. REPORT TYPE Annual report (revised)		3. DATES COVERED (From - To) 1 July 2012-30 June 2013	
4. TITLE AND SUBTITLE Corneal protection for burn patients				5a. CONTRACT NUMBER	
				5b. GRANT NUMBER W81XWH-09-2-0069	
				5c. PROGRAM ELEMENT NUMBER	
6. AUTHOR(S) Anthony Johnson and Irene E. Kochevar email: Anthony.johnson2@amedd.army.mil				5d. PROJECT NUMBER	
				5e. TASK NUMBER	
				5f. WORK UNIT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Brooke Army Medical Center Fort Sam Houston, TX 78234				8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING / MONITORING AGENCY NAME(S) AND ADDRESS(ES) US Army Medical Research and Materiel Command Fort Detrick, Maryland 21702				10. SPONSOR/MONITOR'S ACRONYM(S)	
				11. SPONSOR/MONITOR'S REPORT NUMBER(S)	
12. DISTRIBUTION / AVAILABILITY STATEMENT Approved for public release; distribution unlimited					
13. SUPPLEMENTARY NOTES					
14. ABSTRACT The overall goal of this research is to preserve vision of patients recovering from severe facial burns by providing an improved method to reduce development of corneal defects, inflammation, infection and opacification. Scope: To further improve and understand the properties of the degradation-resistant crosslinked amniotic membranes for treating cornea of burn patients that were produced in Years 1 and 2. Major findings: Identified membrane stiffness as a critical parameter for a successful cornea-protective membrane and quantitatively assessed this parameter. Monolayer crosslinked amnions showed low stiffness and excellent enzyme degradation resistance. Tri-layer membranes showed excellent enzyme degradation resistance but their high stiffness made eliminated them from further consideration. Showed that two of the three crosslinking methods to produce stable membranes also decreased the levels of a soluble pro-healing factor. Constructed an amnion-encapsulated hydrogel lens with an improved enzyme resistance to be used to maintain hydration on the cornea surface of patients with peri-orbital scarring that prevents blinking.					
15. SUBJECT TERMS ectropion, cornea, burn scars, amniotic membrane, protein crosslinks, photomedicine, photochemistry					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT	18. NUMBER OF PAGES	19a. NAME OF RESPONSIBLE PERSON
a. REPORT	b. ABSTRACT	c. THIS PAGE			USAMRMC
U	U	U	UU	17	19b. TELEPHONE NUMBER (include area code)

Table of Contents

	Pg
Introduction	4
Body	5
Key Research Accomplishments	16
Reportable Outcomes	17
Conclusion	17
References	--
Appendices	--

INTRODUCTION

The overall goal of this research is to improve the visual outcomes as well as the quality of life for burn patients during the acute and convalescent phases of their rehabilitation. Scarring from second and third degree facial burns, and from subsequent skin grafts, causes the tissues involved to contract and, if significant enough, the patient is left unable to blink or close their eyes. This results in desiccation of the ocular surface, breakdown of the cornea's defense mechanisms and subsequent events that may lead to cornea opacification and the need for cornea transplant. Currently these patients receive frequent application of topical lubricants and anti-inflammatory medications, an imperfect solution that requires very frequent administration of drops which keeps the wounded warrior at the bedside and can slow down other rehabilitation services that are remote to the inpatient ward. Amniotic membrane (AM) transplantation to the ocular surface can assist in the maintenance of the ocular surface of these patients. However, commercially available membrane is not only very expensive, but enzymes on the inflamed ocular surface degrade and destroy the AM very rapidly; this occurs in one day compared to two weeks in non-burn patients. In this project, our major goal is to stabilize the amniotic membrane by crosslinking its constitutive proteins before applying it to the patient's eye. We will determine the crosslinking method that most effectively decreases the rate of enzymatic degradation of AM while preserving the beneficial anti-inflammatory and pro-healing factors in the membrane. In addition, we will evaluate photobonding as a sutureless, glueless alternative to sutures for attaching AM to cornea. We will also test an approach that combines AM with a hydrogel material to increase the ability of the amnion to hydrate the cornea. These studies will employ a rabbit model of eye inflammation.

BODY

This Grant Agreement is a joint proposal with COL Anthony J. Johnson, MD, PI on Grant Agreement W81XWH-09-2-0069. The Statement of Work includes tasks to be carried at the Massachusetts General Hospital (by Professor Kochevar's group) and the US Army Institute for Surgical Research (USISR) (by Dr. Johnson's group). This report covers results from Dr. Kochevar's lab and Dr. Johnson is submitting an separate Year 3 annual report. In this project period, Drs. Kochevar and Johnson discussed results and progress both in person (at the ATACCC meeting, August 2011 and at the annual meeting of the Association for Vision Research and Ophthalmology, April 2012) and during phone calls.

Objectives of the PRMRP were to enhance the translation of results from bench research to military clinical problems and, in turn, to facilitate learning fundamental information from medical applications. In accord with these objectives, we have made further progress in modifying amniotic membrane for protecting burn patients corneas and the results obtained have lead to basic information regarding the processes involved in crosslinking proteins in tissue.

In Year 3, the studies on several sub-aims have been completed. Briefly, our results indicate that of the two approaches to producing a protective membrane from amnion, namely, crosslinked monolayer and crosslinking multilayer, only the monolayer material has the appropriate properties. We identified and quantified the stiffness of the crosslinked material as an additional critical property for a practical and useful protective membrane. In addition, the results demonstrated that a pro-healing factor in amnion, epidermal growth factor (EGF), is lost after treatment with two of the crosslinking agents (carbodiimide and genipin) and might be partially preserved after Rose Bengal photosensitization; this is being examined further in a no-cost extension period. Also, we demonstrated that carbodiimide crosslinking can be used to construct the encapsulated hydrogel contact lens for maintaining cornea hydration.

Specific aim 1.b. Determine whether a multilayer composite of amnion retards the rate of proteolytic degradation in vitro.

Our studies in year 2 had indicated that carbodiimide treatment of tri-layer amniotic membranes increased their resistance to enzymatic degradation, but the material appeared to be too stiff to conform to the curvature of the cornea. Since intimate contact is needed to bond the modified amnion to the cornea, a stiff highly crosslinked tri-layer membrane could not be used to protect the cornea. Thus, our research question became: Can a tri-layer crosslinked amnion membrane be produced that resists enzymatic degradation while remaining sufficiently flexible to ensure good contact with the cornea surface?

To address this question we quantitatively evaluated the stiffness of the crosslinked amnion and compared it to the percent enzymatic degradation of the same membrane.

Amniotic membrane

Amniotic membrane was prepared at the Massachusetts General Hospital as described in the Year 1 annual report and stored at -80 C until use.

Crosslinking with carbodiimide

The results obtained in Year 1 were used to select carbodiimide concentrations to crosslink amnion monolayers by a 1 h treatment followed by rinsing to remove remaining reagents and side products and drying. Carbodiimide concentrations were 0, 5, 9.4 or 10 mM in MES buffer. To produce amnion tri-layers, 3 circular discs of amnion (13 mm diameter) were placed between fine mesh circular brass screens with only the circumference secured. This arrangement allowed the reagents to diffuse into the membranes through the screens while keeping the layers in tight contact. The AM layers were stacked with each stromal surface in contact with

the basement membrane surface of the next AM layer.

Enzymatic degradation

Bacterial collagenase was used to degrade proteins in amniotic membrane. Quantitative analysis of the small peptides released by degradation was accomplished using the fluorescence assay for free amino groups that was developed and described in our Year 1 annual report. The results are presented as the percent enzymatic degradation compared to untreated (non-crosslinked) control samples.

Stiffness measurements

The stiffness of a material (k) can be related to the elastic modulus (Young's modulus), measured as unconstrained uniaxial tension by: $k = (A E) / L$, where A is the cross-sectional area, E is the elastic modulus and L is the length of the element. We measured the elastic modulus of untreated and treated amnion with uniaxial tensiometry, then calculated the stiffness. This stiffness is not the truly the same as the ability of the amnion to bend to the contour of the cornea. However, the more realistic type of stiffness is not readily measureable, and it is not unreasonable to consider the stiffness we measured to correlate with the ability of the amnion to bend and conform to the shape of the cornea.

Uniaxial tensionmetry measurements were made on 5-mm-wide and 15-mm long strips of amnion (crosslink-treated or untreated). Each strip was mounted in the jaws of a Micro EP Miniature testing machine (Admet, Norwood MA) with a 10 N load cell. The initial distance between the jaws was 5 mm. A small drop of buffer was placed on each sample before beginning the measurement to ensure uniform hydration. Amnion strips were initially subjected to uniaxial tension (3 load cycles up to 0.01 N) before loading to failure. The stretch rate was set at 1 mm/min. The axial tension load generated during the test was recorded (in Newtons, N) and the distance between the jaws (mm) was recorded using an MTESTQuattro controller (Admet, Norwood MA).

The stress was calculated by dividing the axial tension by the cross sectional area (thickness x 5 mm width) of each amnion sample. Strain was calculated by dividing the specimen elongation distance by its initial length. The elastic modulus was then calculated from the linear slope region of the stress-strain curve and used to calculate the stiffness (k) from the formula given above.

Amnion thickness measurement (collaboration with Conor Evans PhD and Yookyung Jung PhD) The thickness of each sample must be known in order to calculate the elastic modulus from stress-strain measurements as described above. Amnion varies in thickness between location on the membrane, between individuals and between methods for preparation. Typically, the untreated samples were between 30 and 60 μ m thick. Amnion thickness was measured using optical coherence tomography (OCT) using a home-built ultrahigh resolution spectral domain system coupled to a custom inverted microscopy system. This OCT system utilized a 120 nm bandwidth superluminescent diode source centered at 855 nm to provide an axial resolution of approximately 3 μ m. A pair of galvanometric mirrors coupled to a Zeiss microscope using a .15NA Zeiss 5X objective was used to scan across the amion samples to collect xyz volumes. These volumes were then processed using a custom Matlab script that extracted amnion thickness measurements across entire 1.5 x 1.5 mm amnion samples.

Relationship between enzymatic degradation and amnion stiffness

Monolayer membranes-- Degradation of the membranes with collagenase was carried out in triplicate and the results are shown in Table 1, column 3 and Figure 1. Consistent with our previous results, increasing the concentration of carbodiimide decreased the extent of enzymatic

degradation. Almost complete protection (95%) was produced by treatment with 10 mM carbodiimide.

Table 1 Carbodiimide crosslinking of amnion monolayers: Effect on enzymatic degradation and membrane stiffness.

Treatment	n	% enzymatic degradation SD	Thickness, pm SD	Stiffness, N/mm SD			
Control, MES buffer	11	100	5	42.2	11.5	0.342	0.156
5 mM carbodiimide	6	71	4 *	26.8	3.2 *	0.884	0.284*
9.4 mM carbodiimide	13	18	3 *	25.2	3.7 *	0.821	0.306*
10 mM carbodiimide	13	5	3 *	20.2	7.7 *	0.856	0.487*

* indicates $p < 0.01$ compared to control.

The thickness of hydrated amnion monolayers, carbodiimide-treated or untreated, was measured (Table 1, column 4) and used to calculate the elastic modulus. The mean amnion thickness of the control amnion was 42.2 pm. All of the carbodiimide-treatments decreased the amnion thickness compared to the control group ($p < 0.01$) by 48-60%. There was no significant differences between the thicknesses of the carbodiimide-treated amnions although there is a trend to decreased thickness with higher carbodiimide concentrations. The decrease in membrane thickness can be attributed to intra-fiber protein-protein crosslinks that decrease the distance between collagen molecules. Inter-fiber crosslinks are not likely to form because the distance between collagen fibers in the amnion is too great to be bridged by the carbodiimide crosslinking which directly connects amino acids. Interestingly, even the lowest carbodiimide concentration decreased the amnion thickness substantially, indicating that the even a low amount of crosslinking can decrease the distance between collagen molecules. Further crosslinking within the fibers decreases the enzymatic degradation but did not produce significant further decrease in amnion thickness.

Treatment with carbodiimide substantially increased the stiffness of amnion monolayers. As shown in Table 1, column 5 and Figure 1, all three carbodiimide treatments increased the mean value for stiffness from 0.342 N/mm (untreated control) by —40%. The stiffness values did not differ significantly between carbodiimide-treatments, but they all differed significantly from the control group ($p < 0.01$). Our previous studies (Year 2 report) indicated that amnion treated with similar concentrations of carbodiimide effectively bonded to cornea indicating that amnion with stiffness of —0.8 N/mm are flexible enough to serve as protective membranes for corneas of ectropion patients.

Enzymatic degradation and stiffness show different patterns of response to treatment with increasing carbodiimide concentration; this is most clearly seen in Figure 1. The stiffness reaches a plateau starting at the lowest carbodiimide concentration (5 mM). Thus, the higher concentrations of carbodiimide that lead to nearly complete protection of the amnion from degradation do not further increase the amnion stiffness. This is good news since it means that we can vary the degree of protection against enzymatic degradation without being concerned that the monolayer membrane will be too stiff to bond to the cornea.

We then tested the tri-layer amnion that had been treated with 8 mM carbodiimide for 1 h (n = 8), conditions which had been shown in our previously reported study to decrease enzymatic degradation to 3% of the control value. Tensiometry was carried out as described above and the thickness of the tri-layer membrane measured with a digital caliper. The stiffness was 1.44 ± 0.51 N/mm. This value is substantially higher than the stiffness of the monolayer amnion (Table 1). Since the tri-layer membrane was too stiff to conform to the shape of the cornea and prevented the membrane from being photobonded to the cornea (Year 2 result), this result suggests that our stiffness measurements correlate with the ability of crosslinked to be bonded to the cornea. This correlation will be further evaluated in the no-cost extension period by directly comparing the stiffness values to the strength of photobonding of the crosslinked membranes to cornea as measured in Year 2.

An important additional outcome of this study will be that we will have a physical measurement to quantitatively assess the stiffness of membranes produced after various crosslinking treatments. This will allow us to assess whether a modified membrane is sufficiently flexible, i.e., non-stiff, to conform to the shape of the cornea, thus reducing the amount of ex vivo or in vivo testing on rabbit eyes.

Summary/ Conclusions

The stiffness of crosslinked membranes was measured as a critical property for success of cornea protective membrane. Monolayer crosslinked amnion remained sufficiently flexible to allow production of highly stable crosslinked membranes that can be used for cornea protection. For tri-layer crosslinked amnion, high stiffness was associated with membranes that showed low enzymatic degradation, indicating that the tri-layer construct is not suitable for this application.

Specific aim 1.e.i. Identify the protein crosslinking method that causes the least reduction in anti-inflammatory and healing factors in amnion.

The ideal modified amniotic membrane for protection of ectropion eyes would contain the protein factor believed to contribute to the pro-healing and anti-inflammatory properties of amnion. In Year 2, we assessed the effect of amnion crosslinking techniques on the levels of TGF- β 1, a proposed pro-healing factor in amnion. Our results showed that the crosslinking treatment conditions that produce degradation-resistant amnion also caused almost complete loss of TGF- β 1. Because TGF- β 1 is stored in tissue linked to LTBP (latent TGF- binding protein) and closely associated with extracellular matrix proteins, we postulated that it became crosslinked to LTBP and/or the extracellular matrix proteins. Thus, TGF- β 1 in crosslinked amnion would not be available for the healing process and could not be measured in our ELISA assay.

We had proposed to test the effect of amnion crosslinking treatments on a pro-healing protein that, in contrast to TGF- β 1, is not stored in close association with extracellular matrix proteins in tissue. Epidermal growth factor (EGF) was selected as a representative of this group of proteins. This study was carried out using carbodiimide and Rose Bengal photosensitization as the crosslinking treatments. As will be shown below, these treatments were not satisfactory and, consequently, we also evaluated another protein crosslinking agent, genipin, that links proteins together by a mechanism that differs from carbodiimide and RB photosensitization.

Effect on EGF level of crosslinking amnion monolayers with carbodiimide or Rose Bengal photosensitization

The methodology for extracting soluble proteins from amnion developed in Year 2 was followed. Briefly, weighed amnion samples (treated or untreated) were homogenized at liquid nitrogen temperature, PBS and protease inhibitor were added and the mixture centrifuged. The supernatant was concentrated and the protein level measured. EGF was measured by ELISA using a commercial kit (R&D Systems, # DY236) according to the manufacturers directions.

Weighed samples of amnion (~25 mg) were treated with carbodiimide (0, 4, 6, 8 mM) for 1 h in MES buffer or treated with 0.1% Rose Bengal in PBS for 5 min, then exposed to 0, 5 or 50 J/cm² 532 nm light from a cw KTP laser, as reported previously. A weighed portion (—1 mg) was used to measure the collagenase degradation as described above and the remainder was used for EGF measurement.

Crosslinking by treating with increasing concentrations of carbodiimide decreased both the percent enzymatic degradation and the EGF content of the amnion (Table 2, column 3 and Figure 2). The EGF content decreased more rapidly than the percent degradation as seen clearly in Figure 2. For example, treatment with 6 mM carbodiimide reduced EGF to — 12% of the MES buffer control whereas the enzymatic degradation was only reduced to —30%. Samples showing —90% protection against enzymatic degradation (treatment with 8 mM carbodiimide) retained only —5% of the EGF originally present (an undesired outcome). These results are similar to those reported in Year 2 for the effect of carbodiimide crosslinking on TGF-

1 in amnion. Thus, carbodiimide crosslinking has the advantages of greatly decreasing the enzymatic degradation of amnion and producing a membrane that is not too stiff to conform to the contour of the cornea surface but appears to reduce the pro-healing activity of the amnion.

Crosslinking amnion by Rose Bengal photosensitization treatment also appeared to decrease the EGF level (Table 2) although this result is difficult to interpret firmly. In this experiment, Rose Bengal (RB) in PBS (no irradiation) decreased the apparent level of EGF by a factor of —2.5 compared to a PBS control suggesting that RB interfered with the ELISA measurements. Irradiation with green light appeared to decrease further the EGF level, although some EGF remained, suggesting that RB photosensitization may be a useful crosslinking method. The enzymatic degradation measurements also seemed to be confounded by the presence of RB. We will remove the RB remaining after crosslinking treatments (or control PBS) from the samples by dialysis before ELISA and enzymatic degradation measurements to remove this interference. These studies will be carried out the no-cost extension period that has been approved for this award.

Treatment	% enzymatic degradation SD	EGF, pg/mg amnion SD				
Carbodiimide treatment						
Control, PBS	100	7		1.82	0.04	
Control, MES buffer	77.5	19.8		1.83	0.06	
4 mM	44.3	17.8	*	0.41 9	0.08 9	*
6 mM	30.8	19.7	*	0.22 5	0.10 4	*
8 mM	10.9	2.2	*	0.11 7	0.17 5	*
Rose Bengal + 532 nm treatment						
RB only	50.9	7.4		0.70 8	0.36 5	
RB + 5 J/cm ²	34.4	23.0		0.31 7	0.33 5	
RB + 50 J/cm ²	57.7	16.8		0.18 0	0.09 4	

Crosslinking proteins in amnion with genipin

Since carbodiimide (and possibly RB photosensitization) decreased pro-healing factors in amnion we tested whether an alternative protein crosslinking agent, genipin, might not alter the EGF level. First, the effect of genipin crosslinking on degradation of amnion by bacterial collagenase was evaluated. As shown in Table 3, column 3, increasing the time of incubation of amnion with 0.1% genipin (in PBS) decreased its susceptibility to enzymatic degradation, reaching 14% after 20 h incubation, a level that would be acceptable for a material to protect cornea of ectropion eyes.

Table 3 Genipin crosslinking of amnion monolayers: Comparison of effect on enzymatic degradation and membrane stiffness.

Treatment	n	% enzymatic degradation SD	Thickness, μ m SD	Stiffness SD				
Control, buffer only	11	100	4	42.2	11.5	0.342	0.158	
Genipin, 7 h	11	75	8 *	32.9	6.9 *	0.921	0.331	*
Genipin, 18 h	11	27	2 *	26.3	3.6 *	0.778	0.391	*
Genipin, 20 h	5	14	3 *	25.2	2.2 *	0.632	0.156	*

* indicates $p < 0.01$ compared to control.

Initial, qualitative observations suggested that the genipin-crosslinked membranes appeared to be less stiff than those produced by carbodiimide treatment. Consequently, we measured the stiffness of the genipin-treated membranes using tensiometry and OCT as described above. However, the stiffness produced by genipin crosslinking was similar to the results obtained with carbodiimide. The range of values for stiffness (0.63–0.92 N/mm) for genipin crosslinking was similar to that obtained for carbodiimide (~0.84 N/mm). The relationship between degradation by collagenase and stiffness (Figure 3) was also similar to that found for carbodiimide crosslinking (Figure 1). Increasing the treatment time with genipin increased the protection against enzymatic degradation, i.e., less degradation, but did not increase the stiffness. These results indicate that highly stable crosslinked amnion monolayers can be produced with genipin crosslinking that are not too stiff to be photobonded to cornea and thus may be an alternative to carbodiimide for producing membranes for cornea protection in ectropion eyes.

Genipin and carbodiimide appeared to produce crosslinked membranes with approximately equivalent beneficial properties. Since carbodiimide treatment drastically reduced the EGF level, it would be of great interest if genipin did not have the same effect. In a pilot study, treatment with 0.1% genipin for 20 h did not significantly reduce the level of EGF ($p > 0.05$). A full study was then carried out in which amnion was treated for varying times with 0.1% genipin in PBS. As shown in Table 4 and Figure 4, the decrease in EGF paralleled the decrease in percent degradation. Thus, genipin crosslinking of amnion did not show any advantage over crosslinking with carbodiimide with regard to loss of EGF; the desired result, namely, decreased enzymatic degradation while preserving EGF or other pro-healing proteins, was not produced under any of the treatment conditions evaluated.

Table 4 Effect of genipin crosslinking of amnion monolayers on EGF content and degradation by collagenase.

Treatment,	% enzymatic degradation SD	EGF, pg/mg amnion SD		
Control, buffer only	100	5	7.62	1.16
Genipin, 5 h	64.1	8.9	4.67	0.74
Genipin, 10 h	24.7	2.3	0.66	0.16
Genipin, 15 h	10.6	0.9	0.30	0.16
Genipin, 20 h	9.23	1.44	0.30	0.07

Genipin, treatment time, hr

Figure 4 Effect of crosslinking monolayer amnion with genipin on EGF and enzymatic degradation. Amnion was incubated for varying times with 0.1% genipin. * indicates $p < 0.01$ compared to MES buffer control

Summary/ Conclusions

Both crosslinking treatments, carbodiimide and genipin, substantially reduced the level of EGF, a pro-healing factor in amnion, using conditions that produced an enzyme degradation resistant membrane that could be used for protecting cornea of ectropion eyes. This result suggests that we may not be able to achieve a goal of this project, namely, producing a protective membrane that retains the pro-healing factors in amnion. The results obtained with Rose Bengal (RB) photosensitized crosslinking may be promising since only partial loss of EGF was found but the results were confounded by residual RB in the membrane. Further studies in a no-cost extension period will be carried out to further evaluate the effect of RB photosensitized crosslinking on EGF in amnion.

Specific aim 1.e.ii. Identify the layering method that causes the least reduction in anti-inflammatory and healing factors in amnion.

Tri-layer amniotic membranes offer the possibility that the pro-healing factors in the inner membrane might not be affected by the crosslinking and thus available to aid the cornea. In a pilot study, direct comparison of EGF remaining in monolayer and tri-layer amnion, both crosslinked by 7.5 mM carbodiimide, showed that >40% EGF remained in the tri-layer membrane whereas only 4% remained in the monolayer.

In a more detailed study, tri-layer membranes were prepared as described above under Specific Aim 1.b using concentrations of carbodiimide of 3, 5, 7.5 and 20 mM in MES buffer and a 1 h incubation time. The percent degradation by bacterial collagenase was measured and the soluble protein was extracted as described under Specific Aim 1.e.i above and used for measurement of EGF by ELISA. The results in Table 5 and Figure 5 show that, as expected based on the results reported in Year 2, these treatments protected the membrane from enzymatic degradation. The amount of EGF extracted also decreased with increasing

carbodiimide treatment time. However, treating with concentration of 5 mM and higher carbodiimide produced membranes that were relatively higher levels of EGF in the tri-layer membranes compared to the monolayer membranes (see Figure 2). Possibly, the EGF in the middle layer of the tri-layer amnion was protected. Although this may be an interesting and useful observation, the stiffness of the tri-layer (as described earlier), does not allow it to be considered further as a protective membrane for ectropion eyes.

Table 5/ Figure 5. Effect on EGF of carbodiimide crosslinking tri-layer amnion membranes.

Cabodiimide treatment,	% enzymatic de gradation SD	EGF, pg/mg amnion SD		
0, MES buffer only	100	2 3	6.81	0.41
3 mM	100	4 5	4.6 0	0.17 *
5 mM	63	6 *	4.3 3	0.67 *
7.5 mM	28	1 0 *	3.86	1.37 *
20 mM	1	3 *	0.72	0.88 *

* indicates p < 0.01 compared to control value.

Carbodiimide, mM

Summary/ Conclusions

Tri-layer amnion crosslinked by carbodiimide treatment showed better retention of EGF than similarly crosslinked monolayer membranes. However, the high stiffness of these enzyme-resistant crosslinked tri-layers precludes their use for cornea protection.


Specific aim 1.f.i. Evaluate the healing properties of crosslinked amnion on the rabbit ectropion model.

To evaluate the healing properties of crosslinkd amnion membrane on the rabbit we conducted 3 experiments, The three experiments were designed to mimic a 28 day experience of a person with ocular surface burns that caused cicitricial ectropon. In all three experiments the rabbits after quarantine were subjected to 1.5cm upper and lower lid blepharoplasties. The lids received antibiotic ointment for one week and then they were returned to the operating room. At the end of the first week, amniotic membrane was sutured to the anterior surface of the rabbits anterior segment. In group one (untreated amniotic membrane was affixed to the surface of the eye. In group two carbodiiamidide cross linked amniotic membrane was sutured to the rabbits ocular surface. In group three, rose bengal cross linked amniotic membrane will be sutured to the ocular surface. The rabbits were examined daily. Over the next 28 days the amniotic membrane on the ocular surface was repaired, replaced or patched as necessary to protect the ocular surface for the 28 day period. Every 3 days tear samples were collected. Due to the inability to get consistent veterinary support we were required to evaluated the tear samples in weekly batches. The tear film analysis involves MMP-9 evaluation and a multiplex

evaluation of 14 different cytokines.

To date the surgical procedures and tear collection of 2 of the three arms have been completed. Due to a two month delay in our study due to the fact the SAMMC terminated our funding, as they could not find the paperwork for our extension, we have started the tear film analysis for the first two arms.

To date there is only very preliminary results.

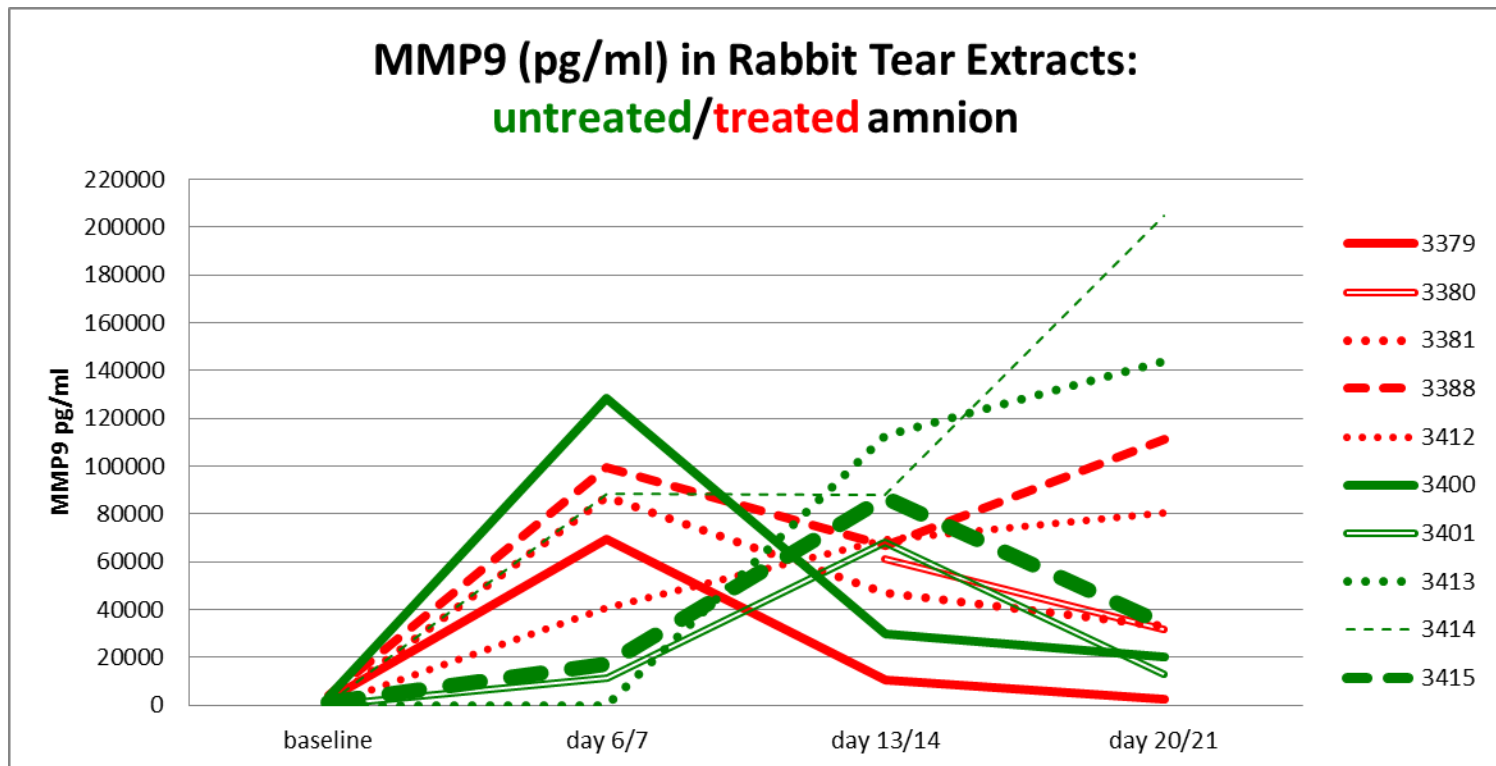

	baseline	day 6/7	day 13/14	day 20/21	treated aminion
3379	2796.75	69230.06	10505.65	2768.6	
3380	1931.1		61448.66	31872.77	
3381	865.77	86982.44	46883.18	33124.33	
3388	3907.29	99368.15	66969.2	111156.25	
3412	272.32	40656.4	69483.48	80369.20	
3400	3612.8	128515.03	30041.18	20268.75	untreated amnion
3401	---	11360.42	68037.5	12765.18	
3413	---	---	112781.25	143808.48	
3414	611.01	88697.47	88171.13	204937.50	
3415	1353.57	17068.01	86702.83	33924.26	

The graft shows that the MMP9 levels increase steadily the first week at which point the amniotic membrane is secured to the the MMP-9 levels drop. We are still evaluating the tear samples utilizing the multiplex consisting of 14 cytokines and MMP-9 levels. Additionally we will soon be starting the third arm of the study.

Specific aim 1.f.ii. Evaluate multilayered amnion construct on the rabbit ectropion model.

The results obtained during Year 2 indicated that tri-layer, but not bi-layer, crosslinked amniotic membranes were more resistant to degradation by bacterial collagenase than monolayer crosslinked amnion receiving the same treatment. However, our results in Year 3 indicate that stable, enzyme-resistant tri-layer membranes, crosslinked with carbodiimide, are too stiff to conform to the contour of the cornea. This factor lead us to conclude that tri-layer amniotic membranes are not a feasible material to use to protect cornea of ectropion eyes. Consequently, they will not be evaluated in the rabbit ectropion model created by Dr. Johnson.

Specific aim 3.a. Construct amnion-covered hydrogel bandage.

In order to provide moisture and prevent tear evaporation from the cornea of ectropion eyes, we had proposed to seal a hydrogel contact lens within an amnion capsule by a crosslinking process and then bond this construct to the cornea using our light-activated crosslinking process. In Year 2 we fabricated amnion-encapsulated hydrogel lenses by photo-crosslinking technique Rose Bengal-stained amnion. We also carried out feasibility studies to test bonding of these constructs to cornea ex vivo. The results reported in Year 2 suggested that this approach was feasible. However, our previously reported results on RB photosensitization and additional recent studies indicate that this crosslinking technique decreased enzymatic degradation by a maximum of ~50%. Since degradation of the amnion during use of the encapsulated lens would shorten its useful lifetime, we tested an alternative method for encapsulating a hydrophilic contact lens in amnion.

Our alternative approach involved using carbodiimide to crosslink the two amnion layers of the capsule since this agent can protect the membrane against enzymatic degradation by >90%. This process bonded the two layers together around the circumference as well as making the amnions resistant to proteolytic degradation. The amnion-contact lens-amnion sandwich was placed between two copper fine mesh screens that were shaped to approximate the contour of the cornea anterior surface. The screens allowed the crosslinking reagents to diffuse into the amnion, as shown previously when the tri-layer amnion constructs were made (Specific Aim 1.b).

The amnion discs were 13 mm diameter and the lens (1 DAY ACUVUE - TRUEye) was cut to 6 mm diameter. Approximately 3 mm at the circumference of the two amnion layers was held in tight contact to facilitate crosslinking between the two layers. In the “sandwich”, the basement membrane surface of one amnion disc was in contact with the stromal surface of the other. The construct was placed in 10 mM carbodiimide/MES buffer and incubated with shaking for 1 h.

To test if this construct could be bonded to cornea ex vivo, we used the method reported in Year 2. Briefly, the material to be tested is stained with 0.1% Rose Bengal for 1 min and placed over the de-epithelialized cornea surface of an ex vivo rabbit eye containing a V-shaped incision. After irradiation

with 532 nm light, the strength of the bond between the construct and the cornea was measured by infusing saline into anterior chamber and measuring the intraocular pressure (IOP) that causes leakage under the construct.

For the carbodiimide crosslinked encapsulated lenses, 200 J/cm² of 532 nm radiation was applied at an irradiance of 0.25 W/cm². The bonding strength was good: IOP = 54.7 ± 28.0 mm Hg (n = 6), after learning to adjust for good fit.

Summary/ Conclusions

Carbodiimide crosslinking can be used to produce amnion-covered hydrophilic contact lenses that can then be bonded to the cornea. This approach has the advantage, over of RB photosensitization, of producing a more enzyme-resistant covering.

Specific aim 3.b. Evaluate bonding amnion-encapsulated hydrating bandage on the rabbit.

We will be supplying Dr. Johnson with amnion-encapsulated contact lenses for evaluation on his rabbit model for ectropion during the no-cost extension period.

KEY RESEARCH ACCOMPLISHMENTS

Identified the stiffness of crosslinked amnion membranes as a physical property critical for development of a cornea protective membrane that conforms to the shape of the cornea and quantitatively evaluated this property. Monolayer crosslinked amnion had sufficiently low stiffness to allow production of highly stable crosslinked membranes that can be used for cornea protection. The stiffness of tri-layer crosslinked amnion that was resistant to enzymatic degradation was too great for this application.

Determined that two of the three crosslinking treatments that stabilize amnion against enzymatic degradation also substantially decrease the level of a soluble protein pro-healing protein, epidermal growth factor (EGF). Crosslinking with carbodiimide and genipin decreased EGF by >90%. Crosslinking with RB photosensitization requires further evaluation.

Determined that tri-layer crosslinked amnion partially retained the EGF in the amnion but was unsuitable as a protective membrane because of its high stiffness. A protease-resistant amnion-covered hydrogel contact lens for providing hydration to the cornea was constructed using carbodiimide crosslinking and demonstrated to photobond to ex vivo cornea. This approach is an alternative to the Rose Bengal photosensitization previously demonstrated and provides the construct with a more enzyme-resistant membrane.

REPORTABLE OUTCOMES: None during this reporting period.

CONCLUSION:

In year 3, we have progressed toward our goal of developing materials to protect the eyes of patients with severe periorbital burns and scarring. These patients cannot blink normally or close their eyes (a condition called ectropion), leading to damage to the ocular surface and possibly the need for corneal transplant. Our approaches are to stabilize and modify amniotic membrane, a beneficial material for cornea surface treatment that cannot be used now because it rapidly degrades in these inflamed eyes, and to develop a hydrating contact lens that can be bonded to the cornea surface.

We have used protein crosslinking to produce amniotic membrane that is resistant to degradation by enzymes in the tears of inflamed eyes. In Years 1 and 2 we had identified two effective protein crosslinking techniques and in Year 3 we identified a third approach. We found that, in addition to providing a membrane that is stable against enzymatic degradation, the membrane must remain flexible enough to conform to the shape of the cornea. During this period we established a method for testing the stiffness of the crosslinked membrane. This testing allows evaluation of crosslinking treatment conditions without requiring ex vivo or in vivo testing. Crosslinked membranes that were resistant to enzymatic degradation were produced that had low stiffness and can be used for further in vivo evaluation. Tri-layer crosslinked amniotic membrane constructs, however, which showed excellent degradation resistance were too stiff to be used on corneas and will not be further considered. Another criteria for a successful cornea protecting membrane is that it retain the pro-healing factors present in amnion. We showed that two of the three protein crosslinking methods decreased substantially these factors in amnion; the third method is being further evaluated. We had previously developed an amnion-encapsulated contact lens designed to provide hydration to the cornea. We have now established an additional approach that provides a more enzyme-resistant crosslinked amnion covering that should extend the period that this lens provides hydration to the cornea and thus inhibit damage to the surface for patients who are unable to supply tears by blinking. These crosslinked amnion-based materials and hydrogel constructs are now ready to be tested on the rabbit model for ectropion developed by the partner Dr. Johnson. The first two arms of our study have been completed. We will be starting the rose bengal cross linked arm of the study the second week of April (when our order of rabbits will clear quarantine after being ordered 14 March 2014).