

Splitting of the Proximal Femur With a New Femoral Nail

MAJ Joseph R. Hsu, MD,* CPT Daniel J. Stinner, MD*
COL David A. Brown, MD† and The Skeletal Trauma Research Consortium (STReC)

Summary: We present a case of a 19-year-old woman with a closed diaphyseal femur fracture and who had fixation of the fracture using a newer lateral entry nail, which resulted in an intraoperative proximal femur fracture. The patient underwent revision the following day and subsequently returned to regular activity without signs of implant failure or loss of reduction at latest follow-up. Caution should be exercised with the use of new implants that require a change in customary technique. In addition, some concern must be raised by the amount of offset from the top of this particular nail to its long axis.

Key Words: lateral entry, trochanteric nail, intramedullary nailing, femur, complication

(*J Orthop Trauma* 2010;24:e40–e43)

INTRODUCTION

Antegrade femoral nailing using a trochanteric starting point has increased in popularity over the past few years.^{1–5} One comparative study showed a trend toward shorter operative times and significantly decreased fluoroscopy times with a trochanteric starting point compared with a piriformis entry portal.⁴ Both of these time differences were significant for obese patients. In addition, there seems to be some preliminary data to support a clinical advantage to nail insertion through the trochanter.¹

Anatomically, the center of the femoral canal is below the junction of the medial aspect of the trochanter and the superior–lateral aspect of the base of the femoral neck.⁶ To access the canal from a more lateral start point without introducing increased strain or malalignment in the proximal femur,⁷ most modern nailing systems include a proximal lateral bend (valgus) of 4–6 degrees. This places the entry point at the tip of the trochanter. Some authors have criticized this starting point due the potential for gluteus medius tendon

injury,⁸ whereas other authors have found greater soft-tissue injury by inserting a nail through the piriformis fossa.^{2,3}

In an effort to eliminate soft-tissue injury when inserting an antegrade femoral nail, a recent nail, the Titanium Cannulated Lateral Entry Femoral Nail (Synthes USA, Paoli, PA) moved the entry point further lateral (10 degrees) and distal to completely avoid the gluteus medius tendon insertion. Furthermore, this nail has a helical shape in an effort to decrease bone stress and reduce the likelihood of iatrogenic intraoperative fracture.⁹ The nail must be inserted with rotation to allow proper seating in the canal. The following is a case report of an intraoperative fracture using the new nail design.

CASE

A 19-year-old woman involved in a head-on motor vehicle collision sustained a closed right diaphyseal femur fracture. The patient had a contralateral closed medial tibial plateau fracture. She had no other injuries and no relevant medical or surgical history. The patient was taking no medicines. Work-up of the patient's femur fracture included plain radiography of the femur (Fig. 1) and a thin-cut computed tomography scan of the proximal femur with 2-dimensional reconstructions (Fig. 2). The work-up confirmed a diaphyseal femur fracture without a concomitant fracture of the proximal femur. The patient was 65 in tall (167.64 cm) and weighed 109.8 lb (49.8 kg).

The patient went to the operating room approximately 5 hours after arrival and underwent supine antegrade nailing of her right femur fracture. The device used was a 10 mm × 40-cm Titanium Cannulated Lateral Entry Femoral Nail (Synthes USA). The entry point angle and location were performed as described in the technique manual for the product. This start point is 10 degrees lateral to the intramedullary canal measured from a point 40 mm distal to the lesser trochanter or 12 mm lateral to the tip of the trochanter.⁹ The provided opening reamer was used under fluoroscopic control. The entire length of the femoral canal was sequentially reamed in increments of 0.5 mm to a diameter of 11.5 mm. A nail of 10 mm diameter was placed. The nail was introduced with the insertion handle in an anterior position to facilitate the proximal turn from the start point into the canal. The nail was allowed to rotate into proper orientation because it was advanced with gentle mallet blows as described in the product manual. Once rotation was confirmed radiographically, proximal and distal interlocking was performed.

Intraoperative fluoroscopy demonstrated a good reduction of the fracture and appropriate implant placement. There was no apparent iatrogenic proximal fracture. Plain

Accepted for publication March 12, 2009.

From the *United States Army Institute of Surgical Research, Fort Sam Houston, TX; and †Orthopedic Service, Brooke Army Medical Center, Fort Sam Houston, TX.

The authors did not receive grants or outside funding in support of their research or preparation of this article.

The opinions or assertions contained are the private views of the authors and are not to be construed as official or as reflecting the views of the Department of the Army or the Department of Defense.

Reprints: CPT Daniel J. Stinner, MD, Orthopedic Research Fellow, United States Army Institute of Surgical Research, 3400 Rawley E. Chambers Avenue, Fort Sam Houston, TX 78234 (e-mail: daniel.stinner@amedd.army.mil).

Copyright © 2010 by Lippincott Williams & Wilkins

Report Documentation Page				Form Approved OMB No. 0704-0188	
Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.					
1. REPORT DATE 04 APR 2010		2. REPORT TYPE N/A		3. DATES COVERED -	
4. TITLE AND SUBTITLE Splitting of the proximal femur with a new femoral nail				5a. CONTRACT NUMBER	
				5b. GRANT NUMBER	
				5c. PROGRAM ELEMENT NUMBER	
6. AUTHOR(S) Hsu J. R., Stinner D. J., Brown D. A.,				5d. PROJECT NUMBER	
				5e. TASK NUMBER	
				5f. WORK UNIT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) United States Army Institute of Surgical Research, JBSA Fort Sam Houston, TX 78234				8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)				10. SPONSOR/MONITOR'S ACRONYM(S)	
				11. SPONSOR/MONITOR'S REPORT NUMBER(S)	
12. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release, distribution unlimited					
13. SUPPLEMENTARY NOTES					
14. ABSTRACT We present a case of a 19-year-old woman with a closed diaphyseal femur fracture and who had fixation of the fracture using a newer lateral entry nail, which resulted in an intraoperative proximal femur fracture. The patient underwent revision the following day and subsequently returned to regular activity without signs of implant failure or loss of reduction at latest follow-up. Caution should be exercised with the use of new implants that require a change in customary technique. In addition, some concern must be raised by the amount of offset from the top of this particular nail to its long axis.					
15. SUBJECT TERMS					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT UU	18. NUMBER OF PAGES 4	19a. NAME OF RESPONSIBLE PERSON
a. REPORT unclassified	b. ABSTRACT unclassified	c. THIS PAGE unclassified			

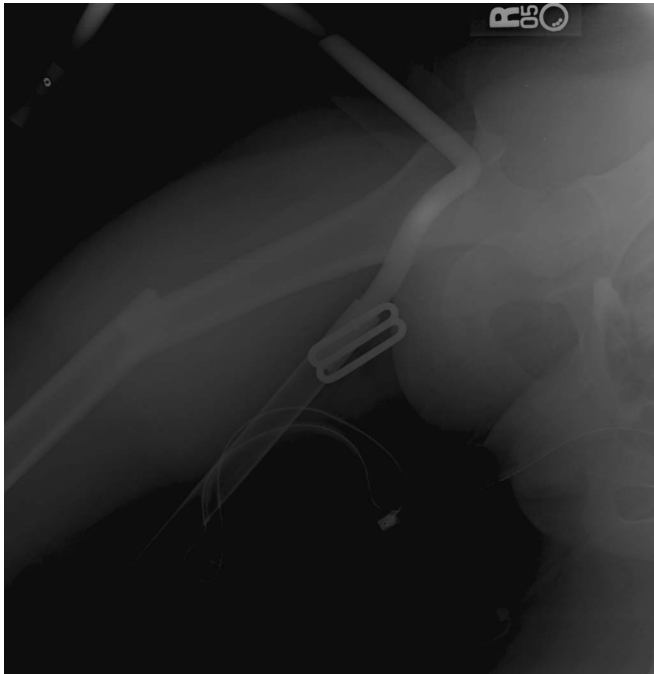


FIGURE 1. A radiograph of the right diaphyseal femur fracture obtained in the trauma bay.

radiographs of the hip taken in the postanesthesia care unit clearly demonstrated an oblique fracture of the proximal femur starting from a lateral point below the vastus ridge to a medial point 1 cm below the lesser trochanter. It did not appear to involve the entry portal (Fig. 3).

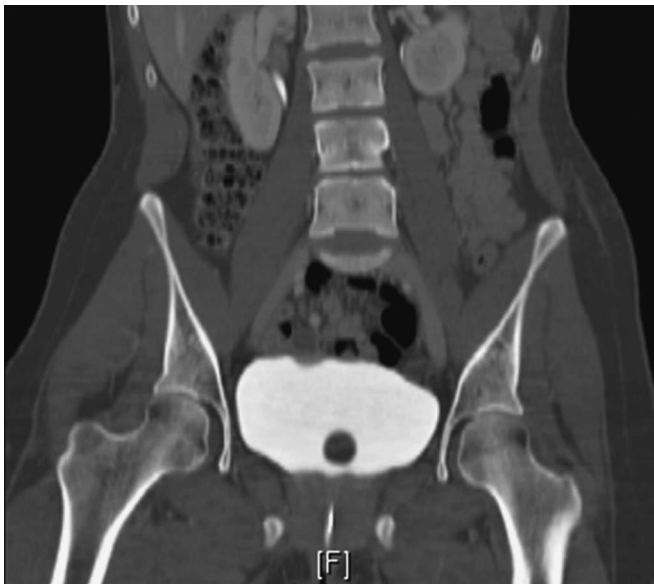


FIGURE 2. A thin-cut computed tomography scan of the proximal femur confirms no preoperative proximal femur fracture.

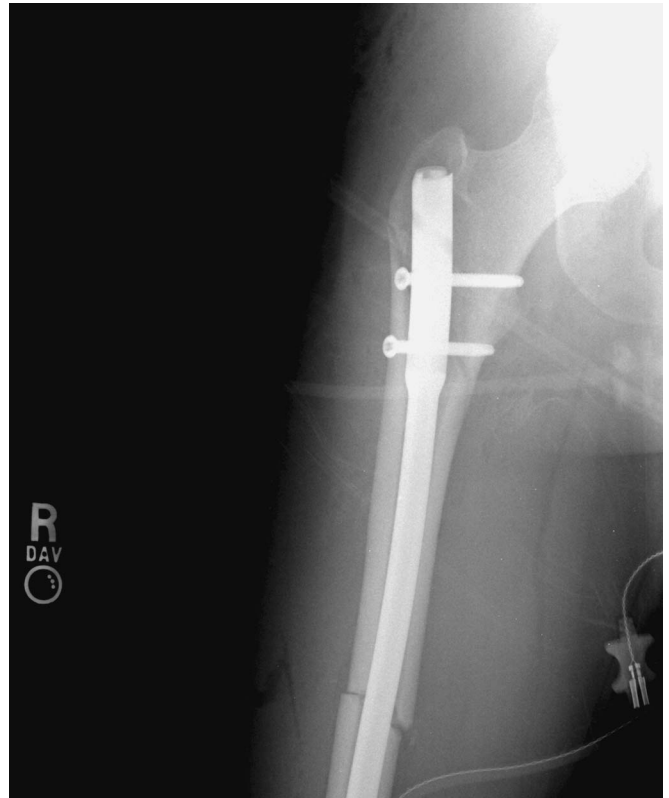


FIGURE 3. Postoperative radiograph of the hip demonstrates an oblique fracture of the proximal femur, which does not appear to involve the starting hole.

The patient and her family were told of the complication immediately after it was identified. Due to the patient having a tibial plateau fracture on the contralateral lower extremity, the decision was made to revise the fixation after discussion with the patient and her family to allow for immediate weight-bearing on her right lower extremity. The patient returned to the operating room the following day for implant removal and revision to a cephalomedullary nail (Fig. 4). The patient subsequently healed her wounds without signs of infection. At latest follow-up (9 months), the patient is full weight-bearing and has returned to regular activity without signs of implant failure or loss of reduction.

DISCUSSION

Using the greater trochanter as an entry point for nailing femur fractures is not a new concept. It was first advocated by Gerhard Küntscher.^{10,11} However, the use of a trochanteric start point with the early straight nails resulted in a mismatch between the contour of the femur and shape of the nail. This mismatch created a bending moment, which resulted in splitting and further comminution of the bone.¹² As use of these stiffer closed section implants evolved, nailing through the piriformis fossa gained popularity.^{12,13} As mentioned, use of the trochanter as a starting point has regained popularity for both practical reasons^{4,14} and to decrease soft-tissue injury^{2,3} for potential improved clinical differences.¹



FIGURE 4. A radiograph showing revision to a cephalomedullary nail.

There is a learning curve associated with using the trochanter as a starting point.^{15,16} One study claimed that the learning curve can be overcome with each surgeon in the group averaging 6.4 cases during the learning curve.¹⁶ The primary surgeon (D.B.) in this report is well beyond this learning curve for a standard trochanteric starting point at the tip of the trochanter.

The design of the Lateral Entry Femoral Nail (Synthes USA) includes a greater lateral proximal (valgus) bend of 10 degrees. This is similar to the proximal bend in the original Gamma Nail, which was subsequently revised to a 4-degree bend. Other common nails in the US market advocated for trochanteric entry are within 4–6 degrees^{4,5,7} to limit their offset to the femoral medullary canal.

The increased bend of the lateral entry femoral nail (LEFN) is to avoid damage to the gluteus medius tendon that occurs with utilizing the tip of the trochanter as a starting point.^{2,3,8} This “fissuring” of the proximal femur that occurred in our case has been reported in Gamma Nail cases in the past due to the exaggerated bend.¹⁶ The LEFN has since been revised because of the excessive bend, which resulted in the fracture documented in our case. Due to the helical nail shape of these newer implants, however, iatrogenic splitting of the proximal femur may still be a problem if, during the rotational insertion of the nail, the bend mismatch causes a stress fracture of the shaft while seating the implant.⁹

It is very possible that the critical factor in this case may have been the size of the patient. She is slightly above average height for American women (63.8 in), but well below the average weight (163 lb.).¹⁷ We would expect, however, that nail design be developed to accommodate a variety of sizes and shapes of femurs, as Asian and Hispanic females often exhibit these smaller and variable shaped femurs. Another critical factor may have been the learning curve associated with this specific device as in addition to a more lateral starting point, it requires a more vertical angle aiming at a point 40 mm below the lesser trochanter. The technique of precision entry and trajectory control using similar implants (4- to 5-degree valgus bends), aiming down the center of the medullary canal distal to the lesser trochanter, has been described.¹⁸ However, many surgeons with trochanteric nailing experience are accustomed to aiming toward the lesser trochanter. Finally, the device used in this case was one of the early 10-mm nails, so it did not have the helical design. Perhaps, the lack of “rifling” contributed to increased proximal stresses. Irrespective of this fact, the excessive lateral bend in this nail created a wedge effect that resulted in a stress fracture when finally seated.

CONCLUSIONS

Caution should be exercised with the use of any new implant requiring a change in customary technique. This case report is an example of the learning curve associated with a new device, and concern must be raised by the amount of offset from the top of this specific nail to its long axis. We would recommend that when using a trochanteric entry portal, consideration should be given to inserting nails that have a lateral offset of no more than 4–5 degrees to minimize proximal stress concentration and iatrogenic fractures of the proximal femur.

REFERENCES

1. Bankston LS, Stannard JP, Futch LA, et al. Functional outcomes following IM nailing of femur: comparison of piriformis vs trochanteric nailing. Presented at: American Academy of Orthopaedic Surgeons Annual Meeting; February 15, 2007; San Diego, CA.
2. Dora C, Leunig M, Beck M, et al. Entry point soft tissue damage in antegrade femoral nailing: a cadaver study. *J Orthop Trauma*. 2001;15:488–493.
3. Moein CM, Verhofstad MH, Bleys RL, et al. Soft tissue injury related to choice of entry point in antegrade femoral nailing: piriform fossa or greater trochanter tip. *Injury*. 2005;36:1337–1342.
4. Ricci WM, Schwappach J, Tucker M, et al. Trochanteric versus piriformis entry portal for the treatment of femoral shaft fractures. *J Orthop Trauma*. 2006;20:663–667.
5. Ricci WM, Devinney S, Haidukewych G, et al. Trochanteric nail insertion for the treatment of femoral shaft fractures. *J Orthop Trauma*. 2005;19:511–517.
6. Gausepohl T, Pennig D, Koebke J, et al. Antegrade femoral nailing: an anatomical determination of the correct entry point. *Injury*. 2002;33:701–705.
7. Ostrum RF, Marcantonio A, Marburger R. A critical analysis of the eccentric starting point for trochanteric intramedullary femoral nailing. *J Orthop Trauma*. 2005;19:681–686.
8. McConnell T, Tornetta P III, Benson E, et al. Gluteus medius tendon injury during reaming for gamma nail insertion. *Clin Orthop Relat Res*. 2003;407:199–202.
9. Ehmke LW, Polzin BM, Madey SM, et al. Femoral nailing through the trochanter: the reamer pathway indicates a helical nail shape. *J Orthop Trauma*. 2006;20:668–674.

10. Gerhard Küntscher. *The Marrow Nailing Method*. Translated by U.S. Fleet. U.S. Naval Forces, Germany Technical Section (Medical). 2nd ed. Schonkirchen, Germany: Stryker Trauma; 2006: 191–199.
11. Gerhard Küntscher. *Practice of Intramedullary Nailing*. Translated by Herman Rinne. Springfield, IL: Thomas Books; 1967:105–115.
12. Winquist RA, Hansen ST Jr, Clawson DK. Closed intramedullary nailing of femoral fractures. A report of five hundred and twenty cases. *J Bone Joint Surg Am*. 1984;66:529–539.
13. Harper MC, Carson WL. Curvature of the femur and the proximal entry point for an intramedullary rod. *Clin Orthop Relat Res*. 1987;220: 155–161.
14. Ostrum RF. A greater trochanteric insertion site for femoral intramedullary nailing in lipomatous patients. *Orthopedics*. 1996;19:337–340.
15. Boriani S, De lura F, Campanacci L, et al. A technical report reviewing the use of the 11-mm Gamma nail: interoperative femur fracture incidence. *Orthopedics*. 1996;19:597–600.
16. Kukla C, Heinz T, Gaebler C, et al. The standard Gamma nail: a critical analysis of 1,000 cases. *J Trauma*. 2001;51:77–83.
17. Statistics NCfH. *Anthropometric Reference Data for Children and Adults: US Population*. Hyattsville, MD: Center for Disease Control; 1999–2002.
18. Russell TA, Mir HR, Stoneback JS, et al. Avoidance of malreduction of proximal femoral shaft fractures with the use of a minimally invasive nail insertion technique (MINIT). *J Orthop Trauma*. 2008;22:391–398.

Amsterdam Foot and Ankle Course 2010, June 24th and 25th, Academic Medical Center, Amsterdam, the Netherlands. This international course is a two-day course on arthroscopy of the ankle and hindfoot, featuring cadaver sessions, lectures, live surgery presentations, case discussions, a workshop, an interactive computer course and a fireside quiz. Each year the course has an international faculty.

Information: www.ankleplatform.com

17th International Conference on Mechanics in Medicine and Biology 2010, September 19–24, Cracow, Poland.

This meeting is organized to present the results of interdisciplinary research concerning engineering, medicine and biology.

Information: <http://www.icmmb17.pwsos.pl>